

Improving continuous-flow analysis of triple oxygen isotopes in ice cores: insights from replicate measurements

Lindsey Davidge¹, Eric J. Steig¹, Andrew J. Schauer¹

¹Department of Earth and Space Science, University of Washington, Seattle, 98195, USA

5 *Correspondence to:* Lindsey Davidge (ldavidge@uw.edu)

Abstract. Stable water isotope measurements from polar ice cores provide high-resolution information about past hydrologic conditions and are therefore important to understanding Earth's climate system. Routine high-resolution measurements of $\delta^{18}\text{O}$, δD , and deuterium excess are made by continuous-flow analysis (CFA) methods that include laser spectrometers. Cavity ring-down laser spectroscopy (CRDS) allows for simultaneous measurements of all stable water isotopes, including $\delta^{17}\text{O}$ and ^{17}O excess ($\Delta^{17}\text{O}$). Here, we explore the reproducibility of $\Delta^{17}\text{O}$ measurements made by a CRDS instrument coupled to a CFA system. We present replicate measurements of an ice core sample taken from Summit, Greenland, and we demonstrate that the CFA-CRDS method can make high-precision measurements of $\Delta^{17}\text{O}$ (<5 per meg). We demonstrate that the magnitude and timing of variability within the core is well matched by discrete CRDS measurements, but we find that small offsets caused by the calibration intercept persist in our data. When these offsets are accounted for, the variability among replicate CFA-
15 CRDS measurements is as precise as expected by an Allan variance analysis. Our work shows that CFA-CRDS methods can detect very highly resolved $\Delta^{17}\text{O}$ information in ice core samples, but it also highlights the importance of developing calibration strategies with attention to $\Delta^{17}\text{O}$.

1 Introduction

Records of water isotopologues from ice cores are fundamental to the study of past climate processes (Dansgaard, 1964).
20 Oxygen ($\delta^{18}\text{O}$) and hydrogen (δD) isotope ratios have been measured routinely in ice core samples and in other natural waters due to their well understood, first-order equilibrium fractionation relationship to atmospheric temperature (Jouzel et al., 1997). Additionally, deuterium excess (d) is commonly used as an indicator of kinetic fractionation processes within the hydrologic cycle (Merlivat and Jouzel, 1979). Deuterium excess is conventionally defined as:

$$d = \delta\text{D} - 8 * \delta^{18}\text{O}. \tag{1}$$

25 Barkan and Luz (2005) showed that measuring $\delta^{17}\text{O}$ and $\delta^{18}\text{O}$ at sufficiently high precision allows for the determination of ^{17}O excess ($\Delta^{17}\text{O}$), a quantity that, like d , also reflects nonequilibrium fractionation processes such as sea-surface humidity (Uemura et al., 2010) and supersaturation effects during snow formation (Schoenemann et al., 2014). $\Delta^{17}\text{O}$ is defined by Luz and Barkan (2010) as the deviation in $\delta^{17}\text{O}$ from the global meteoric water line:

$$\Delta^{17}\text{O} = \ln(\delta^{17}\text{O} + 1) - 0.528 \ln(\delta^{18}\text{O} + 1), \quad (2)$$

30 where δ (“delta”) values are expressed as a unitless fractional deviation from Vienna Standard Mean Ocean Water (VSMOW; see e.g., Schoenemann et al., 2013, for a complete discussion of nomenclature).

Measurements of $\delta^{18}\text{O}$, δD , and d by laser spectroscopy have been demonstrated by many laboratories (e.g., Kerstel et al., 1999; Iannone, 2010; Steen-Larsen, 2014; Schauer et al., 2016; Jones et al., 2017). For water-isotope measurements of ice cores, it is increasingly common to couple a laser spectrometer with a continuous-flow analysis (CFA) system. CFA processing
35 reduces sample handling and can produce very high depth-resolution (originally described by Gkinis et al., 2010; 2011). Highly resolved water isotope measurements are advantageous for a variety of studies, such as those that use the water-isotope diffusion length to infer information about firn processes or to reconstruct temperature histories (e.g., Gkinis et al., 2014; Kahle et al., 2018; 2021; Jones et al., 2017b). It is desirable to obtain measurements of $\delta^{17}\text{O}$ and $\Delta^{17}\text{O}$ at a resolution comparable to that for $\delta^{18}\text{O}$, δD , and d . Corresponding measurements of both $\Delta^{17}\text{O}$ and d – which have differing sensitivities to kinetic
40 fractionation processes – could help to disentangle the various processes that influence water isotope values during evaporation, atmospheric transportation and snow formation (Angert et al., 2004; Uemura et al., 2010). However, measurements of $\Delta^{17}\text{O}$ require much higher precision than the other water-isotope ratios and have therefore generally been obtained by isotope-ratio mass spectrometry (IRMS) (Luz and Barkan, 2010; Landais et al., 2008; 2012; Schoenemann et al., 2013, 2014). Because the IRMS method is relatively expensive and time-consuming, $\Delta^{17}\text{O}$ measurements from ice cores are
45 limited in spatial and temporal resolution (e.g., Landais et al., 2008; Schoenemann et al., 2014; Aron et al., 2021). CFA for $\Delta^{17}\text{O}$ has the potential to address this limitation.

Laser spectroscopy enables simultaneous measurements of $\delta^{17}\text{O}$, $\delta^{18}\text{O}$, and δD (and therefore d and $\Delta^{17}\text{O}$). Steig et al. (2014) developed a cavity-ring-down laser spectrometer (CRDS) for $\Delta^{17}\text{O}$ analysis, sold commercially as the Picarro L2140-*i*; other instruments with different spectroscopic methods have also been developed for $\Delta^{17}\text{O}$ analysis (e.g., Berman et al., 2013; Tian et al., 2016). Schauer et al. (2016) demonstrated that the L2140-*i* CRDS configured with an autosampler can routinely measure
50 $\Delta^{17}\text{O}$ from discrete water samples with precision and accuracy comparable to IRMS methods. Steig et al. (2021) obtained continuous measurements of all water isotope quantities ($\delta^{17}\text{O}$, $\delta^{18}\text{O}$, δD , d , $\Delta^{17}\text{O}$) on an ice core from the South Pole by using the L2140-*i* CRDS coupled to the CFA system developed by Jones et al. (2017). However, despite the potential shown by these studies, the adoption of CFA-CRDS for $\Delta^{17}\text{O}$ faces two primary challenges. First, the integration time required for high-
55 precision $\Delta^{17}\text{O}$ measurements by CRDS – approximately 1000 s to achieve precision of 10 per meg (Steig et al., 2014) – is much greater than the integration time required to achieve meaningful precision for $\delta^{18}\text{O}$, δD or d . Second, the CFA system – i.e., the melting and vaporization process used to introduce an ice core sample into the CRDS – may further degrade the measurement quality by processes that are not yet well understood. For example, Steig et al. (2021) identified occasional large (>20 per meg) offsets in CFA-CRDS $\Delta^{17}\text{O}$ in their measurements of the South Pole ice core; the cause of these offsets was
60 unclear. It is our goal to characterize the reproducibility of replicate ice core measurements of $\Delta^{17}\text{O}$ by CFA-CRDS.

Here, we describe a CFA-CRDS measurement methodology that was designed for high-resolution measurements of $\Delta^{17}\text{O}$. We take advantage of archived ice core samples from Summit, Greenland to make repeated CFA-CRDS measurements of $\Delta^{17}\text{O}$. These samples (collected by Hastings et al., 2009) provide an opportunity to explore the potential and limitations of $\Delta^{17}\text{O}$ measurements by CFA-CRDS more fully. We use replicate measurements made by CFA-CRDS and discrete CRDS methods to assess the reproducibility of CFA-CRDS $\Delta^{17}\text{O}$ data and to identify sources of measurement error.

2 CFA-CRDS design and configuration

We use a CFA processing line in combination with a CRDS laser spectrometer (L2140-*i*, Picarro Inc., as in Steig et al., 2014) to measure $\Delta^{17}\text{O}$ of ice core samples. The function of the CFA line is to generate a continuous supply of constant-humidity sample vapor to the CRDS analyzer; to achieve this, we have built a custom vaporizer unit that is described below. A constant stream of vaporized sample is important because errors in isotope-ratio measurements can arise from inconsistent vapor pressure at the CRDS inlet (Gkinis et al., 2011; Schauer et al., 2016). Finally, we aim to characterize and reduce diffusion and mixing within the CFA system to avoid smoothing the resulting measurements.

2.1 Custom vaporizer design

Continuous and complete vaporization is critical to reducing errors in all CRDS stable water isotope measurements, and it is especially important for attaining the per-meg precision necessary to detect meaningful variations in $\Delta^{17}\text{O}$. Previous studies have achieved continuous vaporization by heating sample water in the presence of dry air, either within an insulated stainless-steel tee (e.g., Gkinis et al., 2010; 2011) or within a concentric glass nebulizer with a vaporizing tube (e.g., Emanuelsson et al., 2015; Jones et al., 2017). Gkinis et al. (2010; 2011) designed a flash vaporization process to instantaneously vaporize a continuous stream of sample water; the flash vaporization process involves a continuous stream of water that is combined with a continuous stream of dry air inside a 0.50-mm internal diameter stainless-steel tee that is maintained at near-ambient pressure. Steig et al. (2021) measured $\Delta^{17}\text{O}$ by CFA-CRDS with the CFA configuration of Jones et al. (2017): a continuous stream of water sample at 1030 kPa (150 psi) is aerosolized within a concentric glass nebulizer; the aerosolized sample droplets then evaporate completely within a 1.8-cm internal diameter, 20-cm-long glass vaporizing tube that is heated to 200 °C. In this configuration, the CRDS analyzer draws vaporized sample from the vaporizing tube, and excess sample vapor is vented to laboratory air (Jones et al., 2017; Steig et al., 2021). Two critical differences between the Gkinis et al. (2010; 2011) and Jones et al. (2017) methods are the volume of the vaporization chamber and the volume of vapor that is generated. The smaller volume of the flash vaporizer should limit signal smoothing between the vaporizer and the analyzer. However, the flash vaporization method described by Gkinis (2010; 2011) generates vapor at approximately the rate that it is required by the analyzer, whereas the nebulizer method of Jones (2017) produces an excess of vapor that is vented prior to reaching the analyzer. Producing excess vapor is another way to limit the signal smoothing upstream of the vapor vent because it increases the velocity of sample through the system.

For this study, we built a custom vaporizer unit that benefits from both the small volume of the flash vaporizer and also the production of excess sample vapor; we also adopted additional monitoring techniques to ensure stability within the system during analysis. We use a 0.50-mm stainless-steel tee as used by Gkinis et al. (2010; 2011), but we operate our vaporizer at a
95 much higher mixing pressure (typically 200 kPa) than is used by Gkinis et al. to produce and vent approximately thirty times more vapor than is required for analysis. A small system volume combined with a high volumetric flow rate leads to a short retention time within the vaporizer that limits mixing of adjacent ice core layers. An additional benefit of the small vaporizer volume is that flow inconsistencies (i.e., changes in sample flow rate caused by flow obstructions or bubble interruptions) that may occur within the vaporizer can be observed by the 1-Hz CRDS measurement values; patterns in water vapor concentration
100 or instantaneous isotope readings provide information about vaporization conditions that is important for identifying and avoiding water isotope fractionation. We use CRDS observations of water concentration and uncalibrated water isotope values as well as electronic pressure sensors to infer vaporization conditions that may affect $\Delta^{17}\text{O}$. This information is used to tune the CFA-CRDS system prior to analysis, with the goal of reducing possible isotope fractionation that may cause errors in $\Delta^{17}\text{O}$; this process is described more fully in Section 3.1.

105 2.2 CFA-CRDS system configuration

Figure 1 illustrates the CFA-CRDS system from ice core to vapor analysis. Glacial ice is melted on a 30×30 mm² aluminium melt head that is fitted with four resistance heater cartridges and held at constant temperature by a PID controller (Bigler et al., 2011). Sample melt is drawn away from the melt head and through an automated selector valve (VICI, p/n C25Z-3186EMH) by a dedicated peristaltic pump, PUMP-1 (MasterFLex L/S 7535-04). The automated valve is configured to select a rotating
110 sequence of calibration standards when ice cores are not being measured. Sample melt is carried by 0.5-mm internal diameter PFA conveyance tubing between all system components prior to the vaporizer; PFA tubing was chosen because its transparency is advantageous for identifying bubbles and investigating flow instability issues. From PUMP-1, water flows through a Darwin Microfluidics gas-permeable membrane bubble trap (44 μL internal volume, p/n LVF-3526) where bubbles are removed and vented to the laboratory air. Excess water pressure is relieved at a vent. Sample water is drawn away from the vent by PUMP-
115 2 (same model as PUMP-1), whose flow rate is set to match the demand of the downstream vaporizer, which is much smaller than the supply of melt water from the ice core. The vent accommodates the differences between PUMP-1 (which controls the melt rate) and PUMP-2 (which controls the vaporization rate). Water flows through 2- μm and 1- μm in-line filters in series to restrict the flow of particulates into the vaporizer. PUMP-2 is also preceded and followed by electronic pressure sensors PI-1 (Elveflow PS3-Small) and PI-2 (Elveflow PS4-Small) to monitor injection pressure conditions and pump and filter
120 performance. Typically, the pressurized dry air entering the vaporizer adds backpressure on the liquid sample injection line, which damps the cyclic pressure fluctuations of the peristaltic pump and leads to more constant vaporizer operations; this allows us to balance the sample pressure with the dry air pressure. The system also includes a flow valve (FV-1) that can be used to adjust the backpressure on PUMP-2.

At the vaporizer, filtered sample water is mixed and heated with dry air to produce a constant-humidity stream of vaporized sample. Immediately before entering the vaporizer, the liquid sample line is reduced to a 100- μm fused silica capillary tube. The 100- μm capillary provides sufficient flow restriction that is important for efficient vaporization while also performing well for periods of several days without clogging. The custom vaporizer includes a 0.50-mm internal diameter tee heated to 170 °C using a PID-controlled resistance heater cartridge, similar to Gkinis et al. (2010; 2011). The vaporizer combines pressurized dry air with liquid sample, and it is set within an aluminium enclosure that is lined with 3.175 cm of calcium silicate insulation. After the sample is vaporized, the vapor is drawn into the optical cavity where it is measured, and excess vapor is vented into the laboratory. Vapor is carried from the vaporizer to the optical cavity within insulated tubing to prevent condensation.

2.3 Design choices to mitigate memory effects

Finally, the CFA system is designed to reduce memory between measurements. Because our automated selector valve is positioned immediately after the ice core melt head, reference waters pass through all components of the sample handling system except the melt head and its tubing; by design, the mixing length expected between measured ice core layers with differing isotopic composition can be approximated by the mixing length represented by transitions in reference waters if all other system conditions are identical. Mixing length within the system is reduced in two ways: overall sample handling system volume and tubing diameters are minimized, and excess sample volume is drawn through the entire system during CFA analysis to limit the sample retention time. During ice core measurements, approximately six times more water is handled by PUMP-1 than is sent by PUMP-2 into the vaporizer; excess liquid volume is vented before PUMP-2. Similarly, approximately thirty times more vapor is generated than is analyzed; excess vapor is driven by the differential between PUMP-2 and the L2140-*i* inlet pump, and it is vented to laboratory air immediately before vapor enters the optical cavity. In this way, the liquid and vapor tubing is flushed with many times more sample volume than is required for analysis.

145 3 CFA-CRDS operations and measurements

We designed an operational sequence for reference water and ice core measurements during a period when lab work was intermittent due to the COVID-19 pandemic. The CFA system was configured to automatically measure an alternating sequence of three in-house reference waters over a period of approximately seven weeks; reference waters included Seattle tap water (SW2), West Antarctic Ice Sheet Divide snow (CW), and South Pole snow (SPS2), as shown in Table 1 and indicated in Fig. 2. Measuring reference waters continuously allows us to explore the long-term changes in system calibration while also informing maintenance requirements over long timescales. When available, an operator prepared and measured an ice core section between reference water measurements. The need for frequent calibration of CRDS data for $\Delta^{17}\text{O}$ has been well documented (e.g., Schauer et al., 2016), and continuous reference water measurements ensured that there was calibration data available adjacent in time to each intermittent ice core analysis.

155 We operate the CFA-CRDS system to measure nine repeated sections of an ice core, in addition to a repeated sequence of internal reference waters that are used to calibrate the ice core measurements; we measure an additional replicate ice core section by discrete CRDS for comparison. Repeated reference water measurements are used to develop a calibration for the ice core data. We compare our calibrated CFA-CRDS $\Delta^{17}\text{O}$ data with the discrete measurements to evaluate this method.

3.1 Operational considerations to maintain efficient vaporization

160 Because the vaporizer is sensitive to small fluctuations in sample flow rate, a careful balance of system pressures is required to control sample flow (Gkinis et al., 2010; 2011); specifically, the pressure of the sample at the vaporizer inlet must be slightly greater than the pressure of the dry air within the vaporizer. Maintaining a balance between the air pressure and sample pressure within the vaporizer requires knowledge of both pressure conditions. We monitor pressures at PI-1 and PI-2 so that it is possible to diagnose the source of system pressure changes when they occur; we also fix the pressure of the dry air line with the
165 backpressure regulator (typically 200 kPa). Vacuum conditions at PI-1 indicate particulate loading across the filter screen at F-1; the filter screen will clog over time and, if the filter screen is not replaced, suction from the inlet of PUMP-1 can draw a vacuum at PI-1. Vacuum conditions at PI-1 can impact the downstream peristaltic pump (PUMP-2) performance, ultimately causing inconsistent flow into the vaporizer and analyzer. Under optimal analysis conditions, the pressure is near ambient at PI-1. A decrease in pressure at PI-2 indicates upstream vacuum conditions or worn peristaltic pump tubing at PUMP-2. An
170 increase in pressure at PI-2 indicates clogging downstream, which can occur as particulate loading within F-2, or as mineral precipitation within the capillary or vaporizer. The pressure at PI-2 generally varied between 200 kPa and 400 kPa, depending on the injection air pressure and the precipitate levels within the vaporizer or capillary tubing. High-pressure vaporizer conditions allow sample to flow despite the inevitable accumulation of precipitate within the vaporizer, which enables the system to operate in balance for days or even weeks. However, over time, precipitate accumulation within the vaporizer can
175 restrict the flow of air, water, or both; this typically requires re-balancing of system flow conditions, but it can occasionally require removing and cleaning vaporizer fittings with soap, water, and physical agitation.

During operation of the CFA-CRDS, intermittent reductions in water vapor concentration can occur within the vaporizer, which can produce perturbations in the isotope data. Gkinis et al. (2010; 2011) described sample flow inconsistencies at their CFA flash vaporizer that cause extreme outliers in isotope data, though the cause of the fluctuations was unclear. We observe
180 similar fluctuations, and the pressure sensor data provide insight into their cause. We find that the most common causes of such variations are microbubbles entering the vaporizer owing to particulate loading, which can cause poor debubbler performance and can also cause blockages to form within small tubing fittings. Microbubbles that remain suspended in the fluid stream after the debubbler cause volumetric flow rate reductions at the vaporizer inlet. Blockages within fittings upstream of PUMP-2 can cause extreme vacuum conditions before the pump (i.e., pressure observations associated with blockages were
185 as low as -140 kPa before PUMP-2 instead of the typical ambient conditions); this can lead to the contamination of system tubing with small bubbles that also cause temporary flow reductions. To avoid these inconsistencies, we find that it is important

to re-seat the debubbler membrane to improve efficiency and to maintain ambient pressure at the PUMP-2 inlet by replacing clogged filter screens or tubing fittings. Although data outliers could be systematically removed (as done in Gkinis et al., (2011)), occasional bubbles do not substantially impact the isotopic mean value of our ice core measurements and are retained here. We do exclude some reference-water calibration data, where bubble interruptions are most frequent due to limited operator oversight during the automated reference water measurements. Calibration measurement criteria are discussed in Section 3.4, below.

In addition to monitoring pressure evolution across the system, we can also observe the quality of vapor at the CRDS analyzer via characteristic patterns that arise in the CRDS data. Specific patterns in water vapor concentration and $\delta^{18}\text{O}$ that emerge from incomplete vaporization or unstable flow into the vaporizer are shown in Fig. 3. Incomplete vaporization is indicated by anticorrelated changes in water vapor concentration and $\delta^{18}\text{O}$. We attribute these anticorrelated patterns in water vapor concentration and $\delta^{18}\text{O}$ to larger droplet formation within the vaporizer, caused by insufficient backpressure on PUMP-2 and pulsating flow conditions. Large-amplitude (>70 kPa) pressure fluctuations from the peristaltic pump cause pulsating flow into the vaporizer that alternates between overwhelming and undersupplying water to the vaporizer. The resulting patterns have a large amplitude (up to 10,000 ppm for water vapor, and several per mil for $\delta^{18}\text{O}$) and a frequency that mirrors that of the peristaltic pump (e.g., Fig. 3a). The observed fractionation that occurs during these vaporization conditions leads to very poor calibration values for $\Delta^{17}\text{O}$, causing errors of 10s to 100s of per meg. If there is sufficient backpressure at PUMP-2, the pressure readings at PI-2 are typically <40 kPa. We attribute small fluctuations in $\delta^{18}\text{O}$ that are anticorrelated with water vapor concentration to the incomplete vaporization of individual droplets (e.g., Fig. 3b). Because inconsistent flow into the vaporizer can cause isotope fractionation and because it is important to measure calibration standards under the same conditions as the ice core samples, we tune the system to maintain steady pressure readings at the vaporizer inlet prior to ice core analysis, as discussed in Section 3.2.; vapor concentration data that is typical of a well-maintained CFA system are shown in Fig. 3d.

3.2 Measuring $\Delta^{17}\text{O}$ by CFA-CRDS in ice core samples

Approximately twelve to twenty-four hours before making an ice core measurement, an operator maintained the CFA system to balance the flow rate into the vaporizer. For example, when indicated by pressure sensor data, filter screens, peristaltic pump tubing, or capillary tubing were replaced. When indicated by CRDS data trends, the vaporizer components were cleaned. Returning the CFA system to a balanced state before making measurements of all reference waters increases the likelihood of having usable, high-quality calibration data against which to calibrate the ice core samples. At other times when ice core measurements were not made, the system occasionally drifted out of balance and was not actively maintained, such that some of the reference water measurements are of lower quality than those used to calibrate the ice core measurements. This is discussed in more detail in Section 3.4.

We cut an 87.5-cm ice core sample, from ~92 m depth beneath the surface at Summit, Greenland, into nine 26-mm square slices to prepare them for continuous analysis. After preparing these nine CFA sticks, a tenth section of core was cut into 63 discrete depth intervals. Discrete ice samples were melted in sealed polyethylene sample bottles in a refrigerator at 4° C. We measured the 87.5-cm section of ice ten times: the nine replicate slices were measured by the CFA-CRDS configuration described above, and the tenth measurement was made by discrete injection of 63 melt samples from the core using the commercially available vaporizer unit (Picarro p/n A0211) and automated injections as in Schauer et al. (2016). The resolution of the discretely measured ice is 1.39 cm.

For all CFA measurements, we made visual observations of the core height to monitor the melt rate during analysis, then later assigned a high-resolution depth equivalent for each analysis time that is based on the value of $\delta^{18}\text{O}$ and the measured depth of discrete samples. Previous work has monitored core depth with electronic distance meters (e.g., Bigler et al., 2011; Jones et al., 2017), and such measurements are critical for depth registration for routine CFA measurement campaigns. Here, we forego electronic depth registration and instead adjust initial depth estimates for each core section by aligning the seasonal cycle of $\delta^{18}\text{O}$ for all core samples. Summit, Greenland has a modern annual accumulation rate of 24 ± 5 cm (ice equivalent) per year (Meese et al., 1994; Dibb and Fahnestock, 2004; Hawley et al., 2008; 2021), and we expect to see two to three years represented by the core sample that we measured in replicate (Hastings et al., 2009). Assigning depths by aligning the $\delta^{18}\text{O}$ variations should largely eliminate depth-registration errors, since the strong seasonal $\delta^{18}\text{O}$ variations must be essentially identical in each replicate sample, and the signal to noise ratio for $\delta^{18}\text{O}$ is very high. We compressed the depth scale of each CFA record to maximize the cross-correlation of $\delta^{18}\text{O}$ ($0.93 < R < 0.99$) between the CFA measurements and the discrete measurements. We then assigned each CFA analysis time a depth equivalent based on the depth of the corresponding discrete $\delta^{18}\text{O}$ data. We note that the magnitude of the seasonal variations in $\delta^{18}\text{O}$ are somewhat compressed in the lower ~30 cm of this core sample, so the depth designations for this interval are likely a greater source of error than in the rest of the ice. Nevertheless, we are confident that our depth registration is precise to within a cm or better throughout the core, determined by assessing the variance in depth assignments at inflection points.

240 3.3 Operational choices to mitigate memory effects

Mitigating memory effects is important for both ice core and reference water measurements; in addition to the design choices highlighted in Section 2.3, there are several operational choices that were made to reduce the memory between isotopically distinct waters. For example, increasing the pump rates at PUMP-1 during ice core analysis should drive shorter retention times within the tubing upstream of the liquid vent, which should reduce system mixing. In this way, the transition times for reference waters (shown in Fig. 2) are a conservative estimate of mixing effects. The transition time between measurements of reference waters generally varied between 180 and 360 s. We therefore assume a conservative mixing time of 360 s during reference water transitions, and we ignore the 360 s that initiate and conclude each reference water measurement. Before measuring each section of ice (which is typically ~1 m long), we also condition the system with at least ten minutes of water

with similar isotopic composition to prevent mixing between isotopically disparate reference waters and ice core samples at the beginning of the analysis. Finally, the replicate CFA-CRDS measurements that are the focus of this study serve as a practical evaluation of the effects of memory on measurement fidelity in this configuration.

3.4 Calibrating CFA-CRDS $\Delta^{17}\text{O}$ data

To achieve an accurate calibration, similar treatment of reference waters and sample melt during vaporization is critical. For this study, we measured the calibration standards after making system adjustments and immediately before measuring an ice core section; this ensures the most comparable treatment of reference waters and sample melt. Achieving similar treatment also requires that the system is stable during the entire measurement period, including reference water measurements and ice sample measurements. Although the CFA system has maintained stable operations for periods of days or weeks and an individual ice core measurement takes only a few hours, we limit our reference water measurements to three hours each to increase the likelihood that the complete sequence of reference waters and ice core samples is measured under similar conditions.

To calibrate our $\Delta^{17}\text{O}$ measurements, we create a two-point linear calibration for $\delta^{17}\text{O}$ and $\delta^{18}\text{O}$ from the nearest measurements of our internal reference waters, SW2 and SPS2; a third reference water (CW) is used as an independent verification of the calibration. The values of SW2, CW, and SPS2 have been measured independently and are normalized to the VSMOW-SLAP scale as in Schoenemann et al. (2013). Three-hour measurements of these alternating reference waters were made between measurements of the ice core sample; to measure a reference water, the selector valve was electronically switched to the next sequential water, causing the peristaltic pump to draw reference water volume from a new standard container. Reference water measurements were automated and typically unsupervised. Because measurement conditions evolve over time due to particulate loading and mineral precipitation within the CFA components and because there were periods of time during the analysis window when no operator was available to monitor system conditions, there were periods of time during which the water vapor concentration was outside the ideal range or during which large bubbles or other flow inconsistencies degraded the quality of reference water data. All supervised reference water measurements are retained and utilized in the ice core data calibration, but we automatically reject calibration data and measurements of CW that were generated from water vapor concentration beyond the targeted range (i.e., $<20,000$ or $>50,000$ ppm) or data with insufficient vaporizer operations, indicated by $\sigma_{\delta^{18}\text{O}} > 0.5$ ‰ across the measurement window. Typical variability of water vapor concentration within a single three-hour period is 0.5% to 5%. We identify transitions from one reference water to the next in the data by the second derivative of δD , and assign known standard values based on the uncalibrated measurement values of δD . We include measurements of SW2 and SPS2 that contain at least 6000 s of analysis time and we trim 360 s of data from the beginning and end of each measurement interval to avoid memory effects. The mean and standard deviation of the analysis time for calibration standard data is $9350 \text{ s} \pm 660 \text{ s}$. For the measurement interval reported in this study, we use a calibration made from 47 continuous, 3-hour measurements of SW2 and 40 continuous, 3-hour measurements of SPS2. All analyses include measurements for $\delta^{17}\text{O}$,

$\delta^{18}\text{O}$, and δD . Calculations of d and $\Delta^{17}\text{O}$ were obtained from the calibrated δ values as given in equations [1] and [2], respectively. Calibration for $\Delta^{17}\text{O}$ is more completely described below.

285 The calibration for the complete measurement window is generated from all measurements of SW2 and SPS2 that meet the screening criteria above; calibration data are shown alongside the complete sequence of measurements in Fig. 4. For each calibration of CW or ice core data, we employ the preceding measurements of SW2 and SPS2 for the calibration. The calibration is performed separately for $\delta^{17}\text{O}$ and $\delta^{18}\text{O}$: using a least-squares approach, we fit a linear equation to the uncalibrated average measurements so that the calibrated SW2 and SPS2 measurements match their known values. The calibration equation therefore becomes:

$$\delta_{\text{calibrated}} = m * \delta_{\text{uncalibrated}} + b, \quad (3)$$

290 where δ represents either $\delta^{17}\text{O}$ or $\delta^{18}\text{O}$. An account of m and b for both $\delta^{17}\text{O}$ and $\delta^{18}\text{O}$ is shown for the complete measurement window in Fig. 4. Finally, $\Delta^{17}\text{O}$ is calculated from the calibrated values of $\delta^{17}\text{O}$ and $\delta^{18}\text{O}$. The mean and standard deviation of all CW measurements of $\Delta^{17}\text{O}$ during the analysis period is 25 ± 12 per meg ($n=53$). The subset of CW measurements with the most consistent CFA operations – and therefore the lowest variability for $\delta^{18}\text{O}$ ($\sigma < 0.06 \text{ ‰}$) – had corresponding $\Delta^{17}\text{O}$ values of 25 ± 6 per meg ($n=36$). Low variability among reference water measurements suggests that our system design and calibration
295 strategy are sufficient for ice core measurements.

3.5 Processing CFA-CRDS $\Delta^{17}\text{O}$ data

After assigning approximate depth values and calibrating the $\sim 1\text{-Hz}$ data, we discretize the CFA-CRDS data by binning the calibrated data into prescribed depth intervals and averaging across the entire interval. This enables quantitative comparison between the continuous CFA-CRDS timeseries and the discrete CRDS measurements. Small differences in the instantaneous
300 melt rate cause some variability in the data-averaging duration for each reported measurement; the typical instantaneous melt rate was ~ 0.3 cm/min, but rates ranged from ~ 0.1 cm/min to ~ 0.4 cm/min during analysis. We report our CFA-CRDS measurements with 1.39-cm resolution to match the resolution of our discrete CRDS measurements. We also explore the effects of depth resolutions that range from 0.5 cm to ~ 40 cm, given that increasing the averaging window of the $\sim 1\text{-Hz}$ spectroscopic measurements reduces instrumental noise (e.g., Werle et al., 1993; Gkinis et al., 2010; 2011; Steig et al., 2014;
305 2021; Schauer et al., 2016; Jones et al., 2017).

4 Results and analysis

Our isotope measurements capture a period of approximately two years of precipitation, as expected for a Greenland ice core from the depth we analyzed (discussed in Section 3.2). The seasonal cycle of $\delta^{18}\text{O}$ is shown in Fig. 5. We estimate that our depth assignments are accurate to < 7 mm throughout the core by determining the variability in depth assignments at all

310 inflection points; this allows us to compare CFA-CRDS measurements of $\Delta^{17}\text{O}$ at the ~cm scale, appreciably finer resolution than has previously been reported. Our comparison quantifies the reproducibility of our measurements and identifies sources of variability among these CFA-CRDS $\Delta^{17}\text{O}$ data.

4.1 Seasonal $\Delta^{17}\text{O}$ variations in replicated CFA and discrete measurements

We compare our CFA-CRDS data for $\Delta^{17}\text{O}$ with discrete CRDS measurements to evaluate the CFA-CRDS method. We present
315 the mean value and standard error of all replicate measurements in Fig. 5 with 1.39-cm averaging (representing approximately 270 s of data per interval for each individual CFA-CRDS replicate); Figure 5 also shows the discrete CRDS measurements with the root mean square error of the corresponding discrete reference water measurements. The mean of all CFA-CRDS measurements (representing more than 2000 s of data per interval) is well correlated with the discrete measurements ($r = 0.52$ with 99% confidence), especially in the upper 50 cm of the core ($r = 0.70$ with 99% confidence). Both the CFA-CRDS data
320 and the discrete CRDS data show clear seasonal $\Delta^{17}\text{O}$ variations at this measurement resolution and are matched in magnitude and timing.

4.2 Error attribution for CFA-CRDS $\Delta^{17}\text{O}$ measurements

Next, we characterize the variability observed among our CFA-CRDS measurements; in addition to the depth alignment errors discussed above, sources of variability introduced by this CFA-CRDS method may include high-frequency instrumental noise,
325 calibration errors, and smoothing or bias generated by mixing within the CFA system. High-frequency, high-amplitude noise (~1 ‰) in the uncalibrated CRDS data is inherent to the instrument and can cause large aberrations from the true value of $\Delta^{17}\text{O}$, especially over short averaging times; long averaging times (>1000 s) are typically used when measuring $\Delta^{17}\text{O}$ by CFA-CRDS to reduce the impact of this instrumental noise. Calibration errors in $\Delta^{17}\text{O}$ occur when measurement treatment differs between calibration standards and samples or between calibration standards; this can cause fractionation to occur in the
330 uncalibrated $\delta^{17}\text{O}$ and $\delta^{18}\text{O}$ measurements, leading to suboptimal calibration slope and intercept information. Despite efforts to stabilize vaporizer system conditions prior to ice core sample analysis and to measure ice core samples with the same treatment, it is likely that some calibration errors persist in our ice core data because it is not possible to measure the standards and the sample at the same time. Finally, CFA measurement error for $\Delta^{17}\text{O}$ may result from mixing isotopically distinct waters during CFA processing or from other processing issues that affect the internal variability (i.e., perceived seasonality) of the
335 continuous ice core measurement.

Typical CRDS characterization studies have used repeated measurements of reference waters to identify measurement error. By measuring reference waters, it is possible to approximate the precision of the uncalibrated measurements by determining the effect of averaging time on the intrinsic noise of the measurement; it is also possible to quantify the variance of the calibrated, averaged data. Our replicate CFA-CRDS measurements provide an opportunity to interrogate the source of CFA-

340 CRDS errors because we can separately analyze the variability internal to each timeseries (e.g., due to the seasonal cycle of $\Delta^{17}\text{O}$ or due to CFA errors) and the variability between the mean values of the nine measurements (e.g., due to calibration offsets).

To isolate the effect of the calibration intercept, we processed the data in two ways: first, we calibrated the data as described and reported above, and second, we removed the mean value of each calibrated CFA-CRDS dataset to eliminate any error
345 contributed by the calibration intercept, b. We discretized the CFA-CRDS data to a series of depth-resolution schemes that ranged from 1.39 cm to 43.75 cm. We calculated the standard error for all depth intervals across all measurement resolutions. The total error for the calibrated data is approximated by the black line in Fig. 6, which represents the mean of the standard error across all depth intervals for all measurement replicates. The total span of the standard error at every depth interval is provided by the grey shaded region. Similarly, the blue shaded region shows the total span of the standard error for the datasets
350 with the mean removed, and the blue line is the mean error. The region between the two solid lines is the fraction of the total error that can be attributed to the calibration intercept, b. The results show that the total error is <10 per meg for all data. The total error is ~ 5 per meg at averaging times longer than ~ 3000 s, which corresponds to depth averages of ~ 15 cm. Figure 6 also shows that the error that arises from differences in internal variability (i.e., the CFA error) for the CFA-CRDS data is <2 per meg with similar averaging and that the total error is dominated by calibration intercept error at long averaging times.

355 Finally, we directly compare the precision of our CFA-CRDS data with the precision of reference waters measured by CFA-CRDS, which is determined by an Allan variance analysis. An Allan variance analysis quantifies the relationship between signal noise and integration time (Allan, 1966; Werle et al., 1993); for CRDS data, this analysis of reference water measurements is commonly used to approximate the measurement precision of the system for any given measurement duration (Gkinis et al., 2010; Steig et al., 2014). We determine the Allan deviation (square-root of the Allan variance) from a long
360 continuous analysis (~ 8.5 hours) of the SW2 reference water made during our analysis window (shown in Fig. 4); the result is shown in Fig. 7. Differences between the Allan deviation and the standard deviation of our measurements should confirm whether the magnitude and timing of the variability is as precise as during reference water measurements, or if there are other changes imparted by the CFA system or calibration that may degrade CFA-CRDS data quality. We find the standard deviation $\sigma_{\text{CFA-}\Delta^{17}\text{O}}$ among all nine calibrated and discretized CFA-CRDS datasets, averaged over integration windows that vary from 5
365 mm to 43.75 cm. This analysis compares the precision of the final, calibrated measurements along the depth of the core sample with the precision of the reference water measurement, and ultimately quantifies the reproducibility of our CFA-CRDS measurements. We track the analysis time associated with each averaging interval and overlay the measured $\sigma_{\text{CFA-}\Delta^{17}\text{O}}$ with corresponding mean integration time for each depth interval on Fig. 7a.

Figure 7a shows generally good agreement between $\sigma_{\text{CFA-}\Delta^{17}\text{O}}$ and $\sigma_{\text{Allan-}\Delta^{17}\text{O}}$ at integration times less than 400 s, but the $\sigma_{\text{CFA-}\Delta^{17}\text{O}}$
370 $\Delta^{17}\text{O}$ data asymptotically approach a limit of 10 per meg at longer averaging times instead of following the trend predicted by the Allan variance analysis. To evaluate to what extent this mismatch between expected and observed σ can be attributed to

errors arising from the calibration intercept (as shown in Fig. 4), we repeat this analysis for the dataset with the mean-adjusted value. Figure 7b shows excellent agreement between $\sigma_{\text{CFA-}\Delta^{17}\text{O}}$ and $\sigma_{\text{Allan-}\Delta^{17}\text{O}}$ at all integration times when the effect of the calibration intercept is eliminated; this demonstrates that the drift in $\sigma_{\text{CFA-}\Delta^{17}\text{O}}$ shown in Fig. 7a can be entirely attributed to calibration effects, and not to the CFA process directly. Figure 7 suggests that the precision of calibrated CFA-CRDS measurements is not limited by the CFA process – nor to limitations of the CRDS instrument – but rather by the quality of the calibration information, which depends on the treatment and frequency of reference water measurements.

5 Discussion and Conclusions

5.1 Comparison of CFA-CRDS $\Delta^{17}\text{O}$ measurements to other $\Delta^{17}\text{O}$ measurements from Greenland

Our work complements previous studies that have examined the seasonal cycle of $\Delta^{17}\text{O}$ in polar regions, and good agreement with earlier work validates our measurements. Consistent with previous measurements from Greenland, the $\Delta^{17}\text{O}$ signal in our data is anticorrelated with d and anticorrelated with the seasonal cycle in $\delta^{18}\text{O}$ (Landais et al., 2008). The measurements presented here were made from core that represents approximately two years of ice accumulation from the 1760s (Hastings et al., 2009). The measured magnitude (peak to trough) of the seasonal cycle in $\Delta^{17}\text{O}$ is ~ 45 per meg at 1.39 cm resolution in our data (Fig. 4), which is in excellent agreement with the magnitude of the seasonal cycle reported previously for Greenland. Specifically, Landais et al. (2012b) reported seasonal magnitudes of ~ 25 per meg from a shallow firn core at NEEM (in Northwest Greenland) that represented accumulation periods between 1962-1963 and between 2003-2005; when we coarsen our measurement resolution to 3.6 cm – which approximates the \sim monthly (5-cm) measurement resolution in the NEEM core (detailed in Steen-Larsen et al., 2011) – the magnitude of the seasonal cycle in our data is ~ 30 per meg. Low errors between replicate values and the good agreement with previous studies strengthen confidence in the CFA-CRDS approach for high-resolution $\Delta^{17}\text{O}$.

Our results reinforce the use of the CFA-CRDS method for high-precision, high-resolution measurements of $\Delta^{17}\text{O}$ in ice cores. CFA-CRDS methods are valuable for detecting detail in $\Delta^{17}\text{O}$ variations in deep ice layers, for measuring $\Delta^{17}\text{O}$ in ice from sites with low accumulation rates, or for measuring $\Delta^{17}\text{O}$ in any glacial ice where high depth resolution is desired.

5.2 Addressing CFA-CRDS calibration errors in $\Delta^{17}\text{O}$

Because precision of all $\Delta^{17}\text{O}$ measurements by CRDS strongly depends on available calibration information, the importance of establishing a robust calibration strategy for CFA-CRDS cannot be understated. We iteratively revised our CFA-CRDS system and designed our calibration strategy as recommended below.

First, the CFA-CRDS configuration must be capable of stable operations that span the total duration of the ice core and reference water measurements. System stability for a given CFA system should be characterized with an Allan variance

analysis. We choose to measure calibration standards immediately before ice core measurements because they are filtered to 0.2 μm and therefore far less likely than the ice core melt to alter the flow conditions within the CFA system. Additionally, limiting system memory and reducing the transition time between reference waters maximizes the useful fraction of reference water data, allowing measurements of longer duration or measurements of more reference waters to be made within a period
405 of consistent CFA operations.

Next, quantifying the drift in calibration information over time (as shown in Fig. 4) can allow an operator to determine the physical controls on fractionation within a CFA-CRDS system. The change in calibration information can be used to inform system maintenance schedules or operational sequences. For example, we have observed that after operating our CFA-CRDS system for several weeks, the fractionation responses for $\delta^{17}\text{O}$ and $\delta^{18}\text{O}$ diverge, degrading the quality of calibration data for
410 $\Delta^{17}\text{O}$. Cleaning the vaporizer fittings appears to “reset” the calibration response, suggesting that the fractionation that occurs over long timescales is a result of physical effects within the vaporizer itself owing to precipitate formation.

Though our system is capable of high-precision measurements for $\Delta^{17}\text{O}$, our analysis suggests that some errors related to the calibration intercept persist, which is unsurprising when considering previously published work on similar methods. Large errors in $\Delta^{17}\text{O}$ were occasionally observed during the analysis of the South Pole ice core (SPC14); Steig et al. (2021) attributed
415 these errors to calibration differences and performed a correction by shifting the mean value of their measurements based on the offset identified by a calibrated reference water measurement. Our work supports the attribution of these errors to the calibration intercept and also supports the calibration adjustment method. However, it would be ideal to identify and eliminate sources of calibration error so that such an adjustment is not necessary. In our vaporizer, it is likely that microphysical, precipitation-based changes to the geometry of the vaporizer chamber lead to incomplete vaporization and impact the
420 calibration as precipitation builds up within the vaporizer over time. When there is clear evidence of inconsistent vaporization (as in Fig. 3), we observe large calibration errors in $\Delta^{17}\text{O}$ by this method (10s to 100s of per meg). Such issues likely also influence the vaporization process in other CFA systems, though they will not be readily detected in measurements of $\delta^{18}\text{O}$ or δD .

Finally, though it is perhaps impractical to measure replicate ice core samples as we have done here, the average of our nine
425 CFA-CRDS measurements shows that, like dual-inlet IRMS operations, stacking the CFA-CRDS data effectively averages over calibration inconsistencies. The results are comparable to highly resolved discrete CRDS or IRMS measurements.

6 Summary

We measured $\Delta^{17}\text{O}$ in nine replicate ice core samples using a continuous flow analysis (CFA) system combined with a cavity-ring down laser spectrometer (CRDS). We measured a tenth replicate sample by discrete CRDS methods. We show that CFA-
430 CRDS can reliably capture cm-scale variability of $\Delta^{17}\text{O}$ in ice core samples; we measured seasonal fluctuations of ~ 45 per

meg in $\Delta^{17}\text{O}$ from an ice core representing the preindustrial period in Greenland that agree with the discrete CRDS data and also with previously published measurements of seasonal $\Delta^{17}\text{O}$ variability in Greenland.

435 While CFA-CRDS measurements resolved to the cm scale still require long measurement times to achieve precise $\Delta^{17}\text{O}$ data, our work shows that leveraging this measurement technique can be valuable when high-precision and highly resolved measurements are desired. Achieving long measurement times while maintaining high depth resolution typically necessitates a reduction of melt rates. In practice, reduced melt rates may be incompatible with other measurement goals (such as trace gases) during an ice core measurement campaign; reduced melt rates may also prevent the measurement of both ice core samples and calibration standards within a period of stable system operations. Our results demonstrate that stacking multiple CFA-CRDS measurements provides a viable alternative strategy.

440 Our results show that mixing within the CFA system does not jeopardize CFA-CRDS measurements of $\Delta^{17}\text{O}$, even at cm-scale resolution. The mean of our stacked measurements exhibits neither a time lag nor any amplitude smoothing in comparison to the discretely prepared CRDS measurements. Rather, we show that the total error (~ 5 per meg) is dominated by dependency on the calibration intercept. We note the importance of developing robust calibration strategies for $\Delta^{17}\text{O}$ when making measurements by CFA-CRDS, but we demonstrate that when calibration is accounted for, CFA-CRDS for $\Delta^{17}\text{O}$ is highly
445 reproducible and can be tailored for high-resolution and high-precision measurements of $\Delta^{17}\text{O}$

450

455

References

- Allan, D.: Statistics of atomic frequency standards, *Proc IEEE*, 52, 221, 1966.
- Angert, A., Cappa, C. D., & DePaolo, D. J.: Kinetic ^{17}O effects in the hydrologic cycle: Indirect evidence and implications. *Geochimica et Cosmochimica Acta*, 68, 3487–3495. <https://doi.org/10.1016/j.gca.2004.02.010>, 2004.
- 460 Aron, P. G., Levin, N. E., Beverly, E. J., Huth, T. E., Passey, B. H., Pelletier, E. M., Poulsen, C. J., Winkelstern, I. Z., and Yarian, D. A.: Triple oxygen isotopes in the water cycle, *Chemical Geology*, 565, 120026. <https://doi.org/10.1016/j.chemgeo.2020.120026>, 2021.
- Barkan, E., and Luz, B.: High precision measurements of $^{17}\text{O}/^{16}\text{O}$ and $^{18}\text{O}/^{16}\text{O}$ ratios in H_2O , *Rapid Commun. in Mass Spectrom.*, 19, 3737–3742, <https://doi.org/10.1002/rcm.2250>, 2005.
- 465 Barkan, E., and Luz, B.: Diffusivity fractionations of $\text{H}_2^{16}\text{O}/\text{H}_2^{17}\text{O}$ and $\text{H}_2^{16}\text{O}/\text{H}_2^{18}\text{O}$ in air and their implications for isotope hydrology. *Rapid Commun. in Mass Spectrom.*, 21, 2999–3005, <https://doi.org/10.1002/rcm.3180>, 2007.
- Berman, E.S.F., Levin, N.E., Landais, A., Li, S., and Owano, T.: Measurement of $\delta^{18}\text{O}$, $\delta^{17}\text{O}$, and ^{17}O -excess in water by Off-Axis Integrated Cavity Output Spectroscopy and Isotope Ratio Mass Spectrometry. *Analytical Chemistry*, 85, 10392–10398, <https://doi.org/10.1021/ac402366t>, 2013.
- 470 Bigler, M., Svensson, A., Kettner, E., Vallenga, P., Nielsen, M. E., & Steffensen, J. P.: Optimization of High-Resolution Continuous Flow Analysis for Transient Climate Signals in Ice Cores, *Environmental Science & Technology*, 45, 4483–4489. <https://doi.org/10.1021/es200118j>, 2011.
- Dibb, J.E. and Fahnestock, M.: Snow accumulation, surface height change, and firn densification at Summit, Greenland: Insights from 2 years of in situ observation, *Journal of Geophysical Research*, 109, 0148–0227, <https://doi.org/10.1029/2003JD004300>, 2004.
- 475 Dansgaard, W.: Stable isotopes in precipitation, *Tellus*, 16, 436–468, <https://doi.org/10.1111/j.2153-3490.1964.tb00181.x>, 1964.
- Emanuelsson, B. D., Baisden, W. T., Bertler, N. A. N., Keller, E. D., and Gkinis, V.: High-resolution continuous-flow analysis setup for water isotopic measurement from ice cores using laser spectroscopy, *Atmospheric Measurement*
- 480 *Techniques*, 8, 2869–2883, <https://doi.org/10.5194/amt-8-2869-2015>, 2015.
- Gkinis, V., Popp, T. J., Johnsen, S. J., and Blunier, T.: A continuous stream flash evaporator for the calibration of an IR cavity ring-down spectrometer for the isotopic analysis of water, *Isotop. Environ. Health Stud.*, 46, 463–475, 2010.
- Gkinis, V., Popp, T. J., Blunier, T., Bigler, M., Schüpbach, S., Kettner, E., and Johnsen, S. J.: Water isotopic ratios from a continuously melted ice core sample, *Atmos. Meas. Tech.*, 4, 2531–2542, doi:10.5194/amt-4-2531-2011, 2011.
- 485 Gkinis, V., Simonsen, S. B., Buchardt, S. L., White, J. W. C., and Vinther, B. M.: Water isotope diffusion rates from the NorthGRIP ice core for the last 16,000 years-Glaciological and paleoclimatic implications, *Earth Planet. Sc. Lett.*, 405, 132–141, 2014.

- Hastings, M. G., Jarvis, J. C., and Steig, E. J.: Anthropogenic Impacts on Nitrogen Isotopes of Ice core Nitrate. *Science*, 324, 5932, 1288–1288, <https://doi.org/10.1126/science.1170510>, 2009.
- 490 Hawley, R. L., Morris, E. M., & McConnell, J. R.: Rapid techniques for determining annual accumulation applied at Summit, Greenland. *Journal of Glaciology*, 54, 839–845. <https://doi.org/10.3189/002214308787779951>, 2008.
- Hawley, R. L., Neumann, T. A., Stevens, C. M., Brunt, K. M., and Sutterly, T. C.: Greenland Ice Sheet elevation change: Direct observation of process and attribution at summit, *Geophysical Research Letters*, 47, <https://doi.org/10.1029/2020GL088864>, 2020.
- 495 Iannone, R. Q., Romanini, D., Cattani, O., Meijer, H.A.J., and Kerstel, E.R.T.: Water isotope ratio (d2H and d18O) measurements in atmospheric moisture using an optical feedback cavity enhanced absorption laser spectrometer, *J. Geophys. Res.*, 115, D10111, <https://doi.org/10.1029/2009JD012895>, 2010.
- Jones, T. R., White, J. W. C., Steig, E. J., Vaughn, B. H., Morris, V., Gkinis, V., Markle, B. R., and Schoenemann, S. W.: Improved methodologies for continuous-flow analysis of stable water isotopes in ice cores, *Atmospheric Measurement Techniques*, 10 617–632, <https://doi.org/10.5194/amt-10-617-2017>, 2017.
- 500 Jones, T. R., Cuffey, K. M., White, J. W. C., Steig, E. J., Buizert, C., Markle, B. R., McConnell, J. R., and Sigl, M.: Water isotope diffusion in the WAIS Divide ice core during the Holocene and last glacial, *Journal of Geophysical Research: Earth Surface*, 122, 290–309, <https://doi.org/10.1002/2016JF003938>, 2017b.
- Jouzel, J. and Merlivat, L.: Deuterium and oxygen 18 in precipitation: Modeling of the isotopic effects during snow formation, *J. Geophys. Res.-Atmos.*, 89, 11749–11757, <https://doi.org/10.1029/JD089iD07p11749>, 1984.
- Jouzel, J., Froehlich, K., and Schotterer, U.: Deuterium and oxygen-18 in present-day precipitation: Data and modelling, *Hydrological Sciences Journal*, 42, 747–763, <https://doi.org/10.1080/02626669709492070>, 1997.
- Kahle, E. C., Holme, C., Jones, T. R., Gkinis, V., and Steig, E. J.: A Generalized Approach to Estimating Diffusion Length of Stable Water Isotopes From Ice-Core Data, *Journal of Geophysical Research: Earth Surface*, 123, 2377–2391. <https://doi.org/10.1029/2018JF004764>, 2018.
- 510 Kahle, E. C., Steig, E. J., Jones, T. R., Fudge, T. J., Koutnik, M. R., Morris, V. A., Vaughn, B. H., Schauer, A. J., Stevens, C. M., Conway, H., Waddington, E. D., Buizert, C., Epifanio, J., and White, J. W. C.: Reconstruction of Temperature, Accumulation Rate, and Layer Thinning From an Ice Core at South Pole, Using a Statistical Inverse Method, *Journal of Geophysical Research: Atmospheres*, 126, <https://doi.org/10.1029/2020JD033300>, 2021.
- 515 Kerstel, E. R. T., van Trigt, R., Dam, N., Reuss, J., and Meijer, H. A. J.: Simultaneous determination of the 2H / 1H, 17O / 16O and 18O / 16O isotope abundance ratios in water by means of laser spectrometry, *Anal. Chem.*, 71, 5297–5303, 1999.
- Landais, A., Barkan, E., and Luz, B.: Record of $\delta^{18}\text{O}$ and ^{17}O -excess in ice from Vostok Antarctica during the last 150,000 years, *Geophys. Res. Lett.*, 35, 2, L02709, doi: [10.1029/2007GL032096](https://doi.org/10.1029/2007GL032096), 2008.

- 520 Landais, A., Ekaykin, A., Barkan, E., Winkler, R., and Luz, B.: Seasonal Variations of ^{17}O -Excess and d -Excess in Snow
Precipitation at Vostok Station, East Antarctica, *J. Glaciol.*, 58, 210, 725–733,
<https://doi.org/10.3189/2012JoG11J237>, 2012.
- Landais, A., Steen-Larsen, H. C., Guillevic, M., Masson-Delmotte, V., Vinther, B., and Winkler, R.: Triple isotopic
composition of oxygen in surface snow and water vapor at NEEM (Greenland), *Geochimica et Cosmochimica Acta*,
525 77, 304–316, <https://doi.org/10.1016/j.gca.2011.11.022>, 2012b.
- Luz, B., & Barkan, E.: Variations of $^{17}\text{O}/^{16}\text{O}$ and $^{18}\text{O}/^{16}\text{O}$ in meteoric waters, *Geochimica et Cosmochimica Acta*, 74, 6276–
6286, <https://doi.org/10.1016/j.gca.2010.08.016>, 2010.
- Merlivat, L., and Jouzel, J.: Global climatic interpretation of the deuterium-oxygen 18 relationship for precipitation, *Journal
of Geophysical Research*, 84, 5029, <https://doi.org/10.1029/JC084iC08p05029>, 1979.
- 530 Meese, D. A., Gow, A. J., Grootes, P., Stuiver, M., Mayewski, P. A., Zielinski, G. A., Ram, M., Taylor, K. C., & Waddington,
E. D.: The Accumulation Record from the GISP2 Core as an Indicator of Climate Change Throughout the Holocene,
Science, 266, 1680–1682, <https://doi.org/10.1126/science.266.5191.1680>, 1994.
- Schauer, A.J., Schoenemann, S.W., and Steig, E.J.: Routine High-Precision Analysis of Triple Water-Isotope Ratios Using
Cavity Ring-down Spectroscopy, *Rapid Commun. Mass Spectrom.*, 30, 18, 2059–2069, 2016.
- 535 Schoenemann, S.W., Schauer, A.J., and Steig, E.J.: Measurement of SLAP2 and GISP $\delta^{17}\text{O}$ and proposed VSMOW-SLAP
normalization for $\delta^{17}\text{O}$ and ^{17}O excess, *Rapid Commun. Mass Spectrom.*, 27, 582, 2013.
- Schoenemann, S. W., Steig, E. J., Ding, Q., Markle, B. R., and Schauer, A. J.: Triple water-isotopologue record from WAIS
Divide, Antarctica: Controls on glacial-interglacial changes in ^{17}O excess of precipitation: WAIS LGM-Holocene
 ^{17}O excess Record, *Journal of Geophysical Research: Atmospheres*, 119, 14, 8741–8763,
540 <https://doi.org/10.1002/2014JD021770>, 2014.
- Schoenemann, S. W., and Steig, E. J.: Seasonal and spatial variations of ^{17}O excess and d excess in Antarctic precipitation: Insights
from an intermediate complexity isotope model, *Journal of Geophysical Research: Atmospheres*, 121,
<https://doi.org/10.1002/2016JD025117>, 2016.
- Steen-Larsen, H. C., Masson-Delmotte, V., Sjolte, J., Johnsen, S. J., Vinther, B. M., Bréon, F.-M., Clausen, H. B., Dahl-Jensen,
545 D., Falourd, S., Fettweis, X., Gallée, H., Jouzel, J., Kageyama, M., Lerche, H., Minster, B., Picard, G., Punge, H. J.,
Risi, C., Salas, D., Schwander, J., Steffen, K., Sveinbjörnsdóttir, A. E., Svensson, A., and White, J.: Understanding
the Climatic Signal in the Water Stable Isotope Records from the NEEM Shallow Firn/Ice Cores in Northwest
Greenland., *J. Geophys. Res.*, 116, D6, D06108, <https://doi.org/10.1029/2010JD014311>, 2011.
- Steen-Larsen, H. C., Masson-Delmotte, V., Hirabayashi, M., Winkler, R., Satow, K., Prié, F., Bayou, N., Brun, E., Cuffey, K.
550 M., Dahl-Jensen, D., Dumont, M., Guillevic, M., Kipfstuhl, S., Landais, A., Popp, T., Risi, C., Steffen, K., Stenni,
B., & Sveinbjörnsdóttir, A. E.: What controls the isotopic composition of Greenland surface snow? *Climate of the
Past*, 10, 377–392. <https://doi.org/10.5194/cp-10-377-2014>, 2014.

- 555 Steig, E.J., Gkinis, V., Schauer, A.J., Schoenemann, S.W., Samek, K., Hoffnagle, J., Dennis, K.J., and Tan, S.M.: Calibrated high-precision ^{17}O -excess measurements using cavity ring-down spectroscopy with laser-current-tuned cavity resonance, *Atmos. Meas. Tech.*, 7, 2421, 2014.
- Steig, E. J., Jones, T. R., Schauer, A. J., Kahle, E. C., Morris, V. A., Vaughn, B. H., Davidge, L., and White, J. W. C.: Continuous-Flow Analysis of $\delta^{17}\text{O}$, $\delta^{18}\text{O}$, and δD of H_2O on an Ice Core from the South Pole, *Frontiers in Earth Science*, 9, 640292, <https://doi.org/10.3389/feart.2021.640292>, 2021.
- 560 Tian, C., Wang, L., and Novick, K. A.: Water vapor $\delta^2\text{H}$, $\delta^{18}\text{O}$ and $\delta^{17}\text{O}$ measurements using an off-axis integrated cavity output spectrometer – sensitivity to water vapor concentration, delta value and averaging-time. *Rapid Communications in Mass Spectrometry*, 30, 2077–2086, <https://doi.org/10.1002/rcm.7714>, 2016.
- Uemura, R., Barkan, E., Abe, O., and Luz, B.: Triple isotope composition of oxygen in atmospheric water vapor: the ^{17}O -excess of water vapor, *Geophysical Research Letters*, 37, L04402, <https://doi.org/10.1029/2009GL041960>, 2010.
- 565 Werle, P., Mücke, R., & Slemr, F.: The limits of signal averaging in atmospheric trace-gas monitoring by tunable diode-laser absorption spectroscopy (TDLAS). *Applied Physics B Photophysics and Laser Chemistry*, 57(2), 131–139. <https://doi.org/10.1007/BF00425997>, 1993.


570

575


580

585


Figures and Tables

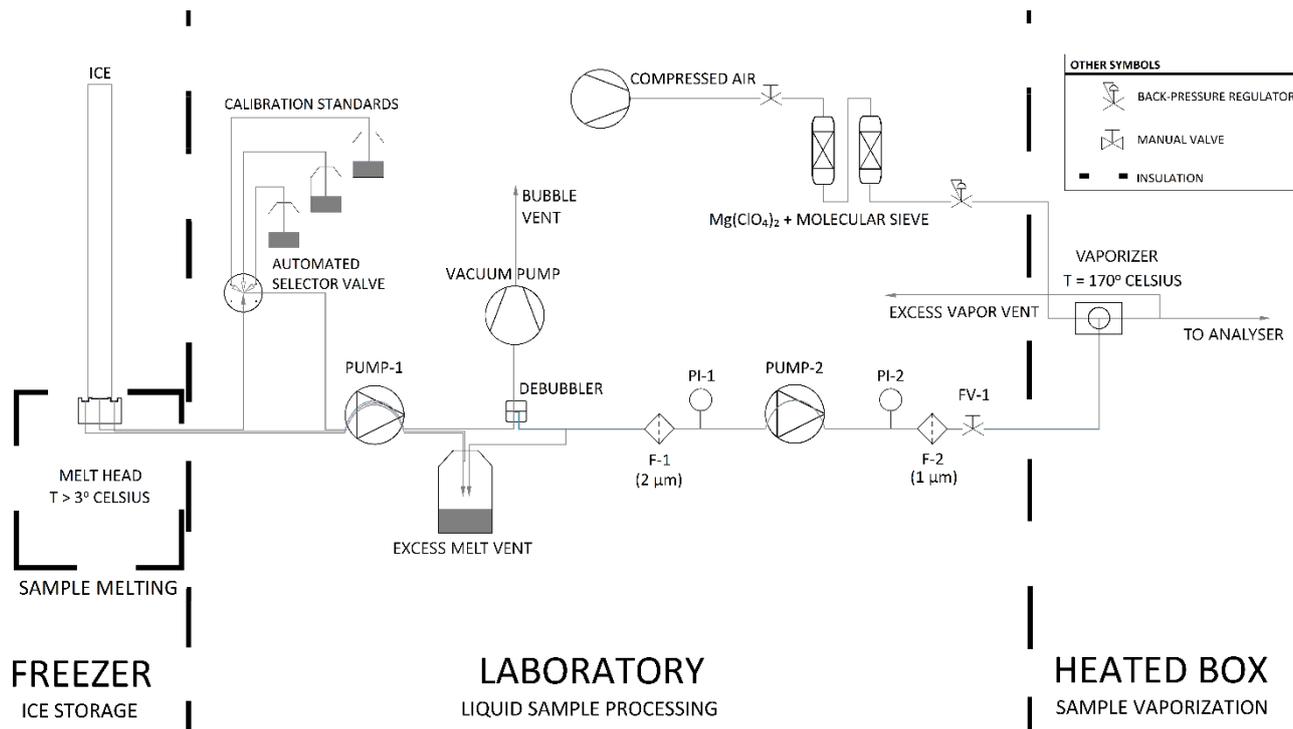


590 **Figure 1: Process flow diagram for our CFA system. Thick dashed lines indicate transitions between temperature-controlled process spaces. Note that F-1 and F-2 are filters, PI-1 and PI-2 are pressure sensors, and FV-1 is a flow valve.**

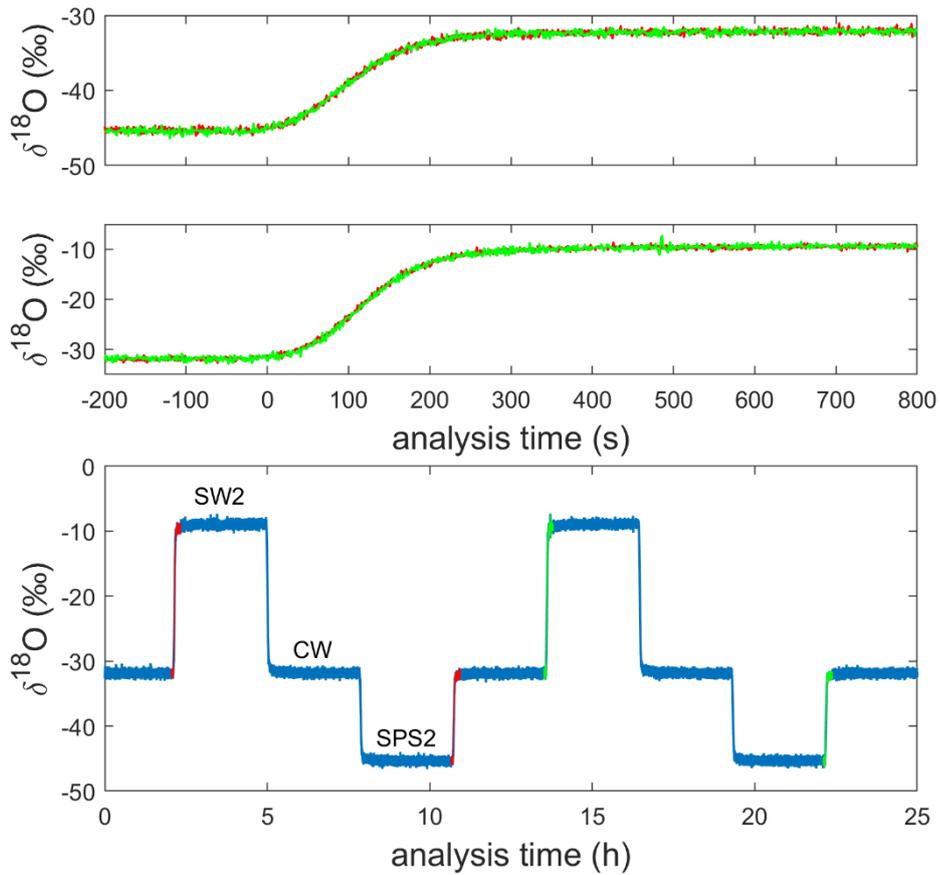


595 **Figure 2: Uncalibrated, 1-Hz measurements of $\delta^{18}\text{O}$ for the alternating sequence of reference waters during a full analysis day (bottom). The 200 s preceding and 800 s following four reference water transitions are shown in the other panels; two transitions (shown in orange and green) from SPS2 to CW are stacked in the top panel and two transitions from CW to SW2 are stacked in the middle panel.**

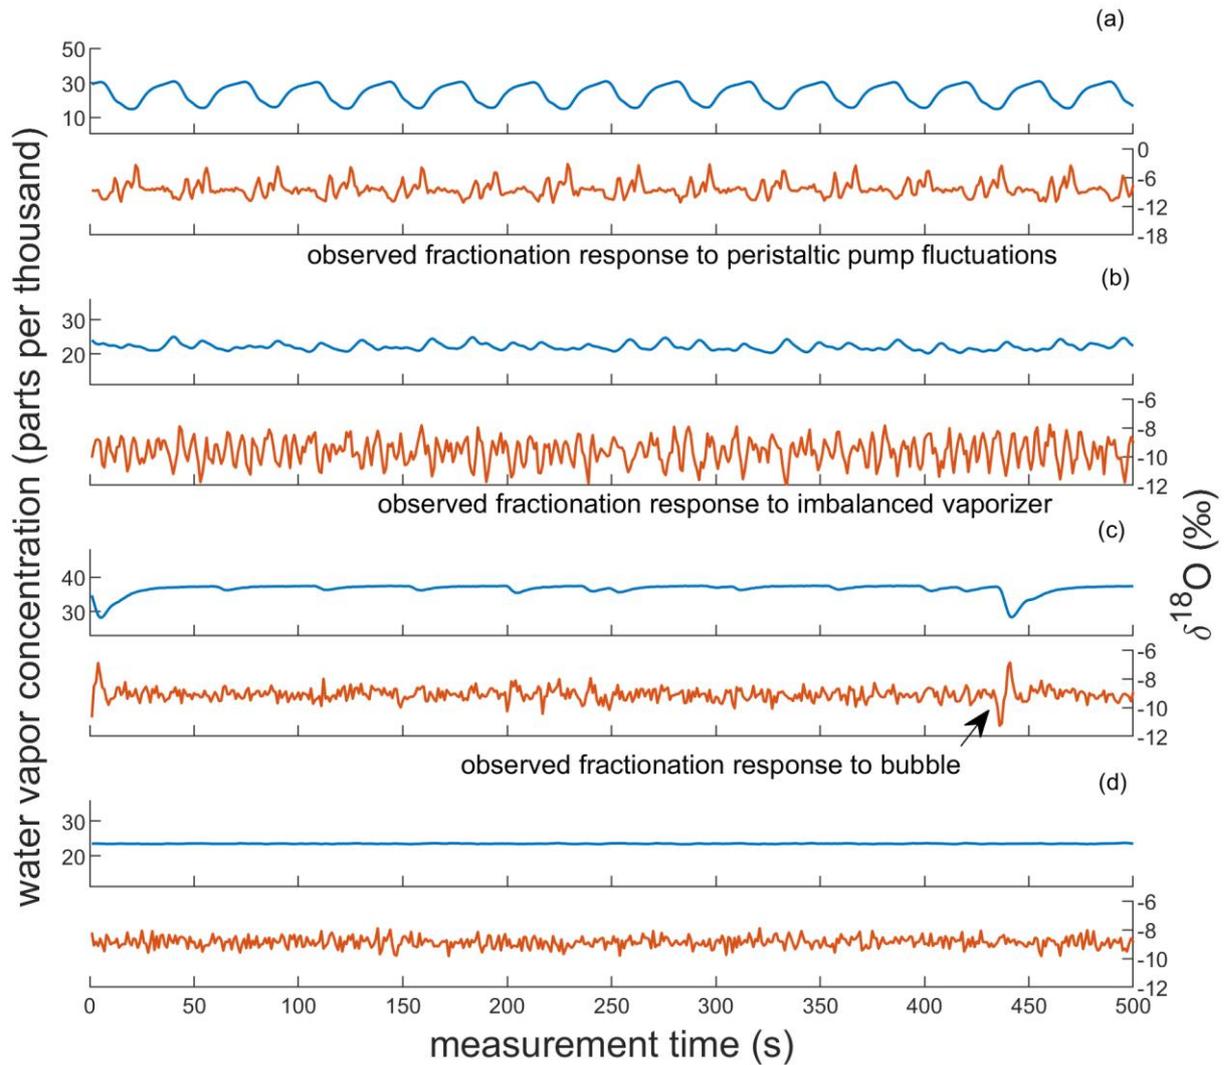


600 **Figure 3: Observations of vapor quality as real-time indicators of vaporizer performance. Each subplot shows corresponding**
observations indicative of imbalanced vaporizer conditions for large and small pressure imbalances, respectively. (A) and (B) show
observations indicative of acceptable vaporizer performance. Though both include low-variability observations of $\delta^{18}\text{O}$ ($\sigma < 0.3$ ‰)
and of water vapor concentration, (C) also includes microbubble interruptions at the vaporizer (e.g., at 5 and 440 s). (D) indicates
605 **optimal vaporizer performance. Note that the vertical scaling of (A) is different from the other panels.**

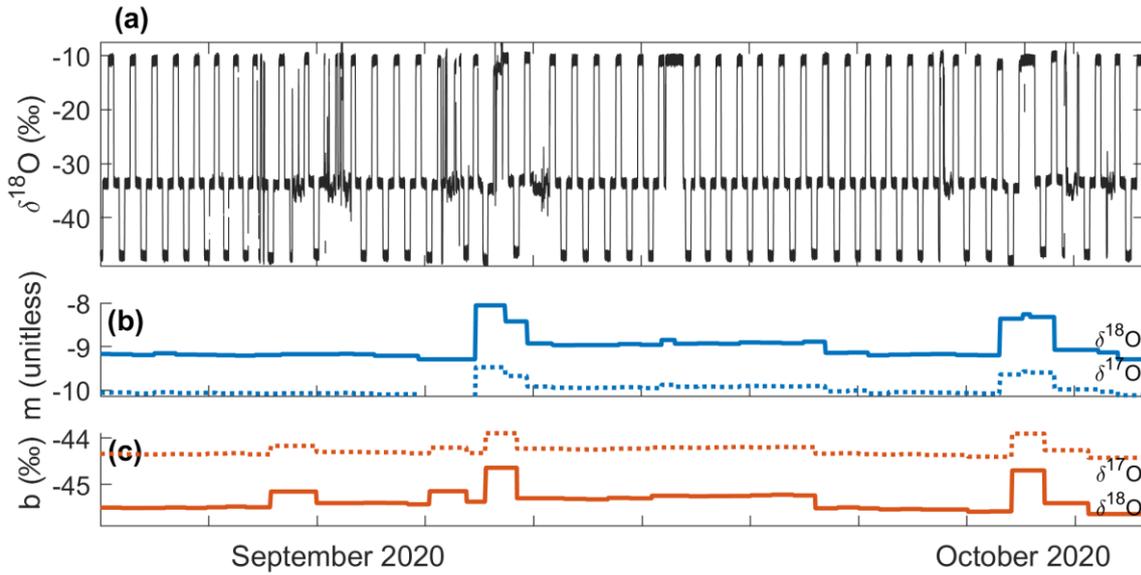


610 **Figure 4: Complete measurement sequence and the calibration data resulting from measurements of SW2 and SPS2. (A) shows the $\delta^{18}\text{O}$ of all measurements, including SW2, CW, SPS2, and ice core data. (B) and (C) show the calibration slope (m) and intercept (b), respectively, for both $\delta^{18}\text{O}$ and $\delta^{17}\text{O}$. Note that the intercept of $\delta^{17}\text{O}$ is shifted by -15 ‰ in this plot for legibility.**

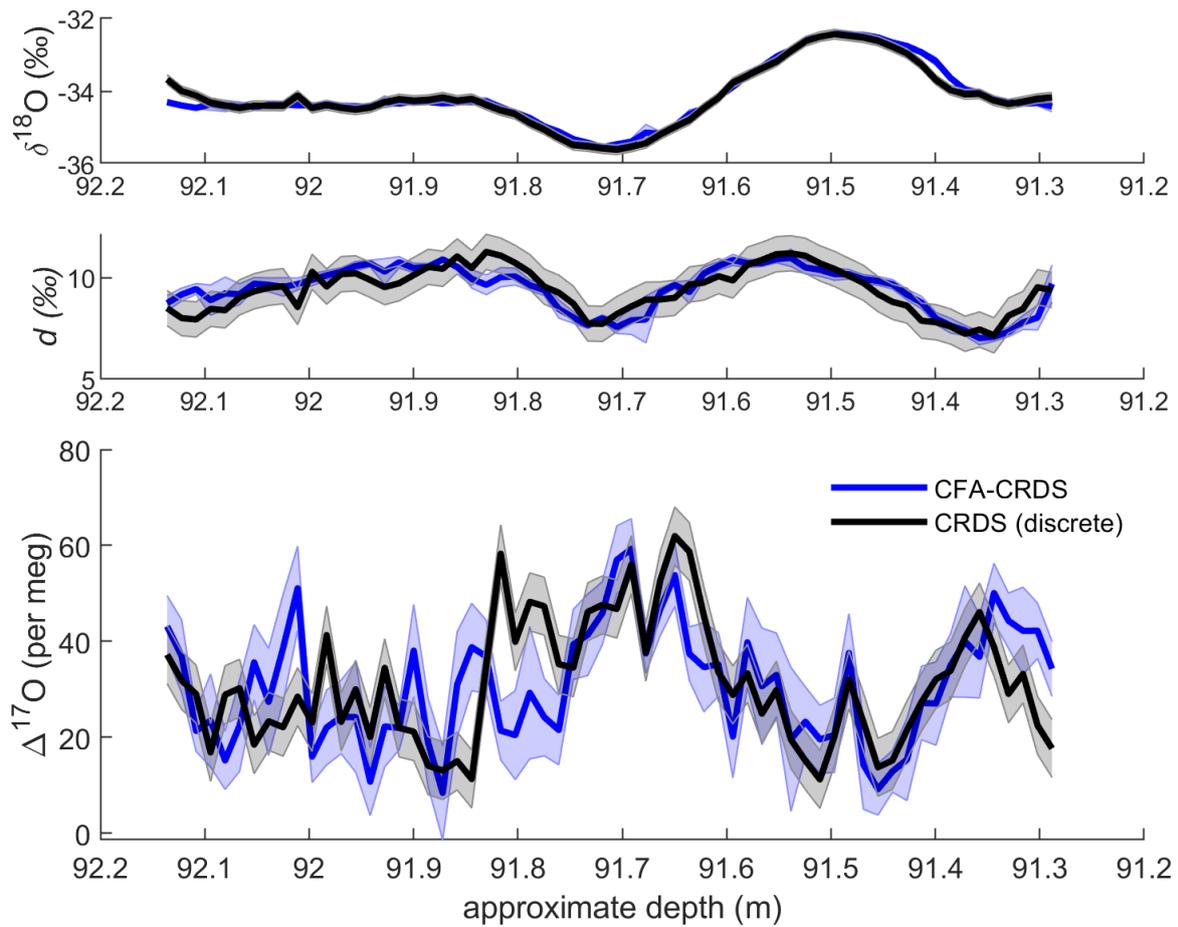

615 **Figure 5: Comparison of discrete CRDS ice core measurements (black) with calibrated CFA-CRDS data averaged over 1.39-cm intervals (blue). Corresponding $\delta^{18}\text{O}$ and d data are shown for seasonal context. Discrete CRDS measurements are shown with the root mean square error of corresponding reference water measurements (grey shading), and CFA-CRDS measurements are shown as the mean of nine measurements with the standard error (blue shading).**

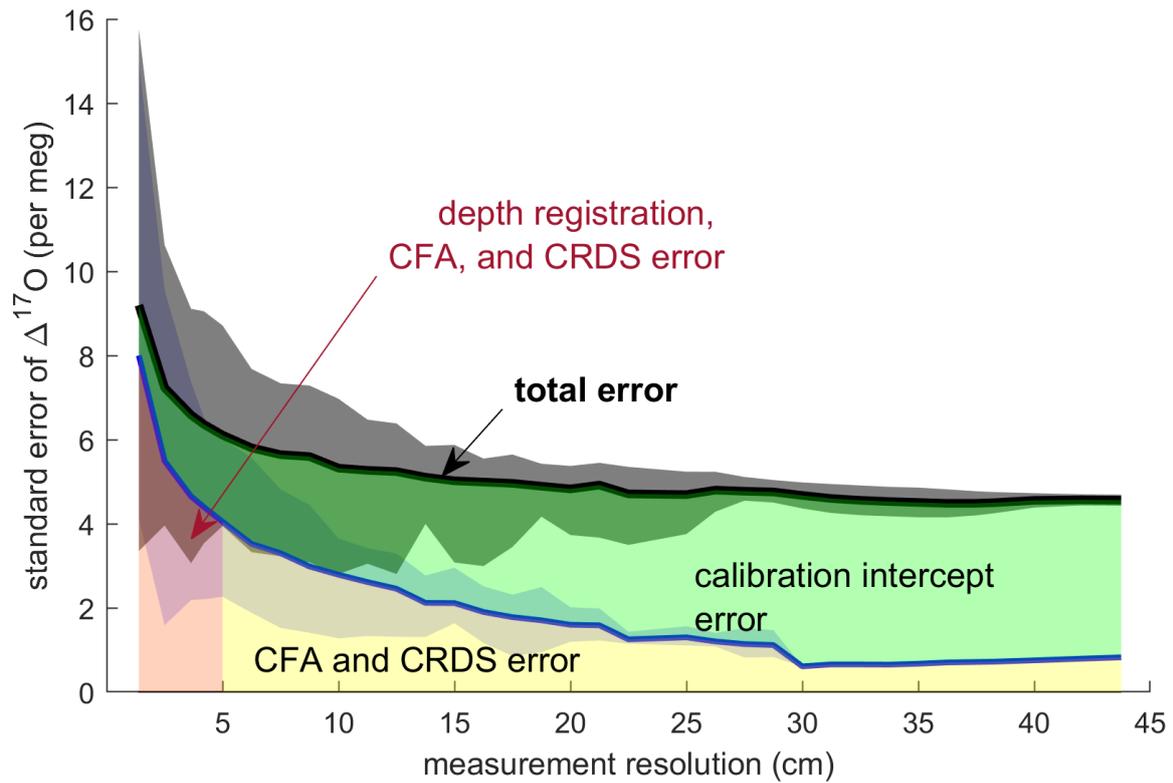

620 **Figure 6: Standard error of all replicate CFA measurements by measurement integration depth. The black line shows the mean of the standard error as calculated for each depth interval; the shaded area indicates the minimum and maximum values of the standard error across all depth intervals. The blue line shows the relationship between the standard error in mean-shifted values and the measurement resolution. The area beneath the total error line is highlighted to indicate error attribution.**

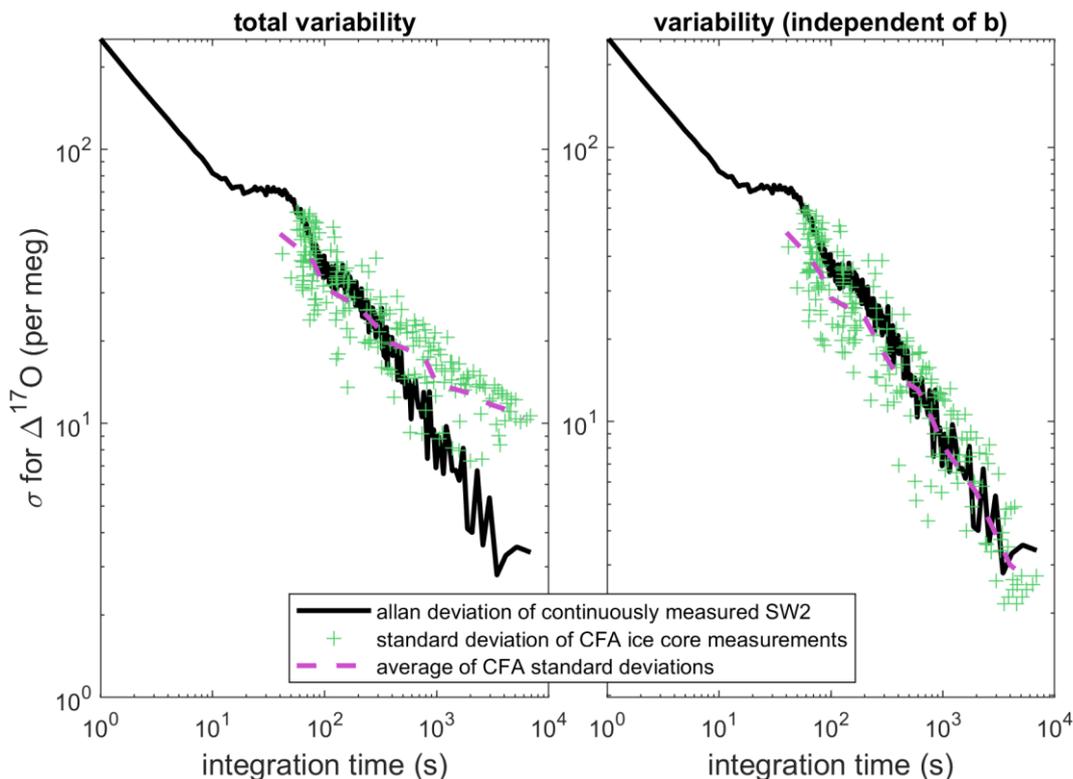

625 **Figure 7: Comparison of Allan deviation of continuous reference water measurements and standard deviation of nine duplicate CFA**
ice core measurements. In both left and right images, the Allan deviation line (black) for a long measurement of SW2 is overlain by
the standard deviation of the CFA-CRDS ice core measurements (green) and the mean of the standard deviations for each integration
time (pink). The standard deviation on the left is calculated from calibrated replicate CFA-CRDS measurements and shows the total
variability between CFA-CRDS replications along the depth of the core. The standard deviation information in the right plot is
630 **calculated from the mean-shifted datasets so that the effect of the calibration intercept (b) is removed; this analysis is still dependent**
upon the calibration slope (m), CFA errors, depth registration errors, and natural variability within the core.

Reference water (origin location)	$\delta^{17}\text{O}$	$\delta^{18}\text{O}$	δD	d	$\Delta^{17}\text{O}$
		% vs. VSMOW			per meg vs. VSMOW
SW2 (Seattle)	-5.7107	-10.85	-77.96	8.84	33
CW (West Antarctica)	-17.8807	-33.64	-265.95	3.17	25
SPS2 (South Pole)	-25.1210	-47.07	-365.20	11.36	15

635 **Table 1: Isotopic values of reference waters. SW2 is Seattle deionized tap water; CW is melt water from the WDC06A core (i.e., West Antarctic Ice Sheet precipitation), and SPS2 is South Pole snow. These three waters were normalized to the VSMOW-SLAP scale using other in-house reference waters that were analyzed against VSMOW, SLAP, and GISP (see Schoenemann et al., 2013).**

Data Availability

Data generated for this study are available from the corresponding author upon reasonable request.

Author Contribution

640 EJS, AJS, and LD conceived of the study. LD developed the measurement method, made the measurements, and completed the analysis with the support of AJS and EJS. All authors contributed to the manuscript.

Competing Interests

The authors declare that they have no conflict of interest.

645