

Improving relative humidity measurements on Mars: New laboratory calibration measurements

Maria Hieta¹, Iina Jaakonaho¹, Jouni Polkko¹, Andreas Lorek², Stephen Garland², Jean-Pierre de Vera^{2,3}, Maria Genzer¹, and Ari-Matti Harri¹

¹Finnish Meteorological Institute, Erik Palmenin aukio 1, 00560 Helsinki, Finland

²Planetary Analog Simulation Laboratory (PASLAB), Deutsches Zentrum für Luft- und Raumfahrt e.V. (DLR), Rutherfordstraße 2, 12489 Berlin

³Space Operations and Astronaut Training, Microgravity User Support Center (MUSC), Geb. 29, Linder Höhe, 51147 Köln, Germany

Correspondence: Maria Hieta (maria.hieta@fmi.fi)

Abstract. In this paper we present new calibration measurements that have been performed with the ground reference models of the relative humidity instruments of the MSL, Mars 2020 and ExoMars missions. All instruments are based on capacitive sensor head technology, and they are developed, manufactured and tested by The Finnish Meteorological Institute (FMI). Calibration of capacitive humidity sensors for the Martian environment has been a challenging task and special facilities are needed in order to create Martian conditions including all relevant environmental parameters: low pressure, low temperature, carbon dioxide environment, and especially humidity that can be accurately controlled and measured. A measurement campaign was performed at DLR PASLAB (Planetary Analog Simulation Laboratory) determining relative humidity calibration data sets for REMS-H, MEDA HS and METEO-H instruments in temperatures from -30 °C down to -70 °C in low pressure CO₂. In addition to the stable point humidity calibration measurements in CO₂, the instrument performance was tested with the actual Martian atmosphere composition, and during long continuous measurements. The new calibration data set has already been used in the flight calibration of the MEDA HS instrument resulting in successful calibration and excellent accuracy. The results from this campaign will further improve relative humidity measurements on Mars by providing the means to reanalyse the current calibration of the REMS-H flight model, and by allowing more accurate comparison between the two instruments currently on the Martian surface.

15 *Copyright statement.* TEXT

1 Introduction

The Finnish Meteorological Institute (FMI) has provided atmospheric relative humidity (RH) instruments based on capacitive sensor heads for several Mars missions, the first operational one being REMS-H on board Curiosity rover (Figure 1) which landed on Mars in 2012. REMS-H was followed by MEDA HS on board Perseverance rover in 2021. Both instruments are still

20 active and producing daily readings of relative humidity. Relative humidity instruments have also been delivered for Mars-96
penetrators and small stations (Harri et al. (1998)), for DREAMS on board ExoMars 2016 Schiaparelli Entry, Descent and
Landing Demonstrator Module (EDM) (Esposito et al. (2018)) and for METEO on the ExoMars 2020 surface platform Kaza-
chok (Zelenyi et al. (2015)). The Mars-96 mission experienced a failure during launch, resulting in the loss of the mission, the
landing of Schiaparelli EDM was not successful, and the ExoMars 2020 mission was suspended in March 2022. The ExoMars
25 rover mission has been restarted but the landing platform will be a new development. In addition to the FMI instruments, only
the Phoenix lander has measured relative humidity directly on the Martian surface (Zent et al. (2009)).

Calibration of capacitive humidity sensors for the Martian environment has proven to be a challenging task. The capaci-
tive sensors, that have been used in all in situ measurements so far, are sensitive not only to relative humidity but also other
variables like temperature, low pressure and carbon dioxide (CO₂) (Harri et al. (2014), Lorek and Majewski (2018), [Tabandeh](#)
30 [Tabandeh and Högström \(2021\)](#)). Special facilities are needed in order to create Martian conditions including all relevant en-
vironmental parameters, and especially to control and measure the humidity inside the measurement chamber with sufficient
accuracy, limiting the existing test facilities. In addition, measurements at low temperatures take time because the stabilisation
of the measurement system can be slow. Typically, the calibration campaign for the flight model needs to find a balance be-
tween the schedule, test scope, and limitations such as cleanliness requirements, which can restrict the extent of any campaign.
35 In fact, previous missions have encountered diverse challenges during the calibration process. The original calibration range
of Phoenix TECP only partially overlapped with the actual operating conditions and the TECP was later re-calibrated using
an engineering model by Fischer et al. (2019). Curiosity's REMS-H returned too low relative humidity readings due to an
unknown transducer electronics artifact, and a calibration compensation was developed (Harri et al. (2014)) but without new
calibration measurements in a relevant environment. The original REMS-H calibration data was measured in ambient pressure
40 air and not in low pressure CO₂.

Building upon the experience from previous missions, a test program was planned for the humidity sensors from Mars
2020 and ExoMars 2020 using extensive ground reference model measurements to supplement the flight model calibration
(Hieta et al. (2022)). The actual flight models would go through only a simplified 2-point calibration in Martian conditions.
An appropriate facility for the supplementary ground reference measurements was identified as the DLR PASLAB (Planetary
45 Analog Simulation Laboratory). This facility is used for habitability-related experiments under Martian conditions and for
humidity sensor studies, for example by Lorek (2014) and Lorek and Majewski (2018).

In this work, we present the measurement campaign at DLR PASLAB and its results encompassing calibration measure-
ments of three relative humidity instruments. The main motivation for the campaign was supplementing the flight calibration
of the MEDA HS instrument on the Perseverance rover, whilst simultaneously gaining information and knowledge of the older
50 sensor type behaviour of the REMS-H instrument. The results of the measurement campaign presented in this paper regarding
the MEDA HS have already been summarised in Hieta et al. (2022) and the data set has been used in formulating the flight cali-
bration for MEDA HS. This paper will provide a more thorough description of the tests, provide equivalent results for REMS-H
and METEO-H, and provide new results of measurements in an accurate Martian gas mixture as well as characterisation of

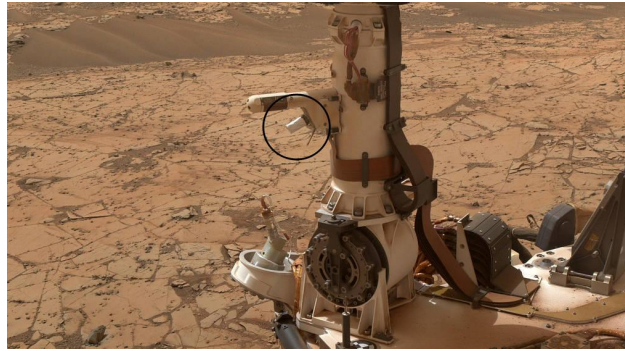


Figure 1. REMS-H attached to the mast of the Curiosity rover. Credits: NASA/JPL-Caltech/MSSS

MEDA HS self-heating during continuous measurements. The implications of these results concerning current REMS-H flight
55 calibration are beyond the scope of this paper but will be a topic of future work.

1.1 Scientific background

Despite Mars' atmosphere being extremely dry, water vapor still holds significant importance as one of the three main cycles that define the present climate of the planet, along with the cycles of CO₂ and dust. Understanding the Martian water cycle is of high scientific importance as it can provide insight into the history and evolution of the planet's climate, geology, and potential
60 for habitability. Furthermore, accurate measurements of water vapor in the Martian atmosphere can inform future missions to the planet, including the search for signs of past or present microbial life (e.g. Kappen et al. (1996), de Vera et al. (2013), Stevenson et al. (2014)).

Over a span of more than 50 years the combined observations from ground-based, satellite, and in situ measurements have provided us with a solid understanding of the current climate on Mars. Most of the water today exists as ice in the polar
65 caps and within the soil providing reservoirs for a planetary scale water cycle between the atmosphere and the polar cap areas. Strong seasonal variability is driven by water sublimating off of the north residual cap, producing the annual local maximum in atmospheric water vapor at high northern latitudes during summertime. The southern summer produces the opposite effect but with a significantly lower amplitude. This seasonal and latitudinal dependence has been known since the Viking era (e.g. Jakosky (1985)) and our understanding of the details of Martian water has inevitably advanced over time due
70 to more observations.

In situ observations have been reviewed by Martínez et al. (2017). They can provide detailed information about local conditions, atmospheric properties, and surface interactions, and support the orbital observations by providing the ground truth. Near-surface humidity measurements have been used in particular for studying the exchange processes between the atmosphere and the regolith (e.g. Jakosky et al. (1997), Savijärvi et al. (2016)), and for studying the potential for brine or ice formation
75 (e.g. Fischer et al. (2016), Martinez et al. (2015)). Furthermore, the significance of in situ atmospheric humidity measurements has been expanded through modeling activities conducted by e.g. Savijärvi et al. (2019) and Savijärvi et al. (2020).

This paper is structured as follows. Section 2 introduces the experimental method, related equations, the FMI's relative humidity instruments and the experimental setup. The campaign results are presented in Section 3. Section 4 explains how the data has been used to formulate the calibration equations for MEDA HS and how the calibrated readings in this paper have
80 been obtained. Section 5 provides conclusions and discussion of the results presented.

2 Experimental method

2.1 Humidity equations

The HUMICAP sensor heads measure relative humidity (RH). The relative humidity is normally expressed as a percentage, representing the amount of water vapor in the air at compared to the to the equilibrium amount (saturation) at that temperature:

$$85 \quad RH = \frac{e}{e_s} * 100\% \quad (1)$$

where e is the water vapor partial pressure in hPa and e_s is the saturation vapor pressure over ice in hPa. Relative humidity in this paper is calculated with respect to ice.

In order to calculate the water vapor volume mixing ratio (VMR), an equation for saturated water vapour pressure e_s over ice is needed. Several different equations exist for this purpose and we used the 1996 revision of the Buck equation (Buck
90 (1981)):

$$e_s = 6.1115 \exp\left(\left(23.036 - \frac{T}{333.7}\right)\left(\frac{T}{279.82 + T}\right)\right), \text{ over ice, } T < 0 \text{ } ^\circ\text{C} \quad (2)$$

where T is the air temperature in $^\circ\text{C}$. VMR in ppm in pressure p (hPa) is then obtained with equation:

$$vmr = e * 10^6 / (p - e) \quad (3)$$

The reference dew point hygrometer measures the dew or frost point of the gas, which can be converted to relative humidity
95 using equation (2).

2.2 FMI's relative humidity instruments

All the FMI's Martian relative humidity instruments are based on polymeric capacitive humidity sensor head technology, HUMICAP®, developed by a private company Vaisala Oyj (Hum (2020)), which makes use of read-out electronics placed in the vicinity of the humidity sensor heads on the same printed circuit board (PCB). A schematic view of the HUMICAP is
100 shown in Figure 2. The sensor heads have integrated heating resistors that are used periodically to regenerate the HUMICAPs, removing possible contaminants that can affect the capacitance, restoring the sensor head performance and correcting for

possible long-term drifts. The read-out electronics are based on an oscillator transducer that converts the output of the capacitive sensors into frequency. The capacitance of the channel is then obtained using the constant reference channels. The instruments contain 8 measurement channels which can include: 2 or 3 HUMICAP sensor heads, capacitive THERMOCAP® temperature
105 sensors, and reference and housekeeping capacitors. The transducer's active components and the multiplexer are implemented into a Vaisala proprietary ASIC (Application Specific Integrated Circuit). The humidity instruments are mounted outside the lander providing ventilation with the ambient atmosphere through a filter protecting the devices from airborne dust.

REMS-H (Figure 3 (a)) represents the first generation of FMI relative humidity sensors including three older type HUMICAP sensor heads. REMS (Rover Environmental Monitoring Station) is a suit of sensors on board the Curiosity rover that measures
110 various environmental parameters on the Martian surface and REMS-H is the sensor measuring relative humidity (Gomez-Elvira et al. (2012), Harri et al. (2014)). Curiosity rover landed at Gale crater in early August 2012 meaning that it has operated on the Martian surface for over 10 years providing valuable long time series of atmospheric measurements including relative humidity data (e.g. Savijärvi et al. (2019)). DREAMS-H of DREAMS (Dust Characterisation, Risk Assessment, and Environment Analyser on the Martian Surface) experiment on board ExoMars 2016 Schiaparelli (Esposito et al. (2018)) was
115 an almost exact copy of REMS-H except for some minor details in the PCB and mechanical design. Before the unsuccessful landing of the Schiaparelli module on Mars, the module's central computer activated the DREAMS instrument and sent back housekeeping data indicating that the DREAMS sensors were performing nominally.

MEDA HS (Figure 3 (b)) and the almost identical METEO-H are the next generation successors of REMS-H. MEDA HS is a relative humidity sensor for the Mars 2020 Perseverance rover and it has measured Martian atmosphere since landing
120 in February 2021 (Rodriguez-Manfredi et al. (2021), Rodriguez-Manfredi et al. (2023), Hieta et al. (2022), Polkko et al. (2023)). METEO-H was delivered for the ExoMars 2020 surface platform but cooperation with Roscosmos on the ExoMars mission has since been terminated. Both MEDA HS and METEO-H are based on next generation HUMICAP sensor heads. The new HUMICAP sensor head has the same polymer and operating principle as the one used in REMS-H, but incorporates several improvements: the sensor heads have a significantly larger dynamic range, faster response time and they include on-
125 chip temperature measurement with Pt1000 platinum resistance temperature sensors. Pt1000 sensors are read directly by the MEDA Instrument Control Unit (ICU). The integrated temperature sensor allows calculation of humidity values with respect to the actual sensor head temperature instead of the PCB board temperature. MEDA HS and METEO-H include two HUMICAP sensor heads and a revised selection of reference and housekeeping channels, as well as two board-mounted THERMOCAP temperature channels. The MEDA HS PCB is shown in Figure 4.

130 Each ground reference model (REF) of these relative humidity instruments is as similar to the flight model as possible, and they have been kept at the Finnish Meteorological Institute for calibration or performance testing. All REF models were regenerated before the measurement campaign. The REF models have been manufactured and tested together with the actual flight models but have not gone through environmental qualification or acceptance tests to avoid stressing the instruments.



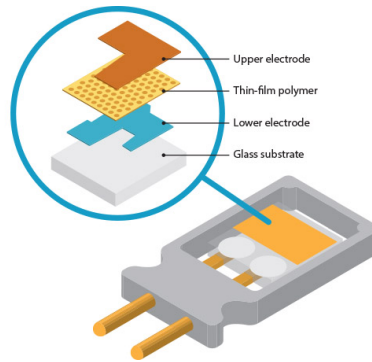


Figure 2. Schematic view of the HUMICAP sensor head. A thin film of active polymer is deposited between two conductive electrodes on top of a substrate. (Hum (2020)).

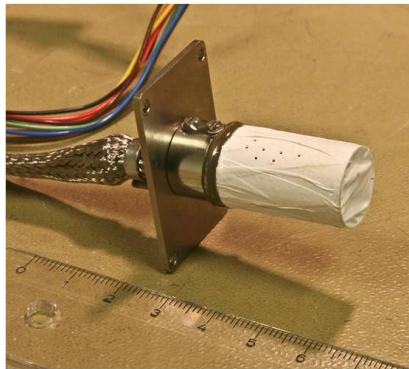

(a)

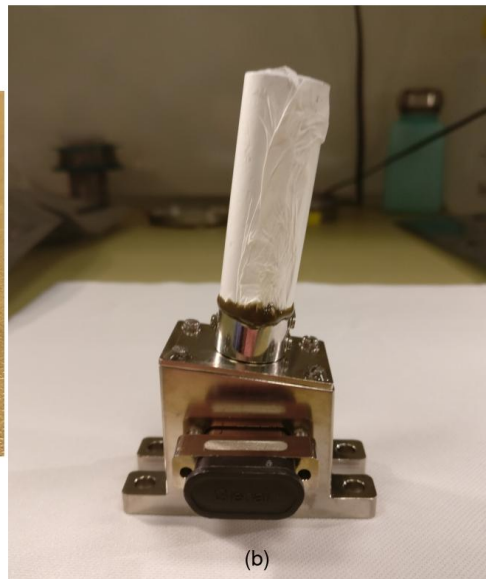

(b)

Figure 3. REMS-H flight model (a) and MEDA HS flight model (b) inside FMI's clean room. The white perforated PTFE filter around the cylindrical Faraday cage protects the instrument from atmospheric dust. MEDA HS is shown in flight configuration with complete mechanics, but during the DLR test campaign the large housing box for mounting the instrument was not installed on the REF model. METEO-H is almost identical to MEDA HS, except that the top of the housing box is not slanted.

2.3 Experimental setup

135 The results presented in this publication were obtained using the sensor calibration facility of PASLAB (Planetary Analog Simulation Laboratory) at the Institute for Planetary research at the German Aerospace Center (DLR) in Berlin. The laboratory is used for habitability-related experiments under Martian conditions as well as humidity sensor studies (Lorek and Koncz

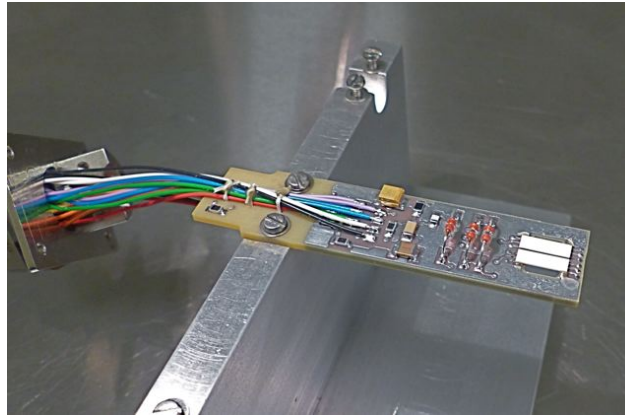


Figure 4. MEDA HS PCB without the mechanics. The HUMICAP sensor heads are facing downwards through a hole in the PCB.

(2013)). Similar sensor studies have been performed previously by Lorek and Majewski (2018) and Lorek (2014). A schematic diagram of the setup is shown in Figure 5. At the core of the setup is a temperature control chamber, KWP240, capable of
140 regulating the temperature inside the chamber in the range -75 to $+130$ °C. The chamber has two ports, one on the left and one on the right, through which cables, gas inlet and vacuum tubing can be laid. It was considered critically important that all the instruments see the same conditions at the same time during the campaign in order to ensure equal calibration for all and to allow comparison between the instruments. For this purpose, a single test chamber including all three instruments was designed. The same chamber has been used previously in FMI for testing relative humidity instruments but for the first time it
145 was modified to house three sensors of different missions with slightly different dimensions and interfaces. Figure 6 shows the instruments placed inside the test chamber facing towards the middle. The gas flow through the chamber across each sensor is equal. A small sized Pt100 temperature sensor was also included in the chamber to measure the temperature independently of the instruments. In addition to the three humidity sensors from the FMI, a series of Sensirion SHT-85 relative humidity sensors from the DLR were installed in a parallel chamber. The results of these measurements will be presented in a separate
150 publication.

The gas composition was generated using the gas mixing system indicated in Figure 5 and the pressure in the chamber was controlled using a vacuum pump. It consists of a gas humidification system where part of the matrix gas, in this case CO_2 is diverted and dispersed in a bottle containing distilled water, thus obtaining close to 100% humidity. This humidified CO_2 is then mixed with CO_2 directly from the gas bottle (99.995% CO_2), at approximately -65 °C frost point, using precision EI-flow Select
155 mass flow controllers from the company Bronkhorst High-Tech B.V. Nine controllers were used for this experiment, allowing control of gas flow down to 0.014 mln/min (milliliter normal per minute) and guaranteeing precise humidity generation over the full range of required humidities with a stability of ± 0.1 °C. Correction factors can be applied to the controllers for a variety of gases, including CO_2 . The humidity generated by the gas mixing system can be estimated to a precision of the order of 1 or 2 °C frost point, however to obtain the high precision necessary for sensor calibration experiments part of the outgoing gas flow was
160 diverted to a dew point mirror (MBW 373) to measure directly the humidity to a precision of 0.1 °C frost point. With knowledge

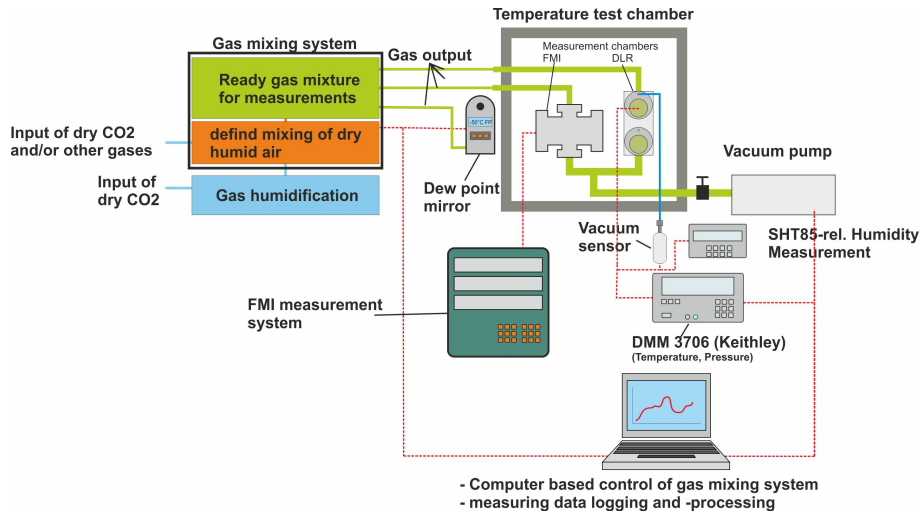


Figure 5. Test setup for the FMI sensors at DLR. The measurement chamber (Figure 6) including all three instruments was placed inside a temperature test chamber and connected to the gas mixing system and the vacuum pump. Part of the gas mixing system output was diverted to a reference dew point mirror.

of the atmospheric pressure and the pressure inside the measurement chamber, the humidity in the measurement chamber can be calculated. A paper analysing MEDA HS instrument uncertainty and also including the error on the humidity measurement has been written by Tabandeh et al [Tabandeh and Högstöm \(2021\)](#). The expanded uncertainty ($k=2$) of the Pt100 sensor inside the chamber is equal to or better than $0.18\text{ }^{\circ}\text{C}$, and for the MEDA HS Pt1000 sensors the expanded uncertainty is equal to or better than $0.22\text{ }^{\circ}\text{C}$. The chamber pressure measurement has an expanded uncertainty of approximately 14 to 17 Pa, while the atmospheric pressure measurement has an expanded uncertainty of 400 Pa.

The entire climate simulation system was controlled using LabVIEW software, allowing automated generation of humidity and pressure control. In addition, the software was used to log data from the climate chamber, dew point mirror, vacuum pump and the relative humidity sensors from the DLR. The reference dew point mirror and pressure sensor were logged every 2 minutes continuously. The FMI humidity sensors were read by another computer with dedicated test equipment, the same equipment that has been used in all calibration tests.

2.4 Experimental procedure

The main part of the measurement campaign consisted of measurements in equilibrium temperature and relative humidity conditions. The goal parameters were set in the control software and the chamber was left to stabilize for a predetermined time period. The gas flow rate through the measurement chamber was 10 NI/h. Controlling of the parameters was automatic, allowing the experiment to run continuously for long periods of time.

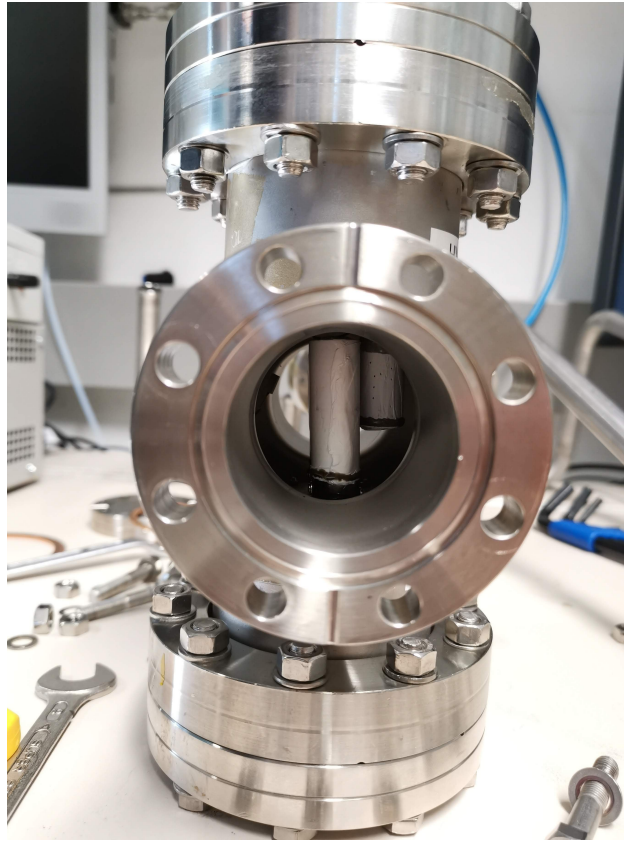


Figure 6. All three instruments inside the measurement chamber (the third one is behind the others). The opening from the front to the back of the chamber that can be seen here is the path of the gas flow when the chamber is placed in the test setup. The other two flanges have the electrical feedthroughs for the instruments and the separate temperature sensor.

Dry measurements were performed as a part of the experiment, but saturation humidities were not planned. Saturation conditions would not cause damage to the sensors but can cause erroneous readings until the sensor heads have dried out.

The following measurement goals were set for these experiments (in priority order):

- 180
1. Measure the instrument response in RH in the range from 0 to <100 %rh in stable Martian temperature (-50 °C or less) and stable Martian pressure of 8 hPa in CO₂ gas.
 2. Repeat the RH measurements at multiple temperatures between -30 °C and -70 °C.
 3. Repeat the RH measurements at higher and lower Martian range pressure in CO₂.
 4. Repeat the measurements in an accurate Martian gas mixture, at least at one temperature and pressure.

Table 1. The measurement points including different temperatures, humidities, pressures and gas mediums that were used. Relative humidity is given with respect to ice.

Temperature (°C)	RH (%)	Pressure (hPa)	Medium
-40, -50, -60, -70	0, 20, 40, 60, 80, 95, 80, 60, 40, 20, 0	6, 8, 10	CO ₂
-60	0, 20, 40, 60, 80, 95, 80, 60, 40, 20, 0	6, 10	CO ₂
-60	0, 10, 20, 30, 40, 50, 60, 70, 80, 90, 95 90, 80, 70, 60, 50, 40, 30, 20, 10, 0	8	CO ₂
-30	0, 5, 10, 20, 30	8	CO ₂
-40	0, 20, 40, 60, 80, 95, 80, 60, 40, 20, 0	8	Mars gas mixture

185 Each instrument was measured with 1 Hz frequency for only 10 seconds in order to avoid self heating. From the 10 s data, seconds 2-5 are averaged in order to get the actual measurement point. Each instrument was measured with a 10 minute period. The measurements were run automatically in a continuous way, also during the environmental changes.

The measurement set points are given in Table 1. The actual achieved input values for pressure and humidity differ slightly compared to the table and the final achieved measurement points are presented in sections 3.1 and 3.2. Parameters like temper-
190 ature and pressure can also drift slowly during the measurements but this is not an issue because all reference values are taken from the reference sensors simultaneously to the instrument measurements.

3 Results

The campaign was carried out successfully and all the campaign objectives were met. The campaign was run from Autumn 2020 to Spring 2021 despite the COVID-19 pandemic. The measurements started from stable temperature and pressure, close to
195 zero humidity, and the humidity inside the chamber was increased in a step-wise manner. After reaching the highest humidity, the steps were repeated again towards zero relative humidity. Figure 7 gives an example of measurements of one humidity instrument during a measurement run in stable temperature and pressure, and changing humidity. In addition to the stable point calibration measurements in CO₂ (Sections 3.1 and 3.2), experiments were performed also in a Martian-like gas mixture (Sections 3.3 and with MEDA HS kept continuously powered on instead of regular short measurements (Section 3.4).

200 3.1 Temperature dependence in the Martian environment

The environmental temperature not only affects the HUMICAP sensor capacitance but also the sensor dynamic range. At low temperatures the dynamic range is significantly reduced compared to room temperature. At +22 °C and atmospheric pressure the dynamic range of the newer HUMICAP sensor head is on the order of 7 pF and at -70°C only 2.5-3 pF. The older sensor type used in REMS-H has a dynamic range of only 0.3 pF in -70°C. An example of humidity measurements at different
205 temperatures is shown in figure 8. Using regression analysis on the data set it was determined that a 2nd degree polynomial

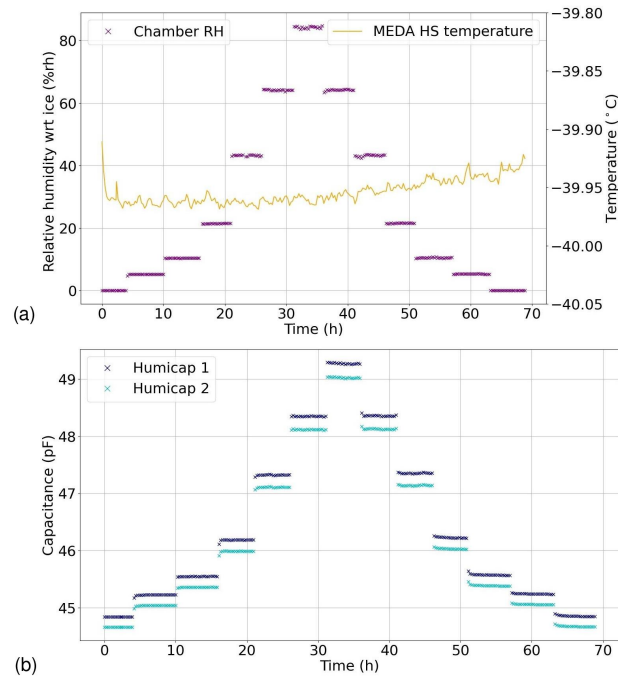


Figure 7. Example of increasing and decreasing RH measurements in -40°C . Panel (a) shows the relative humidity reference measurement calculated from the dew point mirror at instrument temperature (purple) and the instrument temperature evolution during the measurement (orange). In panel (b) HUMICAP 1 and 2 capacitances calculated from raw data are shown for the same run. Each point represents one measurement every 15 minutes.

curve provided the best fit for the observed relationships between the variables with all three measured instruments. Examples of 2nd degree polynomial fits are shown in figure 8. The different temperatures are clearly distinguishable and the reduced dynamic range towards lower temperatures is also evident. Due to limitations in the humidity control system at PASLAB the range of possible relative humidities were limited at higher temperatures, and thus -30°C was the highest test temperature.

210 3.2 Pressure dependence in the Martian environment

In addition to different Martian temperatures, measurements were also taken under different pressures ranging from 5.5 hPa to 9.8 hPa. Figure 9 shows all the successful measurement points for each instrument in CO_2 , resulting from the measurement program given in table 1. The temperatures vary from -30°C to -70°C , and relative humidity from close to zero to almost 100 %rh. As expected, it was more challenging to reach lower humidity levels at lower temperatures. At -70°C the lowest humidities recorded were approximately 0.3 %rh, while at -40°C , the humidity levels ranged between 0.01 %rh and 0.02 %rh.

The measurements revealed a pressure dependency under Martian conditions, increasing towards the coldest temperatures. For example in the case of MEDA HS, at -70°C a pressure difference of 100 Pa would result in a difference of 2.8 % in relative humidity. The difference is on the same order as the measurement uncertainty of the sensor. For reference, the diurnal

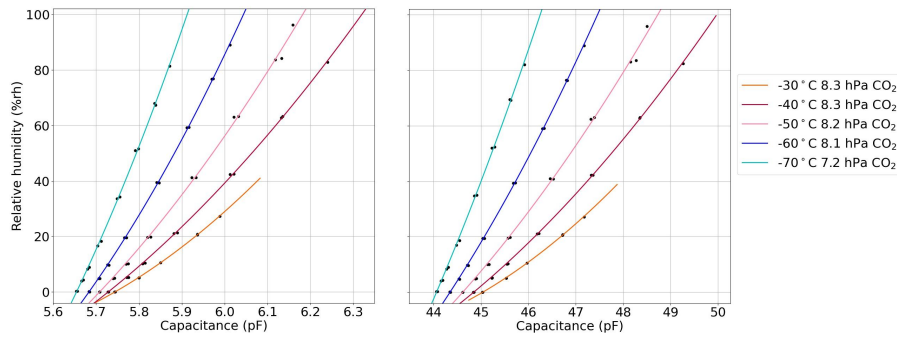


Figure 8. Measurements of REMS-H (left) and MEDA HS (right) at different temperatures and relative humidities between 0 % and 100 %rh at stable Mars pressure. The results are shown in terms of reference relative humidity (y-axis) and the calculated capacitance of one HUMICAP sensor head (x-axis). The HUMICAP behaviour at each temperature was found to be optimally captured by fitting a 2nd degree polynomial function to the data.

pressure amplitude at the Perseverance landing site Jezero crater has been 10...35 Pa and the seasonal pressure variation based
 220 on previous missions can be more than 200 Pa (Harri (In review)). It is therefore clear that the pressure changes on the Martian
 surface must also be taken into account in the calibration of the instruments. An example of 2nd degree polynomial fits to each
 measurement series for one sensor head of MEDA HS REF is given in figure 10.

3.3 Martian-like gas mixture

It has been assumed that because the Martian atmosphere is 95% by volume carbon dioxide, the calibration could be performed
 225 in pure CO₂ without the other trace gases. That assumption was possible to put to the test at PASLAB by comparing measure-
 ments with 100% CO₂ with measurements in a Martian-like gas mixture. The tested Martian-like atmosphere was composed
 of 3.7% air (ca. 2.96% N₂ and 0.74% O₂), 1.6% Ar and 94.7% CO₂. The Martian atmosphere measured by Curiosity's SAM
 (Sample Analysis at Mars) instrument is 95% by volume of carbon dioxide (CO₂), 2.6% molecular nitrogen (N₂), 1.9% argon
 (Ar), 0.16% molecular oxygen (O₂), and 0.06% carbon monoxide (CO) (Trainer et al. (2019)).

230 The Martian gas mixture was tested only at one temperature, -40 °C, and one Martian pressure but at multiple RH points. This
 temperature was selected over lower, maybe more representative, temperatures because the dynamic range of the instruments
 is larger at higher temperature and therefore any difference between the measurements would be more easily seen. Scattering
 of the measurements is also smaller at higher temperatures. The resulting data series was compared to measurements in pure
 CO₂ at the same temperature and at two similar pressures. The results can be seen in figure 11. In the capacitance plot there
 235 is no visible difference between the measurements in pure CO₂ and in the Martian gas mixture. The difference was further
 investigated using calibrated RH data (calibration as described in section 4) from MEDA HS REF. The larger scattering and
 larger calibration error of the measurement points towards higher humidities is typical behaviour of the instrument. There is
 no distinctive pattern in the Martian gas mixture measurements in the difference plot and while the largest discrepancies from

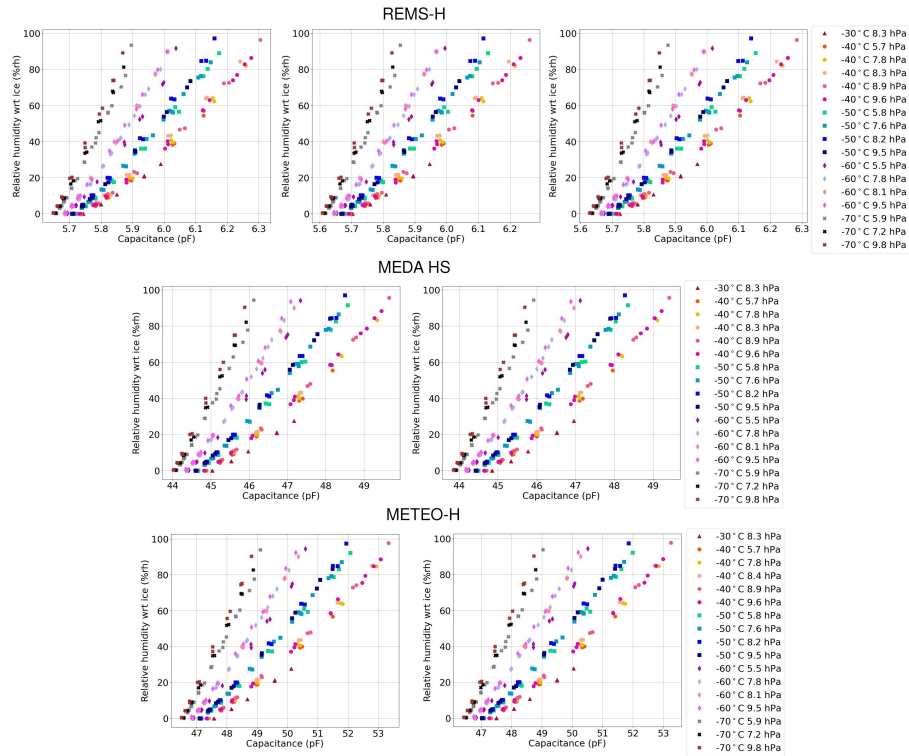


Figure 9. Resulting measurements at different temperatures, humidities and pressures for all HUMICAP sensor heads from the three tested instrument models: REMS-H (top), MEDA HS (middle) and METEO-H (bottom). The relative humidity is calculated from the experimental chamber parameters and the capacitance is calculated from the raw HUMICAP data. Each point is averaged over a 4 s period, calculated from the beginning of a stabilized measurement.

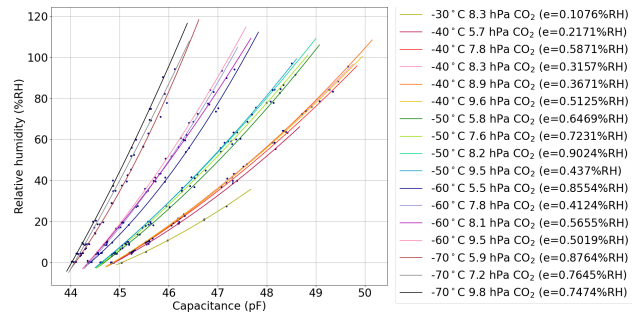


Figure 10. 2nd degree polynomial lines fitted to each measurement series of MEDA HS HUMICAP 1 at one temperature and pressure. The pressure dependence can be seen between the measurements at a fixed temperature. e gives the mean absolute error

the reference, reaching 1.5 %rh, are seen in the Martian gas mixture measurements at humidity of 60 %rh, the measurements are not consistently higher than the CO₂ measurements leading to the conclusion that the measurements show no differences

240

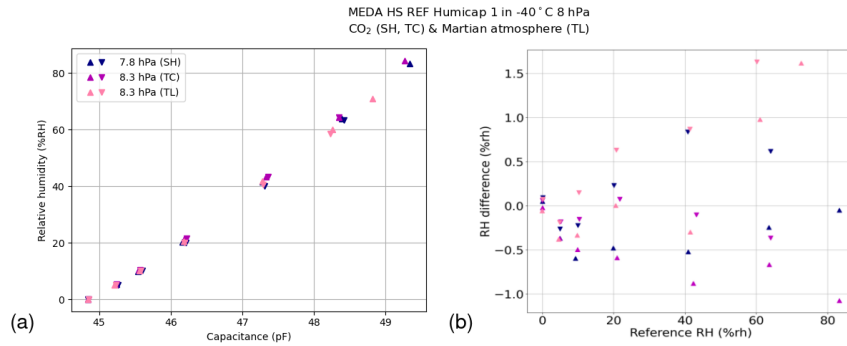


Figure 11. Comparison of CO₂ gas (purple and blue) and the Mars-like gas composition (pink) in capacitance compared to reference RH in panel (a) and the difference between calibrated RH compared to reference RH in panel (b).

related to the gas compositions. Even the largest differences fall within the measurement uncertainty range of approximately 3 %rh (uncertainty of MEDA HS flight model in similar conditions).

3.4 Startup self-heating effect

The calibration of the humidity instruments has been determined by using very short measurements in order to avoid self-heating, however on Mars both MEDA and REMS humidity instruments have been measured continuously, also for longer time periods, for operational reasons.

When the instrument is powered on, a slight warming of the temperature sensors is visible over a time on the order of ten seconds, even though the power consumption of the sensor is only about 20 mW. The sensor self-heating is prominent for approximately 15 to 20 minutes, after which the sensor temperature stabilises. Intrinsically the local relative humidity at the sensor drops when the sensor temperature rises and this can usually be clearly seen in the long continuous measurements of the REMS-H and MEDA HS on Mars.

While the relative humidity is intrinsically affected by the self-heating, in the ideal case the derived absolute VMR should be the same before and after self-heating when the environment stays the same. In that case the relative humidity sensor data could be used as such after the self-heating period. This theory was tested with the MEDA HS ground reference model at the DLR PASLAB in low pressure CO₂ at -60°C.

Figure 12 shows two test measurements. The calibrated relative humidity (calibration as described in Section 4) of the MEDA HS ground reference model is compared to the reference RH, calculated from the dew point mirror frost point temperature and from the MEDA HS temperature, and to chamber RH. Both measurements were performed at -60 °C but in different humidities. In the upper figure the RH was around 9 % during instrument startup and in the lower figure 38 %. A small calibration offset has been added in order to see the difference between the instrument and reference RH more clearly. The plots show that there is no significant difference after the self-heating period has stabilised, and even during self-heating both readings follow the ideal reference curve quite well.

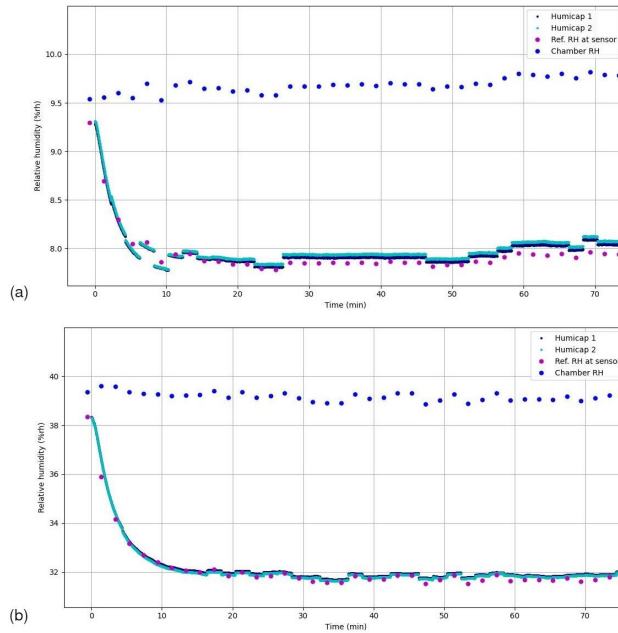


Figure 12. Calibrated RH of MEDA HS compared to the reference during MEDA HS self heating test. Two measurements shown in panels (a) and (b) were acquired with different humidity levels, both at -60°C in 8 hPa. The reference RH is calculated from the reference frost point at HS temperature, while the chamber RH is calculated from the reference frost point at chamber temperature. The MEDA HS RH has been offset-corrected to the same level as the reference RH in order to allow comparison of the two readings. Occasionally disjointed RH values from MEDA HS are due to fluctuations in the chamber reference pressure readings which is used to calculate the calibrated RH.

Figure 13 shows the same measurements as figure 12 but with a derived VMR (average of the two sensor heads) compared to the reference VMR. The reference VMR is calculated from the dew point mirror frost point, chamber temperature and pressure.

265 In the 9 %rh measurement the instrument VMR first rises rapidly 2 ppm above the reference VMR and then drops about 1.5 ppm below the reference before stabilizing slightly above the reference VMR. A similar behaviour is present also in the 38 %rh measurement. This behaviour is most likely due to small temperature gradients developing in the PCB electronics during the self-heating period (Polkko et al. (2023)). At the end of the measurements, 70 minutes after powering up the instrument, the difference between the measured VMR and reference VMR is about 2 ppm. It is very small compared to the measurement

270 uncertainty of the MEDA HS flight model VMR, which would be around 15 ppm in 9 %rh and about 30 ppm in 38 %rh at this temperature.

As the test was only performed at one temperature and in two different humidities, the results can not be considered conclusive yet. But it seems plausible that these instruments can be operated also continuously with the current calibration.

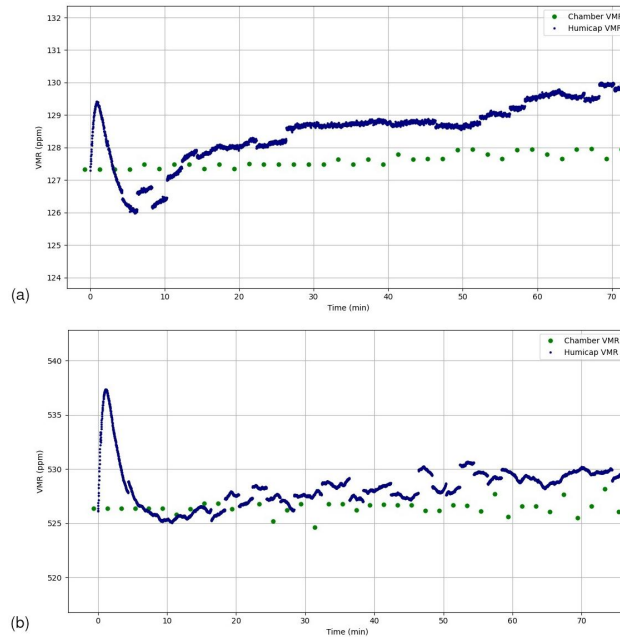


Figure 13. Calibrated average VMR of MEDA HS HUMICAPs compared to the reference during the MEDA HS self heating test in the same cases as in figure 12. Reference VMR is calculated from the reference frost point at chamber temperature and pressure. The sensor VMR first rapidly increases and decreases during the self-heating period before stabilizing slightly above the reference VMR.

4 Calibration equations for MEDA HS

275 The measurements presented in this paper have already been used in Perseverance’s MEDA HS humidity sensor calibration. The measurements of the actual flight model at FMI and the measurements at DLR PASLAB were combined to provide more accurate calibration coefficients that would not have been achieved with the original measurements at FMI alone.

Because all sensor heads and instruments are unique, in order to utilise the ground reference model measurements, information about the differences between the instruments is needed so that the calibration information can be transferred. This is
 280 made possible by simultaneous measurements of flight and reference models at the FMI, the very similar behaviour between the different HS models, and also the statistics of an almost identical METEO-H REF model included in the calibration campaign.

Using data taken at 7...8 hPa, dry and saturation curves were calculated from HUMICAP capacitance readings (in pF) as a function of the HUMICAP temperature. Only the average values of the first 2-5 s of each measurement are used in the calibration. A scaled capacitance was calculated using 100 %rh and 0 %rh curves to give the range of the capacitance at
 285 each temperature. Scaled capacitances of all four HUMICAP sensor heads from MEDA HS and METEO-H were combined to increase statistics, and a calibration curve was fitted to the combined data. This calibration curve was then transferred to MEDA HS flight model HUMICAPS. The calibration of the MEDA HS is presented in more detail in Hieta et al. (2022).

For the ground reference models, a calibration has been calculated separately for each HUMICAP since the averaging is not necessary.

290 The relative humidity reading (in %rh) is calculated from the scaled capacitance with a second-degree polynomial:

$$RH = a_f C_{scaled}^2 + b_f C_{scaled} + c_f \quad (4)$$

Calibration parameters for the MEDA HS ground reference model used in this paper are given in Table 2.

Table 2. MEDA HS ground reference sensor head calibration parameters

Parameter	HUMICAP 1	HUMICAP 2
a_d	-1.902450348e-04	-1.975077126e-04
b_d	5.362532951e-03	4.065874934e-03
c_d	4.536447969e+01	4.514377272e+01
a_w	1.283982106e-01	1.265131607e-01
b_w	5.514342280e+01	5.480986012e+01
a_f	2.122378479e+01	2.122378479e+01
b_f	7.868134001e+01	7.868134001e+01
c_f	-6.406002023e-04	-6.406002023e-04

A comprehensive uncertainty analysis was performed for the MEDA HS flight model by [Tabandeh Tabandeh and Högström \(2021\)](#). Fitting residuals of the method described above were found to be the main uncertainty source for MEDA HS. Therefore a
295 compensation model was developed by studying the correlation between the fitting residuals and temperature, pressure and relative humidity. The compensation model has also been applied to the MEDA HS ground reference model calibrated RH shown in figures 12 and 11.

The compensation is the same for both the MEDA HS reference model and flight model HUMICAPs, defined as

$$\begin{aligned} \bar{C} = & (c_1 + c_2 \cdot T + c_3 \cdot \frac{P}{100} + 0.0181) \cdot RH - 0.08478 \cdot \cos(0.06743 \cdot RH) \\ & - 0.9919 \cdot \sin(0.06743 \cdot RH) + 0.1257 \end{aligned} \quad (5)$$

300 where T is temperature in °C and P is pressure in Pa. Terms c_1 , c_2 and c_3 are defined as:

$$c_1 = -2.362 \cdot \exp(-0.05704 \cdot RH) - 0.4051 \cdot \exp(0.00369 \cdot RH)$$

$$c_2 = 0.01474 \cdot \exp(c_1) - 0.01095$$

$$c_3 = -0.09237 \cdot c_1 + 0.0004843$$

Final corrected RH for the MEDA HS ground reference model is obtained by adding the compensation to the RH obtained
305 through scaled capacitance:

$$RH_{corr,HC1} = RH_{HC1} + \bar{C}$$

$$RH_{corr,HC2} = RH_{HC2} + \bar{C}$$

(6)

5 Conclusions and discussion

The measurement campaign at DLR PASLAB resulted in high quality calibration data sets in a representative Martian environment for REMS-H, MEDA HS and METEO-H relative humidity instruments. The tested models were flight-representative ground reference models which were manufactured and tested together with the actual flight models. Currently REMS-H on board the Curiosity rover and MEDA HS on board the Perseverance rover are operating on Mars, while the ExoMars surface platform mission including METEO-H has been cancelled. Although METEO-H will not be operational on Mars, it has provided important statistics about the behaviour of the new HUMICAP sensor heads.

The new calibration data set has already been used in the flight calibration of the MEDA HS instrument, resulting in excellent accuracy and trustworthiness of the measurements the instrument provides. With this data set and the calibration compensation developed based on it, we were able to improve the calibration uncertainty from an estimated ≤ 10 %rh to ≤ 4.4 %rh at temperatures down to -70 °C (Tabandeh Tabandeh and Högström (2021)). No changes or corrections have been necessary since the calibration presented in Hieta et al. (2022).

The data set also provides the means to reanalyse the current calibration of the REMS-H flight model. The current compensated calibration of REMS-H will be compared to a calibration derived from the data set presented in this paper in order to assess the need for possible recalibration, and in the best case the flight calibration could be improved using the new data. However, the unknown transducer electronics artifact affecting REMS-H is likely more complicated than just a calibration issue, so we don't expect it to reach the same performance as MEDA HS even with recalibration. In any case, the analysis of REMS-H calibration will allow for a better comparison between the two instruments on Mars enhancing the scientific output from the two locations.

In addition to the stable point humidity calibration measurements in carbon dioxide, two other experiments were run with the same setup. Comparative measurements were performed with a realistic Martian atmosphere composition to confirm that there is no difference compared to a pure CO₂ atmosphere, justifying the calibration performed in just CO₂. The measurements were successful and indeed they confirmed that the measurements were fully concordant. Another experiment additional to the normal calibration was to test the continuous measurement mode of MEDA HS where the instrument is kept powered on for longer periods of time, instead of periodic operation, used to avoid self-heating. The conducted tests have produced encouraging results, suggesting that self-heating has a negligible impact on the absolute VMR. However, additional testing and analysis are required to validate these findings over a larger operational temperature range and to determine their applicability to the flight models.

335 *Data availability.* The raw calibration data is partially treated as confidential, however, a processed data set can be provided upon request.

Author contributions. Conceptualization: All authors. Data curation: M.H., I.J., J.P., A.L. and S.G. Formal analysis: M.H., I.J. and J.P. Investigation: M.H., I.J., A.L. and S.G. Methodology: M.H., I.J., J.P., A.L. and S.G. Project administration/supervision: J.-P.d.V., M.G., A.-M.H. Resources: M.H., I.J., J.P., A.L., S.G. and J.-P.d.V. Software: M.H., I.J., A.L. and S.G. Visualization: I.J., A.L. and S.G. Writing—Original draft: M.H., I.J. and J.P. Writing—Review and editing: M.H., I.J., J.P., A.L., S.G. and A.-M.H.

340 *Competing interests.* The authors declare that they have no competing interests. Some authors are members of the editorial board of Geoscientific Instrumentation, Methods and Data Systems. The peer-review process was guided by an independent editor, and the authors have also no other competing interests to declare.

Acknowledgements. Maria Hieta, Iina Jaakonaho, Jouni Polkko and Ari-Matti Harri are thankful for the ~~Finnish Academy~~ [Academy of Finland](#) grant #310509. We would also like to thank Vaisala Oyj for providing the sensor heads for the relative humidity instrument family

345 and for their long term cooperation and support.

References

- HUMICAP technology description, Vaisala Oyj, <https://www.vaisala.com/sites/default/files/documents/HUMICAP-Technology-description-B210781EN.pdf>, ref. B210781EN-D, 2020.
- 350 Buck, A. L.: New equations for computing vapor pressure and enhancement factor, *Journal of Applied Meteorology and Climatology*, 20, 1527 – 1532, [https://doi.org/10.1175/1520-0450\(1981\)020<1527:NEFCVP>2.0.CO;2](https://doi.org/10.1175/1520-0450(1981)020<1527:NEFCVP>2.0.CO;2), 1981.
- de Vera, J.-P., Schulze-Makuch, D., Khan, A., Lorek, A., Koncz, A., Möhlmann, D., and Spohn, T.: Adaption of an Antarctic lichen to Martian niche conditions can occur within 34 days, *Planetary and Space Science*, 98, <https://doi.org/10.1016/j.pss.2013.07.014>, 2013.
- Esposito, F., Debei, S., Bettanini, C., Molfese, C., Arruego Rodríguez, I., Colombatti, G., Harri, A.-M., Montmessin, F., Wilson, C., Aboudan, A., Schipani, P., Marty, L., Álvarez, F. J., Apestigue, V., Bellucci, G., Berthelier, J.-J., Brucato, J. R., Calcutt, S. B., Chiodini, S., Cortecchia, F., Cozzolino, F., Cucciarrè, F., Deniskina, N., Déprez, G., Di Achille, G., Ferri, F., Forget, F., Franzese, G., Friso, E., Genzer, M., Hassen-Kodja, R., Haukka, H., Hieta, M., Jiménez, J. J., Josset, J.-L., Kahanpää, H., Karatekin, O., Landis, G., Lapauw, L., Lorenz, R., Martinez-Oter, J., Mennella, V., Möhlmann, D., Moirin, D., Molinaro, R., Nikkanen, T., Palomba, E., Patel, M. R., Pommereau, J.-P., Popa, C. I., Rafkin, S., Rannou, P., Renno, N. O., Rivas, J., Schmidt, W., Segato, E., Silvestro, S., Spiga, A., Toledo, D., Trautner, R., Valero, F., Vázquez, L., Vivat, F., Witasse, O., Yela, M., Mugnuolo, R., Marchetti, E., and Pirrotta, S.: The DREAMS Experiment Onboard the Schiaparelli Module of the ExoMars 2016 Mission: Design, Performances and Expected Results, *Space Science Reviews*, 214, 103, <https://doi.org/10.1007/s11214-018-0535-0>, 2018.
- 360 Fischer, E., Martínez, G., and Rennó, N.: Formation and Persistence of Brine on Mars: Experimental Simulations throughout the Diurnal Cycle at the Phoenix Landing Site, *Astrobiology*, 16, 937–948, <https://doi.org/10.1089/ast.2016.1525>, PMID: 27912028, 2016.
- Fischer, E., Martínez, G. M., Rennó, N. O., Tamppari, L. K., and Zent, A. P.: Relative Humidity on Mars: New Results From the Phoenix TECP Sensor, *Journal of Geophysical Research: Planets*, 124, 2780–2792, <https://doi.org/10.1029/2019JE006080>, [_eprint: https://onlinelibrary.wiley.com/doi/pdf/10.1029/2019JE006080](https://onlinelibrary.wiley.com/doi/pdf/10.1029/2019JE006080), 2019.
- 375 Gomez-Elvira, J., Armiens, C., Castañer, L., Domínguez, M., Genzer, M., Gómez, F., Haberle, R., Harri, A.-M., Jiménez, V., Kahanpää, H., Kowalski, L., Lepinette, A., Martín, J., Martínez-Frías, J., McEwan, I., Mora, L., Moreno, J., Navarro, S., de Pablo, M. A., Peinado, V., Peña, A., Polkko, J., Ramos, M., Renno, N. O., Ricart, J., Richardson, M., Rodríguez-Manfredi, J., Romeral, J., Sebastián, E., Serano, J., de la Torre Juárez, M., Torres, J., Torrero, F., Urquí, R., Vázquez, L., Velasco, T., Verdasca, J., Zorzano, M.-P., and Martín-Torres, J.: REMS: The Environmental Sensor Suite for the Mars Science Laboratory Rover, *Space Science Reviews*, 170, 583–640, <https://doi.org/10.1007/s11214-012-9921-1>, 2012.
- Harri, A.-M.: Perseverance MEDA Atmospheric Pressure Observations - Initial Results, In review.
- Harri, A. M., Linkin, V., Polkko, J., Marov, M., Pommereau, J. P., Lipatov, A., Siili, T., Manuilov, K., Lebedev, V., Lehto, A., Pellinen, R., Pirjola, R., Carpentier, T., Malique, C., Makarov, V., Khloustova, L., Esposito, L., Maki, J., Lawrence, G., and Lystsev, V.: Meteorological observations on Martian surface: met-packages of Mars-96 Small Stations and Penetrators, *Planetary and Space Science*, 46, 779–793, [https://doi.org/10.1016/S0032-0633\(98\)00012-9](https://doi.org/10.1016/S0032-0633(98)00012-9), 1998.
- 380 Harri, A.-M., Genzer, M., Kempainen, O., Gomez-Elvira, J., Haberle, R., Polkko, J., Savijärvi, H., Rennó, N., Rodriguez-Manfredi, J. A., Schmidt, W., Richardson, M., Siili, T., Paton, M., Torre-Juarez, M. D. L., Mäkinen, T., Newman, C., Rafkin, S., Mischna, M., Merikallio, S., Haukka, H., Martin-Torres, J., Komu, M., Zorzano, M.-P., Peinado, V., Vazquez, L., and Urqui, R.: Mars Science Laboratory relative humidity observations: Initial results, *Journal of Geophysical Research: Planets*, 119, 2132–2147, <https://doi.org/10.1002/2013JE004514>, [_eprint: https://onlinelibrary.wiley.com/doi/pdf/10.1002/2013JE004514](https://onlinelibrary.wiley.com/doi/pdf/10.1002/2013JE004514), 2014.

- Hieta, M., Genzer, M., Polkko, J., Jaakonaho, I., Tabandeh, S., Lorek, A., Garland, S., de Vera, J.-P., Fischer, E., Martínez, G. M., Harri, A.-M., Tamppari, L., Haukka, H., Meskanen, M., de la Torre Juárez, M., and Rodriguez Manfredi, J. A.: MEDA HS: Relative humidity sensor for the Mars 2020 Perseverance rover, *Planetary and Space Science*, 223, 105 590, <https://doi.org/https://doi.org/10.1016/j.pss.2022.105590>, 2022.
- Jakosky, B. M.: The Seasonal Cycle of Water on Mars, *Space Science Reviews*, 41, 131–200, <https://doi.org/10.1007/BF00241348>, 1985.
- Jakosky, B. M., Zent, A. P., and Zurek, R. W.: The Mars Water Cycle: Determining the Role of Exchange with the Regolith, *Icarus*, 130, 87–95, <https://doi.org/https://doi.org/10.1006/icar.1997.5799>, 1997.
- Kappen, L., Schroeter, B., Scheidegger, C., Sommerkorn, M., and Hestmark, G.: Cold resistance and metabolic activity of lichens below 0 degC, *Advances in Space Research*, 18, 119–128, [https://doi.org/10.1016/0273-1177\(96\)00007-5](https://doi.org/10.1016/0273-1177(96)00007-5), 1996.
- Lorek, A.: Humidity measurement with capacitive humidity sensors between -70°C and 25°C in low vacuum, *Journal of Sensors and Sensor Systems*, 3, 177–185, <https://doi.org/10.5194/jsss-3-177-2014>, 2014.
- Lorek, A. and Koncz, A.: Simulation and Measurement of Extraterrestrial Conditions for Experiments on Habitability with Respect to Mars, in: *Habitability of Other Planets and Satellites*, edited by de Vera, J.-P. and Seckbach, J., vol. 28, pp. 145–162, Springer Netherlands, Dordrecht, https://doi.org/10.1007/978-94-007-6546-7_9, series Title: Cellular Origin, Life in Extreme Habitats and Astrobiology, 2013.
- Lorek, A. and Majewski, J.: Humidity Measurement in Carbon Dioxide with Capacitive Humidity Sensors at Low Temperature and Pressure, *Sensors*, 18, 2615, <https://doi.org/10.3390/s18082615>, number: 8 Publisher: Multidisciplinary Digital Publishing Institute, 2018.
- Martinez, G. M., Fischer, E., Rennó, N., Sebastián, E., Kemppinen, O., Bridges, N., Borlina, C., Meslin, P.-Y., Genzer, M., Harri, A.-H., Vicente-Retortillo, , Ramos, M., Juarez, M., Gómez, F., and Gomez-Elvira, J.: Likely frost events at Gale crater: Analysis from MSL/REMS measurements, *Icarus*, 280, <https://doi.org/10.1016/j.icarus.2015.12.004>, 2015.
- Martínez, G. M., Newman, C. N., De Vicente-Retortillo, A., Fischer, E., Renno, N. O., Richardson, M. I., Fairén, A. G., Genzer, M., Guzewich, S. D., Haberle, R. M., Harri, A.-M., Kemppinen, O., Lemmon, M. T., Smith, M. D., de la Torre-Juárez, M., and Vasavada, A. R.: The Modern Near-Surface Martian Climate: A Review of In-situ Meteorological Data from Viking to Curiosity, *Space Science Reviews*, 212, 295–338, <https://doi.org/10.1007/s11214-017-0360-x>, 2017.
- Polkko, J., Hieta, M., Harri, A.-M., Tamppari, L., Martínez, G., Viúdez-Moreiras, D., Savijärvi, H., Conrad, P., Zorzano Mier, M. P., De La Torre Juarez, M., Hueso, R., Munguira, A., Leino, J., Gómez, F., Jaakonaho, I., Fischer, E., Genzer, M., Apestigue, V., Arruego, I., Banfield, D., Lepinette, A., Paton, M., Rodriguez-Manfredi, J. A., Sánchez Lavega, A., Sebastian, E., Toledo, D., Vicente-Retortillo, A., and team, M.: Initial Results of the Relative Humidity Observations by MEDA Instrument Onboard the Mars 2020 Perseverance Rover, *Journal of Geophysical Research: Planets*, 128, e2022JE007 447, <https://doi.org/https://doi.org/10.1029/2022JE007447>, e2022JE007447 2022JE007447, 2023.
- Rodriguez-Manfredi, J. A., de la Torre Juárez, M., Alonso, A., Apéstigue, V., Arruego, I., Atienza, T., Banfield, D., Boland, J., Carrera, M. A., Castañer, L., Ceballos, J., Chen-Chen, H., Cobos, A., Conrad, P. G., Cordoba, E., del Río-Gaztelurrutia, T., de Vicente-Retortillo, A., Domínguez-Pumar, M., Espejo, S., Fairen, A. G., Fernández-Palma, A., Ferrándiz, R., Ferri, F., Fischer, E., García-Manchado, A., García-Villadangos, M., Genzer, M., Giménez, S., Gómez-Elvira, J., Gómez, F., Guzewich, S. D., Harri, A. M., Hernández, C. D., Hieta, M., Hueso, R., Jaakonaho, I., Jiménez, J. J., Jiménez, V., Larman, A., Leiter, R., Lepinette, A., Lemmon, M. T., López, G., Madsen, S. N., Mäkinen, T., Marín, M., Martín-Soler, J., Martínez, G., Molina, A., Mora-Sotomayor, L., Moreno-Álvarez, J. F., Navarro, S., Newman, C. E., Ortega, C., Parrondo, M. C., Peinado, V., Peña, A., Pérez-Grande, I., Pérez-Hoyos, S., Pla-García, J., Polkko, J., Postigo, M., Prieto-Ballesteros, O., Rafkin, S. C. R., Ramos, M., Richardson, M. I., Romeral, J., Romero, C., Runyon, K. D., Saiz-Lopez, A., Sánchez-Lavega, A., Sard, I., Schofield, J. T., Sebastian, E., Smith, M. D., Sullivan, R. J., Tamppari, L. K., Thompson, A. D., Toledo, D., Torrero, F., Torres,

- J., Urquí, R., Velasco, T., Viúdez-Moreiras, D., Zurita, S., and MEDA team: The Mars Environmental Dynamics Analyzer, MEDA. A Suite of Environmental Sensors for the Mars 2020 Mission, *Space Science Reviews*, 217, 48, <https://doi.org/10.1007/s11214-021-00816-9>, 2021.
- Rodriguez-Manfredi, J. A., de la Torre Juarez, M., Sanchez-Lavega, A., Hueso, R., Martinez, G., Lemmon, M. T., Newman, C. E., Munguira, A., Hieta, M., Tamppari, L. K., Polkko, J., Toledo, D., Sebastian, E., Smith, M. D., Jaakonaho, I., Genzer, M., De Vicente-Retortillo, A., Viudez-Moreiras, D., Ramos, M., Saiz-Lopez, A., Lepinette, A., Wolff, M., Sullivan, R. J., Gomez-Elvira, J., Apestigue, V., Conrad, P. G., Del Rio-Gaztelurrutia, T., Murdoch, N., Arruego, I., Banfield, D., Boland, J., Brown, A. J., Ceballos, J., Dominguez-Pumar, M., Espejo, S., Fairén, A. G., Ferrandiz, R., Fischer, E., Garcia-Villadangos, M., Gimenez, S., Gomez-Gomez, F., Guzewich, S. D., Harri, A.-M., Jimenez, J. J., Jimenez, V., Makinen, T., Marin, M., Martin, C., Martin-Soler, J., Molina, A., Mora-Sotomayor, L., Navarro, S., Peinado, V., Perez-Grande, I., Pla-Garcia, J., Postigo, M., Prieto-Ballesteros, O., Raffkin, S. C. R., Richardson, M. I., Romeral, J., Romero, C., Savijärvi, H., Schofield, J. T., Torres, J., Urqui, R., and Zurita, S.: The diverse meteorology of Jezero crater over the first 250 sols of Perseverance on Mars, *Nature Geoscience*, pp. 1–10, <https://doi.org/10.1038/s41561-022-01084-0>, publisher: Nature Publishing Group, 2023.
- Savijärvi, H., Harri, A.-M., and Kempainen, O.: The diurnal water cycle at Curiosity: Role of exchange with the regolith, *Icarus*, 265, 63–69, <https://doi.org/10.1016/j.icarus.2015.10.008>, 2016.
- Savijärvi, H., McConnochie, T. H., Harri, A.-M., and Paton, M.: Annual and diurnal water vapor cycles at Curiosity from observations and column modeling, *Icarus*, 319, 485–490, <https://doi.org/10.1016/j.icarus.2018.10.008>, 2019.
- Savijärvi, H., Martinez, G. M., Fischer, E., Rennó, N., Tamppari, L., Zent, A., and Harri, A.-M.: Humidity observations and column simulations for a warm period at the Mars Phoenix lander site: Constraining the adsorptive properties of regolith, *Icarus*, 343, 113–168, <https://doi.org/10.1016/j.icarus.2020.113688>, 2020.
- Stevenson, A., Burkhardt, J., Cockell, C., Cray, J., Dijksterhuis, J., Fox-Powell, M., Kee, T., Kminek, G., Mcgenity, T., Timmis, K., Timson, D., Voytek, M., Westall, F., Yakimov, M., and Hallsworth, J.: Multiplication of microbes below 0.690 water activity: Implications for terrestrial and extraterrestrial life, *Environmental microbiology*, 17, <https://doi.org/10.1111/1462-2920.12598>, 2014.
- Tabandeh, S.: Uncertainty analysis of MEDA HS sensor aboard NASA's Perseverance rover, in preparation.
- Tabandeh, S. and Högström, R.: Uncertainty evaluation of MEDA HS humidity measurements, Confidential report VTT-CR-01095-21, VTT Technical Research Centre of Finland, 2021.
- Trainer, M. G., Wong, M. H., McConnochie, T. H., Franz, H. B., Atreya, S. K., Conrad, P. G., Lefèvre, F., Mahaffy, P. R., Malespin, C. A., Manning, H. L., Martín-Torres, J., Martínez, G. M., McKay, C. P., Navarro-González, R., Vicente-Retortillo, , Webster, C. R., and Zorzano, M.-P.: Seasonal Variations in Atmospheric Composition as Measured in Gale Crater, Mars, *Journal of Geophysical Research: Planets*, 124, 3000–3024, <https://doi.org/https://doi.org/10.1029/2019JE006175>, 2019.
- Zelenyi, L. M., Korablev, O. I., Rodionov, D. S., Novikov, B. S., Marchenkov, K. I., Andreev, O. N., and Larionov, E. V.: Scientific objectives of the scientific equipment of the landing platform of the ExoMars-2018 mission, *Solar System Research*, 49, 509–517, <https://doi.org/10.1134/S0038094615070229>, 2015.
- Zent, A. P., Hecht, M. H., Cobos, D. R., Campbell, G. S., Campbell, C. S., Cardell, G., Foote, M. C., Wood, S. E., and Mehta, M.: Thermal and Electrical Conductivity Probe (TECP) for Phoenix, *Journal of Geophysical Research: Planets*, 114, <https://doi.org/10.1029/2007JE003052>, [_eprint: https://onlinelibrary.wiley.com/doi/pdf/10.1029/2007JE003052](https://onlinelibrary.wiley.com/doi/pdf/10.1029/2007JE003052), 2009.