

Technical note: Characterization of a Single-Beam Gradient Force Aerosol Optical Tweezer for Droplet Trapping, Phase Transitions Monitoring, and Morphology Studies

Xiangyu Pei¹&Yikan Meng¹, Yueling Chen¹, Huichao Liu¹, Yao Song¹, Zhengning Xu¹, Fei Zhang¹, Thomas C. Preston³, Zhibin Wang^{1,2*}

¹Zhejiang Provincial Key Laboratory of Organic Pollution Process and Control, MOE Key Laboratory of Environment Remediation and Ecological Health, College of Environmental and Resource Sciences, Zhejiang University, Hangzhou 310058, China

²ZJU-Hangzhou Global Scientific and Technological Innovation Center, Zhejiang University, Hangzhou 311215, China

³Department of Atmospheric and Oceanic Sciences and Department of Chemistry, McGill University, 805 Sherbrooke Street West, Montréal, Quebec H3A 0B9, Canada

Correspondence to: Zhibin Wang (wangzhibin@zju.edu.cn)

Xiangyu Pei and Yikan Meng contribute equally to this work.

Abstract. Single particle analysis is essential for a better understanding of the particle transformation process and predicting its environmental impact. In this study, we developed an aerosol optical tweezer (AOT)-Raman spectroscopy system to investigate the phase state and morphology of suspended aerosol droplets in real time. The system comprises four modules: optical trapping, reaction, illumination and imaging, as well as detection. The optical trapping module utilizes a 532 nm laser and a 100x oil immersion objective to stably trap aerosol droplets within 30 seconds. The reaction module allows us to adjust relative humidity (RH) and introduce reaction gases into the droplet levitation chamber, facilitating experiments to study liquid-liquid phase transitions. The illumination and imaging module employs a high-speed camera to monitor the trapped droplets, while the detector module records Raman scattering light. We trapped sodium chloride (NaCl) and 3-methyl glutaric acid (3-MGA) mixed droplets to examine RH-dependent morphology changes. Liquid-liquid phase separation (LLPS) occurred when RH was decreased. Additionally, we introduced ozone and limonene/pinene to generate secondary organic aerosol (SOA) particles in situ, which collided with the trapped droplet and dissolve in it. To determine the trapped droplet's characteristics, we utilized an open-source program which based on Mie theory to retrieve diameter and refractive index from the observed whispering gallery modes (WGMs) in Raman spectra. It is found that mixed droplets formed core-shell morphology when RH was decreased, and the RH dependence of the droplets phase transitions generated by different SOA precursors varied. Our AOT system serves as an essential experimental platform for in-situ assessment of morphology and phase state during dynamic atmospheric processes.

30 **1 Introduction**

31 Atmospheric aerosol particles can absorb and reflect solar radiation, be activated into cloud droplets, participate in ice
32 nucleation processes, and provide interfaces for chemical reactions (Mülmenstädt et al., 2015; Shrivastava et al., 2017). As a
33 result, aerosols play important roles in air pollution, atmospheric chemistry and climate change (Pöschl, 2005). Aerosol
34 particles can have complex compositions including inorganic, metallic, and mineral components, and elemental carbon,
35 organic carbon, as well as an amount of water (Kolb and Worsnop, 2012). Aerosol particles can also have different
36 morphologies. For example, aerosol particles composed of inorganic salts and organic components can have solid, partially
37 engulfed or core-shell, and homogeneous morphologies through phase transitions (Freedman, 2020). Changes in aerosol
38 composition and water content will lead to the evolution of particle morphology and phase state, while altering other
39 physiochemical properties such as pH (Freedman et al., 2019), polarity (Zuend and Seinfeld, 2012), interfacial tensions
40 (Sullivan et al., 2018), and photochemistry (Cremer et al., 2016).

41 To study the physiochemical properties of atmospheric aerosol particles, various measurement methods and techniques are
42 applied. However, traditional measurement methods mainly represent the average properties of the aerosol population, lacking
43 detailed information about individual particles, such as morphology, phase state, composition, and so on. In comparison to
44 methods measuring properties of particle populations, single particle levitation techniques have been developed and applied
45 as effective tools for measuring the physical and optical properties of micron-sized particles (Krieger et al., 2012). Several
46 single particle levitation techniques, such as the electrodynamic balance (EDB), acoustic trap (AT), and optical tweezers (OT),
47 have been widely used to control and conduct direct real-time in-situ measurements of single particles (Davies, 2019; Combe
48 and Donaldson, 2017; Gong et al., 2018b). Using these techniques, various atmospheric aerosol properties during dynamic
49 processes, such as hygroscopicity, volatility, optical properties, viscosity, surface tension, and diffusion characteristics, have
50 been extensively studied (Chan et al., 2005; Davies et al., 2013; Cai et al., 2015). However, the fundamental principles of these
51 techniques determine their applicability for trapping particles of different sizes. For instance, EDB and AT can trap particles
52 with diameter ranges of 5-50 μm and 20-100 μm , respectively, while OT can trap smaller particles with size ranges in the
53 microns and tens of microns in diameter (Krieger et al., 2012).

54 When transparent or weakly absorptive spherical particles, such as droplets, are trapped by ~~Optical Tweezers (OT)~~ and
55 measured with Raman spectroscopy (RS), these spherical droplets can function as high-finesse optical cavities. This results in
56 a significant enhancement of stimulated Raman scattering signals at specific wavelengths, which are referred to as whispering
57 gallery modes (WGM) (Ashkin and Dziedzic, 1981). The diameter and refractive index of the trapped droplet can be
58 determined from the WGM signals (Reid et al., 2007). Additionally, different droplet morphologies can exert a considerable
59 influence on WGM behavior. For instance, if the droplet exhibits a homogeneous or concentric core-shell morphology, WGM
60 signals are generated. However, when liquid-liquid phase separation (LLPS) occurs, and the droplet assumes a partially

61 engulfed morphology, WGM signals will vanish. By combining OT with RS, precise information about droplet size, refractive
62 index, and morphology can be obtained. For example, Rickards et al. (2013) employed OT-RS to investigate the evolution of
63 size and refractive index under varying relative humidity (RH) conditions, exploring the impact of the O/C ratio on aerosol
64 hygroscopicity. Gorkowski et al. (2020) utilized OT-RS to predict phase separation and changes in particle morphology. They
65 studied the mixing behavior of α -pinene secondary organic aerosol (SOA) with different organic phases, including squalene
66 and glycerol, at various relative humidity levels. Boyer et al. (2020) applied OT-RS to achieve highly accurate in-situ pH
67 measurements of NaHSO₄ microdroplets.

68 In this study, we present our custom-made aerosol optical tweezer (AOT) system. We describe the system and the design of
69 the droplet particle levitation chamber. We have innovated the chamber design by adopting a smaller chamber to reduce droplet
70 capture time. Additionally, we have introduced a double-floor chamber room and a replaceable intermediate plate, which
71 facilitates control of the flow exchange rate for different experiments. We have also established methods for Raman spectrum
72 analysis and droplet morphometry determination and have systematically characterized this system, presenting the results. The
73 application of this system includes studying the morphology of aqueous droplet-hydrocarbon experiments and in-situ
74 generation and addition of SOA as the second phase. Furthermore, our chamber design provides the possibility for conducting
75 more gas-liquid phase reaction experiments in the future. This indicates that the AOT system is a powerful tool that can be
76 used to uncover the mechanisms of changes in physical and chemical properties of droplets during their evolution under
77 different conditions.

78 **2 Materials and methods**

79 **2.1 System description**

80 A schematic illustration of the aerosol optical tweezer system is presented in Figure 1, which includes the optical trapping
81 module, illumination and imaging module, detector module, and reaction module. The optical trapping module utilizes a 532
82 nm laser (Opus 532-2W). Depending on the desired particle size and flow turbulence, the laser power is adjusted between 30
83 and 200 mW to maintain steady trapping. Subsequently, the laser passes through expansion lenses to overfill the back aperture
84 of the microscope objective. A 100x oil immersion objective (Olympus, UPLFLN100XO, NA 1.30) is brought into contact
85 with a glass coverslip (Nest, thickness 160-190 μ m) installed at the bottom of the aerosol particle levitation chamber. This
86 convergence of the laser beam above the glass coverslip forms an optical trap.

87 The illumination and imaging module consist of a 450 nm LED (Daheng Optics, GCI060404) and a camera (Thorlabs,
88 CS165CU/M) used for illuminating and imaging the particles. Both the camera and spectrograph capture the LED scattered
89 light and the Raman scattered light from the particle, respectively, using the same microscope objective. To obtain a clear


90 image of the particle, a low-pass filter (Andover, 500FL07-25) is positioned in front of the camera lens to eliminate the
91 influence of backscattered light from the 532 nm laser.

92 The Raman scattering signals are collected through a detector module, with the primary component being a spectrometer. The
93 Raman scattered light passes through two 50:50 beam splitters (CVI Laser Optics, BTF-VIS-50-2501M-C) and a notch filter
94 (Edmund, 86125) before being focused into the Raman spectrograph. A spectrometer (ZOLIX, Omni- λ 5004i) is employed to
95 measure the Stokes-shifted Raman spectra, utilizing a 20 μm entrance slit width and a 1200 groove/mm diffraction grating
96 with a blaze wavelength of 500 nm to achieve a spectral resolution of 0.021 nm. The wavelength position of the spectrograph
97 is calibrated using a Hg-light source. For liquid-liquid phase separation experiments, the center wavelengths of 645 nm for the
98 diffraction grating are configured, and the Raman scattered light is recorded every 4 seconds within a wavelength range of
99 624.24-665.40 nm.

100 The reaction module serves as the area where RH airflow and reactive gases are introduced, and where chemical reactions
101 occur. Its central component is a custom-made aerosol particle levitation chamber (Figure 1(b)), which integrates the inverted
102 oil immersion objective from the optical trapping module and the downward brightfield illumination source from the
103 illumination and imaging module. Further details on the chamber's design will be provided in the following section. For
104 controlling RH airflow, two air streams are combined: one with a relative humidity of 100% and the other air-dried using a
105 silica drier. This mixture results in conditioned air with a specific RH, allowing precise control over humidity within the
106 chamber. The humidification of the airflow is achieved through a water bubbler, and both the humidified and dry airflows are
107 regulated by two mass flow controllers (MFCs) with a total flow rate of 0.3 L/min. Temperature and humidity sensors
108 (Sensirion, SHT85) are employed to measure the temperature and humidity of the airflow at both the inlet and outlet of the
109 chamber, following the design used by Gorkowski et al. (2016). Measuring temperature and humidity directly inside the
110 chamber with a probe is avoided because particle deposition on the probe can affect measurement accuracy. Additionally,
111 placing the probe near the droplet could interfere with droplet capture, making it challenging to maintain stable trapping of the
112 droplet. Other reactive gases can be introduced into the chamber through dedicated ports located on the chamber wall for
113 chemical reactions, and these gases exit through an exhaust port.

114

115

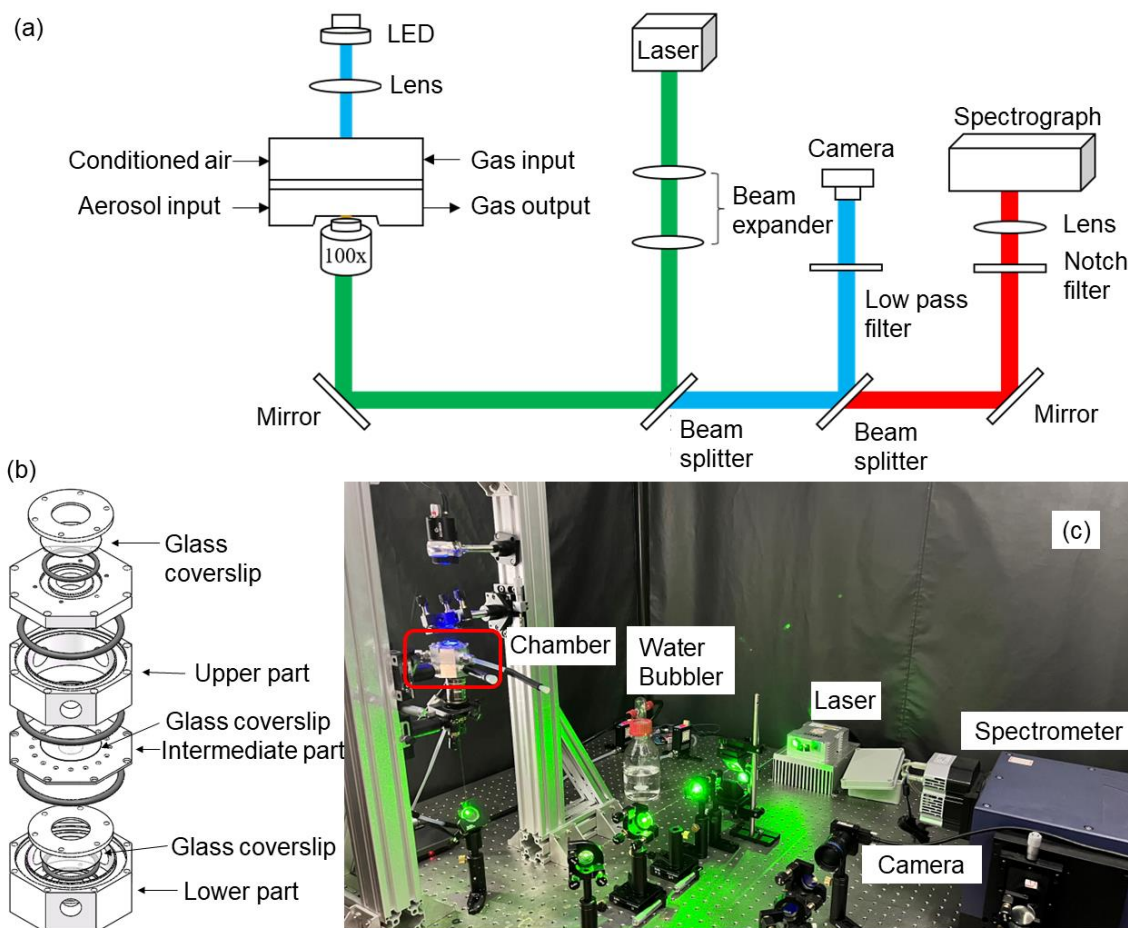

116
 117 **Figure 1. (a) Schematic of the aerosol optical tweezer setup used in this study. (b) Design of the droplet particle levitation chamber.**
 118 **(c) Photo of the main components of the system, including the chamber, water bubbler, laser, camera, and spectrometer.**

119
 120 **2.2 Chamber design**

121 The chamber is designed to provide a sealed environment and to regulate the ambient humidity for the optically trapped droplet,
 122 similar to the chamber design by Gómez Castaño et al. (2019). Our chamber is relatively compact, with a volume of 36 mL,
 123 in contrast to the design by Gorkowski et al. (2016). This smaller size offers several advantages, including improved capture
 124 efficiency. Moreover, we have introduced an innovative double-floor chamber structure. The chamber consists of three main
 125 components: the upper section for introducing RH conditioned airflow and organic aerosol/gas flow, an intermediate plate that
 126 connects the upper and lower compartments for airflow passage, and the lower part for injecting atomized droplets. **The RH**
 127 **measured by the sensor at the outlet of the lower part is used as the actual chamber RH, since this sensor is closed to**
 128 **the droplet trapping position and measures the RH in the lower part.** Both the upper and lower sections feature three ports
 129 for tubing connections. The replaceable intermediate part plays a pivotal role in enhancing the chamber's versatility. Depending
 130 on the specific experimental objectives, the shape, size, and distribution of ventilation holes on the intermediate part can be
 131 customized to control the flow exchange rate. For instance, in experiments involving liquid-liquid phase separation, a flat plate

132 with unobstructed circular holes in the middle is employed to minimize the airflow's impact on liquid droplets. In contrast,
133 during reactivity experiments, the central circular hole is altered from a flat type to a circular barrier type, facilitating better
134 contact between the reactants and the droplet's surface.

135

136 To facilitate the passage of light while preventing the flow of gas, a transparent glass slide is positioned on top of the
137 intermediate section to cover the central holes. This innovative approach allows the illumination LED's light to pass through
138 the window, reaching the trapped particle, while enabling the gas flow to penetrate the intermediate plate through the holes.
139 This design effectively reduces the likelihood of disturbing the stability of particle trapping. In the lower section, the vertical
140 distance between the droplet inlet and the coverslip is set at 6.5 mm. This configuration ensures that atomized droplets can
141 reach the optical trap position in abundance, thereby increasing the probability of successful trapping. Inside the lower part, a
142 glass coverslip is placed and soaked in a surfactant solution (a 50:50 water-to-Decon 90 solution) ~~to prevent droplet deposition.~~
143 The surfactant solution is used to help the deposited droplets to spread on the surface of the coverslip. The openings of the
144 chamber are sealed with O-rings and screws to ensure airtightness. This sealing is applied both between the upper, intermediate,
145 and lower sections, as well as between the window cover, coverslip, and the bottom of the lower part. This design allows for
146 easy disassembly and cleaning of the entire chamber. Under conditions devoid of external disturbances, we are able to stably
147 capture droplets within the chamber for periods exceeding 24 hours.

148 **2.3 Aerosol generation**

149 Aqueous aerosol droplets are created using a medical nebulizer (LANDWIND, PN 100) and can be effectively trapped within
150 30 seconds after introducing the aerosol plume into the chamber. In this study, aqueous NaCl droplets were generated to
151 investigate their response to changes in RH and to assess the accuracy of particle size measurements during the droplet
152 equilibrium experiments. Additionally, mixed droplets containing both NaCl and 3-methyl glutaric acid (3-MGA) were
153 generated to demonstrate the research approach for studying liquid-liquid phase separation (LLPS). Detailed information on
154 each of these experiments is provided below.

155 Following the successful trapping of droplets in the lower layer of the AOT, reaction gases such as ozone and volatile organic
156 compounds (VOC) can be introduced into the chamber. Subsequently, SOA is formed and added to the surface of the droplets
157 through designated ports within the chamber. In this study, both limonene and α -pinene were used as separate SOA precursors.
158 The concentration of limonene within the AOT was controlled by passing dry nitrogen flow over limonene contained in a
159 diffusion vial submerged in a temperature-regulated bath system (Pei et al., 2018). Ozone was generated by passing zero air
160 through a UV lamp unit (SOG-2, UVP). The VOC and ozone reacted in the upper part of the chamber, resulting in the
161 production of SOA particles. These particles settled and subsequently collided with the trapped droplets in the lower section
162 of the chamber.


163 2.4 Detection of the morphology of mixed droplets

164 Droplets exhibit various morphologies in the atmosphere, including homogeneous, partially engulfed, and core-shell
165 morphologies (Song et al., 2013; Veghte et al., 2013). Whispering gallery modes (WGMs), which significantly enhance Raman
166 signals (Ashkin and Dziedzic, 1981), serve as crucial indicators for identifying droplet morphology (Gorkowski et al., 2016;
167 Stewart et al., 2015). These WGMs are observed as distinct peaks superimposed on the broader vibrational modes in the
168 droplet's Raman spectrum. Analyzing the Raman spectrum involves pinpointing the wavelength positions of WGM peaks in
169 the spectrum and fitting these positions to a Mie scattering model. This fitting process allows for the retrieval of the droplet's
170 diameter, denoted as D_p , and its refractive index, represented as n (Preston and Reid, 2013, 2015).

171 Our method for retrieving the values of D_p , and n from the WGMs comprises two essential components: an automatic peak
172 finding algorithm and a Mie scattering fitting program. The peak finding method relies on the `ipeak` code, which was developed
173 by (O'haver, 2022). This approach accurately identifies the desired peaks by smoothing the first derivative of the signal and
174 identifying downward-going zero-crossings that meet specific predefined criteria, such as minimum slope and amplitude
175 thresholds. Once the positions of the WGMs are determined using the peak finding method, we employ the Mie scattering
176 fitting program known as Mie Resonance Fitting (MRFIT), developed by Preston and Reid (2015). MRFIT is utilized to
177 calculate both the diameter and refractive index of a homogeneous droplet. It provides mode assignment information, including
178 the mode number, mode order, and polarization, which is essential for a comprehensive analysis.

179 During the experiment, typically, a homogeneous droplet is initially trapped. Subsequently, as the RH is decreased, the droplet
180 may undergo phase separation and transform into partially engulfed or core-shell morphologies. These transformations have
181 distinct effects on the WGMs. When a droplet transitions into a partially engulfed state, its symmetric structure is disrupted,
182 leading to quenching of the WGMs. In contrast, when the droplet assumes a core-shell structure, the WGMs weaken because
183 the radial uniformity of the droplet is perturbed (Buajarearn et al., 2007; Mitchem et al., 2006). Consequently, applying MRFIT
184 to a partially engulfed or core-shell droplet can render the retrieval of diameter and refractive index implausible, resulting in
185 abnormally high fit errors. To address this issue and retrieve the diameters and refractive indices for core-shell droplets, we
186 employ another program called Mie Resonance Shell Fitting (MRSFIT), developed by [Vennes and Preston \(2019\)](#). MRSFIT
187 is specifically designed to fit observed Mie resonances to the resonances predicted using Mie theory for core-shell particles.
188 The mode assignments provided by MRFIT guide the selection of appropriate parameters for core-shell droplets. After
189 capturing a droplet, its morphology can be identified from the spectra, with examples illustrated in Figure 2.

190

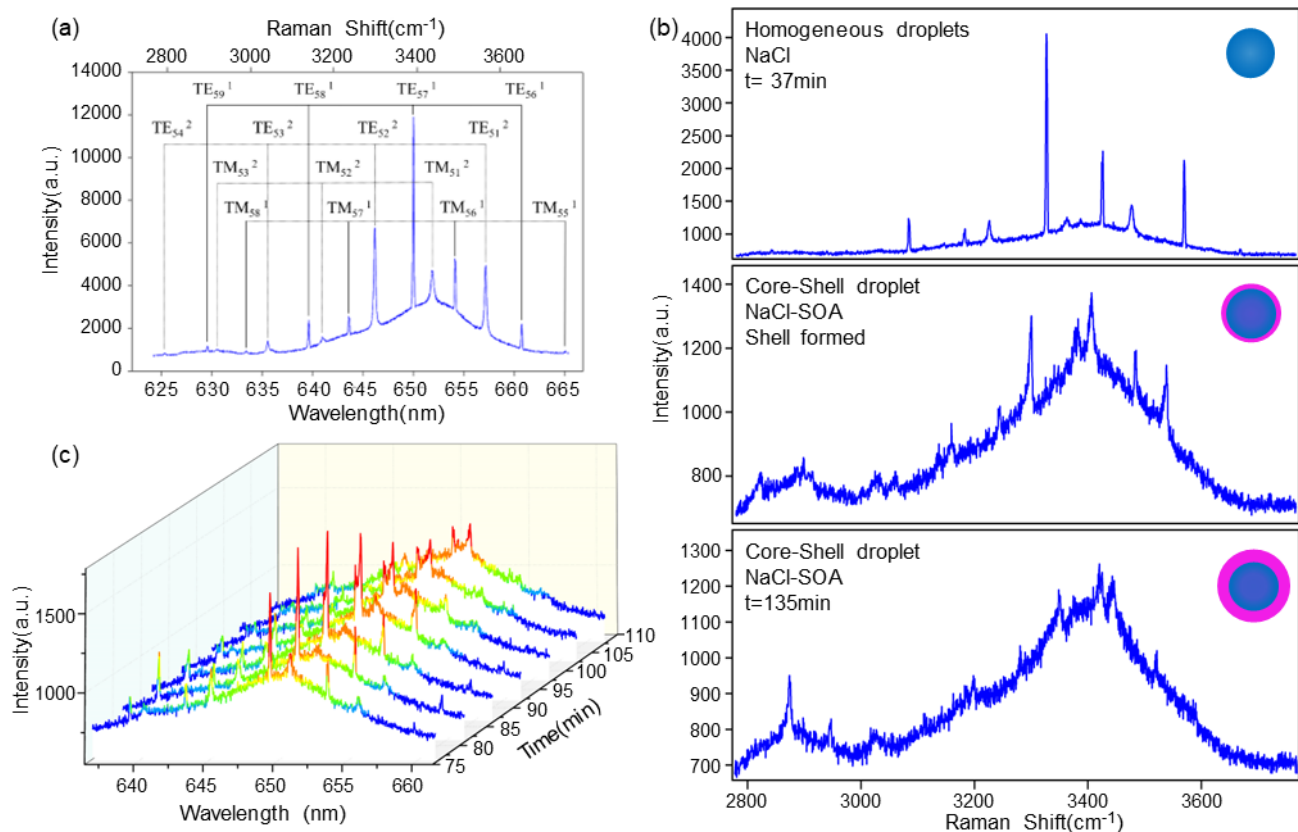

191
 192 **Figure 2. Example of identifying droplet morphology based on spectral features. (a) Example of a Raman scattering signature from**
 193 **a trapped aqueous NaCl droplet. (b) Spectra of different droplet morphologies: Upper subgraph shows the typical spectrum of**
 194 **homogeneous aqueous saturated NaCl droplets. Middle subgraph shows the spectrum when SOA forms a thin shell on the surface**
 195 **of the saturated NaCl droplets. Bottom subgraph shows the spectrum with weakened WGMs peaks when SOA continues to coagulate**
 196 **onto the surface of the saturated NaCl droplets. (c) Example of WGM splitting time series: red peaks gradually split from one into**
 197 **two, and intensity becomes weaker when SOA is added to the droplet, indicating the formation of a core-shell morphology.**

198

199 **3 Results and discussion**


200 **3.1 Performance of trapping chamber**

201 In the initial stages of chamber optimization, a 3D printing technique was employed to create the chamber prototype. However,
 202 for the final chamber design, aluminium was chosen as the construction material instead of 3D printing material. While 3D
 203 printing offers rapid prototyping capabilities, the polymer structure of 3D printing materials can absorb moisture, making it
 204 impractical to maintain a stable RH level within the chamber (Gorkowski et al., 2016). Initially, a single-floor chamber design
 205 was used to achieve successful particle trapping. However, it was challenging to introduce controlled RH flow into the chamber
 206 while maintaining stable droplet trapping. This difficulty arose because the ports on the chamber were located on the sides,
 207 and the flows were delivered directly to the trapping position, thereby disrupting the stability of trapping. Consequently, a
 208 double-floor chamber design was adopted. In this configuration, RH flow is introduced into the upper part of the chamber and
 209 then directed through holes in the intermediate part to reach the lower section. All the experimental data presented in this study

210 were obtained using the double-floor chamber design, which offered improved control over RH conditions and allowed for
211 stable droplet trapping.

212 A saturated aqueous NaCl droplet was trapped to investigate its response to changes in RH. These droplets equilibrate rapidly
213 with variations in the RH of the surrounding air (Gorkowski et al., 2016). When the droplet was successfully trapped, the RH
214 was systematically ramped up and down in approximately 4% steps. This RH cycling ranged from 74% to 98%, and the settings
215 for RH, including the flows of both humid air and dry air, were held constant for 20 minutes at each step. This process of
216 ramping RH up and down was repeated seven times, totaling 31 hours of experimentation. Measurements of RH both before
217 and after the chamber were taken. Simultaneously, Raman scattered light was recorded at intervals of 4 seconds, enabling the
218 calculation of D_p and n through the use of the WGM fitting program known as MRFIT. In Figure 3, the retrieved values for
219 D_p and n , as well as the measured RH before and after the chamber, are displayed. Additionally, the figure provides a time
220 series of Raman spectra for a trapped aqueous NaCl droplet during the first RH cycling experiment. These data offer insights
221 into how the droplet responds to RH variations.

222

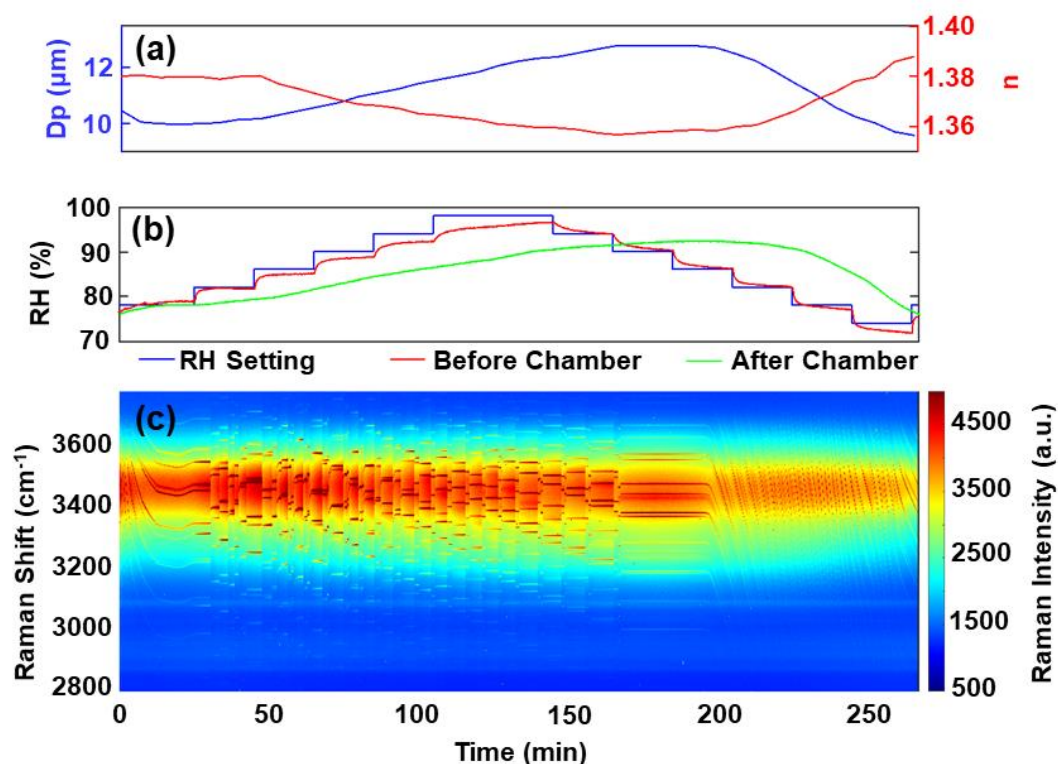

223
224 **Figure 3. (a) Retrieved diameter (D_p) and refractive index (n). (b) RH measured before and after the chamber. (c) Time series of**
225 **Raman spectra for a trapped aqueous NaCl droplet.**


226

227 Figure 3(b) clearly illustrates a significant difference between the RH measurements before and after the chamber. Specifically,
228 the RH measured before entering the chamber closely followed the stepwise setting values, while the RH measured after

229 exiting the chamber exhibited a continuous change with a noticeable lag compared to the RH before entering. When the RH
230 was incrementally increased, the lag between the RH before entering the chamber and the RH after exiting the chamber was
231 20 minutes for an RH of 78% and extended to 80 minutes for an RH of 92%. Conversely, when the RH was decreased, the lag
232 between the RH before entering the chamber and the RH after exiting the chamber was 42 minutes for an RH of 90% and
233 reduced to 20 minutes for an RH of 77%. This observed lag can be attributed to the fact that water vapor can only traverse
234 through the holes in the intermediate part from the upper section to the lower section, which necessitates time for the RH in
235 the lower part to reach the same value as in the upper part. The lag in RH reflects the time required for the chamber's internal
236 conditions to equilibrate with the externally controlled RH levels.

237 Figure 3(c) displays the Raman spectra time series for the trapped aqueous NaCl droplet. This spectrum exhibits the broad O-
238 H vibration mode from water, spanning the range of 3200-3600 cm^{-1} , with sharp WGMs superimposed on top, highlighted in
239 dark red. In Figure 3(a), we observe the retrieved values for D_p and n of the trapped droplet. During the initial 10 minutes of
240 the experiment, the WGM positions blue-shifted to shorter wavelengths (as shown in Figure 3(c)), and the droplet's diameter
241 decreased from 10.47 μm to 9.98 μm . This indicates that the newly nebulized and trapped droplet did not immediately
242 equilibrate with the surrounding air, and water was evaporating from the droplet. Starting from 25 minutes into the experiment,
243 as RH was increased, there was a rapid shift in WGM positions to longer wavelengths within 1 minute. After this initial shift,
244 the positions remained relatively stable, but the intensities of the WGMs increased significantly over the rest of the time.
245 Additionally, there were instances where the WGM positions shifted again abruptly, but the red shift phenomenon was not
246 always observed. Nevertheless, an increase in WGM intensities did occur. This process continued until the RH after exiting
247 the chamber reached its maximum value of approximately 92% and remained stable from 160 minutes to 195 minutes.
248 Subsequently, during the period from 195 minutes to 267 minutes, as RH was decreased, the RH after exiting the chamber
249 gradually declined from 92% to 76%. Interestingly, unlike during the RH increase, there were no abrupt changes in WGMs.
250 Instead, the WGMs consistently shifted to shorter wavelengths, indicating continuous water vapor evaporation from the droplet.
251 This resulted in a decrease in droplet diameter. In general, the trend of D_p correlated well with the RH after exiting the chamber,
252 increasing from 10.0 μm to 12.8 μm as RH increased from 78% to 92%, and decreasing from 12.8 μm to 9.6 μm as RH
253 decreased from 92% to 76%. This suggests that the droplet responded quickly to changes in its surrounding RH. Regarding n ,
254 it exhibited a reverse trend compared to D_p . It decreased from 1.379 to 1.357 as RH increased from 78% to 92%, and increased
255 from 1.357 to 1.388 as RH decreased from 92% to 76%. This indicates that as RH increased, more water molecules were added
256 to the droplet, diluting the NaCl solution and causing the refractive index to approach that of pure water (~ 1.33). This trend
257 aligns with previous studies (Boyer et al., 2020) and demonstrates the effectiveness of the Mie scattering fitting program,
258 MRFIT, developed by Preston and Reid (2015), in providing reasonable and consistent results.

259

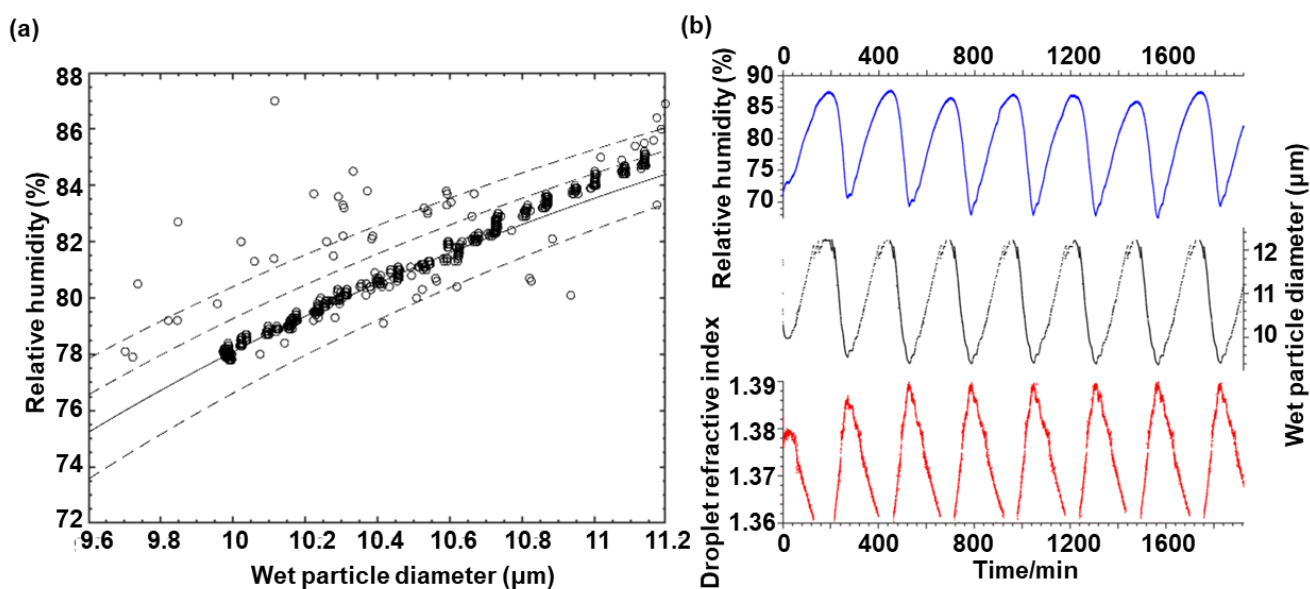


260
 261 **Figure 4. Chamber humidity performance. (a) Comparison between experimental measurements and theoretical calculations of the**
 262 **relationship between wet particle diameter and relative humidity. The lines represent Köhler curves calculated for particles with**
 263 **different diameters: 5.28 μm, 5.38 μm, 5.48 μm, and 5.60 μm from left to right, respectively. The points represent the results obtained**
 264 **using our AOT to observe particles with a 5.48 μm diameter, which is consistent with the predicted result (black solid line). (b) Time**
 265 **series of RH, droplet diameter, and refractive index variation in the chamber.**

266
 267 To assess the accuracy of particle size measurements using the RH balance, the method proposed by Mitchel et al. (2006b)
 268 was employed. This method estimates the particle size of a single droplet by comparing the actual size of the droplet during
 269 equilibrium with the theoretical value calculated using Köhler's theory. In this specific experiment, droplets were generated
 270 using a 0.4 g/mL NaCl aqueous solution, and the results are presented in Figure 4(a). Upon reaching initial equilibrium within
 271 the chamber, the size of the droplet, which initially had a diameter of 9.6 μm, exhibited excellent consistency with the predicted
 272 results based on Köhler's theory for a dry particle with a diameter of 5.48 μm. Figure 4(b) illustrates the variations in droplet
 273 diameter and refractive index within the RH range of 68% to 88% over a span of 32 hours during the droplet equilibrium
 274 experiment. Throughout the process of increasing and decreasing RH, the droplet diameter exhibited a direct proportionality
 275 to RH, while the refractive index displayed an inverse proportionality to RH. These trends highlight how changes in RH
 276 influence the droplet's size and optical properties.

277 3.2 Phase separation of inorganic/ SOA proxy mixed aqueous droplets

278 Droplets were generated using a medical nebulizer (LANDWIND, PN 100) and composed of a mixed saturated solution of
 279 NaCl and trimethyl glutaric acid (3-MGA). The solution had a mass concentration of 100g/L, and the organic-to-inorganic
 280 mass ratio was maintained at 1:1. These droplets, with diameters ranging from 8-12 μm, were subsequently captured using the

281 aerosol optical tweezers. Inside the chamber, the RH was adjusted while Raman spectra were recorded. This allowed for the
 282 monitoring of changes in the droplet's morphology, following the method described in Section 2.4 of the study. The recorded
 283 Raman spectra provided insights into how alterations in RH affected the morphological characteristics of the droplets.
 284

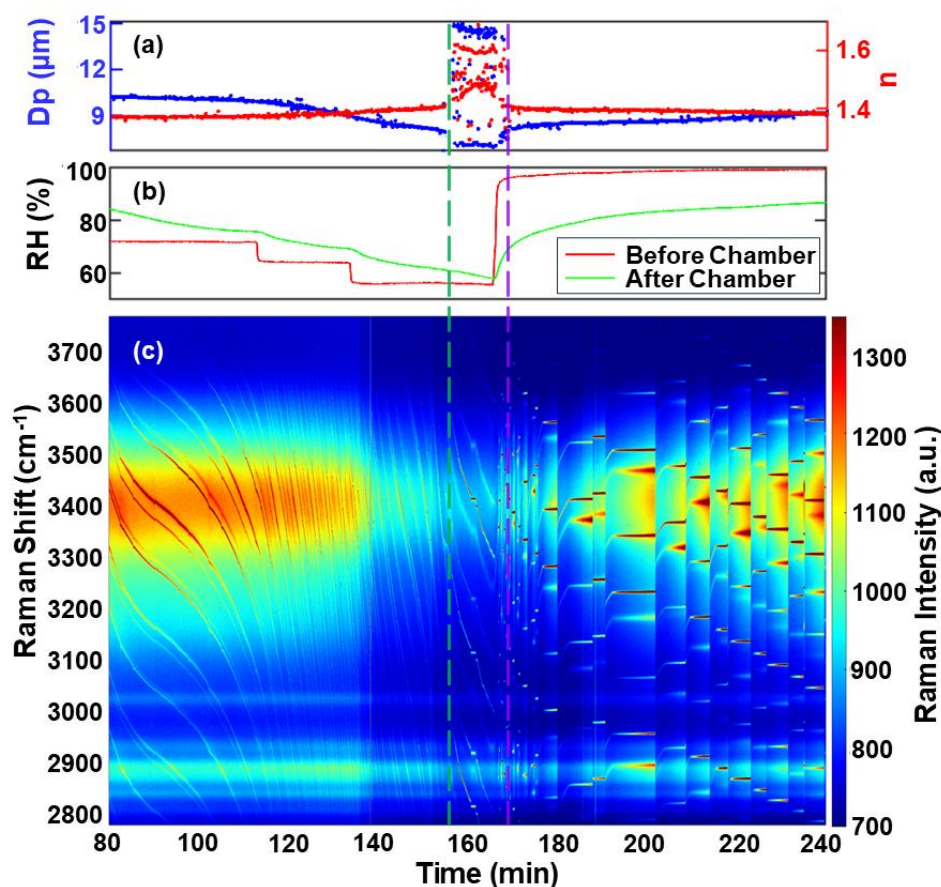

285
 286 **Figure 5. Liquid-liquid phase separation and mixing of a NaCl/3-MGA mixed solution. (a) The droplet diameter and refractive index**
 287 **obtained from WGM fitting, with blue dots representing the droplet diameter and red dots representing the refractive index. (b)**
 288 **The change in RH of the chamber, with red lines representing RH before entering the chamber and green lines representing RH**
 289 **exiting the chamber. (c) Time-resolved Raman spectra, with WGMs marked in dark red. The green dashed line and purple dashed**
 290 **line represent the occurrence of liquid-liquid phase separation and liquid-liquid phase mixing, respectively.**


291
 292 Figure 5 illustrates an experimental example involving the liquid-liquid phase separation and mixing of a NaCl/3-MGA mixed
 293 solution droplet. The experiment began with the chamber's RH being stabilized at 95% for a duration of 20 minutes. During
 294 this phase, the initial droplet diameter was determined to be 11.38 μm , and its refractive index was measured at 1.360.
 295 Subsequently, a RH cycling process was initiated, involving a gradual decrease and then increase in the RH inside the chamber.
 296 During the RH decrease phase, the WGMs shifted towards shorter wavelengths, and the WGM locations exhibited a negative
 297 slope. These observations indicated that the droplet's diameter decreased due to the evaporation of water from within the
 298 droplet. This decrease in diameter resulted in an increase in the solute concentration within the droplet, causing the refractive
 299 index of the droplet to rise. At the 155-minute mark, the WGMs in the Raman spectrum became weakened but did not disappear

300 entirely. Meanwhile, the fitting errors associated with the determination of droplet diameter and refractive index significantly
301 increased. These findings suggested that LLPS had occurred, and a core-shell morphology was formed within the droplet. The
302 separation RH (SRH) for the NaCl/3-MGA mixture was determined to be 61.5%. As the RH was increased during the
303 subsequent phase, the WGMs shifted towards longer wavelengths. When the RH reached 65.5%, the errors associated with the
304 WGMs fitting algorithm returned to the state observed before phase separation, indicating the restoration of a homogeneous
305 state within the droplet. Therefore, the RH level of 65.5% was considered to be the mixed RH (MRH) corresponding to the
306 conditions of the droplet during this experiment.

307 **3.3 Morphology of NaCl droplet coated with SOA**

308 To investigate the morphology of inorganic droplets coated with SOA, SOA precursors such as limonene and α -pinene were
309 oxidized with ozone inside the chamber, generating SOA in situ. Raman-enhanced spectroscopy was used to determine the
310 droplet morphology, revealing that SOA formed a second phase and exhibited a tendency to create a shell on the surface of
311 aqueous droplets. Figure 6 presents an experiment involving droplets coated with limonene SOA. At the start of the experiment,
312 a saturated NaCl droplet was trapped at 0 minutes. The pink stripe in the figure represents the introduction of ozone and
313 limonene into the chamber to generate SOA, with a RH of approximately $73.10 \pm 0.18\%$. The median particle size of the
314 generated SOA particles was measured as 25.67 nm using a scanning mobility particle size (SMPS) instrument. As SOA was
315 introduced into the chamber, the WGMs became weakened but did not completely disappear. Over time, with the continuous
316 introduction of SOA, the SOA shell gradually formed and thickened, disrupting the radial homogeneity of the droplets and
317 leading to the appearance of two phases within the droplet. Consequently, one WGM peak began to split into two peaks (as
318 observed in Figure 2(c) and Figure 6(b)), and the fitting error of the homogeneous Mie algorithm increased (as shown in Figure
319 6(a)). These changes indicated the formation of a core-shell morphology within the droplet. As the organic component content
320 increased due to the presence of SOA, the spontaneous organic peaks in the spectra (in the $2800\text{-}2900\text{ cm}^{-1}$ region) were
321 enhanced. WGMs also emerged in the C-H hydrocarbon region, although they weakened in the OH region. Over time, the
322 intensity of the WGMs peak in the C-H region continued to increase when SOA was continually added, as depicted in Figure
323 6(c). These observations provide insights into the evolving morphology and composition of the droplets as SOA is introduced.


324

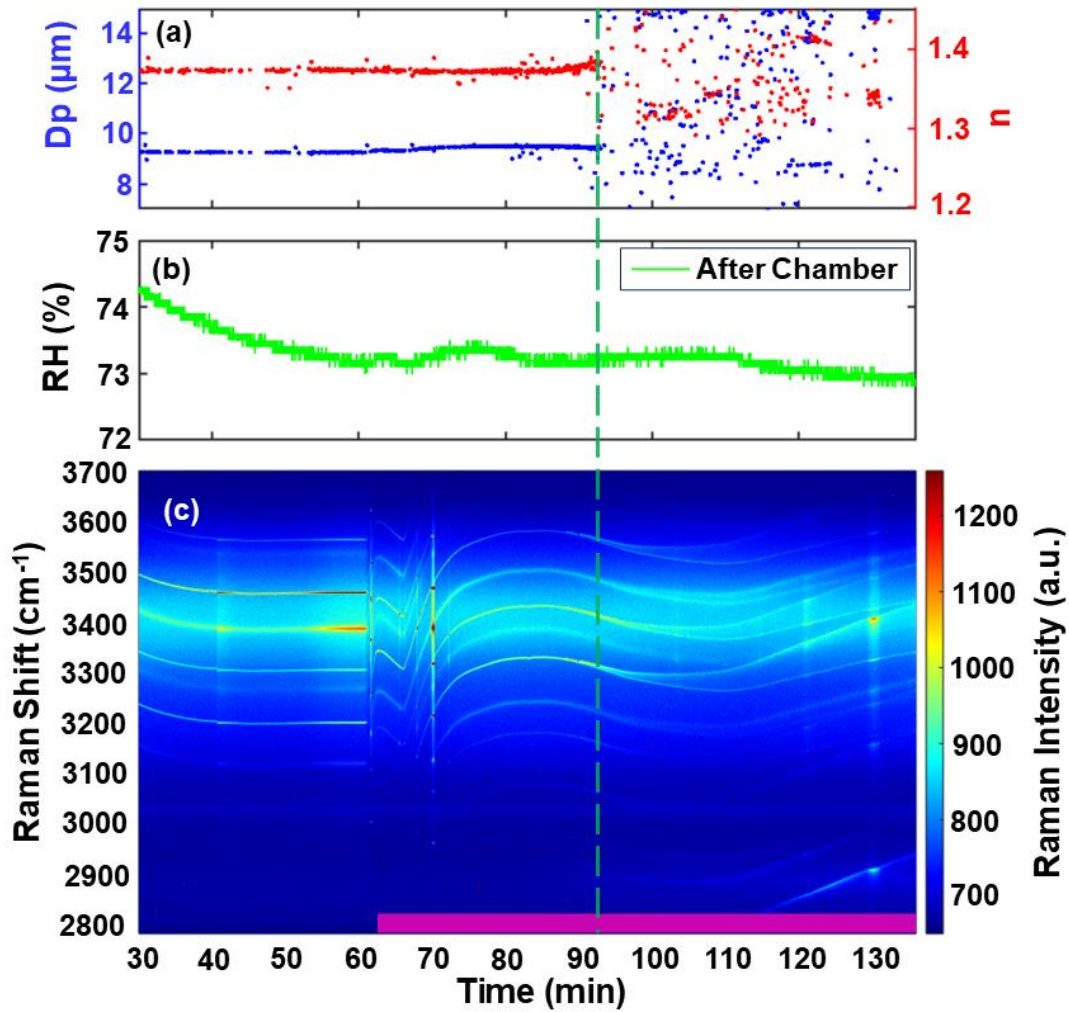

325

326 Figure 6. The experiment of limonene SOA coated on a saturated NaCl droplet. (a) Retrieved diameter (blue dots) and refractive
 327 index (red dots) of the droplet. (b) Relative humidity (RH) of the flow after exiting the chamber. (c) Limonene SOA (purple bar at
 328 the bottom) was added to the droplet, resulting in the formation of a core-shell morphology. The green dashed line indicates the
 329 occurrence of WGM splitting and the formation of a second phase.

330

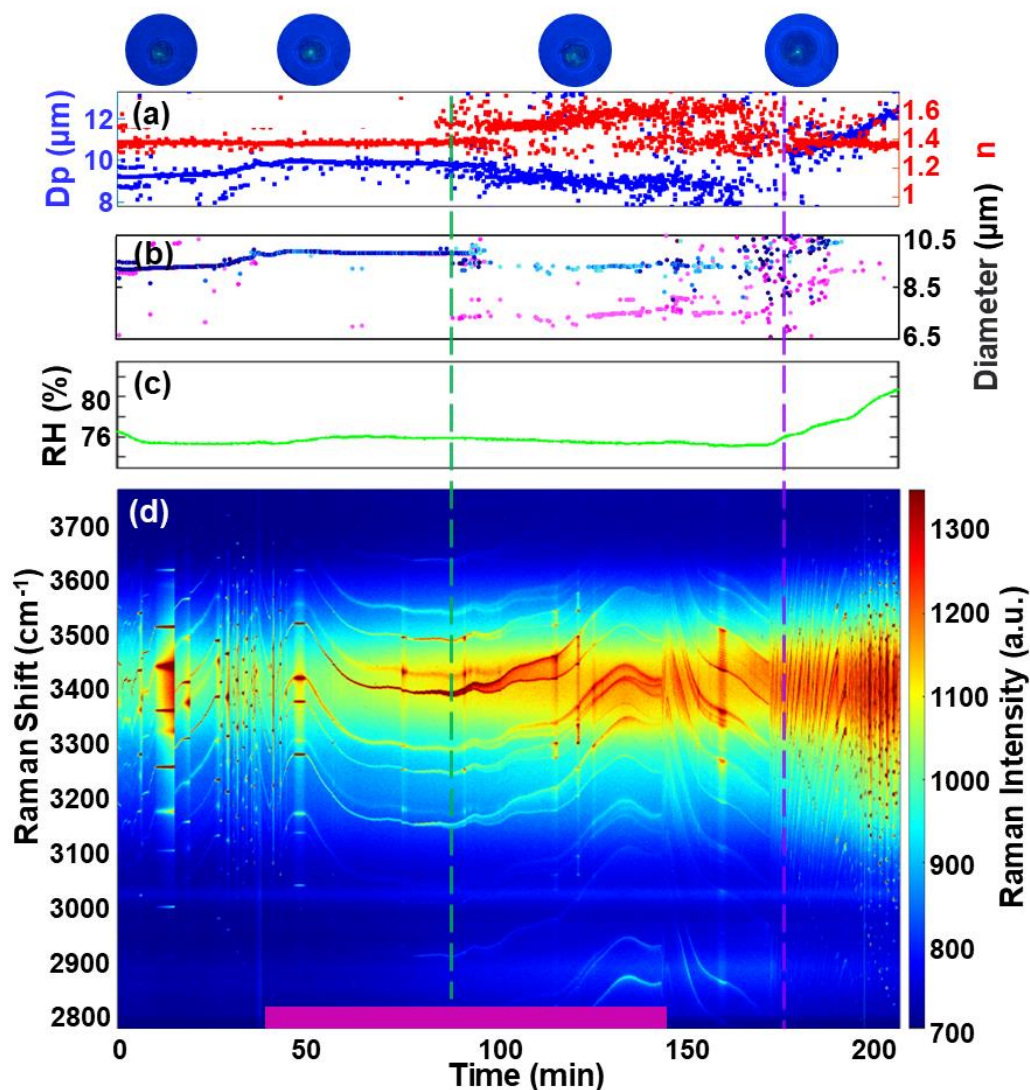

331

332 **Figure 7.** The experiment of α -pinene SOA coated on a saturated NaCl droplet. (a) Retrieved diameter (blue dots) and refractive
 333 index (red dots) of the droplets using the homogeneous droplet model, with real-time images of the droplet at different times. (b)
 334 Retrieved shell diameter (blue dots) and core diameter (red dots) of droplets using the core-shell droplet model. The darker the
 335 color, the smaller the fitting error. Between the green dotted line and purple dotted line, blue dots represent shell diameter, while
 336 pink dots represent core diameter. (c) RH of the flow after exiting the chamber. (d) Limonene SOA (purple bar at the bottom)
 337 was added to the droplet, resulting in the formation of a core-shell morphology. The green dashed line and purple dashed line represent
 338 the occurrence of liquid-liquid phase separation and liquid-liquid phase mixing, respectively.

339

340 Figure 7 presents another experiment involving a droplet coated with α -pinene SOA at a RH of approximately $75.47 \pm 0.29\%$.
 341 Using the same SOA generation conditions, the median diameter of the α -pinene SOA particles was measured at 25.67 nm.
 342 After approximately 40 minutes of introducing SOA into the chamber, significant changes occurred in the WGMs, including
 343 splitting, and the fitting error of the homogeneous Mie algorithm increased significantly. As SOA was generated, ultra-micron
 344 SOA particles formed within the NaCl droplet. This phenomenon can be attributed to the higher polarity of certain compounds
 345 in SOA, which are water-soluble and can dissolve into the aqueous phase (Gong et al., 2018a; Takeuchi et al., 2022; Mutzel
 346 et al., 2021). This behavior has been observed in previous studies using electron microscopy, where the formation of outer

347 shell emulsion droplets in organic/inorganic mixed droplets was observed (Song et al., 2012). Similar phenomena have also
348 been observed in experiments involving AOT (Gorkowski et al., 2017). With continued introduction of SOA, a shell gradually
349 formed on the surface of the aqueous phase of the droplet. To illustrate the development of this shell, a core-shell model
350 developed by Vennes and Preston (2019) was used to calculate the inner core and outer shell diameters of the droplet during
351 the phase addition stage. Eventually, a shell with a thickness of approximately 100 nm was formed (as shown in Figure 7(b)).
352 Some gaps in the data are due to the WGMs' insufficient quality during this stage, which affected the fitting of the core-shell
353 model. The automated peak finding program used may not have recognized WGMs with slightly weaker intensity. Figure 7(b)
354 reveals that before 88 minutes, the core-shell model provided identical values for the fitted core and shell diameters, indicating
355 a homogeneous droplet with no shell. However, after 88 minutes, the difference between the core and shell diameters increased,
356 signifying the development of a core-shell structure within the droplet.

357 Interestingly, the formation of a shell was observed at an RH of 75.47% when α -pinene was used to generate SOA. However,
358 under the same conditions, no shell formation was observed when limonene was used to generate SOA. However, when the
359 RH was reduced to 73.10%, shell formation was observed with limonene SOA. This difference in behavior can be attributed
360 to the chemical properties of the SOA precursors. Limonene contains two double bonds, making it more reactive to ozone and
361 resulting in a higher yield of SOA compared to α -pinene (Chen and Hopke, 2010; Saathoff et al., 2009). Consequently, SOA
362 generated from α -pinene has lower water solubility in saturated NaCl aqueous solution, which explains the different phase
363 states observed in NaCl droplets mixed with α -pinene SOA versus limonene SOA. After introducing α -pinene SOA for 100
364 minutes and stabilizing the droplet for 30 minutes, the RH was increased. When the RH reached 76.20%, the fitting error of
365 the homogeneous Mie algorithm significantly decreased (as shown in Figure 7(a)), indicating a transition from core-shell
366 morphology to a homogeneous morphology. This demonstrates the capability of our AOT to study the water solubility,
367 hygroscopicity, and other properties of SOA. Furthermore, these experimental results align with previous studies (Sullivan et
368 al., 2020), indicating that SOA generated from terpenes tends to form core-shell morphologies during phase separation.

369 **4 Conclusion**

370 In this study, we developed and characterized a new single-beam gradient force aerosol AOT system. A customized droplet
371 particle levitation chamber with a double-floor design was constructed, offering versatility for modifications and enabling
372 rapid droplet trapping. We conducted a comprehensive characterization and performance assessment of this AOT system. Our
373 AOT system demonstrated the ability to efficiently capture micron-sized droplets within 30 seconds, significantly improving
374 capture efficiency. Additionally, the flexibility of the chamber design allowed for adjustments in airflow exchange rate and
375 direction by altering the shape and size of the air holes in the intermediate part, tailored to specific experimental requirements.
376 To evaluate the chamber's performance, we trapped NaCl droplets and used the MRFIT algorithm to retrieve their diameter

377 and refractive index. The experimentally obtained droplet sizes closely matched theoretical values, affirming the chamber's
378 performance. We also investigated the RH-dependent morphology of droplets, using NaCl droplets mixed with 3-MGA to
379 measure SRH and phase MRH. Additionally, we generated and added α -pinene and limonene SOA to inorganic droplets in
380 situ. It is found the formation of a second phase of the droplet occurred, allowing us to study its miscibility and humidity-
381 dependent morphology. Our findings suggest that the AOT system can effectively study the physical and chemical properties
382 of typical atmospheric SOA. Our future research using the new AOT system will explore the interaction between secondary
383 organic matter and various types of trapped droplets, including inorganic salt and organic aerosol droplets.

384

385 **Data availability.** The data used in this paper can be obtained from the corresponding author upon request.

386 **Author contributions.** ZW determined the main goal of this study. XP and YC designed the methods. YC and YM performed
387 the experiments. XP and YM prepared the paper with contributions from all co-authors. ZX, HL and YS participated the
388 building of the AOT system. TP provided the codes for WGM analysis and gives comments. ZX and FZ gave comments.

389 **Competing interests.** At least one of the (co-)authors is a member of the editorial board of Atmospheric Chemistry and Physics.

390 **Acknowledgments.** The study has been supported by the National Natural Science Foundation of China (grant Nos. 91844301,
391 42005086), Key Research and Development Program of Zhejiang Province (grant nos. 2021C03165 and 2022C03084), and
392 the Fundamental Research Funds for the Central Universities (grant no. 2018QNA6008).

393

394

395 **References**

- 396 Ashkin, A. and Dziedzic, J. M.: Observation of optical resonances of dielectric spheres by light scattering, *Appl. Opt.*, 20,
397 1803-1814, 10.1364/AO.20.001803, 1981.
- 398 Boyer, H. C., Gorkowski, K., and Sullivan, R. C.: In situ pH measurements of individual levitated microdroplets using aerosol
399 optical tweezers, *Anal. Chem.*, 92, 1089-1096, 10.1021/acs.analchem.9b04152, 2020.
- 400 Buajarern, J., Mitchem, L., and Reid, J. P.: Characterizing multiphase organic/inorganic/aqueous aerosol droplets, *J. Phys.*
401 *Chem. A*, 111, 9054-9061, 10.1021/jp074366a, 2007.
- 402 Cai, C., Stewart, D. J., Reid, J. P., Zhang, Y.-h., Ohm, P., Dutcher, C. S., and Clegg, S. L.: Organic component vapor pressures
403 and hygroscopicities of aqueous aerosol measured by optical tweezers, *J. Phys. Chem. A.*, 119, 704-718, 10.1021/jp510525r,
404 2015.
- 405 Chan, M. N., Choi, M. Y., Ng, N. L., and Chan, C. K.: Hygroscopicity of water-soluble organic compounds in atmospheric
406 aerosols: amino acids and biomass burning derived organic species, *Environ. Sci. Technol.*, 39, 1555-1562,
407 10.1021/es049584l, 2005.
- 408 Chen, X. and Hopke, P. K.: A chamber study of secondary organic aerosol formation by limonene ozonolysis, *Indoor Air*, 20,
409 320-328, 10.1111/j.1600-0668.2010.00656.x, 2010.
- 410 Combe, N. A. and Donaldson, D. J.: Water evaporation from acoustically levitated aqueous solution droplets, *J. Phys. Chem.*
411 *A.*, 121, 7197-7204, 10.1021/acs.jpca.7b08050, 2017.
- 412 Cremer, J. W., Thaler, K. M., Haisch, C., and Signorell, R.: Photoacoustics of single laser-trapped nanodroplets for the direct
413 observation of nanofocusing in aerosol photokinetics, *Nat. Commun.*, 7, 10941, 10.1038/ncomms10941, 2016.
- 414 Davies, J. F.: Mass, charge, and radius of droplets in a linear quadrupole electrodynamic balance, *Aerosol Sci. Technol.*, 53,
415 309-320, 10.1080/02786826.2018.1559921, 2019.
- 416 Davies, J. F., Haddrell, A. E., Rickards, A. M. J., and Reid, J. P.: Simultaneous analysis of the equilibrium hygroscopicity and
417 water transport kinetics of liquid aerosol, *Anal. Chem.*, 85, 5819-5826, 10.1021/ac4005502, 2013.
- 418 Freedman, M. A.: Liquid-liquid phase separation in supermicrometer and submicrometer aerosol particles, *Acc.Chem. Res.*,
419 53, 1102-1110, 10.1021/acs.accounts.0c00093, 2020.
- 420 Freedman, M. A., Ott, E.-J. E., and Marak, K. E.: Role of pH in aerosol processes and measurement challenges, *J. Phys. Chem.*
421 *A.*, 123, 1275-1284, 10.1021/acs.jpca.8b10676, 2019.
- 422 Gómez Castaño, J. A., Boussekey, L., Verwaerde, J. P., Moreau, M., and Tobón, Y. A.: Enhancing double-beam laser tweezers
423 Raman spectroscopy (LTRS) for the photochemical study of individual airborne microdroplets, *Molecules*, 24, 3325, 2019.
- 424 Gong, Y., Chen, Z., and Li, H.: The oxidation regime and SOA composition in limonene ozonolysis: roles of different double
425 bonds, radicals, and water, *Atmos. Chem. Phys.*, 18, 15105-15123, 10.5194/acp-18-15105-2018, 2018a.

426 Gong, Z., Pan, Y.-L., Videen, G., and Wang, C.: Optical trapping and manipulation of single particles in air: Principles,
427 technical details, and applications, *J. Quant. Spectrosc. Ra.*, 214, 94-119, <https://doi.org/10.1016/j.jqsrt.2018.04.027>, 2018b.

428 Gorkowski, K., Donahue, N. M., and Sullivan, R. C.: Aerosol optical tweezers constrain the morphology evolution of liquid-
429 liquid phase-separated atmospheric particles, *Chem*, 6, 204-220, 10.1016/j.chempr.2019.10.018, 2020.

430 Gorkowski, K., Beydoun, H., Aboff, M., Walker, J. S., Reid, J. P., and Sullivan, R. C.: Advanced aerosol optical tweezers
431 chamber design to facilitate phase-separation and equilibration timescale experiments on complex droplets, *Aerosol Sci. and*
432 *Technol.*, 50, 1327-1341, 10.1080/02786826.2016.1224317, 2016.

433 Kolb, C. E. and Worsnop, D. R.: Chemistry and composition of atmospheric aerosol particles, *Annu. Rev. Phys. Chem.*, 63,
434 471-491, 10.1146/annurev-physchem-032511-143706, 2012.

435 Krieger, U. K., Marcolli, C., and Reid, J. P.: Exploring the complexity of aerosol particle properties and processes using single
436 particle techniques, *Chem. Soc. Rev.*, 41, 6631-6662, 10.1039/C2CS35082C, 2012.

437 Mitchem, L., Buajarn, J., Ward, A. D., and Reid, J. P.: A strategy for characterizing the mixing state of immiscible aerosol
438 components and the formation of multiphase aerosol particles through coagulation, *J. Phys. Chem.*, 110, 13700-13703,
439 10.1021/jp062874z, 2006.

440 Mülmenstädt, J., Sourdeval, O., Delanoë, J., and Quaas, J.: Frequency of occurrence of rain from liquid-, mixed-, and ice-
441 phase clouds derived from A-Train satellite retrievals, *Geophys. Res. Lett.*, 42, 6502-6509,
442 <https://doi.org/10.1002/2015GL064604>, 2015.

443 Mutzel, A., Zhang, Y., Böge, O., Rodigast, M., Kolodziejczyk, A., Wang, X., and Herrmann, H.: Importance of secondary
444 organic aerosol formation of α -pinene, limonene, and m-cresol comparing day- and nighttime radical chemistry, *Atmos. Chem.*
445 *Phys.*, 21, 8479-8498, 10.5194/acp-21-8479-2021, 2021.

446 O'Haver, T. C.: A pragmatic introduction to signal processing with applications in scientific measurement, Kindle Direct 402
447 Publishing, ISBN: 9798611266687, 2022.

448 Pei, X. Y., Hallquist, M., Eriksson, A. C., Pagels, J., Donahue, N. M., Mentel, T., Svenningsson, B., Brune, W., and Pathak,
449 R. K.: Morphological transformation of soot: investigation of microphysical processes during the condensation of sulfuric acid
450 and limonene ozonolysis product vapors, *Atmos. Chem. Phys.*, 18, 9845-9860, 10.5194/acp-18-9845-2018, 2018.

451 Pöschl, U.: Atmospheric Aerosols: Composition, Transformation, Climate and health effects, *Angew. Chem. Int. Ed.*, 44,
452 7520-7540, <https://doi.org/10.1002/anie.200501122>, 2005.

453 Preston, T. C. and Reid, J. P.: Accurate and efficient determination of the radius, refractive index, and dispersion of weakly
454 absorbing spherical particle using whispering gallery modes, *J. Opt. Soc. Am. B*, 30, 2113-2122, 10.1364/JOSAB.30.002113,
455 2013.

456 Preston, T. C. and Reid, J. P.: Determining the size and refractive index of microspheres using the mode assignments from
457 Mie resonances, *J. Opt. Soc. Am. A*, 32, 2210-2217, 10.1364/JOSAA.32.002210, 2015.

458 Reid, J. P., Meresman, H., Mitchem, L., and Symes, R.: Spectroscopic studies of the size and composition of single aerosol
459 droplets, *Int. Rev. Phys. Chem.*, 26, 139-192, 10.1080/01442350601081899, 2007.

460 Rickards, A. M. J., Miles, R. E. H., Davies, J. F., Marshall, F. H., and Reid, J. P.: Measurements of the sensitivity of aerosol
461 hygroscopicity and the κ parameter to the O/C ratio, *J. Phys. Chem. A*, 117, 14120-14131, 10.1021/jp407991n, 2013.

462 Saathoff, H., Naumann, K.-H., Mohler, O., Jonsson, A. M., Hallquist, M., Kiendler-Scharr, A., Mentel, T. F., Tillmann, R.,
463 and Schurath, U.: Temperature dependence of yields of secondary organic aerosols from the ozonolysis of α -pinene and
464 limonene, *Atmos. Chem. Phys.*, 9, 1551-1577, 2009.

465 Shrivastava, M., Cappa, C. D., Fan, J., Goldstein, A. H., Guenther, A. B., Jimenez, J. L., Kuang, C., Laskin, A., Martin, S. T.,
466 Ng, N. L., Petaja, T., Pierce, J. R., Rasch, P. J., Roldin, P., Seinfeld, J. H., Shilling, J., Smith, J. N., Thornton, J. A., Volkamer,
467 R., Wang, J., Worsnop, D. R., Zaveri, R. A., Zelenyuk, A., and Zhang, Q.: Recent advances in understanding secondary organic
468 aerosol: implications for global climate forcing, *Rev. Geophys.*, 55, 509-559, <https://doi.org/10.1002/2016RG000540>, 2017.

469 Song, M., Marcolli, C., Krieger, U. K., Lienhard, D. M., and Peter, T.: Morphologies of mixed organic/inorganic/aqueous
470 aerosol droplets, *Faraday Discuss*, 165, 289-316, 10.1039/c3fd00049d, 2013.

471 Song, M., Marcolli, C., Krieger, U. K., Zuend, A., and Peter, T.: Liquid-liquid phase separation and morphology of internally
472 mixed dicarboxylic acids/ammonium sulfate/water particles, *Atmos. Chem. Phys.*, 12, 2691-2712, 10.5194/acp-12-2691-2012,
473 2012.

474 Stewart, D. J., Cai, C., Nayler, J., Preston, T. C., Reid, J. P., Krieger, U. K., Marcolli, C., and Zhang, Y. H.: Liquid-liquid
475 phase separation in mixed organic/inorganic single aqueous aerosol droplets, *J. Phys. Chem. A*, 119, 4177-4190,
476 10.1021/acs.jpca.5b01658, 2015.

477 Sullivan, R. C., Gorkowski, K., and Jahn, L.: Chapter 12 - Characterization of individual aerosol particles, in: *physical*
478 *chemistry of gas-liquid interfaces*, edited by: Faust, J. A., and House, J. E., Elsevier, 353-402, [https://doi.org/10.1016/B978-](https://doi.org/10.1016/B978-0-12-813641-6.00012-1)
479 [0-12-813641-6.00012-1](https://doi.org/10.1016/B978-0-12-813641-6.00012-1), 2018.

480 Sullivan, R. C., Boyer-Chelmo, H., Gorkowski, K., and Beydoun, H.: Aerosol optical tweezers elucidate the chemistry, acidity,
481 phase separations, and morphology of atmospheric microdroplets, *Acc. Chem. Res.*, 53, 2498-2509,
482 10.1021/acs.accounts.0c00407, 2020.

483 Takeuchi, M., Berkemeier, T., Eris, G., and Ng, N. L.: Non-linear effects of secondary organic aerosol formation and properties
484 in multi-precursor systems, *Nat. Commun.*, 13, ARTN 788310.1038/s41467-022-35546-1, 2022.

485 Veghte, D. P., Altaf, M. B., and Freedman, M. A.: Size dependence of the structure of organic aerosol, *J. Am. Chem. Soc.*,
486 135, 16046-16049, 10.1021/ja408903g, 2013.

487 Vennes, B. and Preston, T. C.: Calculating and fitting morphology-dependent resonances of a spherical particle with a
488 concentric spherical shell, *J. Opt. Soc. Am. A. Opt. Image. Sci. Vis.*, 36, 2089-2103, 10.1364/JOSAA.36.002089, 2019.

489 Zuend, A. and Seinfeld, J. H.: Modeling the gas-particle partitioning of secondary organic aerosol: the importance of liquid-
490 liquid phase separation, *Atmos. Chem. Phys.*, 12, 3857-3882, 10.5194/acp-12-3857-2012, 2012.