

Evaluation of Aeris MIRA, Picarro CRDS G2307, and DNPH-based sampling for long-term formaldehyde monitoring efforts

Asher P. Mouat¹, Zelda A. Siegel¹, Jennifer Kaiser^{1,2}

¹School of Civil and Environmental Engineering, Georgia Institute of Technology, Atlanta, Georgia 30332, USA

²School of Earth and Atmospheric Sciences, Georgia Institute of Technology, Atlanta, Georgia 30332, USA

Correspondence to: Jennifer Kaiser (Jennifer.kaiser@ce.gatech.edu)

Abstract.

10 Current formaldehyde (HCHO) measurement networks rely on the TO-11A offline chemical derivatization technique, which can be resource intensive and limited in temporal resolution. In this work, we evaluate the field performance of three new commercial instruments for continuous in-situ formaldehyde monitoring: the Picarro cavity ringdown spectroscopy G2307 gas concentration analyzer and Aeris Technologies' mid-infrared absorption Pico and Ultra gas analyzers. All instruments require regular drift correction which is accomplished through instrument zeroing using
15 DNPH-coated cartridges, Drierite, or molecular sieves while heated hopcalite failed to remove all incoming HCHO. We show that a modified precision estimate accounting for regular instrument zeroing results in values of 0.09 ppb, 0.20 ppb, and 0.22 ppb at a 20 min integration time for the G2307, Ultra, and Pico, respectively. After applying standard addition and dynamic dilution calibrations, all instruments agreed within 13 % and were well correlated with each other (all $r \geq 0.90$). TO-11A HCHO observations resulted in a normalized mean bias of -58% compared to co-
20 located Picarro G2307 measurements ($r = 0.62$, slope = 0.38, int = 0.07 ppb HCHO). Using a 6-month deployment period in the Atlanta metropolitan area, we determined that the Picarro G2307 and Aeris units have sufficient accuracy and precision to capture the Atlanta spatial HCHO gradient. We find that midday HCHO concentrations have decreased by 22.3 % since 1999 in the city's urban core, and DNPH measurements at a nearby PAMS site show a greater decrease of 53 %.

25 1 Introduction

Observations of formaldehyde (HCHO) provide useful insight into the photochemical formation of secondary pollutants and the sources and fate of volatile organic compounds (VOCs). While direct emissions of HCHO from wildfires, the biosphere, and anthropogenic activities can contribute to ambient mixing ratios (Parrish et al., 2012; Lui
30 et al., 2017; Luecken et al., 2018; Alvarado et al., 2020; Wu et al., 2021), regional HCHO abundance is generally governed by secondary production (Parrish et al., 2012; Zhang et al., 2013; Zhu et al., 2014; Luecken et al., 2018; Zeng et al., 2019). Because HCHO photolysis and oxidation are sources of HO_x radicals, HCHO loss can further propagate oxidative chemistry (Tonnesen and Dennis, 2000; Lin et al., 2012; Valin et al., 2016; Wolfe et al., 2019;

35 Yang et al., 2021). Additionally, HCHO is a known carcinogen ranking highest in health risks among the 187
hazardous air pollutants listed by the US Environmental Protection Agency (EPA) in the Clean Air Act (Scheffe et
al., 2016; Strum and Scheffe, 2016; Zhu et al., 2017b). Due to its central role in atmospheric chemistry, HCHO is a
target molecule at EPA Photochemical Assessment Monitoring Station (PAMS) and National Air Toxics Trends
Station (NATTS) network sites for which observations are typically included in chemically comprehensive field
intensives.

40 Since 1990, the standard EPA approach for HCHO measurements is collection on 2,4-dinitrophenylhydrazine (DNPH)
coated cartridges followed by offline derivative detection via high performance liquid chromatography (HPLC),
known as the TO-11A method (U.S. Environmental Protection Agency, 1999). Sample collection and analysis are
resource and labor intensive with measurements typically reported over sampling times that are on the order of hours.
45 EPA TO-11A measurements in the PAMS and NATTS are 8 or 24 h integrated samples collected every three or six
days, respectively. The low time resolution limits the usefulness of observations for studies of both photochemistry
and air toxics exposure. Previous approaches have used modelled diel cycles or satellite-based observations in
combination with the TO-11A method to infer ground-based diel cycles (Zhu et al., 2017a; Zhu et al., 2017b; Wang
et al., 2022). However, this DNPH method of capturing HCHO has known interferences from NO₂ and O₃ (Karst et
50 al., 1993; Achatz et al., 1999; Tang et al., 2004), can be impacted by relative humidity (RH) (Wisthaler et al., 2008;
Uchiyama et al., 2009; Ho et al., 2014), and has had mixed results in comparison to research-grade observations (Hak
et al., 2005; Wisthaler et al., 2008; Dunne et al., 2018), making the accuracy of these inferred diel cycles difficult to
determine. While other studies have demonstrated the feasibility for continuous measurements via various
spectroscopy-based methods (Yokelson et al., 1999; Cardenas et al., 2000; Dasgupta et al., 2005; Hak et al., 2005;
55 Spinei et al., 2018; St Clair et al., 2019; Dugheri et al., 2021), the number of multi-month, ground-based, continuous,
in-situ HCHO measurements is limited to a handful of studies, all of which a proton-transfer-reaction mass
spectrometer (Warneke et al., 2013; Hansen et al., 2014; Coggon et al., 2021).

A HCHO monitoring instrument more suitable for long-term deployment would reduce manual labor and provide
60 continuous observations, experience little or correctable drift in instrument baseline and sensitivity, and have low
uncertainty and sufficient precision at typical ambient concentrations. In recent years, several commercially available
instruments have been developed towards that goal, including a cavity ring down spectroscopy (CRDS) instrument
from Picarro, a photoacoustic gas analyser from Gasera, and Tunable Diode Laser Spectroscopy (TDLS) instruments
from Aeris Technologies and Aerodyne Research, Inc. Here, we focus on the Aeris mid-infrared absorption (MIRA)
65 and Picarro CRDS G2307 instruments, which have been compared against other instruments in a small number of
informal (Whitehill et al., 2018; Furdyna, 2020) and peer-reviewed (Shutter et al., 2019; Glowania et al., 2021)
intercomparison efforts. Glowania et al. (2021) is the only peer-reviewed work to employ a G2307 using the current
spectral fitting algorithm (version 1.6.015), which updates the procedure for fitting at low-humidity. The Aeris Ultra,
which offers improved thermal stabilization over the Aeris Pico, has not previously been examined in literature.
70 Whereas previous comparisons were conducted either in controlled chamber studies or through analysis of short-term

ambient observations, a full characterization of instrument suitability in measurement networks requires multi-month deployment.

75 Previous intercomparisons involving either Aeris MIRA or Picarro CRDS instruments have highlighted concerns with measurement accuracy as a function of ambient humidity. The Aeris MIRA technique relies on a HDO line (located at $2931.8413 \text{ cm}^{-1}$) for spectral referencing. At low humidity ($<0.2 \text{ \% H}_2\text{O}$), the Aeris Real-Time (ART) fitting algorithm cannot reliably reference its HDO spectral feature and the instrument fails to produce measurements (Shutter et al., 2019). Including CH_4 as a secondary spectral reference in data post-processing extends the range of conditions under which the Aeris instruments work, though the instrument's precision decreases by a factor of 1.2 ± 0.3 . While 80 the G2307 fitting algorithm uses both H_2O and CH_4 spectral references, CH_4 fitting currently remains a research approach for ART. Whitehill et al. (2018) found an inverse correlation between Picarro HCHO measurements and instrument-reported water mixing ratios at typical ambient concentrations and, along with Furdyna (2020), observed that the G2307's measurements were lower by 1-2 ppb HCHO compared to DNPH-based measurements. Glowania et al. (2021) found that variable humidity can decrease reported HCHO concentrations by as much as 1.75 ppb with 85 the most significant offsets at $\leq 0.2\% \text{ H}_2\text{O}$ where the H_2O spectral feature is not clearly observed.

Both Picarro and Aeris instruments periodically sample HCHO-free air to determine an instrument baseline. Several scrubbers are capable of removing HCHO – the most common of which are DNPH-coated cartridges (DNPH), heated catalytic hydrocarbon scrubbers like oxides of copper and manganese (hopcalite, HO), calcium sulfate (Drierite, DR), 90 and molecular sieves (MS) (Herndon et al., 2007; Cazorla et al., 2015; Pei et al., 2015; Shutter et al., 2019; St Clair et al., 2019; Fried et al., 2020). These methods differ in removal mechanism, molecular selectivity, and desiccation efficiency. DNPH-coated cartridges are recommended by Aeris Technologies, and are chemically selective for carbonyls, thus allowing the majority of H_2O to pass through. Heated HO is expected to oxidize HCHO to CO, forming H_2O as a by-product and providing a humidified airstream that may also be suitable for baseline determination. Picarro 95 Inc. recommends instrument zeroing via adsorption by DR. A column of MS is often plumbed in upstream of a DR column (DR+MS) as it both desiccates the gas flowing through it and, with the right pore size, removes molecules with kinetic diameters greater than that of HCHO. This both prevents the DR from becoming saturated and prolongs its HCHO-removal efficiency as only smaller organic compounds can adsorb to it. HO and DR+MS may be less cost-intensive, longer-lasting, and have comparable HCHO-removal efficiency to DNPH-coated cartridges. However, since 100 humidity is known to impact HCHO concentrations, impact of scrubber choice on overall measurement accuracy is unclear.

We use HCHO measurements taken over one year in Atlanta, GA from the Picarro G2307 and the Aeris instruments with aims to determine best calibration procedures, optimal measurement configurations, and to assess suitability for 105 remote, continuous operation. We compare co-located observations from all three monitors as well as observations from the Picarro G2307 and TO-11A DNPH analysis. For each continuous monitor, we assess the performance over a range of zeroing methods and ambient humidities. Finally, we demonstrate the use of Picarro G2307 and Aeris Ultra

and Pico measurements for long-term, continuous observations of HCHO spatial gradients in an urban environment and discuss the feasibility of deploying these instruments to form a spatiotemporally comprehensive network.

110

2 Instrument Description

2.1 Picarro G2307

115

2.1.1 CRDS operating principles

The operating principle of cavity ringdown spectroscopy as used by the G2307 is described fully in Glowania et al. (2021), and briefly summarized here. Air is pulled through a temperature and pressure-controlled cavity at a rate of 0.4 standard liters per minute (SLPM). Laser light is directed into the resonance cavity, where three high-reflectivity mirrors create effective pathlengths on the kilometer scale. After the laser is shut off, the small amount of light transmitted through one mirror is monitored via photodetector. Detected light exponentially decays, with faster decay rates corresponding to higher absorption of light in the cavity. An on-board wavelength monitor measures the absolute laser wavelength with a precision that is three order of magnitude narrower than the HCHO spectral linewidth. The instrument can change the voltage applied to the laser and tune it to wavelengths that HCHO is known to either minimally or maximally absorb at, producing closely clustered spectral features at and around the HCHO absorption peak. The laser scans the 5625.5 to 5626.5 cm^{-1} wavelength range at 100 Hz repetition rate, while the length of the cavity is adjusted to achieve resonance. On-board spectral fitting and signal averaging results in measurements of HCHO, CH_4 , and H_2O reported at 1 Hz. The unit assessed in this work utilizes the same spectral fitting algorithm described in Glowania et al. (2021).

120
125
130

2.1.2 Determining instrument baseline

The G2307 measurements reported here differ from prior studies primarily in that we employed an external zeroing system. The system is equipped to sample from either DNPH (Supelco LpDNPH S10L), DR (Drierite, 8 mesh, >98% CaSO_4 , <2% CoCl_2), or DR+MS (Sigma Aldrich Molecular Sieve, 0.3 nm zeolite beads) to regularly monitor and correct the instrument's baseline. Baseline is defined throughout this work as the signal reported by the instrument when sampling from a HCHO-free source and drift as the rate of change of the baseline. This setup was accomplished by connecting the G2307 inlet to a 3-way PFA solenoid valve which alternated between an ambient sampling line and a zeroing line. The zeroing line was then connected to another 3-way PFA solenoid valve to which the scrubbers were attached. The instrument sampled from DR or DR+MS for 5 min of every hour. Every fourth hour, the instrument sampled for 5 min through DNPH either directly before or after sampling from DR. The relative order of DR/DNPH sampling was found to have no impact on reported instrument baselines.

135
140

2.1.3 Humidity-dependence

Two trials were performed to quantify the impact of humidity on G2307 measurements. HCHO-free air was provided by either a zero-air (ZA) generator (Tofwerk) with DR column (trial 1) or an ultra ZA cylinder (trial 2). A portion of the ZA stream was humidified by using a bubbler containing Milli-Q water. The fraction of ZA humidified was varied using a mass flow controller such that measured H₂O concentrations ranged from 0.05-1.7%.

Fig. 1 shows the reported HCHO concentrations in HCHO-free air as a function of measured % H₂O. As reported in Glowania et al. (2021), data fell into two linear regimes with a demarcation at 0.2 % H₂O. Data were averaged to 5 minutes and each regime fitted using a York regression (York et al., 2004) with standard deviations of the measurements used as uncertainty. We find significantly smaller slopes (lower H₂O influence) than Glowania et al. (2021), indicating that humidity-dependencies may be instrument-specific. The HCHO offset is defined in Eqn. 1:

$$[HCHO]_{offset} = \begin{cases} (-5.67 \pm 0.47) * [H_2O] + (0.13 \pm 0.02), \% H_2O < 0.2 \\ (-0.40 \pm 0.02) * [H_2O] - (0.01 \pm 0.02), \% H_2O \geq 0.2 \end{cases} \quad (1)$$

where $[HCHO]_{offset}$ (ppb) accounts for the HCHO signal lost at some % H₂O and $[H_2O]$ is the corresponding instrument-reported % H₂O mole fraction.

Depending on the instrument zeroing method, ambient and baseline humidities may be very different. These differences could lead to significant biases in reported HCHO differential measurements. For example, Fig. 1 suggests the use of a dessicant such as DR, for sampling ambient air at 1% H₂O would generate a bias of -0.4 ppb if the humidity dependence is not corrected. We emphasize the importance of experimentally determining a correction factor for humidity-effects before deployment.

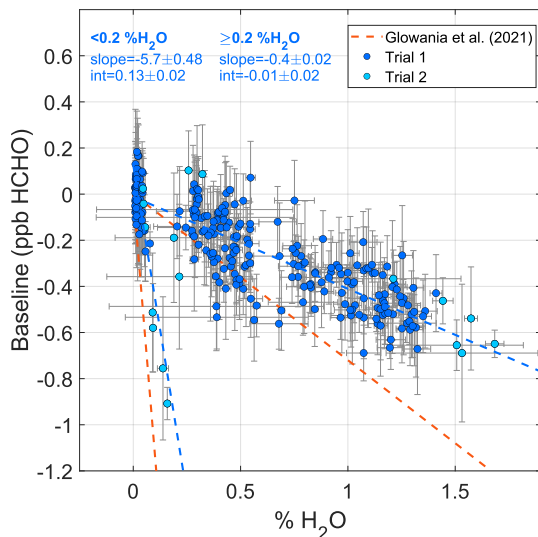


Figure 1 – Picarro G2307 HCHO concentrations as a function of measured H₂O concentrations. Regressions for the two H₂O spectral fitting regimes are plotted alongside the slopes from Glowania et al. (2021). Error bars are the standard deviation in instrument baseline or % H₂O for each 5 min averaged point.

175

2.1.4 Data processing

Averaged HCHO datasets at variable time resolutions (1 – 60 min) were created from the 1 Hz data using the following procedure: first, all 1 Hz data were corrected for humidity-effects by subtracting the $[\text{HCHO}]_{\text{offset}}$ from Eqn. 1. Observations made within 30 s of a valve change were removed and baseline measurements were then averaged to 4.5 min points and linearly interpolated to create an instrument background on the same time basis as ambient data. The interpolated baseline was subtracted from the 1 Hz ambient measurements. Baseline-corrected ambient data were averaged to the desired time resolution with any periods having <50 % data completeness discarded. Data was further screened to exclude points where scrubbers were exhausted and therefor unreliable.

185

2.1.5 Impact of scrubber choice – DNPH, DR, and DR+MS

Before comparing scrubbers, we first examine the HCHO-removal efficiency of DNPH compared to a ZA generator. We find instrument baselines were on average 14 ppt larger than those measured using a ZA generator. This difference was consistent whether sampling the indoor conditions or ambient air. This difference is not statistically significant given the instrument precision and accuracy determined later in Sect. 3. We note DNPH initially off-gases material that produces spectral interferences that subside after a “burn-in” period of ~2 hrs. It’s possible that off-gassing material could have negative effects on instrument performance if used long-term (e.g., mirror degradation). These impacts were not seen in our study and would require further investigation.

195

The impact of DR and DR+MS on the Picarro G2307’s baseline was then assessed using ambient measurements taken from the consecutive sampling of DNPH and DR/DR+MS in the ambient sequencer schedule. We combine the DR and DR+MS measurements as we find the two methods produce baselines with a relative difference that is within instrument measurement uncertainty. The 4.5-min averaged baselines are shown in Fig. 2. Both scrubbing methods produced normally distributed baseline measurements with means and standard deviations of -0.39 ± 0.14 ppb (DNPH) and -0.38 ± 0.15 ppb (DR/DR+MS), and an average absolute difference of <0.03 ppb HCHO. This difference is finer than the 5 min precision of the instrument and demonstrates a comparable performance between the two scrubbing methods.

205

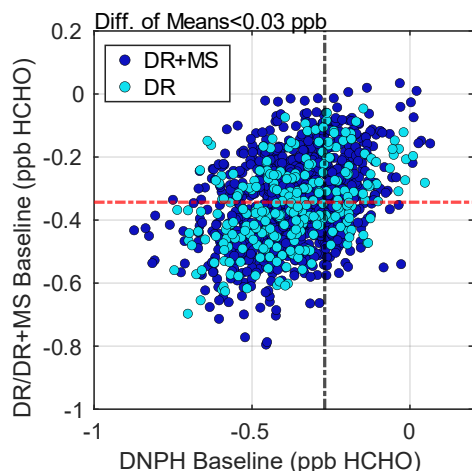


Figure 2 – Picarro G2307 baselines determined using the DR, DR+MS, or DNPB scrubbing methods. Each data point represents a consecutive, 4.5-min averaged DNPB and DR baseline measurement.

210 Previous studies have noted that derivatization of hydrazine to hydrazone, which is the reaction that functionally captures HCHO in the DNPB-coated cartridge, is slowed or stopped at RH < 15 % (Wisthaler et al., 2008; Uchiyama et al., 2009). Few days throughout the G2307’s deployment fell below this threshold, and RH (converted from instrument-reported % H₂O using indoor conditions) was always ≥ 25 %. While low RH likely did not affect our measurements, we note this is a limitation on DNPB as deployment in arid locations could hamper performance whereas DR/DR+MS would operate unaffected.

220 Ho et al. (2014) found that high temperatures (>22 °C) and RH (>50%) led to DNPB-HPLC analysis underestimating ambient HCHO by 35-80%. This could inflate instrument baselines as summer 2022 in Atlanta regularly exceeded these values, with DNPB-derived baselines in Fig. 2 having RH values in the range of 7-87%. As DR-baselines are determined using desiccated air and the average baseline difference with DNPB is within instrument precision, we conclude measurements are not significantly affected at high RH. These results lead us to conclude that either DR/DR+MS or DNPB usage with the G2307 is advisable so long as humidity corrections are applied.

225 **2.1.6 Instrument calibration**

Single-point and dynamic dilution calibrations were conducted at the beginning, middle, and end of the G2307’s deployment. Single-point calibrations were performed by flowing a concentrated standard (either Apel Riemer: 1015 ppb ± 5%, Airgas: 1031 ppb ± 10%, or Airgas: 1044 ± 10%) through a silonert-coated stainless steel (SS) regulator and directly into the instrument. This configuration avoids interaction between the calibration gas and stainless steel surfaces, thereby reducing passivation times to sub-hour lengths. However, this technique relies on the assumption that observations are linear from 0-1 ppm HCHO. The single-point measured concentration was determined as the instrument-reported concentration multiplied by an N₂/air matrix conversion factor of 1.0625 (Bent, 2023).

235 Dynamic dilution calibrations were performed by diluting the HCHO standards with ZA from either a Tofwerk ZA
generator or an ultra ZA cylinder. After a 5 hr passivation time at ~200 ppb HCHO, concentrations were varied in the
0-40 ppb range. Each concentration step was 3 h in duration with 5 min zeroing periods conducted hourly.

240 Slopes from all calibrations (single-point, dynamic dilution, and original factory calibration) agreed within 10 %, with
no systematic bias between calibration method. This indicates both that G2307 measurements are linear up to a ppm
range and that sensitivity remained stable during the 2021-2023 period. Ambient measurements are processed
according to the temporally closest calibration. We determine the uncertainty in ambient measurements to be 10 %
per the uncertainty associated with the standards used for calibration.

245

2.2 Aeris MIRA

2.2.1 MIRA operating principles

250 The operating principle of the Aeris MIRA instruments is described fully in Shutter et al. (2019). Air is pulled at a
rate of 0.45 – 0.75 SLPM into a folded Herriott detection cell, which achieves a path length of 13 m. The laser scans
over the HCHO feature at $2831.6413 \text{ cm}^{-1}$, as well as the nearby HDO spectral feature at $2831.8413 \text{ cm}^{-1}$. The ART
algorithm corrects for broad slope in the raw signal of the instrument baseline, and then calculates measured HCHO
and H₂O concentrations based on absorption features. We use the two commercial Aeris MIRA models in this work:
255 the Pico and the Ultra model. The Ultra is identical in operation but offers higher optical cell temperature stability and
is designed for longer-term, low-drift measurements.

2.2.2 Instrument baseline

260

The Aeris instruments have a two-inlet design allowing for determination of instrument baseline throughout the data
collection process. We run the instruments in the “programmed” mode, which allows the user to select the duration of
sampling through each inlet. The instruments also have a “differential” mode, which produces ambient HCHO
concentrations using on-board baseline subtractions. The zero inlet was connected to either DNPH-coated cartridge
265 or a heated HO (United Filtration) scrubber and teed with the ambient inlet to the main sampling line per the
manufacturer’s recommendation. We sample ambient air for 180 s and scrubbed air for 30 s. This sequence was
determined through visual inspection of Aeris time series with the intention of minimizing DNPH-sampling time while
maintaining sufficient precision for ambient monitoring. We found 180 s to be the longest length of time between
zeroes that either unit achieved where the remained consistently stable. Both units were then set to the same schedule.

270 This led to DNPH-coated cartridges lasting 5-8 days, corresponding to a breakthrough time of 17 – 27 h. Variability
in breakthrough time is dependent on ambient conditions and atmospheric chemical composition.

2.2.3 Impact of scrubber choice – heated HO and DNPH for Aeris MIRA

275 Stated previously, the Aeris ART fitting algorithm requires the presence of H₂O as a spectral reference for finding the
HCHO absorption peak. We therefore do not consider desiccating scrubbers as an option. Throughout deployment,
the Aeris instruments reported an ambient range of 0.18-3.3 % H₂O while sampling through DNPH with only a few
days in winter falling below the 0.2 % H₂O threshold. The heated HO airstream produced humidities in a similar range
to DNPH.

280 Ambient measurements of HCHO-scrubbed air from the Pico were used to assess the HCHO-removal efficiency of
heated HO as compared to DNPH. The zeroing inlet on the Pico was teed to a DNPH-coated cartridge and a stainless-
steel column (length of 8 in, radius of 0.75 in) containing 215 cm³ of HO. The HO column was wrapped in high
temperature heat tape, insulated in a fiberglass sleeve, and heated to 180 °C. Pei et al. (2015) found HO at this
285 temperature achieved nearly 100 % HCHO removal and preserved the scrubber bed from H₂O poisoning. A
condensation trap and second PF were placed downstream of the HO column to protect the instrument against potential
liquid H₂O and particulate matter. Two mass flow controllers were placed upstream of the scrubbers and used as
valves. The Pico sampled from its zeroing inlet while the incoming flow alternated between scrubbers in 40 s intervals.
The first 10 s of data after every switch was removed to preclude any effects from valve-switching. This removal
290 period was determined experimentally.

DNPH-scrubbed baselines exhibited a normal distribution centered around a mean and standard deviation of $-13.63 \pm$
 0.54 ppb. HO-scrubbed baselines exhibited a normal distribution with a larger mean of -12.92 ± 0.34 ppb resulting in
an absolute difference of 0.71 ppb, which falls outside of the instrument's precision (discussed in Sect. 3) and indicates
295 less efficient HCHO removal. Since ambient humidity perennially remained sufficiently high in the Atlanta area, we
recommend the use of DNPH for zeroing the Aeris instruments.

2.2.4 Data processing

300 We generated temporally averaged datasets with variable time resolutions (1–60 min) using a data handling scheme
like that of the Picarro G2307 observations. Zeroes are averaged to single points and interpolated to a 1 Hz resolution,
subtracted from the 1 Hz ambient data, and ≥ 50 % data completeness is required for any averaging interval. We discard
the first 5 s of measurements after a valve switch.

305

2.2.5 Instrument calibration

In Sept 2023, both Aeris instruments were calibrated using dilutions of a HCHO gas standard (either Apel Riemer: 1015 ppb \pm 5%, or Airgas: 1044 ppb \pm 10%) with humidified ultra-ZA. The configurations for humidifying air and diluting the gas standard were as described in sections 2.1.3 and 2.1.6. Both instrument calibrations produced slopes within 5 % of the original factory calibration, which occurred in Feb. 2021. Intercepts were in the range of -0.03-0.12 ppb. These results indicate that the calibration throughout the instruments' respective deployments remained stable. In Oct 2022 and Sept 2023, standard addition calibrations were performed by adding small amounts of the gas standard to the ambient line. Expected concentrations are calculated as the flow weighted average of the gas standard concentration and the ambient concentration. Ambient concentration is measured by a co-located reference instrument. In Oct. 2022, the two Aeris units were co-located and informed one another. In Sep. 2023, Picarro G2307 measurements were used as the reference.

Results for the standard addition calibrations are shown in Fig. 3. York regressions (not plotted) incorporated the 1-min standard deviation of the measured concentrations, cylinder concentration uncertainty, and, for the standard addition calibrations, the measurement uncertainty associated with the corresponding reference instrument.

The Pico's standard addition calibrations agreed closely with the ZA dynamic dilution calibration and produced slopes of 0.94 ± 0.16 and 0.97 ± 0.16 , intercepts of 0.13 ± 0.61 and 0.16 ± 1.18 , and normalized mean biases (NMB) between measured and expected concentrations of -4.9% and -5.5% in 2022 and 2023, respectively. The high uncertainty with the 2023 intercept is attributed to issues with the instrument's thermo-electric cooler which began in Aug. 2023. All Pico data was processed according to the standard addition calibration closest in time.

The Ultra's 2022 standard addition calibration produced a slope of 0.86 ± 0.16 and a NMB of -13.2% between measured and expected concentrations. This calibration and the Ultra's 2023 dynamic dilution calibration agree within the uncertainties of both techniques. However, the 2023 standard addition calibration produced a slope of 0.77 ± 0.08 which has relative decreases of 10.5% from 2022 and 19% from the dynamic dilution calibration, and a NMB of -22.8% between measured and expected concentrations. This NMB persisted in the Ultra's ambient observations and could not be related to any measured instrument parameters.

These results suggest that standard addition calibrations are useful as a secondary check on instrument sensitivity once in the field. All ambient data for the Ultra data were processed using the 2023 standard addition calibration. This decision is owed to the intercomparison results presented in Sect. 5 wherein application of this calibration most effectively reduces the NMB relative to the G2307 and Pico. Correspondingly, a 14 % relative uncertainty from propagating the measurement uncertainties of the G2307 and Ultra in quadrature. A 0.3 ppb offset is added per the Pico/FILIF comparison in Shutter et al. (2019), which falls within the range of calibration offsets seen in this work.

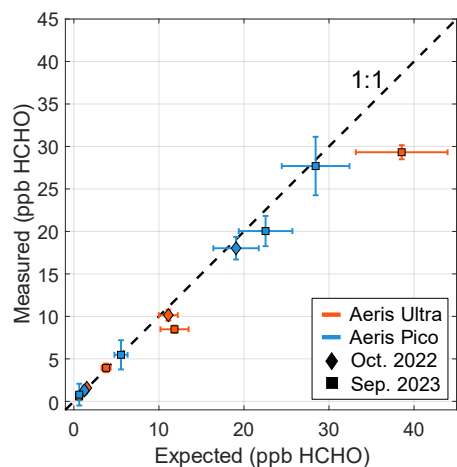


Figure 3 – Results from Aeris standard addition calibrations. Error bars are the uncertainty in each data point, with measured concentrations using the standard deviation of each averaged concentration step and expected concentrations using the cylinder uncertainty. For the standard addition, the measurement uncertainty of the reference instrument is also incorporated.

2.3 DNPH (TO-11A)

Method TO-11A outlines in detail the EPA guidance on preparation of DNPH-coated cartridges and subsequent analysis through HPLC (U.S. EPA, 1999). Formaldehyde was measured using an ATEC Model 8000 Toxic Air Sampler over three consecutive eight-hour periods spanning a full 24 hours with samples collected every three days. Ambient air was drawn at a rate of 0.9 – 1.1 L/min through a KI-coated copper inlet heated to 50°C to remove O₃ before passing through a DNPH-coated cartridge (Supelco LpDNPH S10) which collected carbonyls in their non-volatile, carbonyl-hydrazone derivative form. The denuder is necessary as it minimizes potential O₃-related interferences in the resultant HPLC chromatograms (Vairavamurthy et al., 1992). At the end of the sampling period, the cartridges were capped and stored in a refrigeration unit at ≤ 4 °C until analysis. The cartridges were then eluted with 10 mL of acetonitrile (ACN) and the eluent analysed via a Waters HPLC-UV system with a temperature stabilized (25 ± 1°C), reversed phase C18-coated silica gel (1.7 µm particle size) column (Bridged ethyl hybrid, 2.1 mm x 50 mm ID) at 360 nm wavelength. The eluents used in the HPLC process were deionized H₂O and ACN. The HPLC system was calibrated before each use with known concentrations of HCHO and field samples are analysed in comparison to blank cartridges.

Prior works determine uncertainties in the range of 9-15% for this method (Hak et al., 2005; Wisthaler et al., 2008; Dunne et al., 2018). An uncertainty of 15% is assumed per the uncertainty of the standard used for calibration of the HPLC instrument. We note that this does not account for any biases caused by interfering species such as NO₂ or issues brought on by variable sample flow rates or ambient RH (Karst et al., 1993; Herrington and Hays, 2012; Ho et al., 2014; Souza et al., 2020).

3. Instrument precision and baseline drift

375 The precisions of the three analyzers were characterized in two ways. First, the instruments' inlets were overflowed
using a ZA source for 24 h and precision was calculated via an Allan-Werle curve, as in prior instrument
characterization studies (Shutter et al., 2019; Glowania et al., 2021). Results are shown as the solid lines in Fig. 4. The
G2307 achieves precisions of 0.09 ppb, 0.05 ppb, and 0.03 ppb for integration times of 5, 20, and 60 minutes. This
performance is similar to the 5 min 0.06 ppb precision reported by the manufacturer and results determined in
380 Glowania et al. (2021). The Ultra achieves precisions of 0.20 ppb, 0.20 ppb, and 0.28 ppb for the same periods. The
best precision achieved by the Pico is 0.66 ppb at a 30 s integration time. At longer integration times, fluctuations in
concentrations reported by the Pico instrument can be attributed to thermal instability. Internal instrument
temperatures varied by ± 0.3 - 0.4 °C over the course of 7 h and were well-correlated ($r > 0.85$) with the instrument
baseline. Resultingly, precisions past 40 s integration times quickly became unsuitable for ambient monitoring. During
385 deployment, the Pico's internal temperature was more stable compared to the ZA tests performed in the laboratory.
When using 30 s zeroing periods from the Pico's ambient time series, a precision of 0.40 ppb HCHO is determined,
which is comparable to that of the Ultra for the same integration window.

390

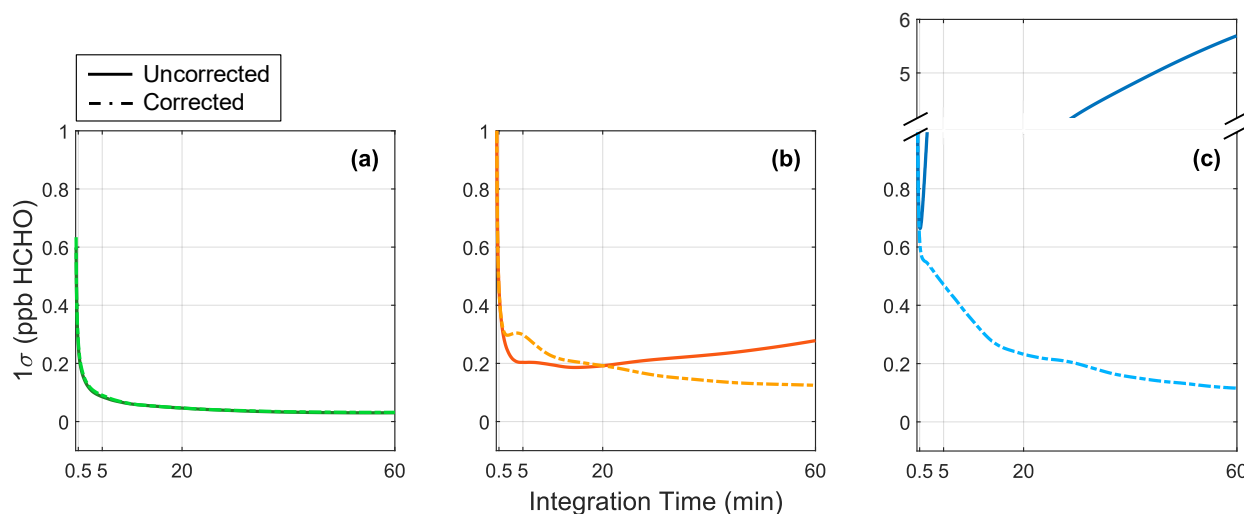


Figure 4 – Allan-Werle curves for a) Picarro G2307 b) Aeris Ultra and c) Aeris Pico instruments. Uncorrected precisions (solid lines) are calculated without accounting for baseline variation, whereas corrected precisions (dashed lines) use the same baseline-characterization method used to process ambient data.

395

As Allan variance is not meant to address systematic errors like temperature effects, we developed a modified, or corrected, Allan-Werle curve that better characterizes the precision of ambient measurements. Still sampling ZA, we

replicated the sampling sequences and data processing methods used for ambient measurements (i.e. the 1 Hz data is drift-corrected by averaging and subtracting out each zeroing period). We then treated the 1 Hz data measured on the “ambient” inlet as contiguous. Results are shown as dashed lines in Fig. 4. For the Picarro G2307 (Fig. 4a), there is no change in precision using this method, as the baseline is relatively constant in this period. Both Aeris units benefited significantly from this correction, reaching 40 min precisions of 0.140 ppb and 0.154 ppb for the Ultra and Pico, respectively. The Pico’s modified precision is within 15 ppt of the 40 min precision of 0.14 ppb observed in Shutter et al. (2019). The corrected Aeris Allan-Werle curves trend similarly to the G2307’s, achieving lower precisions with longer integration times. These results indicate that the ambient sampling sequences used for each instrument are sufficient to account for the influence of any physical instrument-variables on the baseline. As the precision of the ambient measurements (which are calculated differentially) is impacted by both the precision of the ambient and zero baselines, the modified Allan-Werle curves do not account for the precision of the zero measurement. In our ambient dataset, we are limited to a 30 s integration time per the sampling sequence of the Aeris units. The 30 s Allan deviation while sampling through DNPH in our ambient dataset is 0.45 ppb for the Ultra. For the Pico, observations prior to Aug. 2023 have a precision of 0.41 ppb and 0.66 ppb otherwise. This is taken as the true precision of the ambient dataset. Longer zeroing times may achieve higher precision in the dashed lines of Fig. 4 if the baseline has sufficiently low drift through the sampling period.

To quantify instrument baseline drift, we show a typical time series of scrubbed-air observations for all three instruments. The period chosen spans from 3 – 8 Sep 2022 and are shown in Fig. 5. The zero measurements are averaged according to the respective data scheme for each instrument and plotted differentially relative to the first value of each time series. The G2307 exhibits comparatively little drift with a max difference of 1.3 ppb when sampling DR-scrubbed air, occurring late on 4 Sep. Over the same timeframe, the Aeris Ultra’s baseline can shift up to ± 6 ppb while the Aeris Pico baseline exhibits the most variability, changing by as much as ± 20 ppb just over the course of 12 h. This significant drift necessitates more frequent zeroing, thus reducing total time spent sampling ambiently and exhausting scrubbers faster. At their fastest drift rates (1.67 ppb HCHO h^{-1} for the Pico and 0.125 ppb HCHO h^{-1} for the Ultra), the improved thermal stability reduces drift by a factor of 13.36. From our observations, we determined that the Pico should be zeroed at least every 3 min and the Ultra every 10 min under typical indoor-deployment configurations. For the G2307, observations of the instrument baseline drift obtained using DR suggest that hourly zeroing is sufficient.

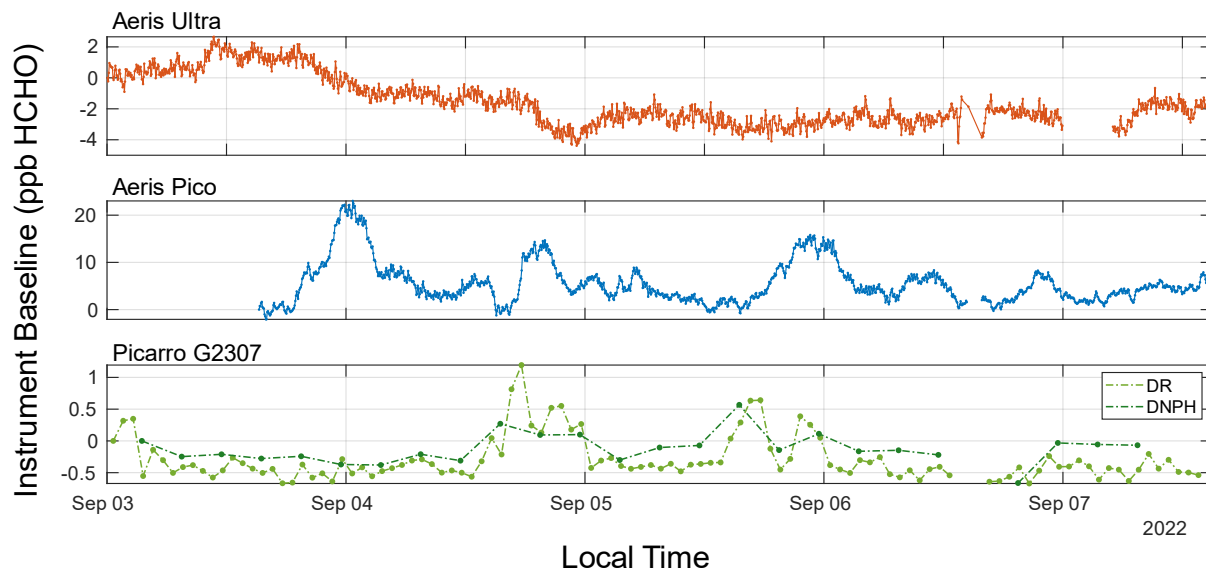


Figure 5 – Instrument baseline time series for all three HCHO monitors plotted differentially to the first point in the time series. The Ultra and G2307, equipped with better thermal stabilization, show significantly less drift than the Pico.

430

4 Intercomparison

4.1 Field site descriptions

435

4.1.1 South DeKalb

440

The location of the South Dekalb (SDK) PAMS is shown in Fig. 6. The site is located approximately 12 mi southeast of the university campus in a less industrialized area with comparatively greater tree coverage. The G2307 was permanently stationed at SDK, with two intercomparisons performed during its deployment. First, the Aeris Pico was co-deployed from 28 July to 13 Sept 2022 according to the configuration shown in Fig. 7a. Then, the Aeris Ultra and Pico were co-deployed from 21-29 Aug. 2023 in their standard ambient configurations without sharing ambient lines. Instruments were housed in a climate-controlled trailer with an indoor temperature maintained at 21-23 °C. All tubing was 0.125 in ID (0.25 in OD) PTFE with 7.5 m extending from inside the trailer and up a mast, where the inlet was situated 5 m above the ground. The G2307 and Pico instruments had flow rates of 450 cm³ min⁻¹, leading to a residence time of approximately 4 s when teed together, and 8 s when separate. The Ultra had a flow rate of 800 cm³ min⁻¹ with a residence time of 5 s. 1µm particulate filters (PFs) in Savillex holders were used, and inlets were shielded by PTFE funnels covered with PTFE mesh. The indoor portion of the sampling lines were heated to 46 °C (≥1 °C above the cavity cell temperature of the instruments) to avoid condensation in the plumbing.

445

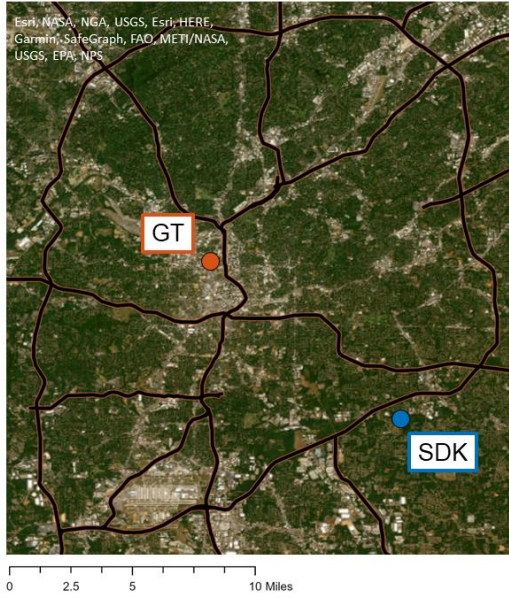


Figure 6 – Locations of the two field sites in the Atlanta, GA area where the Aeris Ultra, Aeris Pico, and Picarro G2307 were deployed.

455

The Aeris instruments' baselines were determined solely using DNPH while the G2307 sampled between DNPH, DR, or DR+MS. When scrubbing only with DR, air was passed through two adsorption columns (length of 16 in, radius of 2 in) in series containing 0.5 kg of material each. For DR+MS, the column first in the series was replaced with the MS material. When the adsorption columns were exhausted, the scrubber bed was replaced with either new or regenerated material. DR was thermally regenerated according to the manufacturer instructions.

460

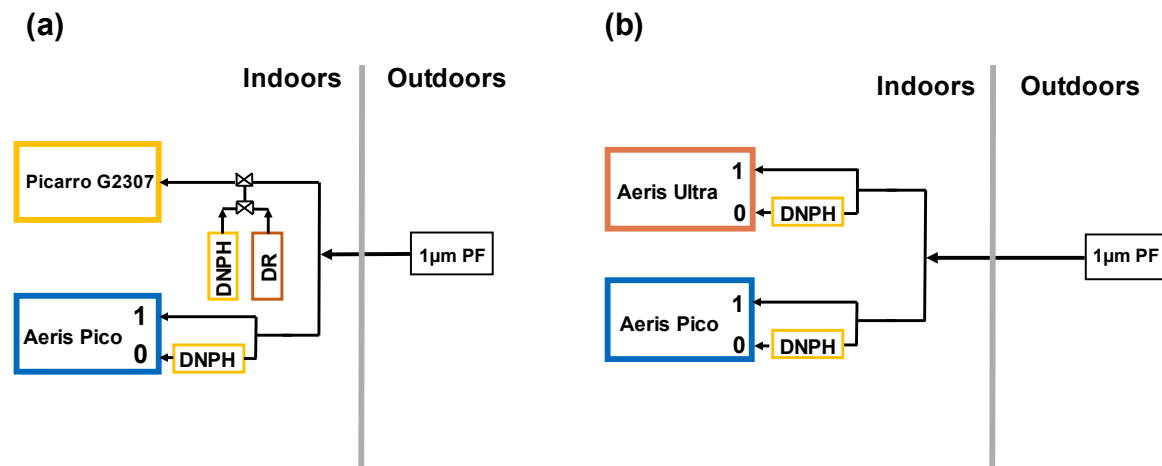


Figure 7 – Configurations of instruments during their respective intercomparisons. (a) shows the teed setup used from 28 July – 13 Sep 2022 for the Aeris Pico and Picarro G2307. When not co-located, the G2307 has the same configuration without being teed to the Pico. (b) shows the setup used for the Aeris instruments while deployed at GT from 25 – 28 July and 4 – 17 Oct 2022. For each panel, “0” references HCHO-scrubbed air, “1” is ambient air, and “PF” is a particle filter.

465

4.1.2 Georgia Tech

470

The Aeris instruments were co-deployed in the penthouse laboratory of the Ford Environmental Science and Technology building (GT) from 25-28 July 2022 and 4-18 Oct 2022 with the setups used during their co-located periods shown in Fig. 7b. Ambient temperature of the lab was maintained at 22 °C. A total of 7 m of 0.25 in OD (0.125 in ID) PTFE line ran from the instruments through a wall port, where the inlet was suspended 3 m above the outdoor roof floor. As before, a 1 μ m PF in a Savillex holder was attached, the inlet shielded with a PTFE funnel, and indoor tubing insulated to prevent condensation from forming. The Aeris instruments solely used the DNPH-scrubbing method for zeroing.

475

4.2 Instrument intercomparisons

480

4.2.1 Continuous HCHO monitor comparison

485

Fig. 8 shows all HCHO observations from the Aeris and Picarro G2307 instruments from their co-location periods. York regressions of 20-min averaged data incorporate the measurement uncertainties defined in Sect. 2. Observations correlate strongly ($r \geq 0.9$) for each comparison.

490

The Pico had a NMB of 12-13% relative to the G2307 (Fig. 8a), with slopes ranging from 1.01 to 1.09. Fig. 8b shows a Pico NMB of 13% compared to the Ultra, with slopes ranging from 1.04 to 1.13. Before applying a standard addition calibration factor, the Ultra's observations were consistently lower compared to the other instruments. The good agreement in the Ultra v G2307 comparison (Fig. 8c, slope = 0.99, NMB = -1%) supports the use of the standard addition calibration. Intercepts for all regressions range from -0.11-0.41 ppb, which is near to or less than the intercomparison offsets observed in Shutter et al. (2019) for ART-fitted measurements.

495

The scatter around the lines of best fit is primarily owed to the low precision of the Aeris ambient measurements, which is determined by the 30 s zeroing intervals. There are occasional periods of large deviations from the lines of best-fit. These periods typically lasted multiple hours, suggesting accuracy (rather than precision) is the cause of the deviations. Specifically, on four separate occasions the Aeris instruments both measured 10-15 ppb HCHO while the Picarro observations remained at ~10 ppb. Reasons underlying this behavior could not be traced to measured instrument parameters or ambient variables.

500

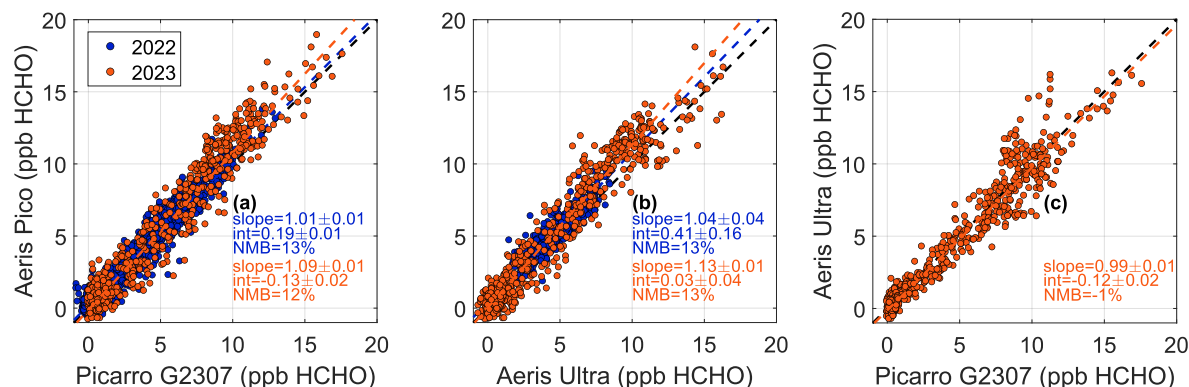


Figure 8 – Comparison of ambient observations from the three HCHO monitors assessed in this work. (a) Pico and G2307 observations taken at SDK in 2022 and 2023, (b) Pico and Ultra with 2022 measurements taken at GT in 2022 and SDK in 2023 (c) Ultra and G2307 observations at SDK 2023.

505


4.2.2 Picarro G2307 and TO-11A DNPH comparison

Fig. 9 compares G2307 observations from June-Aug. 2022 with those from co-located TO-11A measurements. 1 min integrated G2307 concentrations are averaged to the 8 h TO-11A sampling window. We find moderate correlation ($r = 0.62$) and a -58 % NMB of TO-11A observations relative to the G2307 ($\text{slope} = 0.38 \pm 0.02$). Previous studies have demonstrated DNPH-based observations being up to 25 % lower relative to continuous HCHO observations (Hak et al., 2005; Dunne et al., 2018). Hak et al. (2005) determined slopes in the range of 0.64-0.83 when comparing DNPH-HPLC and Hantzsch fluorometric measurements. A comparison of Hantzsch and G2307 observations in Głowania et al. (2021) produced a slope of 1.08.

515

While a low bias is not unusual for TO-11A measurements, the magnitude of the discrepancy presented here is larger than prior studies. We find 8 h G2307 observations are well correlated ($|r| > 0.7$) with temperature, RH, and O_3 , which are expected to either drive ambient HCHO or reflect its secondary chemistry. In contrast, TO-11A observations had weak correlations with these same variables, attaining a maximum r of 0.44 with O_3 and $|r| \leq 0.20$ for all others. TO-11A observations did not correlate notably with NO_2 which would be expected to bias reported HCHO concentrations high (Herrington and Hays, 2012). Noted in Sect. 2.1.5, summertime in Atlanta exhibits high RH and temperatures, which can lead DNPH measurements to underestimate ambient HCHO by 35-80% (Ho et al., 2014). While we are unable to provide a definite reason for this significant discrepancy, the accuracy and stability shown through the G2307's calibrations as well as its agreement with the Aeris units (with independently verified accuracies) lend confidence to its measurements.

520
525

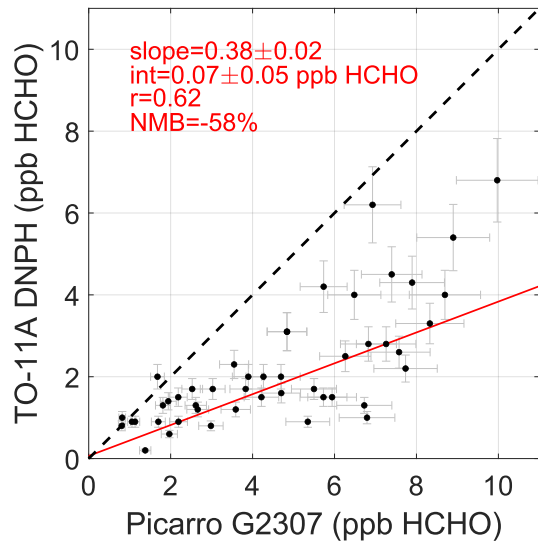


530 **Figure 9 – 8 h TO-11A DNPH observations compared to Picarro G2307 observations at the SDK site from June through August 2022. Error bars represent the 10% uncertainty associated with the TO-11A and G2307 measurements.**

5. Suitability for long-term deployment

535 To demonstrate whether these continuous HCHO monitors capture the urban HCHO gradient, we plot time series from both field sites from Aug. 2022 – Jan. 2023 (Fig. 10) and quantify the HCHO concentration gradient that arises between GT (located in Atlanta’s urban core) and SDK (a less industrialized, rural-urban area). Gaps in data typically result from downtime due to scrubber exhaustion or instrument maintenance. The Aeris instruments overall have less available data due to more frequent and intense scrubber usage, valve failures, and spectral fitting failures that could

540 not self-correct. Over this period, the Pico was stationed at both field sites with only sparse data available after 18 Oct 2022 as it was dedicated to other experiments.

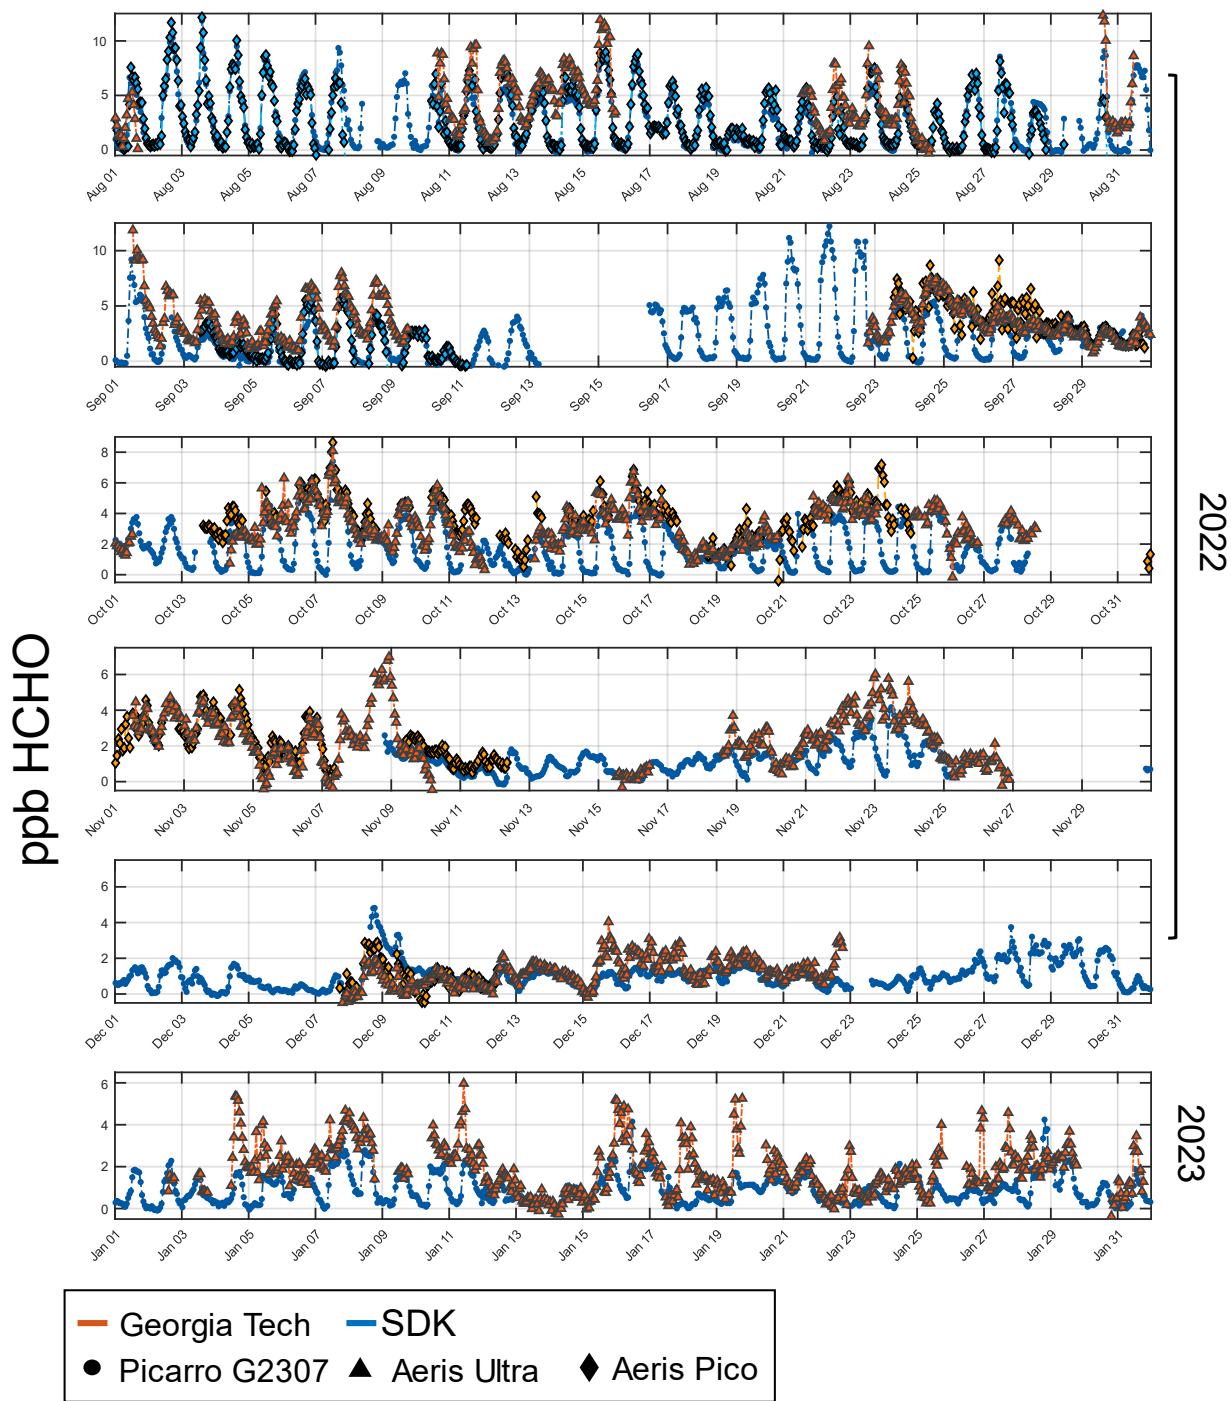

545 **Figure 10 – 1 h averaged HCHO time series from Picarro G2307, Aeris Ultra, and Aeris Pico from Aug. 2022 through Jan**
2023. Observations at GT show less defined diurnal amplitudes than the SDK site and are on average higher regardless of
time of year. Aeris Pico data is sparse past 18 Oct. 2022 as it was periodically dedicated to other experiments.

550 In August, both sites reached their daily maximums around 13:00 LT with monthly-averaged peaks of 7.76 ppb HCHO
at GT and 6.38 ppb HCHO at SDK. On average, HCHO concentrations were 2.12 ppb higher than the SDK site, with
1 h maximums of 12.33 ppb at GT on 30 Aug. and 11.86 ppb at SDK on 3 Aug. Measurements at GT generally had

average night-time minimums above 2 ppb in Aug. and ≤ 1 ppb throughout the winter. Diel cycles showed less definition at GT as the year progressed into the colder months, with SDK maintaining comparatively clearer amplitudes that have sub-ppb night-time minimums throughout the year. Given that the SDK site is located in a less urbanized area and immediately surrounded by trees, this trend matches results found in Wang et al. (2022), who noted that cities with higher levels of biogenic VOCs exhibited larger HCHO diurnal amplitudes. As such, we expect that the influence of isoprene chemistry on HCHO production is stronger at SDK. The consistent night-time threshold at GT could result from a combination of anthropogenic, primary HCHO emission sources local to the city or possibly from stagnant atmospheric conditions leading to localized changes in night-time surface layer mixing heights. Fig. 10 spans a long enough time to capture the ambient extremes of the metropolitan area, showing that the observed HCHO gradient between the two sites is within the measurement capabilities of the G2307 and the Aeris instruments.

These data also allow for a snapshot comparison with previous measurements from both sites to quantify changes in HCHO concentrations. The only prior ground-based campaign to measure HCHO via a continuous monitor in the Atlanta metropolitan area was the 1999 Atlanta Supersite Project (Solomon et al., 2003), where a Hantzsch fluorometric monitor was deployed during the month of August (Dasgupta et al., 2005). HCHO observations taken in the urban core are used to calculate an August diel cycle for their respective years. We employ the PAMS HCHO data taken at SDK in Aug. 1999 (AQS, 1999) to compare with the Aug. 2022 data previously used in Fig. 9. In 1999, DNPH samples were collected every 3 h from 06:00-18:00 LT. Stated previously, samples are now collected every 8 h over a 24 h period starting at 04:00 LT. As such, a 6 h average of the 1999 observations (12-18:00 LT) are compared with the 2022 8 h average (12-20:00 LT) with the results shown in Fig. 11.

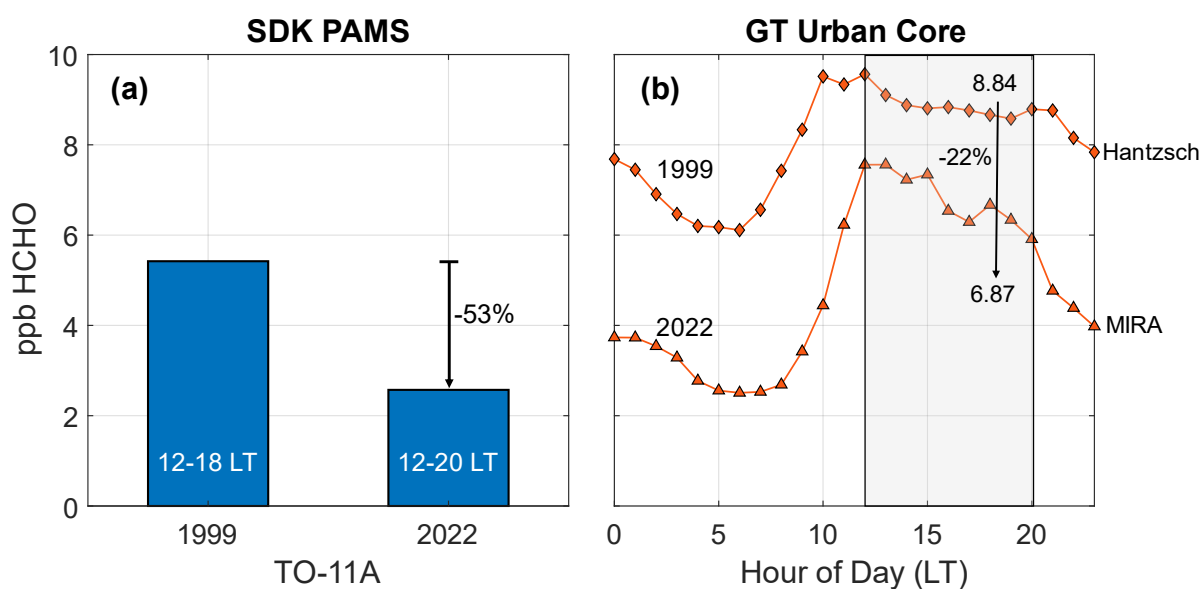


Figure 11 – HCHO concentrations from 1999 and 2022. (a) shows a 53% decrease from July 1999 to 2022 in the midday average (12-20:00 LT) of PAMS measurements taken at SDK and (b) shows a 22% decrease for the same averaging window in August in Atlanta’ urban core.

An average of the August HCHO observations over the 12-20:00 LT window show that concentrations at GT have
580 reduced by 22.3 % since 1999 despite the increasing urbanization of the city over the last two decades. The average
relative decrease in the 1 h monthly maximums and minimums at GT are 22.9 % and 59.0 %, respectively. Dasgupta
et al. (2005) state the possible influence of nearby HCHO emission sources on their observations, but this remains a
nonetheless considerable decrease in nighttime concentrations. A significantly greater midday decrease of 53% is
585 calculated for the SDK PAMS data. However, Picarro G2307 data averaged to the same midday window results in a
relative decrease of only 1.9 %. Monthly-averaged minimum values can't be calculated for SDK as the 1999 data
doesn't span a complete diurnal cycle.

Continuous measurements provide the benefit of comprehensive time series, meaning local chemical trends of HCHO
can be more clearly related to time-dependent atmospheric conditions. In the urban core, maximum HCHO
590 concentrations always occur in the daytime and minimums in the nighttime, with the relative change in minimums
since 1999 being significantly greater than that of the maximums. OH oxidation of isoprene is one of the dominant
sources of HCHO in urban environments that have sufficiently high NO_x concentrations, with the southeast having
comparably higher biogenic influences on its atmospheric chemistry than the rest of the country (Travis et al., 2016).
As significant reductions in U.S. NO_x emissions have been observed over the decades (Duncan et al., 2016), urban
595 daytime HCHO production is then expected to decrease. As OH is largely a daytime oxidant, nighttime decreases in
HCHO are more likely attributable to reductions in direct emissions of both HCHO as well as its anthropogenic VOC
precursors.

6 Conclusions

600 We used year-long ambient datasets from three commercially new in-situ HCHO monitors to quantify instrument
performance and to compare observations with measurements produced from co-located monitors employing the EPA
TO-11A methodology. These continuous monitors offer an advantage given that their measurements are online, have
sufficient precision at finer time resolutions, and don't require special handling or storage of samples or hazardous
605 chemical. However, previous measurements exhibited humidity dependencies, produced significantly lower
concentrations, and showed non-negligible variability in HCHO concentration dependent on zeroing method.
Additionally, all three instruments require frequent zeroing via HCHO scrubbers to account for baseline drift with
each method presenting its own set of practical considerations. We determined calibration procedures and optimal
field setups by assessing how measurements were impacted with usage of four common scrubbing methods: DNPH,
610 DR, DR+MS, and HO.

DNPH-derived baselines were compared to a ZA source, producing values within 14 ppt HCHO on average and
demonstrating their efficacy. Ambient conditions year-round at the GT and SDK field sites had sufficient RH (≥ 25

615 %) to not impede DNPH-derivatization of hydrazine. At high RH (>50%), no clear impact to instrument-baselines
could be observed. DR, DR+MS, and HO-scrubbed baselines were then compared to those resulting from DNPH. HO
performed poorly, exhibiting a mean differential baseline value of 0.71 ppb HCHO. DR and DR+MS performed on
par with DNPH indicating high HCHO-scrubbing efficiency. As such, we recommend use of DR/DR+MS and DNPH
for zeroing the Picarro G2307, and only DNPH for use with the Aeris units given their humidity requirements.
620 Additionally, the G2307's humidity-dependence was quantified experimentally. We emphasize this procedure before
deployment as results here show this relationship to be instrument specific.

We developed a modified method for determining instrument precision that accounts for instrument zeroing. The
G2307, Ultra, and Pico achieved modified precisions of 0.05 ppb, 0.20 ppb, and 0.22 ppb for a 20 min integration
time, respectively. We determined that the sensitivities of the monitors were stable during their respective
625 deployments. The Aeris Ultra exhibited a NMB of -30-36% compared to Aeris Pico and Picarro G2307 measurements
if dynamic dilution calibrations were used as the basis. However, standard addition calibration of the Aeris units led
to all instruments agreeing within 13%. Co-located TO-11A observations exhibited a NMB of -58% relative to the
G2307, which is the largest TO-11A intercomparison discrepancy reported in extant literature.

630 Finally, using time series that span from Aug. 2022 through Jan. 2023 at two fields sites separated by 12 mi, we
demonstrated that these instruments capture the HCHO gradient in the Atlanta metro area over a wide range of ambient
conditions, including summer and wintertime seasonal extremes. Comparison with historical HCHO measurements
revealed a relative decrease in daytime ambient HCHO of 22.3 % at the urban-core site and 53 % at the urban/rural
site. Nighttime HCHO concentrations in the urban core decreased by 59 % during this time. Ultimately, the
635 performance of these instruments and the subsequent results show the feasibility of both deploying across multiple
cities and taking fast, accurate HCHO observations, offering the potential for greater insights into the complex
chemistry of urban HCHO.

640

Competing Interests.

The authors declare that they have no conflicts of interest.

645

Acknowledgements.

The authors kindly thank Jaime Gore and DeAnna Oser from the Georgia Environmental Protection Division for the
input provided for this work.

650 **Financial Support.**

This research has been supported by the National Aeronautics and Space Administration (grant no. 80NSSC21K0944).

Data availability.

All data shown in this work are available at: <https://doi.org/10.5281/zenodo.7682263>. Met and chemical data from

655 Dasgupta et al. (2005) are available at
[https://asdc.larc.nasa.gov/project/NARSTO/NARSTO EPA SS ATLANTA 1999 CHEM PM MET DATA 1](https://asdc.larc.nasa.gov/project/NARSTO/NARSTO_EPA_SS_ATLANTA_1999_CHEM_PM_MET_DATA_1)
(DOI: 10.5067/ASDCDAAC/NARSTO/0060).

660

References:

- 665 Achatz, S., Lörinci, G., Hertkorn, N., Gebefügi, I., and Kettrup, A.: Disturbance of the determination of aldehydes and ketones: Structural elucidation of degradation products derived from the reaction of 2,4-dinitrophenylhydrazine (DNPH) with ozone, *Fresenius' Journal of Analytical Chemistry*, 364, 141-146, 10.1007/s002160051313, 1999.
- Alvarado, L. M., Richter, A., Vrekoussis, M., Hilboll, A., Kalisz Hedegaard, A. B., Schneising, O., and Burrows, J. P.: Unexpected long-range transport of glyoxal and formaldehyde observed from the Copernicus Sentinel-5 Precursor satellite during the 2018 Canadian wildfires, *Atmospheric Chemistry and Physics*, 20, 2057-2072, 2020.
- Bent, J., Wallace, C., Lucic, G., Rella, C., Haffnagle, J., Baumann, K.: G2307: Traceable calibration of Formaldehyde (H2CO), White Paper, 2023.
- 670 Cardenas, L., Brassington, D., Allan, B., Coe, H., Alicke, B., Platt, U., Wilson, K., Plane, J., and Penkett, S.: Intercomparison of formaldehyde measurements in clean and polluted atmospheres, *Journal of Atmospheric Chemistry*, 37, 53-80, 2000.
- Cazorla, M., Wolfe, G., Bailey, S., Swanson, A., Arkinson, H., and Hanisco, T.: A new airborne laser-induced fluorescence instrument for in situ detection of formaldehyde throughout the troposphere and lower stratosphere, *Atmospheric Measurement Techniques*, 8, 541-552, 2015.
- 680 Coggon, M. M., Gkatzelis, G. I., McDonald, B. C., Gilman, J. B., Schwantes, R. H., Abuhassan, N., Aikin, K. C., Arend, M. F., Berkoff, T. A., and Brown, S. S.: Volatile chemical product emissions enhance ozone and modulate urban chemistry, *Proceedings of the National Academy of Sciences*, 118, e2026653118, 2021.
- Dasgupta, P. K., Li, J., Zhang, G., Luke, W. T., McClenny, W. A., Stutz, J., and Fried, A.: Summertime ambient formaldehyde in five US metropolitan areas: Nashville, Atlanta, Houston, Philadelphia, and Tampa, *Environmental science & technology*, 39, 4767-4783, 2005.
- 685 Dugheri, S., Massi, D., Mucci, N., Marrubini, G., Cappelli, G., Speltini, A., Bonferoni, M. C., and Arcangeli, G.: Exposure to airborne formaldehyde: Sampling and analytical methods—A review, *Trends in Environmental Analytical Chemistry*, 29, e00116, 2021.
- Duncan, B. N., Lamsal, L. N., Thompson, A. M., Yoshida, Y., Lu, Z., Streets, D. G., Hurwitz, M. M., and Pickering, K. E.: A space-based, high-resolution view of notable changes in urban NO_x pollution around the world (2005–2014), *Journal of Geophysical Research: Atmospheres*, 121, 976-996, 2016.
- Dunne, E., Galbally, I. E., Cheng, M., Selleck, P., Molloy, S. B., and Lawson, S. J.: Comparison of VOC measurements made by PTR-MS, adsorbent tubes–GC-FID-MS and DNPH derivatization–HPLC during the Sydney Particle Study, 2012: a contribution to the assessment of uncertainty in routine atmospheric VOC measurements, *Atmos. Meas. Tech.*, 11, 141-159, 10.5194/amt-11-141-2018, 2018.
- 695 Fried, A., Walega, J., Weibring, P., Richter, D., Simpson, I. J., Blake, D. R., Blake, N. J., Meinardi, S., Barletta, B., and Hughes, S. C.: Airborne formaldehyde and volatile organic compound measurements over the Daesan petrochemical complex on Korea's northwest coast during the Korea-United States Air Quality

study Estimation of emission fluxes and effects on air quality, *Elementa: Science of the Anthropocene*, 8, 2020.

700 Furdyna, P.: Experiences with Picarro G2307 HCHO Analyzers, New York Department of Environmental Conservation, 2020.

Glowania, M., Rohrer, F., Dorn, H. P., Hofzumahaus, A., Holland, F., Kiendler-Scharr, A., Wahner, A., and Fuchs, H.: Comparison of formaldehyde measurements by Hantzsch, CRDS and DOAS in the SAPHIR chamber, *Atmos. Meas. Tech.*, 14, 4239-4253, 10.5194/amt-14-4239-2021, 2021.

705 Hak, C., Pundt, I., Trick, S., Kern, C., Platt, U., Dommen, J., Ordóñez, C., Prévôt, A., Junkermann, W., and Astorga-Lloréns, C.: Intercomparison of four different in-situ techniques for ambient formaldehyde measurements in urban air, *Atmospheric Chemistry and Physics*, 5, 2881-2900, 2005.

Hansen, R., Griffith, S., Dusanter, S., Rickly, P., Stevens, P., Bertman, S., Carroll, M., Erickson, M., Flynn, J., and Grossberg, N.: Measurements of total hydroxyl radical reactivity during CABINEX 2009–Part 1: field measurements, *Atmospheric Chemistry and Physics*, 14, 2923-2937, 2014.

710 Herndon, S. C., Zahniser, M. S., Nelson Jr, D. D., Shorter, J., McManus, J. B., Jiménez, R., Warneke, C., and De Gouw, J. A.: Airborne measurements of HCHO and HCOOH during the New England Air Quality Study 2004 using a pulsed quantum cascade laser spectrometer, *Journal of Geophysical Research: Atmospheres*, 112, 2007.

715 Herrington, J. S. and Hays, M. D.: Concerns regarding 24-h sampling for formaldehyde, acetaldehyde, and acrolein using 2, 4-dinitrophenylhydrazine (DNPH)-coated solid sorbents, *Atmospheric Environment*, 55, 179-184, 2012.

Ho, S. S. H., Chow, J. C., Watson, J. G., Ip, H. S. S., Ho, K. F., Dai, W. T., and Cao, J.: Biases in ketone measurements using DNPH-coated solid sorbent cartridges, *Analytical Methods*, 6, 967-974, 2014.

720 Karst, U., Binding, N., Cammann, K., and Witting, U.: Interferences of nitrogen dioxide in the determination of aldehydes and ketones by sampling on 2,4-dinitrophenylhydrazine-coated solid sorbent, *Fresenius' Journal of Analytical Chemistry*, 345, 48-52, 10.1007/BF00323325, 1993.

Lin, Y. C., Schwab, J. J., Demerjian, K. L., Bae, M. S., Chen, W. N., Sun, Y., Zhang, Q., Hung, H. M., and Perry, J.: Summertime formaldehyde observations in New York City: Ambient levels, sources and its contribution to HOx radicals, *Journal of Geophysical Research: Atmospheres*, 117, 2012.

725 Luecken, D., Napelenok, S., Strum, M., Scheffe, R., and Phillips, S.: Sensitivity of ambient atmospheric formaldehyde and ozone to precursor species and source types across the United States, *Environmental science & technology*, 52, 4668-4675, 2018.

730 Lui, K. H., Ho, S. S. H., Louie, P. K. K., Chan, C. S., Lee, S. C., Hu, D., Chan, P. W., Lee, J. C. W., and Ho, K. F.: Seasonal behavior of carbonyls and source characterization of formaldehyde (HCHO) in ambient air, *Atmospheric Environment*, 152, 51-60, <https://doi.org/10.1016/j.atmosenv.2016.12.004>, 2017.

Parrish, D., Ryerson, T., Mellqvist, J., Johansson, J., Fried, A., Richter, D., Walega, J., Washenfelder, R. d., De Gouw, J., and Peischl, J.: Primary and secondary sources of formaldehyde in urban atmospheres: Houston Texas region, *Atmospheric Chemistry and Physics*, 12, 3273-3288, 2012.

735 Pei, J., Han, X., and Lu, Y.: Performance and kinetics of catalytic oxidation of formaldehyde over copper manganese oxide catalyst, *Building and Environment*, 84, 134-141, 2015.

Scheffe, R. D., Strum, M., Phillips, S. B., Thurman, J., Eyth, A., Fudge, S., Morris, M., Palma, T., and Cook, R.: Hybrid modeling approach to estimate exposures of hazardous air pollutants (HAPs) for the national air toxics assessment (NATA), *Environmental Science & Technology*, 50, 12356-12364, 2016.

740 Shutter, J. D., Allen, N. T., Hanisco, T. F., Wolfe, G. M., St. Clair, J. M., and Keutsch, F. N.: A new laser-based and ultra-portable gas sensor for indoor and outdoor formaldehyde (HCHO) monitoring, *Atmos. Meas. Tech.*, 12, 6079-6089, 10.5194/amt-12-6079-2019, 2019.

Solomon, P. A., Chameides, W., Weber, R., Middlebrook, A., Kiang, C., Russell, A. G., Butler, A., Turpin, B., Mikel, D., and Scheffe, R.: Overview of the 1999 Atlanta supersite project, *Journal of Geophysical Research: Atmospheres*, 108, 2003.

745 Souza, M. d. O., Sánchez, B., Fuentes, M., Gilaranz, J., and Canela, M. C.: Analytical validation using a gas mixing system for the determination of gaseous formaldehyde, *Analytical Methods*, 12, 5247-5256, 2020.

Spinei, E., Whitehill, A., Fried, A., Tiefenraber, M., Knepp, T. N., Herndon, S., Herman, J. R., Müller, M., Abuhassan, N., and Cede, A.: The first evaluation of formaldehyde column observations by improved Pandora spectrometers during the KORUS-AQ field study, *Atmospheric Measurement Techniques*, 11, 4943-4961, 2018.

750

- 755 St Clair, J. M., Swanson, A. K., Bailey, S. A., and Hanisco, T. F.: CAFE: A new, improved nonresonant laser-induced fluorescence instrument for airborne in situ measurement of formaldehyde, *Atmospheric Measurement Techniques*, 12, 4581-4590, 2019.
- Strum, M. and Scheffe, R.: National review of ambient air toxics observations, *Journal of the Air & Waste Management Association*, 66, 120-133, 2016.
- 760 Tang, S., Graham, L., Shen, L., Zhou, X., and Lanni, T.: Simultaneous determination of carbonyls and NO₂ in exhausts of heavy-duty diesel trucks and transit buses by HPLC following 2, 4-dinitrophenylhydrazine cartridge collection, *Environmental science & technology*, 38, 5968-5976, 2004.
- Tonnesen, G. S. and Dennis, R. L.: Analysis of radical propagation efficiency to assess ozone sensitivity to hydrocarbons and NO_x: 1. Local indicators of instantaneous odd oxygen production sensitivity, *Journal of Geophysical Research: Atmospheres*, 105, 9213-9225, 2000.
- 765 Travis, K. R., Jacob, D. J., Fisher, J. A., Kim, P. S., Marais, E. A., Zhu, L., Yu, K., Miller, C. C., Yantosca, R. M., and Sulprizio, M. P.: Why do models overestimate surface ozone in the Southeast United States?, *Atmospheric Chemistry and Physics*, 16, 13561-13577, 2016.
- U.S. Environmental Protection Agency: Compendium of Methods for the Determination of Toxic Organic Compounds in Ambient Air, 1999.
- 770 Uchiyama, S., Naito, S., Matsumoto, M., Inaba, Y., and Kunugita, N.: Improved measurement of ozone and carbonyls using a dual-bed sampling cartridge containing trans-1, 2-bis (2-pyridyl) ethylene and 2, 4-dinitrophenylhydrazine-impregnated silica, *Analytical chemistry*, 81, 6552-6557, 2009.
- Vairavamurthy, A., Roberts, J. M., and Newman, L.: Methods for determination of low molecular weight carbonyl compounds in the atmosphere: a review, *Atmospheric Environment. Part A. General Topics*, 26, 1965-1993, 1992.
- 775 Valin, L., Fiore, A., Chance, K., and González Abad, G.: The role of OH production in interpreting the variability of CH₂O columns in the southeast US, *Journal of Geophysical Research: Atmospheres*, 121, 478-493, 2016.
- Wang, P., Holloway, T., Bindl, M., Harkey, M., and De Smedt, I.: Ambient Formaldehyde over the United States from Ground-Based (AQS) and Satellite (OMI) Observations, *Remote Sensing*, 14, 2191, 2022.
- 780 Warneke, C., de Gouw, J. A., Edwards, P. M., Holloway, J. S., Gilman, J. B., Kuster, W. C., Graus, M., Atlas, E., Blake, D., Gentner, D. R., Goldstein, A. H., Harley, R. A., Alvarez, S., Rappenglueck, B., Trainer, M., and Parrish, D. D.: Photochemical aging of volatile organic compounds in the Los Angeles basin: Weekday-weekend effect, *Journal of Geophysical Research: Atmospheres*, 118, 5018-5028, <https://doi.org/10.1002/jgrd.50423>, 2013.
- Whitehill, A. R., Long, R., Kaushik, S., Szykman, J., Williams, D., Valin, L., Furdyna, P., and Felton, D.: Evaluation of Continuous Formaldehyde Measurements in Ambient Air, *AGU Fall Meeting Abstracts*, A33G-3207,
- 785 Wisthaler, A., Apel, E., Bossmeyer, J., Hansel, A., Junkermann, W., Koppmann, R., Meier, R., Müller, K., Solomon, S., and Steinbrecher, R.: Intercomparison of formaldehyde measurements at the atmosphere simulation chamber SAPHIR, *Atmospheric Chemistry and Physics*, 8, 2189-2200, 2008.
- 790 Wolfe, G. M., Nicely, J. M., St. Clair, J. M., Hanisco, T. F., Liao, J., Oman, L. D., Brune, W. B., Miller, D., Thames, A., and González Abad, G.: Mapping hydroxyl variability throughout the global remote troposphere via synthesis of airborne and satellite formaldehyde observations, *Proceedings of the National Academy of Sciences*, 116, 11171-11180, 2019.
- Wu, Y., Nehrir, A. R., Ren, X., Dickerson, R. R., Huang, J., Stratton, P. R., Gronoff, G., Kooi, S. A., Collins, J. E., and Berkoff, T. A.: Synergistic aircraft and ground observations of transported wildfire smoke and its impact on air quality in New York City during the summer 2018 LISTOS campaign, *Science of The Total Environment*, 773, 145030, 2021.
- 795 Yang, X., Lu, K., Ma, X., Liu, Y., Wang, H., Hu, R., Li, X., Lou, S., Chen, S., and Dong, H.: Observations and modeling of OH and HO₂ radicals in Chengdu, China in summer 2019, *Science of The Total Environment*, 772, 144829, 2021.
- 800 Yokelson, R. J., Goode, J. G., Ward, D. E., Susott, R. A., Babbitt, R. E., Wade, D. D., Bertschi, I., Griffith, D. W., and Hao, W. M.: Emissions of formaldehyde, acetic acid, methanol, and other trace gases from biomass fires in North Carolina measured by airborne Fourier transform infrared spectroscopy, *Journal of Geophysical Research: Atmospheres*, 104, 30109-30125, 1999.
- 805 Zeng, P., Lyu, X., Guo, H., Cheng, H., Wang, Z., Liu, X., and Zhang, W.: Spatial variation of sources and photochemistry of formaldehyde in Wuhan, Central China, *Atmospheric Environment*, 214, 116826, 2019.
- Zhang, H., Li, J., Ying, Q., Guven, B. B., and Olaguer, E. P.: Source apportionment of formaldehyde during TexAQS 2006 using a source-oriented chemical transport model, *Journal of Geophysical Research: Atmospheres*, 118, 1525-1535, 2013.

- 810 Zhu, L., Mickley, L. J., Jacob, D. J., Marais, E. A., Sheng, J., Hu, L., Abad, G. G., and Chance, K.: Long-term (2005–
2014) trends in formaldehyde (HCHO) columns across North America as seen by the OMI satellite
instrument: Evidence of changing emissions of volatile organic compounds, *Geophysical Research Letters*,
44, 7079-7086, <https://doi.org/10.1002/2017GL073859>, 2017a.
- 815 Zhu, L., Jacob, D. J., Mickley, L. J., Marais, E. A., Cohan, D. S., Yoshida, Y., Duncan, B. N., Abad, G. G., and
Chance, K. V.: Anthropogenic emissions of highly reactive volatile organic compounds in eastern Texas
inferred from oversampling of satellite (OMI) measurements of HCHO columns, *Environmental Research
Letters*, 9, 114004, 2014.
- 820 Zhu, L., Jacob, D. J., Keutsch, F. N., Mickley, L. J., Scheffe, R., Strum, M., González Abad, G., Chance, K., Yang,
K., and Rappenglück, B.: Formaldehyde (HCHO) as a hazardous air pollutant: Mapping surface air
concentrations from satellite and inferring cancer risks in the United States, *Environmental Science &
Technology*, 51, 5650-5657, 2017b.