

1 **Response of protonated, adduct, and fragmented ions in Vocus proton-**  
2 **transfer-reaction time-of-flight mass spectrometer (PTR-ToF-MS)**

3

4 Fangbing Li<sup>1</sup>, Dan Dan Huang<sup>2</sup>, Linhui Tian<sup>1</sup>, Bin Yuan<sup>3</sup>, Wen Tan<sup>4</sup>, Liang Zhu<sup>4</sup>,  
5 Penglin Ye<sup>5</sup>, Douglas Worsnop<sup>5</sup>, Ka In Hoi<sup>1</sup>, Kai Meng Mok<sup>1</sup>, Yong Jie Li<sup>1</sup>

6 <sup>1</sup>Department of Civil and Environmental Engineering, Department of Ocean Science  
7 and Technology, and Centre for Regional Oceans, Faculty of Science and Technology,  
8 University of Macau, Macau, China

9 <sup>2</sup>State Environmental Protection Key Laboratory of Cause and Prevention of Urban Air  
10 Pollution Complex, Shanghai Academy of Environmental Sciences, Shanghai, China

11 <sup>3</sup>Institute for Environment and Climate Research, Jinan University, Guangzhou 510632,  
12 China

13 <sup>4</sup>Tofwerk AG, Nanjing, China

14 <sup>5</sup>Aerodyne Research, Inc., Billerica, Massachusetts 01821, United States

15 *Correspondence to:* Yong Jie Li (yongjieli@um.edu.mo)

16


17 **Abstract**

18 Volatile organic compounds (VOCs) affect secondary pollutant formation via active  
19 chemistry. Proton-transfer-reaction mass spectrometry (PTR-MS) is one of the most  
20 important techniques to study the highly variable spatial and temporal characteristics  
21 of VOCs. The response of protonated, adduct, and fragmented ions in PTR-MS in  
22 changing instrument settings and varying relative humidity (RH) requires rigorous  
23 characterization. Herein, dedicatedly designed laboratory experiments were conducted  
24 to investigate the response of these ions for 21 VOCs, including 12 oxygenated VOCs  
25 and two nitriles, using the recently developed Vocus PTR-MS. Our results show that  
26 the focusing ion-molecule reactor (FIMR) axial voltage increases sensitivity by three  
27 to four orders of magnitude but does not significantly change the fractions of protonated  
28 ions. Reducing the FIMR pressure, however, substantially increases fragmentation.  
29 Applying a high radio frequency (RF) amplitude radially on FIMR can enhance  
30 sensitivity by one to two orders of magnitude without affecting the protonated ion  
31 fractions. The change in big segmented quadrupole (BSQ) amplitude mainly affects  
32 sensitivity and protonated ion fraction by modifying ion transmission. The relationship  
33 between sensitivity and proton-transfer reaction rate constant is complicated by the  
34 influences from both ion transmission and protonated ion fraction. The protonated ions  
35 of most VOCs studied (19 out of 21) show less than 15% variations in sensitivity as RH  
36 increases from ~5% to ~85%, except for some long-chain aldehydes which show a  
37 positive RH variation of up to 30%. Our results suggest that the Vocus PTR-MS can  
38 reliably quantify the majority of VOCs under ambient conditions with varying RH.  
39 However, caution is advised for small oxygenates such as formaldehyde and methanol  
40 due to their low sensitivity, as well as for long-chain aldehydes for their slight RH  
41 dependence and fragmentation.

## 42 **1 Introduction**

43 Atmospheric volatile organic compounds (VOCs) affect atmospheric chemistry by  
44 forming secondary pollutants such as tropospheric O<sub>3</sub> (Shao et al., 2016) and secondary  
45 organic aerosols (SOA) (Shrivastava et al., 2017). In addition to their low mixing ratios  
46 (parts per billion by volume, ppbv, or even lower), the spatial and temporal variabilities  
47 of atmospheric VOCs pose another analytical challenge to the study of their  
48 atmospheric occurrence, sources, and fates. Mass spectrometric (MS) techniques based  
49 on ion-molecule reactions (IMR) (Španěl and Smith, 1996) or specifically proton-  
50 transfer reactions (PTR) (Hansel et al., 1995;Lindinger et al., 1998) in a selected ion  
51 flow tube (SIFT) have been developed to provide fast-responding measurements of  
52 VOCs. These techniques, especially the PTR-MS, have been widely used in VOC  
53 measurements in outdoor and indoor environments (Salazar Gómez et al.,  
54 2021;Sekimoto and Koss, 2021;Pagonis et al., 2019;Pleil et al., 2019;Claflin et al.,  
55 2021;Schripp et al., 2014;Jensen et al., 2021).


56 Quantification of VOCs (denoted as M) by PTR-MS relies heavily on their proton-  
57 transfer reactions with the hydronium ion H<sub>3</sub>O<sup>+</sup> (R1). In early SIFT-MS studies where  
58 reagent ions include a multitude of H<sub>3</sub>O<sup>+</sup>(H<sub>2</sub>O)<sub>n</sub> (n=0, 1, 2, 3...) ion series (Španěl and  
59 Smith, 2000), proton-transfer reactions with more hydrated (n ≥ 1) hydronium ions  
60 (R2a) are also important for species with proton affinity (PA) larger than water clusters.  
61 In addition, ligand switching reactions (R2b) and association reactions (R3, with N  
62 being N<sub>2</sub> or O<sub>2</sub>) are also common, leading to [MH + H<sub>2</sub>O]<sup>+</sup> instead of MH<sup>+</sup>. Under these  
63 circumstances, the quantification of VOCs might be heavily influenced by water vapor  
64 concentration, or relative humidity (RH), of the sample. For instance, acetone  
65 concentrations in exhaled air were overestimated by 13% even using both protonated  
66 (MH<sup>+</sup>) and water adduct ([MH + H<sub>2</sub>O]<sup>+</sup>) ions for quantification, when water vapor  
67 varied in the range of (1 – 10) × 10<sup>12</sup> molecules cm<sup>-3</sup> (Španěl and Smith, 2000). A later  
68 study (Smith et al., 2001) showed that quantification of other oxygenated VOCs  
69 (OVOCs) such as ethyl acetate, diethyl ether, methanol, ethanol, and propanol by SIFT-  
70 MS also suffered from RH dependence to various degrees.






71 For PTR-MS that normally uses the  $MH^+$  for quantification, RH dependence was  
72 also widely reported. For instance, Warneke et al. (2001) reported that the sensitivity of  
73 benzene in PTR-MS decreased significantly with the increase of RH, while Steinbacher  
74 et al. (2004) suggested a slight decrease with the increase of RH. Quantification of  
75 biogenic volatile organic compounds (BVOCs) was also reported to be slightly affected  
76 by RH (Kari et al., 2018). The RH dependence stems from the change of reagent ion  
77 distribution, i.e., among  $H_3O^+$  and  $H_3O^+(H_2O)_n$  ( $n \geq 1$ ), which can lead to  
78 overestimation or underestimation of VOCs if such dependence is strong because  
79 ambient RH is deemed highly variable. Therefore, RH-dependent calibrations for VOC  
80 measurements using PTR-MS were normally recommended (de Gouw and Warneke,  
81 2007; Inomata et al., 2008; Sinha et al., 2009; Vlasenko et al., 2010; Cui et al.,  
82 2016; Michoud et al., 2018).

83 Another complication in VOC measurements using SIFT-MS or PTR-MS is that,  
84 due to the nucleophilicity of the oxygen atom, protonated OVOCs would dehydrate,  
85 forming fragmented ions (R4). This reaction often occurs in heavy alcohols, aldehydes,  
86 and carboxylic acids (Španěl et al., 1997; Španěl and Smith, 1998; Hartungen et al.,  
87 2004; Baasandorj et al., 2015).



89 In addition, cleavage on the C-C bond of the protonated ion (R5) is also possible,  
90 especially for alkyl-substituted VOCs under high-energy conditions (e.g., a high E/N  
91 ratio, which is the reduced electric field parameter with E being the electric field and N  
92 the number density of the gas in the drift tube).



94 For instance, at an E/N ratio of 120 Townsend (Td), substituted monocyclic aromatic  
95 compounds such as ethylbenzene and propylbenzene start to fragment into a benzenium  
96 ion ( $C_6H_7^+$ ) (de Gouw et al., 2003; Gueneron et al., 2015).

97 A newly designed focusing ion-molecule reactor (FIMR) was used for PTR-MS,  
98 termed Vocus, and has been shown to have little RH dependence for the protonated ion  
99 because of the high concentration of water vapor introduced into the FIMR (Krechmer

100 et al., 2018). The concentration of hydronium ion ( $\text{H}_3\text{O}^+$ ) in the FIMR is high enough  
101 to maintain at a constant level and dominate over other side reactions, thereby  
102 minimizing the RH dependence for VOC measurement. Yet, the formation of adduct  
103 ions and fragmented ions in Vocus PTR-MS as a function of RH has not been fully  
104 scrutinized, hindering a complete understanding of the ion chemistry in the Vocus PTR-  
105 MS and potential cross interference when measuring ambient air with complex VOC  
106 mixtures. Herein, we conducted experiments on the effects of instrumental settings and  
107 RH variations on the quantification of 21 VOCs, including 12 OVOCs and 2 nitriles,  
108 using a Vocus PTR-MS. Response of protonated ions ( $\text{MH}^+$ ), adduct ions ( $[\text{MH} +$   
109  $\text{H}_2\text{O}]^+$ ), and fragmented ions ( $[\text{MH} - \text{H}_2\text{O}]^+$  or  $[\text{MH} - \text{C}_x\text{H}_y]^+$ ) of these VOCs was  
110 investigated as a function of instrumental setting and RH. Results are interpreted based  
111 on the PA values and/or proton-transfer reaction rate constants ( $k_{\text{ptr}}$ ). Some caveats on  
112 using the Vocus PTR-MS to measure VOCs, especially OVOCs, are also provided.

## 113 **2 Methodology**

### 114 **2.1 Instrument settings**

115 Experiments were performed with a Vocus proton-transfer-reaction time-of-flight  
116 mass spectrometer (PTR-ToF-MS, Vocus 2R, TOFWERK AG, Thun, Switzerland),  
117 hereinafter referred to as Vocus. The Vocus consists of (i) a discharge ion source, (ii) a  
118 focusing ion-molecule reactor (FIMR), (iii) a big segmented quadrupole (BSQ), (iv) a  
119 series of direct current (DC) optics that further focus and accelerate the primary beam  
120 (PB), and (v) a time-of-flight (ToF) mass analyzer (Krechmer et al., 2018). The ion  
121 source is a plasma discharge composed of two conical surfaces. Water vapor is supplied  
122 by purging 20 to 30 mL of milli-Q water and is ionized by plasma discharge. The  
123 reagent ions pass through a ring offset from the central axis so that the photons  
124 generated by the discharge cannot enter. The drift tube was improved by replacing the  
125 stacked ring electrodes of the traditional PTR-MS with a FIMR, which is a glass tube  
126 with a resistive coating on the inner surface and a quadrupole with a radio frequency  
127 (RF) electric field applied. The FIMR increases ion transmission by a factor of 7 to 9  
128 and sensitivity by more than one order of magnitude (Krechmer et al., 2018). Moreover,  
129 the mean kinetic energy of  $\text{H}_3\text{O}^+$  is increased by three times, and the formation of more  
130 hydrated hydronium ions is reduced, suppressing RH dependence for most VOCs  
131 measured (Krechmer et al., 2018). Meanwhile, the mean kinetic energy of VOCs

132 measured is not significantly increased, thereby minimizing fragmentation (Krechmer  
133 et al., 2018). The ToF mass analyzer offers a mass resolving power of 12,000 at a mass-  
134 to-charge ratio ( $m/Q$ ) of 107 Thomson (Th).


135 In our experiments, sample air was drawn into the instrument using 0.5 m long  
136 perfluoroalkoxy (PFA) Teflon tubing of ~0.5 m length and 1/4" outer diameter, with a  
137 flow rate of 0.5 L·min<sup>-1</sup>. Most of the sample air was directed to the exhaust, while the  
138 actual flow into the FIMR was around 0.15 L·min<sup>-1</sup>. In typical experiments, the FIMR  
139 was operated at a pressure of 2.0 mbar and a temperature of 373.15 K. The axial and  
140 radial voltages were normally set to be 625 and 500 V, respectively, unless stated  
141 otherwise.

142 We also performed experiments by varying the instrument settings such as FIMR  
143 axial voltage (V) and FIMR pressure (p), both of which affect the E/N ratio, as well as  
144 RF and BSQ amplitudes to investigate how protonated, adduct, and fragmented ions  
145 respond to those changes. These experiments were performed under dry (RH ~5%)  
146 conditions, and the concentrations were approximately 12 ppbv for most VOCs (except  
147 for  $\beta$ -caryophyllene at about 1.2 ppbv). The instrument settings were varied by: 1)  
148 changing the FIMR axial voltage from 260 to 700 volts, 2) changing the pressure in  
149 FIMR from 1.5 to 3.5 mbar; 3) changing the RF amplitude from 13 to 500 volts (with  
150 p of 2.0 or 3.5 mbar); 4) changing the BSQ voltage from 50 to 300 volts (with p of 2.0  
151 or 3.5 mbar). The other instrument settings were fixed as the default values while  
152 changing the tested ones. Specifically, RF amplitude was at 500 volts and BSQ  
153 amplitude was at 300 volts when changing E (i.e., V) and N (i.e., p), and an E/N ratio  
154 of 142 Td was used when changing RF and BSQ amplitudes (Table S1).

## 155 **2.2 Experimental setup**

156 The VOCs (Table S2 and Figure 1) in mixtures from two cylinders were separately  
157 delivered to the dilution and/or RH control setup (Figure S1). Dilution air was generated  
158 from a zero-air generator (EnviroNics series 7000, EnviroNics Analytics Group Ltd.,  
159 Canada). Gas cylinder I (Table 1, Apel-Riemer Environmental Inc., US, valid for 12  
160 months) contains mainly hydrocarbons, while gas cylinder II (Table 1, Linde Gases,  
161 US, valid for 12 months) contains mainly OVOCs and nitriles. Most VOCs in the  
162 cylinders are at approximately 1000 ppbv, except for  $\beta$ -caryophyllene that is at  
163 approximately 100 ppbv. Table S2 shows their CAS numbers,  $m/Q$  values of the

164 protonated ions ( $MH^+$ ), as well as PA and  $k_{ptr}$  values. According to their functional  
165 groups, the 21 VOCs are grouped into 9 categories, and Figure 1 shows their structures.  
166 Note that although n-butanal and methyl ethyl ketone are isomers, they are in different  
167 cylinders and measured separately, thus will not interfere with each other.  
168 Dry experiments were performed by diluting the VOCs from the cylinders with dry zero  
169 air with 7 concentrations from 0 to approximately 22 ppbv (or approximately 2 ppbv  
170 for  $\beta$ -caryophyllene). For each concentration step, measurements lasted for about half  
171 an hour for gas cylinder I with hydrocarbons but about two hours for gas cylinder II  
172 with OVOCs and nitriles. The 2-hour stabilization time for cylinder II, which contained  
173 mainly OVOCs and nitriles, should be sufficient because even with half-an-hour  
174 stabilization time for cylinder I, the overlapping species acetone and acetaldehyde  
175 showed deviations of less than  $\pm 1.5\%$  in sensitivity. Other measures such as minimizing  
176 the length of the Teflon tube at the inlet (less than 30 cm) were also undertaken to allow  
177 fast establishment of equilibrium-state concentrations for OVOCs. In RH-dependent  
178 experiments (Figure S1), dilution was made by RH-conditioned air produced from a  
179 humidity generator (OHG-4, Owlstone, US). The accuracy of the RH sensor (RH-USB  
180 Probe, Omega) is within 4% of RH. Nine RH ramping steps from  $\sim 5\%$  to  $\sim 85\%$  with  
181 approximately 10% intervals were used, and the VOCs were set with 4 concentrations  
182 from 0 to approximately 12 ppbv (or approximately 1.2 ppbv for  $\beta$ -caryophyllene).  
183 After the initial equilibration of 0.5 hours under dry conditions (RH  $\sim 5\%$ ), each RH  
184 ramping lasted for 15 min. Triplicate experiments were performed for the highest  
185 concentration.

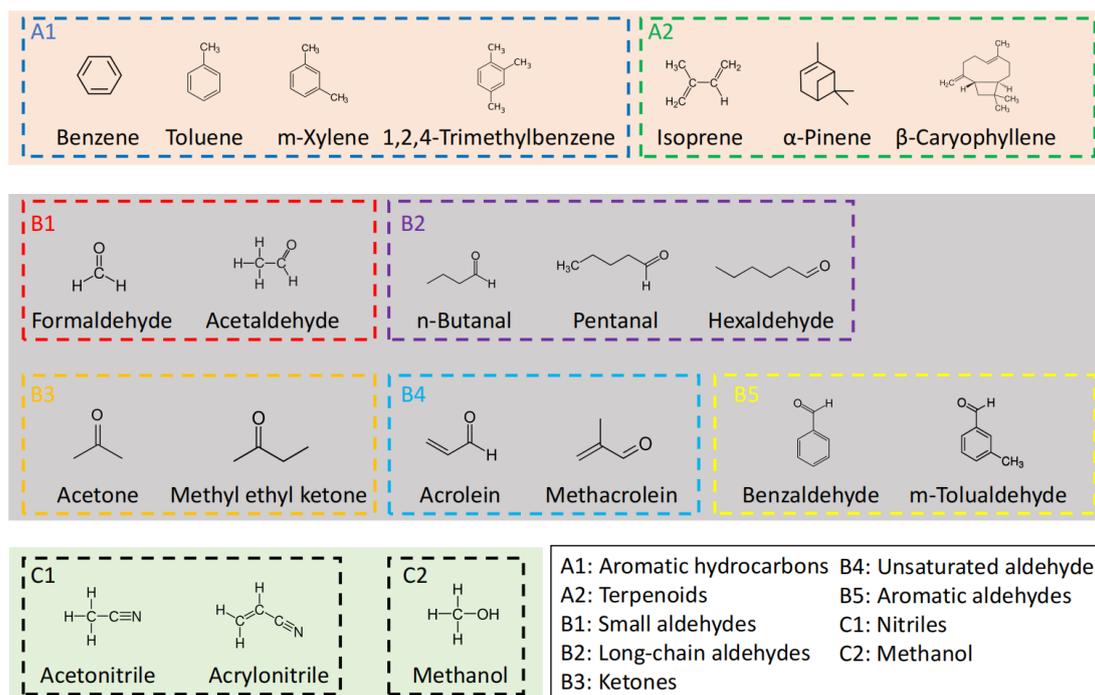

186

187

188

189

190

191

Figure 1. Names, structures, and grouping of the 21 VOCs in this study. These VOCs were prepared in two gas standard cylinders (I and II) with mixing ratios of  $\sim 1000$  ppbv ( $\sim 100$  ppbv for  $\beta$ -caryophyllene), balanced by  $N_2$ . Acetaldehyde and acetone are present in both gas standard cylinders, with concentrations differing by  $<5\%$ . n-Butanal and methyl ethyl ketone are isomers but are in different gas standard cylinders.

192

### 2.3 Data analysis

193

194

195

196

197

198

199


200

201

202

203

The Vocus data were analyzed with the manufacturer-supplied software package Tofware (v3.2.3) based on Igor Pro (Wavemetrics). Peak fitting was performed using Tofware routines and the measured  $m/Q$  values of the protonated ions ( $MH^+$ ) are shown in Table S2 together with their exact  $m/Q$  values. In addition to  $MH^+$ , we also looked for adduct ions ( $[MH + H_2O]^+$ ), and fragmented ions ( $[MH - H_2O]^+$  or  $[MH - C_xH_y]^+$ ), since those ions are also anticipated for VOCs, especially OVOCs, in PTR-MS measurements (Pagonis et al., 2019). Although the VOCs were in mixtures and showed ensemble mass spectra, we constructed the mass spectrum for each VOC by plotting their identified adduct or fragmented ions alongside the protonated ions, as shown in Figures S2-S4 in the SI. Their percentage contributions are presented in Figure 2 and numerically in Table S4.

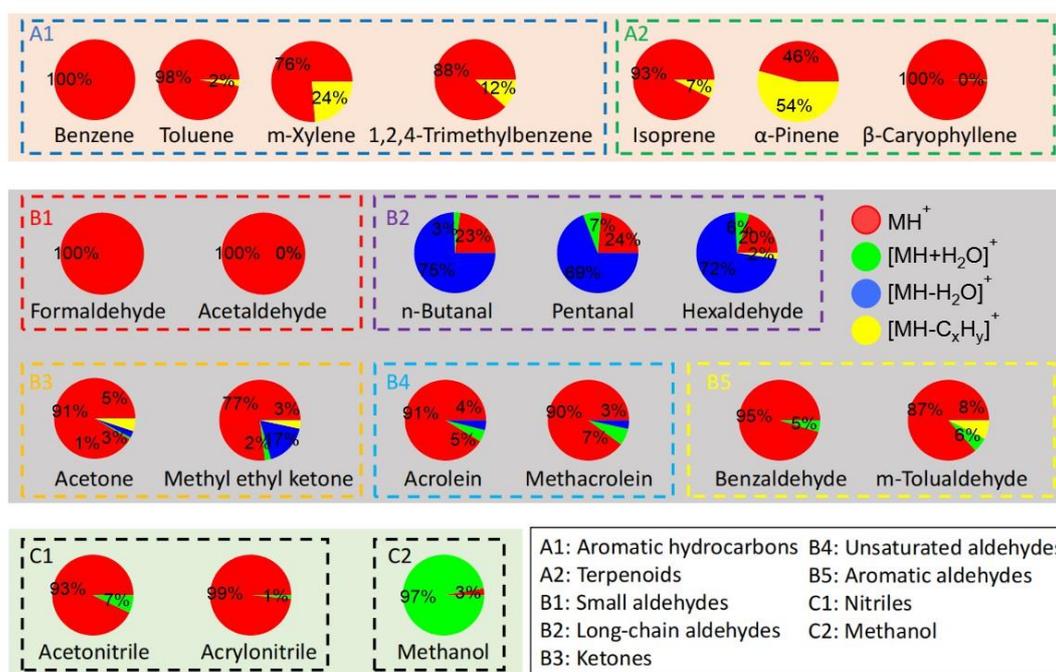

204  
 205 Figure 2. The average signal percentages of protonated, adduct, and fragmented ions  
 206 at a concentration of ~12 ppbv (~1.2 ppbv for β-caryophyllene).

207 For both dry and RH-dependent experiments, from the 1-minute averages from 1-  
 208 Hz datasets, the last five points were averaged to obtain stable signals. Figure S5 shows  
 209 the time series of selected hydrocarbons (groups A1 and A2, aromatic hydrocarbons  
 210 and terpenoids, Figure S5a) and OVOCs (groups B2 and B5, long-chain and aromatic  
 211 aldehydes, Figure S5b) during dry experiments with concentration stepping. Figure S6  
 212 shows the time series of protonated ions (MH<sup>+</sup>), adduct ions ([MH + H<sub>2</sub>O]<sup>+</sup>), and  
 213 fragmented ions ([MH - H<sub>2</sub>O]<sup>+</sup> and/or [MH - C<sub>x</sub>H<sub>y</sub>]<sup>+</sup>) for n-butanal, pentanal and  
 214 hexaldehyde, whose adduct and fragmented ions contributed substantially to the total  
 215 signals (Figure 2 and Table S4). Some dealkylated fragments ([MH - C<sub>x</sub>H<sub>y</sub>]<sup>+</sup>) of long-  
 216 chain aldehydes (e.g., n-butanal and pentanal) might overlap with the protonated ions  
 217 ([MH]<sup>+</sup>) of unsaturated aldehydes (i.e., acrolein and methacrolein). Yet since the  
 218 intensities of the former are expected to be low by analogy with that of hexaldehyde  
 219 (~2%, Figure 2), the ions at those *m/Q* values are only considered as the protonated ions  
 220 of unsaturated aldehydes (the latter).

221 Similar to RH-dependent experiments, the duration of each instrument setting  
 222 experiment was 15 min. The signal intensities and the ratio of MH<sup>+</sup>, [MH + H<sub>2</sub>O]<sup>+</sup> and  
 223 [MH - H<sub>2</sub>O]<sup>+</sup> and/or [MH - C<sub>x</sub>H<sub>y</sub>]<sup>+</sup> to all for two typical hydrocarbons (α-pinene and  
 224 1,2,4-trimethylbenzene) and two OVOCs (acetone and hexaldehyde) as the axial  
 225 voltage and pressure (which both affects the E/N ratio) in the FIMR, RF amplitude, and

226 BSQ amplitude varied are shown in Figures S7 to S10. The reduced electric field  
227 parameter (E/N ratio) was estimated by comparing the signal fraction of fragment of  $\alpha$ -  
228 pinene in Materić et al. (2017), in which detailed examination on fragment signal  
229 fraction at different E/N ratio was performed (Figure S11).

## 230 2.4 Sensitivity estimation

231 The formation of the protonated ion  $MH^+$  via reaction R1 is desirable for  
232 quantification of VOCs, which is described by the kinetics of the proton-transfer  
233 reaction (de Gouw and Warneke, 2007; Yuan et al., 2017):

$$234 \quad [MH^+] = [H_3O^+]_0 (1 - e^{-k[M]\Delta t}) \quad (\text{Eq. 1})$$

235 where  $[MH^+]$  is the number concentration of the protonated ion,  $[H_3O^+]_0$  that of the  
236 initial hydronium ion,  $k$  is the rate constant of R1 ( $k_{\text{ptr}}$ ),  $[M]$  is the number concentration  
237 of the target VOCs in the sample air, and  $\Delta t$  is the reaction time in the FIMR. Two  
238 conditions allow simplification of Eq. 1 to Eq. 2 below for easy quantification of VOCs:  
239 1) The term  $k[M]\Delta t$  is much smaller than 1, such that R1 can be considered essentially  
240 first-order; and 2)  $H_3O^+$  is not significantly depleted and remain more or less constant  
241 after the FIMR. Compared with traditional ion sources, the Vocus ion source produces  
242 sufficient  $H_3O^+$  (Krechmer et al., 2018). Ambient levels of ppbv (or less) for  $[M]$  ( $\sim 10^{10}$   
243 molecule  $\text{cm}^{-3}$ ) generally fulfill such requirements, given that  $k_{\text{ptr}}$  is on the order of  $10^{-9}$   
244  $\text{cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$  and  $\Delta t$  of  $10^{-4}$  s (Ellis and Mayhew, 2014). Therefore,

$$245 \quad [MH^+] = [H_3O^+]k[M]\Delta t \quad (\text{Eq. 2})$$

246 where  $[H_3O^+]$  is the mixing ratio of hydronium ions after the FIMR (i.e., being detected  
247 in the mass spectrometer). Then,

$$248 \quad [M] = \frac{I_{MH^+}}{I_{H_3O^+}} \frac{1}{k\Delta t} \quad (\text{Eq. 3})$$

249 where  $I_{MH^+}$  and  $I_{H_3O^+}$  are signal intensities of the protonated ion and the hydronium ion,  
250 respectively.

251 In general, the sensitivity (S) of PTR-MS for quantification of VOCs is defined as  
252 the ratio between the signal intensity  $I_{MH^+}$  normalized by  $10^6$  cps (counts per second) of  
253  $I_{H_3O^+}$  and 1 ppbv ( $10^{-9} \text{ mol mol}^{-1}$ ) of VOCs, i.e.:

254 
$$S = \frac{\frac{I_{MH^+}}{I_{H_3O^+}} \times 10^6}{\frac{[M]}{N} \times 10^9} \quad (\text{Eq. 4})$$

255 where N is the number density of air in the FIMR. The sensitivity S is thus expressed  
 256 as a normalized signal per ppbv, having a unit of ncps ppbv<sup>-1</sup>. Combining Eq. 3 and Eq.  
 257 4 yields,

258 
$$S = 10^{-3} \times N \Delta t \times k \quad (\text{Eq. 5})$$

259 where 10<sup>-3</sup> × N Δt is specific to the instrumental settings. Eq. 5 dictates that S should  
 260 have a linear relationship with the proton-transfer reaction rate constant (*k*<sub>ptr</sub>) if the  
 261 instrument settings are fixed and can be utilized to predict S if *k*<sub>ptr</sub> values are known  
 262 (Ellis and Mayhew, 2014).

263 In reality, however, quantification of VOCs using MH<sup>+</sup> from PTR-MS  
 264 measurements is complicated by 1) formation of adduct (e.g., with H<sub>2</sub>O) and  
 265 fragmented (e.g., dehydration) ions, and 2) discriminated transmission for MH<sup>+</sup> ions  
 266 with different *m/Q* values (de Gouw and Warneke, 2007; Yuan et al., 2017). The fraction  
 267 of MH<sup>+</sup> in all related ions (*f*<sub>MH<sup>+</sup></sub>) and the relative transmission efficiency (*T*<sub>MH<sup>+</sup></sub>/*T*<sub>H<sub>3</sub>O<sup>+</sup></sub>)  
 268 are used to account for these two effects, respectively:

269 
$$S = 10^{-3} \times N \Delta t \times \frac{T_{MH^+}}{T_{H_3O^+}} \times f_{MH^+} \times k \quad (\text{Eq. 6})$$

270 In our study, the sensitivity is expressed as the slope of signal intensity (in counts  
 271 per second, cps) vs. concentration (in ppbv), having a unit of cps ppbv<sup>-1</sup> (Figure S12).  
 272 Signal normalization to H<sub>3</sub>O<sup>+</sup> (ncps) was not adopted because the signal of H<sub>3</sub>O<sup>+</sup> (*m/Q*  
 273 = 19 Th) was substantially suppressed with low transmission (see below) for those ions  
 274 with small *m/Q* values (but too high intensities) to minimize ion currents.


## 275 **3 Results and Discussion**

### 276 **3.1 Effects of instrumental settings on the ion signals**

277 An increase of the E/N ratio from 48 to 142 Td manifested by the increases of the  
 278 FIMR axial voltage (V, with front from 226 to 666 volts and back keeps at 34 volts) led  
 279 to drastic increases of MH<sup>+</sup> signal intensity by three to four orders of magnitude for all  
 280 VOCs studied (Figure 3a). Such increases were also observed for adduct and

281 fragmented ions (Figures S7 - S10), albeit to different extents. It has been shown that  
282 increasing the axial voltage in the FIMR can substantially increase protonated ion  
283 signals, which is due mainly to three reasons (Krechmer et al., 2018; de Gouw and  
284 Warneke, 2007). First, a high FIMR axial voltage can accelerate the ions and thus  
285 reduce their residence time, thereby preventing diffusional loss. Second, the high  
286 voltage in FIMR significantly increases the concentration of all reagent ions (Figure  
287 S13). Lastly, at high voltage, reactions between some OVOCs (such as acetone) and  
288  $\text{H}_3\text{O}^+$  leads to more protonated ions ( $\text{MH}^+$ ) instead of adduct ions ( $[\text{MH} + \text{H}_2\text{O}]^+$ )  
289 through ligand switching reaction (R2b). The last effect was believed to be less  
290 significant for species that do not readily react with  $\text{H}_3\text{O}^+(\text{H}_2\text{O})_n$  (such as aromatics and  
291 terpenoids).

■ Aromatic hydrocarbons ■ Terpenoids ■ Small aldehydes ■ Long-chain aldehydes  
■ Ketones ■ Unsaturated aldehydes ■ Aromatic aldehydes ■ Nitriles ■ Methanol

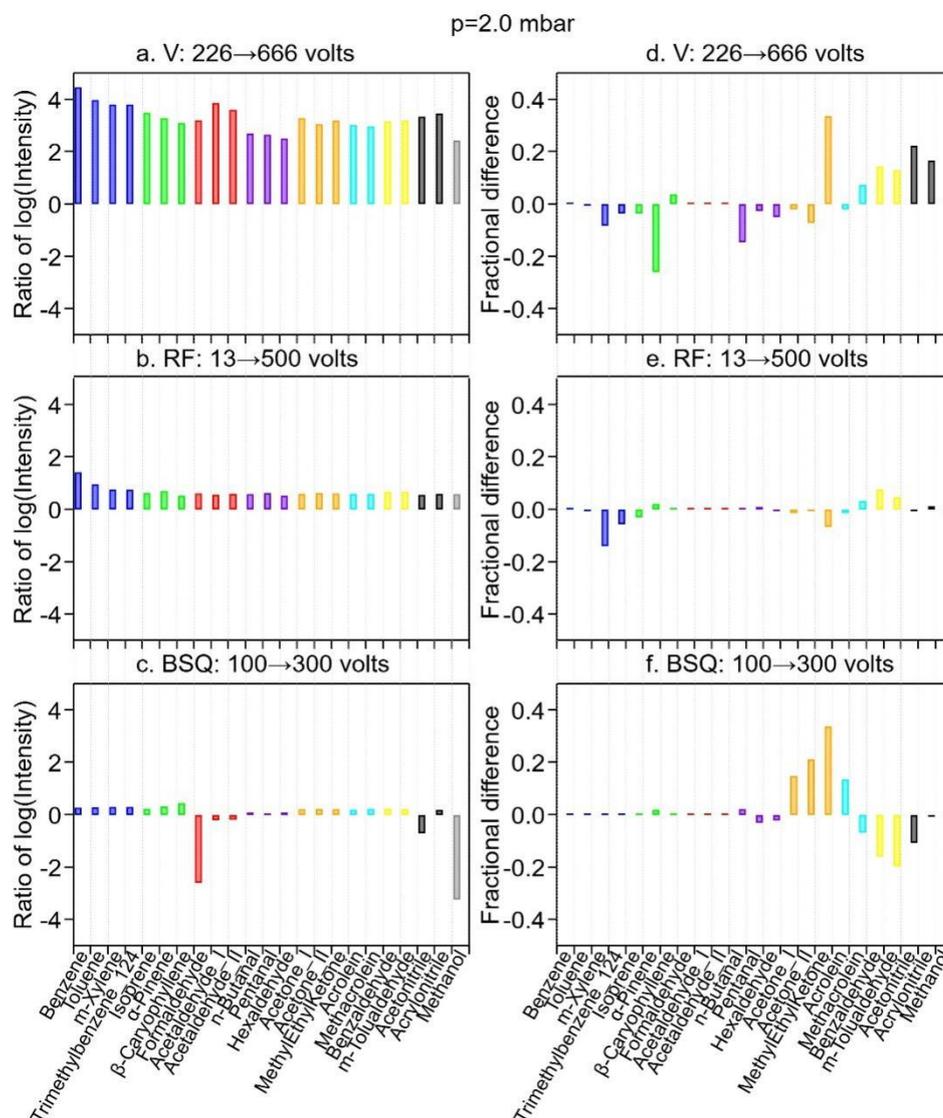

292  
 293 Figure 3. The ratio of the logarithm of intensity (panels a, b, and c) and the difference  
 294 of fractional signal of the protonated ion ( $MH^+$ ) among all ions (panels d, e, and f),  
 295 when changing axial voltage (V) or FIMR pressure (p) (panels a and d), RF amplitude  
 296 (panels b and e), and BSQ amplitude (panels c and f). The ratios were taken after taking  
 297 the logarithm of the signal intensities of  $MH^+$  at the right-hand side of the instrument  
 298 setting (after the arrow) to that at the left-hand side of the instrument setting stated in  
 299 the panel label; likewise, the fractional differences are the fractions of the  $MH^+$  signal  
 300 among the protonated, fragmented, and adduct signals under these two instrumental  
 301 settings.

302 To investigate whether the desired  $\text{MH}^+$  is indeed more favorably formed by  
303 suppressing R2b under high axial voltages, we plot the differences in the signal  
304 fractions of  $\text{MH}^+$  between axial voltages of 666 volts and 226 volts (Figure 3d). The  
305 results show that about one-third of the 21 VOCs do not have significant differences in  
306 the signal fractions: most VOCs in this one-third have the  $\text{MH}^+$  as the sole or  
307 dominating ion observed (*cf.*, Figure 2). Meanwhile, there are about one-third showing  
308 negative differences (i.e., decreasing  $\text{MH}^+$  fractions) of up to 0.2, including the two  
309 hydrocarbons and two OVOCs shown in panel d of Figures S7 – S10. The remaining  
310 one-third show positive differences (i.e., increasing  $\text{MH}^+$  fractions) of up to 0.3, mainly  
311 for unsaturated or aromatic aldehydes, as well as nitriles (Figure 3d). A closer  
312 inspection of the fractional changes as axial voltage increases for acetone (Figure S9d)  
313 and hexaldehyde (Figure S10d) reveals that the fractions of both  $\text{MH}^+$  and  $[\text{MH} + \text{H}_2\text{O}]^+$   
314 decrease, while those of fragmented ions ( $[\text{MH} - \text{H}_2\text{O}]^+$  and/or  $[\text{MH} - \text{C}_x\text{H}_y]^+$ ) increase.  
315 The relative decreases of the signal fractions of  $\text{MH}^+$  (8% for acetone and 51% for  
316 hexaldehyde) are, however, much lower than those of  $[\text{MH} + \text{H}_2\text{O}]^+$  (57% for acetone  
317 and 80% for hexaldehyde). These observations suggest that while fractions of both  $\text{MH}^+$   
318 and  $[\text{MH} + \text{H}_2\text{O}]^+$  decrease, the decreases of the adduct ion ( $[\text{MH} + \text{H}_2\text{O}]^+$ ) are more  
319 significant, supporting the third reason that relatively more  $\text{H}_3\text{O}^+$  (instead of  
320  $\text{H}_3\text{O}^+(\text{H}_2\text{O})_n$ ) at higher axial voltages to react with these OVOCs. However, as the  
321 voltage increases, all ion signals are increasing (Figure S7a-S10a). This observation  
322 illustrates that the ion acceleration and diffusion prevention should be the primary  
323 reason for signal enhancement at high axial voltages. Nevertheless, the signal fractions  
324 of the  $\text{MH}^+$  do not change substantially (within 30%) as the FIMR axial voltage  
325 increases, making quantification reliable even for species with high signal contributions  
326 from adduct and fragmented ions (e.g., long-chain aldehydes, group B2, *cf.*, Figure 2).

327 The increase of E/N ratio by decreasing FIMR pressure from 3.5 to 1.5 mbar  
328 increases signal intensities (Figure S14a) of  $\text{MH}^+$  by less than one order of magnitude,  
329 or even decreases those for some OVOCs such as long-chain aldehydes. The changes  
330 in signal fractions of  $\text{MH}^+$  (Figure S14d), on the other hand, are more than those when  
331 changing axial voltages, especially for ketones, unsaturated aldehydes, aromatic  
332 aldehydes, and nitriles. The increase of pressure in the PTR reactor also favors the  
333 formation of reagent clusters  $\text{H}_3\text{O}^+(\text{H}_2\text{O})_n$ , which leads to the formation of adduct ions  
334 (Wang et al., 2020). For OVOCs acetone and hexaldehyde, the fractions of  $\text{MH}^+$  do

335 increase when FIMR pressure was decreased from 3.5 to 2.5 mbar (E/N ratio from 162  
336 to 95), which is accompanied by significant decreases of the adduct ion  $[\text{MH} + \text{H}_2\text{O}]^+$   
337 (Figure S9j and Figure S10j). This observation suggests less formation of adduct ions  
338 at lower FIMR pressures. Further decrease of FIMR pressure to 1.5 mbar, however,  
339 results in slight decreases of  $\text{MH}^+$  fractions, in lieu of increases of fragmented ions  $[\text{MH}$   
340  $-\text{H}_2\text{O}]^+$  and  $[\text{MH} - \text{C}_x\text{H}_y]^+$  (Figure S9j and Figure S10j); for hydrocarbons  $\alpha$ -pinene  
341 and 1,2,4-trimethylbenzene (Figure S7j and Figure S8j) that only have  $\text{MH}^+$  and  $[\text{MH}$   
342  $-\text{C}_x\text{H}_y]^+$ , continuous decreases of  $\text{MH}^+$  fractions and increases of  $[\text{MH} - \text{C}_x\text{H}_y]^+$  are  
343 observed for the whole range of FIMR pressure tested (3.5 to 1.5 mbar). A recent study  
344 using Vocus PTR-MS to measure organic peroxides also observed that less fragmented  
345 ions were formed under higher FIMR pressure (Li et al., 2022), presumably due to the  
346 efficient transfer of excess kinetic energy by frequent collisions at higher pressures. A  
347 medium FIMR pressure of 2.0 mbar was chosen to have relatively low fractions of both  
348 adduct ions ( $[\text{MH} + \text{H}_2\text{O}]^+$ ) and fragmented ions ( $[\text{MH} - \text{H}_2\text{O}]^+$  and  $[\text{MH} - \text{C}_x\text{H}_y]^+$ ).

349 The radial RF electric field in the FIMR is unique for the Vocus PTR-MS, which  
350 can (1) collimate the ions towards the central axis (especially heavier ions) and (2)  
351 increase the kinetic energy of the ions (especially for lighter ions) (Krechmer et al.,  
352 2018). These effects led to 1 to 1.5 orders of magnitude higher signals for  $\text{MH}^+$  at 2.0  
353 mbar FIMR pressure (Figure 3b) and 1.5 to 2 orders of magnitude at 3.5 mbar (Figure  
354 S14b) when the RF amplitude was changed from 13 to 500 volts. The additional  
355 enhancement of signal intensity at a higher FIMR pressure (i.e., 3.5 mbar as compared  
356 to 2.0 mbar) can be attributed to a longer residence time of the reagent ions (Krechmer  
357 et al., 2018). The more pronounced increase of kinetic energy for lighter ions (e.g.,  
358  $\text{H}_3\text{O}^+$ ) than heavier ions [i.e., clusters  $\text{H}_3\text{O}^+(\text{H}_2\text{O})_n$ ] might imply the favorable  
359 formation of the protonated ion  $\text{MH}^+$  rather than adduct ions. The fractions of  $\text{MH}^+$  for  
360 different RF amplitudes do not change significantly (within  $\pm 0.2$ ) either at 2.0 mbar  
361 (Figure 3e) or 3.5 mbar (Figure S14e). This observation thus suggests that adding the  
362 RF can increase signal intensities by 1 – 2 orders of magnitude but does not affect the  
363 fractional signal for  $\text{MH}^+$ , making it beneficial for accurate quantification.

364 The BSQ amplitude above 100 volts does not change the signal intensities  
365 significantly (Figure 3c and Figure S14c, as well as Figures S7– S10). The BSQ ion  
366 guide provides a high-pass band filter to reduce the number of ions (thus signal intensity)  
367 of low  $m/Q$  values (especially for reagent ions,  $\text{H}_3\text{O}^+$ , with high ion currents),

368 preventing the fast degradation of the microchannel plate (MCP) detector (Krechmer et  
369 al., 2018). This bandpass filter leads to lower ion transmission efficiency ( $<1$ ) for ions  
370 with smaller  $m/Q$  values, which is discussed below. Therefore, the signal reduction  
371 when the BSQ amplitude increased from 100 to 300 volts is more obvious for small  
372 analytes such as formaldehyde, acetonitrile, and methanol (Figure 3c and Figure S14c).  
373 For other analytes whose fragmented ions have  $m/Q$  values of less than 60 Th, the signal  
374 fractions of  $MH^+$  would also be affected (Figure 3f and Figure S14f). For example, the  
375 intensities of fragmented ions  $[MH - H_2O]^+$  ( $CH_3CCH_2^+$ ,  $m/Q = 41$  Th) and  $[MH -$   
376  $C_xH_y]^+$  ( $CH_3CO^+$ ,  $m/Q = 43$  Th) for acetone had substantial decreases when BSQ  
377 amplitude was higher than 200 volts (Figure S9c and Figure S10). The protonated ion  
378  $MH^+$  ( $CH_3COCH_3H^+$ ,  $m/Q = 59$  Th) and adduct ion ( $CH_3COCH_3H_3O^+$ ,  $m/Q = 77$  Th),  
379 however, remained less unaffected. This effect leads to noticeable changes in signal  
380 fractions of  $MH^+$  (maximum 0.4) for small analytes such as ketones, unsaturated  
381 aldehydes, nitriles, as well as methanol (Figure 3f and Figure S14f) as the BSQ  
382 amplitude changes from 100 to 300 volts.

### 383 **3.2 Sensitivity and transmission of protonated ions**

384 We calculated the sensitivity and transmission of protonated ions ( $MH^+$ ) of the 21  
385 VOCs studied when the instrument was under the optimized conditions. Table 1 shows  
386 the sensitivities (cps ppbv<sup>-1</sup>), as slopes of  $MH^+$  signals vs. mixing ratios (average value  
387 from 0 to 22 ppbv at dry condition, except for  $\beta$ -caryophyllene to 2 ppbv) and the limit  
388 of detection (LOD,  $3\sigma$ ). Panels a and b in Figure 4 show the sensitivity vs.  $k_{ptr}$  for all  
389 21 VOCs, while panels c and d show the transmission efficiencies calculated from the  
390 division of the sensitivity vs.  $k_{ptr}$  ratio for each VOC by the slope fitted in Figure 4a and  
391 4b.

392 Most VOCs had sensitivities above 1000 cps ppbv<sup>-1</sup>, except 1) formaldehyde (A2-  
393 1) and methanol (C2-1), whose  $MH^+$  ions have  $m/Q$  values much lower than 60 Th; and  
394 2)  $\beta$ -caryophyllene (A2-3) that came with a very low concentration range. In addition  
395 to its low  $m/Q$  values that limit the transmission, the backward reaction is also an  
396 important reason for the low sensitivity. For instance, formaldehyde has a low PA value  
397 (712.5 kJ mol<sup>-1</sup>) that is not much higher than that of water (691.0 kJ mol<sup>-1</sup>) and has been  
398 shown to have a high tendency of backward reaction of R1 (Inomata et al.,  
399 2008; Vlasenko et al., 2010; Warneke et al., 2011). The two compounds in group B5

400 (aromatic aldehydes), benzaldehyde and m-tolualdehyde, had the highest sensitivities  
 401 of >12000 cps ppbv<sup>-1</sup>. This might be due to their high PA values (>830 kJ mol<sup>-1</sup>), which  
 402 are among the highest except those of terpenoids (Table S2).

403 Table 1. Sensitivity (slope), intercept, and limit of detection (LOD) based on 3 standard  
 404 deviations ( $\sigma$ ) and cylinder numbers (No.). Results were obtained from measurements  
 405 of 0 – 22 ppbv for all VOCs except for  $\beta$ -caryophyllene (up to ~2 ppbv). [The cylinder](#)  
 406 [numbers for the VOCs studied are also shown here.](#)

Group <sup>a</sup>	Name	Cylinder No.	Label	Sensitivity (cps ppbv <sup>-1</sup> )	3 $\sigma$ LOD (pptv), 5 s
A1	Benzene	I	A1-1	2596	35
	Toluene	I	A1-2	5724	2
	m-Xylene	I	A1-3	8669	3
	1,2,4-Trimethylbenzene	I	A1-4	8951	1
A2	Isoprene	I	A2-1	2140	16
	$\alpha$ -Pinene	I	A2-2	4046	2
	$\beta$ -Caryophyllene	I	A2-3	723	1
B1	Formaldehyde	II	B1-1	— <sup>c</sup>	— <sup>c</sup>
	Acetaldehyde	I&II	B1-2	2096 <sup>b</sup>	283
B2	n-Butanal	II	B2-1	1114	343
	Pentanal	II	B2-2	1465	63
	Hexaldehyde	II	B2-3	1595	35
B3	Acetone	I&II	B3-1	9932 <sup>b</sup>	127
	Methyl ethyl ketone	I	B3-3	9636	51
B4	Acrolein	I	B4-1	7224	16
	Methacrolein	I	B4-2	6090	13
B5	Benzaldehyde	II	B5-1	16089	1
	m-Tolualdehyde	II	B5-2	12893	1
C1	Acetonitrile	I	C1-1	1511	6
	Acrylonitrile	I	C1-2	9275	1
C2	Methanol	I	C2-1	— <sup>c</sup>	— <sup>c</sup>


407 Notes:

408 a, A1: aromatic hydrocarbons, A2: terpenoids, B1: small aldehydes; B2: long-chain aldehydes, B3:  
 409 ketones, B4: unsaturated aldehydes, B5: aromatic aldehydes, C1: nitriles, C2: methanol;

410 b, the average value from gas cylinders I and II, [with a deviation of less than  \$\pm 1.5\%\$ .](#);

411 c, low sensitivity and high LOD due to low transmission.

412

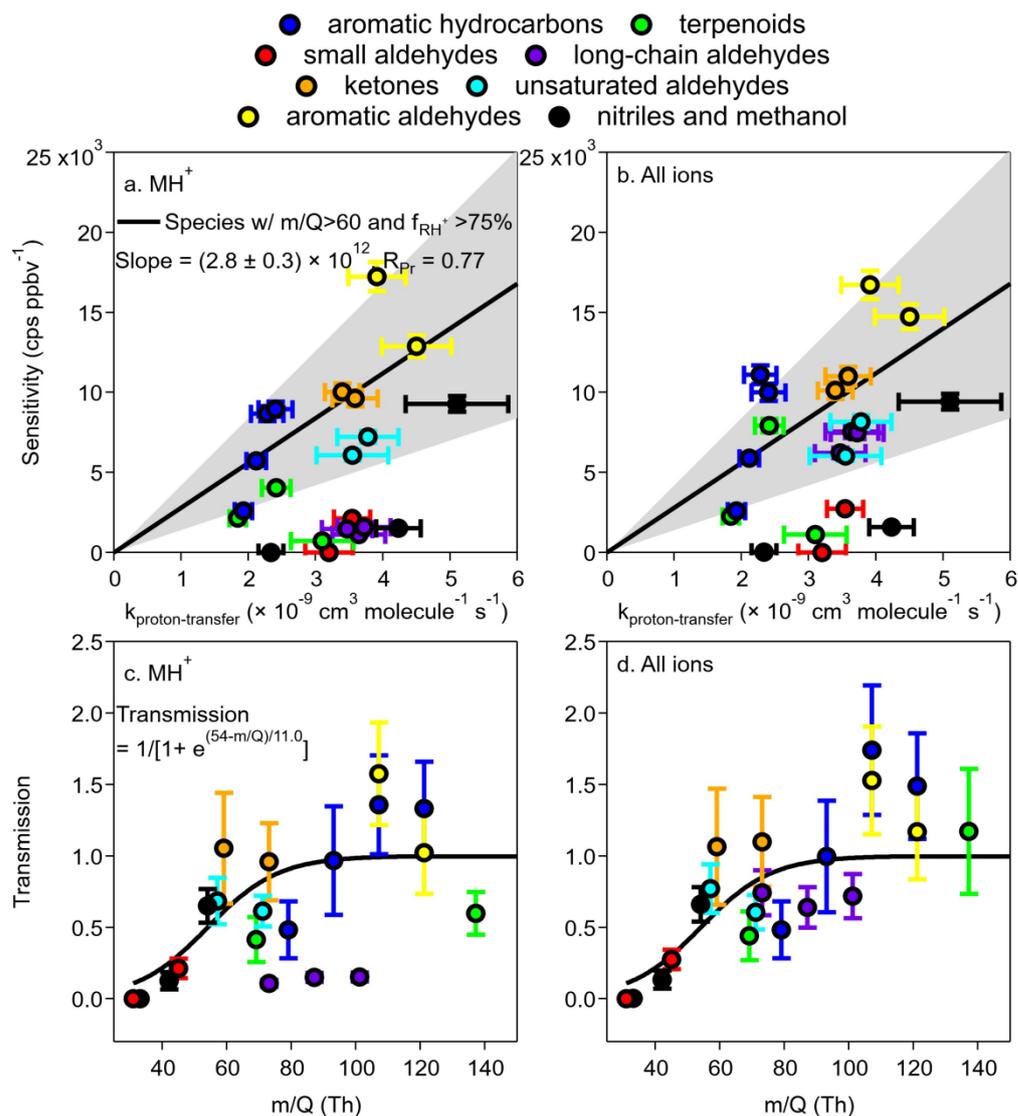

413  
 414 Figure 4. Sensitivity as a function of  $k_{\text{ptr}}$  for (a)  $\text{MH}^+$  and (b) all ions. Linear fitting was  
 415 performed only for  $\text{MH}^+$  sensitivity. Species included in the fitting were those with  $m/Q$   
 416 value  $> 60$  Th (Table S2) and signal percentage of  $\text{MH}^+$  ( $f_{\text{MH}^+}$ )  $> 75\%$  (Table 1). The  
 417 grey-shaded area is bounded by  $0.5 \times \text{Slope}$  and  $2 \times \text{Slope}$ . The fitted curves in panel b  
 418 are the same as in panel a and are for reference only. Panels c and d are transmission  
 419 curves from  $\text{MH}^+$  only and from the sum of all ions, respectively. The sigmoidal curve  
 420 for  $\text{MH}^+$  (same for c and d) was fitted from species except for  $\beta$ -caryophyllene,  $\alpha$ -pinene,  
 421 n-butanal, pentanal, and hexaldehyde whose fragmentation was significant. Note that  
 422 only the  $m/Q$  values of  $\text{MH}^+$  was used in the x axes of panel c and d, although panel d  
 423 contains information of adduct and fragmented ions that have  $m/Q$  values different from  
 424 that of  $\text{MH}^+$ , which does not consider the differences in  $m/Q$  values of adduct and  
 425 fragmented ions.


426 It was shown that the sensitivities for different VOCs in PTR-MS can be calculated  
427 from the kinetics of the proton-transfer reactions (Warneke et al., 2003; Sekimoto et al.,  
428 2017; Cappellin et al., 2012). For Vocus, Krechmer et al. (2018) also pointed out that  
429 the relationship between sensitivity and  $k_{\text{ptr}}$  can be established and used to calculate the  
430 sensitivity for other compounds. We herein compare the relationship between  
431 sensitivity and  $k_{\text{ptr}}$  (Figure 4a). In our data, the uncertainties for sensitivity were  
432 conservatively taken as the maximum percentage uncertainty (5.3%) of fitted slopes.  
433 Values of  $k_{\text{ptr}}$  were calculated as averages of both modeled and experimental results  
434 found from literature (Table S3), with uncertainties propagated from an estimated  
435 percentage error of 15% for both modeled (Zhao and Zhang, 2004) and experimental  
436 values. The anticipated linear relationship of sensitivity vs.  $k_{\text{ptr}}$  is not easily visible,  
437 most likely due to the formation of fragments/adducts for some VOCs and low  
438 transmission efficiencies for others. However, a relatively improved linear relationship  
439 was found if we limit the VOCs to 1)  $m/Q$  values for  $\text{MH}^+ > 60$  Th, and 2) a fraction of  
440  $\text{MH}^+$  ion in all ions (including adduct/fragmented ions) larger than 75% (*cf.* Figure 2).  
441 With these limitations, the fitted linear line gives a slope of  $(2.8 \pm 0.3) \times 10^{12}$  cps ppbv<sup>-1</sup>  
442  $\text{molec s cm}^{-3}$ , approximately 38% lower than that  $[(4.5 \pm 0.4) \times 10^{12}$  cps ppbv<sup>-1</sup> molec  
443  $\text{s cm}^{-3}]$  of Krechmer et al. (2018). Pearson's R ( $R_{\text{Pr}}$ ) is 0.77. A grey area is also shown  
444 by two lines of  $2 \times$  slope and  $0.5 \times$  slope, which includes approximately half (ten) of  
445 the VOCs studied. Those that fall out of the grey area to the lower region are mainly  
446 compounds in groups B2 (long-chain aldehydes, purple), C1 and C2 (nitriles or  
447 methanol, black), B1 (small aldehydes, red), and A2 (terpenoids, green). Using the total  
448 signals of all ions (protonated, adduct, and fragmented), Figure 4b shows the  
449 improvements for compounds in group B2 only, while others (especially those in C1,  
450 C2, and B1) do not move up to the grey area.

451 We also calculated the transmission efficiencies (Figure 4c and 4d) from the  
452 division of the sensitivity vs.  $k_{\text{ptr}}$  ratio for each VOC by the slope fitted in Figure 4a. It  
453 is shown that compounds in groups B1, C1, and C2 are mainly on the rising range of  
454 the sigmoidal curve, while the three long-chain aldehydes in group B2 (purple) are well  
455 below the curve if only  $\text{MH}^+$  ions were used; these three long-chain aldehydes move up  
456 to transmission  $> 0.5$  when all ions are considered (Figure 4d). Of particular interest is  
457 the compound  $\alpha$ -pinene, whose transmission was  $< 0.5$  when only the  $\text{MH}^+$  ion was  
458 used, but it increases to about 1.5 when the fragmented ion was considered. Note that

459 in Figure 4d, the  $m/Q$  value of  $MH^+$  was used in the x axis for the summed ion signals,  
460 which might lead to certain bias as the fragmented and adduct ions have different  $m/Q$   
461 values. Nevertheless, the above analysis suggests that both the formation of  
462 adduct/fragmented ions and transmission affect the relationship between sensitivity and  
463  $k_{ptr}$ , which needs precaution when using predicted sensitivity directly from  $k_{ptr}$ . In  
464 addition, one needs to be cautious about the prediction of transmission efficiency with  
465  $m/Q$  greater than 150.

### 466 3.3 RH dependence of ion signals


467 One of the most important reasons for RH dependence is that the distribution of  
468 reagent ions might vary with ambient RH, especially when the abundance of  $H_3O^+$  in  
469 the PTR reactor is not high. While the Vocus has been shown to have abundant enough  
470  $H_3O^+$  (Krechmer et al., 2018), whether it can substantially minimize RH dependence  
471 for most VOCs deserves scrutinization. Figure 5a-h shows the relative sensitivity,  
472 defined as the relative change of sensitivity of  $MH^+$  ion vs. VOC concentration under  
473 different RH conditions. Among the nine groups of VOCs studied, seven groups show  
474 almost flat relative sensitivities within the RH range of ~5% to ~85% (298 K), with the  
475 exceptions of long-chain aldehydes (group B2) that show increasing sensitivities as RH  
476 increases (Figure 5d) and methanol (group C2) showing large variations (Figure 5h).  
477 Some other compounds, such as  $\beta$ -caryophyllene (A2-3, Figure 5b) and formaldehyde  
478 (B1-1, Figure 5c) also show either relatively large uncertainties or fluctuations, which  
479 can be ascribed to their low intensities (*cf.*, Table 1).

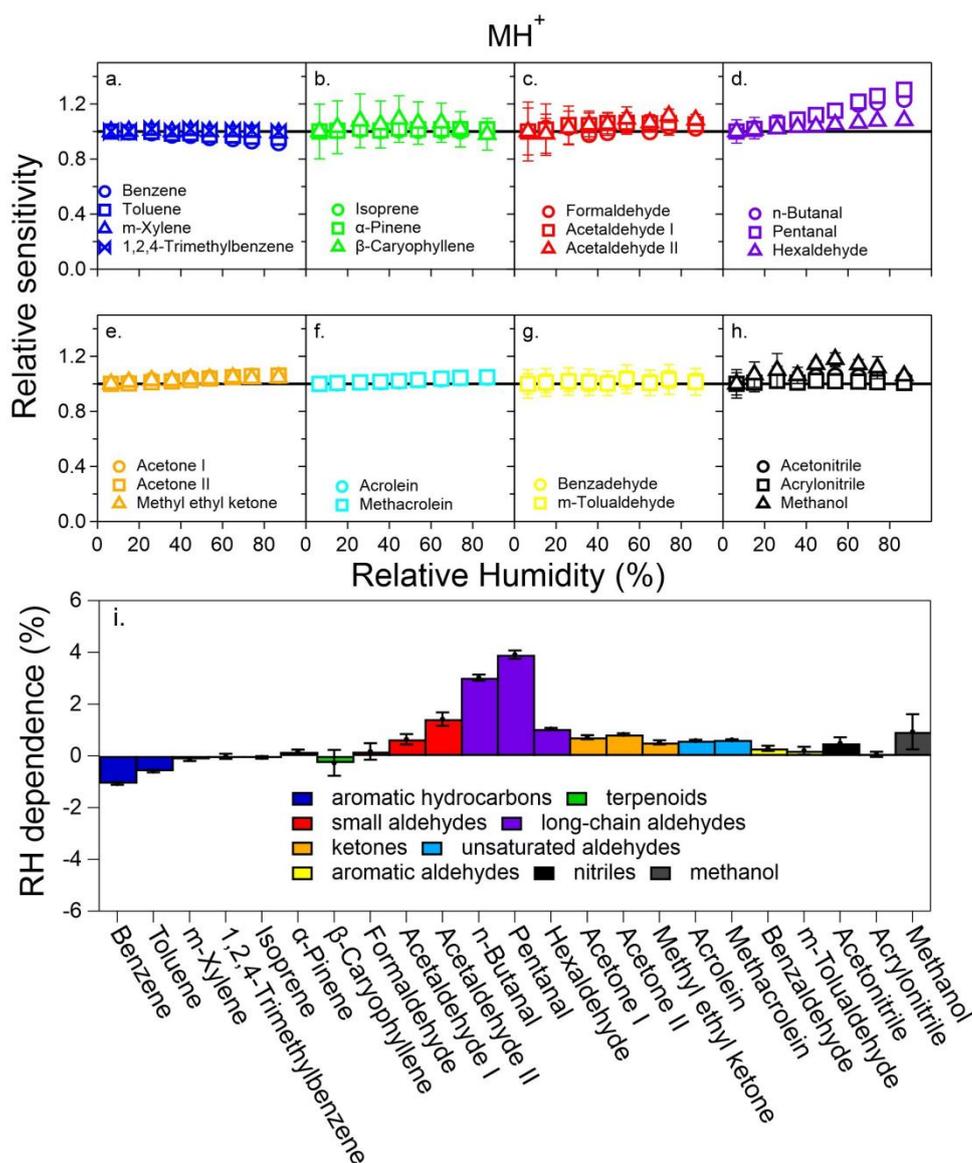

480  
 481 Figure 5. The dependence of the  $MH^+$  signals on RH for the VOCs studied. Panels a-h:  
 482 the relative sensitivity was calculated as the slope (Sensitivity) under all conditions to  
 483 that at the dry (RH<5%) condition. Panel i: the percent change of relative sensitivity  
 484 per 10% RH increase. See Figures S15-S17 for other ion signals.

485 Figure 5i shows the RH dependence of the  $MH^+$  ions, defined as the percentage  
 486 change of sensitivity per 10% RH increase, for all 21 VOCs studied. Aromatic  
 487 hydrocarbons (group A1) show negative RH dependence as in previous studies using  
 488 PTR-MS with a drift tube (Warneke et al., 2001;Steinbacher et al., 2004). While  
 489 previous studies reported decreases in benzene sensitivity by 16 – 56% from dry to  
 490 humid conditions (up to 100% RH), our results show a decrease of less than 1.1% per  
 491 10% RH increase (i.e., <11% in the whole RH range) with a somewhat narrower RH

492 range (up to ~85% RH). In addition, two out of the three terpenoids (group A2) also  
 493 show slightly negative RH dependence, and the **other** one ( $\alpha$ -pinene) shows very small  
 494 positive RH dependence (Figure 5i). These hydrocarbons (aromatics and terpenoids) in  
 495 groups A1 and A2 have relatively low  $k_{\text{ptr}}$  values (mostly  $<2.5 \times 10^{-9} \text{ cm}^3 \text{ molec}^{-1} \text{ s}^{-1}$ ,  
 496 Table S3), and their RH dependence shows a fairly good correlation with the PA value  
 497 (Figure 6a, purple circles and squares). This observation suggests that there might be a  
 498 thermodynamic reason behind the noticeable decrease of sensitivity for hydrocarbons  
 499 such as benzene as RH increases. Since hydrocarbons such as benzene and toluene do  
 500 not readily react with  $\text{H}_3\text{O}^+(\text{H}_2\text{O})$  (Warneke et al., 2001), R1 is the main reaction to  
 501 form  $\text{MH}^+$ . As water vapor concentration increases at high RH, the reverse reaction of  
 502 R1 might be important for compounds with low PA and low  $k_{\text{ptr}}$  values (Inomata et al.,  
 503 2008).

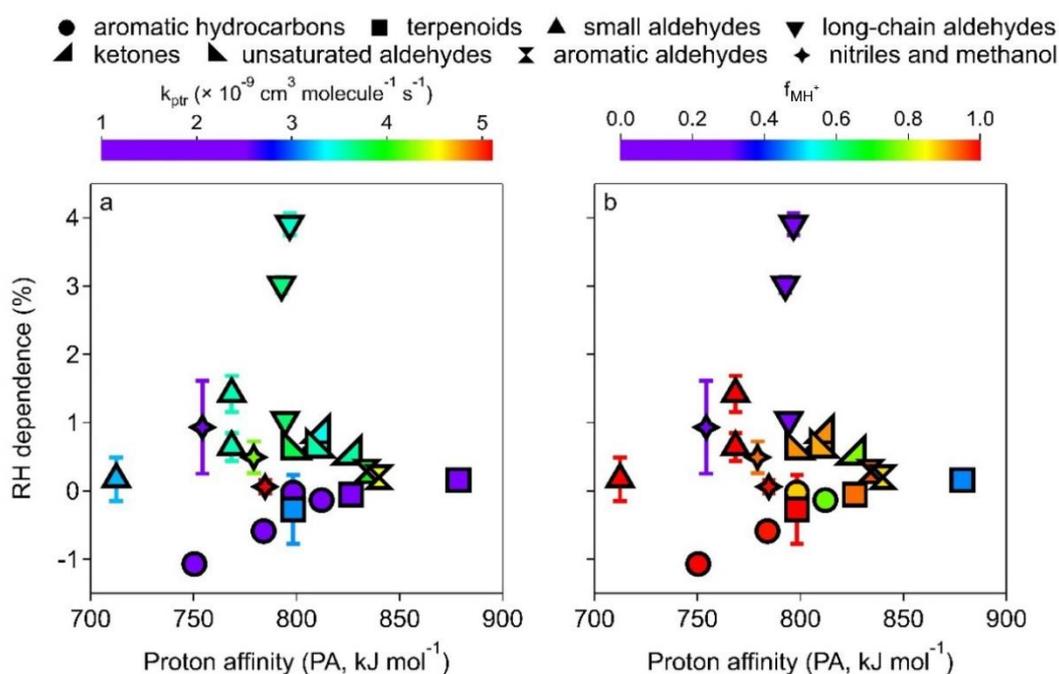

504 Figure 6: The RH dependence of  $\text{MH}^+$  ion plotted against PA, color-coded by (a)  $k_{\text{ptr}}$   
 505 and (b)  $f_{\text{MH}^+}$ .  
 506

507 Long-chain aldehydes (group B2) have the largest RH dependence of 1-4%  
 508 positive deviation per 10% RH increase for the  $\text{MH}^+$  ions. The RH dependence of the  
 509  $[\text{MH} + \text{H}_2\text{O}]^+$  ions (Figure S15g) is even much higher (1.4–8.5% positive deviation per  
 510 10% RH increase). Interestingly, the trends of RH dependence for the  $\text{MH}^+$  ions and  
 511 that for the  $[\text{MH} + \text{H}_2\text{O}]^+$  ions for long-chain aldehydes are exactly opposite (Figure 5i

512 and Figure S15g); that is, pentanal > n-butanal > hexaldehyde. The reason behind this  
513 observation is out of the scope of this study. The dominating  $[\text{MH} - \text{H}_2\text{O}]^+$  ions for  
514 long-chain aldehydes (Figure 2), however, show much less ( $\pm 1\%$  per 10% RH increase)  
515 RH dependence (Figure S16i). Other carbonyl compounds (groups B1, B3, B4, and B5)  
516 also show positive deviations as RH increases (less than 1.5% increase in sensitivity  
517 per 10% RH increase), albeit to various degrees (Figure 5i). Similar to long-chain  
518 aldehydes, their  $[\text{MH} + \text{H}_2\text{O}]^+$  ions also show a large positive deviation (Figure S16g),  
519 and  $[\text{MH} - \text{H}_2\text{O}]^+$  ions show little RH dependence (Figure S16e). These carbonyl  
520 compounds have medium PA values (Figure 6a) except formaldehyde. If we exclude  
521 formaldehyde (with an extremely low PA value, the up triangle to the far left in Figure  
522 6b) and long-chain aldehydes (low percentages of  $\text{MH}^+$  ions, <25%, down triangles in  
523 Figure 6b), the RH dependence of other carbonyl compounds shows a slightly  
524 decreasing trend of RH dependence vs. PA values (Figure 6b, up triangles, left triangles,  
525 right triangles, and double triangles). These observations might hint on the relationships  
526 between the RH dependence of carbonyl compounds and reagent ion distribution as  
527 well as reaction direction for R1-R4, which is different from those for pure  
528 hydrocarbons (groups A1 and A2). Finally, the RH dependence of  $\text{MH}^+$  for compounds  
529 in groups C1 (nitriles) and C2 (methanol) is within +1% per 10% RH increase (Figure  
530 5i).

531 Overall, in the whole RH range studied (~5% to ~85%), the RH dependence of  
532  $\text{MH}^+$  ions for the 21 VOCs studied is less than 30%, with most compounds (except  
533 group B2, long-chain aldehydes) less than 15%. For  $[\text{MH} + \text{H}_2\text{O}]^+$  ions (mainly for  
534 carbonyl compounds), strong RH dependence was observed (Figure S15), being 1.4 –  
535 8.5% per 10% RH increase, or 8.9 – 63.2% from ~5% to ~85% RH. The dehydrated  
536 ions ( $[\text{MH} - \text{H}_2\text{O}]^+$ ), however, show the smallest RH dependence ( $\pm 1\%$  per 10% RH  
537 increase) among all the ions (Figure S16). Fragmented ions with decarbonization ( $[\text{MH}$   
538  $- \text{C}_x\text{H}_y]^+$ ) show mainly negative RH dependence, generally less than 3% per 10% RH  
539 increase (Figure S17).

#### 540 **4 Conclusions**

541 We investigated the response of protonated, adduct, and fragmented ions of 21  
542 atmospherically relevant VOCs in a Vocus PTR-MS as instrument setting and RH  
543 condition vary. For the two ways of increasing the E/N ratio, increasing the FIMR axial

544 voltage can substantially (by three to four orders of magnitude) increase sensitivity but  
545 does not change the fractions of the  $\text{MH}^+$  ions (mostly within 30%); reducing the FIMR  
546 pressure, however, does not enhance sensitivity much but can lead to more substantial  
547 fragmentation. Therefore, a high FIMR axial voltage of 600 – 700 volts and a medium  
548 pressure of around 2.0 mbar are recommended. Increasing the RF amplitude of FIMR  
549 can increase sensitivity by 1 to 1.5 orders of magnitude at 2.0 mbar and 1.5 to 2 orders  
550 of magnitude at 3.5 mbar, and it does not change the  $\text{MH}^+$  ion fractions (within 20%).  
551 Therefore, a high RF amplitude of 500 V is recommended. Increasing the BSQ  
552 amplitude does not increase the sensitivity much but changes the  $\text{MH}^+$  ion fractions of  
553 small ions substantially by changing the transmission efficiency. The choice of this  
554 instrument setting mainly relies on what ions (i.e., those reagent ions with too high an  
555 abundance) one wants to filter out. Our choice is at 300 V, which gives a 50%  
556 transmission at about 55 Th.

557 The relationship between sensitivity and  $k_{\text{pr}}$  is strongly affected by two factors: 1)  
558 whether the  $\text{MH}^+$  ion has a high transmission efficiency, and 2) whether the  $\text{MH}^+$  ion  
559 is the dominating ion. If so, a fairly good correlation ( $R_{\text{Pr}} = 0.77$ ) was observed for the  
560 VOCs studied. The transmission curve is also more reasonably resembling the sigmoid  
561 function only if all the ions (protonated, adduct, and fragmented) are considered. The  
562 low transmission efficiencies of formaldehyde and methanol result in extremely low  
563 sensitivities of these two small OVOCs, although a low PA value is another reason for  
564 the former.

565 As RH increases from ~5% to ~85%, the  $\text{MH}^+$  ions for 19 out of the 21 VOCs  
566 studied have sensitivity variation of less than 15%, but long-chain aldehydes have  
567 positive RH dependence of up to 30%. The RH dependence of  $[\text{MH} + \text{H}_2\text{O}]^+$  ions for  
568 long-chain aldehydes is stronger, while that of the dominating  $[\text{MH} - \text{H}_2\text{O}]^+$  ions is  
569 limited. Therefore, the signal distributions among protonated, adduct, and fragmented  
570 ions are also affected by RH variation. Together with their relatively high background  
571 signals (especially for n-butanal, Figure S5b), quantification of long-chain aldehydes  
572 in the ambient environment using Vocus requires special attention. It is also worth  
573 noting that hydrocarbons generally show slight negative RH dependence, probably due  
574 to their relatively low  $k_{\text{pr}}$  values, although such RH dependence does not affect  
575 quantification significantly; their RH dependence has a fairly good correlation with  
576 their PA values, hinting a thermodynamic reason behind this trend.

577

578 **Competing interests**

579 The authors declare that they have no conflict of interest.

580 **Acknowledgments**

581 This work was supported by funding support from the Science and Technology  
582 Development Fund, Macau SAR (File No. FDCT 0031/2023/AFJ) and a multiyear  
583 research grant (No. MYRG2022-00027-FST) from the University of Macau.

584

- 586 Baasandorj, M., Millet, D. B., Hu, L., Mitroo, D., and Williams, B. J.: Measuring acetic and formic acid  
587 by proton-transfer-reaction mass spectrometry: sensitivity, humidity dependence, and quantifying  
588 interferences, *Atmos. Meas. Tech.*, 8, 1303-1321, <https://doi.org/10.5194/amt-8-1303-2015>, 2015.
- 589 Cappellin, L., Karl, T., Probst, M., Ismailova, O., Winkler, P. M., Soukoulis, C., Aprea, E., Märk, T. D.,  
590 Gasperi, F., and Biasioli, F.: On Quantitative Determination of Volatile Organic Compound  
591 Concentrations Using Proton Transfer Reaction Time-of-Flight Mass Spectrometry, *Environmental  
592 Science & Technology*, 46, 2283-2290, <https://doi.org/10.1021/es203985t>, 2012.
- 593 Claflin, M. S., Pagonis, D., Finewax, Z., Handschy, A. V., Day, D. A., Brown, W. L., Jayne, J. T., Worsnop,  
594 D. R., Jimenez, J. L., Ziemann, P. J., de Gouw, J., and Lerner, B. M.: An in situ gas chromatograph with  
595 automatic detector switching between PTR- and EI-TOF-MS: isomer-resolved measurements of indoor  
596 air, *Atmospheric Measurement Techniques* 14, 133-152, <https://doi.org/10.5194/amt-14-133-2021>, 2021.
- 597 Cui, L., Zhang, Z., Huang, Y., Lee, S. C., Blake, D. R., Ho, K. F., Wang, B., Gao, Y., Wang, X. M., and  
598 Louie, P. K. K.: Measuring OVOCs and VOCs by PTR-MS in an urban roadside microenvironment of  
599 Hong Kong: relative humidity and temperature dependence, and field intercomparisons, *Atmos. Meas.  
600 Tech.*, 9, 5763-5779, <https://doi.org/10.5194/amt-9-5763-2016>, 2016.
- 601 de Gouw, J., and Warneke, C.: Measurements of volatile organic compounds in the earths atmosphere  
602 using proton-transfer-reaction mass spectrometry, *Mass Spectrom Rev*, 26, 223-257,  
603 <https://doi.org/10.1002/mas.20119>, 2007.
- 604 de Gouw, J. A., Goldan, P. D., Warneke, C., Kuster, W. C., Roberts, J. M., Marchewka, M., Bertman, S.  
605 B., Pszenny, A. A. P., and Keene, W. C.: Validation of proton transfer reaction-mass spectrometry (PTR-  
606 MS) measurements of gas-phase organic compounds in the atmosphere during the New England Air  
607 Quality Study (NEAQS) in 2002, *Journal of Geophysical Research: Atmospheres*, 108,  
608 <https://doi.org/10.1029/2003JD003863>, 2003.
- 609 Ellis, A. M., and Mayhew, C. A.: Chemical Ionization: Chemistry, Thermodynamics and Kinetics, in:  
610 *Proton Transfer Reaction Mass Spectrometry*, 25-48, 2014.
- 611 Gueneron, M., Erickson, M. H., VanderSchelden, G. S., and Jobson, B. T.: PTR-MS fragmentation  
612 patterns of gasoline hydrocarbons, *International Journal of Mass Spectrometry*, 379, 97-109,  
613 <https://doi.org/10.1016/j.ijms.2015.01.001>, 2015.
- 614 Hansel, A., Jordan, A., Holzinger, R., Prazeller, P., Vogel, W., and Lindinger, W.: Proton transfer reaction  
615 mass spectrometry: on-line trace gas analysis at the ppb level, *International Journal of Mass Spectrometry  
616 and Ion Processes*, 149-150, 609-619, [https://doi.org/10.1016/0168-1176\(95\)04294-U](https://doi.org/10.1016/0168-1176(95)04294-U), 1995.
- 617 Hartungen, E. v., Wisthaler, A., Mikoviny, T., Jaksch, D., Boscaini, E., Dunphy, P. J., and Märk, T. D.:  
618 Proton-transfer-reaction mass spectrometry (PTR-MS) of carboxylic acids: Determination of Henry's law  
619 constants and axillary odour investigations, *International Journal of Mass Spectrometry*, 239, 243-248,  
620 <https://doi.org/10.1016/j.ijms.2004.09.009>, 2004.
- 621 Inomata, S., Tanimoto, H., Kameyama, S., Tsunogai, U., Irie, H., Kanaya, Y., and Wang, Z.: Technical  
622 Note: Determination of formaldehyde mixing ratios in air with PTR-MS: laboratory experiments and  
623 field measurements, *Atmospheric Chemistry and Physics*, 8, 273-284, [https://doi.org/10.5194/acp-8-273-  
624 2008](https://doi.org/10.5194/acp-8-273-2008), 2008.
- 625 Jensen, A., Liu, Z., Tan, W., Dix, B., Chen, T., Koss, A., Zhu, L., Li, L., and de Gouw, J.: Measurements  
626 of Volatile Organic Compounds During the COVID-19 Lockdown in Changzhou, China, *Geophysical  
627 Research Letters*, 48, e2021GL095560, <https://doi.org/10.1029/2021GL095560>, 2021.
- 628 Kari, E., Miettinen, P., Yli-Pirilä, P., Virtanen, A., and Faiola, C. L.: PTR-ToF-MS product ion  
629 distributions and humidity-dependence of biogenic volatile organic compounds, *International Journal of  
630 Mass Spectrometry*, 430, 87-97, <https://doi.org/10.1016/j.ijms.2018.05.003>, 2018.
- 631 Krechmer, J., Lopez-Hilfiker, F., Koss, A., Hutterli, M., Stoermer, C., Deming, B., Kimmel, J., Warneke,  
632 C., Holzinger, R., Jayne, J., Worsnop, D., Fuhrer, K., Gonin, M., and de Gouw, J.: Evaluation of a New  
633 Reagent-Ion Source and Focusing Ion-Molecule Reactor for Use in Proton-Transfer-Reaction Mass  
634 Spectrometry, *Anal Chem*, 90, 12011-12018, <https://doi.org/10.1021/acs.analchem.8b02641>, 2018.
- 635 Li, H., Almeida, T. G., Luo, Y., Zhao, J., Palm, B. B., Daub, C. D., Huang, W., Mohr, C., Krechmer, J.  
636 E., Kurtén, T., and Ehn, M.: Fragmentation inside proton-transfer-reaction-based mass spectrometers  
637 limits the detection of ROOR and ROOH peroxides, *Atmos. Meas. Tech.*, 15, 1811-1827,  
638 <https://doi.org/10.5194/amt-15-1811-2022>, 2022.
- 639 Lindinger, W., Hansel, A., and Jordan, A.: On-line monitoring of volatile organic compounds at pptv  
640 levels by means of proton-transfer-reaction mass spectrometry (PTR-MS) medical applications, food  
641 control and environmental research, *International Journal of Mass Spectrometry and Ion Processes*, 173,  
642 191-241, [https://doi.org/10.1016/S0168-1176\(97\)00281-4](https://doi.org/10.1016/S0168-1176(97)00281-4), 1998.
- 643 Materić, D., Lanza, M., Sulzer, P., Herbig, J., Bruhn, D., Gauci, V., Mason, N., and Turner, C.: Selective

644 reagent ion-time of flight-mass spectrometry study of six common monoterpenes, *International Journal*  
645 *of Mass Spectrometry*, 421, 40-50, <https://doi.org/10.1016/j.ijms.2017.06.003>, 2017.

646 Michoud, V., Sauvage, S., Léonardis, T., Fronval, I., Kukui, A., Locoge, N., and Dusanter, S.: Field  
647 measurements of methylglyoxal using proton transfer reaction time-of-flight mass spectrometry and  
648 comparison to the DNPH-HPLC-UV method, *Atmospheric Measurement Techniques*, 11, 5729-5740,  
649 <https://doi.org/10.5194/amt-11-5729-2018>, 2018.

650 Pagonis, D., Sekimoto, K., and de Gouw, J.: A Library of Proton-Transfer Reactions of H<sub>3</sub>O<sup>+</sup> Ions Used  
651 for Trace Gas Detection, *J Am Soc Mass Spectr*, 30, 1330-1335, [https://doi.org/10.1007/s13361-019-](https://doi.org/10.1007/s13361-019-02209-3)  
652 [02209-3](https://doi.org/10.1007/s13361-019-02209-3), 2019.

653 Pleil, J. D., Hansel, A., and Beauchamp, J.: Advances in proton transfer reaction mass spectrometry  
654 (PTR-MS): applications in exhaled breath analysis, food science, and atmospheric chemistry, *J Breath*  
655 *Res*, 13, <https://doi.org/10.1088/1752-7163/ab21a7>, 2019.

656 Salazar Gómez, J. I., Sojka, M., Klucken, C., Schlögl, R., and Ruland, H.: Determination of trace  
657 compounds and artifacts in nitrogen background measurements by proton transfer reaction time-of-flight  
658 mass spectrometry under dry and humid conditions, *J Mass Spectrom*, 56, e4777,  
659 <https://doi.org/10.1002/jms.4777>, 2021.

660 Schripp, T., Etienne, S., Fauck, C., Fuhrmann, F., Märk, L., and Salthammer, T.: Application of proton-  
661 transfer-reaction-mass-spectrometry for Indoor Air Quality research, *Indoor Air*, 24, 178-189,  
662 <https://doi.org/10.1111/ina.12061>, 2014.

663 Sekimoto, K., Li, S.-M., Yuan, B., Koss, A., Coggon, M., Warneke, C., and de Gouw, J.: Calculation of  
664 the sensitivity of proton-transfer-reaction mass spectrometry (PTR-MS) for organic trace gases using  
665 molecular properties, *International Journal of Mass Spectrometry*, 421, 71-94,  
666 <https://doi.org/10.1016/j.ijms.2017.04.006>, 2017.

667 Sekimoto, K., and Koss, A. R.: Modern mass spectrometry in atmospheric sciences: Measurement of  
668 volatile organic compounds in the troposphere using proton-transfer-reaction mass spectrometry, *J Mass*  
669 *Spectrom*, 56, <https://doi.org/10.1002/jms.4619>, 2021.

670 Shao, P., An, J., Xin, J., Wu, F., Wang, J., Ji, D., and Wang, Y.: Source apportionment of VOCs and the  
671 contribution to photochemical ozone formation during summer in the typical industrial area in the  
672 Yangtze River Delta, China, *Atmospheric Research*, 176-177, 64-74,  
673 <https://doi.org/10.1016/j.atmosres.2016.02.015>, 2016.

674 Shrivastava, M., Cappa, C. D., Fan, J., Goldstein, A. H., Guenther, A. B., Jimenez, J. L., Kuang, C.,  
675 Laskin, A., Martin, S. T., Ng, N. L., Petaja, T., Pierce, J. R., Rasch, P. J., Roldin, P., Seinfeld, J. H.,  
676 Shilling, J., Smith, J. N., Thornton, J. A., Volkamer, R., Wang, J., Worsnop, D. R., Zaveri, R. A., Zelenyuk,  
677 A., and Zhang, Q.: Recent advances in understanding secondary organic aerosol: Implications for global  
678 climate forcing, *Reviews of Geophysics*, 55, 509-559, <https://doi.org/10.1002/2016RG000540>, 2017.

679 Sinha, V., Custer, T. G., Kluepfel, T., and Williams, J.: The effect of relative humidity on the detection of  
680 pyrrole by PTR-MS for OH reactivity measurements, *International Journal of Mass Spectrometry*, 282,  
681 108-111, <https://doi.org/10.1016/j.ijms.2009.02.019>, 2009.

682 Smith, D., Diskin, A., Ji, Y. F., and Späněl, P.: Concurrent use of H<sub>3</sub>O<sup>+</sup>, NO<sup>+</sup>, and O<sub>2</sub>(<sup>+</sup>) precursor ions  
683 for the detection and quantification of diverse trace gases in the presence of air and breath by selected  
684 ion-flow tube mass spectrometry, *INTERNATIONAL JOURNAL OF MASS SPECTROMETRY*, 209,  
685 81-97, [https://doi.org/10.1016/S1387-3806\(01\)00478-X](https://doi.org/10.1016/S1387-3806(01)00478-X), 2001.

686 Španěl, P., and Smith, D.: SIFT studies of the reactions of H<sub>3</sub>O<sup>+</sup>, NO<sup>+</sup> and O<sub>2</sub><sup>+</sup> with a series of volatile  
687 carboxylic acids and esters, *International Journal of Mass Spectrometry and Ion Processes*, 172, 137-147,  
688 [https://doi.org/10.1016/S0168-1176\(97\)00246-2](https://doi.org/10.1016/S0168-1176(97)00246-2), 1998.

689 Španěl, P., and Smith, D.: Selected ion flow tube: a technique for quantitative trace gas analysis of air  
690 and breath, *Medical and Biological Engineering and Computing*, 34, 409-419,  
691 <https://doi.org/10.1007/BF02523843>, 1996.

692 Španěl, P., Ji, Y., and Smith, D.: SIFT studies of the reactions of H<sub>3</sub>O<sup>+</sup>, NO<sup>+</sup> and O<sub>2</sub><sup>+</sup> with a series of  
693 aldehydes and ketones, *International Journal of Mass Spectrometry and Ion Processes*, 165-166, 25-37,  
694 [https://doi.org/10.1016/S0168-1176\(97\)00166-3](https://doi.org/10.1016/S0168-1176(97)00166-3), 1997.

695 Španěl, P., and Smith, D.: Influence of water vapour on selected ion flow tube mass spectrometric  
696 analyses of trace gases in humid air and breath, *Rapid Communications in Mass Spectrometry*, 14, 1898-  
697 1906, [https://doi.org/10.1002/1097-0231\(20001030\)14:20<1898::AID-RCM110>3.0.CO;2-G](https://doi.org/10.1002/1097-0231(20001030)14:20<1898::AID-RCM110>3.0.CO;2-G), 2000.

698 Steinbacher, M., Dommen, J., Ammann, C., Spirig, C., Neftel, A., and Prevot, A. S. H.: Performance  
699 characteristics of a proton-transfer-reaction mass spectrometer (PTR-MS) derived from laboratory and  
700 field measurements, *International Journal of Mass Spectrometry*, 239, 117-128,  
701 <https://doi.org/10.1016/j.ijms.2004.07.015>, 2004.

702 Vlasenko, A., Macdonald, A. M., Sjostedt, S. J., and Abbatt, J. P. D.: Formaldehyde measurements by  
703 Proton transfer reaction - Mass Spectrometry (PTR-MS): correction for humidity effects, *Atmospheric*

704 Measurement Techniques, 3, 1055-1062, <https://doi.org/10.5194/amt-3-1055-2010>, 2010.

705 Wang, Y., Yang, G., Lu, Y., Liu, Y., Chen, J., and Wang, L.: Detection of gaseous dimethylamine using  
706 vocus proton-transfer-reaction time-of-flight mass spectrometry, Atmospheric Environment, 243, 117875,  
707 <https://doi.org/10.1016/j.atmosenv.2020.117875>, 2020.

708 Warneke, C., van der Veen, C., Luxembourg, S., de Gouw, J. A., and Kok, A.: Measurements of benzene  
709 and toluene in ambient air using proton-transfer-reaction mass spectrometry: calibration, humidity  
710 dependence, and field intercomparison, International Journal of Mass Spectrometry, 207, 167-182,  
711 [https://doi.org/10.1016/S1387-3806\(01\)00366-9](https://doi.org/10.1016/S1387-3806(01)00366-9), 2001.

712 Warneke, C., De Gouw, J. A., Kuster, W. C., Goldan, P. D., and Fall, R.: Validation of atmospheric VOC  
713 measurements by proton-transfer-reaction mass spectrometry using a gas-chromatographic preseparation  
714 method, Environ Sci Technol, 37, 2494-2501, <https://doi.org/10.1021/es026266i>, 2003.

715 Warneke, C., Veres, P., Holloway, J. S., Stutz, J., Tsai, C., Alvarez, S., Rappenglueck, B., Fehsenfeld, F.  
716 C., Graus, M., Gilman, J. B., and de Gouw, J. A.: Airborne formaldehyde measurements using PTR-MS:  
717 calibration, humidity dependence, inter-comparison and initial results, Atmos. Meas. Tech., 4, 2345-2358,  
718 <https://doi.org/10.5194/amt-4-2345-2011>, 2011.

719 Yuan, B., Koss, A. R., Warneke, C., Coggon, M., Sekimoto, K., and de Gouw, J. A.: Proton-Transfer-  
720 Reaction Mass Spectrometry: Applications in Atmospheric Sciences, Chemical Reviews, 117, 13187-  
721 13229, <https://doi.org/10.1021/acs.chemrev.7b00325>, 2017.

722 Zhao, J., and Zhang, R.: Proton transfer reaction rate constants between hydronium ion (H<sub>3</sub>O<sup>+</sup>) and  
723 volatile organic compounds, Atmospheric Environment, 38, 2177-2185,  
724 <https://doi.org/10.1016/j.atmosenv.2004.01.019>, 2004.

725