

# Unlocking the Potential of Melting Calorimetry: A Field Protocol for Liquid Water Content Measurement in Snow

Riccardo Barella<sup>1,\*</sup>, Mathias Bavay<sup>2</sup>, Francesca Carletti<sup>2</sup>, Nicola Ciapponi<sup>1</sup>, Valentina Premier<sup>1</sup>, and Carlo Marin<sup>1,\*</sup>

<sup>1</sup>Institute for Earth Observation, Eurac Research, Viale Druso, 1 - 39100 Bolzano, Italy

<sup>2</sup>WSL Institute for Snow and Avalanche Research SLF, Davos, 7260, Switzerland

\*These authors contributed equally to this work.

**Correspondence:** carlo.marin@eurac.edu

## Abstract.

Melting calorimetry, a classic experiment often conducted in high school chemistry laboratories, holds significant untapped potential for scientific applications beyond its educational context. Traditionally, this technique has been applied to measure the liquid water content in snow using two different formulations: melting calorimetry and freezing calorimetry. In contrast to freezing calorimetry, which is considered as the reference method for measuring liquid water content, melting calorimetry has been perceived as prone to generate significant inaccuracies. This research revisits the formulations for both melting and freezing calorimeters to assess volumetric liquid water content in snow. By incorporating the calorimetric constant, we account for heat exchange with the calorimeter, a critical factor often neglected in melting calorimetry experiments. This paper identifies the most effective and least uncertain method for determining this constant. A central contribution of this work is the introduction of a framework for estimating uncertainty in volumetric liquid water content measurements, adhering to established guidelines for uncertainty expression. This novel framework allows us to revisit past mathematical analyses and demonstrate that melting calorimetry delivers reliable measurements with an uncertainty 0.25% greater than freezing calorimetry. Notably, despite this slightly higher uncertainty, melting calorimetry offers significant practical advantages for field applications. Moreover, we show how the proposed uncertainty framework can be expanded beyond instrumental uncertainty and take into account also the variability from environmental factors and operators, providing a more comprehensive characterization of the uncertainty. By exploiting the proposed uncertainty framework, we finally conduct an in-depth analysis for the optimal tuning of the experimental parameters. This analysis culminates in a robust field protocol for melting calorimetry that transcends common-sense procedural guidelines. Strict adherence to this protocol will maximize measurement accuracy. Applied in field tests in Italy and Switzerland, the melting calorimetry demonstrated to accurately tracking the wet front penetration in the snowpacks, producing results comparable to independent dielectric measurements. These findings highlight the accuracy and the practical advantages of melting calorimetry as a reliable field tool for quantifying snowpack liquid water content. Melting calorimetry can potentially serve as a valuable tool for independent calibration and validation of proximal and remote sensing techniques used for liquid water content retrieval.

**Table 1.** List of Symbols

SYMBOL	Definition
$\theta_w$	Volume fraction of liquid water for a given test sample of snow
$\theta_w^M$	$\theta_w$ obtained with melting calorimeter
$\theta_w^F$	$\theta_w$ obtained with freezing calorimeter
$V_s$	Volume of the snow sample
$M_s$	Mass of the snow sample
$M_i$	Mass of the ice in the snow sample
$M_{LWC}$	Mass of the liquid water inside the sample, it can be expressed as: $M_{LWC} = \theta_w M_s \frac{\rho_w}{\rho_s}$
$M_w, M_o$	Mass of the melting and of the freezing agent, respectively
$M_{cal}$	Calorimeter internal vessel mass
$R$	Ratio between $M_w$ and $M_s$
$E, E^F$	Calorimetric constant expressed in equivalent water mass for the melting and freezing calorimeter, respectively
$T_w, T_o$	Hot water and freezing agent initial temperature
$T_f$	Final temperature of the system at the end of the experiment
$T_{mi}$	Temperature of the ice cube after it is melted, and it is equal to 273.15 K
$T_{cv}$	Temperature of the cold water employed for indirect calorimetric constant estimation
$T_s$	Temperature of the snow sample, that is 273.15 K if no ionic impurities are involved
$C$	Water specific heat i.e., $4.2 \times 10^3 \text{ J kg}^{-1}\text{K}^{-1}$
$C_i$	Ice heat capacity i.e., $2.09 \times 10^3 \text{ J kg}^{-1}\text{K}^{-1}$
$C_o$	Freezing agent specific heat. In the case of using silicone oil, $C_o$ is $1.83 \times 10^3 \text{ J kg}^{-1}\text{K}^{-1}$ at $-10^\circ\text{C}$ .
$C_{cal}$	Calorimeter internal wall specific heat
$L$	Latent heat of ice fusion i.e., $3.34 \times 10^5 \text{ J kg}^{-1}$
$\rho_w$	Water density i.e., $1000 \text{ kg m}^{-3}$
$\sigma_{\theta_w}$	Uncertainty associated to the liquid water content measurement
$\sigma_{M_w}, \sigma_{M_o}$	Uncertainty associated to the mass of melting and freezing agent, respectively
$\sigma_{M_s}$	Uncertainty associated to the mass of the snow sample
$\sigma_{T_w}, \sigma_{T_o}$	Uncertainty associated to the measure of the melting and freezing agent, respectively
$\sigma_{T_f}$	Uncertainty associated to the final temperature of the system
$\sigma_{V_s}$	Uncertainty associated to the volume of the snow sample
$\sigma_E$	Uncertainty associated to the calorimetric constant

## 1 Introduction

25 The presence of liquid water has a profound impact on the physical characteristics of snow, including heat advection through preferential flow, thermal conductivity, density, and mechanical properties, consequently influencing its hydrological and stability responses (Techel and Pielmeier, 2011; Avanzi et al., 2017; Wever et al., 2016; Moure et al., 2023; Valence et al., 2022; Donahue et al., 2022; Schlumpf et al., 2024; Leroux et al., 2020). Therefore, the precise measurement of liquid water content (LWC) within the snowpack assumes critical importance as it provides invaluable information to properly describe the current  
30 conditions of the snowpack and predict its evolution (Hirashima et al., 2019; Wever et al., 2014). Moreover, a proper characterization of liquid water content in the snowpack is essential to characterize the backscattering of radar signal e.g., (Gagliano et al., 2023; Marin et al., 2020).

Calorimetry is the scientific technique used to measure the heat energy transferred during a physical or chemical process, such as a reaction or a state change. This is achieved by utilizing a calorimeter, a specialized device designed to accurately  
35 measure the heat exchanged between a system and its surroundings. It has emerged as a promising technique for LWC determination within the snowpack, e.g., (Yosida, 1960; Jones et al., 1983; Kawashima et al., 1998; Jones, 1979; Boyne and Fisk, 1987; Kinar and Pomeroy, 2015). To measure the LWC in snowpacks, calorimetry offers two distinct approaches based on the process involved: melting and freezing calorimetry. In a melting calorimeter, a snow sample is immersed in hot water. This results in the transition of the solid portion of the sample to a liquid phase, and the heating of the melted ice portion and LWC  
40 to the equilibrium temperature. The measurement of the energy required for this transition is directly related to the amount of ice present in the snow sample. Consequently, LWC can be derived as the difference between the mass (or the volume) of the sample and the ice content. This is why melting calorimetry is considered an indirect measurement (Colbeck, 1978). On the contrary, a freezing calorimeter involves immersing a snow sample in a freezing agent such as cooled silicon oil that induces the transition of any liquid water in the sample to a solid phase, and the cooling of the ice fraction and of the freezed LWC to the  
45 equilibrium temperature. The measurement of the energy required for this transition is directly related to the amount of LWC present in the snow sample. Freezing calorimeter is generally accepted as a reference standard for measurements (Colbeck, 1978) and it was used in the past to calibrate and validate non-destructive methods for LWC measurements (e.g., Denoth et al. (1984); Stein et al. (1997); Kendra et al. (1994)).

The selection of the most suitable approach for implementing calorimetry demands consideration of both field usage and the  
50 accuracy of the obtained results. Firstly, it becomes evident that the practical handling of these methods significantly varies. Specifically, the usage of freezing calorimeter presents several challenges. This calorimeter requires the use of a freezing agent such as silicone oils or toluene, which possess characteristics that make them less desirable for use. For instance, these agents may be toxic and pose difficulties in terms of proper disposal and cleaning of the instruments after their employment. Due to the variability of the employed freezing agents, its specific heat has to be retrieved through a dedicated analysis every time a new  
55 agent is used. Furthermore, operating a freezing calorimeter poses challenges associated with maintaining the freezing agent within a temperature range of  $-50$  to  $-20^{\circ}\text{C}$ . Additionally, active monitoring of temperature changes is required throughout the experiment, lasting at least 15 minutes (Jones et al., 1983), to ensure complete freezing of LWC and the system reaching

thermal equilibrium. During this period, thermal losses can be substantial, introducing significant uncertainties. In contrast, melting calorimetry offers the advantage of using water as melting agent, which can be maintained warm using a portable stove. This also eliminates concerns about conserving the melting agent for multiple measurements in the field. Furthermore, melting calorimetry ensures rapid thermal equilibrium, minimizing heat losses through the calorimeter. These factors contribute to a more efficient experimental process compared to freezing calorimetry.


Regardless of being the established benchmark for measuring LWC, the freezing calorimeter limitations have stimulated the development of alternative methods. These include, among the most established and used, the alcohol calorimeter, which utilizes methanol (Fisk, 1986) and the dilution technique, which employs a 0.01 N hydrochloric acid stock solution (Davis et al., 1985). Laboratory comparisons have demonstrated that these two methods yield equivalent results to the freezing calorimeter and the denothmeter (Boyne and Fisk, 1987), a portable instrument calibrated with freezing calorimetry measurements that measures LWC in snow using its dielectric properties (Denoth and Foglar, 1986). The advantage of the dilution technique lies mainly in its speed compared to the freezing calorimeter. This allowed the gathering of extensive data for calibrating and validating various dielectric models (Perla and Banner, 1988; Perla, 1991), revealing limitations in these models, also in the one used by the denothmeter. Indeed, the variability of snowpack internal compositions, influenced by the specific conditions, can limit the applicability of dielectric models to all cases (Colbeck, 1980; Camp, 1992; Picard et al., 2022). Therefore, a crucial step towards a more accurate dielectric model is collecting a large amount of field measurements. In this sense, melting calorimetry offers several advantages, not only over freezing calorimetry but also over alcohol and dilution methods: i) it eliminates the need to prepare a specific stock solution; ii) it has less stringent temperature requirements for the solution (it does not need to be precisely at 0°C); and iii) it allows for easier mixing. Interestingly, despite these advantages, melting calorimeters have not been widely adopted in the past.

The fact that the melting calorimeter was avoided is likely due to the perception of large errors associated with it (Colbeck, 1978; Fisk, 1986; Boyne and Fisk, 1987; Denoth and Foglar, 1986). In particular, the study conducted by Colbeck (1978), where several measuring techniques including the freezing and melting calorimeter were compared within a theoretical framework of uncertainty propagation, identifies the melting calorimeter as “inherently inaccurate”. The primary objective of Colbeck (1978) was to determine the measuring methodology that would result in lower uncertainty when deriving the water saturation and porosity. The analysis revealed that the uncertainty is propagating in a larger quantity when starting from a measurement of ice volume, i.e., utilizing the melting calorimeter compared to starting from a measurement of water volume, i.e., employing the freezing calorimeter. Based on this analysis, assuming that the relative uncertainty in measuring the ice volume is similar or greater than that in measuring the water volume, the freezing calorimeter was deemed preferable over the melting calorimeter. However, the study provided only an intuitive explanation to support this assumption without actually calculating the relative uncertainties of ice and water, suggesting that freezing a smaller amount of water leads to a reduced error compared to melting a larger amount of ice. Nonetheless, this overlooks the practical challenges associated with freezing a small amount of water within a snow sample under real-world conditions, as discussed previously. Despite Kawashima et al. (1998) attempt to address Colbeck (1978) criticisms of melting calorimetry, their work suffers from limitations. Firstly, they do not account for heat exchange with the calorimeter. This issue has been recognized since the early applications of melting calorimeter (Halliday, 1950)

and has been recently re-emphasized by Fasani et al. (2023). Secondly, their mathematical uncertainty propagation probably relies on simplified assumptions. These shortcomings likely compromise the accuracy of LWC measurements obtained using melting calorimeter. Furthermore, these limitations have already propagated into subsequent studies like (Fasani et al., 2023; Webb et al., 2021; Mavrovic et al., 2020), potentially invalidating their findings. Therefore, while the field applicability of the melting calorimetry is attractive, a critical reevaluation of this technique is necessary.

Our paper addresses and rectifies the limitations of the state of the art for calorimetric analysis for liquid water measurement by proposing a sound mathematical formulation. In this sense, this paper prioritizes unlocking the full potential of the melting calorimeter for LWC measurement, rather than providing a comprehensive review of all existing measurement methods. Moreover, while certain concepts may resemble those in previous works in broad terms, our formulation and its application differ significantly, constituting the primary novelty of our paper. In detail, the novelties lie in the following points

- We present the formulations for both melting and freezing calorimeters, it is expressed in %vol and incorporating the calorimetric constant.
- We clarify the most effective method for estimating the calorimetric constant ( $E$ ).
- We introduce the formulations for estimating the uncertainty of the volumetric LWC measurement for both melting and freezing calorimetry. We tested the influence of the environment and operator on measurement uncertainty and found, through statistical analysis, that they falls within the range of instrumental uncertainty.
- We provide a sensitivity analysis that allows an operator to become more aware of the impact of each measured variable when taking measurements.
- While Colbeck (1978) argued that melting calorimetry is “inherently inaccurate”, a view echoed in later studies, we revisit and refine this analysis. This mathematical refinement, occurring 45 years after Colbeck’s original paper, fundamentally alters the prevailing understanding that the melting calorimeter, an indirect measurement of liquid water content, is not inherently inaccurate, a significant breakthrough that we believe researchers in the field will appreciate.
- We have devised a field protocol that effectively minimizes the uncertainties. The protocol includes specific instructions on the amount of hot water to be used, its temperature, the masses involved, and other crucial details for controlling the uncertainty during the experiment replication.
- The proposed protocol was applied in two different test sites in Italy and Switzerland by two different research groups with different calorimeters to profile LWC. The results, compared to stratigraphic and Denothmeter sampling, show the effectiveness of the proposed melting calorimetry protocol.
- We have made available all the codes necessary for calculating LWC and its associated uncertainty based on the measured variables.

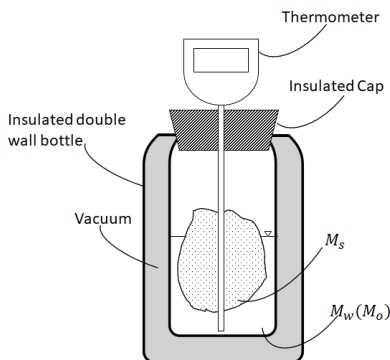

**Figure 1.** The figure illustrates a cross-section of the calorimeter, depicting a schematic representation of its components.

## 2 Formulation of Melting and Freezing Calorimetry

The calorimeter experiment is formulated as an energy budget problem. Each term in the energy budget associated with a  
 125 change in temperature depends on the mass involved, their specific heat, and the temperature difference. Conversely, terms  
 related to phase transitions are determined by the mass involved and the latent heat. Before dealing with the computation of  
 the energy balance, some practical considerations on the setup and measurement operations will be provided.

The setup for calorimetry used to measure LWC in snow involves three essential instruments: i) a specialized instrument  
 known as a calorimeter (see Fig. 1), ii) a scale, and iii) a thermometer. The calorimeter is designed as an insulated container to  
 130 maintain a given temperature and create an insulated environment from the outside, ensuring ideal heat exchange between the  
 snow sample and the melting or freezing agent. The thermometer is generally already part of the calorimeter. It is inserted into  
 the insulated cap of the calorimeter, with particular attention to not introducing any points for heat exchanges, and it is used  
 to monitor temperature changes during the experiment. Prior to the wide availability of modern materials and construction  
 techniques, Yosida conducted extensive research on optimizing calorimeter design (Yosida, 1960). Today, calorimeters can  
 135 be as simple as a commercially available insulated bottle, which provide superior thermal insulation than the Yosida design.  
 The vacuum between the vessels significantly reduces heat transfer by both conduction and convection. Additionally, silvered  
 internal walls minimize heat loss through thermal radiation. These advancements extend the time during which the calorimeter  
 can work as a perfectly insulated environment, eliminating the need for the double-container design (one for hot water and one  
 for snow) and the stirrer introduced by Yosida (1967).

140 From a practical point of view, the calorimetric experiment starts with the placement of a precise mass of either melting agent  
 ( $M_w$ ) or freezing agent ( $M_o$ ) into the insulated container. The most commonly used melting agent is hot water, while the most  
 used freezing agent is silicone oil. The initial temperature of the melting agent ( $T_w \gg 0^\circ C$ ) or the freezing agent ( $T_o \ll 0^\circ C$ ) is  
 recorded. Subsequently, a snow sample of mass  $M_s$  and volume  $V_s$  is added to the calorimeter. The resulting mixture is stirred  
 to facilitate rapid mixing and efficient heat transfer. During this process, the temperature of the mixture is monitored until it  
 145 reaches equilibrium ( $T_f$ ), indicating the completion of the heat exchange between the snow sample and the agent. Minimizing

the duration of these steps is essential to maintain the assumption of an adiabatic system. Any potential losses of the calorimeter, which may be large in the freezing calorimeter giving the longer time of operation, must be accounted for in the analysis e.g., monitoring the temperature for long time (Jones et al., 1983). Calorimetric experiments involve heat exchange between the snow sample and the fluid. During the calorimetric experiment, heat exchange occurs not only between the snow sample and the fluid, but also with the internal metallic calorimeter wall. The wall, due to its high thermal conductivity and vacuum insulation, rapidly reaches thermal equilibrium. While thermal radiative heat transfer represents the most significant energy loss for the calorimeter, the impact of radiation can be considered negligible when compared to the timescale of the experiment (around one minute). Therefore in this study, we will focus primarily on heat conduction as the dominant mechanism for heat exchange as done also in Jones et al. (1983). All the mentioned quantities are then used to calculate the heat exchanged during the process, allowing for an estimation of LWC within the snowpack. As we progress with the paper, when we discuss liquid water content, we will be specifically referring to the volumetric liquid water content (Fierz et al., 2009), which is a measure defined as the ratio of the volume of liquid water content to the volume of the snow sample. Regarding the notation,  $\theta_w^M$  refers to the volumetric LWC measured with the melting calorimeter,  $\theta_w^F$  denotes the same quantity measured with the freezing calorimeter, while  $\theta_w$  refers to the general case as reported in Table 1.

From the heat exchange point of view, in the melting calorimeter, the energy introduced by the hot water  $Q_{hot\ water}$  and the calorimeter internal wall  $Q_{calorimeter}$  must balance with the sum of energy terms for the sinks. These include the heat needed for melting the ice content  $Q_{ice\ melt}$  and the heat required to bring the melted ice and the liquid water already present in the snow to the equilibrium temperature,  $Q_{melted\ ice}$  and  $Q_{LWC}$ . In Eq.(1) is shown the energy budget, detailing the different terms of the equations

$$165 \quad \underbrace{Q_{hot\ water}}_{M_w C(T_f - T_w)} + \underbrace{Q_{calorimeter}}_{M_{cal} C_{cal}(T_f - T_w)} + \underbrace{Q_{ice\ melting}}_{LM_i} + \underbrace{Q_{melted\ ice}}_{M_i C(T_f - T_s)} + \underbrace{Q_{LWC}}_{M_{LWC} C(T_f - T_s)} = 0 \quad (1)$$

Where:

- $C$  represents the specific heat of water ( $4.2 \times 10^3 \text{ J kg}^{-1} \text{ K}^{-1}$ );
- $L$  represents the latent heat of fusion of ice ( $3.34 \times 10^5 \text{ J kg}^{-1}$ );
- $T_s$  is the temperature of the snow sample, that is 273.15 K if no ionic impurities are involved;
- 170 -  $M_{cal}$  represents the mass of the internal wall of the calorimeter in contact with the water;
- $C_{cal}$  represents the specific heat of the internal wall of the calorimeter in contact with the water;
- $M_{LWC}$  is the mass of the liquid water in the snow sample and can be expressed as:  

$$M_{LWC} = \theta_w M_s \frac{\rho_w}{\rho_s};$$
- $M_i$  is the mass of the ice fraction of the snow sample and can be expressed as:  
175 
$$M_i = M_s - M_{LWC};$$

In the operative formulation of the melting calorimeter, the heat exchange contribution of the calorimeter internal wall is expressed as an additive term to the water mass, introducing the so-called calorimetric constant  $E$  (Jones et al., 1983; Fasani et al., 2023). Therefore, as an inherent material property of the calorimeter, the computation of  $E$  can be accomplished as follows

$$180 \quad E = \frac{M_{\text{cal}}C_{\text{cal}}}{C} \quad (2)$$

An accurate estimation of  $E$  requires precise information about the calorimeter construction. Ideally, the manufacturer can provide detailed specifications, including the weight of the internal container and the material used in its construction (typically stainless steel). As a last resort, a destructive approach can be employed. This involves carefully dismantling the calorimeter and precisely measuring the weight of the internal container. Several non-destructive methods for estimating  $E$  have been  
185 proposed, such as mixing fluids at different temperatures (e.g., (Jones et al., 1983; Austin, 1990)) or inverting eq. (3) (e.g., (Fasani et al., 2023)), given that wet snow samples are prepared at a given  $\theta_w$ . However, these methods often suffer from significant uncertainty propagation. For instance, applying the method used by Jones et al. (1983); Austin (1990) yields a relative uncertainty on  $E$  of 40%, in a standard calorimetry configuration. Similarly, creating artificial wet snow samples (Fasani et al., 2023) can further increase relative uncertainty to unacceptable levels i.e., 75%, even if we assume that  $\theta_w$  is  
190 known without uncertainty. Therefore, although non-destructive, these methods are associated with significant uncertainties and are thus recommended to be avoided. The complete mathematical derivations for estimating the uncertainty associated with  $E$  using various methods from the literature are provided in Appendix A.

From Eq.(1) and Eq.(2),  $\theta_w^M$  can be derived as follows:

$$\theta_w^M = \frac{M_s}{V_s \rho_w} \left( 1 - \frac{C}{L} \left[ \frac{(M_w + E)(T_w - T_f)}{M_s} - (T_f - T_s) \right] \right) \quad (3)$$

195 This formulation differs from Kawashima et al. (1998) in the inclusion of the parameter  $E$ , its simplification of the involved masses, and its use of density for volumetric conversion (i.e., snow density  $M_s/V_s$ , and water density  $\rho_w$ ).

The freezing calorimeter operates on a similar principle to the melting calorimeter, however in this case the freezing agent and the container extract heat from the ice content and  $\theta_w$  in the snow, causing it to freeze. The corresponding energy balance equation is given by:

$$200 \quad \underbrace{Q_{\text{freezing agent}}}_{M_o C (T_f - T_o)} + \underbrace{Q_{\text{calorimeter}}}_{M_{\text{cal}} C_{\text{cal}} (T_f - T_o)} + \underbrace{Q_{\text{cooling ice}}}_{M_i C_i (T_f - T_s)} + \underbrace{Q_{\text{freezed } \theta_w}}_{-M_{\text{LWC}} L} + \underbrace{Q_{\text{cooling freezed } \theta_w}}_{M_{\text{LWC}} C_i (T_f - T_s)} = 0 \quad (4)$$

Where:

- $C_o$  is the heat capacity of the freezing agent, and  $C_i$  is the heat capacity of ice ( $2.09 \times 10^3 \text{ J kg}^{-1} \text{ K}^{-1}$ ). In the case of using silicone oil,  $C_o$  is  $1.83 \times 10^3 \text{ J kg}^{-1} \text{ K}^{-1}$  at  $-10^\circ \text{C}$ .



- $C_o$  is the heat capacity of the freezing agent. In the case of using silicone oil,  $C_o$  is  $1.83 \times 10^3 \text{ J kg}^{-1}\text{K}^{-1}$  at  $-10^\circ\text{C}$ ;
- 205 -  $C_i$  is the heat capacity of ice ( $2.09 \times 10^3 \text{ J kg}^{-1}\text{K}^{-1}$ );

As for the melting calorimeter, the heat exchange contribution of the calorimeter internal wall is expressed as an additive term, but this time on the freezing agent mass  $M_o$ . The calorimetric constant  $E^F$  in that case can be obtained as:

$$E^F = \frac{M_{\text{cal}}C_{\text{cal}}}{C_o} \quad (5)$$

In the freezing case, the  $\theta_w^F$  is directly related to the temperature difference induced by the freezing of water present in the snow and, as shown in (Jones et al., 1983), it is derived from Eq.(4) and Eq.(5) as follows:

$$\theta_w^F = \frac{M_s}{V_s \rho_w} \left( \frac{(M_o + E^F)C_o(T_f - T_o)}{LM_s} - \frac{C_i(T_s - T_f)}{L} \right) \quad (6)$$

### 3 Propagation of the Uncertainty in Calorimetry

#### 3.1 Instrumental uncertainty propagation: Melting vs Freezing Calorimetry

Instrumental uncertainty, which arises from the limitations and imperfections of the measuring instruments used in the calorimetric experiment, propagates into the final estimation of  $\theta_w$ . In both melting and freezing calorimetry, the uncertainties are associated with temperature measurements and mass determinations. To quantify uncertainty propagation, we employ a statistical method for uncertainty propagation in accordance with the Guide to the Expression of Uncertainty in Measurement (GUM) (IEC et al., 1993). In previous studies, different uncertainty estimators have been used like the sum of the relative uncertainty (Colbeck, 1978), or the sum of the absolute uncertainty (Jones, 1979; Kawashima et al., 1998) to calculate the uncertainty in the percentage of mass liquid water content. This paper breaks new ground by providing the uncertainty of the volume LWC that adheres to the GUM guidelines.

In detail, the uncertainty  $\sigma_{\theta_w^{M,F}}$  can be determined as the square root of the sum of the squared partial derivatives of  $\theta_w^{M,F}$  with respect to the variables with an associated uncertainty, each, multiplied by the squared associated error. By assuming independent variables, the general formulation is reported in Eq. (7) (IEC et al., 1993; Moffat, 1988).

$$\sigma_{\theta_w^{M,F}} = \sqrt{\sum_{m_i} \left( \frac{\partial \theta_w^{M,F}}{\partial m_i} \right)^2 \sigma_{m_i}^2} \quad (7)$$

In Eq. (7),  $m_i$  represents a single measurement affected by uncertainty, and  $\sigma_{m_i}$  is the associated uncertainty. For the melting calorimeter, the required measurements are  $V_s$ ,  $M_w$ ,  $M_s$ ,  $T_w$ ,  $T_f$  and  $E$  (see Eq. (3)) with associated instrumental uncertainties  $\sigma_{M_w}$  and  $\sigma_{M_s}$ , which depends on the accuracy of the scale,  $\sigma_{T_w}$  and  $\sigma_{T_f}$ , which depends on the accuracy of the thermometer,

230  $\sigma_{V_s}$ , which depends on the uncertainties in measuring the volume of the sampler; and finally on  $\sigma_E$ , which depends on the uncertainty of the estimation of  $E$  (see Appendix A).

Equation (7) can be applied to Eq. (3) and expanded as follows

$$\sigma_{\theta_w^M} = \sqrt{\left(\frac{\partial\theta_w^M}{\partial M_w}\right)^2 \sigma_{M_w}^2 + \left(\frac{\partial\theta_w^M}{\partial M_s}\right)^2 \sigma_{M_s}^2 + \left(\frac{\partial\theta_w^M}{\partial T_w}\right)^2 \sigma_{T_w}^2 + \left(\frac{\partial\theta_w^M}{\partial T_f}\right)^2 \sigma_{T_f}^2 + \left(\frac{\partial\theta_w^M}{\partial V_s}\right)^2 \sigma_{V_s}^2 + \left(\frac{\partial\theta_w^M}{\partial E}\right)^2 \sigma_E^2} \quad (8)$$

The partial derivatives in Eq. (8), known as sensitivity coefficients, are calculated as follows (to preserve the explicit dependence on snow density i.e.,  $\rho_s = M_s/V_s$ , we refrain from simplifying terms involving  $M_s$ ):

$$235 \quad \frac{\partial\theta_w^M}{\partial M_w} = -\frac{M_s}{V_s\rho_w} \frac{C}{L} \frac{T_w - T_f}{M_s} \quad (9)$$

$$\frac{\partial\theta_w^M}{\partial T_w} = -\frac{M_s}{V_s\rho_w} \frac{C}{L} \frac{M_w + E}{M_s} \quad (10)$$

$$\frac{\partial\theta_w^M}{\partial T_f} = \frac{M_s}{V_s\rho_w} \frac{C}{L} \left(\frac{M_w + E}{M_s} + 1\right) \quad (11)$$

$$\frac{\partial\theta_w^M}{\partial M_s} = \frac{1}{V_s\rho_w} \left(1 - \frac{C}{L} (T_f - T_s)\right) \quad (12)$$

$$\frac{\partial\theta_w^M}{\partial V_s} = -\frac{M_s}{V_s^2\rho_w} \left(1 - \frac{C}{L} \left(\frac{(M_w + E)(T_w - T_f)}{M_s} - (T_f - T_s)\right)\right) \quad (13)$$

$$240 \quad \frac{\partial\theta_w^M}{\partial E} = -\frac{M_s}{V_s\rho_w} \frac{C}{L} \frac{T_w - T_f}{M_s} \quad (14)$$

It is important to note that although there are significant differences in our calorimetric equations, Kawashima et al. (1998) calculated some of the same derivatives we present. However, they used an approximation to transition from Eq. (1) to Eq. (4) in their original paper, via Eq. (3), that is not clear. This ambiguity results in different values when properly calculating the derivatives.

245 Similarly, for the Freezing Calorimeter, we can analyze the error propagation associated with temperature and weight measurements of Eq. (6). In detail, by applying Eq. (7) we obtain

$$\sigma_{\theta_w^F} = \sqrt{\left(\frac{\partial\theta_w^F}{\partial M_o}\right)^2 \sigma_{M_o}^2 + \left(\frac{\partial\theta_w^F}{\partial M_s}\right)^2 \sigma_{M_s}^2 + \left(\frac{\partial\theta_w^F}{\partial T_o}\right)^2 \sigma_{T_o}^2 + \left(\frac{\partial\theta_w^F}{\partial T_f}\right)^2 \sigma_{T_f}^2 + \left(\frac{\partial\theta_w^F}{\partial V_s}\right)^2 \sigma_{V_s}^2 + \left(\frac{\partial\theta_w^F}{\partial E}\right)^2 \sigma_E^2} \quad (15)$$

The partial derivatives in Eq. (15) are calculated as follows:

$$\frac{\partial \theta_w^F}{\partial M_o} = \frac{M_s}{V_s \rho_w} \frac{C_o(T_f - T_o)}{LM_s} \quad (16)$$

$$250 \quad \frac{\partial \theta_w^F}{\partial T_o} = -\frac{M_s}{V_s \rho_w} \frac{(M_o + E)C_o}{LM_s} \quad (17)$$

$$\frac{\partial \theta_w^F}{\partial T_f} = \frac{M_s}{V_s \rho_w L} \left( \frac{(M_o + E)C_o}{M_s} + C_i \right) \quad (18)$$

$$\frac{\partial \theta_w^F}{\partial M_s} = -\frac{1}{L} \left( \frac{(M_o + E)C_o(T_f - T_o)}{V_s \rho_w M_s} + \frac{1}{V_s \rho_w} \left( \frac{(M_o + E)C_o(T_f - T_o)}{M_s} - C_i(T_s - T_f) \right) \right) \quad (19)$$


$$\frac{\partial \theta_w^F}{\partial V_s} = -\frac{M_s}{V_s^2 \rho_w} \left( \frac{(M_o + E)C_o(T_f - T_o)}{LM_s} - \frac{C_i(T_s - T_f)}{L} \right) \quad (20)$$

$$\frac{\partial \theta_w^F}{\partial E} = \frac{M_s}{V_s \rho_w} \frac{C_o(T_f - T_o)}{LM_s} \quad (21)$$

255 Similar derivatives have been presented in (Jones, 1979) for the propagation of the instrumental uncertainty for the liquid water content expressed in percentage of mass LWC.

By evaluating Eqs. (8) and (15) it is possible to compare the two methods as done in Colbeck (1978). In detail, by assuming  $V_s = 200 \text{ cm}^3$ , a value consistent with the density measurement sampler (Proksch et al., 2016), which ensures compact dimensions for both the snow sampler and the calorimeter, facilitating transportation, and considering a snow density of the  
260 dry snow of  $366 \text{ kg m}^{-3}$  as a legacy of (Colbeck, 1978), to which we add a given percentage of liquid water increasing the density of consequence. We set the temperature and mass of hot water at  $40^\circ\text{C}$  and 2 times  $M_s$ , respectively, in line with the analysis of next Section 3.2 and (Kawashima et al., 1998). Similarly, we set the temperature and mass of the freezing agent at  $-30^\circ\text{C}$  and 1.3 times  $M_s$ , respectively, as per (Jones et al., 1983). The calorimetric constant was assumed to be equal to 6.58g.  $\theta_w$  was varied from 0 to 12%, considering the most common values in melting snowpack. Additionally, we consider a scale  
265 with uncertainty of 0.1 g, a thermometer with uncertainty  $0.2^\circ\text{C}$ , an uncertainty in the estimation of the calorimeter constant  $E$  of 0.1 g. Regarding the uncertainty associated with the sample volume, to the best of our knowledge, no studies have been conducted in that specific direction. However from our practical experience, a value of  $2 \text{ cm}^3$  can be realistic according to the tools we are using.

By substituting these values into Eqs. (8) and (2), we quantified the uncertainty associated to  $\theta_w$ . The results are illustrated  
270 in Fig. 2. The comparison demonstrates the superior performance of the freezing calorimeter, particularly for high  $\theta_w$  values,

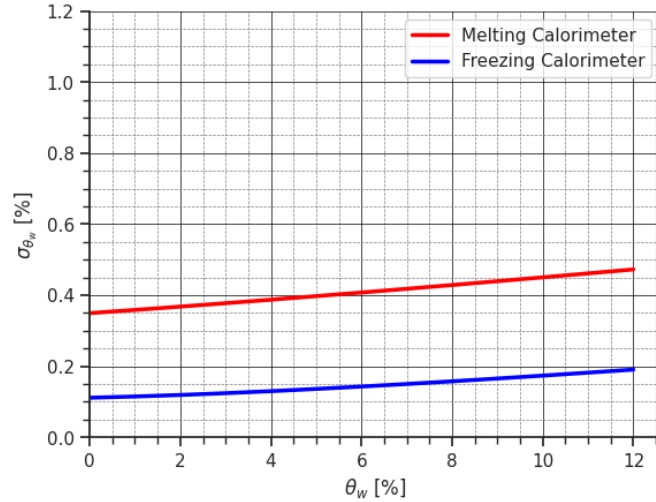


**Figure 2.** The figure provides a comparison of uncertainty in estimating  $\theta_w$  by propagating instrumental uncertainty using both the melting and freezing calorimeter methods.

where the melting calorimetry reaches almost 0.5% uncertainty whereas the freezing calorimetry stops at 0.2% uncertainty, a similar value obtained by Jones et al. (1983); Jones (1979) when converted to the sum of the absolute errors and in percentage of mass (note that the sum of the absolute uncertainties is always larger than the root mean square of the uncertainties). However, the general low value of  $\sigma_{\theta_w^M}$ , indicates that the melting calorimeter can still provide a significant and reliable measurement of  $\theta_w$ . Coupled with its notable practical advantages, the melting calorimeter becomes an attractive and compelling choice for field applications, particularly in remote areas.

It is important to highlight that, the uncertainty analysis presented here produces the same results as the paper of Colbeck (1978): by applying Eq. (8) for water saturation  $S_w$ , we can find that its relative uncertainty  $\Sigma_{S_w}$  is 5.1 times the relative uncertainty of the ice volume  $\Sigma_{V_i}$ , whereas by applying Eq. (15),  $\Sigma_{S_w}$  is 0.84 times the relative uncertainty of the water volume  $\Sigma_{V_w}$ , considering the values used in the original paper of Colbeck (1978). Nevertheless, it is essential to note that the relative uncertainty produced by the melting calorimeter on the estimation of the ice volume  $\Sigma_{V_i}$  is one order of magnitude lower than the relative uncertainty produced by the freezing calorimeter on the water volume  $\Sigma_{V_w}$ , something that was not calculated in the original paper. This renders the final uncertainty of the two methods comparable, as shown in Fig. 2. All the mathematical details are reported in Appendix B and relative codes. Therefore, while Colbeck (1978) argued that melting calorimetry is “inherently inaccurate”, our mathematical refinement, fundamentally alters the prevailing understanding that the melting calorimeter, an indirect measurement of LWC, is not inherently inaccurate.

Finally, Figure 2 shows an opposite trend compared to Figure 3 in Kawashima et al. (1998). In our study, the uncertainty  $\sigma_{\theta_w}$  increases with increasing  $\theta_w$ . This is because we compared snow samples with the same volume and ice content but varied liquid water content, mimicking an introduction of liquid water in the snow filling the voids. Consequently, as the liquid

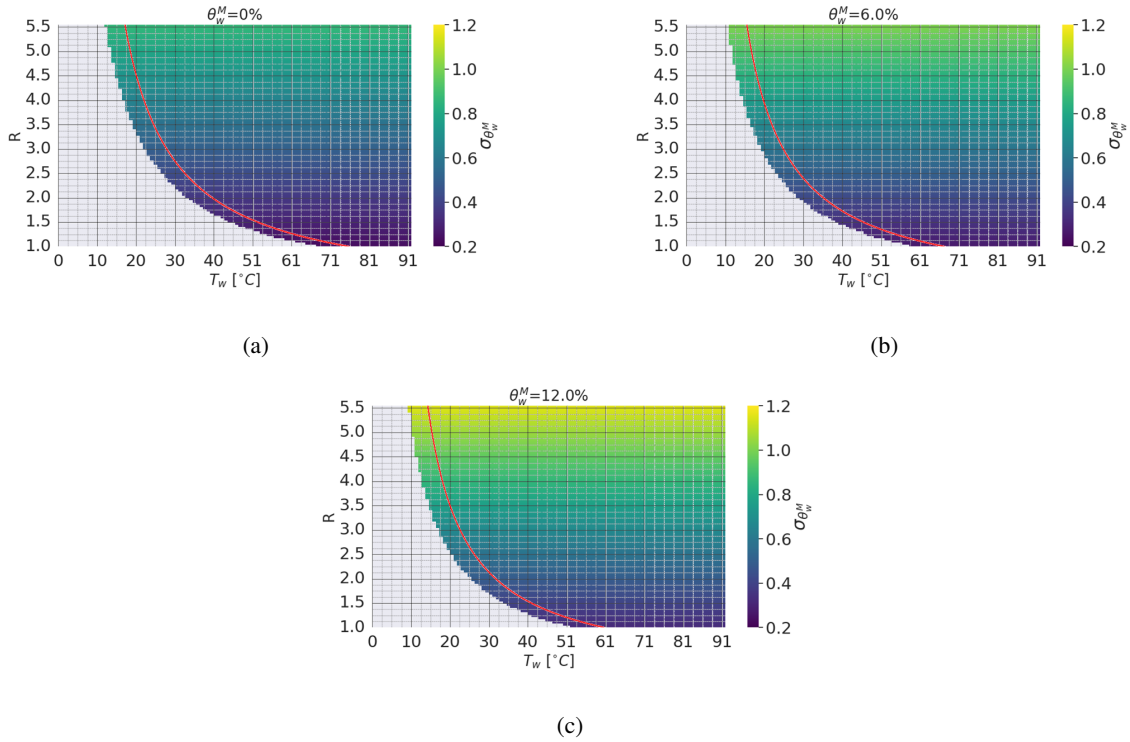

**Figure 3.** In the figure the uncertainty associated to  $\theta_w^M$  is presented as a function of the experiment parameter  $R$  and  $T_w$ . In detail, the uncertainty is presented for 3 representative scenarios of  $\theta_w^M$  i.e., 0%, 6%, and 12%. In (a) the dry snow scenario with  $\theta_w^M = 0\%$  is presented; in (b) the medium wetness scenario with  $\theta_w^M = 6\%$  is presented and in (c) the limit wetness scenario with  $\theta_w^M = 12\%$  is presented. Gray areas represent the cases where the calorimetric experiment results in a final temperature lower than  $0^\circ\text{C}$ . The indicated red boundary signifies a "safety" threshold constrained by a final temperature of  $5^\circ\text{C}$ , i.e. the points laying on the red line result in a  $T_f = 5^\circ\text{C}$ .

290 water content increases, so does the snow density. In contrast, Kawashima et al. (1998) does not account for volume in their  
 formulation, instead adapting the snow mass to the water mass based on the parameter  $R = \frac{M_w}{M_s}$  and maintaining fixed  $T_f$  to  
 10°C. While both approaches are mathematically correct, adjusting the snow density according to the liquid water content and  
 letting  $T_f$  vary according, aligns more closely with the practical reality of measuring LWC in the snowpack.

### 3.2 Minimizing the Instrumental Uncertainty of the Melting Calorimetry


295 Leveraging the framework established in Section 3.1, we can now analyze how the uncertainties in variables measurement  
 propagate to the final water content uncertainty  $\sigma_{\theta_w^M}$  through the melting calorimetry formula (Eq. 3) helping us to identify  
 the optimal operational range for achieving the least uncertain measurements. Given the substantial differences between our  
 approach (volumetric formulation with compensation for the calorimetric constant) and previous methods, a new analysis is  
 necessary with respect (Kawashima et al., 1998). As described in Section 2, some of the variables involved in the calorimetry

300 are free to be selected during the experiment. These are  $V_s$ ,  $M_s$ ,  $M_w$ ,  $T_w$ , and  $E$  (see Eq. (3)). However, all these variables are strictly connected to each other with some implications that it is better to account for.

305 Firstly, by increasing the volume sample  $V_s$ , we expect that the uncertainty is decreasing being  $V_s$  at the denominator for all the terms in Eq. (8). Nonetheless, the volume of the sample is linked to its mass, which increases by increasing the volume, this has an effect of compensation on  $\sigma_{\theta_w^M}$ . This outcome paves the way for dedicated investigations into employing various sample volumes for characterizing liquid water transport within the snowpack. Although such research lies outside the scope of this paper, we provide here some ideas that explain the volume selected in the context of this paper. As discussed in Section 3.1,  $V_s$  is generally constrained by the snow sampler used, which is normally fixed e.g., the Taylor–LaChapelle density cutter. Similarly with the measuring of the density (Proksch et al., 2016),  $V_s$  is selected focusing primarily on the resolution required to describe  $\theta_w$  in the snowpack: a small snow cutter allows to sample the small difference in  $\theta_w$  within the snowpack, whereas a large volume provides a more aggregated bulk information. In practice, by considering a calorimeter with a capacity of 0.5L,  $V_s$  should fall between 100 and 300 cm<sup>3</sup>. For melting snow, this corresponds to a  $M_s$  that ranges approximately between 60 and 150g. Within these values the influence of  $V_s$  on the overall uncertainty  $\sigma_w^M$  is limited. For samples of this volume, it is advisable to prioritize a smaller vertical footprint—such as a cylindrical sampler with a diameter of 4 cm and a depth of 18 cm—over a shallower penetration depth with a larger vertical footprint. This strategy aids in identifying saturated layers and ensures smoother insertion of the snow sample into the calorimeter i.e., the diameter of the sampler is smaller than the opening of the calorimeter.

315 At this point, the remaining variables are  $M_w$ ,  $T_w$ , and  $E$ . It is then mathematically convenient to introduce a new variable  $R = \frac{M_w}{M_s}$  as done in (Kawashima et al., 1998). This allows us to plot the uncertainty as a function of the water temperature and the ratio between the masses for different levels of  $\theta_w$  (see Fig. 3). Considering a  $V_s = 200\text{cm}^3$ , a dry snow density of 366kgm<sup>-3</sup> and a calorimeter with  $E = 6.58$  g, it is possible to show that low values of  $R$  and high water temperature  $T_w$  are the ones that produce the best results in terms of uncertainty. However, high  $T_w$  means a large temperature loss when the calorimeter is open to insert the snow sample. To minimize this loss, which otherwise has to be considered in the calorimetric formulation, a  $T_w$  of 40 to 50 °C together with a quick insertion of the snow sample in the calorimeter, is a good trade-off for all the possible cases, as also indicated by Kawashima et al. (1998). On the other hand it is worth stressing the fact that, even though low values of  $R$  produce the best results, this has two practical implications that should not be neglected: i) if an immersion thermometer is used (as the one represented in Fig. 1) particular attention should be devoted to the fact that the probe is properly immersed inside the water-snow mixture, to avoid measuring errors, and ii) if the snow sample is too big with respect to the water mass, or the water temperature is too low, the heat exchange cannot be completed i.e.,  $T_f < 0^\circ\text{C}$ . As recommendation a value of  $R = 2$  is a good trade-off for all the possible real cases and  $T_f > 5^\circ\text{C}$  should be obtained to consider the measurement as valid (see Fig. 3).

330 Finally it is important to mention that different values of  $E$  imply a change in the uncertainty (see Eq. (9)-(14)). However, we stress the fact that this change is limited and therefore different sizes, shapes and qualities of calorimeter can potentially be employed. Differently, a wrong estimation of the calorimeter constant can have a big impact on the accuracy of the measure of  $\theta_w$  (see next section).

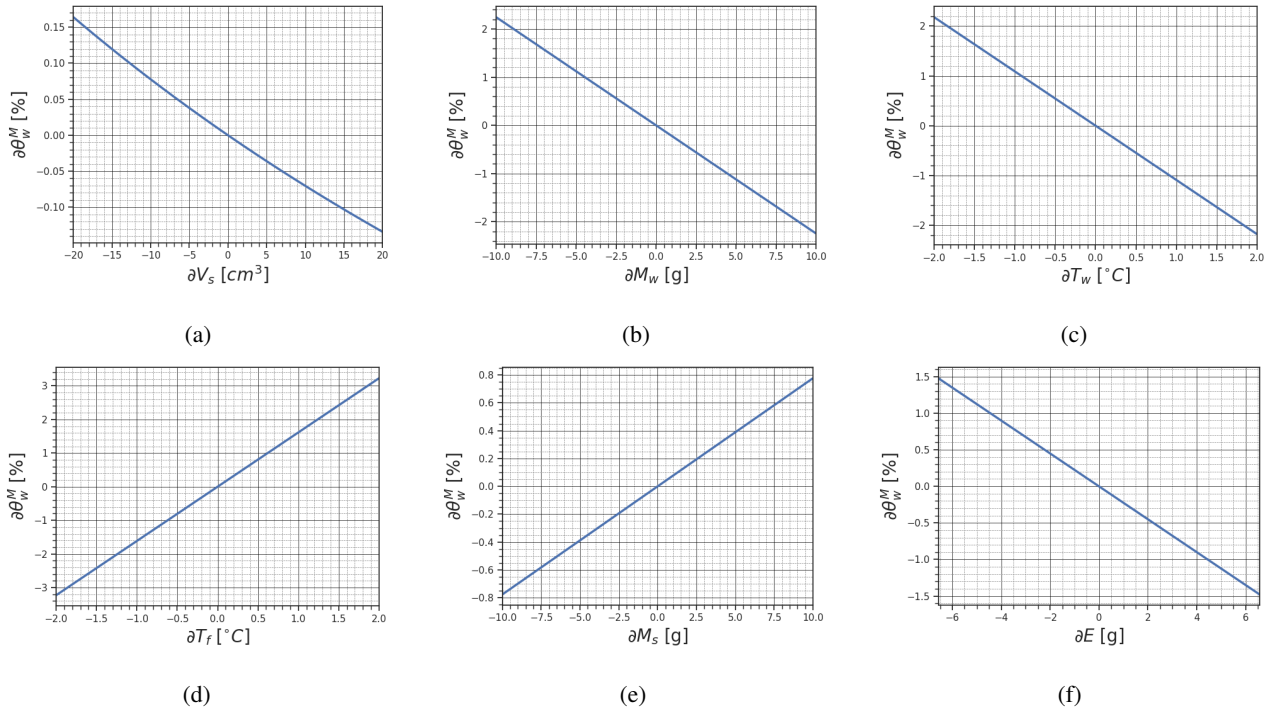

**Figure 4.** In the figure the variation of  $\theta_w^M$  with respect to the six parameters that define the experiment is reported. In detail, we report in (a) the variation of  $\theta_w^M$  with respect to  $V_s$ , in (b) the variation of  $\theta_w^M$  with respect to  $M_w$ , in (c) the variation of  $\theta_w^M$  with respect to  $T_w$ , in (d) the variation of  $\theta_w^M$  with respect to  $T_f$ , in (e) the variation of  $\theta_w^M$  with respect to  $M_s$  and in (e) the variation of  $\theta_w^M$  with respect to  $E$ .

### 335 3.3 Sensitivity Analysis of the Melting Calorimetry

By studying the so-called sensitivity coefficients i.e., Eqs. (9)-(14), we can derive important information about the sensitivity of melting calorimetry to variation of the input variables  $V_s$ ,  $M_s$ ,  $M_w$ ,  $T_w$ , and  $E$  to the final value of  $\theta_w^M$ . In fig.4 the variation in  $\theta_w^M$  associated with the change of the experiment parameters is reported for a realistic case where the snow density is  $416\text{kgm}^{-3}$ ,  $M_s = 83.4\text{g}$ ,  $M_w = 166.8\text{g}$ ,  $T_f = 4.8^{\circ}\text{C}$ ,  $T_w = 40^{\circ}\text{C}$ ,  $E = 6.58\text{g}$  and  $\theta_w^M = 5.0\%$ . Note how  $R$  and  $T_w$  are  
 340 derived from the considerations discussed in Section 3.2. This section, especially Fig.4, is designed to inform operators about the impacts of potential variations of their measurements on  $\theta_w^M$ . Experiments in Section 5 will show how the strict application of the proposed protocol will avoid the introduction of such errors.

Figure 4a illustrates that the error in  $V_s$  is directly proportional to  $\theta_w$ . However, the impact of this error is relatively limited. For instance, in the considered scenario where a snow box cutter with dimensions of  $4 \times 2.75 \times 18\text{cm} = 198\text{cm}^3$  is employed,  
 345 and a portion of  $20\text{cm}^3$  is lost due to incomplete filling i.e., the snow cutter is not filled to a depth of 2cm, the resulting  $\theta_w$  measurement is overestimated by a mere 0.10%. This suggests the feasibility of utilizing snow samplers with variable depth, such as samplers with a moving piston, to adapt the sample size according to  $\theta_w$  distribution in the snowpack.

In Fig. 4b, one can observe how even a small error of a few grams in the measurement of hot water mass can significantly impact the resulting  $\theta_w$ , causing a nearly 1 % difference. For example, a  $1.15^\circ$  tilt of the scale can result in a measurement error of 0.1g. This highlights the crucial significance of ensuring a stable, level, and well-prepared position for the scale, protected by the influence of wind gusts. The plate of the balance should be also sufficiently large compared to the calorimeter.

The accurate measurement of the hot water temperature is equally important (see Fig. 4c). An overestimation of  $1^\circ\text{C}$  in  $T_w$  results in an approximate 1% underestimation of  $\theta_w^M$ . Additionally, it is crucial to emphasize the importance of measuring  $T_w$  only after the entire calorimeter reaches a stable temperature. Using a well-insulated container and promptly inserting the snow sample into the calorimeter, so that the hot water is not cooling down, are vital factors to minimize errors in the measurement of  $T_w$ . The specification regarding the depth of immersion for the thermometer probe must be satisfied e.g., partially immersing the thermometer can lead to a temperature reading that is up to  $1^\circ\text{C}$  lower than the actual temperature.

The misreading of  $T_f$  leads to a directly proportional error in the final  $\theta_w$  measurement (see Fig. 4d). Achieving an accurate measurement of  $T_f$  necessitates ensuring that the heat exchange process is fully completed. To facilitate this, it is recommended to gently shake the calorimeter, and the completion of the process can be verified by observing a clear stabilization in the temperature reading. This is usually occurring within 30 seconds after inserting the snow sample into the calorimeter. Even under harsh conditions, heat loss from the closed calorimeter remains minimal. The negligible temperature loss holds true even when the calorimeter is exposed to sunlight or experiences internal-external temperature differences exceeding  $40^\circ\text{C}$ . These conditions far surpass typical operating environmental conditions.

An error in the mass measurement of the snow sample  $M_s$  introduces a directly proportional error in  $\theta_w^M$  (see Fig. 4e). To ensure accurate measurements, the same precautions as those taken for the measurements of  $M_w$  should be followed.

Finally, it is crucial to note that an error in  $E$  is inversely proportional to  $\theta_w$  (see Fig. 4f). Neglecting the heat exchange with the calorimeter wall, i.e., assuming  $E = 0\text{g}$ , results in significant errors in the final measurement of  $\theta_w^M$ . Therefore, when using a new calorimeter, proper time and effort should be dedicated to accurately estimating  $E$ .

The selection of the values will be summarized in section 4 in form of a protocol that all the researchers and practitioners can follow during field experiments.

#### 4 Melting Calorimeter Protocol

In this section, we will provide a comprehensive summary of the analyses conducted throughout the paper and propose a practical measurement protocol to be followed during field campaigns. First, the necessary materials need to be prepared, including:

**Calorimeter** This could be a commercially available insulated container designed to maintain the temperature of beverages or food. The calorimeter constant must be known or derived for accurate measurements (e.g., with Eq. (2)). In this work we used a commercial insulated container i.e., Stanley Classic Legendary Food Jar made of stainless steel (i.e., SAE 304)  $C_{\text{cal}} = 500 \text{ Jkg}^{-1} \text{ K}^{-1}$  and  $M_{\text{cal}} = 69.1 \text{ g}$ ,  $E = 6.58 \text{ g}$ . The uncertainty of this measurement is only related






(a)



(b)

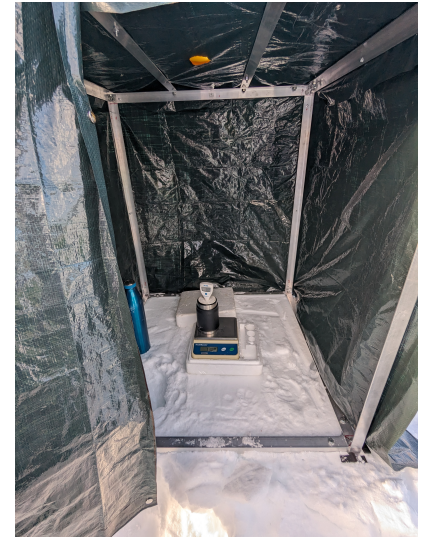

(c)

**Figure 5.** In (a) is reported the essential materials for the melting calorimeter experiment. From left to right: the calorimeter, its thermometer, the thermos storing the hot water used in the experiment, and the scale for measuring mass placed on a stable plexiglass panel. In (b) is reported from left to right, the snow cutter, used for sampling the snowpack at the Weissfluhjoch site and the ~~Denometer~~Denothmether used during the measurement campaign. In (c) it is possible to see the measurement configuration in case it is not possible to dig a snow pit deep enough to protect the calorimeter from wind and solar radiation. However, measurements under extreme weather conditions are not recommended.

380 to the uncertainty of the scale used to weigh the container i.e., 0.1g. These values have been measured, and they are not provided by the producer.

**High-Precision Immersion Thermometer** Used to monitor temperature changes during the experiment (we used a Hanna Instruments HI98501).

385 **Precision Balance** Utilized for measuring the mass of hot water and snow samples. The scale should be at least splash proof (IPX4). We used a RS-PRO 805-6688 and a Kern PCB-10000-1.

**Supportive Surface** A level, hard and supportive surface such as Plexiglass.

**Wind Shield** A well dug shelter or an external barrier, such as a plexiglas container can be used to shield the scale from wind.

**Insulated bottle** The bottle acts as a reservoir of hot water, ensuring a continuous supply for the experiment.

390 **Snow sampler** This can be any of the available snow samplers for density measurements. The shape and size of the sampler must be compatible with the shape and size of the calorimeter.

The snow pit should be dug so that the snow wall is shaded from the sun. Once the snow pit is prepared, a shaded area for the scale should be established (see Fig. 5a), protecting it from solar radiation and wind. If shade is unavailable for the scale, measurements should be avoided. Alternatively, a shading protection system like the one shown in Fig. 5c can be used. Another hole should be dug for storing the snow sampler and auxiliary tools needed for sample preparation to maintain them  
395 at low temperatures. The outer surface of the pit profile should be smoothed, and the bottom should be level to ensure accurate measurement of the snow height at which the  $\theta_w^M$  measurement will be taken.

Following these preparations, the following steps should be followed:

1. Dig a snow pit and verify that  $T_s = 273.15\text{K}$  ( $0^\circ\text{C}$ )
2. Warm up the water at the temperature of  $40$  to  $50^\circ\text{C}$  and store it in the insulated bottle;
- 400 3. Tare the scale with the calorimeter and the lid with the thermometer on top;
4. Prepare the hot water inside the calorimeter in a quantity that meets the minimum immersion requirement of the thermometer and is approximately two times the sample mass (annotate it as  $M_w$ ); If a volume of  $200\text{cm}^3$  is used, approximately  $200\text{g}$  of hot water should be used;
5. Close the calorimeter and wait for the temperature to stabilize;
- 405 6. Record the temperature  $T_w$ . It should be around  $40^\circ\text{C}$ ;
7. Tare the scale with the calorimeter and hot water (otherwise the uncertainty of the two measurements must be propagated through Eq.(7)).
8. Retrieve the snow sampler from the shaded hole and collect a snow sample from the designated height, ensuring no phase changes occur (i.e. take the sample on shade) or any loss;
- 410 9. Open the calorimeter and place the snow sample inside. Minimize the time for this step;
10. Gently shake the calorimeter;
11. Weigh the snow mass  $M_s$  by placing the calorimeter on the tared scale waiting for the temperature to stabilize;
12. Once the temperature stabilizes, approximately 30 seconds - 1 minute after sample insertion, read the temperature  $T_f$ .
- 415 13. Empty and dry the calorimeter ~~for~~ thoroughly before subsequent measurements. While carefully drying the calorimeter is advised, the residual water inside the calorimeter will be included in the mass and temperature measurement of the hot water, whereas the potential water or snow attached on the outside part of the calorimeter has to be clean out (even though their mass is in general negligible).

By following this protocol meticulously, the measurement of  $\theta_w^M$  in the snowpack can be conducted with the accuracy and the uncertainty shown in this paper (see next section on the experimental results). By using the shared code provided with the  
420 paper  $\theta_w^M$  and the relative uncertainty can be derived starting from the measured data.

## 5 Experimental Results: Application of the Melting Calorimeter Protocol

### 5.1 Dry Snow Experiment: the Effectiveness of Melting Calorimetry Protocol and Impact of Heat Loss

In the first experiment, we used dry snow samples and measured the final system temperature. This experiment serves as a proxy for evaluating the effectiveness of melting calorimeter when employed by skilled operators. While using reference samples with a known  $\theta_w$  would be ideal, preparing such samples artificially introduces significant uncertainties. The methods employed by Kawashima et al. (1998) and by Fasani et al. (2023), which introduce liquid water into dry snow, require that both the snow sample, the air, and the added liquid water to be at exactly 0°C. Moreover, the mixing operation should be done gently in order to not alter the effective  $\theta_w$  of the reference sample. Therefore, given the inherent difficulty in achieving such precise control, we avoided this approach. As done for Eq. (1), we can derive the expression for the energy budget in case of dry snow:

$$\underbrace{M_w C(T_f - T_w)}_{Q_{hot\ water}} + \underbrace{M_{cal} C_{cal}(T_f - T_w)}_{Q_{calorimeter}} + \underbrace{M_{dry\_snow} C_{ice}(T_f - T_{dry\_snow})}_{Q_{warming\ snow}} + \underbrace{LM_{dry\_snow}}_{Q_{snow\ melting}} - \underbrace{M_{dry\_snow} C(T_f - T_{mi})}_{Q_{melted\ snow}} = 0 \quad (22)$$

From eq. 22 can be retrieved the final temperature of the system as:

$$T_f = \frac{C_i M_{dry\_snow} T_{dry\_snow} - LM_{dry\_snow} + C(M_w + E)T_w}{C(M_w + E) + M_{dry\_snow}C} \quad (23)$$

The associated instrumental uncertainty can be derived as follows (IEC et al., 1993):

$$\sigma_{T_f}^{Ins} = \sqrt{\left(\frac{\partial T_f}{\partial M_s}\right)^2 \sigma_{M_s}^2 + \left(\frac{\partial T_f}{\partial T_s}\right)^2 \sigma_{T_s}^2 + \left(\frac{\partial T_f}{\partial M_w}\right)^2 \sigma_{M_w}^2 + \left(\frac{\partial T_f}{\partial T_w}\right)^2 \sigma_{T_w}^2 + \left(\frac{\partial T_f}{\partial E}\right)^2 \sigma_E^2} \quad (24)$$

Where  $T_s$  and  $M_s$  are respectively the temperature and the mass of the dry snow sample.

The dry snow experiment revealed a lower overall uncertainty than the inherent instrumental uncertainty (refer to Fig. 6a). The results demonstrate that well-trained operators can significantly minimize uncertainties associated with sample handling and lid opening during calorimetric analysis proving the practical effectiveness of melting calorimetry. Since for this experiment we always obtained an experimental uncertainty lower than the instrumental uncertainty, we made only a total of 5 experiments. We instead focus on the heat lost when the calorimeter is opened for snow sample insertion. We observed a temperature loss of 0.2°C after 10 seconds with a 40°C difference between the air and the water temperature. Since sample insertion itself takes a maximum of 2 seconds by a skilled operator, the heat lost is negligible. This is another evidence that the instrumental uncertainty found in Section 3.1 can be applied in this case. This last finding aligns with the observations from Kawashima et al. (1998) (see Section titled “the effect of the heat loss by opening the lid” of the original paper).

## 5.2 Ice Cube Experiment: Effect of Different Operators Measuring at Different Environmental Temperature


In the second experiment, we investigated the combined effects of performing the calorimetric measurements by different operators under different air temperature. To this end, we recruited a group of volunteers to perform a large number  $N$  of calorimetric experiments i.e.,  $N > 30$  following the proposed protocol. To simulate variations in air temperature we performed  
 450 the measurements in a controlled chamber spanning temperatures from  $-5$  to  $20$  °C. In this experiment we used ice cubes as surrogate for wet snow samples, to avoid the introduction of additional uncertainties as described in the section before. The substantial temperature differential between the ice cubes and the ambient environment enabled us to replicate worst-case scenarios that may arise due to operator inefficiency in adhering to the measurement protocol i.e., slowly moving the ice cube inside the opened calorimeter or/and not waiting for the thermal equilibrium.

455 The experimental setup, resembling the dry snow calorimetric experiment described in the section before, aims to compare the measured final temperature  $T_f^{\text{Exp}}$  of the mixture of hot water after the addition of the ice cube with the theoretical temperature  $T_f$  calculated using the calorimetric formula. Specifically, the experiment involved a predetermined mass  $M_{ice\_cube}$  of ice sample at a known temperature  $T_{ice\_cube}$  and a mass  $M_w$  of water at a known temperature  $T_w$ .  $R$  was kept equals to 10 for all the experiments in order to guarantee the correct immersion of the thermometer and allow the ice cube ( $T_{ice\_cube} \approx -35^\circ\text{C}$ )  
 460 to completely melt. The temperature of the ice cubes was determined by leaving the cubes for at least 24 hours in a refrigerator with monitored temperature. As done in Eq. (1), we can express the experiment as an energy budget by equalizing the energy carried by the hot water ( $Q_{hot\ water}$ ) and the internal wall of the calorimetry, in thermal equilibrium with the hot water ( $Q_{calorimeter}$ ), with the sinks consisting of the ice cube ( $Q_{ice\ melting}$ ) and the water derived by melted ice ( $Q_{melted\ ice}$ ). Starting from the energy balance presented in Eq. (22) the final temperature  $T_f$  can be derived from Eq. (23) by changing the mass  
 465 and temperature of the dry snow with the mass and the temperature of the ice cube.

The outcome of the experiment is presented in Fig. 6b. From a qualitative point of view, the figure demonstrates a good agreement between the measured and theoretical values indicating the effectiveness of the melting calorimetry. The small spread of the data indicates that the experiment is largely reproducible among different operators, even though some operators generate larger errors. The missing of a bias indicates that there are no systematic errors. From a quantitative point of view,  
 470 the experimental uncertainty can be calculated from this data as the Root Mean Square (RMS) of the differences between the measured final temperature  $T_f^{\text{Exp}}$  and the theoretical final temperature  $T_f$  as follows (IEC et al., 1993).

$$\sigma_{T_f}^{\text{Exp}} = \sqrt{\frac{\sum_i^N (T_{f_i} - T_{f_i}^{\text{Exp}})^2}{N}} \quad (25)$$

This results in  $\sigma_{T_f}^{\text{Exp}} = 0.5^\circ\text{C}$ . However, strictly speaking, in our setup the thermometer uncertainty of  $0.1^\circ\text{C}$  and the scale uncertainty of  $0.1\text{g}$  limited our ability to definitively isolate the impact of environmental and operator variability on the measured  
 475  $T_f$ . A z-test for null hypothesis verification (Rouder et al., 2009) applied to Eq. (25) sometimes rejected the null hypothesis i.e., statistically insignificant differences between the estimated and measured temperatures.

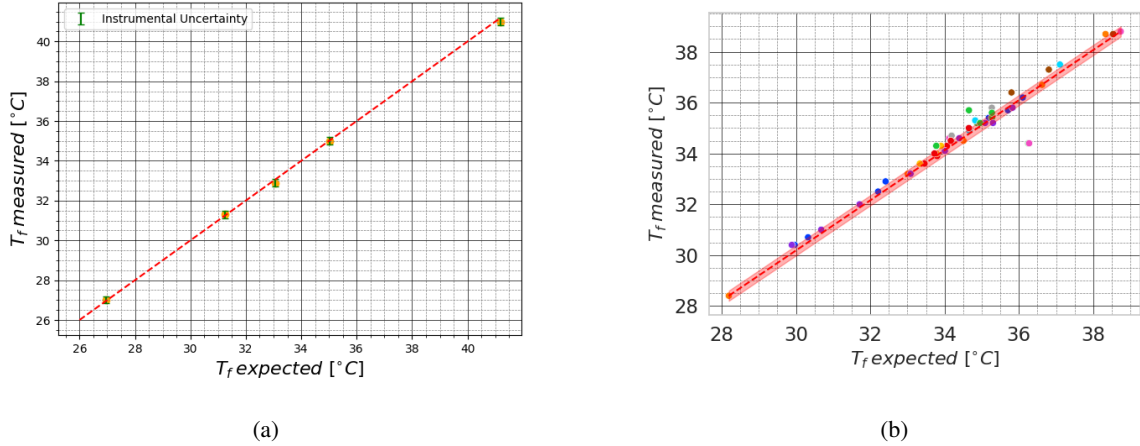

**Figure 6.** Results of the calorimetric experiment performed using (a) dry snow; and (b) ice cubes by a group of volunteers. The measured final temperature (y-axis) is compared with the theoretical final temperature (x-axis) derived from Eq. (23). In (a) the green bars (barely visible due to their low values) represents the instrumental uncertainty of all the measurements using Eq. (24). In (b) the different colors of the dots represent the different people who performed the experiment. The red area represents the instrumental uncertainty of all the measurements using Eq. (26).


Despite the limitations of our current instrumentation, let us explore a hypothetical scenario where  $\sigma_{T_f}^{\text{Exp}} = 0.5^\circ\text{C}$ . This total uncertainty can be further broken down as the sum of the instrumental uncertainty  $\sigma_{T_f}^{\text{Ins}}$ , the operator induced uncertainty  $\sigma_{T_f}^{\text{Ope}}$  and the environment induced uncertainty  $\sigma_{T_f}^{\text{Env}}$ . The instrumental uncertainty  $\sigma_{T_f}^{\text{Ins}}$  can be calculated as follows (IEC et al., 1993):

$$480 \quad \sigma_{T_f}^{\text{Ins}} = \sqrt{\left(\frac{\partial T_f}{\partial M_i}\right)^2 \sigma_{M_i}^2 + \left(\frac{\partial T_f}{\partial T_i}\right)^2 \sigma_{T_i}^2 + \left(\frac{\partial T_f}{\partial M_w}\right)^2 \sigma_{M_w}^2 + \left(\frac{\partial T_f}{\partial T_w}\right)^2 \sigma_{T_w}^2 + \left(\frac{\partial T_f}{\partial E}\right)^2 \sigma_E^2} \quad (26)$$

At this point, the uncertainty associated to the operator variations  $\sigma_{T_f}^{\text{Ope}}$  and the environmental factors  $\sigma_{T_f}^{\text{Env}}$  can be retrieved as a simple difference i.e.,  $\sigma_{T_f}^{\text{Ope}} + \sigma_{T_f}^{\text{Env}} = 0.3^\circ\text{C}$ . Given the fact that the operational steps of this experiment are exactly the same of the operational steps for the melting calorimeter, we can use the derived  $\sigma_{T_f}^{\text{Ope+Env}}$  to update the uncertainty calculated in Section 3.1 by adding this uncertainty to  $\sigma_{T_f}$ . In Fig. 7, we observe how this new characterization of the uncertainty affects  
 485 the uncertainty in the estimation of  $\theta_w$  with respect to only considering the instrumental uncertainty. While the limitations of our current instrumentation prevent definitive conclusions from this analysis (i.e., non-statistically significant results), this exercise demonstrates the value of a quantitative approach to understanding complex uncertainty sources, like the variations due to unskilled operators.

### 5.3 Fan Experiment: the Effect of Harsh Environmental Conditions

490 Field campaigns often expose researchers or practitioners to challenging environmental conditions, encompassing factors such as wind, snowfall, rain, or high solar radiation. Experiments with excessively harsh environmental conditions and/or those

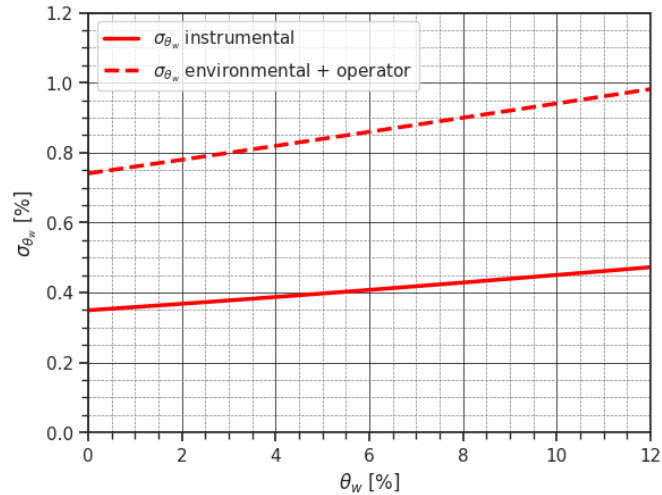


**Figure 7.** Comparison of the propagation of uncertainty considering the instrumental uncertainty (solid red line) and the potential random uncertainty introduced by variations in operators and environmental temperature (dashed red line) for the melting calorimeter derived from the ice cube experiments.

that deviate from established snow pit measurement practices will yield unreliable results and hinder uncertainty estimation, compromising the validity of the measurement. Wind impacting the scale and direct solar radiation exposure of the snow sample are prime examples of such conditions. To quantify the impact of wind on measurement uncertainty, we conducted an experiment where a controlled breeze (around 15 km/h) generated by a fan was directed at the scale. This resulted in a tenfold increase in scale uncertainty, from 0.1g to 1.5g. By applying  $\sigma_{M_w} = 1.5\text{g}$  and  $\sigma_{M_s} = 1.5\text{g}$  to Eq. 8, a significant uncertainty of more than 1% will be associated to the measurement of liquid water content. These results highlight that wind is a major factor that can invalidate calorimetric measurements by introducing excessive uncertainty. Similar to wind, solar radiation and sample handling can significantly impact  $\theta_w$ . Rough handling, and prolonged air and sun exposure can all alter  $\theta_w$  of the snow sample. As will be shown in the next sections, where profiles of LWC are successfully measured in the fields, following basic snow pit practices like shielding the scale from wind and protecting the sample and instruments from direct sunlight can prevent measurement failure and allow us to consider only the instrumental uncertainty as the main source of uncertainty. However, when the environments conditions becomes extreme, the calorimetric measurements should be avoided.

### 5.3.1 Weissfluhjoch: An Intermediate Complexity $\theta_w^M$ Profiles in the Field

The Weissfluhjoch site, located at an altitude of 2536 m a.s.l. in the Davos area of Graubünden, Switzerland, features a flat terrain that is partially sheltered from wind. The site includes a fenced research area and two huts equipped with tools, electricity, heating, and internet, making it ideal for high-level snowpack measurement campaigns (see Fig. 8).

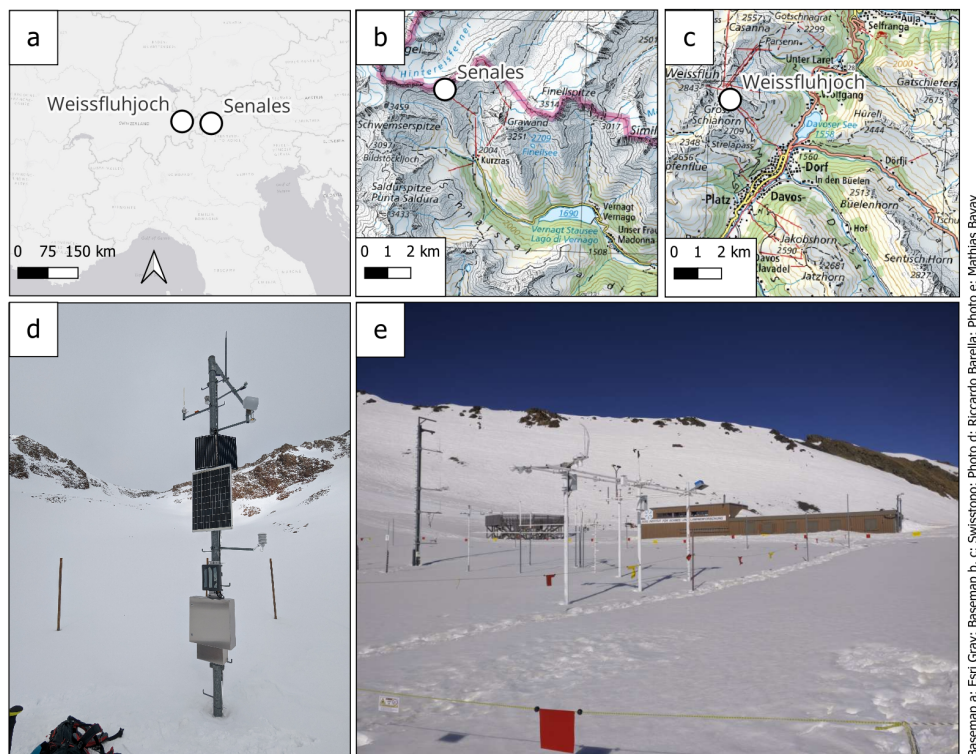


Basemap at: Esri Gray; Basemap b, c: Swisstopo; Photo d: Riccardo Barella; Photo e: Mathias Baya

**Figure 8.** The figure gives an overview of the two sites used for testing the calorimeter. In a) the two sites can be visualized in the Alpine context, while in b) and c) the Weissfluhjoch and Senales sites can be respectively visualized in the local context. In the end in d) is shown a picture of the Senales site and in e) is shown a picture of the Weissfluhjoch site.

On 22 May 2023, measurements began at 08:00 Local Time (LT) under overcast skies, with an air temperature of 7 °C and negligible winds. The snowpack height was 164 cm, characterized by a smooth surface and no new snowfall in the previous 24 hours. Temperature profiles at intervals of 10 cm indicated an isothermal snowpack. Snowpack observations revealed surface melt over a transformed snow layer, with ice lenses identified between H=124 and H=121 cm. Other dry layers were observed until H=98 cm, spaced out by two more ice lenses. Just below the last ice lens the snow seemed dry, but it was observed to become wetter towards the ground. Finally, water runoff was found on the bottom of the snow pit.


Figures 9(a) and (b) show  $\theta_w^M$  obtained from the melting calorimeter and Denoth method, sampled at 5 and 2 cm intervals, respectively. Figure 9(c) depicts snow density measured every 3 cm, and Figure 9(d) showcases a schematic representation of the profile. Both instruments detected surface melt, though the calorimeter indicated higher surface  $\theta_w^M$  values. Ice lenses were characterized by drops in  $\theta_w^M$  and density, blocking the drainage of liquid water. Notably, at 87 cm from the bottom, the highest  $\theta_w^M$  value corresponded with an extremely wet layer confirmed by the calorimeter, while the Denoth did not capture this layer, suggesting localized saturation. Measurements indicated that below H=87 cm, the snowpack was releasing meltwater, with  $\theta_w^M$  values increasing from nearly zero to 2 and 10% near the bottom. Comparisons between the Denoth and

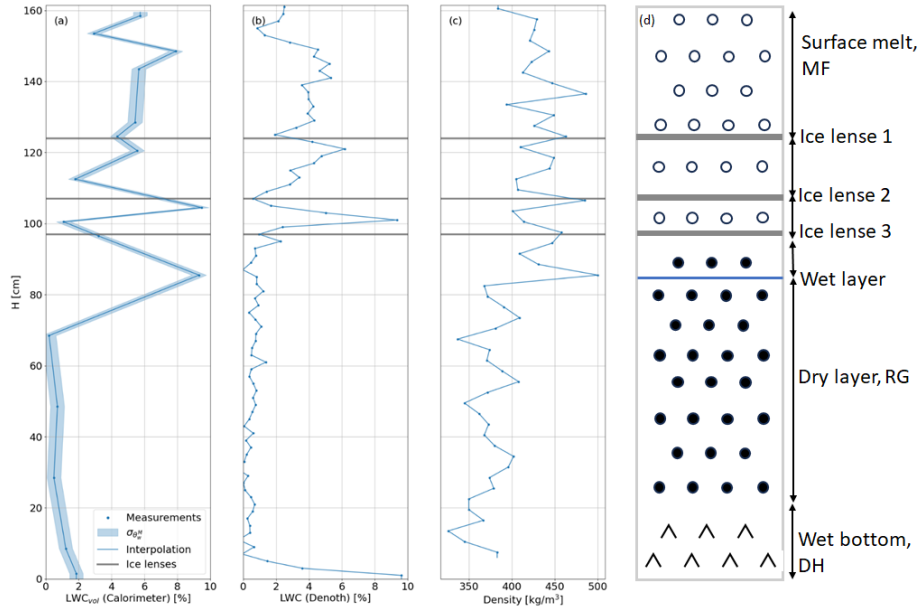

**Figure 9.** Snow profile at Weissfluhjoch on 22 May 2023. Panel (a) shows the volumetric  $\theta_w^M$  profile sampled every 5 cm with the melting calorimeter and its associated uncertainty computed with Eqs. (3) and (8). Panel (b) shows  $\theta_w^M$  profile sampled every 2 cm with the Denoth-meter. Panel (c) shows the snow density sampled every 3 cm with the snowcutter. In panel (d) it is reported a scheme of the profile.

melting calorimetry measurements revealed that the Denoth tended to underestimate  $\theta_w$  in non-saturated layers (Perla, 1991). ~~An analysis following Boyne and Fisk (1987) of~~ Following the procedure outlined in Boyne and Fisk (1987), we analyzed 16 corresponding measurements measurements where both instruments sampled the same LWC conditions for the profile shown in Fig. 9, excluding the measurements at H=87 and H=0 cm. These points were omitted due to the high horizontal variability in LWC, which made it impossible to ensure that we were sampling identical conditions (see Techel and Pielmeier (2011)). The results showed a mean difference of ~~0.96%~~ 0.96% and a standard deviation of ~~1%~~ 1% between the two methods, aligning closely with previous findings for alcohol calorimeters and Denothmeters. While the setup for this experiment did not allow sampling at the exact same location with both techniques, the exclusion of certain data points ensures a clearer and more accurate representation of the tool's performance under comparable conditions. The calorimetric profile vertical consistency and good correlation with density and stratigraphy demonstrate the reliability and stability of melting calorimetry. Lastly, it is interest to note that using the original formulation by Kawashima et al. (1998) may overestimate liquid water content by approximately 3.5% on average compared to the proposed method.



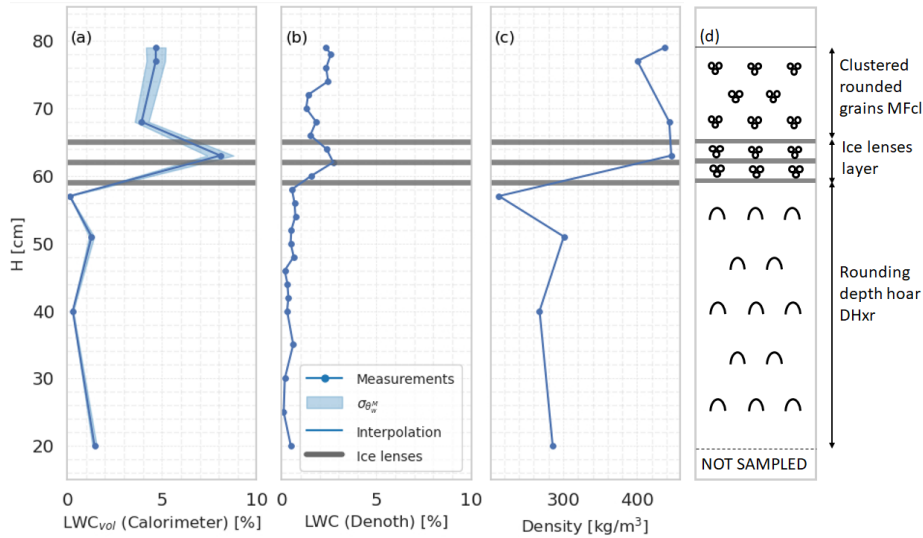

**Figure 10.** Snow profile at Schnalstal on 7 June 2023. Panel (a) displays  $\theta_w^M$  profile generated using the melting calorimeter, including its associated uncertainty calculated through Eq. (3). Panel (b) exhibits the  $\theta_w$  profile sampled with the Denoth. Panel (c) illustrates the snow density associated with the calorimeter measurement points. In panel (d) it is reported a scheme of the profile.

### 5.3.2 Schnalstal: A Typical $\theta_w^M$ Profiles in the European Alps for Late Spring 2023

The Italian test site is located in Schnalstal, in South Tyrol. This site has been chosen because the high altitude ( $\sim 3000\text{m}$ )  
 535 guarantees the presence of abundant snow and a long-lasting melting season, and it is well-served by lifts and roads, making it  
 easy to access (see Fig. 8).

The snowpack at the Schnalstal field site, with a height of 79 cm, was profiled on 7 June 2023, at 12:30 LT. During the  
 measurements, the air temperature stood at  $1.8^\circ\text{C}$ , and there was negligible wind speed, ensuring relatively stable conditions  
 for the assessment. The snowpack structure was as follows: from the surface down to 65 cm, a layer of recent snow was  
 540 observed, which had undergone wetting due to temperature and solar radiation, which were relatively high that day. The  
 subsequent layer, spanning from 65 cm to 57 cm, contained three prominent ice lenses. Notably, a significant amount of  $\theta_w$   
 was trapped within this layer, contributing to its distinctive characteristics.

Continuing downwards, the layer from 57 cm to the base at 0 cm was characterized by coarse snow crystals with size from  
 1 to 2 mm, exhibiting lower water retention capability. Importantly, there was no noticeable  $\theta_w^M$  presence within this layer.  
 545 However, the lowermost 20 cm of the snowpack presented some noticeable challenges. This section displayed loose and coarse  
 crystals, leading to difficulties in proper sampling and ensuring optimal coupling between the Denoth instrument and the snow.  
 Consequently, these lower 20 cm were excluded from the subsequent analysis to ensure data accuracy and reliability.

Figure 10 (a) depicts the volumetric liquid water content ( $\theta_w^M$ ) profile, measured with the melting calorimeter technique,  
 along with its corresponding uncertainty, as computed using Eqs. (3) and (8). Panel (b) of the figure portrays  $\theta_w$  profile derived

550 from Denoth measurements. Panel (c) showcases the snow density associated with the measurement points obtained from the calorimeter. These profiles collectively provide valuable insights into the internal structure of the snowpack and its distribution of liquid water. Specifically, the  $\theta_w$  profile reflects the typical conditions in 2023 of the European alpine snowpacks, where ice lenses were often present. Despite a significant amount of snowfall occurring in spring, the melting process was hindered by the presence of these ice lenses, impeding the transport of water to the ground. We can notice how the Denothmeter underestimates  
555 the superficial  $\theta_w$ . ~~However Although~~ the coherence of the profile along the vertical axis and ~~the good correlation with the density and stratigraphy lead us to favor its correlation with density and stratigraphy are in favor of calorimetric measurements.~~ additional data and analysis are required to fully support the preference of the calorimetry profile over the Denothmeter.

Finally, to better verify the consistency of our measurements, we repeated a subset of measurements at very close distances on a uniform layer. The results of these repeated measurements yielded the following  $\theta_w$  values: 7.27, 7.10, 7.19, and 7.20, with  
560 corresponding standard deviations of 0.50, 0.46, 0.56, and 0.52 respectively. These values were found to be very similar and fell within the uncertainty range, demonstrating the good stability of the melting calorimetry technique. Additionally, a z-test for null hypothesis verification (Rouder et al., 2009), applied at the difference between these values confirmed the evidence.

## 6 Discussion

The primary objective of this study was to provide a rigorous exposition of the melting calorimetric technique for estimating  
565 liquid water content. The literature outlines two calorimetric approaches used for the estimation of  $\theta_w$ . Prior to our paper, a rigorous mathematical analysis by Colbeck (1978) argued against the use of melting calorimetry, a concept that echoed in subsequent works, thus becoming widely accepted. We have clarified and expanded upon Colbeck's findings, demonstrating unequivocally that the two techniques are comparable in terms of accuracy. While freezing calorimetry still holds an edge, particularly considering instrumental uncertainty alone, our analysis serves to dismiss the melting calorimeter accusations. The  
570 additional sources of uncertainties that stem from the challenging operational conditions of using a freezing calorimeter still require further investigation but might result in large uncertainty especially when used by inexperienced operators (Fisk, 1986). However, the melting calorimetry reputation for inaccuracy is partially justified by limitations in its mathematical modeling and uncertainty analysis. Building new concepts upon these unconsolidated works leads to the propagation of errors that may hinder the advancement of liquid water content measurement techniques.

575 We present the formulations i.e., Eq. (3) and Eq. (6) for both melting and freezing calorimeters, respectively expressed in %vol and incorporating the calorimetric constant. While the freezing formulation was established upon its introduction in literature (Jones et al., 1983), the melting formulation lacked compensation for heat exchange within the calorimeter, a discrepancy we noted since Yoshida's initial works and reiterated by Kawashima et al. (1998). This was pointed out from the first applications of the melting calorimeter Halliday (1950). The concept of the calorimetric constant, was initially introduced  
580 for freezing calorimeters (Jones et al., 1983; Boyne and Fisk, 1987; Austin, 1990), but had not been extended to melting calorimetry until a recent study by Fasani et al. (2023). We clarify the most effective method for estimating  $E$ , considering

various approaches documented in the literature and evaluating their impact on uncertainty, showing that non-destructive methods based on calorimetry itself are largely uncertain and should be avoided.

We generally doubt the effectiveness of preparing artificial samples as reference samples with a given  $\theta_w$  as done in (Fasani et al., 2023; Kawashima et al., 1998), because the assumption that the added water exchange heat with the whole ice matrix cannot be always satisfied. Therefore, the selected approach for estimating  $E$  in (Fasani et al., 2023), which is characterized by a significant uncertainty propagation, coupled with strong assumption and non-stringent experimental protocols such as elevated values of  $R$  (as depicted in Fig. 3 the impact of high  $R$  on measurement uncertainty is large), yields results impacted with noise. This renders the interpretation of the presented results challenging and subject to dispute. The impression is that the manner in which water is added to the snow samples, introduces a systematic bias, varying with the amount added to which a large uncertainty is added (see Fig. 5 of the original paper).

We introduce a formulation for estimating volume measurement uncertainty according to the GUM (IEC et al., 1993), emphasizing its importance for facilitating comparisons between measurements. While the error propagation for the freezing calorimetry proposed by Jones et al. (1983) aligns with our approach (and leads to similar results when expressed in sum of absolute uncertainty per mass), the Kawashima et al. (1998) formulation for melting calorimeters relies on erroneous approximations and misleading presentation of the results. In this paper, we also attempt to quantify random uncertainty related to environmental and operator variability. While the limitations of the available instrument prevented a fully comprehensive uncertainty analysis, we believe that the investigating of the impact of more complex sources of uncertainty on  $\theta_w$  measurements remains an intriguing topic for future research and development.

Leveraging our proposed formulation, we have developed and validated a field protocol for measuring liquid water content using the melting calorimeter. While some steps of the field protocol may resemble those in Kawashima et al. (1998), there are some difference in the theoretical foundation. Our analysis provides guidance on various aspects, however the sample handling during extraction from the snowpack remains a key source of uncertainty. Mechanical shocks, contact with sampler material, large temperature difference from the snow and air, and solar radiation during extraction can all generate liquid water. Additionally, the impact of potentially prolonged pit exposure, a necessity for obtaining spatially detailed liquid water content profiles for deep snowpack, on water transport within the snowpack remains an open question. While our primary focus here is on the melting calorimeter accuracy for field-based  $\theta_w$  measurements, and not its application in water transport studies, the results suggest that following the protocol strictly, including measures like shading the pit from solar radiation, can mitigate this issue and provide important information about water transport inside the snowpack. Further investigation is anyway require to properly assess the influence of pit exposure.

In a field comparison at the Italian and Swiss sites, we measured liquid water content using both the melting calorimeter and the Denothmeter. By comparing our findings with results from Boyne and Fisk (1987) (which compared the freezing calorimeter, alcohol calorimeter, dilution technique, and Denothmeter), we established that our novel formulation for the melting calorimeter yields results indirectly comparable to the established freezing and dilution methods. This finding validates our approach and strengthens the case for the melting calorimeter as a reliable measurement tool. This challenges the general notion propagated by Linlor et al. (1975) of the melting calorimeter overestimation compared to freezing methods, which at this

point should be possibly attributed to the missed calorimetric constant. This insight could be leveraged in (Webb et al., 2021), and related datasets, which at the moment show a bias similar to our WFJ measurements when the calorimetry compensation is not applied.

620 Finally, the obtained liquid water profiles of Figures 9 and 10 corroborate the observations in (Perla, 1991) that the Denoth-  
meter provides accurate measurements for low liquid water content  $\theta_w$  – typically below 5 – 8% the uncertainty is between  
0.5 – 1% – but underestimates  $\theta_w$  in very wet or soaked snow. The melting calorimeter, when employed with the proposed  
formulation, has the potential to expand the already substantial data set established by (Perla, 1991). This expanded data set  
could be instrumental in refining the calibration of the relationship between wet snow dielectric constant and  $\theta_w$ , potentially  
625 leading to a clearer understanding of the physical factors that limit the unique determination of water content through dielectric  
measurements (Picard et al., 2022; Colbeck, 1980; Camp, 1992).

## 7 Conclusions

The potential of melting calorimetry for measuring snow liquid water content has long been overshadowed by misconceptions about its accuracy.

630 This paper, challenged this perception by comparing the melting and freezing calorimetry techniques, focusing on their  
applicability for measurements in the field. While freezing calorimetry still holds an edge, our findings indicated that the  
measurements obtained using the melting calorimeter are still accurate enough for a meaningful analysis of liquid water content  
in the snowpack, offering at the same time notable practical advantages. To support our claims, we had thoroughly examined  
and propagated uncertainties, encompassing not only instrumental factors but also variations arising from the operational  
635 procedures and environmental conditions. As a result, we devised a field protocol that effectively minimizes these uncertainties.  
The protocol includes specific instructions on the amount of hot water to be used, its temperature, the size of the calorimeter, the  
masses involved, and other crucial details for controlling the uncertainty during the experiment replication. This protocol was  
applied in two different test sites in Italy and Switzerland by two different research groups with different melting calorimeters.  
The results, compared to independent measurements of dielectric constant of the snow, showed how the application of the  
640 proposed protocol to the melting calorimetric measurements is able to properly track the wet front penetration inside the  
snowpack in an accurate way.

In conclusion, this research promotes the wider adoption of melting calorimetry as a reliable field tool for quantifying liquid water content in snowpacks. This capability offers significant advantages for calibrating or validating new and potentially non-destructive methods based on electromagnetic interactions with wet snow.

645 *Code and data availability.* The code to calculate  $\theta_w$  and its uncertainty from the melting calorimetry analysis will be made available along with the code for generating the figures in the paper in a dedicated GitLab of the Snowtinel project.

## Appendix A

In order to derive the calorimetric constant  $E$ , if information regarding the material and mass of the calorimeter cannot be obtained, the heat-balance principle can be applied. In the literature, the calorimeter constant was determined using a basic heat-balance principle (Jones et al. (1983); Austin (1990)). When warm fluid is mixed with cold fluid in the calorimeter bottle, the heat lost by the warm fluid must be equal to the heat gained by the cold fluid and the bottle itself.

For the case of water, the heat-balance equation is given by:

$$\underbrace{Q_{hot\ water}}_{M_w C(T_f - T_w)} + \underbrace{Q_{cold\ water}}_{M_{cw} C(T_f - T_{cw})} + \underbrace{Q_{calorimeter}}_{M_{cw} C_{cal}(T_f - T_{cw})} = 0 \quad (A1)$$

Therefore we can obtain the calorimetric constant expressed in equivalent water mass as follows

$$E = \frac{M_w(T_f - T_w)}{(T_{cw} - T_f)} - M_{cw} \quad (A2)$$

In this equation,  $M_w$  and  $T_w$  represent the mass and temperature of the hot water, while  $M_{cw}$  and  $T_{cw}$  represent the mass and temperature of the cold water, respectively. By analyzing the uncertainty propagation of the measurements on  $E$  with the same approach presented in 3.1 we can retrieve the uncertainty on the estimation of  $E$ ,  $\sigma_E$ :

$$\sigma_E = \sqrt{\left(\frac{\partial E}{\partial M_w}\right)^2 \sigma_{M_w}^2 + \left(\frac{\partial E}{\partial M_{cw}}\right)^2 \sigma_{M_{cw}}^2 + \left(\frac{\partial E}{\partial T_w}\right)^2 \sigma_{T_w}^2 + \left(\frac{\partial E}{\partial T_f}\right)^2 \sigma_{T_f}^2 + \left(\frac{\partial E}{\partial T_{cw}}\right)^2 \sigma_{T_{cw}}^2} \quad (A3)$$

The partial derivatives in Eq. (A3) are calculated as follows:

$$\frac{\partial E}{\partial M_w} = \frac{T_f - T_w}{T_{cw} - T_f} \quad (A4)$$

$$\frac{\partial E}{\partial M_{cw}} = -1 \quad (A5)$$

$$\frac{\partial E}{\partial T_w} = -\frac{M_w}{T_{cw} - T_f} \quad (A6)$$

$$\frac{\partial E}{\partial T_f} = \frac{M_w(T_{cw} - T_f) + M_w(T_f - T_w)}{(T_{cw} - T_f)^2} \quad (A7)$$

$$665 \quad \frac{\partial E}{\partial T_{cw}} = -M_w \frac{T_f - T_w}{(T_{cw} - T_f)^2} \quad (\text{A8})$$

It becomes evident that  $\sigma_E$  is strongly related to the difference  $T_f - T_{cw}$ , which should be maximized. To achieve this, we aim to maximize the difference between  $T_{cw}$  and  $T_h$ , while minimizing  $M_{cw}$ . However, in a hypothetical scenario with  $M_{cw} = 5$  g,  $M_w = 495$  g,  $T_{cw} = 273\text{K}$ ,  $T_w = 373\text{K}$ , and  $E = 6.58$  g, the uncertainty  $\sigma_E$  associated with  $E$  is equal to 2.6 g, which is approximately  $\frac{1}{3}$  of the value of  $E$ . Realistically, this experiment is challenging to conduct, primarily because it would  
670 be extremely difficult to maintain thermal equilibrium for 5 g of water with the internal wall. This was also recongized in Austin (1990).

An alternative way for estimating the calorimetric constant  $E$  is discussed in Fasani et al. (2023). Here the parameter  $E$  is retrieved using the same energy balance as in Eq. 1, and in detail inverting Eq. 3 expliciting  $E$  as a function of  $\theta_w^M$ . This approach requires the employment of wet snow samples with known liquid water content, with all the relative associated difficulties in  
675 controlling the process. We present here the analysis on the uncertainty  $\sigma_E$  associated to the parameter  $E$  following the same approach as in Eq. 3.1. In detail, by inverting Eq. 3, we can obtain  $E$  as:

$$E = \frac{(T_f - T_s)M_s + \frac{L}{C}(M_s - \theta_w^M V_s \rho_w)}{T_w - T_f} - M_w \quad (\text{A9})$$

By analyzing the uncertainty propagation of the measurements on  $E$  with the same approach presented in 3.1 we can retrieve the uncertainty on the estimation of  $E$ ,  $\sigma_E$ :

$$680 \quad \sigma_E = \sqrt{\left(\frac{\partial E}{\partial T_f}\right)^2 \sigma_{T_f}^2 + \left(\frac{\partial E}{\partial T_w}\right)^2 \sigma_{T_w}^2 + \left(\frac{\partial E}{\partial M_s}\right)^2 \sigma_{M_s}^2 + \left(\frac{\partial E}{\partial \theta_w^M}\right)^2 \sigma_{\theta_w^M}^2 + \left(\frac{\partial E}{\partial V_s}\right)^2 \sigma_{V_s}^2 + \left(\frac{\partial E}{\partial M_w}\right)^2 \sigma_{M_w}^2} \quad (\text{A10})$$

The partial derivatives in Eq. (A10) are calculated as follows:

$$\frac{\partial E}{\partial T_f} = \frac{M_s(T_w - T_s) + \frac{L}{C}(M_s - \theta_w^M V_s \rho_w)}{(T_w - T_f)^2} \quad (\text{A11})$$

$$\frac{\partial E}{\partial T_w} = -\frac{M_s(T_f - T_s) + \frac{L}{C}(M_s - \theta_w^M V_s \rho_w)}{(T_w - T_f)^2} \quad (\text{A12})$$

$$\frac{\partial E}{\partial M_s} = \frac{T_f - T_s}{T_w - T_f} + \frac{L}{C(T_w - T_f)} \quad (\text{A13})$$

$$685 \quad \frac{\partial E}{\partial \theta_w^M} = -\frac{V_s \rho_w L}{C(T_w - T_f)} \quad (\text{A14})$$

$$\frac{\partial E}{\partial V_s} = -\frac{\theta_w^M \rho_w L}{C(T_w - T_f)} \quad (\text{A15})$$

$$\frac{\partial E}{\partial M_w} = -1 \quad (\text{A16})$$

It is evident that  $\sigma_E$  is strongly related to the difference  $T_f - T_w$ , which should be maximized. However, in a hypothetical scenario with  $M_w = 167$  g,  $M_s = 83$  g,  $T_w = 313$ K, the uncertainty  $\sigma_E$  associated with  $E$  is equal to 4.87 g, which is more than  $\frac{2}{3}$  of the value of  $E$ , here set to 6.58 g.

A possible mitigation for the large error associated to the estimation of  $E$ , it is to use hot water and ice instead of water at different temperatures. However, it is again important to use the propagation of uncertainty to find how uncertainty is such kind of measurement of  $E$ . For the ice-water case, the heat-balance equation to retrieve  $E$  becomes:

$$\underbrace{M_w C(T_f - T_w)}_{Q_{hot\ water}} + \underbrace{M_{cal} C_{cal}(T_f - T_w)}_{Q_{calorimeter}} + \underbrace{M_i C_i(T_f - T_i)}_{Q_{warming\ ice}} + \underbrace{LM_i}_{Q_{melting\ ice}} + \underbrace{M_i C(T_f - T_{mi})}_{Q_{melted\ ice}} = 0 \quad (\text{A17})$$

From where we can derive  $E$  as follow:

$$E = \frac{M_i(C_i T_i - L - T_f)}{C(T_f - T_w)} - M_w \quad (\text{A18})$$

Here,  $M_i$  and  $T_i$  represent the mass and temperature of ice, while  $M_w$  and  $T_w$  represent the mass and temperature of hot water.  $T_{mi}$  instead is the temperature of the water coming from the melted ice cube, and it is equal to 273.15 K. Also for this case we can propagate the measurements uncertainty and find the associated  $\sigma_E$

$$\sigma_E = \sqrt{\left(\frac{\partial E}{\partial M_i}\right)^2 \sigma_{M_i}^2 + \left(\frac{\partial E}{\partial M_h}\right)^2 \sigma_{M_h}^2 + \left(\frac{\partial E}{\partial T_h}\right)^2 \sigma_{T_h}^2 + \left(\frac{\partial E}{\partial T_f}\right)^2 \sigma_{T_f}^2 + \left(\frac{\partial E}{\partial T_i}\right)^2 \sigma_{T_i}^2} \quad (\text{A19})$$

The partial derivatives in Eq. (A19) are calculated as follows:

$$\frac{\partial E}{\partial M_i} = \frac{C_i T_i - L - C T_f}{C(T_f - T_h)} \quad (\text{A20})$$

$$\frac{\partial E}{\partial M_h} = -1 \quad (\text{A21})$$

$$\frac{\partial E}{\partial T_h} = \frac{M_i(C_i T_i - L - C T_f)}{C(T_f - T_w)^2} \quad (\text{A22})$$

$$705 \quad \frac{\partial E}{\partial T_f} = \frac{-CM_i(T_f - T_h) - M_i(C_i T_i - L - CT_f)}{C(T_f - T_w)^2} \quad (\text{A23})$$

$$\frac{\partial E}{\partial T_i} = \frac{M_i C_i}{C(T_f - T_w)} \quad (\text{A24})$$

Analyzing the error for this case, we observe that it is strongly influenced by the difference between  $T_f$  and  $T_w$ . In a hypothetical scenario with  $M_h = 300g$ ,  $M_i = 200g$ ,  $T_h = 373K$ ,  $T_i = 244.5K$ , and  $E = 6.58g$ , the uncertainty  $\sigma_E$  associated with  $E$  is equal to 1.6 g, which is approximately  $\frac{1}{4}$  of the value of  $E$ . This is still an high uncertainty, but unlike the water-water case, this experiment does not suffer from the same limitations. Hence, if it is impossible to retrieve the exact mass and specific heat of the calorimeter, the best way to estimate  $E$  would be using hot water and ice. It is important to note that for both cases, using ice and water at extreme temperatures would lead to noticeable heat dispersion in a short amount of time, making it challenging to obtain exact temperature measurements.

Because of these reasons we destructively analyzed our calorimeters to estimate  $E$  using Eq. (2). Fortunately this process has to be done once, and other users can use  $E$  provided in the paper i.e.,  $E = 6.58g$  given that they use the same calorimeter.

## Appendix B

In this Appendix, we will show all the formulations partly presented in (Colbeck, 1978) that allows us to prove that the relative uncertainty produced by the melting calorimeter on the estimation of the ice volume is one order of magnitude lower than the relative uncertainty produced by the freezing calorimeter on the water volume. With this mathematical step we unlock the melting calorimeter for being “inherently inaccurate”.

We compute the relative uncertainty produced by the melting calorimeter on the estimation of the ice volume starting from Eq. (3) in the main paper, written in terms of  $V_i$ :

$$V_i = \frac{C}{\rho_i L} [M_w(T_w - T_f) - M_s(T_f - T_s)] \quad (\text{B1})$$

Note that we do not account for  $E$  to be consistent with the Colbeck’s formulation. Hence, we compute the partial derivatives for each of the measured variables, by assuming  $k = \frac{C}{L}$ :

$$\begin{cases} \frac{\partial V_i}{\partial T_w} = \frac{k}{\rho_i} M_w \\ \frac{\partial V_i}{\partial T_f} = -\frac{k}{\rho_i} (M_w + M_s) \\ \frac{\partial V_i}{\partial M_w} = \frac{k}{\rho_i} (T_w - T_f) \\ \frac{\partial V_i}{\partial M_s} = -\frac{k}{\rho_i} (T_f - T_s) \end{cases} \quad (\text{B2})$$



**Table B1.** Variable values used for the computation of the relative uncertainty produced by the melting calorimeter on the estimation of the ice volume.

Variable	Value	Unit
C	$4.2 \cdot 10^3$	$\text{J kg}^{-1} \text{K}^{-1}$
L	$3.34 \cdot 10^5$	$\text{J kg}^{-1}$
$\rho_i$	917	$\text{kg m}^{-3}$
$M_w$	1.067	kg
$T_w$	313.15	K
$T_f$	277.04	K
$M_s$	0.5335	kg
$T_s$	273.15	K

and calculate the relative uncertainty  $\Sigma_{V_i}$  as sum of each term:

$$\Sigma_{V_i} = \left| \frac{\partial V_i}{\partial T_w} \right| \left| \frac{T_w}{V_i} \right| \left| \frac{dT}{T_w} \right| + \left| \frac{\partial V_i}{\partial T_f} \right| \left| \frac{T_f}{V_i} \right| \left| \frac{dT}{T_f} \right| + \left| \frac{\partial V_i}{\partial M_w} \right| \left| \frac{M_w}{V_i} \right| \left| \frac{dM}{M_w} \right| + \left| \frac{\partial V_i}{\partial M_s} \right| \left| \frac{M_s}{V_i} \right| \left| \frac{dM}{M_s} \right| \quad (\text{B3})$$

By simplifying, we obtain:

$$730 \quad \Sigma_{V_i} = \left| \frac{\partial V_i}{\partial T_w} \right| \left| \frac{dT}{V_i} \right| + \left| \frac{\partial V_i}{\partial T_f} \right| \left| \frac{dT}{V_i} \right| + \left| \frac{\partial V_i}{\partial M_w} \right| \left| \frac{dM}{V_i} \right| + \left| \frac{\partial V_i}{\partial M_s} \right| \left| \frac{dM}{V_i} \right| \quad (\text{B4})$$

By considering the values reported in Table B1, we obtain  $\Sigma_{V_i} = 0.007426\text{m}^3$ . The values in the table are obtained by considering a snow sample with  $M_w = 2 \cdot M_s$ ,  $V_s = 10^{-3}\text{m}^3$ ,  $V_i = 500 \cdot 10^{-6}\text{m}^3$ ,  $V_a = 75 \cdot 10^{-6}\text{m}^3$  and  $V_a = 425 \cdot 10^{-6}\text{m}^3$ .

Similarly, for the freezing calorimeter we can compute the relative uncertainty on the estimation of the water volume starting from the equation of Jones, Eq. (6) in the main paper, written in terms of  $V_w$ :

$$735 \quad V_w = \frac{M_o C_o (T_{fo} - T_o) + M_s C_s (T_{fo} - T_s)}{\rho_w L} \quad (\text{B5})$$

Hence, we compute the partial derivatives for each of the measured variables, by assuming  $k = \frac{C}{L}$ :

$$\left\{ \begin{array}{l} \frac{\partial V_w}{\partial T_o} = -\frac{M_o C_o}{\rho_w L} \\ \frac{\partial V_w}{\partial T_{fo}} = \frac{M_o C_o + M_s C_s}{\rho_w L} \\ \frac{\partial V_w}{\partial M_o} = \frac{C_o (T_{fo} - T_o)}{\rho_w L} \\ \frac{\partial V_w}{\partial M_s} = \frac{C_s (T_{fo} - T_s)}{\rho_w L} \end{array} \right. \quad (\text{B6})$$

and calculate the relative uncertainty  $\Sigma_{V_w}$  as sum of each term:

**Table B2.** Variable values used for the computation of the relative uncertainty produced by the freezing calorimeter on the estimation of the water volume.

Variable	Value	Unit
$C_o$	$1.83 \cdot 10^3$	$\text{J kg}^{-1} \text{K}^{-1}$
$C_s$	$2.09 \cdot 10^3$	$\text{J kg}^{-1} \text{K}^{-1}$
$L$	$3.34 \cdot 10^5$	$\text{J kg}^{-1}$
$\rho_w$	1000	$\text{kg m}^{-3}$
$M_o$	0.69355	kg
$T_o$	243.15	K
$T_{fo}$	267.69	K
$M_s$	0.5335	kg
$T_s$	273.15	K

$$\Sigma_{V_w} = \left| \frac{\partial V_w}{\partial T_o} \right| \left| \frac{T_o}{V_w} \right| \left| \frac{dT}{T_o} \right| + \left| \frac{\partial V_w}{\partial T_{fo}} \right| \left| \frac{T_{fo}}{V_w} \right| \left| \frac{dT}{T_{fo}} \right| + \left| \frac{\partial V_w}{\partial M_o} \right| \left| \frac{M_o}{V_w} \right| \left| \frac{dM}{M_o} \right| + \left| \frac{\partial V_w}{\partial M_s} \right| \left| \frac{M_s}{V_w} \right| \left| \frac{dM}{M_s} \right| \quad (\text{B7})$$

740 By simplifying, we obtain:

$$\Sigma_{V_w} = \left| \frac{\partial V_w}{\partial T_o} \right| \left| \frac{dT}{V_w} \right| + \left| \frac{\partial V_w}{\partial T_{fo}} \right| \left| \frac{dT}{V_w} \right| + \left| \frac{\partial V_w}{\partial M_o} \right| \left| \frac{dM}{V_w} \right| + \left| \frac{\partial V_w}{\partial M_s} \right| \left| \frac{dM}{V_w} \right| \quad (\text{B8})$$

$dM$  and  $dT$  are the instrumental uncertainties and are fixed to  $10^{-4}$  g and 0.1 K respectively. By considering the values reported in Table B2, we obtain  $\Sigma_{V_w} = 0.014809\text{m}^3$  that results twice the error  $\Sigma_{V_i}$  calculated for the melting calorimeter. The values in the table are obtained by considering a snow sample with  $M_o = 1.3 \cdot M_s$ ,  $V_s = 10^{-3}\text{m}^3$ ,  $V_i = 500 \cdot 10^{-6}\text{m}^3$ ,  
745  $V_i = 75 \cdot 10^{-6}\text{m}^3$  and  $V_a = 425 \cdot 10^{-6}\text{m}^3$ .

*Author contributions.* RB and CM designed the research, carried out the experiments, processed the data, and wrote the paper; VP helped with the mathematical formulation and wrote the Appendix with the relative codes; NC contributed with the field experiments; MB and FC contributed to the WFJ data collection; all the authors contributed to the analysis and interpretation of the results and provided feedback on the final text.

750 *Competing interests.* The authors declare that they have no conflict of interest.

*Acknowledgements.* This work was supported by the joint project Swiss National Science Foundation (SNF) - Autonomous Province of Bolzano (Italy) "Snowtinel: Sentinel-1 SAR assisted catchment hydrology: toward an improved snow-melt dynamics for alpine regions" Contract No. 200021L205190.

## References

- 755 Austin, R. T.: Determination of the liquid water content of snow by freezing calorimetry, Tech. rep., 1990.
- Avanzi, F., Petrucci, G., Matzl, M., Schneebeli, M., and De Michele, C.: Early formation of preferential flow in a homogeneous snowpack observed by micro-CT, *Water Resources Research*, 53, 3713–3729, <https://doi.org/https://doi.org/10.1002/2016WR019502>, 2017.
- Boyne, H. and Fisk, D.: A comparison of snow cover liquid water measurement techniques, *Water Resources Research*, 23, 1833–1836, 1987.
- 760 Camp, P. R.: Determination of the water content of snow by dielectric measurements, vol. 92, US Government Printing Office, 1992.
- Colbeck, S. C.: The difficulties of measuring the water saturation and porosity of snow, *Journal of Glaciology*, 20, 189–201, 1978.
- Colbeck, S. C.: Liquid distribution and the dielectric constant of wet snow, in: *Goddard Space Flight Center Microwave Remote Sensing of Snowpack Properties*, 1980.
- Davis, R. E., Dozier, J., LaChapelle, E. R., and Perla, R.: Field and Laboratory Measurements of Snow Liquid Water by Dilution, *Water Resources Research*, 21, 1415–1420, <https://doi.org/https://doi.org/10.1029/WR021i009p01415>, 1985.
- 765 Denoth, A. and Foglar, A.: Recent developments of snow moisture dielectric devices, in: *Proceedings of the International Snow Science Workshop*, Lake Tahoe, CA, pp. 22–25, 1986.
- Denoth, A., Foglar, A., Weiland, P., Mätzler, C., Aebischer, H., Tiuri, M., and Sihvola, A.: A comparative study of instruments for measuring the liquid water content of snow, *Journal of Applied Physics*, 56, 2154–2160, <https://doi.org/10.1063/1.334215>, 1984.
- 770 Donahue, C., Skiles, S. M., and Hammonds, K.: Mapping liquid water content in snow at the millimeter scale: an intercomparison of mixed-phase optical property models using hyperspectral imaging and in situ measurements, *The Cryosphere*, 16, 43–59, 2022.
- Fasani, D., Cernuschi, F., and Colombo, L.: Calorimetric determination of wet snow liquid water content: The effect of test conditions on the calorimeter constant and its impact on the measurement uncertainty, *Cold Regions Science and Technology*, 214, 103 959, <https://doi.org/https://doi.org/10.1016/j.coldregions.2023.103959>, 2023.
- 775 Fierz, C., Armstrong, R., Durand, Y., Etchevers, P., E., G., McClung, D., Nishimura, K., P.K., S., and Sokratov, S.: The International Classification for Seasonal Snow on the Ground, IHP-VII Technical Documents in Hydrology N°83, IACS Contribution N°1, UNESCO/IHP, 2009.
- Fisk, D.: Method of Measuring Liquid Water Mass Fraction of Snow by Alcohol Solution, *Journal of Glaciology*, 32, 538–539, <https://doi.org/10.3189/S0022143000012272>, 1986.
- 780 Gagliano, E., Shean, D., Henderson, S., and Vanderwilt, S.: Capturing the Onset of Mountain Snowmelt Runoff Using Satellite Synthetic Aperture Radar, *Geophysical Research Letters*, 50, e2023GL105 303, <https://doi.org/https://doi.org/10.1029/2023GL105303>, e2023GL105303 2023GL105303, 2023.
- Halliday, I. G.: The Liquid Water Content of Snow Measurement in the Field, *Journal of Glaciology*, 1, 357–361, <https://doi.org/10.3189/S0022143000012521>, 1950.
- 785 Hirashima, H., Avanzi, F., and Wever, N.: Wet-Snow Metamorphism Drives the Transition From Preferential to Matrix Flow in Snow, *Geophysical Research Letters*, 46, 14 548–14 557, <https://doi.org/https://doi.org/10.1029/2019GL084152>, 2019.
- IEC, IFCC, ISO, IUPAC, and OIML: *Guide to the Expression of Uncertainty in Measurement (GUM)*, 1993.
- Jones, E. B., Rango, A., and Howell, S. M.: Snowpack Liquid Water Determinations Using Freezing Calorimetry, *Hydrology Research*, 14, 113–126, <https://doi.org/10.2166/nh.1983.0010>, 1983.

- 790 Jones, R. N.: Comparison of centrifuge and freezing calorimeter methods for measuring free water in snow, NASA STI/Recon Technical Report N, 80, 13 319, 1979.
- Kawashima, K., Endo, T., and Takeuchi, Y.: A portable calorimeter for measuring liquid-water content of wet snow, *Annals of Glaciology*, 26, 103–106, <https://doi.org/10.3189/1998AoG26-1-103-106>, 1998.
- Kendra, J., Ulaby, F., and Sarabandi, K.: Snow probe for in situ determination of wetness and density, *IEEE Transactions on Geoscience and Remote Sensing*, 32, 1152–1159, <https://doi.org/10.1109/36.338363>, 1994.
- 795 Kinar, N. J. and Pomeroy, J. W.: Measurement of the physical properties of the snowpack, *Reviews of Geophysics*, 53, 481–544, <https://doi.org/https://doi.org/10.1002/2015RG000481>, 2015.
- Leroux, N. R., Marsh, C. B., and Pomeroy, J. W.: Simulation of preferential flow in snow with a 2-D non-equilibrium Richards model and evaluation against laboratory data, *Water Resources Research*, 56, e2020WR027 466, 2020.
- 800 Linlor, W. I., Clapp, F. D., Meier, M. F., and Smith, J. L.: Snow wetness measurements for melt forecasting, in: *Operational Appl. of Satellite Snowcover Observations*, vol. 1, p. 375, 1975.
- Marin, C., Bertoldi, G., Premier, V., Callegari, M., Brida, C., Hürkamp, K., Tschiersch, J., Zebisch, M., and Notarnicola, C.: Use of Sentinel-1 radar observations to evaluate snowmelt dynamics in alpine regions, *The Cryosphere*, 14, 935–956, <https://doi.org/10.5194/tc-14-935-2020>, 2020.
- 805 Mavrovic, A., Madore, J.-B., Langlois, A., Royer, A., and Roy, A.: Snow liquid water content measurement using an open-ended coaxial probe (OECF), *Cold Regions Science and Technology*, 171, 102 958, <https://doi.org/https://doi.org/10.1016/j.coldregions.2019.102958>, 2020.
- Moffat, R. J.: Describing the uncertainties in experimental results, *Experimental thermal and fluid science*, 1, 3–17, 1988.
- Moure, A., Jones, N., Pawlak, J., Meyer, C., and Fu, X.: A Thermodynamic Nonequilibrium Model for Preferential Infiltration and Re-freezing of Melt in Snow, *Water Resources Research*, 59, e2022WR034 035, <https://doi.org/https://doi.org/10.1029/2022WR034035>, e2022WR034035 2022WR034035, 2023.
- Perla, R.: Real permittivity of snow at 1 MHz and 0°C, *Cold Regions Science and Technology*, 19, 215–219, [https://doi.org/https://doi.org/10.1016/0165-232X\(91\)90011-5](https://doi.org/https://doi.org/10.1016/0165-232X(91)90011-5), 1991.
- Perla, R. and Banner, J.: Calibration of capacitive cells for measuring water in snow, *Cold Regions Science and Technology*, 15, 225–231, [https://doi.org/https://doi.org/10.1016/0165-232X\(88\)90069-9](https://doi.org/https://doi.org/10.1016/0165-232X(88)90069-9), 1988.
- 815 Picard, G., Leduc-Leballeur, M., Banwell, A. F., Brucker, L., and Macelloni, G.: The sensitivity of satellite microwave observations to liquid water in the Antarctic snowpack, *The Cryosphere*, 16, 5061–5083, <https://doi.org/10.5194/tc-16-5061-2022>, 2022.
- Proksch, M., Rutter, N., Fierz, C., and Schneebeli, M.: Intercomparison of snow density measurements: bias, precision, and vertical resolution, *The Cryosphere*, 10, 371–384, <https://doi.org/10.5194/tc-10-371-2016>, 2016.
- 820 Rouder, J. N., Speckman, P. L., Sun, D., Morey, R. D., and Iverson, G.: Bayesian t tests for accepting and rejecting the null hypothesis, *Psychonomic bulletin & review*, 16, 225–237, 2009.
- Schlumpf, M., Hendrikx, J., Stormont, J., and Webb, R.: Quantifying short-term changes in snow strength due to increasing liquid water content above hydraulic barriers, *Cold Regions Science and Technology*, 218, 104 056, 2024.
- Stein, J., Laberge, G., and Lévesque, D.: Monitoring the dry density and the liquid water content of snow using time domain reflectometry (TDR), *Cold Regions Science and Technology*, 25, 123–136, [https://doi.org/https://doi.org/10.1016/S0165-232X\(96\)00022-5](https://doi.org/https://doi.org/10.1016/S0165-232X(96)00022-5), 1997.
- 825 Techel, F. and Pielmeier, C.: Point observations of liquid water content in wet snow; investigating methodical, spatial and temporal aspects, *The Cryosphere*, 5, 405–418, <https://doi.org/10.5194/tc-5-405-2011>, 2011.

- Valence, E., Baraer, M., Rosa, E., Barbecot, F., and Monty, C.: Drone-based ground-penetrating radar (GPR) application to snow hydrology, *The Cryosphere*, 16, 3843–3860, 2022.
- 830 Webb, R. W., Marziliano, A., McGrath, D., Bonnell, R., Meehan, T. G., Vuyovich, C., and Marshall, H.-P.: In Situ Determination of Dry and Wet Snow Permittivity: Improving Equations for Low Frequency Radar Applications, *Remote Sensing*, 13, <https://doi.org/10.3390/rs13224617>, 2021.
- Wever, N., Fierz, C., Mitterer, C., Hirashima, H., and Lehning, M.: Solving Richards Equation for snow improves snowpack meltwater runoff estimations in detailed multi-layer snowpack model, *The Cryosphere*, 8, 257–274, <https://doi.org/10.5194/tc-8-257-2014>, 2014.
- 835 Wever, N., Vera Valero, C., and Fierz, C.: Assessing wet snow avalanche activity using detailed physics based snowpack simulations, *Geophysical Research Letters*, 43, 5732–5740, <https://doi.org/https://doi.org/10.1002/2016GL068428>, 2016.
- Yosida, Z.: Instruments and Methods: A Calorimeter for Measuring the Free Water Content of Wet Snow, *Journal of Glaciology*, 3, 574–576, <https://doi.org/10.3189/S0022143000023698>, 1960.
- Yosida, Z.: Free water content of wet snow, *Physics of Snow and Ice: proceedings*, 1, 773–784, 1967.