



# Accuracy and sensitivity of NH<sub>3</sub> measurements using the Dräger Tube Method

Alexander Kelsch<sup>1</sup>, Matthias Claß<sup>1</sup>, and Nicolas Brüggemann<sup>1</sup>

<sup>1</sup>Forschungszentrum Jülich GmbH, Institute of Bio- and Geosciences – Agrosphere (IBG-3), Jülich, 52428, Germany

**Correspondence:** Alexander Kelsch (a.kelsch@fz-juelich.de)

**Abstract.** Regional estimates of ammonia (NH<sub>3</sub>) emissions are often missing data from heterogeneous or small fields. Areas with no experienced staff or in-field power supply also prevent the use of accurate and fully established micrometeorological measurement techniques. The Dräger Tube Method (DTM) is a calibrated open-dynamic chamber method, which requires little training to use and is comparatively inexpensive. It uses NH<sub>3</sub> detector tubes (Dräger Tubes), an automatic pump, as well as a chamber system comprised of four stainless steel chambers connected with PTFE tubing. Even though the DTM is often used in countries such as Germany and China, the detection accuracy, precision and sensitivity have not been tested yet. In order to quantify those for the DTM, we simultaneously measured defined NH<sub>3</sub> mixing ratios with the Dräger Tubes, with direct laser absorption spectroscopy (MGA<sup>7</sup>, MIRO Analytical AG, Switzerland) and with cavity ring-down spectroscopy (G2103, Picarro, Inc., USA). Second, we tested the exchange of the tubing material and heating of the tubing under laboratory conditions, as well as PTFE film attachments or wiping of the DTM chamber system with ethanol during outdoor measurements, on performance improvements. Results showed that the Dräger Tubes had a detection limit between 150 and 200 ppb, which is three to four times higher than originally assumed. Dräger Tube concentration measurements also underestimated NH<sub>3</sub> concentrations by 43 up to 100 % for mixing ratios between 50 and 300 ppb, and by 28 up to 46 % for mixing ratios between 500 and 1500 ppb. The PTFE tubing material showed similar performances to the polyester-polyurethane tubing material regarding response time, which was further improved by heating of the tubing to 50 °C. The modifications of the chamber surface and cleaning in the outdoor experiment did not lead to any improvements of NH<sub>3</sub> concentration measurements. The results suggest that the DTM should only be used where alternatives are unfeasible and high NH<sub>3</sub> emissions are to be expected. A further assessment of calibrated DTM with reference methods is required for a comprehensive evaluation and alternative developments for a more appropriate method replacing the DTM in small plot applications is encouraged.

## 20 1 Introduction

Ammonia (NH<sub>3</sub>) is one of the main air pollutants in Europe (European Environment Agency, 2023). Volatilization of NH<sub>3</sub> from agriculture is by far the largest source of anthropogenic NH<sub>3</sub> emissions and is responsible for 94 % of emissions in the European Union (European Environment Agency, 2023). NH<sub>3</sub> is highly reactive and combines with other molecules in the atmosphere such as sulphuric acid, nitric acid or hydrochloric acid to form particulate matter less than 2.5 μm in size, which has been shown to cause premature death, respiratory infections and diseases, lung cancer and cerebrovascular disease (Lelieveld



et al., 2015; Lim et al., 2012; Wang et al., 2017). Most of the volatilized  $\text{NH}_3$  is transported by the wind and redeposited on the earth's surface, either by rainwater or in combination with other molecules (Cameron et al., 2013). Deposition in aquatic and terrestrial ecosystems can lead to eutrophication and acidification, which has been shown to result in biodiversity loss (Behera et al., 2013). In addition, the volatilization of  $\text{NH}_3$  causes indirect greenhouse gas emissions once it is partially converted to nitrous oxide through bacterial nitrification after re-deposition into the soil. The reduction potential of  $\text{NH}_3$  in the EU is 20–35 % compared to year 2000 emission levels, and the environmental, health and economic benefits (including the reduced need for fertilizers) far exceed the necessary reduction costs (Zhang et al., 2020). Therefore, the NEC Directive 2016/2284 requires the EU member states to reduce their total  $\text{NH}_3$  emissions by 19 % by 2030 compared to year 2005 levels (EU Directive, 2016). To reduce the impact of agriculture on  $\text{NH}_3$  volatilization, it is crucial to accurately quantify emissions from various types of fertilizers and evaluate effective mitigation options. However, the large uncertainties in  $\text{NH}_3$  field measurements make it difficult to estimate precise national or regional emission inventories (Bouwman et al., 2002; Behera et al., 2013; Wang et al., 2018).

There are various approaches to measuring  $\text{NH}_3$  emissions in the field. The most common are micrometeorological and chamber methods (Di Perta et al., 2020). The main advantage of chamber measurements is their ease of use and relatively fast measurement. The disadvantage, however, is that the fluxes are linearly interpolated and also known - when not scaled by calibration - to underestimate the actual flux rates (Pacholski et al., 2006; Di Perta et al., 2020; Kamp et al., 2024; Roelcke et al., 2002). Micrometeorological methods are considered to be the most accurate. However, they are unsuitable for comparisons between several plots close to each other or for smaller, heterogeneous fields and those with no power supply (Pacholski et al., 2006; Roelcke et al., 2002). One of the biggest uncertainties in estimating global  $\text{NH}_3$  volatilization is the lack of field measurement data, especially in tropical agroecosystems (Bouwman et al., 2002) where micrometeorological methods could be impractical because of smaller and heterogeneous plot sizes. A cost-effective and practical solution proposed by Pacholski et al. (2006) is to use a dynamic chamber method calibrated with a micrometeorological method.

The Dräger Tube Method (DTM) was developed as a simple and cost-effective alternative for quantifying  $\text{NH}_3$  volatilization from soils, also covered by arable vegetation. It does not require a local power source or special laboratory equipment. This method allows measurements on smaller or heterogeneous fields (Pacholski et al., 2006; Roelcke et al., 2002). The current DTM system consists of four conical stainless steel chambers connected by several short PTFE tubes. Ambient air is drawn from the chambers and passed through an  $\text{NH}_3$  detector tube (Dräger Tube) from Drägerwerk AG & Co. KGaA (Lübeck, Germany) with the aid of a hand or automatic pump. The Dräger Tubes contain bromophenol blue, a pH indicator that turns blue as a result of the reaction with  $\text{NH}_3$ . The intensity of the blue coloration is proportional to the amount of reacting gas. Earlier comparisons of  $\text{NH}_3$  fluxes measured in the laboratory and 15N field studies showed good correlations, but the DTM underestimated the flux by an order of magnitude, which was attributed to the low air exchange rate (Rees et al., 1996; Roelcke et al., 2002). The DTM was later calibrated by Pacholski et al. (2006) with simultaneous measurements using the Integrated Horizontal Flux method (IHF). This calibration approach was later on validated by other comparative trials involving micrometeorological measurements (Gericke et al., 2011; Quakernack et al., 2012; Ni et al., 2015). However, an inherent underestimation of  $\text{NH}_3$  fluxes by the uncalibrated DTM could mean that the DTM also has a high detection limit, which could lead to unmeasurable



NH<sub>3</sub> mixing ratios in low-emitting plots. If this is the case, it makes sense to look for ways to improve the sensitivity of the DTM.

The DTM is susceptible to the same measurement errors that occur with other chamber systems for measuring NH<sub>3</sub>. Wall effects caused by the adhesion of NH<sub>3</sub> to the chamber and tubing surface can lead to an underestimation or hysteresis of the mixing ratio measurements of up to 50 % (Sintermann et al., 2012). This is due to the fact that NH<sub>3</sub> is a highly reactive gas that can combine very quickly with other molecules. As a result, NH<sub>3</sub> is very soluble in water and adheres to even the smallest water film on any surface, which delays the path from the chamber system into the measuring device. This delay is greater at temperatures of 5 °C or less, and less at higher temperatures such as 25 °C, as the volatility of NH<sub>3</sub> increases at higher temperatures (Fogg, 1991). In the past, the DTM had been used to perform NH<sub>3</sub> concentration measurements with different materials and methods. Roelcke et al. (2002) and Richter (1972) originally used four tin chambers with a total surface area of 400 cm<sup>2</sup> and inserted a polyethylene funnel into the chambers. Roelcke et al. (2002) used 35 cm PTFE tubing to connect the chambers and flushed 2–3 litres of air from the bottom surface through the chambers and into a used Dräger Tube each time before starting the measurements. This was intended for NH<sub>3</sub> to achieve a state of equilibrium in the chambers. This approach was further modified by Pacholski et al. (2006) by using stainless steel as the chamber material with a total surface area of 415 cm<sup>2</sup> for the chambers. The rinsing volume to reach a state of equilibrium was set to 2 l in the latest version of his method (Pacholski, 2016). The measuring time ranges from 1–5 min. Wall effects of the chamber system, the short measurement duration and the low flow rate could all contribute to reduced measurement accuracy.

There have also been a number of studies aimed at improving or testing the detection sensitivity of different chamber measurement systems, but none of them directly testing the influence of different materials used for dynamic chambers on NH<sub>3</sub> mixing ratios (Di Perta et al., 2020). Yang et al. (2019) compared NH<sub>3</sub> measurements from four chamber methods with predicted values and found that the portable ammonia detector method had the highest detection sensitivity and the lowest detection limit of the four. Regarding the material used for the tubing that transports NH<sub>3</sub> inside the instrument, Shah et al. (2006) tested the adsorption rate of NH<sub>3</sub> in five different tubing materials after 2 h at 1 and 10 parts per million (ppm) and at a flow rate of 10 l min<sup>-1</sup>. They found no significant difference between the selected materials. The flow rate was much higher than that used in the DTM and the adsorption dynamics at lower and higher time intervals were not studied. A significant part of the contribution to lower capture efficiencies could also come from the use of a stainless steel surface of the chambers. In a tubing material experiment, Yokelson et al. (2003) observed a longer response time of NH<sub>3</sub> within their experiment when they replaced part of the PTFE tubing with a stainless steel tubing at room temperature. This delay increased further at a temperature of 5°C.

Apart from the chamber system, the Dräger Tubes themselves also have a standard deviation of 10–15 % for NH<sub>3</sub> measurement precision. There are no publicly available results of tests on the sensitivity and detection accuracy of the Dräger Tubes. In addition, the original main purpose of the Dräger Tubes was the direct measurement of hazardous gas mixing ratio variations in the workplace or in enclosed spaces prior to entry, and the detection of gas leaks in process pipelines (Drägerwerk AG, 2011). For these applications, high accuracy and sensitivity are not required.




95 The main objective of this study was to test the detection accuracy, precision and sensitivity of the Dräger Tubes when used for the uncalibrated DTM.  $\text{NH}_3$  was measured in various mixing ratios from 50 to 1500 parts per billion (ppb). The influence of tubing material and temperature on response time was tested under laboratory conditions with a multicomponent gas analyzer based on mid-infrared laser absorption spectroscopy (MGA<sup>7</sup>, MIRO Analytical AG, Wallisellen, Switzerland). Due to the dependence of temperature on the adsorption of  $\text{NH}_3$ , it was expected that the heated tubes would perform better, i.e., feature a lower response time to changes in  $\text{NH}_3$  mixing ratio. Finally, the material used for the chamber system was tested for effects on the measured  $\text{NH}_3$  mixing ratios under field conditions. Uncalibrated DTM measurements with modifications to the chamber system were compared with measurements with the MGA<sup>7</sup>. The MGA<sup>7</sup> was able to display the  $\text{NH}_3$  mixing ratios entering the system in real time. This minimized the risk of underestimating the  $\text{NH}_3$  mixing ratios due to adsorption associated with short measurement times. The hypothesis was that the uncalibrated DTM would underestimate mixing ratios compared to the MGA<sup>7</sup>. The modifications tested on the Dräger system included changing the tubing material to polyester-polyurethane (PU) or Synflex 1300, wiping the inner surface of the chambers with ethanol after each use, and applying a thin PTFE film to the inner surface of the chambers.

## 2 Material and Methods

The study was divided into three experiments. The first experiment focused on quantifying the Dräger Tube detection accuracy, precision, and sensitivity for  $\text{NH}_3$ . The second experiment investigated the influence of tubing material and temperature on the response time. The third experiment evaluated the modifications to the chamber system during outdoor measurements.

### 2.1 Laboratory experimental setup

A sketch of the experimental setup can be found in Fig. 1. Two flow regulators were used to mix compressed  $\text{NH}_3$ -free air with a standard  $\text{NH}_3$  gas (50 ppm  $\text{NH}_3$  in  $\text{N}_2$ ) to achieve the desired  $\text{NH}_3$  mixing ratios. The compressed air was humidified with a bubbler to achieve ambient water vapor concentration. The  $\text{NH}_3$  and  $\text{H}_2\text{O}$  contents were determined using the G2103, a cavity ring-down spectrometer from Picarro Inc. (Santa Clara, CA, USA). Both tubing lines could be shut off with a valve that controlled the flow of gas to the main sampling line. The main sampling line was connected to a pump controlled with a needle valve and a mass flow meter to set the flow rate. For the tubing material and heating experiment, the tubing inserted between the regulated pump and the MGA<sup>7</sup> was interchangeable. The fixed tubing was PTFE with an outer diameter of 6.35 mm. To eliminate the adsorption effects of the fixed tubing, sample gas was constantly flushed through the system. An excess port was installed upstream of both gas line valves to prevent overpressure in the gas analyzers. Another excess port was installed upstream of the mass flow meter to prevent over- and under-pressure within the analyzers and to allow simultaneous measurements with the Dräger Tubes for quantification of the detection accuracy.

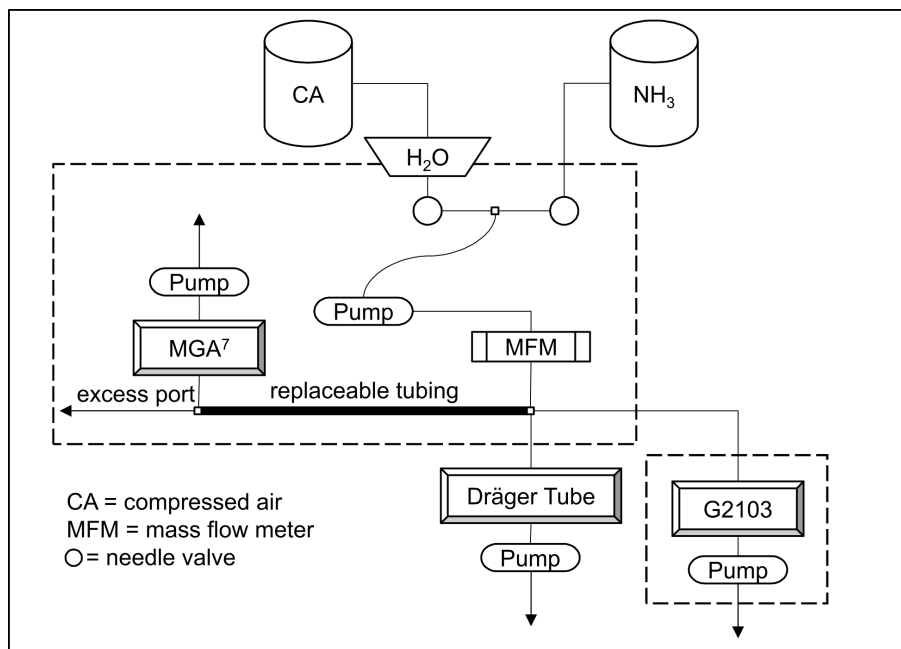

**Figure 1.** A sketch of the experimental setup used to test the  $\text{NH}_3$  detection accuracy of the Dräger Tubes and MGA<sup>7</sup> and the performance of different tubing materials at room temperature and when heated. The tubing connected to the Dräger Tube acted as a second excess port whenever the Dräger Tubes were not used. The pump behind the Dräger Tube was the Dräger X-act® 5000 Basic electric pump.

## 2.2 Quantification of the Dräger Tube detection accuracy, precision and sensitivity for $\text{NH}_3$

125 To determine the  $\text{NH}_3$  detection accuracy of both the MGA<sup>7</sup> and the Dräger Tubes, humid air with a defined  $\text{NH}_3$  mixing ratio was passed independently through both the MGA<sup>7</sup> and the G2103 in the laboratory setup. The mixing ratio was set at approximately 50, 100, 150, 200, 250, 300, 500, 1000, and 1500 ppb, respectively. The G2103 readings were used as a reference. The  $\text{NH}_3$  readings of both the MGA<sup>7</sup> and the G2103 were allowed to stabilize before starting the Dräger Tube measurements. The Dräger Tubes were inserted into the  $\text{NH}_3$ -rich air excess port as shown in Fig. 1 and then air was pumped

130 into the Dräger Tubes using the Dräger X-act 5000 Basic electric pump from Drägerwerk AG & Co. KGaA (Lübeck, Germany). A minimum of 10 and a maximum of 50 pump strokes were used for the measurements. Ten pump strokes were performed with a used Dräger Tube before each measurement. The Dräger Tube measurements were repeated three times for each mixing ratio level. The detection accuracy was determined by the difference in detected mixing ratios between the G2103 analyzer and the other instruments. The Dräger Tube measurements taken with more than 10 pump strokes (where 10 pump strokes equal 1

135 l of air volume) were scaled back to 1 l of air volume to make them comparable to the MGA<sup>7</sup> and G2103 measurements.



### 2.3 Influence of tubing material and tubing temperature on NH<sub>3</sub> response time

The response time of the MGA<sup>7</sup> to NH<sub>3</sub> was tested using different tubing materials. We selected PTFE (CS - Chromatographic Service GmbH, Langerwehe, Germany), PU (Landefeld Druckluft und Hydraulik GmbH, Kassel-Industriepark, Germany) and Synflex 1300 (Megaflex Limited, Bideford, England) tubing for the tests. The tubing had an outer diameter of 6.35 mm and an inner diameter of 4.3 mm for PTFE and Synflex 1300 and 4.2 for PU. The same laboratory setup was used as described in 2.2, but with a fixed NH<sub>3</sub> mixing ratio of 600 ppb. A 3 m section of the respective tubing was connected between the excess port next to the MGA<sup>7</sup> and the mass flow meter (Fig. 1). The tubing performance was tested at room temperature and then in a heated state by wrapping a 5 m long 20 W aquarium heating cable (Dennerle Eco-Line ThermoTronic, Dennerle GmbH, Münchweiler, Germany) around the tubing section and insulating it with ArmaFlex AF-2-012 (inner diameter 12 mm, insulation thickness 13 mm). The response time was defined as the time required for the sensor to detect 10–90 % of total NH<sub>3</sub> at increasing mixing ratios, and the time required for the sensor to detect 90–10 % at decreasing mixing ratios.

### 2.4 Outdoor experimental setup

We tried different modifications of the chamber system for the outdoor experiment and compared the differences in the measured mixing ratios of the Dräger Tubes and the MGA<sup>7</sup>. The chamber system for DTM and MGA<sup>7</sup> was the same as that used in Pacholski et al. (2006) and the modification changes were applied to the chamber systems of both devices. In the first trial, we compared the NH<sub>3</sub> mixing ratios of both devices without any changes to the chamber system. In the second trial, we wiped the inner surface of the chamber with 99 % ethanol before each measurement. Since NH<sub>3</sub> has a lower solubility in ethanol than in water, this was intended to replace the water film on the inner chamber surface. In the third trial, we replaced the PTFE tubing with PU tubing. Both PTFE and PU are hydrophobic. However, PU is much less expensive and more flexible, making it more practical to use during measurements. In the final trial, in an attempt to minimize potential water films on the inner surface of the chamber, the inside of the chambers was covered with 0.05 mm thick PTFE sheet. The PTFE sheet was attached to the surface of the chamber with a double-sided adhesive tape.

Four boxes measuring 56.5 × 36.0 × 17 cm filled with agricultural soil were placed next to a laboratory building on the campus of Forschungszentrum Jülich, Germany. The location ensured that the MGA<sup>7</sup> had both power and shelter nearby in the event of rain. The soil used was agricultural soil (silty loam, pH 6.4) collected from arable land at the agricultural research site Klein-Altendorf near Bonn, Germany. The coordinates of the soil collection point were 50.61618° N, 6.99489° E. A ClimaVUE50 all-in-one weather sensor and a CR300 data logger from Campbell Scientific (Logan, USA) were stationed near the soil boxes to record real-time weather data with a measurement interval of 1 min. Soil moisture was recorded with a TRIME PICO64 moisture sensor connected to an HD2 mobile reader (IMKO Micromodultechnik GmbH, Ettlingen, Germany), and soil temperature was recorded with a digital thermometer (Checktemp® 1 HI98509, Hanna Instruments Woonsocket, RI, USA) prior to each NH<sub>3</sub> measurement. Four stainless steel soil rings with a diameter of 11.5 cm were placed on the soil of each box. A solid urea fertilizer with 46 % nitrogen content (Piagran 46®, SKW Stickstoffwerke Piesteritz GmbH, Lutherstadt Wittenberg, Germany) was used for the fertilized plots. Urea was applied only within the soil rings, and approximately 0.135 g was applied



170 to each soil ring, corresponding to 60 kg N ha<sup>-1</sup>. After fertilization, each soil box was evenly irrigated with 1–2 mm of water whenever the soil was determined to be too dry to dissolve the urea. Soil boxes were re-fertilized when NH<sub>3</sub> was no longer detectable by the Dräger Tubes.

## 2.5 Outdoor measurements

The MGA<sup>7</sup> and its chamber system were connected to an electric pump and flow meter to maintain an air exchange rate of approximately 1 l min<sup>-1</sup>. The Dräger X-act® 5000 Basic pump used for the DTM takes approximately 1 min for 10 strokes of 175 0.1 l of air each stroke, which also corresponds to an air exchange rate of approximately 1 l min<sup>-1</sup>. Prior to the start of each measurement with the MGA<sup>7</sup>, the chamber system was placed on the soil rings of the respective box and flushed with air for 30 min. After a further 30 min, the indicated mixing ratio was recorded. At the same time, a second identical chamber system was flushed with another electric pump on another set of soil rings in preparation for the next measurement. DTM measurements were taken immediately after the completion of each MGA<sup>7</sup> measurement. Measurements were performed according to the 180 instructions from Pacholski (2016).

The air volume passing through the Dräger Tube depends on the number of pump strokes performed and was therefore always converted back to 10 pump strokes (equivalent to 1 l of air) for comparability.

## 2.6 Data Analysis

Data transformation and statistical analysis were performed using R version 4.3.2. In the intercomparison test of all instruments 185 for NH<sub>3</sub> mixing ratios, the detection accuracy of Dräger Tubes ( $y_{DT}$ ) and of the MGA<sup>7</sup> ( $y_{MGA^7}$ ) was defined as:

$$y_{DT,MGA^7} = \frac{NH_{3,DT,MGA^7} - NH_{3,G2103}}{NH_{3,G2103}} \cdot 100 \quad (1)$$

Detection precision was defined as the relative standard error of the measurements. Detection sensitivity was defined as the beta coefficient of a linear regression fitted to predict measured G2103 NH<sub>3</sub> mixing ratios from measured NH<sub>3</sub> mixing ratios of either the MGA<sup>7</sup> or Dräger Tubes.

190 A modified Hill function with an offset (Hill1, see Eq. 2) was fitted to the NH<sub>3</sub> response curves of the response time tests using OriginPro 2022b (64-bit) SR1 version 9.9.5.171. Where  $x$  was the duration in seconds;  $y$  was the NH<sub>3</sub> mixing ratio at a given duration; START was the NH<sub>3</sub> mixing ratio at  $x=0$ ; END was the maximum NH<sub>3</sub> mixing ratio for rising response curves or the minimum for falling response curves;  $k$  was the duration to reach 50 % of maximum NH<sub>3</sub> mixing ratios;  $n$  was the Hill coefficient. Response time was defined as the duration from  $y_{10\%}$  (EC<sub>10</sub>) to  $y_{90\%}$  (EC<sub>90</sub>) for rising curves and from EC<sub>90</sub> to 195 EC<sub>10</sub> for falling curves (see Eq. 3 and Eq. 4). To test the response time of rising response curves for statistical significance, a one-way ANOVA was used. For falling response curves, which did not follow a normal distribution, the Kruskal–Wallis rank sum test was used.

$$y = \text{START} + (\text{END} - \text{START}) \cdot \frac{x^n}{k^n + x^n} \quad (2)$$



$$EC_{10} = \frac{k}{9^{\frac{1}{n}}} \quad (3)$$

$$200 \quad EC_{90} = k \cdot 9^{\frac{1}{n}} \quad (4)$$

Finally, linear regression was used to compare the differences between the DTM and MGA<sup>7</sup> NH<sub>3</sub> measurements for each outdoor modification trial.

### 3 Results

#### 3.1 Quantification of the Dräger Tube detection accuracy, precision and sensitivity for NH<sub>3</sub>


205 The detection accuracy and precision relative to the G2103 measurements is displayed in Fig. 2. The MGA<sup>7</sup> measured slightly higher NH<sub>3</sub> mixing ratios compared to the G2103 and Dräger Tubes and had a detection accuracy of 97–114 % across the different NH<sub>3</sub> levels. The Dräger Tubes on the other hand measured lower mixing ratios and had a detection accuracy of 0–72 % across the different NH<sub>3</sub> levels. The detection accuracy was higher at high NH<sub>3</sub> levels and decreased up to 0 % at lower levels. The detection precision ranged between 0.04–1.80 % for the MGA<sup>7</sup> measurements and between 0–115.47 % for the  
210 Dräger Tubes.

The mean NH<sub>3</sub> detection sensitivity determined a beta coefficient of a fitted linear model to predict measured G2103 NH<sub>3</sub> mixing ratios with measured NH<sub>3</sub> mixing ratios using the MGA<sup>7</sup> or Dräger Tubes, which was statistically significant and 1.12 for the MGA<sup>7</sup> (95 % confidence interval (CI) [1.11, 1.13],  $t(34) = 372.11$ ,  $p < .001$ ;  $R^2 = 1.00$ ,  $F(1, 34) = 1.38e+05$ ,  $p < .001$ , adj.  $R^2 = 1.00$ ) and 0.72 for the Dräger Tubes (95 % CI [0.69, 0.76],  $t(34) = 41.03$ ,  $p < .001$ ;  $R^2 = 0.98$ ,  $F(1, 34) = 1683.44$ ,  $p <$   
215  $.001$ , adj.  $R^2 = 0.98$ ). However, the data of both the MGA<sup>7</sup> and Dräger Tube mixing ratios did not follow a normal distribution (Shapiro-Wilk test results:  $W = 0.75$ ,  $p < 0.001$  for MGA<sup>7</sup>;  $W = 0.72$ ,  $p < 0.001$  for Dräger Tubes).

#### 3.2 Influence of tubing material and tubing temperature on NH<sub>3</sub> response time

The main effect of the tubing material and temperature for rising NH<sub>3</sub> levels (Fig. 3a) was significant and large ( $F(5, 13) = 12.97$ ,  $p < .001$ ;  $\eta^2 = 0.83$ , 95 % CI [0.61, 1.00]) according to the performed one-way ANOVA. The response time of heated  
220 PTFE tubing was 10.71 min (standard deviation (SD) 0.92) and significantly shorter than both unheated and heated PU and Synflex tubing, but not significantly shorter than unheated PTFE tubing. The response time of unheated Synflex tubing was 51.25 min (SD 8.25) and significantly longer than both heated and unheated PTFE tubing and heated PU tubing. The main effect was significant for falling NH<sub>3</sub> levels (Fig. 3b) ( $F(5, 13) = 332.74$ ,  $p < .001$ ;  $\eta^2 = 0.89$ , 95 % CI [0.71, 0.96]) according to the performed Kruskal–Wallis test. The response time of heated PTFE tubing was 4.73 min (SD 0.23) and significantly shorter  
225 than both unheated and heated Synflex tubing, but not significantly shorter than the other tubing materials. The response time of unheated Synflex tubing was 25.11 min (SD 0.81) and significantly longer than unheated PU and heated PTFE tubing.



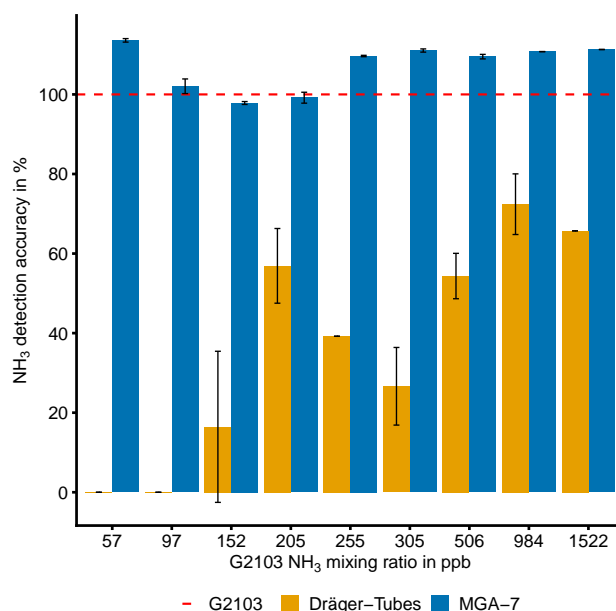


**Figure 2.** Detection accuracy of NH<sub>3</sub> with the Dräger Tube and MGA<sup>7</sup> relative to the NH<sub>3</sub> mixing ratio measurement of the G2103. Error bars indicate the detection precision as one standard deviation.

### 3.3 Chamber system modifications during outdoor measurements

A linear model was fitted to predict DTM NH<sub>3</sub> measurements from MGA<sup>7</sup> NH<sub>3</sub> measurements during four different trials where the chamber system was left unchanged or was slightly modified (Fig. 4). In the unchanged chamber system trial, the model explained a statistical significant and substantial proportion of variance ( $R^2 = 0.86$ ,  $F(1, 12) = 72.38$ ,  $p < .001$ , adj.  $R^2 = 0.85$ ). The model's intercept, corresponding to MGA<sup>7</sup> = 0 ppm, was at -0.09 ppm (95 % CI [-0.4, 0.23],  $t(12) = -0.59$ ,  $p = 0.564$ ). The unchanged chamber system had the highest beta coefficient of the four trials (beta = 0.68, 95 % CI [0.50, 0.85],  $t(12) = 8.51$ ,  $p < .001$ ).

During the trial where the inner chamber surfaces were cleaned with ethanol, the model explained a statistically significant, but only moderate proportion of the variance ( $R^2 = 0.22$ ,  $F(1, 20) = 5.52$ ,  $p = 0.029$ , adj.  $R^2 = 0.18$ ). The model's intercept was at 0.32 ppm (95 % CI [-0.10, 0.74],  $t(20) = 1.61$ ,  $p = 0.123$ ). This trial had the second lowest beta coefficient of the four trials (beta = 0.38, 95 % CI [0.04, 0.71],  $t(20) = 2.35$ ,  $p = 0.029$ ).

During the trial where the PTFE tubing was replaced with PU tubing, the model explained a statistically significant and substantial proportion of variance ( $R^2 = 0.85$ ,  $F(1, 33) = 182.02$ ,  $p < .001$ , adj.  $R^2 = 0.84$ ). The model's intercept was at 0.36 ppm (95 % CI [0.23, 0.50],  $t(33) = 5.50$ ,  $p < .001$ ). This trial had the second highest beta coefficient of the four trials (beta = 0.55, 95 % CI [0.46, 0.63],  $t(33) = 13.49$ ,  $p < .001$ ).

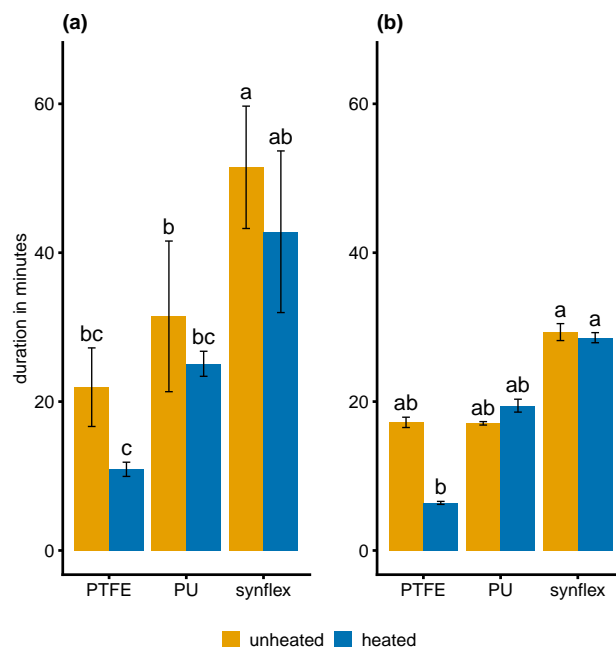


**Figure 3.** Response time for  $\text{NH}_3$  mixing ratios measured with the MGA<sup>7</sup> for (a) increasing from 10–90 % and (b) decreasing from 90–10 % of the  $\text{NH}_3$  target level, using different tubing materials unheated at room temperature or heated with a wire to 50 °C.

During the trial where a PTFE film was attached to the inner chamber surfaces, the model explained a statistical significant and substantial proportion of variance ( $R^2 = 0.61$ ,  $F(1, 61) = 94.13$ ,  $p < .001$ , adj.  $R^2 = 0.60$ ). The model's intercept was at 0.19 ppm (95 % CI [0.11, 0.28],  $t(61) = 4.51$ ,  $p < .001$ ). This trial had the lowest beta coefficient of the four trials (beta = 0.37, 245 95 % CI [0.29, 0.44],  $t(61) = 9.7$ ,  $p < .001$ ).

## 4 Discussion

### 4.1 Quantification of the Dräger Tube detection accuracy, precision and sensitivity for $\text{NH}_3$

Slightly higher  $\text{NH}_3$  mixing ratios were measured with the MGA<sup>7</sup> than with the G2103. The detection accuracy was between 97 % and 114 % for the various  $\text{NH}_3$  values. The mean detection sensitivity was 0.89. This means that the MGA<sup>7</sup> slightly 250 overestimated the  $\text{NH}_3$  mixing ratios in most cases compared to the G2103. This is in line with the results of the case study by the manufacturer of the MGA<sup>7</sup> (MIRO Analytical, 2021), which also compared  $\text{NH}_3$  measurements of the MGA with a cavity ring down spectroscopy device and found an average detection sensitivity of 0.748 at mixing ratios between 3 and 9 ppb. Since the detection accuracy was good even at low  $\text{NH}_3$  mixing ratios and comparable to that of the G2103, it was concluded that the MGA<sup>7</sup> could be safely used for response time and field measuring.

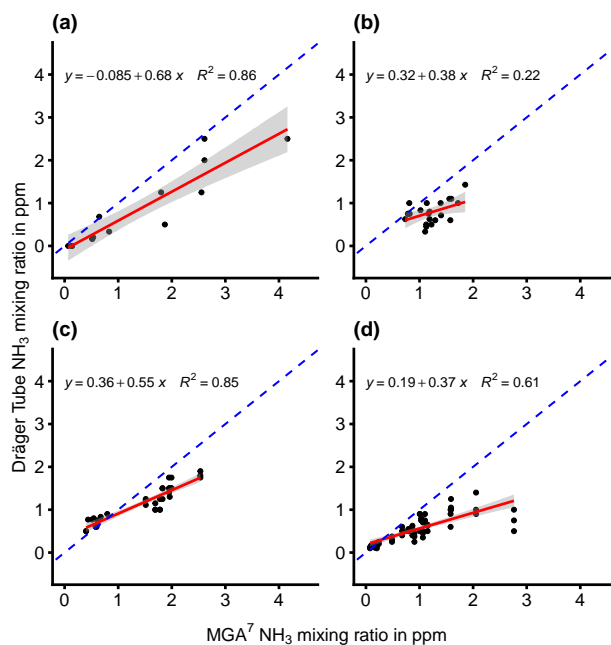

**Figure 4.** Linear regression relationships between Dräger Tube and MIRO measurements of the  $\text{NH}_3$  mixing ratio in ppb under different measurement conditions. (a) = unchanged DTM chambers connected to PTFE tubing; (b) = wiping of chambers with ethanol; (c) = connected to PU tubing and (d) = chambers with PTFE film attached to the inner surface.

255 The Dräger Tubes had a detection accuracy of 0 % at lower  $\text{NH}_3$  mixing ratios and a detection accuracy of up to 72 % at higher mixing ratios. This means that the Dräger Tubes considerably and significantly underestimated the  $\text{NH}_3$  mixing ratios compared to the G2103 device, with a trend of increasing underestimation at decreasing  $\text{NH}_3$  levels. It is already known that the DTM underestimates  $\text{NH}_3$ , but previous work on the DTM has cited the low air flow rate of the pump as the most likely reason for the underestimation of  $\text{NH}_3$  mixing ratios (Pacholski et al., 2006; Roelcke et al., 2002). This is correct, as shown by

260 Svensson and Ferm (1993), which tested the relationship between air flow rate and measured  $\text{NH}_3$  in chambers. However, the flow rate of the pumps in this test was set to that of the Dräger pump, which was approximately  $1 \text{ l min}^{-1}$ , for all instruments and  $\text{NH}_3$  was constantly flowing at a uniform rate throughout the entire tubing line, so there must be other factors contributing to the lower detection accuracy of the Dräger Tubes compared to the other devices.

One reason for this could be the short measuring time of the Dräger Tubes. While we gave the other devices sufficient time to

265 measure 100 % of the  $\text{NH}_3$  target value, this was not possible with the Dräger Tubes, as the tubes would be saturated with  $\text{NH}_3$  if air was pumped through the tubes for too long. Another reason could be that the Dräger Tubes were not designed for precise atmospheric measurements. According to the official instructions, only 10 strokes are intended for the measurement with the Dräger Tubes, which corresponds to an air volume of 1 l. Throughout the experiment, we used the 0.25/a  $\text{NH}_3$  detector tubes, whose indicator line ranges from 250–3000 ppb. At values below 300 ppb, therefore, more than the recommended amount of

270 1 l of air would have to be pumped through the Dräger Tube for  $\text{NH}_3$  to be detectable. This would explain the sharp drop in



detection accuracy in the Dräger Tubes for mixing ratios below 200 ppb, where 5 l of air had to be pumped through the Dräger Tube instead of 1 l (Fig. 2). The original use of the Dräger Tubes was to measure excess  $\text{NH}_3$  concentrations after fumigation of enclosed spaces, such as containers (Drägerwerk AG, 2011). The Dräger Tubes were therefore not designed for high detection accuracy, especially at lower  $\text{NH}_3$  concentrations.

275 The originally assumed detection limit of the Dräger Tubes, as used in the DTM, was 50 ppb. However, the results suggest that the detection limit is instead somewhere between 152 ppb and 205 ppb. The originally proposed detection limit was based on the assumption that increasing the number of pump strokes per measurement to 50 instead of 10 would proportionally improve the detection limit of the Dräger Tubes, which indicated 250 ppb on the lowest indicator line, down to 50 ppb (Roelcke, 1994). Since the previous detection limit was based on an assumption and not on empirical measurements, we suggest that a  
280 detection limit between 152 and 205 ppb is more correct.

A less sensitive detection limit than originally assumed could lead to erroneous  $\text{NH}_3$  measurements in two different ways. The first is that the actual  $\text{NH}_3$  mixing ratios at the fertilized soil surface are below the detection limit and are no longer detectable. In this case, the  $\text{NH}_3$  flux rates would be underestimated. The second case is that both the mixing ratios at the fertilized soil surface are detectable and the background mixing ratios are unusually high, but still below the detection limit.  
285 In this case, the  $\text{NH}_3$  flux rates would be overestimated. Therefore, instruments with the highest possible detection limit are preferred.

Table 1 shows the effect that a detection limit of 175 ppb would have on the daily  $\text{NH}_3$  flux rates measured and calculated with the DTM. In the underestimation scenario,  $\text{NH}_3$  mixing ratios above the soil surface were assumed to be around the detection limit of 175 ppb at constant wind speeds for 12 h during the day. No  $\text{NH}_3$  fluxes were assumed during the night. This  
290 number was divided by the  $\beta$ -coefficient of 1.36 from the detection sensitivity experiment and converted to an observed mixing ratio of 126 ppb. Average wind speed levels were set starting at  $0.1 \text{ m s}^{-1}$  and then matching the upper limits of the Beaufort scale, ranging from calm to gentle breeze. They were capped at  $4 \text{ m s}^{-1}$ , since that is the upper limit for which the DTM was calibrated for (Pacholski et al., 2006). In addition, the temperature was kept constant at  $20 \text{ }^\circ\text{C}$  and the air pressure at 1013 hPa. The same conditions plus an undetectable elevated background mixing ratio of 175 ppb were assumed for the overestimation.  
295 The DTM flux rate  $F_{\text{DTM}}$  (in  $\text{kg N ha}^{-1}$ ) was calculated according to Pacholski et al. (2006) as follows:

$$F_{\text{DTM}} = \text{volume} \cdot \text{lconc.l} \cdot 10^{-9} \cdot \rho_{\text{NH}_3} \cdot U_{\text{N}} \cdot U_{\text{F}} \cdot U_{\text{Z}} \quad (5)$$

Where volume is the air volume sucked through the chambers, in this case 5 l;  $\text{lconc.l} \cdot 10^{-9}$  is the mixing ratio of  $\text{NH}_3$  in ppb as was displayed in the Dräger Tubes, in this case 630 ppb for 5 l;  $\rho_{\text{NH}_3}$  is the temperature-dependent density of  $\text{NH}_3$  in  $\text{kg l}^{-1}$ ;  $U_{\text{N}}$  is the molecular weight conversion factor of  $\text{NH}_3$  to N;  $U_{\text{F}}$  is the surface area conversion factor from the chamber  
300 surface area of  $415 \text{ cm}^2$  to  $\text{ha}$ ;  $U_{\text{Z}}$  is the time conversion factor from seconds to days. Finally, the calibrated flux rate  $F_{\text{cal}}$  was calculated by incorporating wind speed  $\nu$  according to the following equation:

$$F_{\text{cal}} = \exp(0.444 \cdot \ln(F_{\text{DTM}}) + 0.59 \cdot \ln(\nu)) \quad (6)$$



**Table 1.** Possible underestimation of daily  $\text{NH}_3$  fluxes assuming constant wind speeds during a 12 h daily period and if the  $\text{NH}_3$  mixing ratio at the ground surface is 175 ppb, making it undetectable by the DTM, and overestimation assuming background mixing ratios are also 175 ppb and also undetectable.

Wind speed in $\text{m s}^{-1}$	Beaufort scale	Wind description	Underestimation of daily $\text{NH}_3$ flux in $\text{kg N ha}^{-1} \text{ d}^{-1}$	Overestimation of daily $\text{NH}_3$ flux in $\text{kg N ha}^{-1} \text{ d}^{-1}$
0.1	0	Calm	0.04	0.06
0.2	0	Calm	0.06	0.09
1.5	1	Light air	0.21	0.29
3.3	2	Light breeze	0.34	0.46
4	3	Gentle breeze	0.38	0.51

It can be seen that a detection limit of 175 ppb could either lead to an underestimation of the  $\text{NH}_3$  flux of 0.04–0.67  $\text{kg N ha}^{-1} \text{ d}^{-1}$  or an overestimation of 0.06–0.92  $\text{kg N ha}^{-1} \text{ d}^{-1}$ . If these numbers were applied to an emission factor of 15 % for urea (Asman, 1992), this would lead to a daily relative error of between -0.4...-4.2 % or +0.4...+5.7 % for an application rate of 60  $\text{kg N ha}^{-1}$ . If, on the other hand, these figures were applied to a fertilizer with a low  $\text{NH}_3$  emission factor, such as calcium ammonium sulphate with an emission factor of 2 % (Asman, 1992), this would lead to a daily relative total error of between -3.3...-31.7 % or +5.0...+42.5 % for an application rate of 60  $\text{kg N ha}^{-1}$ . The total mean relative error range of the calibration function 6 given by (Pacholski et al., 2006) is  $17 \pm 5$  %. This relative error range would be exceeded at the former emission factor and average wind speeds of 1.5  $\text{m s}^{-1}$  after at least seven days, and at the latter emission factor after just one day during measurements below the detection limit. The use of the DTM should therefore only be considered if other measurement alternatives are not feasible and if high  $\text{NH}_3$  fluxes are to be expected during the entire measurement campaign. Therefore, when combined with passive samplers, it was recommended to use the DTM with a high emission source for measurements of absolute emissions (Pacholski, 2016). A similar method to the DTM that could be considered for such comparisons is the dositube method (van An del et al., 2017). It uses an  $\text{NH}_3$  detector tube similar to the DTM, but instead places the tube directly into a semi-open chamber and allows it to passively absorb the  $\text{NH}_3$  over a longer period of time. The advantages over the DTM would be less manpower and a longer time-weighted average of  $\text{NH}_3$  loss. This would allow detection of lower flux rates. The dositube method showed good agreement in  $\text{NH}_3$  loss estimates when compared to wind tunnel measurements but has not yet been validated with a micrometeorological or mass balance method. In a recent comparative study by Kamp et al. (2024), the calibrated DTM also underestimated emissions compared to micrometeorological measurements while wind tunnel measurement tended to overestimate emissions. Between micrometeorological methods final emission varied by 30 %. The error evaluation in Table 1 assumes the calibration is accurate and unbiased. To fully validate this approach, the calibration itself must also be tested. Consequently, additional comparative measurements are required for a more comprehensive and conclusive assessment of the calibrated DTM.



#### 325 4.2 Influence of tubing material and tubing temperature on NH<sub>3</sub> response time

The response time was longest in both heated and unheated Synflex tubing for both increasing and decreasing NH<sub>3</sub> mixing ratios. The response time was shortest in heated PTFE tubing, although we could not find a significant reduction in response time between heated and unheated tubing and between PTFE and PU. Whitehead et al. (2008) on the other hand was able to find a reduction in response time for heated PTFE tubing. However, they measured the response time at lower NH<sub>3</sub> mixing ratios, a much shorter measurement interval of 300 seconds and with a Quantum Cascade Laser Absorption Spectrometer, which has a resolution of up to 10 Hz, which might together contribute to the differences in results. The lower sample size of 3 might have also caused a possible false negative in the results. It was also difficult to keep NH<sub>3</sub> levels constant between comparisons, but they did not differ by more than 20 %. On the other hand, Shah et al. (2006) could not find a significant difference in NH<sub>3</sub> adsorption to other plastic tubing materials at air flow rates of 10 l min<sup>-1</sup> either.

#### 335 4.3 Chamber system modifications during outdoor measurements

In both the unchanged and PU tubing chamber system, the linear model of the DTM was able to predict MGA<sup>7</sup> measurements with the highest coefficient of determination, followed by PTFE coated chamber, and finally by chambers wiped with ethanol. The unchanged chamber system also had the highest beta coefficient out of the four trials, closely followed by PU tubing, then PTFE coating, and finally wiping with ethanol. Continuing to use unchanged chamber systems is therefore the best choice out of the four options. While PU tubing performed similarly to PTFE tubing and is less expensive, PTFE tubing is well known for its low water absorption and low permeability to gases and moisture vapor (Harper, 2000). The advantage of the lower cost of PU is negligible in the case of the DTM because the total length of tubing does not exceed 3 m. However, it is recommended that the PTFE tubing be replaced periodically because degradation over time is known to increase response time and increase losses of gases such as H<sub>2</sub>O (Lee et al., 1991; Whitehead et al., 2008).

345 Wiping the inner surface of the chamber with ethanol reduced the performance of the chamber system. Dry wiping of the chamber surfaces is therefore preferred. The lower performance compared to the MGA<sup>7</sup> is likely due to the fact that the ethanol did not completely evaporate from the surface during the Dräger Tube measurements, while the ethanol from the chamber system used for the MGA<sup>7</sup> completely or mostly evaporated during the 30 min measuring period. The use of a PTFE sheet for the inner chamber surface also decreased the detection sensitivity. A halocarbon wax coating could be used instead of a PTFE film for future testing, as it was found that a halocarbon wax coating of a stainless steel surface was able to improve the travel time of NH<sub>3</sub> to a similar level as PTFE, even at lower temperatures (Yokelson et al., 2003). It is also worth exploring whether active passivation of the chamber surface and inner tubing surface with 1H,1H-perfluorooctylamine could similarly enhance the sensitivity of Dräger Tubes, since Roscioli et al. (2016) discovered a reduction in response time from 30 to 2 s of their Dual Quantum Cascade Laser instrument for 90 % NH<sub>3</sub> recovery.



## 355 5 Conclusions

This paper evaluated the detection accuracy, precision, and sensitivity of DTM  $\text{NH}_3$  measurements and explored potential chamber system improvements. It was found that the Dräger Tubes used for the DTM were underestimating the measured concentrations, had decreasing detection accuracy at lower mixing ratios, and had higher detection limits in the range of 152-205 ppb than initially assumed. The use of the DTM is therefore unsuitable for measurements on low  $\text{NH}_3$  emitting  
360 (acidic) soils, under low temperature conditions, with low  $\text{NH}_3$  emitting N fertilizers such as calcium ammonium nitrate or fertilizers combined with inhibitors, and for experiments with low N application rates. However, the use of DTM can still be considered in field experiments where high emissions are expected and other more reliable alternatives are not feasible. Unfortunately, there are no feasible alternatives for small plot  $\text{NH}_3$  measurements yet, as wind tunnels are prone to errors and are difficult to translocate to different fields. The development of similar chamber or easy-to-use measurement methods that  
365 are inexpensive, mobile, and have a low detection limit is therefore encouraged. Detection accuracy, precision, and sensitivity should be compared with high-precision real-time measurement techniques such as cavity ring-down spectroscopy or direct laser absorption spectroscopy. Further assessment of the calibrated DTM in comparison reference method involving also the calibration approach is desirable for a comprehensive and conclusive evaluation of this measurement approach. A similar method to the DTM, the dositube method (van Andel et al., 2017), showed potential advantages and could be considered for  
370 comparisons.

This study also identified options that should be excluded or used in the development of a new chamber method. Dry wiping of the chambers should be preferred over the use of ethanol. The use of an external heating source in combination with PTFE could improve response times for  $\text{NH}_3$  measurements and could be implemented for outdoor use of open dynamic chamber systems. However, the additional use of heating wires around the tubing would require careful preparation of the tubing and an  
375 additional portable power supply, which would complicate handling and limit the mobility of the chamber system.

*Data availability.* All the data and R scripts used in this work can be accessed from: <https://doi.org/10.26165/JUELICH-DATA/0LAIFH>

## Appendix A



**Table A1.** NH<sub>3</sub> measuring devices used during the experiments.

Device	Company	Measurement technique
Dräger-Tube: Ammonia 0.25/a	<b>Drägerwerk AG &amp; Co. KGaA</b> Moislinger Allee 53-55 23558 Lübeck Germany	bromophenol blue pH-indicator
MGA <sup>7</sup>	<b>MIRO Analytical AG</b> Widenholzstrasse 1 CH-8304 Wallisellen Switzerland	direct laser absorption spectroscopy
G2103	<b>Picarro, Inc.</b> 3105 Patrick Henry Dr. Santa Clara, CA 95054 USA	cavity ring-down spectroscopy





**Table A2.** Tubing material used during the experiments.

Tubing material	Company	Product number	Diameter
PTFE	<b>CS - Chromatographie Service GmbH</b> Am Parir 27 (Gewerbegebiet) 52379 Langerwehe Germany	198026-01	outer diameter: 6.35 mm inner diameter: 4.3 mm
Polyester-polyurethane	<b>Landefeld Druckluft und Hydraulik GmbH</b> Konrad-Zuse-Straße 1 34123 Kassel-Industriepark Germany	PUN 1/4 SCHWARZ	outer diameter: 6.35 mm inner diameter: 4.2 mm
Synflex 1300	<b>Megaflex Limited</b> Old Rectory Landercross Bideford Devon EX39 5JA United Kingdom	DEK1/4	outer diameter: 6.35 mm inner diameter: 4.3 mm
PTFE	<b>Landefeld Druckluft und Hydraulik GmbH</b> Konrad-Zuse-Straße 1 34123 Kassel-Industriepark Germany	TFL 8X6 NATUR	outer diameter: 8 mm inner diameter: 6 mm
Polyester-polyurethane	<b>Landefeld Druckluft und Hydraulik GmbH</b> Konrad-Zuse-Straße 1 34123 Kassel-Industriepark Germany	PU 8X6 NATUR	outer diameter: 8 mm inner diameter: 6 mm



**Table A3.** Material used for the unmodified chamber system.

Device/Material	Company	Product number	Specs
PTFE tubing	<b>Landefeld Druckluft und Hydraulik GmbH</b> Konrad-Zuse-Straße 1 34123 Kassel-Industriepark Germany	TFL 8x6 NATUR	outer diameter: 8 mm diameter: 6 mm
Stainless steel chambers	<b>Metallindustriewerk Heinr. Hofmann GmbH</b> Seekoppelweg 6 24113 Kiel Germany	“V2A-Ringe 1.5 mm stark”	custom made
Stainless steel soil rings	<b>Metallindustriewerk Heinr. Hofmann GmbH</b> Seekoppelweg 6 24113 Kiel Germany	“V2A-Kammersystem pieces”	custom made
Y push in fitting	<b>Landefeld Druckluft und Hydraulik GmbH</b> Konrad-Zuse-Straße 1 34123 Kassel-Industriepark Germany	IQSY 80	8 mm diameter: 6 mm
Hose clamps	<b>Carl Roth GmbH + Co. KG</b> Schoemperlenstr. 3-5 76185 Karlsruhe Germany	AEH1.1	outer diameter: 8–12 mm
Dräger X-act® 5000 Basic	<b>Drägerwerk AG &amp; Co. KGaA</b> Moislinger Allee 53-55 23558 Lübeck Germany	Dräger X-act® 5000 Basic	
Dräger Accuro hand pump	<b>Drägerwerk AG &amp; Co. KGaA</b> Moislinger Allee 53-55 23558 Lübeck Germany	Dräger Accuro	
Deluxe tube opener Dräger	<b>Drägerwerk AG &amp; Co. KGaA</b> Moislinger Allee 53-55 23558 Lübeck Germany	Dräger TO 7000	



**Table A4.** Other material and devices used.

Device/Material	Company	Product number	Specs
Checktemp® 1 digital thermometer	<b>Hanna Instruments Deutschland GmbH</b> An der Alten Ziegelei 7 89269 Vöhringen Germany	HI98509	
Soil moisture sensor	<b>IMKO Micromodultechnik GmbH</b> Am Reutgraben 2 D-76275 Ettlingen Germany	TRIME PICO 64	
Soil moisture logger	<b>IMKO Micromodultechnik GmbH</b> Am Reutgraben 2 D-76275 Ettlingen Germany	HD2	
All in one weather station	<b>Campbell Scientific Ltd.</b> Fahrenheitstraße 13 28359 Bremen Germany	ClimaVUE50	
Weather data logger	<b>Campbell Scientific Ltd.</b> Fahrenheitstraße 13 28359 Bremen Germany	CR300	
MIRO Field Enclosure	<b>MIRO Analytical AG</b> Widenholzstrasse 1 CH-8304 Wallisellen Switzerland		
Heating wire	<b>Dennerle GmbH</b> Industriestr. 4 66981 Münchweiler/Rodalb Germany	Dennerle Eco-Line ThermoTronic	20 W
ArmaFlex	<b>Armacell GmbH</b> Robert-Bosch-Straße 10 48153 Münster Germany	ArmaFlex AF-2-012	inner diameter: 12 mm insulation thickness: 13 mm
Virginal PTFE Sheet	<b>Hightechflon GmbH &amp; Co. KG</b> Macairestr. 4 78467 Konstanz Germany	PTFE.SFL.005.VIR	thickness: 0.05 mm



*Author contributions.* AK, MC and NB designed the experiments and AK and MC carried them out. AK wrote the first version of the manuscript, did the formal analysis and created the figures. MC installed and wrote the section on the laboratory setup, assisted with the  
380 MGA<sup>7</sup> measurements, and provided advice on the experimental design. NB gave advice on performing the experiment and the statistical analysis, formulated the research idea, acquired the funding and helped with the planning and execution of the experiment. All authors reviewed and revised the manuscript.

*Competing interests.* The authors declare that they have no conflict of interest.

*Disclaimer.* The project was supported by funds of the German Federal Government's Special Purpose Fund held at Landwirtschaftliche  
385 Rentenbank under grant no. 894 820.

*Acknowledgements.* We want to thank Muhammad Humza for their contribution to the execution of the experiments described in this paper. Their assistance was instrumental in the completion of this research.



## References

- Asman, W. A.: Ammonia emission in Europa: Upyearly emission and emission variations, Tech. rep., National Institute of Public Health and Environmental Protection, <http://hdl.handle.net/10029/258542>, 1992.
- 390 Behera, S. N., Sharma, M., Aneja, V. P., and Balasubramanian, R.: Ammonia in the Atmosphere: A Review on Emission Sources, Atmospheric Chemistry and Deposition on Terrestrial Bodies, *Environ. Sci. Pollut. R.*, 20, 8092–8131, <https://doi.org/10.1007/s11356-013-2051-9>, 2013.
- Bouwman, A., Boumans, L., and Batjes, N.: Estimation of global NH<sub>3</sub> volatilization loss from synthetic fertilizers and animal manure applied to arable lands and grasslands, *Global Biogeochem. Cy.*, 16, 1–11, <https://doi.org/10.1029/2000gb001389>, 2002.
- 395 Cameron, K., Di, H., and Moir, J.: Nitrogen losses from the soil/plant system: A review, *Ann. Appl. Biol.*, 162, 145–173, <https://doi.org/10.1111/aab.12014>, 2013.
- Di Perta, S. E., Fiorentino, N., Carozzi, M., Cervelli, E., and Pindozi, S.: A Review of Chamber and Micrometeorological Methods to Quantify NH<sub>3</sub> Emissions from Fertilisers Field Application, *Int. J. Agron*, 2020, 1–16, <https://doi.org/10.1155/2020/8909784>, 2020.
- 400 Drägerwerk AG: Dräger-Tube Handbook - Soil, Water and Air Investigations as Well as Technical Gas Analysis, Tech. rep., Drägerwerk Aktiengesellschaft Lübeck, ISBN 3926762063, 2011.
- EU Directive: Directive (EU) 2016/2284 of the European Parliament and of the Council of 14 December 2016 on the reduction of national emissions of certain atmospheric pollutants, <https://eur-lex.europa.eu/eli/dir/2016/2284/oj>, 2016.
- European Environment Agency: European Union emission inventory report 1990–2021 under the UNECE convention on long-range trans-boundary air pollution (air convention), Tech. rep., Publications Office of the European Union, <https://doi.org/10.2800/68478>, 2023.
- 405 Fogg, P. C.: Solubility of gases in liquids : A critical evaluation of gas/liquid systems in theory and practice, Wiley, 1 edn., ISBN 0471929255, 1991.
- Gericke, D., Pacholski, A., and Kage, H.: Measurement of Ammonia Emissions in Multi-Plot Field Experiments, *Biosyst. Eng.*, 108, 164–173, <https://doi.org/10.1016/j.biosystemseng.2010.11.009>, 2011.
- 410 Harper, C. A.: Modern plastics handbook, McGraw Hill Professional, 1 edn., ISBN 0070267146, 2000.
- Kamp, J. N., Hafner, S. D., Huijsmans, J., van Boheemen, K., Götze, H., Pacholski, A., and Pedersen, J.: Comparison of two micrometeorological and three enclosure methods for measuring ammonia emission after slurry application in two field experiments, *Agr. Forest Meteorol.*, 354, 110 077, <https://doi.org/10.1016/j.agrformet.2024.110077>, 2024.
- Lee, J. H., Chen, Y., and Tang, I. N.: Heterogeneous Loss of Gaseous H<sub>2</sub>O<sub>2</sub> in an Atmospheric Air Sampling System, *Environ. Sci. Technol.*, 25, 339–342, <https://doi.org/10.1021/es00014a019>, 1991.
- 415 Lelieveld, J., Evans, J., Fnais, M., Giannadaki, D., and Pozzer, A.: The contribution of outdoor air pollution sources to premature mortality on a global scale, *Nature*, 525, 367–371, <https://doi.org/10.1038/nature15371>, 2015.
- Lim, S. S., Vos, T., Flaxman, A. D., Danaei, G., and Shibuya, K. et al.: A comparative risk assessment of burden of disease and injury attributable to 67 risk factors and risk factor clusters in 21 regions, 1990–2010: a systematic analysis for the Global Burden of Disease Study 2010, *Lancet*, 380, 2224–2260, [https://doi.org/10.1016/S0140-6736\(12\)61766-8](https://doi.org/10.1016/S0140-6736(12)61766-8), 2012.
- 420 MIRO Analytical: Single Device for Monitoring of All Greenhouse Gases & Pollutants, Comparison with Other Methods, Tech. rep., MIRO Analytical AG, 2021.
- Ni, K., Köster, J. R., Seidel, A., and Pacholski, A.: Field Measurement of Ammonia Emissions after Nitrogen Fertilization—A Comparison between Micrometeorological and Chamber Methods, *Eur. J. Agron.*, 71, 115–122, <https://doi.org/10.1016/j.eja.2015.09.004>, 2015.



- 425 Pacholski, A.: Calibrated passive sampling - Multi-plot field measurements of NH<sub>3</sub> emissions with a combination of dynamic tube method and passive samplers, *J. Visualized Exp.*, p. 1–15, <https://doi.org/10.3791/53273>, 2016.
- Pacholski, A., Cai, G., Nieder, R., Richter, J., Fan, X., Zhu, Z., and Roelcke, M.: Calibration of a simple method for determining ammonia volatilization in the field - Comparative measurements in Henan Province, China, *Nutr. Cycl. Agroecosys.*, 74, 259–273, <https://doi.org/10.1007/s10705-006-9003-4>, 2006.
- 430 Quakernack, R., Pacholski, A., Techow, A., Herrmann, A., Taube, F., and Kage, H.: Ammonia volatilization and yield response of energy crops after fertilization with biogas residues in a coastal marsh of Northern Germany, *Agr. Ecosyst. Environ.*, 160, 66–74, <https://doi.org/10.1016/j.agee.2011.05.030>, 2012.
- Rees, R., Roelcke, M., Li, S., Wang, X., Li, S., Stockdale, E., McTaggart, I., Smith, K., and Richter, J.: The effect of fertilizer placement on nitrogen uptake and yield of wheat and maize in Chinese loess soils, *Nutr. Cycl. Agroecosys.*, 47, 81–91, <https://doi.org/10.1007/BF01985721>, 1996.
- 435 Richter, J.: Zur Methodik des Bodengashaushaltes. II. Ergebnisse und Diskussion, *Z. Pflanzenernähr. Bodenkd.*, 132, 220–239, <https://doi.org/10.1002/jpln.19721320306>, 1972.
- Roelcke, M.: Die Ammoniak-Volatilisation nach Ausbringung von Mineraldünger-Stickstoff in carbonatreichen chinesischen Löss-Ackerböden, Ph.D. thesis, ISBN 3884527487, 1994.
- 440 Roelcke, M., Li, S., Tian, X., Gao, Y., and Richter, J.: In situ comparisons of ammonia volatilization from N fertilizers in Chinese loess soils, *Nutr. Cycl. Agroecosys.*, 62, 73–88, <https://doi.org/10.1023/A:1015186605419>, 2002.
- Roscioli, J. R., Zahniser, M. S., Nelson, D. D., Herndon, S. C., and Kolb, C. E.: New Approaches to Measuring Sticky Molecules: Improvement of Instrumental Response Times Using Active Passivation, *J. Phys. Chem. A*, 120, 1347–1357, <https://doi.org/10.1021/acs.jpca.5b04395>, 2016.
- 445 Shah, S. B., Grabow, G. L., and Westerman, P. W.: Ammonia adsorption in five types of flexible tubing materials, *Appl. Eng. Agric.*, 22, 919–923, 2006.
- Sintermann, J., Neftel, A., Ammann, C., Häni, C., Hensen, A., Loubet, B., and Flechard, C. R.: Are ammonia emissions from field-applied slurry substantially over-estimated in European emission inventories?, *Biogeosciences*, 9, 1611–1632, <https://doi.org/10.5194/bg-9-1611-2012>, 2012.
- 450 Svensson, L. and Ferm, M.: Mass Transfer Coefficient and Equilibrium Concentration as Key Factors in a New Approach to Estimate Ammonia Emission from Livestock Manure, *J. Agr. Eng. Res.*, 56, 1–11, <https://doi.org/10.1006/jaer.1993.1056>, 1993.
- van Andel, M., Warland, J., Zwart, P., Van Heyst, B., and Lauzon, J.: Development of a simple and affordable method of measuring ammonia volatilization from land applied manures, *Can. J. Soil Sci.*, 97, 541–551, <https://doi.org/10.1139/cjss-2016-0103>, 2017.
- Wang, H., Zhang, D., Zhang, Y., Zhai, L., Yin, B., Zhou, F., Geng, Y., Pan, J., Luo, J., Gu, B., and Liu, H.: Ammonia emissions from paddy fields are underestimated in China, *Environ. Pollut.*, 235, 482–488, <https://doi.org/10.1016/j.envpol.2017.12.103>, 2018.
- 455 Wang, J., Yin, Q., Tong, S., Ren, Z., Hu, M., and Zhang, H.: Prolonged continuous exposure to high fine particulate matter associated with cardiovascular and respiratory disease mortality in Beijing, China, *Atmos. Environ.*, 168, 1–7, <https://doi.org/10.1016/j.atmosenv.2017.08.060>, 2017.
- Whitehead, J. D., Twigg, M., Famulari, D., Nemitz, E., Sutton, M. A., Gallagher, M. W., and Fowler, D.: Evaluation of laser absorption spectroscopic techniques for eddy covariance flux measurements of ammonia, *Environ. Sci. Technol.*, 42, 2041–2046, <https://doi.org/10.1021/es071596u>, 2008.
- 460



- Yang, Y., Ni, X., Liu, B., Tao, L., Yu, L., Wang, Q., Yang, Y., Liu, J., and Wu, Y.: Measuring field ammonia emissions and canopy ammonia fluxes in agriculture using portable ammonia detector method, *J. Clean. Prod.*, 216, 542–551, <https://doi.org/10.1016/j.jclepro.2018.12.109>, 2019.
- 465 Yokelson, R. J., Christian, T. J., Bertschi, I. T., and Hao, W. M.: Evaluation of adsorption effects on measurements of ammonia, acetic acid, and methanol, *J. Geophys. Res.-Atmos.*, 108, 1–9, <https://doi.org/10.1029/2003JD003549>, 2003.
- Zhang, X., Gu, B., van Grinsven, H., Lam, S. K., Liang, X., Bai, M., and Chen, D.: Societal benefits of halving agricultural ammonia emissions in China far exceed the abatement costs, *Nat. Commun.*, 11, 1–10, <https://doi.org/10.1038/s41467-020-18196-z>, 2020.