

Towards a high quality in-situ observation network for oxygenated volatile organic compounds (OVOCs) in Europe: transferring traceability to the International System of Units (SI) to the field

Maitane Iturrate-Garcia¹, Thérèse Salameh², Paul Schlauri³, Annarita Baldan⁴, Martin K. Vollmer³,
5 Evdokia Stratigou², Sebastian Dusanter², Jianrong Li⁴, Stefan Persijn⁴, Anja Claude⁵, Rupert Holzinger⁶,
Christophe Sutour⁷, Tatiana Macé⁷, Yasin Elshorbany⁸, Andreas Ackermann¹, Céline Pascale¹, Stefan
Reimann³

¹ Department of Chemical and Biological Metrology, Federal Institute of Metrology (METAS), Bern-Wabern, 3003, Switzerland

10 ² IMT Nord Europe, Institute Mines-Télécom, Univ. Lille, Centre for Energy and Environment, F-59000 Lille, France

³ Laboratory for Air Pollution and Environmental Technology, Empa, Swiss Federal Laboratories for Materials Science and Technology, Dübendorf, 8600, Switzerland

⁴ VSL-National Metrology Institute, Delft, 2629 JA, the Netherlands

⁵ Meteorologisches Observatorium Hohenpeissenberg, Deutscher Wetterdienst (DWD), 82383 Hohenpeissenberg, Germany

15 ⁶ Institute for Marine and Atmospheric Research, IMAU, Utrecht University, Utrecht, the Netherlands

⁷ Department of Gas Metrology, Laboratoire National de Métrologie et d'Essais – LNE, Paris CEDEX 15, 75724, France

⁸ School of Geosciences, College of Arts & Sciences, University of South Florida, Florida, USA

Correspondence to: Maitane Iturrate-Garcia (maitane.iturrate@metas.ch)

Abstract. Volatile organic compounds (VOCs) have a large impact on the oxidising capacity of the troposphere and are major
20 precursors of tropospheric ozone and secondary atmospheric aerosols. Accurate measurements and data comparability of
VOCs among monitoring networks are essential to assess the trends of these secondary air pollutants. Metrological traceability
of the measurements to the international system of units (SI-traceability) contributes to both: measurement consistency and
data comparability. Accurate, stable and SI-traceable reference gas mixtures (RGMs) and working standards are needed to
achieve SI-traceability through an unbroken chain of calibrations of the analytical instruments used to monitor VOCs.
25 However, for many oxygenated VOCs (OVOCs), such RGMs and working standards are not available at atmospheric amount
of substance fraction levels ($< 10 \text{ nmol mol}^{-1}$). Here, we present the protocols developed to transfer SI-traceability to the field
by producing two types of SI-traceable working standards for selected OVOCs. These working standards, based on RGMs
diluted dynamically with dry nitrogen and on certified spiked whole air samples, were then assessed using Thermal Desorption -
Gas Chromatography-Flame Ionization Detector (TD-GC-FID) and Proton Transfer Reaction-Time of Flight-Mass
30 Spectrometry (PTR-ToF-MS) as analytical methods. For that purpose, we calibrated five analytical instruments using in-house
calibration standards and treated the new SI-traceable working standards as samples. Due to analytical limitations, the
assessment was only possible for acetaldehyde, acetone, methanol and methyl ethyl ketone (MEK). Relative differences
between assigned and measured values were used to assess the working standards based on dilution of RGMs. The relative
differences were within the measurement uncertainty for acetone, MEK, methanol and acetaldehyde at amount of substance

35 fractions around 10 nmol mol^{-1} . For the working standards based on certified spiked whole air samples in pressurized cylinders, results showed a good agreement among the laboratories (i.e., differences within the measurement expanded uncertainties (U) ranging between $0.5 \text{ nmol mol}^{-1}$ and $3.3 \text{ nmol mol}^{-1}$) and with the certified amount of substance fraction value for acetaldehyde ($15.7 \text{ nmol mol}^{-1} \pm 3.6 \text{ (U) nmol mol}^{-1}$), acetone ($17 \text{ nmol mol}^{-1} \pm 1.5 \text{ (U) nmol mol}^{-1}$) and MEK ($12.3 \text{ nmol mol}^{-1} \pm 2.3 \text{ (U) nmol mol}^{-1}$). Despite the promising results for the working standards based on the dilution of RGMs and on certified spiked
40 whole air samples filled into pressurized cylinders, the assessment must be considered with care due to the large measurement uncertainty, particularly for methanol. Active collaboration among metrological, meteorological and atmospheric chemistry monitoring communities is needed to tackle the challenges of OVOC monitoring, such as the lack of stable and SI-traceable calibration standards (i.e., RGMs and working standards). Besides from this collaboration, other research applications, such as modelling and remote sensing, may benefit from the transfer of SI-traceability to monitoring stations.

45

Keywords

Calibration, metrological traceability, uncertainty, VOCs, tropospheric ozone, reference gas mixtures, GC-FID, PTR-MS

1 Introduction

Tropospheric ozone plays a key role in the oxidative capacity of the atmosphere (Iglesias-Suarez et al., 2018; Monks et al.,
50 2015; Schultz et al., 2015) ~~through different chemical reactions, such as~~ ~~Despite its relatively low atmospheric abundance and short lifetime (20–25 days or even lower) (Young et al., 2013),~~ ~~ozone photodissociation, which~~ is the dominant source of hydroxyl radical (OH) in the troposphere (e.g., Lelieveld and Dentener, 2000; Zhang et al., 2014). Besides being a strong oxidant with direct impact on human respiratory health, vegetation growth and crop productivity (Van Dingenen et al., 2009; Schultz et al., 2017; Mills et al., 2018), tropospheric ozone is also a greenhouse gas and a secondary air pollutant (Gaudel et
55 al., 2018; Szopa et al., 2023). In the troposphere, ozone abundance depends on its transport from the stratosphere, formation and destruction through photochemical reactions and dry deposition (Cooper et al., 2014; Fleming et al., 2018; Jacob, 2000; Stohl et al., 2003; Wild, 2007). Volatile organic compounds (VOCs) – a group of chemical compounds with one or more atoms of carbon and a complex speciation that encompasses thousands of species (Goldstein and Galbally, 2007; Yang et al., 2016) – are one of the major tropospheric ozone precursors (Shao et al., 2009; Xue et al., 2014; Simon et al., 2015). VOC oxidation
60 in the presence of significant amount of substance fractions of nitrogen oxides (NO_x) results in a net production of ozone (Collins et al., 2002; Pugliese et al., 2014).

Oxygenated VOCs (OVOCs) are an important fraction of VOCs, which includes alcohols, carbonyls (aldehydes and ketones) and carboxylic acid (Legreid et al., 2007; Wu et al., 2020). OVOCs are precursors of tropospheric ozone and secondary organic aerosols and have, thus, an impact on air quality and climate (Boucher et al., 2013; Seinfeld et al., 2016; Shrivasta et al., 2017).
65 OVOCs can be formed by atmospheric photooxidation of hydrocarbons (Atkinson, 2000) and can be emitted directly from vegetation, biomass burning, vehicle exhaust and industrial processes (Placet, 2000; Legreid et al., 2007; Worton et al., 2022).

OVOCs with low molecular weights (e.g., methanol, acetone, acetaldehyde, methyl ethyl ketone (MEK)) are found at relatively high amount of substance fractions in the global atmosphere and play an important role in the tropospheric photochemistry. For these OVOCs, the main sinks are the oxidation with the OH radicals and degradation initiated by photolysis leading to the formation of hydrogen oxide radicals (HO_x). For example, oxidation products of methanol are formaldehyde and CO (Bates et al., 2021; Hu et al., 2011), which also impact the oxidation capacity of the troposphere. Acetone, acetaldehyde and MEK are oxidised to peroxy radicals that react with NO_2 to form peroxyacetyl nitrate (PAN), which is an important precursor of tropospheric ozone (Millet et al., 2010; Fischer et al., 2012; Khan et al., 2015; Wang et al., 2019) and can lead to the transport of radicals and NO_2 over long distances. Production of radicals (e.g., OH, HO_x) and PAN further affect the chemistry of the tropospheric ozone (Volkamer et al., 2010; Fischer et al., 2014; Tan et al., 2019; Brewer et al., 2020; Zborowska et al., 2021). Therefore, accurate OVOC monitoring is crucial to assess tropospheric ozone burdens, trends and variability.

The Tropospheric Ozone Assessment Report – Phase I (TOAR-I) identified uncertainties associated to ozone precursors' emissions, including VOCs, as one of the main contributors to the uncertainty of modelled spatial and temporal distribution of ozone (Young et al., 2018). Long-term accurate measurements of ozone precursors are required to reduce the uncertainties of their emissions. This need of accurate measurements was also highlighted in TOAR-I as part of the scientific tasks, goals and requirements for tropospheric ozone monitoring (Tarasick et al., 2019). Other programs and infrastructures for atmospheric monitoring emphasises the importance of monitoring VOCs, particularly OVOCs, because of their active role and impact on chemistry of the atmosphere, air quality and climate change. The World Meteorological Organisation Global Atmosphere Watch (WMO-GAW) programme has listed methanol, ethanol, acetone and formaldehyde as part of reactive gas compounds to be monitored (Schultz et al., 2015). The European Aerosol, Clouds and Trace Gases Research Infrastructure (ACTRIS) (Laj et al., 2024) – through its Centre for Reactive Trace Gases In Situ Measurements (CiGas) – includes OVOCs as one of the four compound clusters to be monitored, together with non-methane hydrocarbons, condensable vapours and NO_x (Hoerger et al., 2015; Simon et al., 2023). Metrological traceability of the measurements, ideally to the International System of Units (SI), is essential to guarantee data comparability among the different monitoring networks (Brewer et al., 2018; Güttler and Richter, 2009; Worton et al., 2023).

Metrological traceability is achieved through an unbroken chain of calibrations, each contributing to the uncertainty of measurements (De Bièvre and Taylor, 1997). One way of ensuring SI-traceability is to calibrate analytical instruments, which are used to monitor atmospheric compounds, against a primary reference material produced by a National Metrology Institute (NMI). NMIs prepare these materials following reference procedures, provide complete uncertainty budgets of the assigned values, ensure their stability period, and participate in international comparisons with other NMIs to achieve SI-traceability (Brewer et al., 2018). However, for certain reactive compounds, such as many OVOCs (e.g., methanol, ethanol), producing reference material is particularly challenging because of surface, non-linearity and matrix effects, as well as because of stability issues and the low amount of substance fractions (at nmol mol^{-1} level) required (Grenfell et al., 2010; Leuenberger et al., 2015; Persijn and Baldan, 2023; Rhoderick et al., 2019).

100 SI-traceable reference gas mixtures (RGMs) have been developed at NMIs for an increasing number of OVOCs in the last
decade (e.g., Brown et al., 2013; Worton et al., 2023). Nevertheless, RGMs are only available at higher amount of substance
fractions than atmospheric ones (Rhoderick et al., 2019; Worton et al., 2022). When monitoring atmospheric OVOCs, these
higher amount fractions imply that RGMs must be diluted at monitoring stations before calibrating the analytical instruments.
Depending on the dilution procedure, SI-traceability might be lost because of inadequate dilutions (e.g., using dilution devices
105 such as thermal mass flow controllers, whose calibration is not SI-traceable). Another issue faced by OVOC monitoring
stations regarding these RGMs is that the matrix gas of the mixture is not the same as ambient air. Quite often, nitrogen is used
as matrix gas to ensure the inertness of OVOCs like acetaldehyde. The use of dry nitrogen instead of humidified synthetic air
may influence the calibration results. The lack of SI-traceability and long-term stability of OVOC RGMs produced at low
amount fraction levels are other limitations that often have negative effects particularly on long-term OVOC measurements.
110 All these aspects have an impact on data comparability and thus on OVOC trend identification.

Here we present the efforts done between the metrological and atmospheric monitoring communities to transfer SI-
traceability to the field. For that purpose, protocols to produce two types of SI-traceable working standards – based on dynamic
dilution of RGMs with dry nitrogen and on certified spiked whole air samples – of selected OVOCs were developed and
assessed. OVOCs were selected in close collaboration with stakeholders (e.g., WMO-GAW, ACTRIS) based on their relevance
115 for atmospheric and climate research, on their role as tropospheric ozone precursors and on the lack of accurate, stable and SI-
traceable calibration standards. The selected OVOCs were acetaldehyde, acetone, ethanol, methacrolein, methanol, methyl
ethyl ketone (MEK) and methyl vinyl ketone (MVK). The amount of substance fractions of the produced working standards
were as close as technically feasible to the ambient air amount of substance fractions ($< 10 \text{ nmol mol}^{-1}$). In this work, we used
the quantity amount of substance fraction (a.k.a. amount fraction) – the accepted metrological ~~accepted~~ term (Matschat et al.,
120 2023; Richter, 2007) – instead of concentration and/or mixing ratio. We expressed this quantity in SI units of nmol mol^{-1} ,
which can be considered equivalent to part per billion (ppb) under tropospheric conditions (Galbally et al., 2013).

2 Traceable Working standards based on dynamic dilution of reference gas mixtures traceable to the international system of units (SI)

125 Two types of SI-traceable OVOC working standards were prepared and assessed in this work (Fig. 1): working standards based
on the dynamic dilution of SI-traceable reference gas mixtures and working standards based on certified spiked whole air
samples. While for the former a dilution step was needed before assessment, the latter was assessed directly without further
dilution. The target amount fraction of each OVOC (acetaldehyde, acetone, ethanol, methacrolein, methanol, MEK and MVK)
was 10 nmol mol^{-1} or lower, to be as close as possible to the OVOC ambient levels. The assessment of the SI-traceable working
standards was performed using several analysers based on two analytical techniques (Fig. 1; Appendix A): Thermal
130 Desorption-Gas Chromatography-Flame Ionization Detector (TD-GC-FID) and Proton Transfer Reaction-Time of Flight-Mass

Spectrometry (PTR-ToF-MS). The analysers were calibrated with the participants' in-house working standards (Appendix D.1). The SI-traceable working standards were treated as samples.

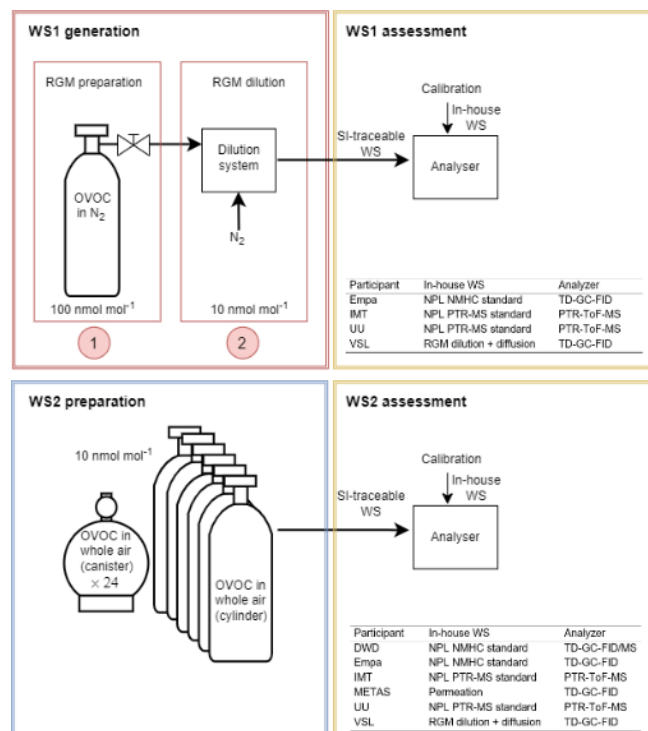


Figure 1: Scheme showing the two types of working standards traceable to the international system of units (SI) prepared in this work, based on the dilution of reference gas mixtures (RGM) of oxygenated volatile organic compounds (OVOC) in nitrogen (N₂) (WS1; for details, see section 2.1) and on certified spiked whole air samples (WS2; for details, see section 2.2). Participants in the assessment, analysers (thermal desorption (TD)-gas chromatography (GC)-flame ionization detector (FID) and proton transfer reaction (PTR)-Time of Flight (ToF)-mass spectrometry (MS) systems) and in-house working standards used to calibrate them are indicated.

The first type of SI-traceable working standards developed was based on the dilution of SI-traceable RGMs containing the selected OVOCs at amount fractions slightly higher than in the atmosphere (ca. 100 nmol mol⁻¹). However, the target amount fraction of the SI-traceable working standards was 10 nmol mol⁻¹ or lower. Thereby, RGMs were diluted using two dilution systems, both calibrated against national primary standards. Dry nitrogen of high purity (≥ 99.99990 %) was used as matrix and dilution gas to prevent any possible reaction (e.g., oxidation) of OVOCs. The potential presence of water and OVOCs in the matrix and the dilution gas was assessed following standard procedures (ISO 19229:2019, 2019).


2.1 Generation of SI-traceable working standards based on dynamic dilution of reference gas mixtures

The first type of SI-traceable working standards developed was based on the dilution of SI-traceable RGMs containing the selected OVOCs at amount fractions slightly higher than in the atmosphere (of ca. 100 nmol mol⁻¹). However, To achieve the

150 10 nmol mol⁻¹ or lower target amount fraction of the SI-traceable working standards was 10 nmol mol⁻¹ or lower. Thereby, dynamic dilution of the produced RGMs was needed (Fig. 1). ~~ere diluted using two dilution systems, both calibrated against national primary standards.~~ Dry nitrogen of high purity (> 99.99990 %) was used as matrix and dilution gas to prevent any possible reaction (e.g., oxidation) of OVOCs. The potential presence of water and OVOCs in the matrix and the dilution gas was assessed following standard procedures (ISO 19229:2019, 2019).

2.1.1 Gravimetric preparation of RGMs

155 Four RGMs of OVOCs in dry, high-purity (> 99.99990 %) nitrogen (BIP+ Built-in-Purifier, Air Products Inc., PA, USA) were prepared at VSL, the National Metrology Institute (NMI) of the Netherlands, in August 2021. For that purpose, the primary gravimetric method was used by means of a high-resolution mass comparator (ISO 6142-1:2015, 2015). In this method, pure liquid compounds are injected in high-pressure gas cylinders. Prior to the injection, the purity of the selected liquid OVOCs was analysed (Appendix B.1, Table B1). ~~Prior to the injection, the purity of the liquid OVOCs was analysed (ISO 19229:2019, 2019) using a gas chromatographic (GC) system (6890, Agilent Technologies Inc., CA, USA) with a mass spectrometer (MS) and a flame ionization detector (FID). A GS GASPRO capillary column (60 m length, 0.32 mm internal diameter and 0.25 µm film thickness; Agilent Technologies Inc., CA, USA) was used for these measurements. For acetaldehyde, it was not possible to perform the purity analysis because of the physical properties of the liquid chemical, which made its handling difficult. The water content in the liquid OVOCs was determined by the Karl Fischer titration (Coulometric KF titrator, Metrohm).~~

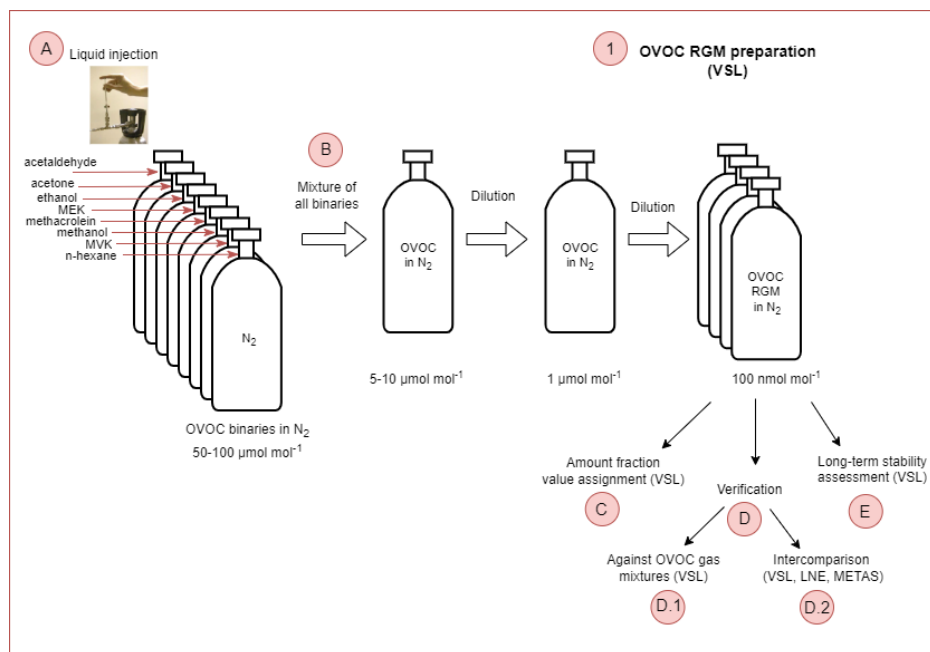

165 **Figure 2: Schematic diagram illustrating the steps needed to prepare the reference gas mixtures (RGMs) of the selected oxygenated volatile organic compounds (OVOCs).**

A. Liquid OVOC injection

Known amounts of the pure liquid OVOCs were injected in high-pressure gas cylinders to obtain binary gas mixtures at around 50–100 $\mu\text{mol mol}^{-1}$ in a first step (Fig. 2-A). Besides the injected OVOCs, n-hexane was added as internal standard to assess RGM stability (Table B1). The injected OVOCs were acetaldehyde (Acros Organics™, PA, USA; purity 99.9 %), acetone (Sigma Aldrich, MA, USA; purity ≥ 99.99 %), ethanol (Merck KGaA, Germany; purity ≥ 99.99 %), methacrolein (MACR; Thermo Fisher Scientific Inc., PA, USA; 98.5 %), methanol (Sigma Aldrich®, MO, USA; purity 99.99 %), methyl ethyl ketone (MEK; Acros Organics™, PA, USA; purity 99.9 %) and methyl vinyl ketone (MVK; Acros Organics™, PA, USA; purity 97 %). Prior to the injection, the purity of the liquid OVOCs was analysed (ISO 19229:2019, 2019) using a gas chromatographic (GC) system (6890, Agilent Technologies Inc., CA, USA) with a mass spectrometer (MS) and a flame ionization detector (FID). A GS-GASPRO capillary column (60 m length, 0.32 mm internal diameter and 0.25 μm film thickness; Agilent Technologies Inc., CA, USA) was used for these measurements. For acetaldehyde, it was not possible to perform the purity analysis because of the physical properties of the liquid chemical, which made its handling difficult. The water content in the liquid OVOCs was determined by the Karl Fischer titration (Coulometric KF titrator, Metrohm).

Besides the selected OVOCs, n-hexane (Merck KGaA, Germany; purity ≥ 99.0 %) was injected as internal standard to assess RGM stability.

B. Mixture of binaries and further dilution

Then, the binary gas mixtures were combined and further diluted to obtain OVOC RGMs at nominal amount fractions around 100 nmol mol^{-1} and at a pressure of 12 MPa (Fig. 2-B). The RGMs were prepared in 10 L aluminium cylinders (Luxfer Inc., CA, USA) with an Experis® proprietary treatment (Air Products Inc., PA, USA) and a low dead-volume stainless steel cylinder valve D304 (Rotarex, Luxemburg).

C. -Amount fraction value assignment

RGM amount fraction value assignment was based on gravimetry, with exception of methanol and ethanol. For these compounds, the value was assigned by analysis against dynamically prepared OVOC RGMs. Metrological traceability of the gravimetric RGMs was ensured by mass weighing and purity determination, while for methanol and ethanol, by mass weighing, volume and purity determination.

D. and ~~v~~ Verification

D.1. Verification against OVOC gas mixtures

RGM amount fraction value assignment was based on gravimetry, with exception of methanol and ethanol. For these compounds, the value was assigned by analysis against dynamically prepared OVOC RGMs. Metrological traceability of the

~~gravimetric RGMs was ensured by mass weighing and purity determination, while for methanol and ethanol, by mass weighing, volume and purity determination.~~

After preparation (between end of August and mid-September 2021), RGMs were verified against OVOC gas mixtures that contained acetone, ethanol, methacrolein, methanol, MVK and MEK and were generated by a diffusion method (ISO 6145-8:2005, 2005). ~~Other dynamic preparation methods: For acetaldehyde, continuous syringe injection (ISO 6145-4:2004, 2004) and dynamic dilution of a RGM at high amount fraction (ISO 6145-7:2018, 2018) were used for acetaldehyde.~~ The verification process was ~~performed by VSL (Appendix B.2.1), repeated three times using VSL thermal desorption (TD) GC-FID described in Appendix A. The RGMs were connected to an autosampler built by VSL, sharing therefore the same pressure reducer. Lines and pressure reducer were coated (SilcoNert® 2000). To guarantee the same sampling conditions (20 mL min⁻¹ sampling flow during 15 minutes, total volume 300 mL at 293 K and 101.3 kPa) for gravimetric and dynamically prepared RGMs, the mass flow controller (MFC) of the thermal desorber was operated in light vacuum mode by means of a pump. Each gas mixture was analysed 20 times.~~ For each compound, a response factor was calculated according to Eq. (1), which was used to estimate the compound amount fraction in the gravimetric RGM following Eq. (2). RGM verification was based on the evaluation of the relative difference between the calculated amount fraction and the gravimetric value.

$$RF_i = \frac{(\bar{A}_{cal_i} - \bar{A}_{0i})}{x_{cal_i}} \quad (1)$$

where,

RF_i : compound i response factor

\bar{A}_{cal_i} : average peak area of compound i in the calibration standard (last five replicates)

\bar{A}_{0i} : average peak area of compound i in the blanks (last five replicates)

x_{cal_i} : amount fraction of compound i in the calibration standard

$$x_i = \frac{(\bar{A}_i - \bar{A}_{0i})}{RF_i} \quad (2)$$

where,

x_i : estimated amount fraction of compound i in the sample

\bar{A}_i : average peak area of compound i in the RGM (last five replicates)

\bar{A}_{0i} : average peak area of compound i in the blanks (last five replicates)

RF_i : response factor of compound i calculated according to Eq. (1)

D.2. Interlaboratory comparison

~~A comparison between three laboratories took place to complete the RGM amount fraction verification. During this interlaboratory comparison (Appendix B.2.2), one of the verified VSL RGMs (VSL221418) was analysed at VSL and at the~~

NMIs of France (LNE) and Switzerland (METAS) between January and April 2022 using the analytical methods described in Table B3.

E. Long-term stability assessment

In order to assess the long-term stability of the RGMs, repeated analysis with two to three measurement series ~~Four additional analyses~~ were performed 5 months, 7 months, 13 months and 18 months after preparation ~~to assess the long-term stability of the RGMs. In each period, two to three series of measurements were performed.~~ Relative differences between averaged measured values for each period and gravimetric values were used as an indicator of temporal stability. ~~Furthermore, a comparison between three laboratories took place to complete the RGM amount fraction verification. During this interlaboratory comparison (Appendix B.4), one of the verified VSL RGMs (VSL221418) was analysed at VSL and at the NMIs of France (LNE) and Switzerland (METAS) between January and April 2022 using the analytical methods described in Table B4.~~

2.1.3 Uncertainty of the RGMs

The uncertainty of the RGMs, provided together with the assigned value of the amount fraction of each OVOC, was evaluated after the verification and long-term stability assessment. Preparation and verification uncertainty sources were considered to estimate the uncertainty of the RGMs based on the measurement model proposed in ISO 6142-1:2015 (2015). Regarding the preparation sources, uncertainties from weighing, molar masses ([Coplen et al., 2020](#); [van der Veen et al., 2021](#)) and the purity of the materials used was propagated using the law of uncertainty propagation (JCGM 100:2008, 2008). The uncertainty was evaluated using an in-house made software based on the work described in Alink and Van Der Veen (2000). Uncertainty sources linked to RGM verification included the repeatability of each series of measurements and the spread among the series of measurements. A Student's t-test was used to determine whether the mean difference between a average analytical observed values and gravimetric values was significant. When significant, the uncertainty ~~of the recovery~~ due to initial loss was included in the uncertainty evaluation (Eq. (3)).

$$u_c = \frac{1}{2} \cdot \sqrt{u^2(\text{prep}) + u^2(\text{ver}) + u^2(\text{reeloss})} \quad (3)$$

where,

u_c : combined uncertainty of the amount fraction of the compound

$u(\text{prep})$: gravimetric preparation standard uncertainty

$u(\text{ver})$: analytical verification standard uncertainty

$u(\text{reeloss})$: standard uncertainty ~~of the recovery~~ due to initial loss

An additional term was added to the combined uncertainty of the RGMs sent around for SI-working standard assessment (VSL221420 and VSL221421) to account for potential temporal instabilities during the shipment period. The expanded uncertainty was then calculated as the combined uncertainty multiplied by the coverage factor ($k = 2$).

2.1.2 RGM Dilution systems

SI-traceable ~~W~~working standards containing OVOCs at atmospheric amount fractions (10 nmol mol^{-1}) were ~~prepared~~ generated by diluting the described RGMs with clean and dry nitrogen using two different dilution systems (Fig. 1). Both dilution systems were warmed up for at least 24 hours and flushed with zero gas (i.e., dry high-purity nitrogen) to prevent presence of water or any other contaminant, before the preparation of working standards.

The first dilution system was developed by VSL and consisted of one-stage gas dilution with dilution flows ranging 2–50 L min^{-1} , allowing dilution ratios up to 1:1000 (Appendix A.2). ~~Flows of the RGM (0.1 L min^{-1}) and of the dilution gas (nitrogen, AP BIP Plus grade 6.0) were accurately controlled using three MFCs (EL FLOW® Select series, Bronkhorst, Netherlands), operating up to 10 L min^{-1} and 25 L min^{-1} . The dilution system was mostly built in inert glass. Other materials in contact with the OVOC gas mixtures were PTFE, 316 SS (small surfaces) or coated 316 SS (SilcoNert® 2000, SilcoTek, PA, USA). A coated (SilcoNert® 2000) pressure regulator was connected to the RGMs and flushed thoroughly before attaching it to the dilution system. For the purpose of this assessment, the MFCs were set and calibrated using two mercury piston prover volumeters (Bronkhorst, Netherlands), which were in turn calibrated at the VSL Flow Department, at working ranges of $0\text{--}0.5 \text{ L min}^{-1}$ and $0\text{--}10 \text{ L min}^{-1}$. Temperature and pressure were measured by equipment calibrated at the VSL Temperature and Pressure Department to convert flow to standard temperature and pressure (STP) conditions (293.15 K , 101.3 kPa). This dilution system was used only during the working standard assessment performed by VSL.~~

The second dilution system – referred to as "VeRDi" (Versatile Reactive Gas Diluter) and developed by METAS in collaboration with Swagelok® Switzerland – was a two-stage gas dilutor allowing dilution ratios up to 1:175000 (Appendix A.2). This dilution system was transferred to the institutes assessing the SI-traceable working standards except to VSL. ~~The main components of this two-stage gas dilution system were four MFCs (two MFCs up to 0.1 L min^{-1} (Red-y, Vögtlin Instruments, GmbH, Switzerland) and two MFCs up to 5 L min^{-1} (Sensirion AG, Switzerland)), two pressure controllers (Bronkhorst High Tech B.V., Netherlands), a valve terminal (MPA-L, Feste Beteiligungen GmbH & Co. KG, Germany) and a vacuum pump. Elements in contact with RGM flow were coated (SilcoNert® 2000), including all the stainless steel tubing of $1/4$ " internal diameter used to build VeRDi. The tubes were welded, instead of joined through fittings, in order to reduce dead volumes and potential leaks. MFCs and pressure regulators were calibrated using clean and dry nitrogen against METAS primary standards to ensure traceability of the dilution. The software controlling VeRDi was developed in LabVIEW (National Instruments, Austin, TX).~~

~~Both dilution systems were warmed up for at least 24 hours and flushed with zero gas (i.e., dry high-purity nitrogen) to prevent presence of water or any other contaminant, before the preparation of working standards.~~

2.23 Preparation of SI-Traceable working standards based on certified spiked whole air samples

The second type of SI-traceable working standards developed consisted ~~on~~of certified whole air samples that were previously spiked with the selected OVOCs to obtain amount fractions around 10 nmol mol^{-1} . A schematic of the steps given to prepare these SI-traceable working standards is shown in Figure 3.

295

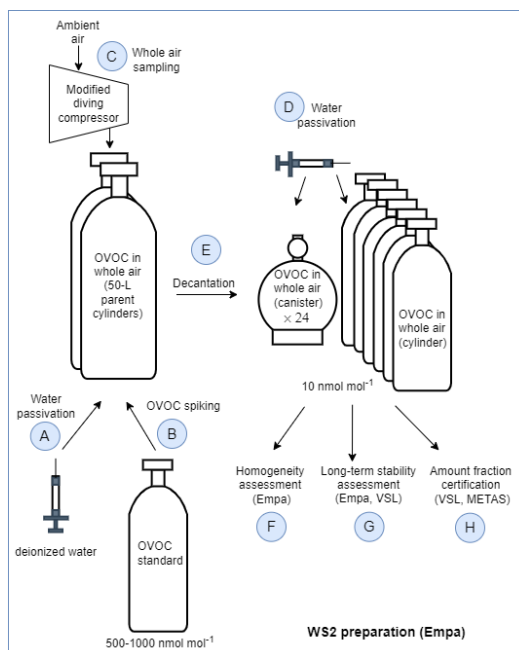


Figure 3: Schematic diagram illustrating the steps needed to prepare the SI-traceable working standard based on certified spiked whole air samples (WS2).

3.1 Air sampling and vessel filling

300

A. Water passivation of the parent cylinders

Two 50 L aluminium cylinders (parent cylinders) were selected ~~to be and~~ filled with ambient air by the Swiss Federal Laboratories for Materials Science and Technology (Empa). Before filling ~~them, the parent cylinders were spiked with water to passivate their inner walls with a layer of water to reduce adsorption and surface reactions of the compounds of interest.~~ ~~First,~~ both cylinders were evacuated in parallel for one hour (cylinder pressure < 10 hPa) with a membrane pump. Then, ~~to passivate their inner walls with a layer of water to reduce adsorption and surface reactions of the compounds of interest,~~ 0.73 mL of deionized water (Merck Millipore, Germany) was injected individually in each parent cylinder at Empa on 31 March 2021.

305

B. OVOC spiking

310

OVOC spiking was done using a high-pressure cylinder containing an SI-traceable RGM of OVOCs in dry high-pure nitrogen (VSL, Netherlands) at amount fraction levels between $500 \text{ nmol mol}^{-1}$ and $1000 \text{ nmol mol}^{-1}$ (Table C1). This SI-traceable

~~RGM was connected to. The OVOC spiking was performed by connecting the parent cylinders to the SI traceable RGM~~ via a ~~1/4"~~ cross connector (~~Swagelok Co., OH, USA~~) and a vacuum pump fitted with an on/off valve to isolate the pump from the cylinders. The spiking took place at Empa ~~on 21 April 2021~~ three weeks after the water passivation of the parent cylinders.

315 Both, water and OVOC spiking were carried out at room temperature.

C. Whole air sampling

320 ~~One day~~ After ~~after~~ the spiking, the two parent cylinders were filled with ambient air at the National Air Pollution Monitoring Network (NABEL) station at "Rigi Seebodena lp" (ca. 1000 m above sea level; Switzerland) on 22 April 2021. The filling was done using a modified diving compressor (RIX Industries, SA-6). The compressor air inlet was about 2 m above ground and placed upwind of the compressor. Both cylinders were filled in parallel during three hours to a final pressure of ca. 145 bar. After the sampling and once back in the laboratory, the parent cylinders were stored tilted (ca. 30° inclination) over night with the top facing downward. Then, the two parent cylinders were taken outdoors and stored for another hour at ambient temperature (10 °C) vertically upside down, before the valves were opened to release the liquid water that was potentially formed during the filling. Since each the spiking and air filling took place with the two parent cylinders connected in parallel, it was assumed that OVOC amount fractions in both cylinders were identical (Table C1).

D. Water passivation of cylinders and canisters

330 Six cylinders and 24 canisters (Table C2) were selected for decanting the parent cylinders to produce several identical subsamples (i.e., working standards). Prior to decanting, the working standard cylinders and canisters were spiked with water – following the same procedure described for the parent cylinders – to achieve a 20 % water saturation level.

E. Filling of cylinders and canisters (decantation)

335 The parent and working standard cylinders, as well as the canisters, were placed in a climate chamber at 40 °C for at least three hours to ensure thermal equilibration before decanting. The interconnecting tubing was kept as short as possible and several tanks of the same type were filled simultaneously. After decanting the parent cylinders, the absolute pressure ranges in the working standard cylinders and canisters were 9.9–10.5 MPa and 0.38–0.41 MPa, respectively.

~~3.2 Certification of the spiked whole air samples~~

F. Homogeneity assessment

340 The homogeneity of the spiked air samples was evaluated before certification (Table C3). For that purpose, seven whole air samples in different vessel types and the two parent cylinders after decantation were analysed three times using Empa GC-FID described in Appendix A.1. The obtained amount fractions were averaged and the variations within the same vessel type and among different vessel types were calculated.

345 **G. Long-term stability assessment**

Furthermore, during the certification process, the long-term temporal stability of the whole air samples in the cylinders was assessed by repeated measurements after 2 months, 8 months and 14 months. Variations due to temporal instability were included in the certified values.

350 **H. Certification of the spiked whole air samples**

Certification measurements were carried out by VSL and METAS using the two analytical methods described in Table C3-C4 and following the same measurement protocol (Appendix C). Each whole air sample was analysed at least six times. In total, three series of measurements for whole air samples in cylinders were performed, but only one measurement series for the samples in canisters was possible due to the limited sample volume. The amount fraction of each compound per whole air sample was calculated according to Eq. (2). The uncertainty of the assigned amount fraction values included the main uncertainty sources of the sample analysis – such as spread of the analyser response, background noise, blank issues, potential overlapping of GC peaks and detector drift among others – and the uncertainty of the analyser calibration (i.e., uncertainty of the RGMs and possible lack of linearity in the measured range: 0–10 nmol mol⁻¹) (Appendix C). The consistency of the assigned amount fraction values for acetone, ethanol, methacrolein, methanol and MVK measured in the same type of vessel was evaluated according to the criterion described by Eq. (4).

$$|x_{VSL} - x_{METAS}| \leq k \cdot \sqrt{u_{VSL}^2 + u_{METAS}^2} \quad (4)$$

where,

x_{VSL} : amount fraction value of each OVOC under study assigned by VSL

x_{METAS} : amount fraction value of each OVOC under study assigned by METAS

365 k : coverage factor ($k = 2$)

u_{VSL} : standard uncertainty of the amount fraction value assigned by VSL according to Eq. (C1)

u_{METAS} : standard uncertainty of the amount fraction value assigned by METAS according to Eq. (C1)

Certified reference values for each type of vessel were assigned only when the criterion (Eq. (4)) was met for all OVOCs in the same type of vessel. In this case, the certified reference value of each OVOC was the average of VSL and METAS assigned values for that compound. The relative uncertainty of the certified reference values was the combined uncertainty of the assigned values provided by VSL and METAS, including the spread of the assigned values due to potential temporal instability (one year period).

4 Assessment of the SI-traceable working standards

375 4.1 Measurement procedure

The SI-traceable working standards were assessed by comparing them against in-house working standards ([Appendix D.1](#)), which were used for routine [analyser](#) calibrations by the participants in the assessment ([Fig. 1](#)): [Deutscher Wetterdienst \(DWD\)](#), [Empa](#), [Institute Mines-Télécom \(IMT\)](#), [METAS](#), [Utrecht University \(UU\)](#) and [VSL](#) ([Table 2](#)). For that purpose, ~~the selected analysers (Table A1) were calibrated using the in-house working standards (Appendix D.1) at different amount fraction levels between March and November 2022.~~ The SI-traceable working standards were treated as samples and analysed following the same procedure as for the analyser calibration. The detailed analytical method, calibration standards and measurement procedure to assess both types of SI-traceable working standards are described in [Appendix D](#).

~~The assessment of working standards based on the dilution of RGMs with dry nitrogen (Table 1) was performed by the Institute Mines-Télécom (IMT), VSL, Utrecht University (UU) and Empa. The measurement sequence consisted of the measurement of dry pure nitrogen samples to estimate the blank of the system, followed by the measurement of samples prepared by dynamic dilution of RGMs, which were analysed among the in-house standards.~~

~~To assess the SI working standards based on certified spiked whole air samples, the same air sample cylinders were measured by the participants in the round robin comparison: Deutscher Wetterdienst (DWD), IMT, VSL, UU and Empa. However, different canisters were sent to the participants because of the low sample volume, which was enough only for one analysis (Table C2). After some blank measurements, in-house working standards were assessed at a minimum of two amount fraction levels between 1 nmol mol⁻¹ and 16 nmol mol⁻¹. Samples were measured between in-house working standards. After the second calibration amount fraction level, blank measurements were performed again.~~

Table 42: Information on the assessment of working standards (WS) based on dilution of RGMs with dry nitrogen (WS1) and on certified spiked whole air samples (WS2). ECN refers to the effective carbon number. [Detailed information on WS2 samples is shown in Table C2.](#)

Participant	Dates	WS	Samples (assessed WS)	In-house WS*	Analytical method
IMT	Jun. 2022	WS1	RGM VSL221421 + VeRD _i	NPL PTR-MS standard	PTR-ToF-MS
VSL	Aug. 2022	WS1	RGM VSL221419 + VSL dilutor	VSL diffusion standard	TD-GC-FID
UU	Sep./Oct. 2022	WS1	RGM VSL221421 + VeRD _i	NPL PTR-MS standard	PTR-ToF-MS
Empa	Nov. 2022	WS1	RGM VSL221420 + VeRD _i	NPL NMHC standard + ECN	TD-GC-FID
METAS	Feb. 2022	WS2	001C cyl, 002A cyl, 003A can, 004A can, 004B can, 005E can, 006B can, 007A can, 008A can	METAS permeation standard	TD-GC-FID
DWD	Mar. 2022	WS2	001B cyl, 002B cyl, 003B can, 005D can, 008B can	NPL NMHC standard	TD-GC-FID/MS

<u>IMT</u>	<u>Jun. 2022</u>	<u>WS2</u>	<u>001B cyl, 002B cyl, 003B can, 004C can, 006C can</u>	<u>NPL PTR-MS standard</u>	<u>PTR-ToF-MS</u>
<u>VSL</u>	<u>Jul. 2021/Aug. 2022</u>	<u>WS2</u>	<u>001A cyl, 002A cyl, 003A can, 005B can, 005C can, 006D can, 007B can, 008D can</u>	<u>VSL diffusion standard</u>	<u>TD-GC-FID</u>
<u>UU</u>	<u>Sep. 2022</u>	<u>WS2</u>	<u>001B cyl, 002B cyl, 003B can, 004D can, 007C can,</u>	<u>NPL PTR-MS standard</u>	<u>PTR-ToF-MS</u>
<u>Empa</u>	<u>Nov. 2022</u>	<u>WS2</u>	<u>001B cyl, 002B cyl, 003B can, 004E can, 005A ccan, 006A can, 007D can, 008C can</u>	<u>NPL NMHC standard + ECN</u>	<u>TD-GC-FID</u>

^aAll the in-house working standards were SI-traceable except for the effective carbon number (ECN)

~~The assessment of working standards based on the dilution of RGMs with dry nitrogen (Table 1) was performed by the Institute Mines Télécom (IMT), VSL, Utrecht University (UU) and Empa. The measurement sequence consisted of the measurement of dry pure nitrogen samples to estimate the blank of the system, followed by the measurement of samples prepared by dynamic dilution of RGMs, which were analysed among the in-house standards.~~

~~To assess the SI-working standards based on certified spiked whole air samples, the same air sample cylinders were measured by the participants in the round-robin comparison (Table 2): Deutscher Wetterdienst (DWD), IMT, VSL, UU and Empa. However, different canisters were sent to the participants because of the low sample volume, which was enough only for one analysis (Table C2). After some blank measurements, in-house working standards were assessed at a minimum of two amount fraction levels between 1 nmol mol⁻¹ and 16 nmol mol⁻¹. Samples were measured between in-house working standards. After the second calibration amount fraction level, blank measurements were performed again.~~

410 4.2 Working standard amount fractions and uncertainty

4.2.1 Measured amount fractions and uncertainties

The measured amount fractions of the SI-traceable working standards were calculated using different equations depending on the analytical method and the calibration standard used.

415 VSL estimated the amount fractions of the SI-traceable working standards based on the dilution of RGMs with dry nitrogen according to Eq. (2), using only the last five measurements for the calculations. Uncertainty of these measured amount fractions was calculated following Eq. (B+C1).

DWD and Empa followed ACTRIS procedures to estimate the OVOC measured amount fractions and their uncertainties (Reimann et al., 2018). The main uncertainty sources considered by DWD and Empa were the reproducibility of the measurement method (i.e., standard deviation of the multiple measurements of the sample) and measurements close to limit of

420 ~~detection, the uncertainty of the in-house working standard (i.e., calibration standard). Sources linked to the uncertainty of the~~
~~instrument (peak integration uncertainty due to peak overlay, tailing and/or bad peak separation, sampling line artefacts, carry~~
~~over and changes of split flow rates) were considered in the standard deviation of the multiple calibration measurements. For~~
~~OVOCs that were no present in the NPL NMHC standard (Grenfell et al., 2010), Empa used the effective carbon number~~
425 ~~calibration using an NPL NMHC standard (Grenfell et al., 2010) as the in-house standard. This assessment procedure led to~~
~~measurement results. The ECN was the only in-house standard used in this assessment that are not metrologically traceable,~~
~~was not SI-traceable. In addition to the sources of uncertainty described above for DWD and Empa, other uncertainties~~
~~considered in this approach were. The uncertainty of the estimated amount fraction was the combination of the standard~~
~~deviation of the multiple measurements of the sample,~~ the mean relative deviation of the NPL NMHC standard certified
430 uncertainties of the six compounds (ethane, ethene, propane, propene, isobutane and butane) contributing to the carbon
response factor (CRF) and the relative standard deviation of the six calculated CRFs. ~~Uncertainty sources linked to the~~
~~uncertainty of the instrument (sampling line artefacts, carry over and changes of split flow rates) were considered in the~~
~~standard deviation of the multiple calibration measurements.~~

IMT estimated the amount fractions of the selected OVOCs according to the calibration approach described in de Gouw and
435 Warneke (2007) ~~(Appendix D.4)~~. The combined measurement uncertainty, $u(x_i)$, was calculated as the square root of the sum
of quadrats of each relative uncertainty term ~~(Appendix D.4)~~. Sources of uncertainty associated to the measured amount
fractions included precision of the system and calibration accuracy ~~(Appendix D.4)~~.

UU followed the method described in Holzinger et al. (2019) to estimate the OVOC amount fractions. The uncertainty of the
measured amount fractions was given as the standard deviation of 4–6 repetitions of the same measurement type.

440

4.2.2 Assigned amount fractions and uncertainty

For the SI-traceable working standards based on the dilution of RGMs with dry nitrogen, the assigned amount fraction of each
sample was estimated according to Eq. (5).

$$x_{th} = \frac{(x_{RGM} \cdot q_{v_RGM} + x_{res} \cdot q_{v_dil})}{(q_{v_RGM} + q_{v_dil})} \quad (5)$$

445 where,

x_{th} : assigned amount fraction of the generated SI-traceable working standard (in nmol mol⁻¹)

x_{RGM} : amount fraction of the OVOC under study in the diluted VSL RGM (in nmol mol⁻¹)

x_{res} : amount fraction of the OVOC under study present as residual in the dilution gas (in nmol mol⁻¹)

q_{v_RGM} : flowrate of VSL RGM (in mL min⁻¹)

450 q_{v_dil} : flowrate of the dilution gas (in mL min⁻¹)

The uncertainty of the assigned values was calculated following the law of uncertainty propagation (JCGM 100:2008, 2008) according to Eq. (6). Calculations were done using GUM Workbench Pro version 2.4.1.406 (Metrodata GmbH, Germany).

$$455 \quad u(x_{th}) = \sqrt{[c_1 \cdot u(x_{RGM})]^2 + [c_2 \cdot u(q_{v_RGM})]^2 + [c_3 \cdot u(x_{res})]^2 + [c_4 \cdot u(q_{v_dil})]^2} \quad (6)$$

where,

$u(x_{th})$: uncertainty of the assigned amount fraction of the generated SI-traceable working standard

$u(x_{RGM})$: uncertainty of the VSL RGM used in the comparison (provided in the calibration certificate according to Eq. (3))

$u(q_{v_RGM})$: uncertainty of VSL RGM flow rate

460 $u(q_{v_dil})$: uncertainty of the dilution gas flow rate

$u(x_{res})$: uncertainty due to the presence of the compound under study in the dilution and matrix gas as impurity

c_1 : sensitivity coefficient given by the partial derivative of x_{th} respect x_{RGM}

c_2 : sensitivity coefficient given by the partial derivative of x_{th} respect q_{v_RGM}

c_3 : sensitivity coefficient given by the partial derivative of x_{th} respect x_{res}

465 c_4 : sensitivity coefficient given by the partial derivative of x_{th} respect q_{v_dil}

Assigned amount fractions and uncertainty of the workings standards based on certified spiked whole air samples were estimated following the procedure described for the air sample certification (in Appendix C). The relative expanded uncertainty of the certified reference values was two times the combined uncertainty of the assigned values provided by VSL and METAS, including the spread of the assigned values due to potential temporal instability (one year period) (Eq. (C1)).

4.2.3 Relative differences between working standards

The assessment of the SI-traceable working standards based on the dilution of RGMs with dry nitrogen was done by calculating the relative difference between the measured and assigned amount fractions described above-, while for the SI-traceable working standards based on certified spiked whole air samples, the relative difference between the measured and the certified amount fractions was calculated.

The expanded uncertainty of each assessment was calculated as two times the combined uncertainty (u_{diff}) between the uncertainty of the theoretical assigned (Table D1) or certified (Table 3) amount fraction ($u(x_{th})$) and the uncertainty of the measured amount fraction $u(x_i)$ reported by the participants (Table D2 and Table D3) for each compound (Eq. (7)).

$$480 \quad u_{diff} = \sqrt{u^2(x_{th}) + u^2(x_i)} \quad (7)$$

~~Measured amount fractions of the SI-traceable working standards based on air samples were compared against the certified OVOC amount fraction values provided by VSL and METAS.~~

5 Results

485 ~~Results regarding the amount fraction assignment and verification of the RGMs used to generate the SI-traceable working standards based on the dilution of RGMs and of the assessment of these working standards are shown in this section, together with the certification and assessment results of the SI-traceable working standards based on certified spiked whole air samples.~~

5.1 ~~Results of the SI-traceable working standards based on dilution of RGMs~~

5.1.1 ~~RGM amount fraction assignment and, verification and stability evaluation~~

490 RGM amount fractions were assigned gravimetrically taking into consideration the purity of the liquid chemicals injected into the cylinders and results from the mass weighing during the preparation. Results showed purity values > 99.9 % for all the liquid compounds, except for methacrolein (98.5 %) and MVK (94.0 %). Water was a common impurity in all the liquid compounds. For methacrolein, MVK and MEK, other organic impurities were found (Table B1). Values of the assigned gravimetric amount fractions ranged between 98 nmol mol⁻¹ and 105 nmol mol⁻¹ with expanded uncertainties of the preparation
495 ≤ 5 % (coverage factor $k = 2$) in general (Table 32). However, greater uncertainties were calculated for methanol (5.3 % in VSL221419 and 6.8 % in VSL221420), acetaldehyde (9.6 % in VSL221420 and 9.5 % in VSL221421) and MVK (5.8 % in VSL221421) to take into account initial losses and potential instability of these compounds in the cylinders.

Table 23: Gravimetric assigned amount fraction values (x_i) for the reference gas mixtures (RGMs) and their expanded uncertainty (U) with a coverage factor of two ($k = 2$)

RGM code	$x_i \pm U$ [nmol mol ⁻¹]						
	acetaldehyde	acetone	ethanol	methacrolein	methanol	MEK	MVK
VSL221418	103.1 ± 2.6	98.1 ± 1.6	98.0 ± 2.4	100.7 ± 1.6	98.0 ± 3.4	100.2 ± 1.8	101.8 ± 3.0
VSL221419	101.9 ± 2.1	99.3 ± 2.2	99.2 ± 3.2	99.6 ± 2.5	99.2 ± 5.3	99.1 ± 2.5	100.7 ± 4.3
VSL221420	103.3 ± 9.6	97.9 ± 4.4	93.3 ± 3.8	101.0 ± 4.2	99.8 ± 6.8	100.4 ± 3.9	102.1 ± 3.6
VSL221421	101.2 ± 9.5	99.9 ± 3.6	96.6 ± 5.0	99.0 ± 4.1	105.1 ± 5.0	98.4 ± 3.4	100.0 ± 5.8


500

Results from the verification analysis (Table B2), where the prepared RGMs were compared against dynamically generated gas mixtures, showed similar relative differences between analytical and gravimetric values for acetone in the four cylinders (average difference < +0.54 %). These results, similar to the relative differences found for the internal standard (n-hexane), suggest that surface effects (i.e., adsorption losses) were negligible for both compounds. For MEK, the analytical values were
505 also greater than the gravimetric ones and quite similar among different cylinders (average difference < +3.2 %). Lower analytical values than gravimetric ones were found for acetaldehyde, methacrolein and MVK. Average differences were < +2

510 % and similar among different cylinders for acetaldehyde and methacrolein, which suggests minimal or even negligible adsorption effects with the cylinder wall. The difference was higher for MVK (between -2.5 % and 3.7 %), which might be explained not only by surface effects but also by isomerization reactions. All the relative differences were within the expanded uncertainty of the verification analysis. The relative differences for ethanol were around -5 %. Compound loss after preparation due to surface effects might explain ~~these relative differences of around -5 % for ethanol.~~ Initial losses were also suggested by the great heterogeneity among cylinders for methanol (relative difference between -5.2 % and +3.1 %) like described in Persijn and Baldan (2023).

515 ~~Long-term stability results (Table B3) suggested very good stability (i.e., relative differences between analytical and gravimetric values smaller than $\pm 5\%$) for acetone with relative differences $\leq +2\%$ even 13–14 months after RGM preparation, although a questionable result (-4.7 %) was obtained at a stability testing period of 18–19 months. Acetone results were similar to those for the internal standard (n-hexane). A good stability was also found for methacrolein. After initial relative differences of ca. -1.5 %, positive values around +0.7 % were found 7–8 months after preparation. The positive values increased up to 3.4–3.7 % during the last stability period (18–19 months). MVK and MEK showed respectively fluctuating positive (up to +5.7 %) and negative (up to -6.4 %) relative differences most likely due to analytical issues, isomerization reactions and/or surface effects. Ethanol showed a negative relative difference which remained within the $\pm 5\%$ threshold, except for one of the measurement results obtained at months 18–19 (-5.1 %). Acetaldehyde and methanol long-term stability had the largest biases. Varying relative differences $> \pm 5\%$ (positive for acetaldehyde and negative for methanol) were already found after 5–6 months after preparation, which could be explained by analytical issues, matrix effects and initial compound losses due to adsorption effects.~~

525 During the interlaboratory comparison organized as part of the RGM verification process (Appendix B.4.2.2), the three participant laboratories (VSL, METAS and LNE) measured acetone, ethanol and methanol. Results demonstrated a very good comparability and degree of equivalence for acetone (Fig. 14). For methanol, a good agreement among laboratories was also found (Fig. B1), as well as for ethanol. However, due to the great expanded uncertainty (37 %) of the ethanol measurement associated to METAS analytical issues, these results were not considered. It can be noted that although different calibration and analytical methods were used, the measurement results of the RGMS were aligned giving confidence on the quality of the work.

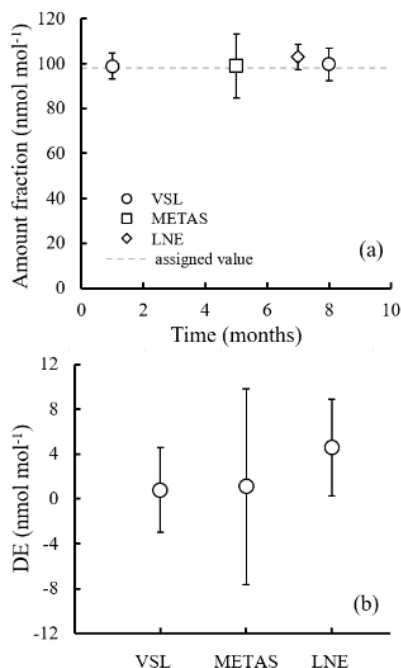

535 **Figure 14:** Interlaboratory comparison results for (a) acetone and (b) its degree of equivalence (DE; i.e., the deviation of each laboratory from the reference value). For VSL, only the first measurement period was considered (month 1) to estimate the DE. The measured amount fractions reported by the laboratories were the average of 5 measurements, except for month 1 results, which were the average of 3 measurements. Error bars show the expanded uncertainty of the measurements (coverage factor $k = 2$). The dashed line indicates the gravimetric amount fraction of the compound.

540 Long-term stability results (Table B4) suggested very good stability (i.e., relative differences between analytical and gravimetric values smaller than $\pm 5\%$) for acetone with relative differences $< +2\%$ even 13–14 months after RGM preparation, although a questionable result (-4.7%) was obtained at a stability testing period of 18–19 months. Acetone results were similar to those for the internal standard (n-hexane). A good stability was also found for methacrolein. After initial relative differences of ca. -1.5% , positive values around $+0.7\%$ were found 7–8 months after preparation. The positive values increased up to $3.4\text{--}3.7\%$ during the last stability period (18–19 months). MVK and MEK showed respectively fluctuating positive (up to $+5.7\%$) and negative (up to -6.4%) relative differences most likely due to analytical issues, isomerization reactions and/or surface effects. Ethanol showed a negative relative difference which remained within the $\pm 5\%$ threshold, except for one of the measurement results obtained at months 18–19 (-5.1%). Acetaldehyde and methanol long-term stability had the largest biases. Varying relative differences $> \pm 5\%$ (positive for acetaldehyde and negative for methanol) were already found after 5–

545 6 months after preparation, which could be explained by analytical issues, matrix effects and initial compound losses due to

550 adsorption effects.

5.3.1.2 Assessment of SI-traceable working standards based on dilution of RGMs


The assessment of the SI-traceable working standards based on the dilution of RGMs with dry nitrogen took place during a long period of time (ca. six months between the first and last participants). Potential temporal instabilities were considered when comparing results through the certified expanded uncertainty provided with the RGMs (Table 23). The long-term RGM stability of each compound was evaluated and taken into account as an uncertainty term (Table B3B4). The type of in-house standard, sampling method and analytical instrument used, as well as the amount fraction level of the samples generated, were most likely the parameters explaining the differences found between VSL and the other participants for certain compounds, such as MEK (Fig. 25) and methanol (Fig. 36).

Despite relative differences around $\pm 20\%$ for IMT and Empa, a good agreement between assigned and analytical values (i.e., relative difference around 0 considering the uncertainty of the difference) was found for acetone, even at amount fractions $< 5 \text{ nmol mol}^{-1}$ (Fig. 25). This agreement demonstrated the reliability of the dilution systems, RGMs and calibration methods. The great relative differences obtained by Empa for acetone were explained by technical issues with the analytical method (i.e., a leak in the heated valve and flow overshooting when measuring with the Stirling cooling unit). The error was estimated to be around $\pm 30\%$ and was included in the uncertainty budget. These issues also affected Empa MEK and methanol measurements. Therefore, care should be taken in the interpretation of these results.


Similar results to acetone working standards were obtained for MEK at amount fractions around 10 nmol mol^{-1} (Fig. 25). At lower amount fraction levels ($< 5 \text{ nmol mol}^{-1}$), some of the measurements showed analytical fraction values lower than the assigned ones.

Methanol relative differences were relatively small (1–14 %) and within the uncertainty range at amount fractions between 10 nmol mol^{-1} and 17 nmol mol^{-1} (Fig. 36). However, at lower amount fractions ($< 5 \text{ nmol mol}^{-1}$) relative differences were between 25–65 %, which suggest an overestimation of the analytical amount fraction values most likely due to artefacts in the analytical system. Moreover, the temporal instability of methanol within the gas cylinder, with an increase in the amount fraction observed during the first year after preparation for one of the RGMs, might contribute to explain part of the overestimation. Methanol instability in gas cylinders was observed in other works (Persijn and Baldan, 2023; Rhoderick et al., 2019). Methanol assessment results suggest, thus, that this OVOC remains a challenging compound to measure.

Acetaldehyde measured and assigned amount fractions showed relatively good agreement, i.e., all the differences were within the uncertainty range (Fig. 47). However, these results must be taken with care because of the large uncertainties. Reactions in the gas cylinders and/or artefacts of the analytical methods might have contributed to analytical amount fractions greater than the theoretical values for acetaldehyde, as well as to uncertainties greater than for the other OVOCs.

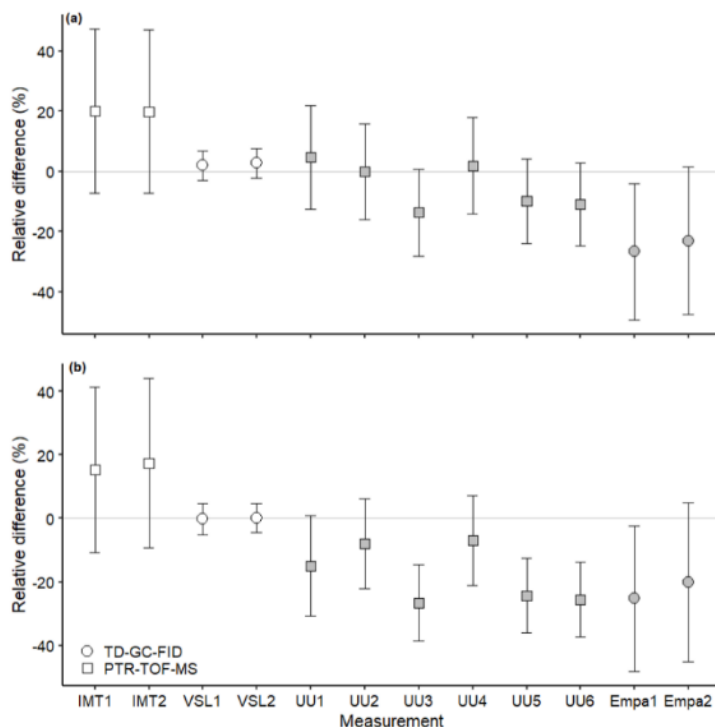


600 **Figure 25:** Assessment of the SI-traceable working standards based on the dilution of reference gas mixtures with dry nitrogen for (a) acetone and (b) MEK at amount fractions $< 5 \text{ nmol mol}^{-1}$ (grey symbols) and between $10\text{--}17 \text{ nmol mol}^{-1}$ (white symbols). Error bars indicate the expanded uncertainty (coverage factor $k = 2$) of the relative difference between in-house and dilution working standards. Measurement labels show the participant and the number of SI-traceable working standards generated by dilution. Measurements were performed in July 2022 (IMT1, IMT2), August 2022 (VSL1, VSL2), September 2022 (UU1-UU6) and November 2022 (Empa1, Empa2).

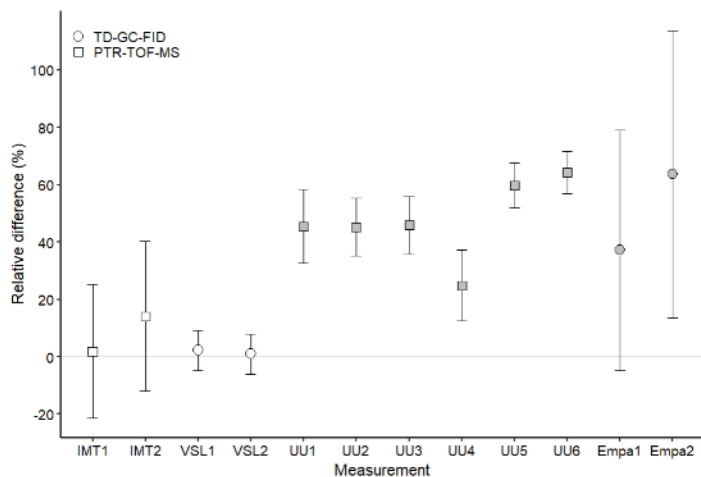

615 **Figure 36:** Assessment of the SI-traceable working standards based on the dilution of reference gas mixtures with dry nitrogen for methanol at amount fractions $< 5 \text{ nmol mol}^{-1}$ (grey symbols) and between $10\text{--}17 \text{ nmol mol}^{-1}$ (white symbols). Error bars indicate the expanded uncertainty (coverage factor $k = 2$) of the relative difference between in-house and dilution working standards. Measurement labels show the participant and the number of SI-traceable working standards generated by dilution. Measurements

were performed in July 2022 (IMT1, IMT2), August 2022 (VSL1, VSL2), September 2022 (UU1-UU6) and November 2022 (Empa1, Empa2).

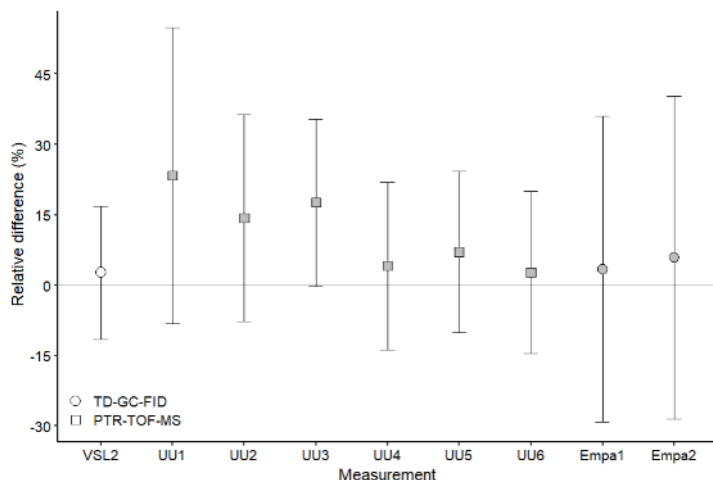

630 **Figure 47:** Assessment of the SI-traceable working standards based on the dilution of reference gas mixtures with dry nitrogen for acetaldehyde at amount fractions $< 5 \text{ nmol mol}^{-1}$ (grey symbols) and between $10\text{-}17 \text{ nmol mol}^{-1}$ (white symbols). Error bars indicate the expanded uncertainty (coverage factor $k = 2$) of the relative difference between in-house and dilution working standards. Measurement labels show the participant and the number of SI-traceable working standards generated by dilution. Measurements were performed in August 2022 (VSL2), September 2022 (UU1-UU6) and November 2022 (Empa1, Empa2).

635

Assessment results for amount fraction levels around 10 nmol mol^{-1} suggests that SI-traceable working standards based on dilution of RGMs can be used as calibration standard at monitoring stations for key OVOCs, such as acetone, MEK, methanol and acetaldehyde. However, For other OVOCs, like methanol, acetaldehyde and MEK, suitability is not so clear due to the large uncertainty and result dispersion, particularly at lower amount fractions ($< 5 \text{ nmol mol}^{-1}$), suitability of the SI-traceable working standards for MEK, methanol and acetaldehyde is also questionable. The different analytical methods used, the calibration procedure followed and the dilution factors applied to measure and prepare the SI-traceable working standards contributed to that large uncertainty and result dispersion. Further research where the same methodology is followed: following the same calibration procedure (e.g., same in-house working standard) and assessment protocol (e.g., setting the same dilution factors to generate SI-traceable working standards at the same amount fractions) may reduce both uncertainty and dispersion and help to draw conclusions. Moreover, using coated (e.g., SilcoNert 2000) lines – as short as possible – and low-dead volume pressure regulators/reducer, as well as performing long enough-flushing and repeated measurements to guarantee the stability of analyser and dilutor, may reduce the uncertainty of the generated working standards. Even if results are not conclusive, the low RGM uncertainty ($< 5 \%$) and long temporal stability (at least up to 15-18 months after preparation) are promising to provide atmospheric monitoring stations with SI-traceable accurate OVOC working standards at very low amount fractions.

650

5.2 Results of the SI-traceable working standards based on certified spiked whole air samples

5.2.1 Homogeneity assessment, stability evaluation and amount fraction certification of the spiked whole air samples

Results of the analysis of variance (ANOVA) performed on the data from the homogeneity test of the subset of vessels filled with the spiked whole air samples (Table C3) showed good homogeneity (variation < 5 %) within the same vessel type for all selected OVOCs. The greatest variation was found for methanol (+3.2 %). For the rest of OVOCs, the variation was $\leq +1.5$ % (e.g., +0.6 % for acetone, +0.9 % for MVK, +1.2 % for MEK and +1.5 % for acetaldehyde and ethanol). Variation among different vessel types suggested that the vessel material may play a role in the lack of homogeneity particularly for methanol (+22.6 %) and ethanol (+9.7 %). Variation was relatively great also for acetaldehyde (+6.6 %), MEK (+6.6 %) and MVK (+7.0 %). However, good homogeneity was found for acetone (+2.8 %) and toluene (+2.4 %). Although toluene is not an OVOC and, thus, was not spiked into the whole air sample vessels, the compound was naturally present in the ambient air.

Temporal stability of the air samples was evaluated by Empa considering the ratio between each OVOC and the internal standard (i.e., n-hexane). Acetone to n-hexane ratios showed good temporal stability (i.e., differences in ratio values among measurements within the uncertainty of the measurement) during the measuring period from August 2021 to September 2022. Except for the uncertainties that were greater, similar results were found for other compounds (methanol, ethanol, acetaldehyde, MVK and MEK). Because the ratio differences observed were within the uncertainty of the measurements and the homogeneity among vessels of the same type was good (variation < +2 % except for methanol (+3.2 %)), air samples in the same type of vessel were considered stable.

Certification results obtained for whole air samples contained in pressurised 10 L aluminium cylinders showed good consistency between the two laboratories performing the certification (i.e., VSL, METAS), with exception of MVK (criterion was not met (Eq. (4)) (Table C5, Figure C1). Regarding the other type of pressurised cylinders (3.6 L stainless steel SilcoNert® coated), the criterion was neither met for MVK. For methanol, the criterion was met only when METAS results were compared against the results obtained for the first measurements performed by VSL (i.e., July 2021). Certified OVOC amount fractions in both cylinders (Table 5) ranged between 7.6 nmol mol⁻¹ (ethanol) and 17.3 nmol mol⁻¹ (acetone) with expanded uncertainties ($k = 2$) ≤ 2.6 nmol mol⁻¹ (Table 54). The smallest uncertainties were found for methacrolein and acetone (≤ 1.5 nmol mol⁻¹). Amount fractions were in line with the estimated spiked values (Table C1) suggesting that, except for acetone, the amount fractions of the selected OVOCs in the sampled air were not significant (close to zero). The higher amount fractions measured for acetone compared to the spiked estimated amount fractions suggested acetone background levels in the sampled whole air of around 6.5 nmol mol⁻¹.

Results of the low-pressure canisters were less consistent: the criterion was only met for methacrolein for four canisters (Table C5). For methanol and acetone, the criterion was only met in two canisters. The discrepancy between results for the 15 L canister suggested homogeneity issues for this batch.

Table 54: Certified amount fraction values (x) and their expanded uncertainty (U ; coverage factor $k = 2$) estimated for the air samples filled in the high-pressure cylinders: 10 L cylinder (MVOC151-001) and 3.6 L (MVOC151-002).


compound	$x_{MVOC151-001} \pm U$ {(nmol mol ⁻¹)}	$x_{MVOC151-002} \pm U$ {(nmol mol ⁻¹)}
methanol	12.8 ± 2.0	9.8 ± 2.5*
ethanol	11.2 ± 2.6	7.6 ± 1.9
acetone	17.0 ± 1.5	17.3 ± 1.1
methacrolein	10.7 ± 1.0	10.2 ± 0.9
MVK	9.4 ± 2.6*	8.4 ± 2.3*
MEK	12.3 ± 2.3**	12.1 ± 2.4**

* no compliance with evaluation criterion described in Eq. (4)


685 ** measurement carried out by only one of the laboratories

5.4.1.2 Assessment of SI-traceable working standards based on certified spiked whole air samples

Amount fractions of the OVOCs measured in air samples showed good agreement (Fig. 85, Fig. 69, Fig. 10) among partners. These values were comparable to the certified amount fractions for whole air samples in cylinders (pressurised at 9.8–10.5 MPa). Only for methanol (Fig. 610), values were more discrepant. Empa results, as for the SI-traceable working standards based on dilution of RGMs with dry nitrogen, must be interpreted with caution because of the technical issues with the analytical system.

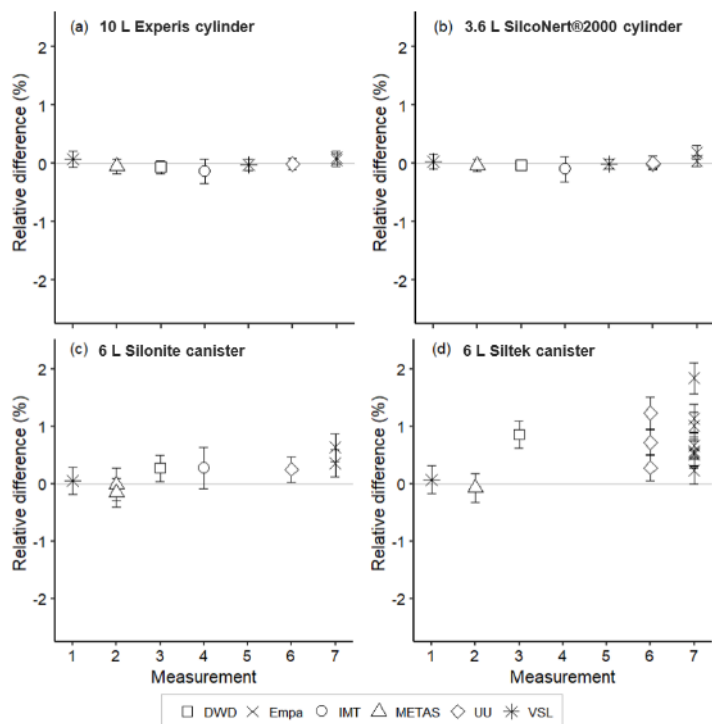


710 Figure 58: Assessment of the SI-traceable working standards based on certified spiked whole air samples for acetone in (a) 10 L
 715 Experis® aluminium cylinders, (b) 3.6 L SilcoNert® 2000 stainless steel cylinders, (c) 6 L Silonite™ stainless steel canisters and (d) 6 L Siltek® stainless steel canisters. ~~Spiked amount fraction (solid grey line), certified amount fraction (solid green line) and their expanded uncertainty (dashed lines) are shown.~~ Error bars indicate the expanded uncertainty (coverage factor $k = 2$) of the relative difference between the measured and the certified amount fraction values of the working standards in-house and dilution working standards. Measurements were performed in Jul. 2021 (1), Feb. 2022 (2), Mar. 2022 (3), Jun. 2022 (4), Aug. 2022 (5), Sep. 2022 (6) and Nov. 2022 (7).

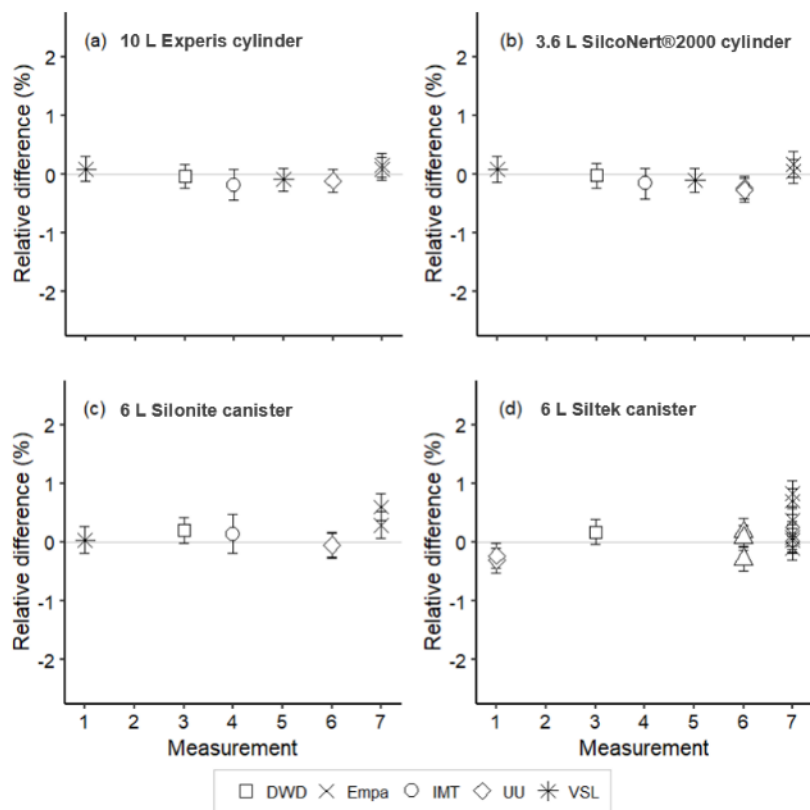

735 Figure 9: Assessment of the SI-traceable working standards based on certified spiked whole air samples for methyl ethyl ketone (MEK) in (a) 10 L Experis® aluminium cylinders, (b) 3.6 L SilcoNert® 2000 stainless steel cylinders, (c) 6 L Silonite™ stainless steel canisters and (d) 6 L Siltek® stainless steel canisters. Error bars indicate the expanded uncertainty (coverage factor $k = 2$) of the relative difference between the measured and the certified amount fraction values of the working standards. Measurements were performed in Jul. 2021 (1), Feb. 2022 (2), Mar. 2022 (3), Jun. 2022 (4), Aug. 2022 (5), Sep. 2022 (6) and Nov. 2022 (7).

740 For whole air samples in canisters (pressurised at 0.35 MPa), results were quite heterogeneous. Relatively good results were
 found for acetone (Fig. 610) and MEK in the Silonite™ stainless steel canisters. However, for methanol and acetaldehyde,
 disagreement was found both among most of the participants and with the certified values. Lack of agreement was also
 observed for air samples in the Siltek® stainless steel canisters. Even if the same cleaning procedure was followed by both
 745 type of canisters before filling, the history (i.e., previous fillings) of the Siltek® stainless steel canisters and/or the surface
 treatment could explain the differences between canister types. History and surface treatments effects on VOC amount

fractions have been reported in previous works (e.g., Rhoderick et al., 2019; Persijn and Baldan, 2023). Furthermore, vessel pressure might explain the differences in result agreement between cylinders and canisters. Gas pressure effects on the stability of gas mixtures in cylinders have been observed for different compounds, such as CO₂ (e.g., Leuenberger et al., 2015; Miller et al., 2015). In these studies, after an initial wall adsorption when the cylinders were filled, desorption took place. This adsorption-desorption process resulted in increasing amount fractions. In Silonite™ canisters, the treatment might have contributed to a lower initial wall adsorption compared to the Siltek® canisters and, therefore, to the lower discrepancies.

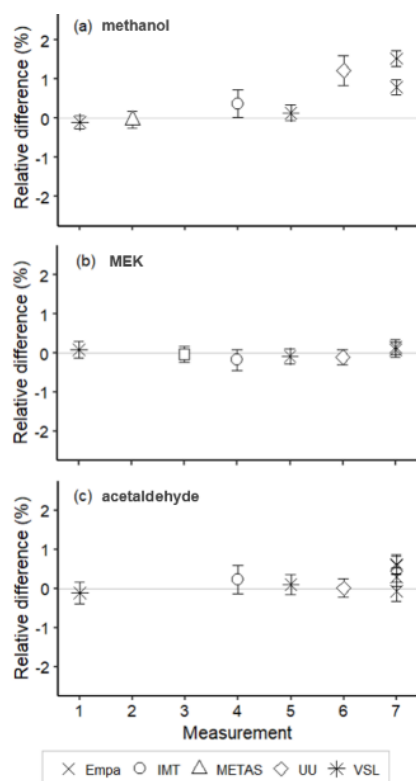

755 **Figure 610:** Assessment of the SI-traceable working standards based on certified spiked whole air samples in 10 L Experis® aluminium cylinders for (a) methanol, (b) methyl ethyl ketone (MEK) and (c) acetaldehyde. **Spiked amount fraction (solid grey line), certified amount fraction (solid green line) and their expanded uncertainty (dashed lines) are shown.** Error bars indicate the expanded uncertainty (coverage factor $k = 2$) of the relative difference between **the measured and the certified amount fraction values of their in-house and dilution** working standards. Measurements were performed in Jul. 2021 (1), Feb. 2022 (2), Mar. 2022 (3), Jun. 2022 (4), Aug. 2022 (5), Sep. 2022 (6) and Nov. 2022 (7).

760 Assessment results suggest that certified spiked whole air samples at low amount fractions ($<20 \text{ nmol mol}^{-1}$) in compressed gas cylinders may be used as SI-traceable working standards for most of the selected OVOCs, except for methanol, at monitoring stations. Using the same matrix gas as the ambient air monitored at atmospheric stations may improve the accuracy of the observations by reducing artefacts and other effects related to the matrix gas.

6 Conclusions

765 VOCs are one of the major tropospheric ozone precursors. Despite the importance of performing accurate and comparable
VOC measurements to assess tropospheric ozone burdens and trends, several challenges regarding VOC monitoring remain
currently open. For example, the lack of stable and SI-traceable gas reference materials for many OVOCs at ambient levels
and adapted to constraints of monitoring stations (e.g., limited dilution gas supply) among others.

This research has shown that producing SI-traceable RGMs at amount fractions around $100 \text{ nmol mol}^{-1}$, with expanded
770 uncertainties of the preparation $< 5 \%$ and temporal stability of at least 14 months, is doable for acetone, methacrolein, MEK,
MVK and, to some extent, for ethanol. However, for methanol and acetaldehyde, further research is needed to find suitable
cylinder materials and optimal preparation and analytical procedures (e.g., cylinder wall passivation) to minimize surface
adsorption and reaction effects, which greatly contributed to the temporal instability of RGMs for methanol and
acetaldehyde both compounds. These stable and accurate RGMs are produced at amount fraction levels greater than ambient
775 levels of the selected OVOCs (i.e., $4\text{--}10 \text{ nmol mol}^{-1}$). RGM dilution is thus needed to achieve the amount fraction range
required by monitoring stations. To guarantee that SI-traceability is maintained, the dilution needs to be done by a dilution
system that is traceable. For that purpose, the elements of the dilution system (e.g., thermal mass flow controller) have to be
calibrated against traceable flow standards by NMIs and/or accredited calibration laboratories. Moreover, to reduce as much
as possible the uncertainty of the dilution associated to surface effects, the components in contact with the RGM should be
780 coated (e.g., SilcoNert® 2000), low dead-volume pressure reducers should be used and enough time for reaching stability of
the dilution and analytical systems should be recommended. The procedure and recommendations described correspond to the
SI-traceable working standards based on RGMs diluted with dry nitrogen described in this work, which can be generated at
amount fractions around 10 nmol mol^{-1} with acceptable relative expanded uncertainties (coverage factor $k = 2$) $< 10 \%$ (for
acetone and MEK, the expanded uncertainty is even lower than 4%). This first type of SI-traceable working standard seems
785 to be suitable for calibration of acetone, MEK, methanol and (with larger uncertainties) acetaldehyde at monitoring stations,
guaranteeing comparability of the VOC measurements within and among monitoring stations.

Besides RGMs, SI-traceable working standards at lower amount fractions (i.e., ambient levels; $4\text{--}10 \text{ nmol mol}^{-1}$) to calibrate
VOC analyzers at monitoring stations are needed to ensure comparability of the VOC measurements within and among
monitoring networks. Here, we presented the developed and assessed protocols to generate two different types of SI-traceable
790 working standards. The first type, based on RGMs diluted with dry nitrogen, using for that a portable dilution system that
ensures SI-traceability after dilution, seems to be suitable for calibration of acetone, MEK and methanol at amount fractions
around 10 nmol mol^{-1} . Different vessel types were filled with the second type of SI-traceable working standards based on
certified whole air samples: high-pressure ($> 9.5 \text{ MPa}$) cylinders with different treatments (Experis® and SilcoNert® 2000)
and low-pressure ($< 0.45 \text{ MPa}$) canisters with two different coatings (Silonite™ and Siltek®). Assessment results suggest that
795 certified spiked whole air samples filled into high-pressure cylinders at amount fractions around 10 nmol mol^{-1} , valid for 12–
14 months might become a valid alternative for calibrating analytical systems measuring acetone, acetaldehyde and MEK at

800 monitoring stations. Even if VOC RGMs in nitrogen are more stable, this second type of SI-traceable working standard will allow monitoring stations to calibrate their instruments with standards that use similar matrix gas than the ambient air analyzed. Matrix gas effects on the analytical systems are not fully understand yet, but these working standards might provide some insights on the topic. Before going forward with this option, in addition to matrix gas effects on the analytical systems, water passivation and vessel wall effects on the stability of the OVOC amount fractions of these working standards should be explored. Although results of this research suggest that stability might be material dependent, the observed differences might be due to other factors, such a pressure and volume differences among vessels. Specific experiments using new vessels of same volume and pressure (i.e., vessels that were not previously used) should be designed to find the vessel material performing the
805 best.

~~The second type, based on certified spiked whole air samples filled into high pressure cylinders might become also a valid alternative for calibrating instruments measuring acetone, acetaldehyde and MEK at monitoring stations.~~ Despite these promising findings, conclusions must be driven with caution because of the large values and the broad range obtained for the measurement uncertainties (i.e., 5–31 %; coverage factor $k = 2$). Moreover, Ffor both types of working standards, methanol calibration remains challenging.

810 The RGMs and working standards described in this work are a first step to fulfil the remaining needs of VOC monitoring. Through an active collaboration among metrological, meteorological and atmospheric chemistry monitoring communities, harmonization and comparability among monitoring stations will be promoted (e.g., by estimating uncertainty budgets that are common to the different monitoring programs). Moreover, this collaboration might provide a better understanding of the impact that pressure, sampling material, moisture and matrix have on the preparation of RGMs and working standards. This knowledge may contribute, thus, to improve calibration standards (i.e., RGMs and SI-traceable working standards) and uncertainties of VOC measurements. Furthermore, other research applications, such as modelling and remote sensing, might benefit from the transfer of SI-traceability to monitoring stations.

Appendix A: Analytical instruments and dilution systems

820 A.1 Analytical instruments

Thermal Desorption ~~(TD)~~-Gas Chromatography (GC)-Flame Ionization Detector ~~(TD-GC-FID)~~ and Proton Transfer Reaction (PTR)-Time of Flight (ToF)-Mass Spectrometry ~~(PTR-ToF-MS)~~ were the two selected analytical methods in this work. The specific analytical instruments used by the laboratories are summarised in Table A1.

DWD (Deutscher Wetterdienst)

825 DWD deployed a GC-FID/MS system (6890, 7590 inert XL MS, Agilent Technologies Inc., CA, USA), which was coupled to a custom-made sample pre-concentration unit that included sampling valves, sampling ports and the preconcentration trap in a box heated to 150 °C. Materials in the sampling path were mainly treated stainless steel or capillaries. Samples were preconcentrated on multibed sorbent tubes (Tenax TA 60/80 mesh, Carboxen X 40/60 mesh and Carboxen 695 20/45 mesh

in a ¼” glass tube, Merck KGaA (Supelco), MO, USA) at 30 °C with a sampling flow of 80 mL min⁻¹. Desorption to a cryo-
830 focus trap (inert capillary cooled to -180 °C) took place at 200 °C with a flow of 10 mL min⁻¹. After heating the cryo-focus to
60 °C, the sample was injected splitless onto a BPX-5 capillary column (50 m length, 0.32 mm internal diameter, 0.5 µm film
thickness, Trajan Scientific and Medical (SGE), Australia). The GC oven was held at 13 °C for 18 min. Then, the oven
temperature was increased up to 240 °C at a rate of 6 °C min⁻¹. Hydrogen (H₂ 5.0 from Air Liquide, France) cleaned using a
gas filter (Super Clean gas filter, Restek, PA, USA) was used as a carrier gas at 3.5 mL min⁻¹. Subsequent to the separation on
835 the column, the carrier gas flow was split onto the MS and the FID in parallel. For the analysis of the SI-traceable working
standards based on spiked whole air, the MS detector was used to achieve sufficient peak separation.

Empa (Swiss Federal Laboratories for Materials Science and Technology)

Empa used a GC-FID (7890, Agilent Technologies Inc., CA, USA) coupled to a thermal desorber UNITY™-xr (Markes
840 International Ltd., UK) to evaluate the stability and homogeneity of the air samples and to assess the SI-traceable OVOC
working standards (Table A1). Samples went through an in-house dehumidifier – consisting of a Stirling cooler (set to -42 °C)
and two insulated in-line glass fingers – before sampling, which was done using a UNITY™-Air Server (Markes International
Ltd., UK) equipped with three ports. From UNITY™-Air server, samples passed to the thermal desorber, which collected and
concentrated the OVOCs under study. The UNITY cold trap (ozone precursors cold trap, U-T1703P-S2; Markes International
845 Ltd., UK) temperature was set to -29 °C before the cold trap was heated up to 250 °C. The two capillary columns were
OxyPLOT (30 m length, 0.53 mm internal diameter and 10 µm film thickness; Agilent Technologies Inc., CA, USA) and
Al₂O₃ HP-PLOT (50 m length, 0.53 mm internal diameter and 10 µm film thickness; Agilent Technologies Inc., CA, USA).
Sample flow was set at 15 mL min⁻¹ during 20 min. The GC oven was held at 40 °C for 3.25 min and then heated up to 200
°C with a temperature ramp of 7 °C min⁻¹. The GC oven was held at 200 °C for 20 min. The carrier gas was helium, which
850 was set at 5 mL min⁻¹ for 20 min and then increased at 25 mL min⁻¹ for 26 min.

IMT (Institute Mines-Télécom)

IMT performed the assessment of SI-traceable working standards using a second generation PTR-ToF-MS (Kore Technology
Ltd., UK) (Table A1). Sampling was done through a SilcoNert® 1000 heated line at a flow rate of 200 mL min⁻¹. An in-house
855 system of solenoid valves was coupled to the PTR-ToF-MS to switch automatically between samples and zero air.
Measurement time resolution was set to 10 seconds.

LNE (Laboratoire National de Métrologie et d'Essais; National Metrology Institute (NMI) of France)

LNE used a GC-FID (7890, Agilent Technologies Inc., CA, USA), equipped with an on-column pre-concentration system,
860 during the OVOC RGM comparison (Table A1). The selected capillary column was HP-Plot-U (30 m length, 0.53 mm internal
diameter and 20 µm film thickness; Agilent Technologies Inc., CA, USA). The GC oven was held at a constant temperature
of 150 °C. The carrier was helium BIP® (Air Products and Chemicals, PA, USA). The sampling was done using a coated

(SilcoNert® 2000) sample loop, which injected a sample volume of 60 mL. The pre-concentration system was cooled down to -60 °C by a liquid nitrogen cryo trap system (JAS 66601 CryoTrap, Joint Analytical Systems GmbH, Germany), which was
865 heated up to 150 °C for final injection.

METAS (Federal National Metrology Institute; NMI of Switzerland)

METAS used a GC-FID Clarus 500 (PerkinElmer Inc., MA, USA) coupled to a thermal desorber TurboMatrix 350 (PerkinElmer Inc., MA, USA) (Table A1). The capillary column was DuraBond DB-624 (30 m length, 0.32 mm internal
870 diameter and 1.8 µm film thickness; Agilent Technologies Inc., CA, USA). The carrier gas was helium. The system had a Tenax-TA sorbent cold trap (Perkin Elmer Inc., MA, USA), which was cooled at -30 °C and heated up to 280 °C at a temperature rate of 40 °C s⁻¹. The GC oven was held at 40 °C for 2 min and then heated up to 200 °C at 5 °C min⁻¹. The GC oven was held at 200 °C for 2 min. The sampling was done using conditions multibed sorbent tubes: Carbograph 2TD (mesh 60/80)– Carbograph 1TD (mesh 40/60)– Carbosieve™ SIII (mesh 60/80) (Camsco, TX, USA). Loading of the sorbent tubes
875 were done by means of an in-house loading system at loading volumes between 300 mL (10 min at 30 mL min⁻¹) and 450 mL (15 min at 30 mL min⁻¹).

UU (Utrecht University)

UU used a PTR-ToF-MS with hexapole and ion funnel (PTR-TOF4000, Ionicon Analytik GmbH, Austria) to assess the SI-
880 traceable working standards (Table A1). A SulfiNert® coated 4-port valve (VICI® Valco Instruments Co. Inc., TX, USA) kept at 120 °C was used to switch between zero air and sample inlet. Samples were connected to a PEEK capillary that, depending on the pressure in cylinders and canisters, produced a flow between 80 mL min⁻¹ and 300 mL min⁻¹.

VSL (NMI of the Netherlands)

VSL used TRACE™ GC (Thermo Fisher Scientific Inc., PA, USA) coupled to a thermal desorber UNITY™ 2 (Markes
885 International Ltd., UK) during the OVOC comparison, the certification of air samples and the assessment of SI-traceable working standards (Table A1). A Deans switch in the GC sent the gas sample to two FID detectors and two capillary columns: Stabilwax (30 m length, 0.32 mm internal diameter and 1.0 µm film thickness; Restek Corporation, PA, USA) for MVK and PoraBOND U (25 m length, 0.32 mm internal diameter and 7 µm film thickness; Agilent Technologies Inc., CA, USA) for the
890 other OVOCs. The cold trap filled with multi-bed sorbent trap (Air Toxics, Markes International Ltd., UK) was cooled down to -20 °C and heated up to 300 °C. Sampling flow was set at 20 mL min⁻¹ during 30 min. The GC oven was held at 40 °C for 2 min and then heated up to 230 °C with three temperature ramps of 20 °C min⁻¹ (up to 120 °C), 5 °C min⁻¹ (up to 180 °C) and 10 °C min⁻¹ (up to 230 °C). The GC oven was held at 200 °C for 20 min. The carrier gas was helium.

895 **Table A1: Information on the analytical instruments used in this work.**

Lab	Measurements	Analytical method	Analytical instrument
DWD	Assessment ²	TD-GC-FID/MS	6890 GC-FID (Agilent), 7590 inter XL MS (Agilent) Custom made TD unit (DWD)
Empa	Assessment ^{1,2}	TD-GC-FID	7890 GC-FID (Agilent) TD UNITY™-xr (Markes International)
IMT	Assessment ^{1,2}	PTR-ToF-MS	second-generation PTR-ToF-MS (Kore Technology)
LNE	Comparison	TD-GC-FID	7890 GC-FID (Agilent)
METAS	Comparison, certification	TD-GC-FID	Clarus 500 GC-FID (Perkin Elmer) TD TurboMatrix 350 (Perkin Elmer)
UU	Assessment ^{1,2}	PTR-ToF-MS	PTR-TOF4000 (Ionicon Analytik)
VSL	Comparison, certification, assessment ^{1,2}	TD-GC-FID	Thermo Trace GC-FID; TD UNITY™ 2 (Markes International)

¹Assessment SI-traceable working standards based on dilution of [Reference Gas Mixtures \(RGMs\)](#) with dry nitrogen

²Assessment SI-traceable working standards based on certified spiked whole air samples

A.2 Dilution systems

900 Two dilution systems were used to generate the SI-traceable working standards based on the dynamic dilution of RGMs.

905 The first system, developed by VSL, was a one-stage gas dilutor with dilution flows ranging 2–50 L min⁻¹, allowing dilution ratios up to 1:1000. Flows of the RGM (0.1 L min⁻¹) and of the dilution gas (nitrogen, AP BIP Plus grade 6.0) were accurately controlled using three MFCs (EL-FLOW® Select series, Bronkhorst, Netherlands), operating up to 10 L min⁻¹ and 25 L min⁻¹. The dilution system was mostly built in inert glass. Other materials in contact with the OVOC gas mixtures were

910 polytetrafluoroethylene (PTFE), 316 stainless steel (SS) (small surfaces) or coated 316 SS (SilcoNert® 2000, SilcoTek, PA, USA). A coated (SilcoNert® 2000) pressure reducer was connected to the RGMs and flushed thoroughly before attaching it to the dilution system. For the purpose of this assessment, the MFCs were set and calibrated using two mercury piston prover volumeters (Bronkhorst, Netherlands), which were in turn calibrated at the VSL Flow Department, at working ranges of 0–0.5 L min⁻¹ and 0–10 L min⁻¹. Temperature and pressure were measured by equipment calibrated at the VSL Temperature and

910 Pressure Department to convert flow to standard temperature and pressure (STP) conditions (293.15 K, 101.3 kPa).

The second system ("VeRDi" (Versatile Reactive Gas Diluter)), developed by METAS in collaboration with Swagelok® Switzerland, was a two-stage gas dilution system allowing dilution ratios up to 1:175000. The main components of this two-stage gas dilution system were four MFCs (two MFCs up to 0.1 L min⁻¹ (Red-y, Vögtlin Instruments, GmbH, Switzerland)

and two MFCs up to 5 L min⁻¹ (Sensirion AG, Switzerland), two pressure controllers (Bronkhorst High-Tech B.V., Netherlands), a valve terminal (MPA-L, Festo Beteiligungen GmbH & Co. KG, Germany) and a vacuum pump. Elements in contact with RGM flow were coated (SilcoNert® 2000), including all the stainless steel tubing of ¼" internal diameter used to build VeRD_i. The tubes were welded, instead of joined through fittings, in order to reduce dead volumes and potential leaks. MFCs and pressure regulators were calibrated using clean and dry nitrogen against METAS primary standards to ensure traceability of the dilution. The software controlling VeRD_i was developed in LabVIEW (National Instruments, Austin, TX).

Appendix B: Purity analysis, stability evaluation and verification of the Reference Gas Mixtures (RGMs)

B.1 Purity analysis

Prior to their injection in the pressurised cylinders, the pure liquid oxygenated volatile organic compounds (OVOCs), selected used to prepare the gravimetric RGMs, were analysed to determine their purity according ISO 19229:2019 (2019). For that purpose, VSL (the national metrology institute (NMI) of the Netherlands) used a gas chromatographic (GC) system (6890, Agilent Technologies Inc., CA, USA) with a mass spectrometer (MS) and a flame ionization detector (FID) equipped with a GS-GASPRO capillary column (60 m length, 0.32 mm internal diameter and 0.25 µm film thickness; Agilent Technologies Inc., CA, USA). For acetaldehyde, it was not possible to perform the purity analysis because of the physical properties of the liquid chemical, which made its handling difficult. The water content in the liquid OVOCs was determined by the Karl Fischer titration (Coulometric KF titrator, Metrohm). Results of the purity analysis are included in (Table B1).

Table B1: Purity of the liquid OVOCs used to prepare the gravimetric reference gas mixtures including the amount fraction of compounds and impurities (x_i) and its expanded uncertainty ($U(x_i)$; coverage factor $k = 2$). CAS refers to the chemical abstract service registry number. The purity analysis of acetaldehyde (CAS 75-07-0) was not possible because of handling difficulties associated to the physical properties of the liquid chemical.

Liquid chemical	CAS	Supplier	Compound	x_i (mol mol ⁻¹)	$U(x_i)$ (mol mol ⁻¹)
acetaldehyde	75-07-0	Acros Organics™, PA, USA	acetaldehyde	0.999 ¹⁾	NA
acetone	67-64-1	Sigma-Aldrich®, MA, USA	acetone	0.999380	0.000124
			water	0.000620	0.000124
ethanol	64-17-5	Merck KGaA, Germany	ethanol	0.999733	0.000054
			water	0.000267	0.000054
methacrolein	78-85-3	Thermo Fischer Scientific Inc., PA, USA	methacrolein	0.985646	0.001683
			methylal	0.003458	0.000692
			1,1-dimethoxy-2-butene	0.003600	0.000720
			hydroquinone	0.001000	0.000500

Liquid chemical	CAS	Supplier	Compound	x_i (mol mol ⁻¹)	$U(x_i)$ (mol mol ⁻¹)
			water	0.006296	0.001260
m Methanol	67-56-1	<u>Sigma-Aldrich®, MA, USA</u>	methanol	0.999724	0.000056
			water	0.000276	0.000056
m Methyl e Ethyl k Ketone (MEK)	78-93-3	<u>Acros Organics™, PA, USA</u>	MEK	0.999297	0.000147
			2,4-dimethyl-hexane ²⁾	0.000234	0.000118
			trichlorodocosyl-silane ³⁾	0.000037	0:000019
			water	0.000431	0.000087
m Methyl v Vinyl k Ketone (MVK)	78-94-4	<u>Acros Organics™, PA, USA</u>	MVK	0.940938	0.005352
			Acetonitrile	0.008389	0:001678
			4-(acetyloxy)-2-butanone	0.006077	0.001216
			2-acetyl-5-methyl-2,3-dihydro-4H-pyran ⁴⁾	0.020687	0.002069
			p-benzoquinone	0.001564	0.000313
			water	0.022346	0.004470
n-Hexane	110-54-3	<u>Merck KGaA, Germany</u>	n-hexane	0.991224	0.001307
			3-methyl-pentane	0.002943	0:000589
			methyl-cyclopentane	0.005831	0:001167
			water	0.000002	0.000001

935 ~~⁴⁾The impurity might also be MVK dimer.~~

¹⁾Purity value provided by the manufacturer

²⁾According to MS database, the first hit with highest probability is 2,4-dimethyl-hexane, but the probability is only around 10 %.

³⁾According to MS database, the first hit with highest probability is trichlorodocosyl-silane, but the probability is only around 15 %.

⁴⁾The impurity might also be MVK dimer.

940

B.23 RGM verification

B.23.1 Verification measurement results

945 The verification process was repeated three times using VSL thermal desorption (TD)-GC-FID described in Appendix A.1. The RGMs were connected to an autosampler built by VSL, sharing therefore the same pressure reducer. Lines and pressure reducer were coated (SilcoNert® 2000). To guarantee the same sampling conditions (20 mL min⁻¹ sampling flow during 15 minutes, total volume 300 mL at 293 K and 101.3 kPa) for gravimetric and dynamically prepared RGMs, the mass flow

controller (MFC) of the thermal desorber was operated in light vacuum mode by means of a pump. Each gas mixture was analysed 20 times. Results of the verification measurements performed one month after preparation of the RGMs, estimated according Eq. (2), are shown in Table B2. Three verification measurements were carried out for each RGM.

950

Table B2: Verification results obtained one month after preparation of the Reference Gas Mixtures (RGMs) gravimetrically prepared RGMs at the National Metrology Institute of the Netherlands (VSL). Three verification measurements (M1, M2 and M3) of the amount fraction of each compound (x_i) were performed per RGM. The relative standard deviation (RSD) and the relative difference between analytical and gravimetric values (Δ) are also shown. NA indicates not available data due to an analytical issue during a measurement.

Compound	RGM code	$x_{i,M1}$ (nmol mol ⁻¹)	$x_{i,M2}$ (nmol mol ⁻¹)	$x_{i,M3}$ (nmol mol ⁻¹)	RSD (%)	Δ (%)
acetaldehyde	VSL221418	101	102	99.2	1.40	-2.24
	VSL221419	NA	101	102	1.61	-1.48
	VSL221420	99.0	102	102	1.78	-2.22
	VSL221421	95.5	97.6	106	5.68	-1.47
acetone	VSL221418	98.7	99.4	98.9	0.37	0.90
	VSL221419	NA	98.9	101	1.03	0.41
	VSL221420	98.4	97.4	99.5	1.10	0.53
	VSL221421	100	101	99.7	0.53	0.33
ethanol	VSL221418	97.6	95.8	95.5	1.19	-1.75
	VSL221419	NA	95.7	98.7	5.90	-5.12
	VSL221420	93.3	91.0	93.8	1.57	-5.26
	VSL221421	96.6	97.8	90.8	3.93	-4.75
methacrolein	VSL221418	98.9	99.8	99.6	0.48	-1.29
	VSL221419	NA	97.0	99.4	1.23	-1.62
	VSL221420	99.2	98.4	101	1.29	-1.47
	VSL221421	97.0	97.7	99.1	1.08	-1.05
methanol	VSL221418	103	98.8	97.6	2.77	1.78
	VSL221419	NA	96.7	102	10.2	-5.21
	VSL221420	93.5	98.1	101	4.08	-0.14
	VSL221421	106	105	98.2	4.00	3.11
	VSL221418	103	104	103	0.64	3.29
<u>methyl ethyl</u>	VSL221419	NA	101	103	0.80	2.91
<u>ketone (MEK)</u>	VSL221420	103	103	104	0.78	3.07
	VSL221421	101	102	102	0.42	3.21
	VSL221418	99.0	99.2	99.1	0.11	-2.66
<u>methyl vinyl</u>	VSL221419	NA	96.3	98.5	1.40	-3.71
<u>ketone (MVK)</u>	VSL221420	99.0	97.4	99.1	0.99	-3.50
	VSL221421	95.6	97.7	99.3	1.93	-2.48

955

B.23.2 RGM interlaboratory comparison


The National Metrology Institutes (NMIs) of France (LNE), Switzerland (METAS) and the Netherlands VSL took part in an interlaboratory comparison to verify the produced RGMs. Three different Thermal Desorption-Gas Chromatography-Flame Ionization Detector (TD-GC-FID) systems and calibration methods (Table B43) were used to analyse the amount fraction of acetone, ethanol and methanol in the RGM sent around (VSL221418).

The same coated (SilcoNert® 2000) pressure reducer (RX 2400, Rotarex, Luxemburg) and line (1/16" coated line of 1 m length) were used, for at least one series measurements, by LNE and METAS. VSL used an autosampler (VSL spin) equipped with a multi-position valve (VICI AG International, Switzerland), a coated (SilcoNert® 2000) pressure ~~regulator-reducer~~ (Tescom, TX, USA) and coated lines (SilcoNert® 2000, 1/16" diameter, ca. 1 m length). Five series of measurements were performed by LNE and by METAS. VSL performed three series of measurements before shipping the comparison standard to the other laboratories (September 2021) and five series of measurements after the shipment (April 2022). At least five replicates per series were analysed. Individual measurement sequences consisted in the analysis of blank samples (at the beginning and end of each measurement), calibration standard samples (at two amount fraction levels) and comparison standard samples, which were (analysed between the calibration standards to minimise drift effects and prevent biases). LNE sampling was done through a coated (SilcoNert® 2000) sample loop of 20 mL volume; total sample volume was 60 mL. VSL sampling was done by means of the autosampler (Unity 2, Markes International, Ltd., UK) coupled to the TD-GC-FID at a sampling flow rate of 20 mL min⁻¹ during 15 minutes (300 mL sample volume). Multibed sorbent tubes (Carbograph 2 (mesh 60/80) – Carbograph 1 (mesh 40/60) – Carbosieve™ SIII (mesh 60/80); Camsco, TX, USA) were used for sampling by METAS; loading volume ranged between 150 mL and 450 mL.

Amount fraction values of the comparison standard were assigned applying Eq. (1) and Eq. (2). Following standard procedures used in key comparisons, the degree of equivalence of each laboratory for acetone was estimated as the difference between analytical measurement values obtained by each laboratory and the gravimetric reference value provided by VSL.

Table B34: Information on the interlaboratory comparison measurements of one of the OVOC reference gas mixtures (RGMs; VSL221418) prepared by VSL to generate SI-traceable working standards based on its dilution using dry nitrogen.

Lab	Date	Analytical instrument	Capillary column (length, internal diameter, film thickness)	Calibration method
LNE	March 2022	Agilent 7890 GC-FID	Agilent HP-Plot-U (30 m, 0.53 mm, 20 µm)	Dynamic dilution (ISO 6145-7:2018)
METAS	January 2022	Perkin Elmer Clarus 500 GC-FID; thermal desorber TurboMatrix 350	Agilent DuraBond DB-624 (30 m, 0.32 mm, 1.8 µm)	Permeation (ISO 6145-10:2002)
VSL	September 2021, April 2022	Thermo Trace GC-FID; Markes International thermal desorber Unity 2	Agilent PoraBond U (25 m, 0.32 mm, 7 µm)	Diffusion (ISO 6145-8:2005)

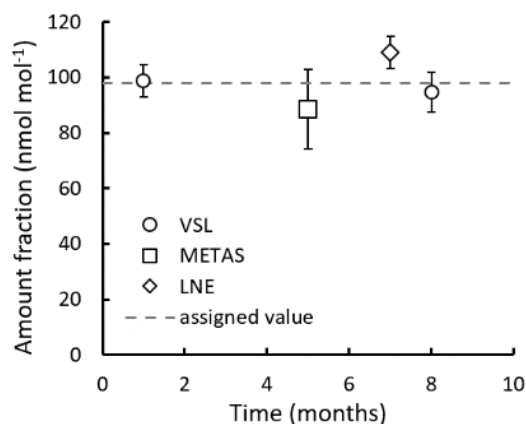

985 **Figure B1: Interlaboratory comparison results for methanol. Reported values were the average of 5 measurements, except for month 1 results, which were the average of 3 measurements. Error bars show the expanded uncertainty of the measurements (coverage factor $k = 2$). The dashed line indicates the gravimetric amount fraction of the compound.**

B.3 RGM stability evaluation

990 Results of the long-term stability evaluation for two of the prepared RGMs (VSL221418 and VSL221419) are shown in Table B4. The evaluation was carried out immediately after preparation (0–1 month). Other stability periods considered were 5–6 months, 7–8 months, 13–14 months and 18–19 months after preparation of the RGMs.

Table B4: Temporal stability of two of the gravimetric RGMs. Results are expressed as relative difference (Δ) of the average analytical value with respect to the gravimetric value. Deviations larger than $\pm 5\%$ are in bold. The stability period is indicated as the number of months after RGM preparation. NA indicates not available data due to an analytical issue during a measurement.

RGMs	Stability period (months)	$\Delta_{\text{acetaldehyde}}$ (%)	Δ_{acetone} (%)	Δ_{ethanol} (%)	$\Delta_{\text{methacrolein}}$ (%)	Δ_{methanol} (%)	Δ_{MEK} (%)	Δ_{MVK} (%)	$\Delta_{\text{n-hexane}}$ (%)
VSL221418	0–1	-2.2	0.9	-1.8	-1.3	1.8	3.3	-2.7	0.8
	5–6	NA	NA	NA	NA	NA	NA	NA	NA
	7–8	9.6	1.2	-3.5	0.7	-7.1	4.9	-3.6	0.9
	13–14	16.1	1.9	-2.6	3.7	-8.4	0.1	-6.4	1.8
	18–19	5.8	0.2	-1.4	3.4	-4.5	-0.1	-0.6	0.5
VSL221419	0–1	-0.6	0.6	-2.0	-1.4	0.2	3.1	-3.3	0.3
	5–6	-7.1	0.4	-2.5	0.9	7.6	5.7	-4.4	-0.6
	7–8	8.3	0.9	-0.2	0.7	7.1	4.6	-4.4	0.3
	13–14	14.7	1.5	0.1	3.2	5.9	-0.1	-6.2	1.2
	18–19	5.7	-4.7	-5.1	3.7	-2.5	0.2	-0.7	-4.7

995

Appendix C: Whole air sample spiking and certification

To spike the two parent cylinders with the selected [oxygenated volatile organic compounds \(OVOCs\)](#), a certified [Reference Gas Mixture \(RGM\)](#) filled into a high-pressure 5 L aluminium cylinder (D249650, VSL, Netherlands) was used. The RGM contained acetaldehyde, acetone, ethanol, methacrolein, methanol, [methyl ethyl ketone \(MEK\)](#), [methyl vinyl ketone \(MVK\)](#), benzene, n-hexane and propane in dry nitrogen at amount fractions between 500 and 1004 nmol mol⁻¹ (Table C1). The cylinder content was transferred to the parent cylinders through a cross connector joined to the outlet of the RGM cylinder (that was heated to avoid condensation), to the parent cylinders and to the vacuum pump used to evacuate the RGM cylinder. Because dilution factors of around 0.011 were expected after whole air filling of the parent cylinders, the RGM cylinder was fully evacuated into the parent cylinders to reach OVOC spiked values between 5 nmol mol⁻¹ and 10 nmol mol⁻¹ (Table C1).

Table C1: Amount fraction (x_{cyl}) and certified expanded uncertainty ($U(x_{cyl})$) of the OVOCs contained in the gas cylinder used for spiking the air samples. Estimated spiked amount fractions (x_{spiked}) and uncertainties ($U(x_{spiked})$) in the parent cylinders are also included. The coverage factor of the uncertainty is two ($k = 2$).

Compound	x_{cyl} (nmol mol ⁻¹)	$U(x_{cyl})$ (nmol mol ⁻¹)	Dilution factor (ratio)	x_{spiked} (nmol mol ⁻¹)	$U(x_{spiked})$ (nmol mol ⁻¹)
acetaldehyde	1000	40	0.011	10.61	0.60
acetone	1001	30	0.011	10.62	0.54
ethanol	866	43	0.011	9.19	0.59
methacrolein	991	30	0.011	10.52	0.53
methanol	721	36	0.011	7.65	0.49
MEK	999	100	0.011	10.60	1.15
MVK	1002	50	0.011	10.63	0.68
benzene	1004	30	0.011	10.66	0.54
n-hexane	500	15	0.011	5.31	0.27
propane	997	30	0.011	10.58	0.53

To produce the SI-traceable working standards of certified spiked whole air samples, six cylinders and 24 canisters (Table C2) were filled with the spiked whole air contained in the two parent cylinders. For that purpose, the parent cylinders were decanted into the selected cylinders and canisters to produce several identical subsamples (i.e., working standards). Four cylinders were 10 L aluminium cylinders with Experis® treatment for non-methane hydrocarbon (NMHC) VOC (Air Products Inc., PA, USA) and two were 3.6 L coated (SilcoNert® 2000) stainless steel cylinders (Swagelok Co., OH, USA). Twelve of the selected canisters were coated with Silonite™ (ten 6 L stainless steel canisters and two 15 L stainless steel canisters; Entech Instruments, CA, USA) and twelve were coated with Silcosteel® (6 L stainless steel; Restek Corporation, PA, USA).

Table C2: Air sample cylinders (cyl) and canisters (can) used to perform one of the described actions: certification, assessment and/or stability. ~~Actions performed on the vessels were~~ certification (C), assessment (A) and stability (S).

Vessel MVOC151-	Tank S/N	Tank wall material	Coating/ Treatment	Tank volume (L)	Tank final pressure ($\cdot 10^3$ hPa)	Action	Participant
001A <u>cyl</u>	APE201891	Aluminium ¹	Experis®	10	105	C	VSL ^a
001B <u>cyl</u>	APE917209	Aluminium ¹	Experis®	10	105	A	<u>Empa^b</u> , <u>DWD^c</u> , <u>IMT^d</u> , <u>UU^e</u>
001C <u>cyl</u>	APE1047602	Aluminium ¹	Experis®	10	105	C	<u>METAS^f</u>
001D <u>cyl</u>	APE152484	Aluminium ¹	Experis®	10	105	S	<u>Empa^b</u>
002A <u>cyl</u>	UD2034	Stainless steel ²	SilcoNert® 2000	3.6	98.8	C	VSL ^a , <u>METAS^f</u>
002B <u>cyl</u>	UU9013	Stainless steel ²	SilcoNert® 2000	3.6	98.8	A/S/A	<u>Empa^b/Empa^b</u> , <u>DWD^c</u> , <u>IMT^d</u> , <u>UU^e</u>
003A <u>can</u>	2566	Stainless steel ³	Silonite™	15	4.08	C	VSL ^a , <u>METAS^f</u>
003B <u>can</u>	2565	Stainless steel ³	Silonite™	15	4.08	A/S/A	<u>Empa^b/Empa^b</u> , <u>DWD^c</u> , <u>IMT^d</u> , <u>UU^e</u>
004A <u>can</u>	12938	Stainless steel ³	Silonite™	6	3.50	C	<u>METAS^f</u>
004B <u>can</u>	5690	Stainless steel ³	Silonite™	6	3.50	C	<u>METAS^f</u>
004C <u>can</u>	12200	Stainless steel ³	Silonite™	6	3.50	A	<u>IMT^d</u>
004D <u>can</u>	11330	Stainless steel ³	Silonite™	6	3.50	A	<u>UU^e</u>
004E <u>can</u>	12202	Stainless steel ³	Silonite™	6	3.50	S/A	<u>Empa^b</u>
005A <u>can</u>	5358	Stainless steel ³	Silonite™	6	3.50	S/A	<u>Empa^b</u>
005B <u>can</u>	3590	Stainless steel ³	Silonite™	6	3.50	C	VSL ^a
005C <u>can</u>	5685	Stainless steel ³	Silonite™	6	3.50	C	VSL ^a
<u>005D can</u>	<u>12204</u>	<u>Stainless steel³</u>	<u>Silonite™</u>	<u>6</u>	<u>3.50</u>	<u>A</u>	<u>DWD^c</u>
005E <u>can</u>	12201	Stainless steel ³	Silonite™	6	3.50	C	<u>METAS^f</u>
006A <u>can</u>	5032	Stainless steel ⁴	Siltek®	6	4.09	S/A	<u>Empa^b</u>
006B <u>can</u>	5040	Stainless steel ⁴	Siltek®	6	4.09	C	<u>METAS^f</u>
006C <u>can</u>	5043	Stainless steel ⁴	Siltek®	6	4.09	A	<u>IMT^d</u>
006D <u>can</u>	5033	Stainless steel ⁴	Siltek®	6	4.09	C	VSL ^a
007A <u>can</u>	5041	Stainless steel ⁴	Siltek®	6	4.16	C	<u>METAS^f</u>
007B <u>can</u>	5036	Stainless steel ⁴	Siltek®	6	4.16	C	VSL ^a
007C <u>can</u>	5045	Stainless steel ⁴	Siltek®	6	4.16	A	<u>UU^e</u>
007D <u>can</u>	5038	Stainless steel ⁴	Siltek®	6	4.16	S/A	<u>Empa^b</u>
008A <u>can</u>	5037	Stainless steel ⁴	Siltek®	6	4.08	C	<u>METAS^f</u>
<u>008B can</u>	<u>5039</u>	<u>Stainless steel⁴</u>	<u>Siltek®</u>	<u>6</u>	<u>4.08</u>	<u>A</u>	<u>DWD^c</u>
008C <u>can</u>	5030	Stainless steel ⁴	Siltek®	6	4.08	S/A	<u>Empa^b</u>
008D <u>can</u>	5034	Stainless steel ⁴	Siltek®	6	4.08	C	VSL ^a

¹Air Products, ²Swagelok, ³ENTECH Instruments, ⁴RESTEK

1025 **Table C3: Results of the homogeneity test performed on a subset of vessels filled with the SI-traceable working standards based on certified spiked whole air samples. The amount fractions (x_a) and standard deviations (SD) correspond to three replicates analysed by Empa for each vessel, including the parent cylinders (E-202A, E-202B).**

vessel	acetaldehyde (nmol mol ⁻¹)		acetone (nmol mol ⁻¹)		ethanol (nmol mol ⁻¹)		MEK (nmol mol ⁻¹)		methanol (nmol mol ⁻¹)		MVK (nmol mol ⁻¹)	
	\bar{x}_a	SD	\bar{x}_a	SD	\bar{x}_a	SD	\bar{x}_a	SD	\bar{x}_a	SD	\bar{x}_a	SD
MVOC151-001D	18.91	0.02	16.74	0.15	7.52	0.10	10.32	0.05	6.19	0.15	5.62	0.03
MVOC151-002B	20.66	0.08	16.56	0.18	7.14	0.08	10.20	0.21	6.97	0.11	6.29	0.08
MVOC151-003B	19.67	0.13	19.70	0.22	9.34	0.10	11.03	0.14	20.69*	0.27	6.46	0.06
MVOC151-004E	18.82	0.36	17.15	0.07	8.61	0.08	11.09	0.07	9.08	0.66	6.51	0.06
MVOC151-006A	21.09	0.50	17.28	0.06	7.99	0.10	11.48	0.22	9.42	0.18	6.84	0.09
MVOC151-007D	19.74	0.45	17.61	0.06	8.66	0.21	12.17	0.14	10.19	0.07	7.13	0.05
MVOC151-008C	19.76	0.32	17.27	0.08	8.96	0.08	11.78	0.09	10.22	0.10	7.00	0.03
E-202A	17.48	0.10	16.36	0.11	7.52	0.16	10.18	0.12	7.32	0.07	6.86	0.07
E-202B	17.53	0.09	17.58	0.06	7.44	0.14	10.62	0.07	5.61	0.10	6.82	0.06

*outlier

1030 Certification of the air samples was done using two [Thermal Desorption-Gas Chromatography-Flame Ionization Detector \(TD-GC-FID\) systems](#) (Table [C3C4](#)) and following the same measurement sequence: blanks, air sample, calibration standard at low amount fraction level (1–24 nmol mol⁻¹, depending on the compound), air sample and calibration standard at high amount fraction level (10–45 nmol mol⁻¹, depending on the compound). VSL calibration standards consisted of two multi-compound gas mixtures at 2 nmol mol⁻¹ and 10 nmol mol⁻¹ for acetone, methanol, ethanol, acetaldehyde, methacrolein, methyl vinyl ketone (MVK) and methyl ethyl ketone (MEK) in nitrogen. The calibration standards were prepared by diluting two gravimetric RGMs containing these OVOCs in nitrogen, as well as n-hexane and propane, at 100 nmol mol⁻¹ and 1000 nmol mol⁻¹. An additional calibration standard containing acetone, ethanol, methanol and n-hexane in clean and dry air at ca. 10 nmol mol⁻¹ was obtained by diffusion. METAS generated calibration standards containing acetaldehyde, acetone, ethanol, methacrolein, methanol and MVK in nitrogen at around 10 nmol mol⁻¹ by the permeation method (ISO 6145-10:2002 (ISO, 1040 2002)) using a magnetic suspension balance (Waters, DE, USA) and a portable generator (Pascale et al., 2017).

Table [C3C4](#): Analytical methods used for the certification of air samples

Lab	Date	Analytical instrument	Capillary column (length, internal diameter, film thickness)	Sampling method
VSL	Jul. 2021	Thermo Trace GC-FID; Markes International thermal desorber Unity 2	Agilent PoraBond U (25 m, 0.32 mm, 7 μm) Restek Stabilwax for MVK (30 m, 0.32 mm, 1.0 μm)	Autosampler (600 mL sampling volume)

METAS	Feb. 2022	Perkin Elmer Clarus 500 GC-FID; thermal desorber TurboMatrix 350	Agilent DuraBond DB-624 (30 m, 0.32 mm, 1.8 µm)	Carbograph 2 (60/80) – Carbograph 1 (40/60) – Carbosieve™ SIII (60/80) multitubed sorbent tubes (300–750 mL loading volume)
-------	-----------	--	--	--

The uncertainty of the assigned amount fraction of each compound and air sample was the result of multiplying the combined uncertainty of each air sample by the coverage factor ($k = 2$). The combined uncertainty was estimated as the combination of the uncertainty of the calibration standards, the mean standard deviation of the measurements results and the pooled standard deviation of the measurements (Eq. (B4C1)).

$$u^2(x_{sample}) = x_{sample}^2 \left(\frac{u^2(x_{cal})}{x_{cal}^2} + \frac{u^2(RF_{cal})}{RF_{cal}^2} + \frac{u^2(\bar{y}_{sample})}{\bar{y}_{sample}^2} + u^2(pooled_sd) \right) \quad (C1)$$

where,

$u(x_{sample})$: uncertainty of the assigned amount fraction of the compound in the air sample

x_{sample} : assigned amount fraction of the compound in the air sample

$u(x_{cal})$: uncertainty of the amount fraction of the compound in the calibration standard

x_{cal} : amount fraction of the compound in the calibration standard

$u(\overline{RF}_{cal})$: mean standard deviation of the response factor of the compound calibration standard

\overline{RF}_{cal} : average response factor of the compound calibration standard (average of three measurements)

$u(\bar{y}_{sample})$: mean standard deviation of the GC-FID compound responses (average of three measurements)

\bar{y}_{sample} : average GC-FID compound response (average of three measurements)


$u(pooled_sd)$: pooled standard deviation of the measurement results

Table E4C5: Analytical amount fraction values (x_a) and their expanded uncertainty (U ; coverage factor $k = 2$) obtained by the two National Metrology Institutes (NMIs) certifying the air samples: VSL and METAS.

vessel	NMI	date	methanol (nmol mol ⁻¹)		ethanol (nmol mol ⁻¹)		acetone (nmol mol ⁻¹)		methacrolein (nmol mol ⁻¹)	
			x_a	$U(x_a)$	x_a	$U(x_a)$	x_a	$U(x_a)$	x_a	$U(x_a)$
MVOC151-										
001A	VSL	07/2021	11.5	0.7	11.1	1.0	18.2	1.9	11.5	0.7
001A	VSL	09/2022	14.6	1.5	10.0	0.5	16.6	0.6	10.0	0.6
001C	METAS	02/2022	12.3	1.8	12.4	6.5	16.2	1.4	10.6	0.9
002A	VSL	07/2021	9.2*	0.5	8.7	0.8	17.9	1.8	11.0	0.7
002A	METAS	02/2022	8.1*	1.3	7.8	3.7	16.8	1.4	10.1	0.9
002A	VSL	09/2022	12.1*	2.0	6.3	0.3	17.1	1.2	9.6	0.6

003A	VSL	07/2021	21.9*	1.8	11.8*	1.1	18.9*	1.9	18.1*	1.0
003A	METAS	02/2022	15.2*	1.4	6.0*	2.7	15.4*	1.5	9.9*	0.9
005B	VSL	07/2021	8.2	0.8	10.1*	0.9	14.1*	1.4	8.5	0.5
005E	METAS	02/2022	8.9	1.5	1.4*	0.8	11.4*	1.6	8.9	1.3
007B	VSL	07/2021	4.2*	0.8	10.2*	0.9	14.3	1.4	8.7	0.5
007A	METAS	02/2022	7.5*	0.9	2.0*	1.1	12.5	1.6	9.3	0.9

1060 * values for which the criterion described in Eq. (4) was not fulfilled

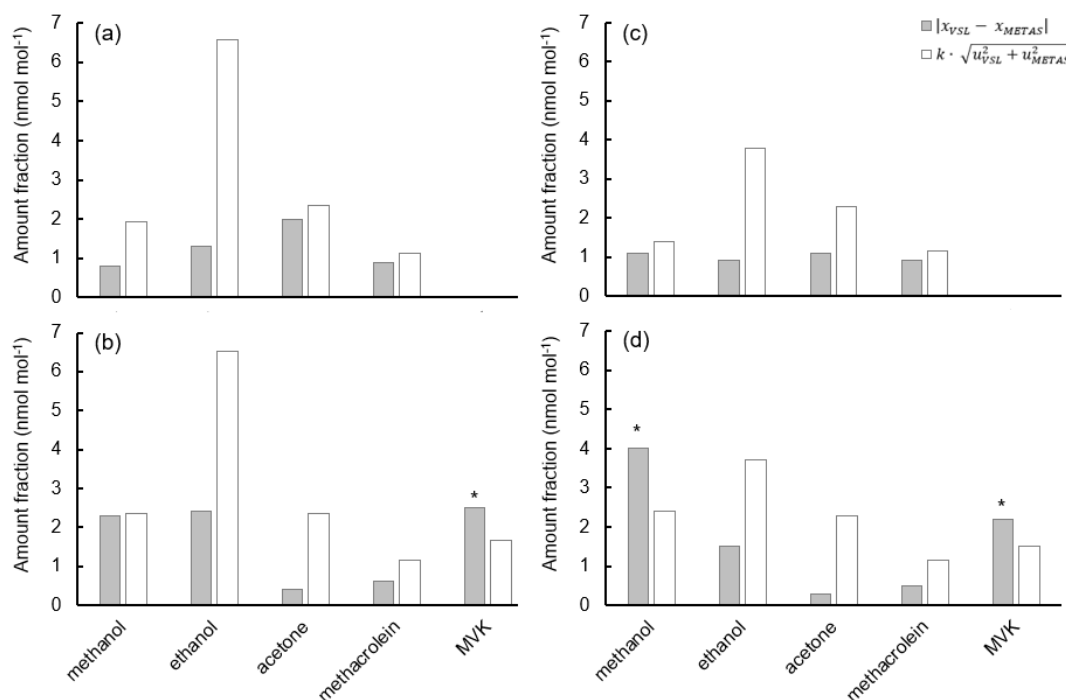

1065 **Figure C1: Representation of the consistency of the amount fraction values assigned to the 10 L Experis cylinders according the criterion described in Eq. (4). METAS measurements (vessel 001C and 002A) performed in February 2022 were compared to the VSL measurements carried out in July 2021 on vessel 001A (a) and 002A (c) and in September 2022 on vessel 001A (b) and 002A (d). The asterisks show those measurements for which the absolute difference of the measured amount fractions ($x_{VSL} - x_{METAS}$) was greater than twice (coverage factor $k = 2$) the square root of the sum of squares of the measurement standard uncertainties (u_{VSL}, u_{METAS}).**

Appendix D: Assessment of the ~~SI-traceable~~ working standards traceable to the international system of units (SI)

1070 D.1 In-house working standards

The analytical instruments selected to assess the SI-traceable working standards (Appendix A; Table A1) were calibrated with in-house working standards generated using different methods.

1075 The [Thermal Desorption-Gas Chromatography-Flame Ionization Detector/Mass Spectrometry \(TD-GC-FID/MS\)](#) system used by DWD ([Deutscher Wetterdienst](#)) to assess the working standards based on certified spiked whole air samples was calibrated using one of the [Reference Gas Mixtures \(RGMs\)](#) prepared by [the national metrology institute \(NMI\) of the Netherlands \(VSL\)](#) for this work ([oxygenated volatile organic compounds \(OVOCs\)](#) in nitrogen at $100 \text{ nmol mol}^{-1}$) ~~without further dilution. The RGM was diluted with dry nitrogen to achieve amount fraction levels $< 10 \text{ nmol mol}^{-1}$.~~ In addition, DWD TD-GC-FID/MS system was calibrated using a primary reference material containing 30 non-methane hydrocarbons (NMHCs) considered ozone precursors [at amount fraction levels of \$2 \text{ nmol mol}^{-1}\$](#) (NPL NMHC standard; Grenfell et al., 2010). ~~NPL NMHC standard was diluted at 1 nmol mol^{-1} amount fraction for the calibration.~~ The same type of standard (NPL NMHC) ~~at 2 nmol mol^{-1} amount fraction~~ was used to calibrate Empa TD-GC-FID.

1080 The ion transmission curves of both [Proton Transfer Reaction-Time of Flight-Mass Spectrometry \(PTR-ToF-MS\)](#) were determined using a SI-traceable certified reference material produced by [the National Physical Laboratory \(NPL\), the NMI of the United Kingdom \(NPL PTR-MS standard\)](#) (Worton et al., 2023) as in-house working standards ([NPL PTR-MS standard](#)). 1085 The in-house working standards (NPL D961410 used by [Institute Mines-Télécom \(IMT\)](#) and D961397 used by [Utrecht University \(UU\)](#)) contained 20 compounds at amount fractions around $1 \mu\text{mol mol}^{-1}$ covering a mass spectrum from m/z 33 to m/z 671. Prior [to](#) instrument calibration, the in-house working standards were diluted with zero air (i.e. dry nitrogen) down to amount fractions $< 10 \text{ nmol mol}^{-1}$.

1090 VSL TD-GC-FID was calibrated using RGMs based on the diffusion method (dynamic preparation method ISO 6145-8) as in-house working standards for acetone, ethanol, methacrolein, methanol, [methyl ethyl ketone \(MEK\)](#) and [methyl vinyl ketone \(MVK\)](#). For acetaldehyde, an in-house working standard was obtained by dynamic dilution of a $1 \mu\text{mol mol}^{-1}$ multi-component RGM containing acetaldehyde, acetone, ethanol, methacrolein, methanol, MEK, MVK and propane in nitrogen. Three to six in-house working standards were prepared in the range $4\text{--}20 \text{ nmol mol}^{-1}$.

1095 **D.2 Measurement procedure for assessing the working standards based on dynamic dilution of RGMs**

Samples were prepared by dynamic dilution of RGMs. VSL, IMT and UU generated two samples. VSL set the same dilution factor for both samples (10 times dilution to obtain OVC amount fractions close to 10 nmol mol^{-1}), while [the Swiss Federal Laboratories for Materials Science and Technology \(Empa\)](#) and IMT used different dilution factors (Table D1). UU prepared six samples using different dilution factors (Table D1).

1100 Before performing the measurement sequence, VSL sampled and analysed 15 times the pure nitrogen used for dilution to clean the analytical system and to assess the system blank. Each in-house standard (three to six in total) and sample (i.e., SI-traceable working standard) was sampled at a flow rate of 20 mL min^{-1} for 30 minutes.

1105 Empa ran five to ten GC runs with a sample of similar humidity level and composition that the matrix gas to condition the GC-FID. After the conditioning, six consecutive runs without injecting any sample were measured to estimate the system blank. Then, six in-house working standard runs were followed by six runs for each sample (i.e., SI-traceable working

standard). In-house working standard and blank runs (12 runs in total) were repeated after the last sample measurement. Sampling volume was set at 300 mL (20 minutes at 15 mL min⁻¹).

1110 IMT measurement sequence started with 30 minutes of zero air sampling to quantify background signals and to verify signal stability. The zero air was obtained using a catalytic converter containing platinum wool (high sensitivity catalyst for TOC analyser, Shimadzu Corporation, Japan), which was heated up to 350 °C. Blank measurements were performed before and after each new sample test and calibration. After the first blank measurements, the calibration took place by analysing in-house working standards during 60–90 minutes. The in-house working standards (5 mL min⁻¹) were diluted with a zero-air flow rate of 1 L min⁻¹. Flows were regulated by MFCs in a Gas Calibration Unit (GCU, Ionico Analytik GmbH, Austria). Then, each sample was analysed for 90 minutes. The same sampling line coated with SilcoNert® 1000 and sampling flow rate of 100 mL min⁻¹ were used for blanks, calibration standards and samples.

1115 UU measured each sample 2–4 times for at least 30 seconds. Before and after each sample measurement, UU analysed blanks (i.e., zero air produced by a heated platinum catalyst) and the in-house working standard (NPL-PTR-MS standard). Blanks, in-house working standards and samples were injected through a sample loop (250 µL volume) according the procedure described in Holzinger et al. (2019). The in-house working standards (loop flow of 10 mL min⁻¹) were diluted with a zero-air flow of 240 mL min⁻¹. Sample flows, depending on the pressure in cylinders and canisters, were produced between 80 mL min⁻¹ and 300 mL min⁻¹.

D.3 Measurement procedure for assessing working standards based on certified whole air samples

The same air sample cylinders were assessed by the participants (round-robin comparison). However, different canisters were sent to the participants because of the low sample volume, which was enough only for one analysis (Table C2). Participants followed a similar measurement sequence than the measurement procedure described for the SI-traceable working standards based on RGM dilution. After some blank measurements (six times for GC-FID and 30 minutes for PTR-ToF-MS), in-house working standards were measured at minimum two amount fraction levels (six times per level for GC-FID and for PTR-ToF-MS, IMT measured for 90 min and UU for 1 min). Samples were measured between calibration levels (6 times each sample for GC-FID and 90 minutes per sample for PTR-ToF-MS measurements at IMT and 1 min at UU). Blank measurements were performed again after the second amount fraction level of the calibration.

1135 **Table D1: ~~VeRD1-Flow rates (in mL min⁻¹) and relative expanded uncertainty (coverage factor $k = 2$) of the dilution systems used to dilute VSL SI-traceable RGM during the assessment of SI-traceable working standards by each laboratory. Gas flow rates correspond to the flow rate of VSL SI-traceable RGM (q_{v_RGM}), first-step dilution flow rate (q_{v_d1}), split flow rate (q_{v_sp}) and second-step dilution flow (q_{v_d2}). ~~The relative expanded uncertainties (coverage factor $k = 2$) of the flow rates are shown between brackets. The assigned amount fractions of the selected compounds are shown together with their expanded uncertainties ($k = 2$), both expressed in nmol mol⁻¹.~~~~**

	q_{v_RGM} $\pm U$ (%)	q_{v_d1} $\pm U$ (%)	q_{v_sp} $\pm U$ (%)	q_{v_d2} ($\pm 0.3\%$)	$x_{acetaldehyde}$ $\pm U$	$x_{acetone}$ $\pm U$	$x_{methanol}$ $\pm U$	x_{MEK} $\pm U$	x_{MVK} $\pm U$
VSL1	109 \pm 0.5	917 \pm 0.5	-	-	NA	10.58 \pm 0.38	10.57 \pm 0.64	10.56 \pm 0.34	10.74 \pm 0.38
VSL2	109 \pm 0.5	913 \pm 0.5	-	-	10.87 \pm 0.99	10.59 \pm 0.38	10.58 \pm 0.64	10.57 \pm 0.34	10.74 \pm 0.38
IMT1	100 \pm 0.4	520 \pm 0.3	-	-	16.4 \pm 1.5	16.12 \pm 0.59	16.96 \pm 0.81	15.87 \pm 0.56	16.13 \pm 0.94
IMT2	60 \pm 0.4	520 \pm 0.3	-	-	10.56 \pm 0.99	10.34 \pm 0.38	10.88 \pm 0.52	10.18 \pm 0.35	10.34 \pm 0.61
UU1	45 \pm 0.4	1455 \pm 0.3	100 \pm 0.5	1400 \pm 0.3	0.30 \pm 0.09	0.21 \pm 0.02	0.22 \pm 0.02	0.20 \pm 0.01	0.20 \pm 0.02
UU2	90 \pm 0.4	1400 \pm 0.3	100 \pm 0.5	1410 \pm 0.3	0.49 \pm 0.09	0.40 \pm 0.02	0.42 \pm 0.03	0.38 \pm 0.02	0.39 \pm 0.03
UU3	12 \pm 0.4	1488 \pm 0.3	-	-	0.91 \pm 0.11	0.81 \pm 0.04	0.85 \pm 0.05	0.79 \pm 0.03	0.80 \pm 0.05
UU4	24 \pm 0.4	1476 \pm 0.3	-	-	1.72 \pm 0.18	1.61 \pm 0.06	1.69 \pm 0.09	1.58 \pm 0.06	1.60 \pm 0.10
UU5	30 \pm 0.4	1470 \pm 0.3	-	-	2.12 \pm 0.21	2.01 \pm 0.08	2.11 \pm 0.11	1.97 \pm 0.07	2.00 \pm 0.12
UU6	60 \pm 0.4	1440 \pm 0.3	-	-	4.14 \pm 0.39	4.00 \pm 0.16	4.21 \pm 0.21	3.94 \pm 0.14	4.00 \pm 0.24
Empa1	14 \pm 0.4	650 \pm 0.3	-	-	2.34 \pm 0.23	2.14 \pm 0.10	2.18 \pm 0.15	2.18 \pm 0.09	2.22 \pm 0.08
Empa2	20 \pm 0.4	1450 \pm 0.3	-	-	1.51 \pm 0.15	1.35 \pm 0.07	1.37 \pm 0.10	1.37 \pm 0.06	1.40 \pm 0.06

D.4 IMT measured amount fractions

1140 IMT estimated the amount fractions of the selected OVOCs according to the calibration approach described in de Gouw and Warneke (2007) and following Eq. (D1). In practice, a sensitivity factor of H_3O^+ normalized to 10^6 cps ($S_N(RH^+)$) is derived for each targeted compound during calibration experiments. This sensitivity factor comprises the parameters: k_{PTR} , Δt , $T(RH^+)$ and $T(H_3O^+)$. The approach used in de Gouw and Warneke (2007) to account for humidity-dependent sensitivities was applied in this work.

$$1145 \quad x_i = \frac{1}{k_{PTR} \cdot \Delta t} \cdot \frac{I(RH^+)}{T(RH^+)} \cdot \left(\frac{I(H_3O^+)}{T(H_3O^+)} \right)^{-1} = \frac{I(RH^+) \cdot 10^6}{I(H_3O^+) \cdot S_N(RH^+)} \quad (D1)$$

where,

x_i : amount fraction of the compound R (i.e., OVOC under study)

k_{PTR} : proton-transfer-reaction rate coefficient of $R + H_3O^+ \rightarrow RH^+ + H_2O$

Δt : reaction time in the drift tube

1150 $I(RH^+)$: observed signal (counts per second, cps) for the protonated ion RH^+

$I(H_3O^+)$: observed signal (cps) for the reagent ion H_3O^+

$T(RH^+)$: transmission efficiency for RH^+

$T(H_3O^+)$: transmission efficiency for H_3O^+

$S_N(RH^+)$: sensitivity factor of H_3O^+ normalized to 10^6 cps.

Sources of uncertainty associated to the measured amount fractions included the precision of the system and the calibration accuracy. The uncertainty linked to the precision of the system (u_{prec}) was calculated according Eq. (D2). The uncertainty associated to the calibration accuracy (u_{cal_acc}) was estimated applying Eq. (D3).

$$1160 \quad u_{prec} = \frac{\sqrt{I_m(RH^+) + I_z(RH^+)}}{S_N(RH^+) \cdot I(H_3O^+)} \cdot 10^6 \quad (D2)$$

where,

u_{prec} : measurement precision expressed as a amount fraction

$I_m(RH^+)$: RH^+ signal (cps) observed when a sample was measured

1165 $I_z(RH^+)$: RH^+ signal (cps) observed when zeroing the instrument

$I(H_3O^+)$: observed signal (cps) for the reagent ion H_3O^+

$S_N(RH^+)$: sensitivity factor of H_3O^+ normalized to 10^6 cps

$$1170 \quad \frac{u_{cal_acc}}{x_{cal}} = \sqrt{\left(\frac{u(x_{cyl})}{x_{cyl}}\right)^2 + \frac{1}{(q_{v_cal} + q_{v_dil})^2} \cdot \left(\frac{q_{v_dil}^2}{q_{v_cal}^2} \cdot u(q_{v_cal})^2 + u(q_{v_dil})^2\right)} \quad (D3)$$

1170 where,

u_{cal_acc} : relative combined uncertainty of the calibration accuracy

x_{cal} : OVOC amount fraction generated after dilution of the calibration standard

$u(x_{cyl})$: standard uncertainty of the OVOC amount fraction in the calibration standard (calibration certificate)

x_{cyl} : OVOC amount fraction in the calibration standard (calibration certificate)

1175 q_{v_cal} : flow rate of the calibration standard

q_{v_dil} : flow rate of the dilution gas

$u(q_{v_cal})$: standard uncertainty of the calibration standard flow rate

$u(q_{v_dil})$: standard uncertainty of the dilution gas flow rate

1180 **D.5 Uncertainty of the measurements performed to assess the SI-traceable working standards**

Tables D2 and D3 show the amount fraction results of the measurements performed by the participants on the assessment of the SI-traceable working standards for each of the selected OVOCs.

1185 **Table D2: Amount fractions (x_i) of the selected OVOCs measured by the participants on the assessment of the SI-traceable working standards based on the dilution of RGMs. Expanded uncertainty (U, coverage factor $k = 2$) of the measurements are indicated together with the amount fractions, both expressed in nmol mol^{-1} .**

<u>Sample</u>	<u>analytical</u> <u>method</u>	<u>calibration</u> <u>standard</u>	<u>$x_{\text{acetaldehyde}}$</u> <u>$\pm U$</u>	<u>x_{acetone}</u> <u>$\pm U$</u>	<u>x_{methanol}</u> <u>$\pm U$</u>	<u>x_{MEK}</u> <u>$\pm U$</u>	<u>x_{MVK}</u> <u>$\pm U$</u>
<u>IMT1</u>	<u>PTR-ToF-MS</u>	<u>NPL PTR-MS</u>	<u>26.2±3.9</u>	<u>19.3±4.4</u>	<u>17.3±3.9</u>	<u>18.3±4.1</u>	<u>NA*</u>
<u>IMT2</u>	<u>PTR-ToF-MS</u>	<u>NPL PTR-MS</u>	<u>17.0±3.8</u>	<u>12.4±2.8</u>	<u>12.4±2.8</u>	<u>11.9±2.7</u>	<u>NA*</u>
<u>UU1</u>	<u>PTR-ToF-MS</u>	<u>NPL PTR-MS</u>	<u>0.23±0.03</u>	<u>0.22±0.03</u>	<u>0.12±0.02</u>	<u>0.17±0.03</u>	<u>NA*</u>
<u>UU2</u>	<u>PTR-ToF-MS</u>	<u>NPL PTR-MS</u>	<u>0.42±0.06</u>	<u>0.40±0.06</u>	<u>0.23±0.03</u>	<u>0.35±0.05</u>	<u>NA*</u>
<u>UU3</u>	<u>PTR-ToF-MS</u>	<u>NPL PTR-MS</u>	<u>0.75±0.11</u>	<u>0.70±0.11</u>	<u>0.46±0.07</u>	<u>0.58±0.09</u>	<u>NA*</u>
<u>UU4</u>	<u>PTR-ToF-MS</u>	<u>NPL PTR-MS</u>	<u>1.65±0.25</u>	<u>1.64±0.25</u>	<u>1.27±0.19</u>	<u>1.47±0.22</u>	<u>NA*</u>
<u>UU5</u>	<u>PTR-ToF-MS</u>	<u>NPL PTR-MS</u>	<u>1.97±0.3</u>	<u>1.81±0.27</u>	<u>0.85±0.13</u>	<u>1.49±0.22</u>	<u>NA*</u>
<u>UU6</u>	<u>PTR-ToF-MS</u>	<u>NPL PTR-MS</u>	<u>4.03±0.6</u>	<u>3.56±0.53</u>	<u>1.50±0.23</u>	<u>2.93±0.44</u>	<u>NA*</u>
<u>Empa1</u>	<u>TD-GC-FID</u>	<u>NPL NMHC</u>	<u>2.42±0.73</u>	<u>1.35±0.62</u>	<u>2.99±0.91</u>	<u>1.63±0.64</u>	<u>1.40±0.43</u>
<u>Empa2</u>	<u>TD-GC-FID</u>	<u>NPL NMHC</u>	<u>1.45±0.45</u>	<u>1.11±0.38</u>	<u>2.03±0.62</u>	<u>0.99±0.39</u>	<u>0.83±0.26</u>
<u>VSL1</u>	<u>TD-GC-FID</u>	<u>VSL diffusion</u>	<u>NA</u>	<u>10.79±0.35</u>	<u>10.81±0.37</u>	<u>10.54±0.34</u>	<u>10.55±0.35</u>
<u>VSL2</u>	<u>TD-GC-FID</u>	<u>VSL diffusion</u>	<u>11.2±1.2</u>	<u>10.88±0.35</u>	<u>10.68±0.37</u>	<u>10.58±0.34</u>	<u>10.38±0.34</u>

* MVK data not available because PTR-ToF-MS can only provide the sum of MVK and methacrolein.

1190

Table D3: Amount fractions (x_i) of the selected OVOCs measured by the participants on the assessment of the SI-traceable working standards based certified spiked whole air samples. Expanded uncertainty (U , coverage factor $k = 2$) of the measurements are indicated together with the amount fractions, both expressed in nmol mol^{-1} . The analytical methods correspond to TD-GC-FID (AM1) and to PTR-ToF-MS (AM2) and the calibration standards to NPL NMHC standard (Std1), METAS permeation standard (Std2), VSL diffusion standard (Std3) and NPL PTR-MS standard (Std4).

<u>Participant</u>	<u>Vessel</u>	<u>analytical</u> <u>method</u>	<u>calibration</u> <u>standard</u>	<u>x_{acetone}</u> <u>$\pm U$</u>	<u>x_{methanol}</u> <u>$\pm U$</u>	<u>x_{MEK}</u> <u>$\pm U$</u>	<u>x_{MVK}</u> <u>$\pm U$</u>
<u>DWD</u>	<u>cyl-001B</u>	<u>AM1</u>	<u>Std1</u>	<u>15.98±0.97</u>	<u>NA</u>	<u>11.88±0.86</u>	<u>8.43±0.62</u>
<u>METAS</u>	<u>cyl-001C</u>	<u>AM1</u>	<u>Std2</u>	<u>16.2±1.4</u>	<u>12.3±1.8</u>	<u>NA</u>	<u>8.1±1.5</u>
<u>VSL</u>	<u>cyl-001A</u>	<u>AM1</u>	<u>Std3</u>	<u>16.60±0.60</u>	<u>14.6±1.5</u>	<u>11.20±0.50</u>	<u>10.60±0.60</u>
<u>Empa</u>	<u>cyl-001D</u>	<u>AM1</u>	<u>Std1</u>	<u>15.99±0.88</u>	<u>13.69±0.84</u>	<u>10.83±0.62</u>	<u>5.32±0.28</u>
<u>IMT</u>	<u>cyl-001B</u>	<u>AM2</u>	<u>Std4</u>	<u>14.7±3.3</u>	<u>17.7±4.0</u>	<u>10.1±2.3</u>	<u>NA*</u>
<u>UU</u>	<u>cyl-001B</u>	<u>AM2</u>	<u>Std4</u>	<u>16.90±0.68</u>	<u>28.4±4.6</u>	<u>11.00±0.66</u>	<u>NA*</u>
<u>DWD</u>	<u>cyl-002B</u>	<u>AM1</u>	<u>Std1</u>	<u>16.7±1.1</u>	<u>NA</u>	<u>11.82±0.86</u>	<u>7.86±0.60</u>
<u>METAS</u>	<u>cyl-002A</u>	<u>AM1</u>	<u>Std2</u>	<u>16.8±1.4</u>	<u>8.1±1.3</u>	<u>NA</u>	<u>7.3±1.4</u>

VSL	cyl-002A	AM1	Std3	17.1±1.2	12.1±2.0	10.90±0.60	9.5±0.6
Empa	cyl-002B	AM1	Std1	17.9±1.1	12.22±0.72	12.70±0.74	NA*
IMT	cyl-002B	AM2	Std4	15.6±3.6	8.0±1.9	10.2±2.3	NA*
UU	cyl-002A	AM2	Std4	16.90±0.34	7.4±0.8	9.30±0.37	8.27±0.46
DWD	can-005D	AM1	Std1	16.96±0.92	NA	11.97±0.64	8.02±0.46
METAS	can-004A	AM1	Std2	13.3±2.6	8.8±1.2	NA	6.6±1.4
VSL	can-005B	AM1	Std3	14.1±1.4	8.2±0.8	10.4±0.9	NA
UU	can-004D	AM2	Std4	16.80±0.34	13.50±0.81	9.50±0.57	NA*
IMT	can-004C	AM2	Std4	17.1±3.9	26.6±6.0	11.4±2.6	NA*
Empa	can-005A	AM1	Std1	18.2±1.4	17.1±2.0	12.9±1.1	8.27±0.62
DWD	can-008B	AM1	Std1	24.9±1.4	NA	15.60±0.84	7.06±0.40
METAS	can-007A	AM1	Std2	12.5±1.6	8.00±0.90	NA	6.7±1.4
VSL	can-007B	AM1	Std3	14.3±1.4	4.20±0.80	10.30±0.90	NA
UU	can-007C	AM2	Std4	29.9±2.4	22.60±0.90	15.5±1.9	NA*
Empa	can-007D	AM2	Std1	16.47±0.90	14.19±0.88	14.45±0.88	7.53±0.40

* MVK data not available because PTR-ToF-MS can only provide the sum of MVK and methacrolein.

Data availability

Data will be made available after acceptance in MetClim VOC Zenodo community

(https://zenodo.org/communities/19env06_metclimvoc/about).

1200 Author contribution

SR, PS, CP, MI-G, AB, TS, AC and RH designed the study. AB, JL and SP prepared the reference gas mixtures (RGMs) used for generated SI-traceable working standards based on the dilution of RGMs. PS, MH and MKV prepared the SI-traceable working standards based on air samples, which were certified by AB and MI-G. AA designed and coordinated the development of the VerDi dilution system, with supervision of CP. For the assessment measurements, ES, SD, TS and RH performed the PTR-ToF-MS measurements and PS, MH, AB and AC performed the TD-GC-FID measurements. AB, JL, CS and MI-G carried out the OVOC RGM comparison. MI-G wrote the paper with assistance from all authors, who provided information on instrument description and data. All authors reviewed and approved the latest version of the paper.

Competing interests

The contact author has declared that none of the author has any competing interests.

1210 Acknowledgments

We acknowledge the technical staff at ACTRIS CiGaS units (IMT Nord Europe, Empa, DWD) and the participating laboratories for their support. Special thanks to the Tropospheric Ozone Precursors Focus Working group for their valuable comments to improve the paper. Utrecht University received support from the Ruisdael Observatory, a scientific infrastructure co-financed by the Dutch Research Council (NOW, grant number 184.034.015).

1215 Financial support

This research was performed within the framework of the project 19ENV06 MetClim VOC, which has received funding from the EMPIR programme cofinanced by the Participating States and from the European Union's Horizon 2020 research and innovation programme.

References

- 1220 Alink, A. and Van Der Veen, A. M. H.: Uncertainty calculations for the preparation of primary gas mixtures Part 1: Gravimetry, *Metrologia*, 37, 641–650, 2000.
- Apel, E. C., Calvert, J. G., Greenberg, J. P., Riemer, D., Zika, R., Kleindienst, T. E., Lonneman, W. A., Fung, K., and Fujita, E.: Generation and validation of oxygenated volatile organic carbon standards for the 1995 Southern Oxidants Study Nashville Intensive, *Journal of Geophysical Research Atmospheres*, 103, 22281–22294, <https://doi.org/10.1029/98JD01383>, 1998.
- 1225 Atkinson, R.: Atmospheric chemistry of VOCs and NO_x, *Atmos Environ*, 34, 2063–2101, [https://doi.org/10.1016/S1352-2310\(99\)00460-4](https://doi.org/10.1016/S1352-2310(99)00460-4), 2000.
- Bates, K. H., Jacob, D. J., Wang, S., Hornbrook, R. S., Apel, E. C., Kim, M. J., Millet, D. B., Wells, K. C., Chen, X., Brewer, J. F., Ray, E. A., Commane, R., Diskin, G. S., and Wofsy, S. C.: The Global Budget of Atmospheric Methanol: New Constraints on Secondary, Oceanic, and Terrestrial Sources, *Journal of Geophysical Research: Atmospheres*, 126, <https://doi.org/10.1029/2020JD033439>, 2021.
- 1230 De Bièvre, P. and Taylor, P. D. P.: Traceability to the SI of amount-of-substance measurements: From ignoring to realizing, a chemist's view, *Metrologia*, 34, 67–75, <https://doi.org/10.1088/0026-1394/34/1/10>, 1997.

- 1235 Boucher, O., Randall, D., Artaxo, P., Bretherton, C., Feingold, G., Forster, P., Kerminen, V.-M., Kondo, Y., Liao, H.,
Lohmann, U., Rasch, P., Satheesh, S.K., Sherwood, S., Stevens, B., and Zhang, X. Y.: Clouds and aerosols in *Climate
Change 2013: The Physical Science Basis. Contribution of Working Group I to the Fifth Assessment Report of the
Intergovernmental Panel on Climate Change* (eds Stocker, T.F., Qin, D., Plattner, G.-K., Tignor, M., Allen, S.K.,
Doschung, J., Nauels, A., Xia, Y., Bex, V., and Midgley, P. M.), Cambridge University Press, 571–657,
<https://doi.org/10.1017/CBO9781107415324.016> (2013).
- 1240 Brewer, J. F., Fischer, E. V., Commane, R., Wofsy, S. C., Daube, B. C., Apel, E. C., Hills, A. J., Hornbrook, R. S., Barletta,
B., Meinardi, S., Blake, D. R., Ray, E. A., and Ravishankara, A. R.: Evidence for an Oceanic Source of Methyl Ethyl
Ketone to the Atmosphere, *Geophys Res Lett*, 47, <https://doi.org/10.1029/2019GL086045>, 2020.
- Brewer, P. J., Brown, R. J. C., Tarasova, O. A., Hall, B., Rhoderick, G. C., and Wielgosz, R. I.: SI traceability and scales for
underpinning atmospheric monitoring of greenhouse gases, *Metrologia*, 55, S174–S181, <https://doi.org/10.1088/1681->
1245 [7575/aad830](https://doi.org/10.1088/1681-7575/aad830), 2018.
- Brown, A. S., Milton, M. J. T., Brookes, C., Vargha, G. M., Downey, M. L., Uehara, S., Augusto, C. R., Fioravante, A. de L.,
Sobrinho, D. G., Dias, F., Woo, J. C., Kim, B. M., Kim, J. S., Mace, T., Fükö, J. T., Qiao, H., Guenther, F., Rhoderick, J.,
Gameson, L., Botha, A., Tshilongo, J., Ntsasa, N. G., Val'ková, M., Durisova, Z., Kustikov, Y., Konopelko, L., Fatina, O.,
and Wessel, R.: Final report on CCQM-K93: Preparative comparison of ethanol in nitrogen, *Metrologia*, 50, 08025–08025,
1250 <https://doi.org/10.1088/0026-1394/50/1A/08025>, 2013.
- Collins, W. J., Derwent, R. G., Johnson, C. E., and Stevenson, D. S.: The oxidation of organic compounds in the troposphere
and their global warming potentials, *Clim Change*, 52, 453–479, <https://doi.org/10.1023/A:1014221225434>, 2002.
- Cooper, O. R., Parrish, D. D., Ziemke, J., Balashov, N. V., Cupeiro, M., Galbally, I. E., Gilge, S., Horowitz, L., Jensen, N. R.,
Lamarque, J. F., Naik, V., Oltmans, S. J., Schwab, J., Shindell, D. T., Thompson, A. M., Thouret, V., Wang, Y., and
1255 Zbinden, R. M.: Global distribution and trends of tropospheric ozone: An observation-based review, *Elem Sci Anth*, 2,
[000029](https://doi.org/10.12952/journal.elementa.000029), <https://doi.org/10.12952/journal.elementa.000029>, 2014.
- [Coplen, T.B., Holden, N.E., Ding, T., Meijer, H.A.J., Vogl, J., and Zhu, X. The table of standard atomic weights – An exercise
in consensus. *Rapid Communication in Mass Spectrometry*, 36, e8864, <https://doi.org/10.1002/rcm.8864>, 2020.](https://doi.org/10.1002/rcm.8864)
- 1260 Van Dingenen, R., Dentener, F. J., Raes, F., Krol, M. C., Emberson, L., and Cofala, J.: The global impact of ozone on
agricultural crop yields under current and future air quality legislation, *Atmos Environ*, 43, 604–618,
<https://doi.org/10.1016/j.atmosenv.2008.10.033>, 2009.

Faiola, C. L., Erickson, M. H., Fricaud, V. L., Jobson, B. T., and Vanreken, T. M.: Quantification of biogenic volatile organic compounds with a flame ionization detector using the effective carbon number concept, *Atmos Meas Tech*, 5, 1911–1923, <https://doi.org/10.5194/amt-5-1911-2012>, 2012.

1265 Fischer, E. V., Jacob, D. J., Millet, D. B., Yantosca, R. M., and Mao, J.: The role of the ocean in the global atmospheric budget of acetone, *Geophys Res Lett*, 39, <https://doi.org/10.1029/2011GL050086>, 2012.

Fischer, E. V., Jacob, D. J., Yantosca, R. M., Sulprizio, M. P., Millet, D. B., Mao, J., Paulot, F., Singh, H. B., Roiger, A., Ries, L., Talbot, R. W., Dzepina, K., and Pandey Deolal, S.: Atmospheric peroxyacetyl nitrate (PAN): A global budget and source attribution, *Atmos Chem Phys*, 14, 2679–2698, <https://doi.org/10.5194/acp-14-2679-2014>, 2014.

1270 [Fleming, Z. L., Doherty, R. M., Von Schneidmesser, E., Malley, C. S., Cooper, O. R., Pinto, J. P., Colette, A., Xu, X., Simpson, D., Schultz, M. G., Lefohn, A. S., Hamad, S., Moolla, R., Solberg, S., and Feng, Z.: Tropospheric Ozone Assessment Report: Present-day ozone distribution and trends relevant to human health, *Elementa*, 6, <https://doi.org/10.1525/elementa.273>, 2018.](https://doi.org/10.1525/elementa.273)

Galbally, I. E., Schultz, M. G., Buchmann, B., Gilge, S., Guenther, F., Koide, H., Oltmans, S., Patrick, L., Scheel, H.-E., Smit, H., Steinbacher, M., Steinbrecht, W., Tarasova, O., Viallon, J., Volz-Thomas, A., Weber, M., Wielgosz, R., and Zellweger, C.: Guidelines for Continuous Measurement of Ozone in the Troposphere, GAW Report No 209, Publication WMO-No. 1110, WMO, Geneva, 1–76 pp., 2013.

1280 [Gaudel, A., Cooper, O. R., Ancellet, G., Barret, B., Boynard, A., Burrows, J. P., Clerbaux, C., Coheur, P. F., Cuesta, J., Cuevas, E., Doniki, S., Dufour, G., Ebojic, F., Foret, G., Garcia, O., Granados-Muñoz, M. J., Hannigan, J. W., Hase, F., Hassler, B., Huang, G., Hurtmans, D., Jaffe, D., Jones, N., Kalabokas, P., Kerridge, B., Kulawik, S., Latter, B., Leblanc, T., Le Flochmoën, E., Lin, W., Liu, J., Liu, X., Mahieu, E., McClure-Begley, A., Neu, J. L., Osman, M., Palm, M., Petetin, H., Petropavlovskikh, I., Querel, R., Rapp, N., Rozanov, A., Schultz, M. G., Schwab, J., Siddans, R., Smale, D., Steinbacher, M., Tanimoto, H., Tarasick, D. W., Thouret, V., Thompson, A. M., Trickl, T., Weatherhead, E., Wespes, C., Worden, H. M., Vigouroux, C., Xu, X., Zeng, G., and Ziemke, J.: Tropospheric Ozone Assessment Report: Present-day distribution and trends of tropospheric ozone relevant to climate and global atmospheric chemistry model evaluation, *Elementa*, 6, <https://doi.org/10.1525/elementa.291>, 2018.](https://doi.org/10.1525/elementa.291)

1285 Goldstein, A. H. and Galbally, I. E.: Known and Unexplored Organic Constituents in the Earth's Atmosphere, *Environ Sci Technol*, 41, 1502–1800, <https://doi.org/10.1021/es072476p>, 2007.

de Gouw, J. and Warneke, C.: Measurements of volatile organic compounds in the earth's atmosphere using proton-transfer-reaction mass spectrometry, *Mass Spectrom Rev*, 26, 223–257, <https://doi.org/10.1002/mas.20119>, 2007.

1290

- Grenfell, R. J. P., Milton, M. J. T., Harling, A. M., Vargha, G. M., Brookes, C., Quincey, P. G., and Woods, P. T.: Standard mixtures of ambient volatile organic compounds in synthetic and whole air with stable reference values, *Journal of Geophysical Research Atmospheres*, 115, D14302, <https://doi.org/10.1029/2009JD012933>, 2010.
- 1295 Güttler, B. and Richter, W.: Traceability of chemical measurement results, *Chimia (Aarau)*, 63, 619–623, <https://doi.org/10.2533/chimia.2009.619>, 2009.
- Hoerger, C. C., Claude, A., Plass-Duelmer, C., Reimann, S., Eckart, E., Steinbrecher, R., Aalto, J., Arduini, J., Bonnaire, N., Cape, J. N., Colomb, A., Connolly, R., Diskova, J., Dumitrean, P., Ehlers, C., Gros, V., Hakola, H., Hill, M., Hopkins, J. R., Jäger, J., Junek, R., Kajos, M. K., Klemp, D., Leuchner, M., Lewis, A. C., Locoge, N., Maione, M., Martin, D., Michl, K., Nemitz, E., O'Doherty, S., Pérez Ballesta, P., Ruuskanen, T. M., Sauvage, S., Schmidbauer, N., Spain, T. G., Straube, E., Vana, M., Vollmer, M. K., Wegener, R., and Wenger, A.: ACTRIS non-methane hydrocarbon intercomparison experiment in Europe to support WMO GAW and EMEP observation networks, *Atmos Meas Tech*, 8, 2715–2736, <https://doi.org/10.5194/amt-8-2715-2015>, 2015.
- 1300 Holzinger, R., Joe Acton, W. F., Bloss, W. W., Breitenlechner, M., Crilley, L. L., Dusanter, S., Gonin, M., Gros, V., Keutsch, F. F., Kiendler-Scharr, A., Kramer, L. L., Krechmer, J. J., Languille, B., Locoge, N., Lopez-Hilfiker, F., Materi, D., Moreno, S., Nemitz, E., Quéléver, L. L., Sarda Esteve, R., Sauvage, S., Schallhart, S., Sommariva, R., Tillmann, R., Wedel, S., Worton, D. D., Xu, K., and Zaytsev, A.: Validity and limitations of simple reaction kinetics to calculate concentrations of organic compounds from ion counts in PTR-MS, *Atmos Meas Tech*, 12, 6193–6208, <https://doi.org/10.5194/amt-12-6193-2019>, 2019.
- 1310 Hu, L., Millet, D. B., Mohr, M. J., Wells, K. C., Griffis, T. J., and Helmig, D.: Sources and seasonality of atmospheric methanol based on tall tower measurements in the US Upper Midwest, *Atmos Chem Phys*, 11, 11145–11156, <https://doi.org/10.5194/acp-11-11145-2011>, 2011.
- Iglesias-Suarez, F., Kinnison, D. E., Rap, A., Maycock, A. C., Wild, O., and Young, P. J.: Key drivers of ozone change and its radiative forcing over the 21st century, <https://doi.org/10.5194/acp-18-6121-2018>, 3 May 2018.
- 1315 ISO 6145-10:2002 Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 10: Permeation method, 1st edition, International Organization for Standardization (ISO), Geneva, Switzerland, 16 pp., 2002. <https://iso.org/standard/25916.html>, last access: 20 October 2023.
- ISO 6145-4:2004 Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 4: Continuous syringe injection method, 2nd edition, International Organization for Standardization (ISO), Geneva, Switzerland, 15 pp., 2004. <https://iso.org/standard/36478.html>, last access: 20 October 2023.

- 1320 ISO 6145-8:2005 Gas analysis – Preparation of calibration gas mixtures using dynamic volumetric methods – Part 8: Diffusion method, 1st Edition, International Organization for Standardization (ISO), 19 pp., 2005. <https://iso.org/standard/36480.html>, last access: 20 October 2023.
- ISO 6142-1:2015 Gas analysis – Preparation of calibration gas mixtures – Part 1: Gravimetric method for Class I mixtures, 1st edition, International Organization for Standardization (ISO), Geneva, Switzerland, 39 pp., 2015.
- 1325 <https://iso.org/standard/59631.html>, last access: 20 October 2023.
- ISO 6145-7:2018 Gas analysis – Preparation of calibration gas mixtures using dynamic methods – Part 7: Thermal mass-flow controllers, 3rd edition, International Organization for Standardization (ISO), 14 pp., 2018. <https://iso.org/standard/73212.html>, last access: 20 October 2023.
- ISO 19229:2019: Gas analysis – Purity analysis and the treatment of purity data, 2nd Edition, International Organization for Standardization (ISO), Geneva, Switzerland, 18 pp., 2019. <https://iso.org/standard/72010.html>, last access: 20 October 2023.
- 1330 Jacob, D. J.: Heterogeneous chemistry and tropospheric ozone, *Atmospheric Environment*, 2131–2159 pp., [https://doi.org/10.1016/S1352-2310\(99\)00462-8](https://doi.org/10.1016/S1352-2310(99)00462-8), 2000.
- JCGM 100:2008 BIPM, IEC, IFCC, ILAC, ISO, IUPAC, IUPAP and OIML. Evaluation of measurement data – Guide to the expression of uncertainty in measurement (GUM). Joint Committee for Guides in Metrology (JCGM), 134 pp., 2008. https://www.bipm.org/documents/20126/2071204/JCGM_100_2008_E.pdf/cb0ef43f-baa5-11cf-3f85-4dcd86f77bd6, last access: 20 October 2023.
- 1335 Khan, M. A. H., Cooke, M. C., Utembe, S. R., Archibald, A. T., Maxwell, P., Morris, W. C., Xiao, P., Derwent, R. G., Jenkin, M. E., Percival, C. J., Walsh, R. C., Young, T. D. S., Simmonds, P. G., Nickless, G., O’Doherty, S., and Shallcross, D. E.: A study of global atmospheric budget and distribution of acetone using global atmospheric model STOCHEM-CRI, *Atmos Environ*, 112, 269–277, <https://doi.org/10.1016/j.atmosenv.2015.04.056>, 2015.
- 1340 Laj, P., Lund Myhre, C., Riffault, V., Amiridis, V., Fuchs, H., Eleftheriadis, K., Petäjä, T., Salameh, T., Kivekäs, N., Juurola, E., Saponaro, G., Philippin, S., Cornacchia, C., Alados Arboleda, L., Baars, H., Claude, A., De Mazière, M., Dils, B., Dufresne, M., Evangeliou, N., Favez, O., Fiebig, M., Haeffelin, M., Herrmann, H., Höhler, K., Illmann, N., Kreuter, A., Ludewig, E., Marinou, E., Möhler, O., Mona, L., Murberg, L.E., Nicolae, D., Novelli, A., O’Connor, E., Ohneiser, K., Petracca Altieri, R. M., Picquet-Varrault, B., van Pinxteren, D., Pospichal, B., Putaud, J. P., Reimann, S., Siomos, N., Stachlewska, I., Tillmann, R., Avoudouri, K.A., Wandinger, U., Wiedenschohler, A., Apituley, A., Comerón, A., Gysel-Beer, M., Mihalopoulos, N., Nikolova, N., Pietruczuk, A., Sauvage, S., Sciare, J., Skov, H., Svendby, T., Swietlicki, E., Toney, D., Vaughan, G., Zdimal, V., Baltensperger, U., Doussin, J.-F., Kulmala, M., Pappalardo, G., Sorvari S. S., and

- 1350 Vana, M.: Aerosol, Clouds and Trace Gases Research Infrastructure – ACTRIS, the European research infrastructure supporting atmospheric science. *Bull Am Meteorol Soc.*, <https://doi.org/10.1175/BAMS-D-23-0064.1>, 2024.
- Legreid, G., Lööv, J. B., Staehelin, J., Hueglin, C., Hill, M., Buchmann, B., Prevot, A. S. H., and Reimann, S.: Oxygenated volatile organic compounds (OVOCs) at an urban background site in Zürich (Europe): Seasonal variation and source allocation, *Atmos Environ*, 41, 8409–8423, <https://doi.org/10.1016/j.atmosenv.2007.07.026>, 2007.
- 1355 Lelieveld, J. and Dentener, F. J.: What controls tropospheric ozone?, *Journal of Geophysical Research Atmospheres*, 105, 3531–3551, <https://doi.org/10.1029/1999JD901011>, 2000.
- Leuenberger, M. C., Schibig, M. F., and Nyfeler, P.: Gas adsorption and desorption effects on cylinders and their importance for long-term gas records, *Atmos Meas Tech*, 8, 5289–5299, <https://doi.org/10.5194/amt-8-5289-2015>, 2015.
- Matschat, R., Richter, S., Vogl, J., and Kipphardt, H.: On the way to SI traceable primary transfer standards for amount of substance measurements in inorganic chemical analysis, *Anal Bioanal Chem*, 415, 3057–3071, <https://doi.org/10.1007/s00216-023-04660-4>, 2023.
- 1360 Miller, W. R., Rhoderick, G. C., and Guenther, F. R.: Investigating adsorption/desorption of carbon dioxide in aluminum compressed gas cylinders, *Anal Chem*, 87, 1957–1962, <https://doi.org/10.1021/ac504351b>, 2015.
- Millet, D. B., Guenther, A., Siegel, D. A., Nelson, N. B., Singh, H. B., De Gouw, J. A., Warneke, C., Williams, J., Eerdeken, G., Sinha, V., Karl, T., Flocke, F., Apel, E., Riemer, D. D., Palmer, P. I., and Barkley, M.: Atmospheric Chemistry and Physics Global atmospheric budget of acetaldehyde: 3-D model analysis and constraints from in-situ and satellite observations, *Atmos. Chem. Phys*, 3405–3425 pp., <https://doi.org/10.5194/acp-10-3405-2010>, 2010.
- 1365 Mills, G., Pleijel, H., Malley, C. S., Sinha, B., Cooper, O. R., Schultz, M. G., Neufeld, H. S., Simpson, D., Sharps, K., Feng, Z., Gerosa, G., Harmens, H., Kobayashi, K., Saxena, P., Paoletti, E., Sinha, V., and Xu, X.: Tropospheric ozone assessment report: Present-day tropospheric ozone distribution and trends relevant to vegetation, *Elementa*, 6, <https://doi.org/10.1525/elementa.302>, 2018.
- 1370 Monks, P. S., Archibald, A. T., Colette, A., Cooper, O., Coyle, M., Derwent, R., Fowler, D., Granier, C., Law, K. S., Mills, G. E., Stevenson, D. S., Tarasova, O., Thouret, V., Von Schneidmesser, E., Sommariva, R., Wild, O., and Williams, M. L.: Tropospheric ozone and its precursors from the urban to the global scale from air quality to short-lived climate forcer, <https://doi.org/10.5194/acp-15-8889-2015>, 13 August 2015.
- 1375 Pascale, C., Guillevic, M., Ackermann, A., Leuenberger, D., and Niederhauser, B.: Two generators to produce SI-traceable reference gas mixtures for reactive compounds at atmospheric levels, *Meas Sci Technol*, 28, <https://doi.org/10.1088/1361-6501/aa870c>, 2017.

- 1380 Persijn, S. T. and Baldan, A.: A new look at the sorption kinetics in reference gas standards, *Meas Sci Technol*, 34, <https://doi.org/10.1088/1361-6501/ace9ee>, 2023.
- Placet, M.: Emissions of ozone precursors from stationary sources: a critical review, *Atmos Environ*, 34, 2183–2204, [https://doi.org/10.1016/S1352-2310\(99\)00464-1](https://doi.org/10.1016/S1352-2310(99)00464-1), 2000.
- Pugliese, S. C., Murphy, J. G., Geddes, J. A., and Wang, J. M.: The impacts of precursor reduction and meteorology on ground-level ozone in the Greater Toronto Area, *Atmos Chem Phys*, 14, 8197–8207, <https://doi.org/10.5194/acp-14-8197-2014>, 2014.
- 1385 [Reimann, S., Wegener, R., Claude, A., and Sauvage, S. Deliverable 3.17. Updated measurement guideline for NO_x and VOCs. ACTRIS report, 103 pp., \[https://actris.eu/sites/default/files/Documents/ACTRIS-2/Deliverables/WP3_D3.17_M42.pdf\]\(https://actris.eu/sites/default/files/Documents/ACTRIS-2/Deliverables/WP3_D3.17_M42.pdf\), 2018.](#)
- 1390 Rhoderick, G. C., Cecelski, C. E., Miller, W. R., Worton, D. R., Moreno, S., Brewer, P. J., Viallon, J., Idrees, F., Moussay, P., Kim, Y. D., Kim, D., Lee, S., Baldan, A., and Li, J.: Stability of gaseous volatile organic compounds contained in gas cylinders with different internal wall treatments, *Elementa*, 7, <https://doi.org/10.1525/elementa.366>, 2019.
- Richter, W.: Recommendations on quantities, symbols and measurement units for publications in ACQUAL, *Accreditation and Quality Assurance*, 12, 497–498, <https://doi.org/10.1007/s00769-007-0273-6>, 2007.
- 1395 Seinfeld, J. H., Bretherton, C., Carslaw, K. S., Coe, H., DeMott, P. J., Dunlea, E.J., Feingold, G., Ghan, S., Guenther, A. B., Kahn, R., Kraucunas, I., Kreidenweis, S. M., Molina, M. J., Nenes, A., Penner, J.E., Prather, K. A., Ramanathan, V., Ramaswamy, V., Rasch, P. J., Ravishankara, A. R., Rosenfeld, D., Stephens, G., and Wood, R.: Improving our fundamental understanding of the role of aerosol-cloud interactions in the climate system. *PNAS*, 113, 5781–5790. <https://doi.org/10.1073/pnas.1514043113>, 2016.
- 1400 Schultz, M. G., Akimoto, H., Bottenheim, J., Buchmann, B., Galbally, I. E., Gilge, S., Helmig, D., Koide, H., Lewis, A. C., Novelli, P. C., Plass-Dölmer, C., Ryerson, T. B., Steinbacher, M., Steinbrecher, R., Tarasova, O., Tørseth, K., Thouret, V., and Zellweger, C.: The Global Atmosphere Watch reactive gases measurement network, *Elementa*, 3, 000067, 2015.
- 1405 Schultz, M. G., Schröder, S., Lyapina, O., Cooper, O. R., Galbally, I., Petropavlovskikh, I., Von Schneidemesser, E., Tanimoto, H., Elshorbany, Y., Naja, M., Seguel, R. J., Dauert, U., Eckhardt, P., Feigenspan, S., Fiebig, M., Hjellbrekke, A. G., Hong, Y. D., Kjeld, P. C., Koide, H., Lear, G., Tarasick, D., Ueno, M., Wallasch, M., Baumgardner, D., Chuang, M. T., Gillett, R., Lee, M., Molloy, S., Moolla, R., Wang, T., Sharps, K., Adame, J. A., Ancellet, G., Apadula, F., Artaxo, P., Barlasina, M. E., Bogucka, M., Bonasoni, P., Chang, L., Colomb, A., Cuevas-Agulló, E., Cupeiro, M., Degorska, A., Ding, A., Fröhlich, M., Frolova, M., Gadhavi, H., Gheusi, F., Gilge, S., Gonzalez, M. Y., Gros, V., Hamad, S. H., Helmig, D., Henriques, D., Hermansen, O., Holla, R., Hueber, J., Im, U., Jaffe, D. A., Komala, N., Kubistin, D., Lam, K. S., Laurila,

- 1410 T., Lee, H., Levy, I., Mazzoleni, C., Mazzoleni, L. R., McClure-Begley, A., Mohamad, M., Murovec, M., Navarro-Comas, M., Nicodim, F., Parrish, D., Read, K. A., Reid, N., Ries, L., Saxena, P., Schwab, J. J., Scorgie, Y., Senik, I., Simmonds, P., Sinha, V., Skorokhod, A. I., Spain, G., Spangl, W., Spoor, R., Springston, S. R., Steer, K., Steinbacher, M., Suharguniawan, E., Torre, P., Trickl, T., Weili, L., Weller, R., Xiaobin, X., Xue, L., and Zhiqiang, M.: Tropospheric Ozone Assessment Report: Database and metrics data of global surface ozone observations, *Elementa*, 5, <https://doi.org/10.1525/elementa.244>, 2017.
- 1415 Shao, M., Lu, S., Liu, Y., Xie, X., Chang, C., Huang, S., and Chen, Z.: Volatile organic compounds measured in summer in Beijing and their role in ground-level ozone formation, *Journal of Geophysical Research Atmospheres*, 114, <https://doi.org/10.1029/2008JD010863>, 2009.
- 1420 Shrivastava, M., Cappa, C. D., Fan, J., Goldstein, A. H., Guenther, A. B., Jimenez, J. L., Kuang, C., Laskin, A., Martin, S. T., Ng, N. L., Petaja, T., Pierce, J. R., Rasch, P. J., Roldin, P., Seinfeld, J. H., Shilling, J., Smith, J. N., Thornton, J. A., Volkamer, R., Wang, J., Worsnop, D. R., Zaveri, R. A., Zelenyuk, A., and Zhang, Q.: Recent advances in understanding secondary organic aerosol: Implications for global climate forcing, *Rev Geophys*, 55, 509–559, <https://doi.org/10.1002/2016RG000540>, 2017.
- Simon, H., Reff, A., Wells, B., Xing, J., and Frank, N.: Ozone trends across the United States over a period of decreasing NO_x and VOC emissions, *Environ Sci Technol*, 49, 186–195, <https://doi.org/10.1021/es504514z>, 2015.
- 1425 Simon, L., Gros, V., Petit, J. E., Truong, F., Sarda-Estève, R., Kalalian, C., Baudic, A., Marchand, C., and Favez, O.: Two years of volatile organic compound online in situ measurements at the Site Instrumental de Recherche par Télédétection Atmosphérique (Paris region, France) using proton-transfer-reaction mass spectrometry, *Earth Syst Sci Data*, 15, 1947–1968, <https://doi.org/10.5194/essd-15-1947-2023>, 2023.
- 1430 Sternberg, J. C., Gallaway, W. S., and Jones, D. T. L.: The mechanism of response of flame ionization detectors, in: *Gas Chromatography: Third International Symposium Held Under the Auspices of the Analysis Instrumentation Division of the Instrument Society of America*, edited by: Brenner, N., Callen, J. E., and Weiss, M. D., Academic Press, New York and London, 231–267, 1962.
- 1435 Stohl, A., Bonasoni, P., Cristofanelli, P., Collins, W., Feichter, J., Frank, A., Forster, C., Gerasopoulos, E., Gäggeler, H., James, P., Kentarchos, T., Kromp-Kolb, H., Krüger, B., Land, C., Meloen, J., Papayannis, A., Priller, A., Seibert, P., Sprenger, M., Roelofs, G. J., Scheel, H. E., Schnabel, C., Siegmund, P., Tobler, L., Trickl, T., Wernli, H., Wirth, V., Zanis, P., and Zerefos, C.: Stratosphere-troposphere exchange: A review, and what we have learned from STACCATO, *Journal of Geophysical Research Atmospheres*, 108, <https://doi.org/10.1029/2002jd002490>, 2003.

[Szopa, S., Naik, V., Ahikary, B., Artaxo, P., Berntsen, T., Collins, W., Fuzzi, S., Gallardo, L., Kiendler-Scharr, A., Kimont, Z., Liao, H., Unger, N., and Zanis, P.: Short-lived Climate Forcers, in: *Climate Change 2021 – The Physical Science Basis.*](#)

- 1440 [Contribution of Working Group I to the Sixth Assessment Report of the Intergovernmental Panel on Climate Change. Cambridge University Press, 817–922.https://doi.org/10.1017/9781009157896.008, 2023.](https://doi.org/10.1017/9781009157896.008)
- Tan, Z., Lu, K., Hofzumahaus, A., Fuchs, H., Bohn, B., Holland, F., Liu, Y., Rohrer, F., Shao, M., Sun, K., Wu, Y., Zeng, L., Zhang, Y., Zou, Q., Kiendler-Scharr, A., Wahner, A., and Zhang, Y.: Experimental budgets of OH, HO₂, and RO₂ radicals and implications for ozone formation in the Pearl River Delta in China 2014, *Atmos Chem Phys*, 19, 7129–7150, 1445 <https://doi.org/10.5194/acp-19-7129-2019>, 2019.
- Tarasick, D., Galbally, I. E., Cooper, O. R., Schultz, M. G., Ancellet, G., Leblanc, T., Wallington, T. J., Ziemke, J., Liu, X., Steinbacher, M., Staehelin, J., Vigouroux, C., Hannigan, J. W., García, O., Foret, G., Zanis, P., Weatherhead, E., Petropavlovskikh, I., Worden, H., Osman, M., Liu, J., Chang, K. L., Gaudel, A., Lin, M., Granados-Muñoz, M., Thompson, A. M., Oltmans, S. J., Cuesta, J., Dufour, G., Thouret, V., Hassler, B., Trickl, T., and Neu, J. L.: Tropospheric ozone 1450 assessment report: Tropospheric ozone from 1877 to 2016, observed levels, trends and uncertainties, <https://doi.org/10.1525/elementa.376>, 2019.
- [van der Veen, A.M.H. Meija, J., Possolo, A., Hibbert, D.B.: Interpretation and use of standard atomic weights \(IUPAC Technical Report\). Pure Appl Chem, 93, 629–646.https://doi.org/10.1515/pac-2017-1002, 2021.](https://doi.org/10.1515/pac-2017-1002)
- Volkamer, R., Sheehy, P., Molina, L. T., and Molina, M. J.: Oxidative capacity of the Mexico City atmosphere-Part 1: A 1455 radical source perspective, *Atmos Chem Phys*, 10, 6969–6991, <https://doi.org/10.5194/acp-10-6969-2010>, 2010.
- Wang, S., Hornbrook, R. S., Hills, A., Emmons, L. K., Tilmes, S., Lamarque, J. F., Jimenez, J. L., Campuzano-Jost, P., Nault, B. A., Crouse, J. D., Wennberg, P. O., Kim, M., Allen, H., Ryerson, T. B., Thompson, C. R., Peischl, J., Moore, F., Nance, D., Hall, B., Elkins, J., Tanner, D., Huey, L. G., Hall, S. R., Ullmann, K., Orlando, J. J., Tyndall, G. S., Flocke, F. M., Ray, E., Hanisco, T. F., Wolfe, G. M., St. Clair, J., Commane, R., Daube, B., Barletta, B., Blake, D. R., Weinzierl, B., Dollner, 1460 M., Conley, A., Vitt, F., Wofsy, S. C., Riemer, D. D., and Apel, E. C.: Atmospheric Acetaldehyde: Importance of Air-Sea Exchange and a Missing Source in the Remote Troposphere, *Geophys Res Lett*, 46, 5601–5613, <https://doi.org/10.1029/2019GL082034>, 2019.
- Wild, O.: Atmospheric Chemistry and Physics Modelling the global tropospheric ozone budget: exploring the variability in current models, *Atmos Chem Phys*, <https://doi.org/10.5194/acp-7-2643-2007>, 2007.
- 1465 WMO-BIPM: Metrology for Climate Action, Instruments and Observing Methods Report No. 142, Geneva, 88 pp., 2023. <https://library.wmo.int/idurl/4/66028>, last access: 25 January 2024.
- Worton, D. R., Moreno, S., Brewer, P. J., Li, J., Baldan, A., and van der Veen, A. M. H.: Bilateral comparison of primary reference materials (PRMs) containing methanol, ethanol and acetone in nitrogen, *Accreditation and Quality Assurance*, 27, 265–274, <https://doi.org/10.1007/s00769-022-01513-y>, 2022.

- 1470 Worton, D. R., Moreno, S., O'Daly, K., and Holzinger, R.: Development of an International System of Units (SI)-traceable transmission curve reference material to improve the quantitation and comparability of proton-transfer-reaction mass-spectrometry measurements, *Atmos Meas Tech*, 16, 1061–1072, <https://doi.org/10.5194/amt-16-1061-2023>, 2023.
- Wu, C., Wang, C., Wang, S., Wang, W., Yuan, B., Qi, J., Wang, B., Wang, H., Wang, C., Song, W., Wang, X., Hu, W., Lou, S., Ye, C., Peng, Y., Wang, Z., Huangfu, Y., Xie, Y., Zhu, M., Zheng, J., Wang, X., Jiang, B., Zhang, Z., and Shao, M.: Measurement report: Important contributions of oxygenated compounds to emissions and chemistry of volatile organic compounds in urban air, *Atmos Chem Phys*, 20, 14769–14785, <https://doi.org/10.5194/acp-20-14769-2020>, 2020.
- 1475 Xue, L. K., Wang, T., Gao, J., Ding, A. J., Zhou, X. H., Blake, D. R., Wang, X. F., Saunders, S. M., Fan, S. J., Zuo, H. C., Zhang, Q. Z., and Wang, W. X.: Ground-level ozone in four Chinese cities: Precursors, regional transport and heterogeneous processes, *Atmos Chem Phys*, 14, 13175–13188, <https://doi.org/10.5194/acp-14-13175-2014>, 2014.
- 1480 Yang, M., Nightingale, P.D., Beale, R., Liss, P.S., Blomquist, B., and Fairall, C.: Atmospheric deposition of methanol over the Atlantic Ocean, *PNAS*, 110, 20034–20039, <https://doi.org/10.1073/pnas.1317840110>.
- Yang, Y., Shao, M., Wang, X., Nölscher, A. C., Kessel, S., Guenther, A., and Williams, J.: Towards a quantitative understanding of total OH reactivity: A review, *Atmos Environ*, 134, 147–161, <https://doi.org/10.1016/j.atmosenv.2016.03.010>, 2016.
- 1485 ~~Young, P. J., Archibald, A. T., Bowman, K. W., Lamarque, J.-F., Naik, V., Stevenson, D. S., Tilmes, S., Voulgarakis, A., Wild, O., Bergmann, D., Cameron-Smith, P., Cionni, I., Collins, W. J., Dalsøren, S. B., Doherty, R. M., Eyring, V., Faluvegi, G., Horowitz, L. W., Josse, B., Lee, Y. H., MacKenzie, I. A., Nagashima, T., Plummer, D. A., Righi, M., Rumbold, S. T., Skeie, R. B., Shindell, D. T., Strode, S. A., Sudo, K., Szopa, S., and Zeng, G.: Pre-industrial to end 21st century projections of tropospheric ozone from the Atmospheric Chemistry and Climate Model Intercomparison Project (ACCMIP), *Atmos Chem Phys*, 13, 2063–2090, <https://doi.org/10.5194/acp-13-2063-2013>, 2013.~~
- 1490 Young, P. J., Naik, V., Fiore, A. M., Gaudel, A., Guo, J., Lin, M. Y., Neu, J. L., Parrish, D. D., Rieder, H. E., Schnell, J. L., Tilmes, S., Wild, O., Zhang, L., Ziemke, J., Brandt, J., Delcloo, A., Doherty, R. M., Geels, C., Hegglin, M. I., Hu, L., Im, U., Kumar, R., Luhar, A., Murray, L., Plummer, D., Rodriguez, J., Saiz-Lopez, A., Schultz, M. G., Woodhouse, M. T., and Zeng, G.: Tropospheric Ozone Assessment Report: Assessment of global-scale model performance for global and regional ozone distributions, variability, and trends, *Elem Sci Anth* 6: 10, 49 pp, <https://doi.org/10.1525/elementa.265>, 2018.
- 1495 Zborowska, A. G., MacInnis, C. Y., Ye, C. Z., and Osthoff, H. D.: On the photolysis branching ratio of methyl ethyl ketone, *Atmos Environ*, 254, 118383, <https://doi.org/10.1016/j.atmosenv.2021.118383>, 2021.
- Zhang, H., Wu, S., Huang, Y., and Wang, Y.: Effects of stratospheric ozone recovery on photochemistry and ozone air quality in the troposphere, *Atmos Chem Phys*, 14, 4079–4086, <https://doi.org/10.5194/acp-14-4079-2014>, 2014.