

Influence of ambient NO and NO₂ on the quantification of total peroxy nitrates (Σ PNs) and total alkyl nitrates (Σ ANs) by thermal dissociation cavity ring-down spectroscopy (TD-CRDS)

5 Laura Wüst¹, Patrick Dewald¹, Gunther N. T. E. Türk¹, Jos Lelieveld¹ and John N. Crowley¹

¹Atmospheric Chemistry Department, Max Planck Institute for Chemistry, Mainz, 55128, Germany

Correspondence to: John N. Crowley (john.crowley@mpic.de)




Abstract

Measurement of total peroxy nitrates (Σ PNs) and alkyl nitrates (Σ ANs) by instruments that use thermal dissociation (TD) inlets
10 to convert the organic nitrate to detectable NO₂ may suffer from systematic bias (both positive and negative) resulting from
unwanted secondary chemistry in the heated inlets. Here we review the sources of the bias and the methods used to reduce it
and/or correct for it and report new experiments using (for the first time) atmospherically relevant, unsaturated, biogenic alkyl
nitrates as well as two different peroxyacetyl nitrate (PAN) sources. We show that the commonly used commercial C3-alkyl-
nitrate (isopropyl nitrate, IPN) [inlet](#) for characterising the chemistry of ANs is not appropriate for real-air samples that contain
15 longer chain nitrates. [Mixing ratios of ANs generated in the NO₃-induced oxidation of limonene are strongly positively biased](#)
in the presence of NO. By detecting NO_x rather than NO₂, we provide a simple solution to avoid the bias caused by the
conversion of NO to NO₂ by primary and secondary peroxy radicals resulting from the complex chemistry in the thermal
degradation of long-chain, alkyl nitrates in air at TD-temperatures. We also show that using a photochemical source of PAN
to characterise the TD-inlets can result in a much stronger apparent bias from NO to NO₂ conversion than for a diffusion source
20 of synthesised (“pure”) PAN at similar mixing ratios, [especially if high acetone concentrations \(and thus radical](#)
[concentrations\) are involved.](#) This is explained by the presence of thermally labile trace gases such as peracetic acid
(CH₃C(O)OOH) and hydrogen peroxide (H₂O₂).


1 Introduction

Nitrogen monoxide (NO) and nitrogen dioxide (NO₂), together known as NO_x, have a significant impact on air quality and
25 human health (Crutzen, 1979; Lelieveld et al., 2015). Measurements of trace gases that act as NO_x reservoirs or sinks are
essential to gain a deeper insight into the degradation and transport mechanisms of NO_x. Organic compounds with nitrate
functionality, such as alkyl (aliphatic) nitrates (ANs, RONO₂) and peroxy nitrates (PNs, RO₂NO₂), influence the lifetime and
transport of NO_x in the atmosphere (Perring et al., 2013; Horowitz et al., 2007) and represent a large fraction of the tropospheric
nitrogen reservoir (Roberts, 1990). PNs are formed by the reaction between organic peroxy radicals (RO₂) and NO₂ (R1), while
30 ANs are formed by the reaction between RO₂ and NO (R2) in competition with the formation of alkoxy radicals (R3), which


is usually the dominant reaction pathway (Orlando and Tyndall, 2012). PNs with a carbonyl group on the α -carbon, such as PAN, have lifetimes with respect to thermal dissociation to NO_2 of minutes to hours in the boundary layer, extending to years in the cold upper troposphere (Atkinson et al., 2006). In contrast, RO_2NO_2 , which do not possess a α -carbonyl group decompose within seconds in the temperate boundary layer and these PNs have been detected only at ground level in polar regions (Slusher et al., 2002) or at high altitudes (Murphy et al., 2004).




Organic peroxy radicals are formed during the day by the OH-initiated oxidation of volatile organic compounds (VOCs) (R4) (Lightfoot et al., 1992). During night, OH levels are much lower and the O_3 -initiated oxidation of VOCs (R5) gains importance as a source of RO_2 (Ng et al., 2017).





Nitrate radicals (NO_3) and dinitrogen pentoxide (N_2O_5) play important roles in atmospheric nitrogen chemistry, especially at nighttime (Brown and Stutz, 2012). The reaction of NO_2 with O_3 produces the NO_3 radical (R6), which is in thermal equilibrium with NO_2 and N_2O_5 (R7) (Wayne et al., 1991).



During the day, NO_3 is rapidly photolysed (Liebmann et al., 2018) or reacts with NO to form NO_2 (Wayne et al., 1991). At night, however, NO_3 can reach concentrations of up to several tens of pptv (Brown et al., 2003; Geyer et al., 2001; Dewald et al., 2022; Heintz et al., 1996) and initiates the oxidation of many unsaturated VOCs (R8), especially terpenoids (Ng et al., 2017). In environments with high levels of biogenic VOCs, NO_3 also contributes to their oxidation during the day (Liebmann et al., 2019; Dewald et al., 2024).



PNs and ANs have often been measured using chromatographic (Flocke et al., 2005) and mass spectrometric methods (Wu et al., 2021; Zheng et al., 2011; Slusher et al., 2004) that allow identification and quantification of the individual components. An alternative method for measuring total, non-specified PNs and ANs (i.e. $\sum \text{PNs}$ and $\sum \text{ANs}$) is thermal dissociation to NO_2 (R9-R10) and subsequent detection by cavity ring-down spectroscopy (TD-CRDS) or laser induced fluorescence (TD-LIF) (Paul and Osthoff, 2010; Paul et al., 2009; Day et al., 2002; Sobanski et al., 2016; Thieser et al., 2016).






This method makes use of the very different bond-strengths of ROO-NO₂ and RO-NO₂ to separate their detection in inlets at appropriate temperatures (Day et al., 2002), typically around 473 K for PNs and 673 K for ANs for instruments developed in this group for example (Thieser et al., 2016; Sobanski et al., 2016). As discussed below, the thermal dissociation of PNs and ANs to NO₂ can however result in deviation from ideal (1:1) conversion as a result of unwanted, secondary chemistry.

2 Sources of potential bias in TD-CRDS measurements of PNs and ANs

The quantitative measurement of Σ ANs and Σ PNs as NO₂ following thermal dissociation can be influenced by secondary reactions that either generate or consume the NO₂ product. The origin of the bias and the various methods that have been used to reduce it or correct for it are summarised below.

The three types of reactions that can modify the concentration of NO₂ formed in thermal dissociation of Σ ANs or Σ PNs are its reduction to NO (R11-R12), the oxidation of ambient NO to NO₂ via reaction with O₃ or with RO₂ formed in the TD-inlet (R3, R13) and the conversion of NO₂ back to an organic/inorganic nitrate (R14, R15) (Day et al., 2002; Paul et al., 2009; Paul and Osthoff, 2010; Di Carlo et al., 2013; Thieser et al., 2016; Sobanski et al., 2016).



The size of the bias caused by these reactions depends sensitively on characteristics of the heated inlet, in particular the pressure at which it is operated. Instruments that use CRDS setups to detect NO₂ are usually operated at cavity pressures (and thus inlet pressures) above 500 hPa, whereas the TD-inlets of instruments using LIF to detect NO₂ can be operated at any pressure above that of the LIF-module, which is typically at 3-5 hPa (Day et al., 2002). Operation at low pressures is generally preferred as it enhances the rate of diffusive loss of radicals to the inlet walls, minimising the bias. A potential disadvantage of operation at low temperatures is the enhancement of the O(^3P) concentration as its (termolecular) reaction with O₂ (the reverse of R11) to reform O₃ is greatly reduced (Lee et al., 2014). Recognising that many of the secondary processes involve radicals and atoms formed in the heated inlets, Sobanski et al. (2016) added glass beads in the TD-section of the inlet of their CRD-based device to scavenge peroxy and OH radicals. While this successfully reduced the impact of O(^3P), OH and RO₂ radical reactions (reducing the observed bias), the use of glass beads with a large surface area was later shown to reduce the temperature at which unsaturated (e.g. biogenic) ANs are converted to NO₂ in the presence of O₃, resulting in the partial detection of ANs in the PNs channel with an inlet at 473 K (Dewald et al., 2021). This effect was weaker, but still apparent when using a quartz inlet without glass beads. This observation led Dewald et al. (2021) to switch to a Teflon (PFA) inlet which does not support the formation of reactive surface sites (S-O) that catalyse the multistep conversion of ANs to NO₂. Note that such effects are

95 not observed for saturated ANs (e.g. isopropyl nitrate, which has often been used as easily available “standard” to test inlet effects), which do not react with O₃.

An alternative approach to the physical reduction of bias (e.g. by removing radicals in the TD-inlet) is a correction based on laboratory characterisation of the effects of adding O₃, NO and NO₂ to the inlets in the presence of PN_s and AN_s followed by numerical simulation of the results using reaction schemes that describe the gas-phase and heterogeneous reactions taking
100 place (Thieser et al., 2016; Sobanski et al., 2016).

Table 1 presents a summary of the bias measured by various groups using TD-inlets coupled to various NO₂ detection schemes and the approaches used to minimise and /or correct them.

Table 1: Overview of the bias from secondary chemistry occurring when using TD-inlets and various detection methods for NO₂.

Process	TD-Inlet	Method	Organic Nitrate	Bias	Size of bias	Corrective approach	Reference
O(³ P) + NO ₂	>603 K	LIF	--	-ve	< 3.5 % loss of NO ₂ (200 – 240 ppbv O ₃)	--	Day et al. (2002)
O(³ P) + NO ₂	653 K	LIF	--	-ve	6 % loss of NO ₂ (30 ppbv O ₃)	a) Expression based on laboratory data	Lee et al. (2014)
O(³ P) + NO ₂	723 K	CRDS	--	-ve	< 4 % loss of NO ₂ (50 ppbv O ₃)	b) Expression based on laboratory data	Thieser et al. (2016)
O(³ P) + NO ₂	648 K	CRDS	--	-ve	1.5 % loss of NO ₂ (50 ppbv O ₃)	Glass beads, numerical simulation	Sobanski et al. (2016)
O(³ P) + NO ₂	653 K	CEAS	--	-ve	Not significant	--	Li et al. (2021)
O ₃ + NO	873 K	LIF	--	+ve	1.6 % of the NO converted to NO ₂ (100 ppbv O ₃)	Bias quantified in laboratory data	Day et al. (2002)
O ₃ + NO	673 K	LIF	--	+ve	< 1 % of the NO	Reduced pressure (< 5 HPa), numerical simulation.	Wooldridge et al. (2010)
O ₃ + NO	473 K 723 K	CRDS	--	+ve	0.13 ppbv (1 ppbv NO and 50 ppbv O ₃) 0.33 ppbv (1 ppbv NO and 50 ppbv O ₃)	c) Expression based on laboratory data	Thieser et al. (2016)
O ₃ + NO	448 K 648 K	CRDS	--	+ve	1.0 ppbv (1 ppbv NO and 50 ppbv O ₃) 1.7 ppbv (1 ppbv NO and 50 ppbv O ₃)	Glass beads, numerical simulation	Sobanski et al. (2016)
O ₃ + NO	453 K 653 K	CEAS	--	+ve	Not significant (within the measurement uncertainty)	--	Li et al. (2021)
RO ₂ + NO	523 K	CRDS	PAN	+ve	Factor 1.20 (1 ppbv PAN and 4 ppbv NO)	Second order polynomial expression based on laboratory data	Paul and Osthoff (2010)
RO ₂ + NO	473 K	LIF	PAN	+ve	< Factor 1.05 (NO < 3 ppbv)	Reduced pressure (< 5 HPa), numerical simulation.	Wooldridge et al. (2010)
RO ₂ + NO	463 K	CIMS	PPN	-ve	Factor 2 (2.2 ppbv PPN and 5 ppbv NO)	Laboratory data. Suppression of ion signal from matrix effects.	Mielke and Osthoff (2012)
RO ₂ + NO	473 K	CRDS	PAN	+ve	Factor 1.80 (1 ppbv PAN and 4 ppbv NO)	Numerical simulation	Thieser et al. (2016)
RO ₂ + NO	723 K	CRDS	PAN	+ve	Factor 1.25 (1 ppbv PAN and 4 ppbv NO)	Numerical simulation	Thieser et al. (2016)
RO ₂ + NO	448 K	CRDS	PAN	+ve	Factor 1.40 (3 ppbv PAN and 8 ppbv NO)	Glass beads, numerical simulation	Sobanski et al. (2016)
RO ₂ + NO	648 K	CRDS	PAN	+ve	Factor 1.04 (3 ppbv PAN and 8 ppbv NO)	Glass beads, numerical simulation	Sobanski et al. (2016)
RO ₂ + NO	433 K 633 K	CAPS	--	+ve	Not mentioned	--	Sadanaga et al. (2016)
RO ₂ + NO	523 K	PERCA-CRDS	PAN	+ve	Factor 4.0 (2 ppbv PAN and 0.75 ppmv NO)	Numerical simulation	Taha et al. (2018)
RO ₂ + NO	403 K	CAPS	--	+ve	Not determined	Numerical simulation	Keehan et al. (2020)
RO ₂ + NO	453 K	CEAS	PAN	+ve	Factor 1.56 (2.8 ppbv PAN and 5 ppbv NO)	Numerical simulation	Li et al. (2021)
RO ₂ + NO	653 K	CEAS	PAN	+ve	Factor 1.40 (2.8 ppbv PAN and 5 ppbv NO)	Numerical simulation	Li et al. (2021)
RO ₂ + NO	453 K	CRDS	PAN	+ve	Factor 1.12 (2.11 ppbv PAN and 5 ppbv NO)	Glass beads	Lin et al. (2024)
RO ₂ + NO	633 K	CRDS	PAN	+ve	Not significant	Glass beads, laboratory data	Lin et al. (2024)
RO ₂ + NO	433 K	CAPS	PAN	+ve	Factor 4.10 (0.8 ppbv PAN and 8.5 ppbv NO)	Detection of NO _x	Ohara et al. (2024)
RO ₂ + NO	448 K	CRDS	PAN	+ve	Factor 1.55 (2 ppbv PAN and 4 ppbv NO).	Detection of NO _x	This work
RO ₂ + NO	648 K	CRDS	PAN	+ve	Factor 1.70 (2 ppbv PAN and 4 ppbv NO).	Detection of NO _x	This work
RO ₂ + NO	673 K	LIF	NPN	+ve	0.7 % conversion of NO to NO ₂ per ppbv of AN	Reduced pressure (2.7-5.3 HPa)	Day et al. (2002)
RO ₂ + NO	723 K	CRDS	IPN	+ve	74-6 % conversion of NO to NO ₂ per ppbv of AN	Numerical simulation	Thieser et al. (2016)
RO ₂ + NO	648 K	CRDS	IPN	+ve	Factor 1.2 (1.4 ppbv IPN and 6 ppbv NO)	Glass beads, numerical simulation	Sobanski et al. (2016)

RO ₂ + NO	653 K	CEAS	MN	+ve	Not mentioned	Numerical simulation	Li et al. (2021)
RO ₂ + NO	633 K	CRDS	EHN	+ve	Factor 1.12 (3.36 ppbv EHN and 6 ppbv NO)	Glass beads, standard addition experiments	Lin et al. (2024)
RO ₂ + NO	633 K	CAPS	IPN	+ve	Factor 2.8 (0.97 ppbv IPN and 6 ppbv NO)	Detection of NO _x	Ohara et al. (2024)
RO ₂ + NO	648 K	CRDS	Limonene-nitrate	+ve	25 % conversion of NO to NO ₂ per ppbv of AN	Detection of NO _x	This work
RO ₂ + NO	648 K	CRDS	Isoprene-nitrate	+ve	5.1 % conversion of NO to NO ₂ per ppbv of AN	Detection of NO _x	This work
RO ₂ + NO ₂	523 K	CRDS	PAN	-ve	Not significant	--	Paul et al. (2009)
RO ₂ + NO ₂	473 K	LIF	PAN	-ve	> Factor 1.05 (NO _x < 3 ppbv)	Simulations and operate at a pressure of < 5 Hpa	Wooldridge et al. (2010)
RO ₂ + NO ₂	463 K	CIMS	PPN	-ve	Factor 1.25 (2.2 ppbv PPN and 5 ppbv NO)	Laboratory data. Suppression of ion signal from matrix effects	Mielke and Osthoff (2012)
RO ₂ + NO ₂	473 K	LIF	PAN	-ve	3 pptv per ppbv NO ₂	--	Di Carlo et al. (2013)
RO ₂ + NO ₂	473 K	CRDS	PAN	-ve	Factor 1.52 (0.7 ppbv PAN and 8 ppbv NO ₂)	Numerical simulation	Thieser et al. (2016)
RO ₂ + NO ₂	723 K	CRDS	PAN	-ve	Not significant	--	Thieser et al. (2016)
RO ₂ + NO ₂	448 K	CRDS	PAN	-ve	Factor 1.06 (9 ppbv PAN and 8 ppbv NO ₂)	Numerical simulation	Sobanski et al. (2016)
RO ₂ + NO ₂	648 K	CRDS	PAN	-ve	Not significant	--	Sobanski et al. (2016)
RO ₂ + NO ₂	403 K	CRDS	Carene-nitrate	-ve	Factor 2.33 (1 ppbv PNs and 10 ppbv NO ₂)	Numerical simulation	Keehan et al. (2020)
RO ₂ + NO ₂	453 K	CEAS	PAN	-ve	Factor 1.43 (3.3 ppbv PAN and 10.5 ppbv NO ₂)	Numerical simulation	Li et al. (2021)
RO ₂ + NO ₂	653 K	CEAS	PAN	-ve	Factor 1.08 (3.3 ppbv PAN and 10.5 ppbv NO ₂)	Numerical simulation	Li et al. (2021)
RO ₂ + NO ₂	453 K	CRDS	PAN	-ve	Factor 1.15 (2.8 ppbv PAN and 10 ppbv NO ₂)	Glass beads, standard addition experiments	Lin et al. (2024)
RO ₂ + NO ₂	633 K	CRDS	PAN	-ve	Factor 1.04 (1.71 ppbv PAN and 10 ppbv NO ₂)	Glass beads, standard addition experiments	Lin et al. (2024)
RO ₂ + NO ₂	448 K	CRDS	PAN	-ve	Factor 1.61 (2 ppbv PAN and 11 ppbv NO ₂)	Numerical simulation	This work
RO ₂ + NO ₂	648 K	CRDS	PAN	-ve	Factor 1.08 (2 ppbv PAN and 11 ppbv NO ₂)	Numerical simulation	This work
RO ₂ + NO ₂	723 K	LIF	EN	-ve	Not significant	--	Di Carlo et al. (2013)
RO ₂ + NO ₂	723 K	CRDS	IPN	-ve	Factor 1.05 (12 ppbv NO ₂)	Numerical simulation	Thieser et al. (2016)
RO ₂ + NO ₂	648 K	CRDS	IPN	-ve	Factor 1.03 (6 ppbv NO ₂)	Numerical simulation	Sobanski et al. (2016)
RO ₂ + NO ₂	633 K	CRDS	EHN	-ve	Factor 1.27 (2.03 ppbv EHN and 12 ppbv NO ₂)	Glass beads, standard addition experiments	Lin et al. (2024)
RO ₂ + NO ₂	648 K	CRDS	Limonene-nitrate	-ve	Upper limit: Factor 1.09 (3.37 ppbv Limonene-nitrate and 20 ppbv NO ₂)	--	This work
RO ₂ + NO ₂	433 K	CAPS	PAN	-ve	Not significant	--	Ohara et al. (2024)
RO ₂ + NO ₂	633 K		IPN				

105 Notes:

CRDS = cavity ring-down-spectroscopy, CAPS = cavity attenuated phase shift spectroscopy, CEAS = cavity-enhanced absorption spectroscopy, CIMS = chemical ionization mass spectrometry, LIF = laser induced fluorescence, PERCA = peroxy radical amplifier. PAN is CH₃C(O)OONO₂, PPN is C₂H₅C(O)OONO₂, IPN is isopropyl nitrate ((CH₃)₂CH₂ONO₂,CH₃), MN is methyl-nitrate (CH₃ONO₂), EN is ethyl-nitrate (C₂H₅ONO₂), NPN is n-propyl-nitrate (CH₃CH₂CH₂ONO₂), EHN is 2-ethylhexyl-nitrate. a) $S'_{380} = S_{380} / (0.0694 \times \ln(S_{380}) - 0.308) \times (0.0115 \times [O_3] + 0.557)$ where S_{380} is the observed total signal and S'_{380} is the corrected signal. b) NO₂ loss (L_{NO_2} (ppbv) = $7.43 \times 10^{-4} [NO_2][O_3]$). c) $k_{eff}(473 \text{ K}) = 2.5 \times 10^{-14} \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$, $k_{eff}(723 \text{ K}) = 6.2 \times 10^{-14} \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$ where k_{eff} is an effective rate coefficient for the reaction between O₃ and NO.

In this study we assess the bias caused by ambient NO on Σ PNs and Σ ANs measurements, with a focus on biogenically derived ANs formed in the NO₃-induced oxidation of isoprene and limonene, which so far have been neglected in the studies reviewed in Tab. 1. We show that the use of unsaturated surrogate alkyl-nitrates (e.g. IPN) to estimate bias in TD-inlets leads to a different effect compared to alkyl nitrates derived from the oxidation of common biogenic trace gases such as terpenoids and as such is inappropriate for estimating and correcting bias.

3 Experimental

3.1 TD-Cavity ring-down spectrometer

120 The measurements were performed using a 5-channel cavity ring-down spectrometer, which has been described in detail previously (Sobanski et al., 2016; Dewald et al., 2021). In this study, we use only the three cavities that detect NO₂. Each cavity consists of a stainless steel tube (70 cm length and inner diameter 8 mm) that is internally coated with Teflon (Chemours, FEP, TE 9568) to reduce losses of trace-gases during transmission. Perfluoroalkoxy polymer (PFA) T-pieces at both ends of the tubes provide connections to the sample inlet-line (see Fig. 1) and the outlet to the pump. Sample air enters the cavities at
125 a flow rate of 2.1 L (STP) min⁻¹ (slpm) in each channel. Two highly reflective mirrors (transmission of 20 ppm at 409 nm, FiveNine Optics) are located behind each PFA T-piece at a distance of 93.5 cm (*d*) apart. The mirrors are purged with dry zero air (CAP 180, Fuhr GmbH) which results in a reduction of the effective optical path length, *l*, compared to the mirror distance. To record a ring-down signal, light emitted by a laser diode is coupled into the cavities using 50 µm core optical fibres and collimators. Using a photomultiplier tube, which converts the transmitted light intensity into an analogue electrical signal, an
130 exponential decay can be observed when the laser is ~~temporarily switched~~ modulated off. The concentration of NO₂ in each cavity is calculated from:

$$[\text{NO}_2] = \frac{d}{l} \frac{(k - k_0)}{c \cdot \sigma_\lambda}, \quad (1)$$

where *k*₀ and *k* are the decay rate coefficients without and with absorbing/scattering medium, *c* is the speed of light and σ_λ is the effective absorption cross section resulting from the overlap of the laser emission and the NO₂ absorption spectrum
135 (Vandaele et al., 1998). The effective cross-section was obtained by regularly measuring the laser spectrum using a dedicated CCD camera (Ocean Optics HR4000) and was typically close to 6.4 × 10⁻¹⁹ cm² molecule⁻¹.



In the original version of this instrument (Dewald et al., 2021; Sobanski et al., 2016), three cavities were operated at 409 nm to detect either NO₂ or ΣPNs + NO₂ or ΣANs + ΣPNs + NO₂. We refer to these as the “NO₂-cavity”, the “PNs-cavity” and
140 the “ANs-cavity”, respectively. The NO₂-cavity sampled air via a 60 cm long PFA inlet (8 mm inner diameter) at ambient temperature. The PNs-cavity sampled via a 55 cm long PFA tubular (8 mm inner diameter), the first 20 cm of which were heated to 448 K to convert PNs to NO₂. The ANs-cavity sampled air via a 55 cm long quartz tube (12 mm inner diameter), where the first 20 cm were heated to 648 K, to convert ANs to NO₂.

In this work, we examine the advantages of detecting NO_x rather than NO₂ when using a TD-CRDS to measure peroxy nitrates
145 and alkyl nitrates derived from biogenic precursors. The instrument was modified to detect NO_x by adding O₃ (Fig. 1) which was generated by passing zero air over a low-pressure Hg-lamp emitting at 185 nm. The O₃ was divided equally by critical orifices into three identical reaction volumes made of 88 cm long PFA tubing (0.5 inch outer diameter, residence time of 1.8 s). About 12 ppmv O₃ were needed to fully convert NO to NO₂. This was determined experimentally by changing the flow

through the critical orifices while monitoring NO₂ for a fixed amount of NO. A numerical simulation of the reactions describing the formation and loss of NO₂ (Fig. S1) indicated a conversion efficiency of 98.7 %.

3.2 PAN sources

Two different sources of PAN were used in this study. In the first, PAN was prepared via the photolysis of acetone in air in the presence of NO as described originally by Warneck and Zerbach (1992) and improved by e.g. Flocke et al. (2005). In this case, 5 cm³ (STP) min⁻¹ (-sccm) of acetone (4.6 % in synthetic air, Air Liquide) and 10 sccm of NO (1 ppmv, Air Liquide) were mixed with 100 sccm of zero air before flowing into a quartz reactor equipped with a phosphor-coated, low-pressure mercury lamp (Pen-Ray) to photolyse acetone at ~ 285 nm (R16). Based on the volume flow rate and the volume of the reactor (~ 243 cm³), the residence time of the gas flowing through the reactor was calculated to be ~ 120 s. PAN is formed at a yield of ~ 90-95 % (relative to NO consumed) by the sequence of reactions (R16-R19). The yield may be improved by using UV-LED sources that do not generate heat and thus cause PAN to thermally dissociate (Rider et al., 2015).



The mixture exiting the photochemical reactor was diluted with 5.2 slpm zero air to provide PAN mixing ratios of ~21.7 ppbv. In order to ensure a known concentration of PAN, such photochemical PAN-sources are operated in the NO-limited chemical regime, i.e. sufficient peroxy radicals are present to initially convert each NO to NO₂ and then to PAN. High radical densities implies that result in other chemical processes involving peroxy radicals take place. In section 4.1, we later discuss the concentrations and role of the organic and inorganic photochemical products other than PAN that are generated in the reactor. Alternatively, PAN was synthesised using wet-chemical methods (Gaffney et al., 1984; Talukdar et al., 1995). Tridecane (10 mL, ≥ 99 %, Sigma-Aldrich) and peroxyacetic acid (PAA) (2.5 mL, 35 % by weight in dilute acetic acid, Acros Organics) were placed in a 100 mL wide-necked round-bottom flask and cooled to 273 K in an ice-water bath. Cold sulphuric acid (2.5 mL, 98 %, Roth) and then cold nitric acid (1.3 mL, ≥ 65 %, Sigma-Aldrich) were added dropwise while stirring. The contents of the flask were allowed to stand for 25 minutes at 273 K with vigorous stirring and then transferred to a separatory funnel containing ice-cold Milli-Q water (25 mL). The aqueous phase was discarded and the organic phase was shaken four times with 25 mL of cold Milli-Q water each time. The organic phase was then dried for 30 minutes at 273 K with magnesium sulphate (1 spatula, Alfa Aesar). After filtration, PAN was obtained as a colourless liquid in tridecane and stored at 243 K until use. During experiments, PAN was cooled to 273 K in a cryostat and evaporated into the gas-phase by flowing 100 sccm

of air over the sample, with further dilution with 5.2 slpm zero air resulting in mixing ratios between ~ 2 and 6.5 ppbv. Note that safety precautions must be taken when working with samples of PAN, which has been known to explode under certain circumstances (e.g. when distilled from its tridecane solvent).

3.3 AN sources

Limonene nitrates and isoprene nitrates were formed by the reaction of limonene or isoprene with NO_3 in air in the 1 m³ simulation chamber SCHARK (Simulation Chamber for Atmospheric Reactions and Kinetics), which was operated at ambient pressure and temperature (1 atm, 298 K) in dynamic-flow mode (Dewald et al., 2021). Residence times in the chamber were between 57 and 92 minutes depending on the flow rate. Gases entering the chamber passed through a circular loop of PFA tubing (located at the bottom of the chamber) with 10, equally spaced, 1 mm-diameter holes pointing upwards. The velocity of gas at the exit of the holes is estimated at $\sim 2 \text{ m s}^{-1}$, which causes rapid turbulent mixing. Mixing is also assisted by a $\sim 5 \text{ cm}$ diameter, teflon coated fan located centrally at the bottom of the chamber. Experiments with pulsed addition of O_3 , showed that the mixing time in the chamber was $< 40 \text{ s}$, which is negligible compared to the overall residence time.

Two methods were used to produce NO_3 . In the first, NO_3 was formed by the thermal decomposition of N_2O_5 (R7) which was evaporated into the chamber by passing zero air (50 - 600 sccm) over N_2O_5 crystals held at temperatures between 205 K and 195 K (acetone-dry ice bath). N_2O_5 was synthesised by flowing 150 sccm of NO (5% in N_2 , Westfalen) and 200 sccm of O_3 in O_2 ($\sim 10\%$ O_3 , generated via electrical discharge in O_2) through a $\sim 2 \text{ L}$, glass reaction vessel and trapped as colourless crystals at 195 K (acetone-dry ice bath). N_2O_5 crystals formed this way were stored at 243 K until use. Alternatively, NO_3 was obtained by bubbling 50-200 sccm of zero air through a 0.5 M solution of cerium(IV) ammonium nitrate (CAN) in 6 M HNO_3 that was irradiated at 365 nm (Lambe et al., 2023). The flow containing the NO_3 was diluted by 15 slpm zero air before entering the chamber. The thermal decomposition of N_2O_5 has the advantage that the lifetime of N_2O_5 is sufficiently long ($\sim 23 \text{ s}$ at 298 K) to ensure that NO_3 is formed reasonably homogeneously throughout the chamber. The disadvantage of using N_2O_5 is the release of NO_2 during its thermal decomposition. The photochemical CAN source suffers from the disadvantage that the NO_3 (added via a point source) may react before mixing is complete. i.e. the lifetime of NO_3 in the presence of (typically) 30 ppbv of limonene or isoprene is only 0.1 - 2 s, which is shorter than the mixing time. Isoprene and limonene were introduced into the chamber via flow-controllers attached to steel canisters containing isoprene (98%, Acros Organics, 45 ppmv in He) or limonene (96%, Sigma-Aldrich, 44 ppmv in He) in He (5.0, Westfalen), resulting in ANs mixing ratios between 0.47 and up to ~ 4.4 ppbv (see later).

The nitrates generated in this manner from isoprene are a mixture of C5-nitrooxyhydroperoxides, C5-nitrooxycarbonyl, C5-hydroxynitrate and also C10-nitrooxyperoxide (ROOR), with the relative concentrations depending on the fate of the initially formed nitrooxyperoxy radicals (IUPAC 2024) (Schwantes et al., 2015; Ng et al., 2017; Iupac, 2024). The limonene nitrates formed are mainly C10-hydroxynitrates at yields of $\sim 20\%$ (Spittler et al., 2006).

3.4 Experimental procedure



215 In order to investigate the influence of NO and NO₂ on the detection of PAN and biogenically derived ANs via TD-CRDS, different amounts of NO (0 – 22.5 ppbv) and NO₂ (0 – 20 ppbv) were added to the TD-inlet of the CRDS along with various amounts of PAN, isoprene-derived ANs and limonene-derived ANs. These experiments were carried out with the cavities operating both in “NO₂-mode” and in “NO_x-mode” by adding O₃ (see section 3.2).

4 Results and discussion


220 4.1 The influence of NO on the measurement of PNs (Photochemical PAN source, PAN measured as NO₂)

The presence of NO during the measurement of PNs using TD-inlets leads to a positive bias in ambient PNs concentration, which is related to the oxidation of NO to NO₂ via reactions with peroxy radicals (see section 2) (Sobanski et al., 2016; Thieser et al., 2016). To re-investigate this measurement artefact, extend previous studies from this group and provide a solution to improve the reliability of TD-CRDS instruments designed to measure ΣPNs, we have performed experiments using both a
225 photochemical source and a diffusion PAN source (see section 3.2). Fig. 2 summarises the results of an experiment in which NO was added to photochemically produced PAN (≈ 1.72 ppbv). In these experiments, O₃ was NOT added to the tubing in front of the cavities (low-pressure Hg-lamp off) so that the cavities detected only NO₂ (and not NO_x). The mixing ratios of NO₂ measured in the cavities with inlet temperatures of 448 and 648 K are plotted against the amount of NO added, which was calculated from its partial flow and mixing ratio in the bottle (1 ppmv in N₂). For both datasets, the NO₂ measured in the
230 room temperature cavity (present as an impurity in the PAN sample) has already been subtracted.

Ideally, only one molecule of NO₂ would be generated for each PAN molecule thermally dissociated and the data would describe a horizontal line at ≈ 1.72 ppbv. As Fig. 2a shows this is clearly not the case. In both cavities with heated inlets the addition of NO leads to the formation of additional NO₂. This is related to co-formation of the acetyl peroxy radical from PAN in the heated inlet at 448 K (R20) which reacts with NO (R21) to form NO₂ and (in air) a methyl peroxy radical (R21a-b). The
235 methyl peroxy radical can react with NO to form a further NO₂ and HO₂ (R22); the latter can form a third NO₂ in the reaction between HO₂ and NO (R23). The OH radical formed in this process reacts either with NO to form HONO or with NO₂ to form HNO₃ both of which are thermally stable resist dissociation in the 448 K TD-inlet (Thieser et al., 2016; Friedrich et al., 2020).



The two initially formed peroxy radicals (R16-17 and R21b) $\text{CH}_3\text{C}(\text{O})\text{O}_2$ and CH_3O_2 can undergo self- and cross-reactions in the photochemical reactor, a sub-set of which are shown below:



The CH_3CO_2 thermally decompose in air to form CH_3 and CO_2 (R21a) so that $\text{CH}_3\text{C}(\text{O})\text{O}_2$, CH_3O_2 and HO_2 are initially present. HO_2 , formed in R33 reacts with all organic peroxy radicals in both radical termination and radical propagation steps:



290 The OH formed in reaction R37 will react with acetone (which is present in large excess) to form another peroxy radical:




The acetonyl peroxy radical ($\text{CH}_3\text{C}(\text{O})\text{CH}_2\text{O}_2$) will also undergo reaction with other RO_2 , eventually forming peroxides and C1 and C2-peroxy radicals. In summary, the chemistry taking place in the PAN-photochemical source generates a large variety of oxidised organic trace gases (not only PAN) that may enter the TD-inlet at 648 K. Of particular interest with respect to explaining the data of Fig. 2 are the thermally unstable peroxides such as $\text{CH}_3\text{C}(\text{O})\text{OOH}$, CH_3OOH and H_2O_2 . These trace gases are stable at room temperature but CH_3OOH and $\text{CH}_3\text{C}(\text{O})\text{OOH}$ have lifetimes with respect to thermal dissociation of the order of seconds to at ~ 650 K, OH of 0.06 s (Sahetchian et al., 1992), 0.6 s (Kirk, 1965). In contrast, the thermal lifetime of H_2O_2 at 650 K is several minutes (Baulch et al., 2005), and 41 s (Yang et al., 2021) at 648 K, respectively which strongly suggests that its decomposition in our heated inlet is catalysed by the quartz tubing.

300

The thermal dissociation of $\text{CH}_3\text{C}(\text{O})\text{OOH}$ in the TD-inlet leads (via the thermal dissociation of initially formed CH_3CO_2 (R21)) to the formation of an OH radical and CH_3O_2 (R40) (Schmidt and Sehon, 1963; Atkinson et al., 2006):



The CH_3O_2 thus formed can, via reactions R22 and R23, account for some of the conversion of NO to NO_2 observed. However, both R23 and R40 generate OH radicals, which can react with acetone in the TD-inlet. The rate coefficient for OH + acetone at 648 K is $1.4 \times 10^{-12} \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$ (Vasudevan et al., 2005) which results in an OH-lifetime in the heated inlet of ~ 1 ms with respect to reaction with acetone. This results in the formation of the acetonyl peroxy radical (R39) which then also reacts with NO (R41) to form other peroxy radicals (HO_2 , $\text{CH}_3\text{C}(\text{O})\text{O}_2$ and CH_3O_2 via reactions R42 and R43) that can also convert NO to NO_2 .

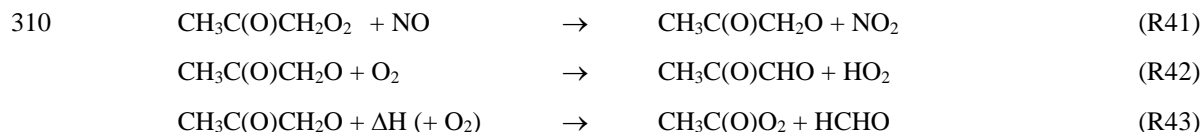

The hypothesised role of the thermal dissociation of $\text{CH}_3\text{C}(\text{O})\text{OOH}$ ([PAA](#)) and H_2O_2 at 648 K as source of peroxy radicals in
 315 the TD-inlet was tested by flowing $\text{CH}_3\text{C}(\text{O})\text{OOH}$ (~ 1 ppbv [from a permeation source](#)) or H_2O_2 (2 – 10 ppmv, calculated from
 vapour pressure) sample through the TD-inlet in the presence of various amounts of NO (Fig. 4). Note that the NO_2 measured
 in the room temperature cavity (present as an impurity of 3.5 % in the NO bottle) has been subtracted from the data obtained
 in the 648 K TD-inlet. As can be seen in Fig. 4a, the addition of up to 17.5 ppbv NO to ~ 1 ppbv PAA or 2-10 ppmv H_2O_2
 results in 0.6 ppbv or 5 ppbv NO_2 , respectively, confirming that the thermal decomposition of PAA and H_2O_2 at 648 K is a
 320 source of peroxy radicals. The hypothesis was further tested by varying the TD-inlet temperature when flowing either PAA
 or H_2O_2 in the presence of 12 ppbv NO. As shown in Fig. 4b, in both cases we observed efficient conversion of NO to NO_2 at
 temperatures above 500 K for PAA and above 400 K for H_2O_2 . In separate experiments, we observed that [\(in the presence of](#)
[NO\)](#) the thermal dissociation of acetone also accounts for a small fraction of the ~~overestimation~~-excess of NO_2 formed (400
 pptv NO_2 at 43 ppmv acetone and 16 ppbv NO), which is confirmed by its thermogram (Fig. S2). [This is presumably a result](#)
 325 [of surface catalysed dissociation of acetone to form \(in the presence of air\) peroxy radicals that convert NO to \$\text{NO}_2\$.](#)
 In order to gain insight into the identity and relative concentrations of the trace gases exiting the photochemical reactor, ~~two~~
~~sets of~~ numerical simulations ([Tab. S1](#)) were carried out with FACSIMILE (Curtis and Sweetenham, 1987), ~~both with and~~
~~without the addition of NO to the photochemical PAN source (i.e. with and without PAN formation, Tab. S1).~~ The results are
 summarised in Fig. S3 which displays the evolution of products in the photochemical reactor as a function of time. At 89 ppbv
 330 NO (Fig S3a) 88 ppbv PAN is produced. Note that, following dilution, this would result in ~ 2 ppbv of acetone in the TD-
 inlets as observed experimentally. The simulation indicates ppmv mixing ratios of several organic trace gases in the
 photochemical reactor with 570 ppmv HCHO, 60 ppmv CH_3OOH and 1 ppmv H_2O_2 after 120 s reaction time. ~~In the absence~~
~~of NO (and thus PAN, Fig. S3b) higher mixing ratios of these organics are generated, as expected. In this case the simulation~~
~~predicts 1650 ppmv HCHO, 125 ppmv CH_3OOH , 37 ppmv $\text{CH}_3\text{C}(\text{O})\text{CH}_2\text{O}_2$, 15 ppmv PAA and 2 ppmv H_2O_2 .~~
 335 In summary, [use of a](#)the photochemical PAN source [using high levels of acetone and high radical densities](#) is not well suited
 for characterising the inlet chemistry for alkyl nitrate detection via thermal decomposition to NO_2 as it results in significant
 NO to NO_2 conversion owing to the presence of thermally labile trace gases such as peracetic acid and hydrogen peroxide.
[Used at high acetone concentrations the photochemical source is also likely to cause matrix effects when deployed as a](#)
[calibration source for mass-spectrometric detection of PAN. Indeed, t](#)The presence of organic acids and their possible
 340 interference in chemical-ionisation mass spectrometric studies of PAN has been documentede previously (Mielke and
 Osthoff, 2012). [This can be alleviated by using much lower acetone concentrations \(and thus radical production rates\) which](#)
[however limits the amount of PAN that can be generated.](#)

4.2 The influence of NO and NO₂ on the measurement of PNs (PAN diffusion source)

The results presented above clearly demonstrate that the photochemical PAN source generates not only PAN but a number of oxidised organics that can influence the chemistry in the TD-inlet. This precludes an accurate assessment of the bias caused by the presence of NO or NO₂ when attempting to measure ΣPNs in real air masses. For this reason, further experiments were performed with a PAN diffusion source which is not expected to have any significant impurities. The IR spectrum (Fig. S4) of a gas sample ~~evaporated~~ from the PAN diffusion source is in good agreement with the literature and does not reveal the presence of high levels of impurities.

Figure 5 shows the results of three experiments in which PAN was added to zero air at mixing ratios of ~~~2.0~~ and ~~~6.5~~ ppbv and detected (following thermal dissociation) in both the 448 K and 648 K inlets as NO₂. As described in the experiments above, the addition of various amounts of NO to the inlet results in a strong positive bias to the measurement, with a factor ~2 more NO₂ measured at 15 ppbv NO. Compared to the photochemical PAN source, the bias (NO₂ formed per ppbv NO added) is smaller, which is related to the absence of ~~thermally unstable products~~ ~~impurities~~ such as CH₃C(O)OOH. The solid lines in these plots are the results of numerical simulations that consider the formation and loss of radicals (both gas-phase and heterogeneous) in the TD-inlets and the resultant oxidation of NO to NO₂. The simulations are described in detail in previous publications from this group (Thieser et al., 2016; Sobanski et al., 2016). While the simulations reproduce the bias caused by NO oxidation to NO₂ reasonably well in these laboratory experiments with only one major trace-gas present (PAN) apart from NO, the situation in the real atmosphere will be more complex with potentially several different PAN species and many other trace gases that also interact with OH in the TD-inlets to form other peroxy radicals that may react with NO.

An effective approach to remove the bias caused by NO oxidation to NO₂ has been described for ~~a~~ TD-inlet systems ~~in this group~~, designed to detect NO_y via conversion to NO₂ (Friedrich et al., 2020; Wild et al., 2014). In this case, the air exiting the TD-inlet is allowed to cool before adding sufficient O₃ to convert NO to NO₂ (see section 3.1) and PAN is measured as NO_x rather than NO₂. The results of an experiment in which PAN was detected as NO_x is displayed as the red and blue lines in Fig. 5. In this case, ~~~43.7~~ ppbv PAN were initially present and up to 17 ppbv of NO were added. The clear dependence of the retrieved PAN mixing ratio on the NO mixing ratio is no longer apparent when using either the 448 K or 648 K TD-inlet and alleviates the need to perform numerical simulations to correct the data.

The bias caused by the recombination of NO₂ with CH₃C(O)O₂ (section 2) was investigated when both NO₂ and NO_x were detected. The results of two experiments in which either ~~~2.0~~ or ~~~6.5~~ ppbv PAN from the diffusion source were sampled into the TD-CRDS with the addition of various amount of NO₂ are shown in Fig. 6. The effect of the recombination of the acetyl peroxy radical with NO₂ at 448 K can be seen in the data. Initial mixing ratios of PAN of ~~~2.0~~ ppbv and ~~~6.5~~ ppbv are ~~only~~ detected as ~~only~~ 1.1 ppbv and 3.4 ppbv NO₂, respectively. At 648 K the effect is significantly smaller than at 448 K, reflecting the thermal instability of CH₃C(O)O₂ at the higher temperature. The solid black and grey lines in this plot are the results of numerical simulations (Thieser et al., 2016; Sobanski et al., 2016). For the detection of NO_x (blue and red symbols in Fig. 6) a similar effect was observed as for the detection of NO₂. Thus, numerical simulations are still required to correct for the bias

caused by the ~~oxidation-recombination of the acetyl peroxy radical of~~ with NO_2 . Within the experimental uncertainty, there is no significant difference in the size of the negative bias when detecting PAN as either NO_2 or NO_x . This is readily understandable, as the recombination of $\text{CH}_3\text{C}(\text{O})\text{O}_2$ with NO_2 to reform PAN after the gas flow cools down (after the heated inlets) is not influenced by the presence of O_3 which is added later.

380 4.3 Influence of NO on the measurement of ΣANs


As described in section 2, a saturated, C3-alkyl-nitrate (IPN) has been widely used to characterise instruments using thermal dissociation to convert alkyl nitrates to (detectable) NO_2 . In previous work (Dewald et al., 2021), we have shown ~~that~~ IPN differs in its TD-inlet chemistry from biogenically derived, unsaturated nitrates which undergo surface catalysed reactions (e.g. with ozone) on hot quartz surfaces at 448 K, resulting in the unwanted detection of ANs in the PNs channel and a bias to measurements obtained in environments dominated by biogenic nitrates. Dewald et al. (2021), were able to remove this effect in their measurements of ΣPNs by using a 448 K inlet made of PFA rather than quartz. The instrument still however suffered from the positive bias caused by reactions of peroxy radicals with NO, which was enhanced compared to a quartz inlet, as the RO_2 radical losses to the PFA-tubing were reduced. Correction of the data obtained with that configuration thus required numerical simulations, which were based on laboratory experiments using IPN (Ohara et al., 2024; Thieser et al., 2016; Sobanski et al., 2016). We have extended these experiments by using atmospherically more relevant (unsaturated) alkyl nitrates formed by the NO_3 -initiated degradation of isoprene and limonene.

The results of experiments in which ~~~0.5 either 0.47 or ~4.4~~ ppbv isoprene nitrate (derived by mixing N_2O_5 with isoprene in a reaction chamber, see section 3.3) was sampled into the TD-CRDS with the addition of various amounts of NO are illustrated in Fig. 7a. In these experiments, either NO_x (blue symbols) or NO_2 (i.e. the O_3 source was switched off, orange symbols) was measured. For the “ NO_2 -mode” experiments NO_2 was present at (14.8 ± 0.2) ppbv which is a consequence of using N_2O_5 in the chamber to generate NO_3 .

In the “ NO_2 -mode” experiment using isoprene derived nitrate(s), the addition of ~ 22 ppbv of NO results in a doubling of the NO_2 signal (factor 2.3). This contrasts the results of Thieser et al. (2016), who, using IPN as surrogate alkyl-nitrate observed larger effects as represented by the black line in Fig. 7a (Thieser et al., 2016).

400 For limonene derived nitrate(s) (~~hereafter LIMO-NIT~~), the bias when measuring in “ NO_2 -mode” is very large with the addition of the same amount of NO (22 ppbv) resulting in a 690 % overestimation of LIMO-NIT (in the presence of (19.3 ± 0.2) ppbv NO_2). This contrasts previous results from this group obtained using IPN as surrogate alkyl-nitrate and observed much smaller effects which are represented by the black line in Fig. 7b (Thieser et al., 2016). In summary, at a NO mixing ratio of 20 ppbv (and $\text{NO}_2 \sim 20$ ppbv), the fractional conversion of NO to NO_2 per 1 ppb of AN present in the sample flow is 7.0 % for IPN, 5.1 % for ISOP-NIT and 25 % for LIMO-NIT. Clearly, the conversion of NO to NO_2 in the heated TD-inlet is not only dependent on the amount of NO available to react but also on the nature of the alkyl nitrate. This result is partially intuitive, as the secondary chemistry resulting from degradation of the longer chain alkyl nitrates will generate more organic peroxy radicals (to oxidize NO to NO_2) than IPN. In order to gain some insight into the secondary chemistry involved, numerical

simulations of the laboratory data were conducted. The starting point was the reaction scheme used to correct the PNs data as described previously. Rather than attempt to simulate all of the processes occurring at 648 K in the TD-inlet (for which rate coefficients are not available) we varied the number of peroxy radicals generated from the decomposition of the alkoxy radicals formed in the first reaction of the biogenic derived RO₂ with NO and allowed them to react with NO at a rate coefficient of $2.55 \times 10^{-12} \times \exp(380/T) \text{ cm}^3 \text{ molecule}^{-1} \text{ s}^{-1}$.



To approximately simulate the data, a value of $n = 1$ was sufficient for isoprene nitrate, whereas a value of 5 was required to reproduce the very large effect observed for limonene nitrate. This is related to the different number of carbon atoms and chemical structure and the different chemical reactions in the presence of NO in the TD-inlet. From our results, it is apparent, that, [when TD-CRDS instruments are operated in NO₂ mode](#), 1) IPN is not a suitable surrogate molecule for the correction of Σ ANs, as has previously been practised and 2) given that ambient measurements will normally mixture of many alkyl nitrates, corrections based on numerical simulations that have been optimised for IPN will not provide reliable data unless NO levels are very low. [This would limit the usefulness of such devices to locations with NO < ~ 2 ppbv](#) (Sobanski et al., 2016) [as found in remote/rural environments or nighttime when NO levels are often low unless nearby emission sources are present \(as e.g. in urbanized regions\)](#).

Experiments in “NO_x-mode” (Fig. 7, blue symbols) in which 22.5 ppbv NO was added to either limonene nitrates (Fig. 7b) or isoprene nitrate (Fig. 7a, both formed by the reaction of NO₃ and the corresponding terpene) in the simulation chamber were also conducted and the results are strikingly different to those when NO₂ was detected. As expected, there is no significant dependence on NO added between zero and 22 ppbv.

5 Conclusions

We have shown that the use of a conventional, photochemical (acetone based) source of PAN can result in incorrect characterisation of TD-inlets when used to detect PANs and ANs, [especially when high concentrations of acetone are used](#). This is caused [\(at least in part\)](#) by the presence of thermally labile, peroxidic trace gases, which lead to a strong positive bias of NO to NO₂ conversion in the ANs inlet. The use of “pure” PAN samples is considered to be superior as it results in more accurate thermograms and NO dependencies in the heated inlet designed to detect ANs.

For the first time, we have [quantified](#) ~~investigated~~ the potential bias from secondary chemistry (e.g. oxidation of ambient NO to NO₂) when using biogenic nitrates derived from terpenoids. The results indicate a larger bias for limonene nitrates and a smaller bias for isoprene nitrates than obtained using a saturated organic nitrate such as IPN. While IPN has the undoubted advantage of being commercially available and easy to handle, its use to characterise TD-inlets to detect ANs will not lead to results that can be transferred to other (longer chain) nitrates as has been frequently [assumed](#) ~~performed~~. The effect is partially

understood in terms of the sequential breakdown of the C10 backbone (e.g. for terpenes) to peroxy radicals that convert NO to NO₂.

445 Inspired by the success of our instrument to detect inorganic and organic NO_y species as NO_x subsequent to thermal dissociation (Friedrich et al., 2020) we have modified our PANs / ANs instrument in a similar manner (i.e. by detecting NO_x rather than NO₂). The results indicate that, when sampling the real atmosphere with NO present, this mode of operation is to be preferred over NO₂ detection as the positive bias caused when RO₂ formed e.g. from biogenic precursors reacts with ambient NO is eliminated.

450 In the instrument configuration described here with the PANs TD-inlet made of PFA, the ANs TD-inlet made of quartz and the addition of O₃ downstream of the TD-inlets to convert NO to NO₂, corrections for the oxidation of NO by O₃ and RO₂ is no longer necessary and channel cross-talk (i.e. the detection of a fraction of ANs at the PANs inlet) is avoided. The only requirement for simulation is to remove the (negative) bias caused by the recombination of acyl peroxy radicals with NO₂ downstream of the TD-inlets. As the dominant atmospheric acyl peroxy nitrate is PAN itself, for which detailed experiments exist to characterise the system, this does not introduce significant uncertainty into the measurement of ΣPNs unless NO₂ levels are very large.

455 6 Author contribution

LW and PD performed the experiments, GT assisted with development and deployment of NO₃ sources and data acquisition. LW evaluated the data and wrote the first draft of the manuscript. JC conceptualised the SCHARK experiments and with JL contributed to the manuscript. This study was carried out in part fulfilment of the PhD of LW at the Johannes Gutenberg University Mainz.

460 7 Competing Interests

The authors declare that they have no conflict of interest.

8 Acknowledgements

We thank Chemours for provision of a FEP sample used to coat the cavities.

465 PD gratefully acknowledges [funding from](#) the Deutsche Forschungsgemeinschaft (project “MONOTONS”, project number: 522970430).

9 References

- Atkinson, R., Baulch, D. L., Cox, R. A., Crowley, J. N., Hampson, R. F., Hynes, R. G., Jenkin, M. E., Rossi, M. J., and Troe, J.: Evaluated kinetic and photochemical data for atmospheric chemistry: Volume II - reactions of organic species, *Atmospheric Chemistry and Physics*, 3625-4055, 10.5194/acp-6-3625-2006, 2006.
- Baulch, D. L., Bowman, C. T., Cobos, C. J., Cox, R. A., Just, T., Kerr, J. A., Pilling, M. J., Stocker, D., Troe, J., Tsang, W., Walker, R. W., and Warnatz, J.: Evaluated kinetic data for combustion modeling: Supplement II, *Journal of Physical and Chemical Reference Data*, 34, 757-1397, 2005.
- Brown, S. S. and Stutz, J.: Nighttime radical observations and chemistry, *Chem. Soc. Rev.*, 41, 6405–6447, 2012.
- 475 Brown, S. S., Stark, H., Ryerson, T. B., Williams, E. J., Nicks, D. K., Trainer, M., Fehsenfeld, F. C., and Ravishankara, A. R.: Nitrogen oxides in the nocturnal boundary layer: Simultaneous in situ measurements of NO₃, N₂O₅, NO₂, NO, and O₃, *Journal of Geophysical Research-Atmospheres*, 108, art. 4299, 10.1029/2002JD002917, 2003.
- Carr, S. A., Baeza-Romero, M. T., Blitz, M. A., Pilling, M. J., Heard, D. E., and Seakins, P. W.: OH yields from the CH₃CO+O₂ reaction using an internal standard, *Chemical Physics Letters*, 445, 108-112, 2007.
- 480 Carr, S. A., Glowacki, D. R., Liang, C.-H., Baeza-Romero, M. T., Blitz, M. A., Pilling, M. J., and Seakins, P. W.: Experimental and modeling studies of the pressure and temperature dependences of the kinetics and the OH yields in the acetyl + O₂ reaction, *J. Phys. Chem. A*, 115, 1069-1085, 2011.
- Chen, S.-Y. and Lee, Y.-P.: Transient infrared absorption of t-CH₃C(O)OO, c-CH₃C(O)OO, and α-lactone recorded in gaseous reactions of CH₃CO and O₂, *J. Chem. Phys.*, 132, 114303, doi: 10.1063/1.3352315, 2010.
- 485 Crutzen, P. J.: The role of NO and NO₂ in the chemistry of the troposphere and stratosphere, *Ann. Rev. Earth Planet. Sci.*, 7, 443-472, 1979.
- Curtis, A. R. and Sweetenham, W. P.: Facsimile, Atomic Energy Research Establishment, Report R-12805, Facsimile, Atomic Energy Research Establishment, Report R-12805, 1987.
- Day, D. A., Wooldridge, P. J., Dillon, M. B., Thornton, J. A., and Cohen, R. C.: A thermal dissociation laser-induced fluorescence instrument for in situ detection of NO₂, peroxy nitrates, alkyl nitrates, and HNO₃, *Journal of Geophysical Research-Atmospheres*, 107, doi:10.1029/2001jd000779, 2002.
- Dewald, P., Dörich, R., Schuladen, J., Lelieveld, J., and Crowley, J. N.: Impact of ozone and inlet design on the quantification of isoprene-derived organic nitrates by thermal dissociation cavity ring-down spectroscopy (TD-CRDS), *Atmos. Meas. Tech.*, 14, 5501-5519, 10.5194/amt-14-5501-2021, 2021.
- 495 Dewald, P., Nussbaumer, C. M., Schuladen, J., Ringsdorf, A., Edtbauer, A., Fischer, H., Williams, J., Lelieveld, J., and Crowley, J. N.: Fate of the nitrate radical at the summit of a semi-rural mountain site in Germany assessed with direct reactivity measurements, *Atmos. Chem. Phys.*, 22, 7051-7069, 10.5194/acp-22-7051-2022, 2022.
- Dewald, P., Seubert, T., Andersen, S. T., Türk, G. N. T. E., Schuladen, J., McGillen, M. R., Denjean, C., Etienne, J. C., Garrouste, O., Jamar, M., Harb, S., Cirtog, M., Michoud, V., Cazaunau, M., Bergé, A., Cantrell, C., Dusanter, S., Picquet-Varrault, B., Kukui, A., Xue, C., Mellouki, A., Lelieveld, J., and Crowley, J. N.: NO₃ reactivity during a summer period in a temperate forest below and above the canopy, *Atmos. Chem. Phys.*, 24, 8983-8997, 10.5194/acp-24-8983-2024, 2024.
- 500 Di Carlo, P., Aruffo, E., Busilacchio, M., Giammaria, F., Dari-Salisburgo, C., Biancofiore, F., Visconti, G., Lee, J., Moller, S., Reeves, C. E., Bauguutte, S., Forster, G., Jones, R. L., and Ouyang, B.: Aircraft based four-channel thermal dissociation laser induced fluorescence instrument for simultaneous measurements of NO₂, total peroxy nitrate, total alkyl nitrate, and HNO₃, *Atmos. Meas. Tech.*, 6, 971-980, 10.5194/amt-6-971-2013, 2013.
- 505 Flocke, F. M., Weinheimer, A. J., Swanson, A. L., Roberts, J. M., Schmitt, R., and Shertz, S.: On the measurement of PANs by gas chromatography and electron capture detection, *Journal of Atmospheric Chemistry*, 52, 19-43, 2005.

- Friedrich, N., Tadic, I., Schuladen, J., Brooks, J., Darbyshire, E., Drewnick, F., Fischer, H., Lelieveld, J., and Crowley, J. N.: Measurement of NO_x and NO_y with a thermal dissociation cavity ring-down spectrometer (TD-CRDS): instrument characterisation and first deployment, *Atmos. Meas. Tech.*, 13, 5739-5761, 10.5194/amt-13-5739-2020, 2020.
- Gaffney, J. S., Fajer, R., and Senum, G. I.: An improved procedure for high-purity gaseous peroxyacyl nitrate production - use of heavy lipid solvents, *Atmos. Env.*, 18, 215-218, Doi 10.1016/0004-6981(84)90245-2, 1984.
- Geyer, A., Ackermann, R., Dubois, R., Lohrmann, B., Muller, T., and Platt, U.: Long-term observation of nitrate radicals in the continental boundary layer near Berlin, *Atmospheric Environment*, 35, 3619-3631, 10.1016/S1352-2310(00)00549-5, 2001.
- Groß, C. B. M., Dillon, T. J., Schuster, G., Lelieveld, J., and Crowley, J. N.: Direct Kinetic Study of OH and O₃ Formation in the Reaction of CH₃C(O)O₂ with HO₂, *The Journal of Physical Chemistry A*, 118, 974-985, 10.1021/jp412380z, 2014.
- Heintz, F., Platt, U., Flentje, H., and Dubois, R.: Long-term observation of nitrate radicals at the tor station, Kap Arkona (Rugen), *Journal of Geophysical Research-Atmospheres*, 101, 22891-22910, 1996.
- Horowitz, L. W., Fiore, A. M., Milly, G. P., Cohen, R. C., Perring, A., Wooldridge, P. J., Hess, P. G., Emmons, L. K., and Lamarque, J.-F.: Observational constraints on the chemistry of isoprene nitrates over the eastern United States, *J. Geophys. Res.*, 112, D12S08-, 2007.
- IUPAC Task Group on Atmospheric Chemical Kinetic Data Evaluation, (Ammann, M., Cox, R.A., Crowley, J.N., Herrmann, H., Jenkin, M.E., McNeill, V.F., Mellouki, A., Rossi, M. J., Troe, J. and Wallington, T. J.). Last access April. 2024
- Keehan, N. I., Brownwood, B., Marsavin, A., Day, D. A., and Fry, J. L.: A thermal-dissociation-cavity ring-down spectrometer (TD-CRDS) for the detection of organic nitrates in gas and particle phases, *Atmos. Meas. Tech.*, 13, 6255-6269, 10.5194/amt-13-6255-2020, 2020.
- Kirk, A. D.: The Thermal Decomposition of Methyl Hydroperoxide, *Can. J. Chem.*, 43, 2236-2242, 1965.
- Lambe, A. T., Bai, B., Takeuchi, M., Orwat, N., Zimmerman, P. M., Alton, M. W., Ng, N. L., Freedman, A., Claflin, M. S., Gentner, D. R., Worsnop, D. R., and Liu, P.: Technical note: Gas-phase nitrate radical generation via irradiation of aerated ceric ammonium nitrate mixtures, *Atmos. Chem. Phys.*, 23, 13869-13882, 10.5194/acp-23-13869-2023, 2023.
- Lee, J., Chen, C.-J., and Bozzelli, J. W.: Thermochemical and kinetic analysis of the acetyl radical (CH₃CO) + O₂ Reaction System, *journal of Physical Chemistry A*, 106, 7155-7170, doi:10.1021/jp014443g, 2002.
- Lee, L., Wooldridge, P. J., Gilman, J. B., Warneke, C., de Gouw, J., and Cohen, R. C.: Low temperatures enhance organic nitrate formation: evidence from observations in the 2012 Uintah Basin Winter Ozone Study, *Atmospheric Chemistry and Physics*, 14, 12441-12454, doi:10.5194/acp-14-12441-2014, 2014.
- Lelieveld, J., Evans, J. S., Fnais, M., Giannadaki, D., and Pozzer, A.: The contribution of outdoor air pollution sources to premature mortality on a global scale, *Nature*, 525, 367-371, 10.1038/nature15371, 2015.
- Li, C., Wang, H., Chen, X., Zhai, T., Chen, S., Li, X., Zeng, L., and Lu, K.: Thermal dissociation cavity-enhanced absorption spectrometer for measuring NO₂, RO₂NO₂, and RONO₂ in the atmosphere, *Atmos. Meas. Tech.*, 14, 4033-4051, 10.5194/amt-14-4033-2021, 2021.
- Liebmann, J., Karu, E., Sobanski, N., Schuladen, J., Ehn, M., Schallhart, S., Quéléver, L., Hellen, H., Hakola, H., Hoffmann, T., Williams, J., Fischer, H., Lelieveld, J., and Crowley, J. N.: Direct measurement of NO₃ radical reactivity in a boreal forest, *Atmospheric Chemistry and Physics* 2018, 3799-3815, 10.5194/acp-18-3799-2018, 2018.
- Liebmann, J., Sobanski, N., Schuladen, J., Karu, E., Hellén, H., Hakola, H., Zha, Q., Ehn, M., Riva, M., Heikkinen, L., Williams, J., Fischer, H., Lelieveld, J., and Crowley, J. N.: Alkyl nitrates in the boreal forest: formation via the NO₃-, OH- and O₃-induced oxidation of biogenic volatile organic compounds and ambient lifetimes, *Atmos. Chem. Phys.*, 19, 10391-10403, 10.5194/acp-19-10391-2019, 2019.

- Lightfoot, P. D., Cox, R. A., Crowley, J. N., Destriau, M., Hayman, G. D., Jenkin, M. E., Moortgat, G. K., and Zabel, F.: Organic Peroxy-radicals - Kinetics, Spectroscopy and Tropospheric Chemistry, *Atmospheric Environment Part A-general Topics*, 26, 1805-1961, 1992.
- Lin, C., Hu, R., Xie, P., Zhang, G., Liu, X., Tong, J., and Liu, W.: A three-channel thermal dissociation cavity ring-down spectrometer for simultaneous measurement of ambient total peroxy nitrates, total alkyl nitrates, and NO₂, *Talanta*, 270, 125524, <https://doi.org/10.1016/j.talanta.2023.125524>, 2024.
- Mielke, L. H. and Osthoff, H. D.: On quantitative measurements of peroxy-carboxylic nitric anhydride mixing ratios by thermal dissociation chemical ionization mass spectrometry, *International Journal of Mass Spectrometry*, 310, 1-9, <https://doi.org/10.1016/j.ijms.2011.10.005>, 2012.
- Murphy, J. G., Thornton, J. A., Wooldridge, P. J., Day, D. A., Rosen, R. S., Cantrell, C., Shetter, R. E., Lefer, B., and Cohen, R. C.: Measurements of the sum of HO₂NO₂ and CH₃O₂NO₂ in the remote troposphere, *Atmospheric Chemistry and Physics*, 4, 377-384, 2004.
- Ng, N. L., Brown, S. S., Archibald, A. T., Atlas, E., Cohen, R. C., Crowley, J. N., Day, D. A., Donahue, N. M., Fry, J. L., Fuchs, H., Griffin, R. J., Guzman, M. I., Herrmann, H., Hodzic, A., Iinuma, Y., Jimenez, J. L., Kiendler-Scharr, A., Lee, B. H., Luecken, D. J., Mao, J., McLaren, R., Mutzel, A., Osthoff, H. D., Ouyang, B., Picquet-Varrault, B., Platt, U., Pye, H. O. T., Rudich, Y., Schwantes, R. H., Shiraiwa, M., Stutz, J., Thornton, J. A., Tilgner, A., Williams, B. J., and Zaveri, R. A.: Nitrate radicals and biogenic volatile organic compounds: oxidation, mechanisms, and organic aerosol, *Atmospheric Chemistry and Physics*, 17, 2103-2162, 10.5194/acp-17-2103-2017, 2017.
- Ohara, N., Shioji, T., Matsumoto, J., Inomata, S., Sakamoto, Y., Kajii, Y., Shiigi, H., and Sadanaga, Y.: Improved continuous measurement system for atmospheric total peroxy and total organic nitrate under the high NO_x condition, *Review of Scientific Instruments*, 95, 10.1063/5.0172219, 2024.
- Orlando, J. J. and Tyndall, G. S.: Laboratory studies of organic peroxy radical chemistry: an overview with emphasis on recent issues of atmospheric significance, *Chemical Society Reviews*, 41, 6294-6317, 2012.
- Papadimitriou, V. C., Karafas, E. S., Gierczak, T., and Burkholder, J. B.: CH₃CO + O₂ + M (M = He, N₂) reaction rate coefficient measurements and implications for the OH radical product yield, *Journal of Physical Chemistry A*, 119, 7481-7497, doi:10.1021/acs.jpca.5b00762, 2015.
- Paul, D. and Osthoff, H. D.: Absolute Measurements of Total Peroxy Nitrate Mixing Ratios by Thermal Dissociation Blue Diode Laser Cavity Ring-Down Spectroscopy, *Analytical Chemistry*, 82, 6695-6703, doi:10.1021/ac101441z, 2010.
- Paul, D., Furgeson, A., and Osthoff, H. D.: Measurements of total peroxy and alkyl nitrate abundances in laboratory-generated gas samples by thermal dissociation cavity ring-down spectroscopy, *Review Of Scientific Instruments*, 80, Art. 114101, 10.1063/1.3258204 2009.
- Perring, A. E., Pusede, S. E., and Cohen, R. C.: An observational perspective on the atmospheric impacts of alkyl and multifunctional nitrates on ozone and secondary organic aerosol, *Chemical Reviews*, 113, 5848-5870, doi:10.1021/cr300520x, 2013.
- Rider, N. D., Taha, Y. M., Odame-Ankrah, C. A., Huo, J. A., Tokarek, T. W., Cairns, E., Moussa, S. G., Liggio, J., and Osthoff, H. D.: Efficient photochemical generation of peroxy-carboxylic nitric anhydrides with ultraviolet light-emitting diodes, *Atmospheric measurement techniques*, 8, 2737-2748, 10.5194/amt-8-2737-2015, 2015.
- Roberts, J. M.: The atmospheric chemistry of organic nitrates, *Atmospheric Environment, Part A: General Topics*, 24, 243-287, 10.1016/0960-1686(90)90108-y, 1990.
- Sadanaga, Y., Takagi, R., Ishiyama, A., Nakajima, K., Matsuki, A., and Bandow, H.: Thermal dissociation cavity attenuated phase shift spectroscopy for continuous measurement of total peroxy and organic nitrates in the clean atmosphere, *Rev. Sci. Instrum.*, 87, 10.1063/1.4958167, 2016.

- Sahetchian, K. A., Rigny, R., Tardieu de Maleissye, J., Batt, L., Anwar Khan, M., and Mathews, S.: The pyrolysis of organic hydroperoxides (ROOH), Symposium (International) on Combustion, 24, 637-643, [https://doi.org/10.1016/S0082-0784\(06\)80078-0](https://doi.org/10.1016/S0082-0784(06)80078-0), 1992.
- Schmidt, C. and Sehon, A. H.: Thermal decomposition of peracetic acid in vapor phase, Canadian Journal of Chemistry-Revue Canadienne De Chimie, 41, 1819-&, 10.1139/v63-261, 1963.
- Schwantes, R. H., Teng, A. P., Nguyen, T. B., Coggon, M. M., Crounse, J. D., St Clair, J. M., Zhang, X., Schilling, K. A., Seinfeld, J. H., and Wennberg, P. O.: Isoprene NO₃ Oxidation Products from the RO₂ + HO₂ Pathway, Journal of Physical Chemistry A, 119, 10158-10171, 10.1021/acs.jpca.5b06355, 2015.
- Slusher, D. L., Huey, L. G., Tanner, D. J., Flocke, F. M., and Roberts, J. M.: A thermal dissociation-chemical ionization mass spectrometry (TD-CIMS) technique for the simultaneous measurement of peroxyacyl nitrates and dinitrogen pentoxide, Journal of Geophysical Research-Atmospheres, 109, Art Nr. D19315, doi:10.1029/2004JD004670, 2004.
- Slusher, D. L., Huey, L. G., Tanner, D. J., Chen, G., Davis, D. D., Buhr, M., Nowak, J. B., Eisele, F. L., Kosciuch, E., Mauldin, R. L., Lefer, B. L., Shetter, R. E., and Dibb, J. E.: Measurements of pernitric acid at the South Pole during ISCAT 2000, Geophysical Research Letters, 29, Art. 2011, doi:10.1029/2002gl015703, 2002.
- Sobanski, N., Schuladen, J., Schuster, G., Lelieveld, J., and Crowley, J. N.: A five-channel cavity ring-down spectrometer for the detection of NO₂, NO₃, N₂O₅, total peroxy nitrates and total alkyl nitrates, Atmospheric Measurement Techniques, 9, 5103-5118, 10.5194/amt-9-5103-2016, 2016.
- Spittler, M., Barnes, I., Bejan, I., Brockmann, K. J., Benter, T., and Wirtz, K.: Reactions of NO₃ radicals with limonene and alpha-pinene: Product and SOA formation, Atmospheric Environment, 40, S116-S127, 10.1016/j.atmosenv.2005.09.093, 2006.
- Taha, Y. M., Saowapon, M. T., Assad, F. V., Ye, C. Z., Chen, X., Garner, N. M., and Osthoff, H. D.: Quantification of peroxyacetic acid and peroxyacetyl nitrates using an ethane-based thermal dissociation peroxy radical chemical amplification cavity ring-down spectrometer, Atmos. Meas. Tech., 11, 4109-4127, 10.5194/amt-11-4109-2018, 2018.
- Talukdar, R. K., Burkholder, J. B., Schmoltner, A. M., Roberts, J. M., Wilson, R. R., and Ravishankara, A. R.: Investigation of the loss processes for peroxyacetyl nitrate in the atmosphere: UV photolysis and reaction with OH, Journal of Geophysical Research-Atmospheres, 100, 14163-14173, doi:10.1029/95jd00545, 1995.
- Thieser, J., Schuster, G., Phillips, G. J., Reiffs, A., Parchatka, U., Pöhler, D., Lelieveld, J., and Crowley, J. N.: A two-channel, thermal dissociation cavity-ringdown spectrometer for the detection of ambient NO₂, RO₂NO₂ and RONO₂, Atmos. Meas. Tech., 9, 553-576, 10.5194/amt-9-553-2016, 2016.
- Tyndall, G. S., Staffelbach, T. A., Orlando, J. J., and Calvert, J. G.: Rate coefficients for the reactions of OH radicals with methylglyoxal and acetaldehyde, International Journal of Chemical Kinetics, 27, 1009-1020, 1995.
- Vandaele, A. C., Hermans, C., Simon, P. C., Carleer, M., Colin, R., Fally, S., Merienne, M. F., Jenouvrier, A., and Coquart, B.: Measurements of the NO₂ absorption cross-section from 42 000 cm⁻¹ to 10 000 cm⁻¹ (238-1000 nm) at 220 K and 294 K, Journal of Quantitative Spectroscopy & Radiative Transfer, 59, 171-184, 1998.
- Vasudevan, V., Davidson, D. F., and Hanson, R. K.: High temperature measurements of the reactions of OH with toluene and acetone, JPC, 109, 3352-3359, 2005.
- Warneck, P. and Zerbach, T.: Synthesis of peroxyacetyl nitrate in air by acetone photolysis, Environmental Science & Technology, 26, 74-79, 1992.
- Wayne, R. P., Barnes, I., Biggs, P., Burrows, J. P., Canosa-Mas, C. E., Hjorth, J., Le Bras, G., Moortgat, G. K., Perner, D., Poulet, G., Restelli, G., and Sidebottom, H.: The nitrate radical: Physics, chemistry, and the atmosphere, Atmos. Env. A, 25A, 1-206, 1991.
- Wild, R. J., Edwards, P. M., Dube, W. P., Baumann, K., Edgerton, E. S., Quinn, P. K., Roberts, J. M., Rollins, A. W., Veres, P. R., Warneke, C., Williams, E. J., Yuan, B., and Brown, S. S.: A measurement of total reactive nitrogen, NO_y, together with

635 NO₂, NO, and O₃ via cavity ring-down spectroscopy, *Environmental Science & Technology*, 48, 9609-9615, doi:10.1021/es501896w, 2014.

Wooldridge, P. J., Perring, A. E., Bertram, T. H., Flocke, F. M., Roberts, J. M., Singh, H. B., Huey, L. G., Thornton, J. A., Wolfe, G. M., Murphy, J. G., Fry, J. L., Rollins, A. W., LaFranchi, B. W., and Cohen, R. C.: Total Peroxy Nitrates (Σ PNs) in the atmosphere: the Thermal Dissociation-Laser Induced Fluorescence (TD-LIF) technique and comparisons to speciated PAN measurements, *Atmospheric measurement techniques*, 3, 593-607, doi:10.5194/amt-3-593-2010, 2010.


640 Wu, R., Vereecken, L., Tsiligiannis, E., Kang, S., Albrecht, S. R., Hantschke, L., Zhao, D., Novelli, A., Fuchs, H., Tillmann, R., Hohaus, T., Carlsson, P. T. M., Shenolikar, J., Bernard, F., Crowley, J. N., Fry, J. L., Brownwood, B., Thornton, J. A., Brown, S. S., Kiendler-Scharr, A., Wahner, A., Hallquist, M., and Mentel, T. F.: Molecular composition and volatility of multi-generation products formed from isoprene oxidation by nitrate radical, *Atmos. Chem. Phys.*, 21, 10799-10824, 10.5194/acp-21-10799-2021, 2021.

645 Yang, X., Shen, X., Zhao, P., and Law, C. K.: Statistical Analysis on Rate Parameters of the H₂-O₂ Reaction System, *The Journal of Physical Chemistry A*, 125, 10223-10234, 10.1021/acs.jpca.1c08250, 2021.

Zheng, W., Flocke, F. M., Tyndall, G. S., Swanson, A., Orlando, J. J., Roberts, J. M., Huey, L. G., and Tanner, D. J.: Characterization of a thermal decomposition chemical ionization mass spectrometer for the measurement of peroxy acyl nitrates (PANs) in the atmosphere, *Atmos. Chem. Phys.*, 11, 6529-6547, 2011.

650

10 Figures

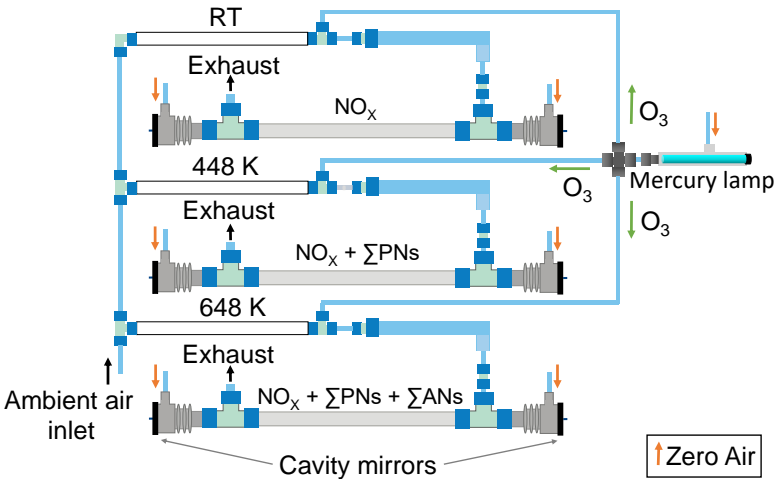

655 **Figure 1:** Schematic representation of the 409 nm cavities of the 5-channel TD-CRDS for measuring mixing ratios of NO_x, NO_x + Σ PNs and NO_x + Σ PNS + Σ ANs (Hg-lamp on). Alternatively, when the Hg-lamp is off NO₂ is measured instead of NO_x. The coloured arrows represent the gas flows. The temperatures of the different TD-inlets (measured at the outside surface) are shown for each channel.

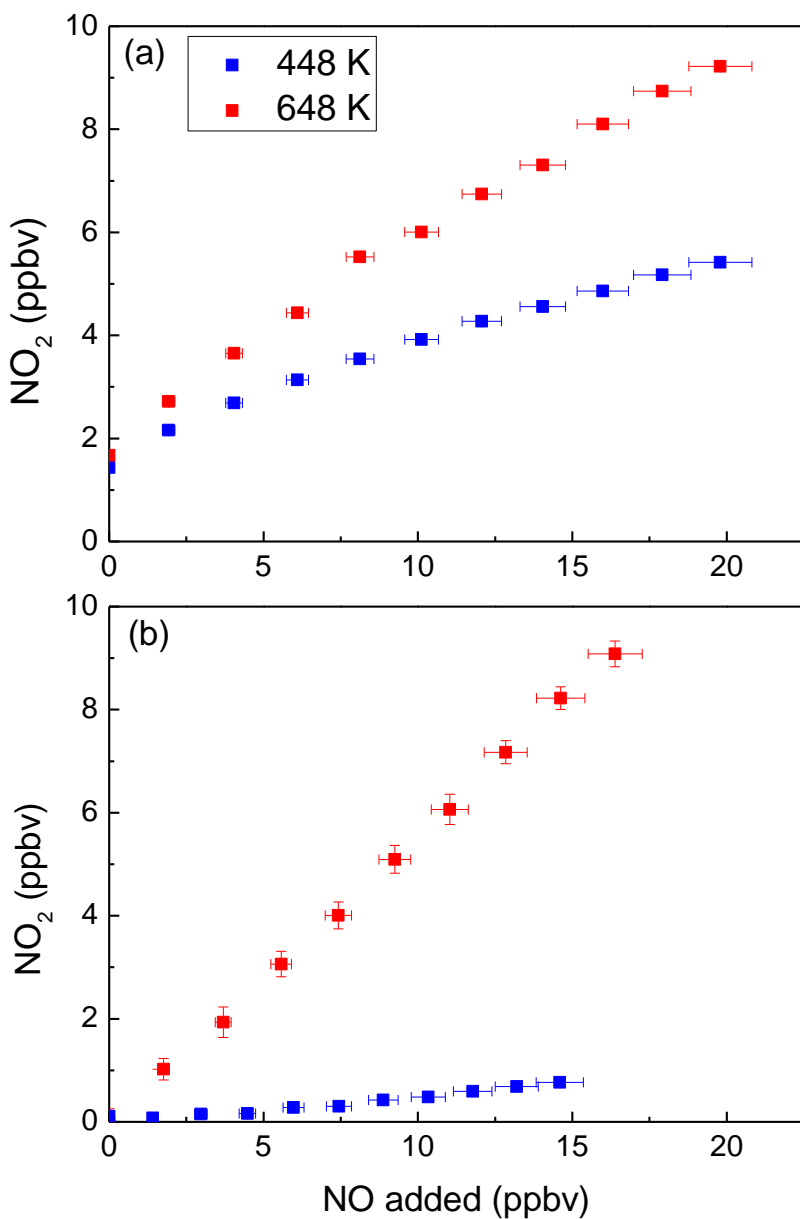


Figure 2: (a) NO₂ measured in the cavities with inlet temperatures of 448 K and 648 K in the presence of while adding different amounts of NO to photochemically produced PAN with (a) and without (b) PAN present. For each dataset, the NO₂ measured in the room temperature cavity has already been subtracted. The error bars in the x-direction include uncertainty in the mass flow controllers (1 % of the maximum flow of the MFC) and the uncertainty in the mixing ratio of the NO bottle (5 %). The error bars in the y-direction (smaller than the symbols in panel b) include the standard deviations (1 σ) of the NO₂ mixing ratios both at 648 K and at room temperature. (b) Same as panel (a) but without NO flow into the photochemical PAN source (i.e. no PAN formation).

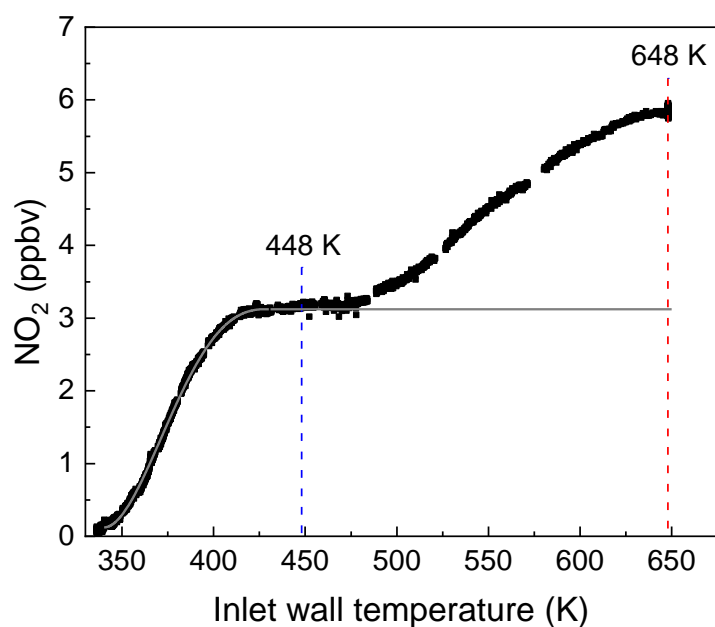
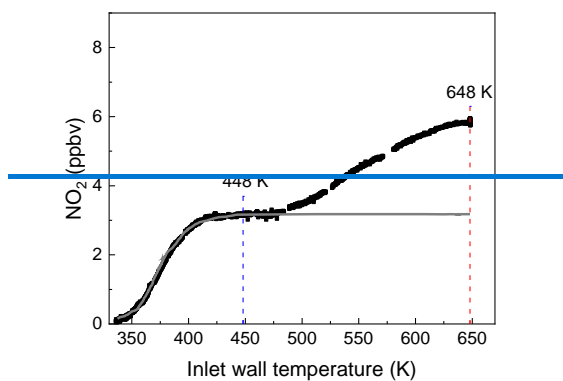


Figure 3: Thermogram obtained by adding 13 ppbv NO to ≈ 1 ppbv PAN from the photochemical PAN source. The vertical red and blue lines indicate the normal operating temperatures of the two heated inlets associated with the Σ ANs and Σ PNs cavities, respectively. Note that the NO_2 measured in the room temperature cavity (impurity present in the NO and PAN flows) has already been subtracted. The grey line represents the expected thermogram for PAN (i.e. no increase after full dissociation at ~ 450 K).

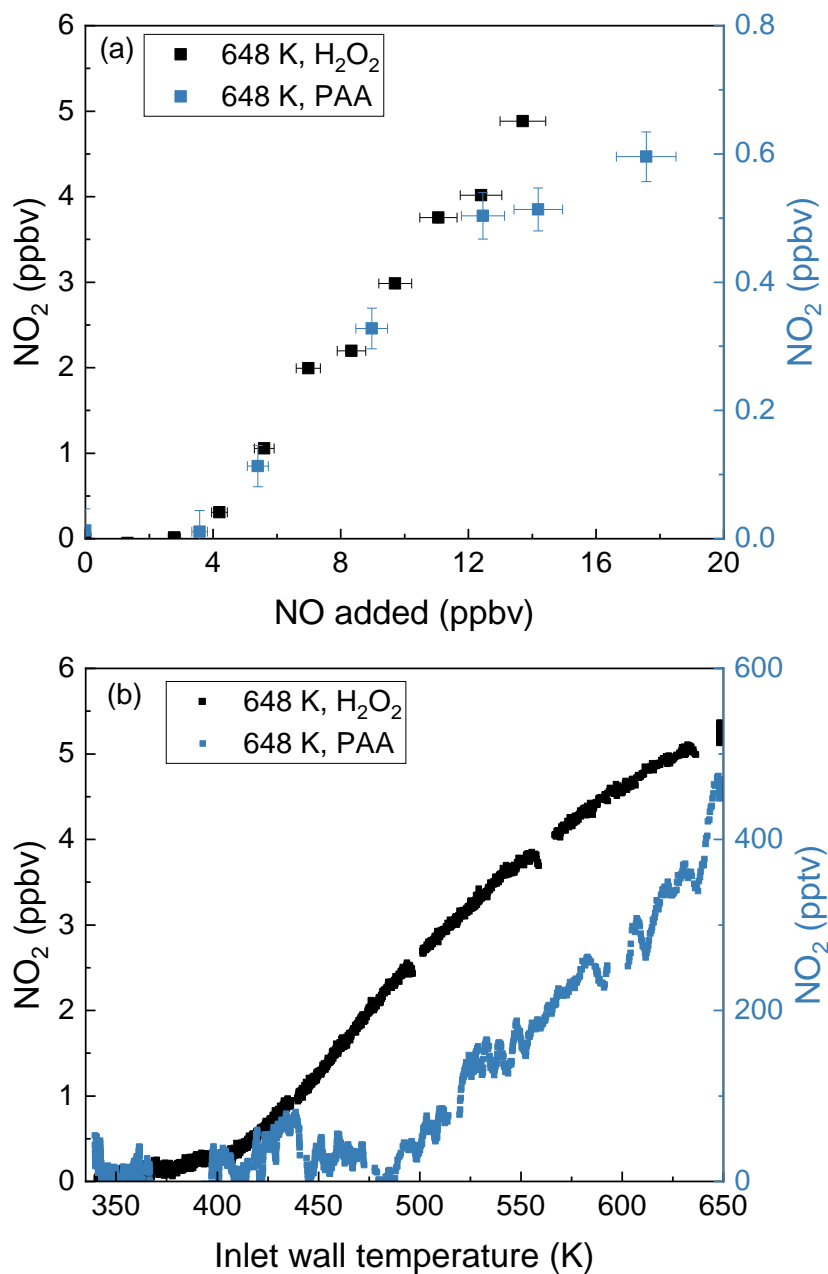


Figure 4: (a) NO₂ measured in the cavity with an inlet temperature at 648 K while adding NO to PAA (≈ 1 ppbv) and H₂O₂ (2 – 10 ppmv). For both datasets, the NO₂ measured in the room temperature cavity has already been subtracted. The error bars in the x-direction accounts for uncertainty in the mass flows (1 % of the maximum flow of the MFC) and the uncertainty of the mixing ratio of the NO bottle (5 %). The error bars in the y-direction account for uncertainty (1 σ) in the NO₂ mixing ratios both at 648 K and at room temperature. (b) Thermograms measured in the ANs-cavity while adding 12 ppbv NO to PAA (≈ 0.3 ppbv) and H₂O₂ (2 – 10 ppmv). For both datasets, the NO₂ measured in the room temperature cavity has already been subtracted.

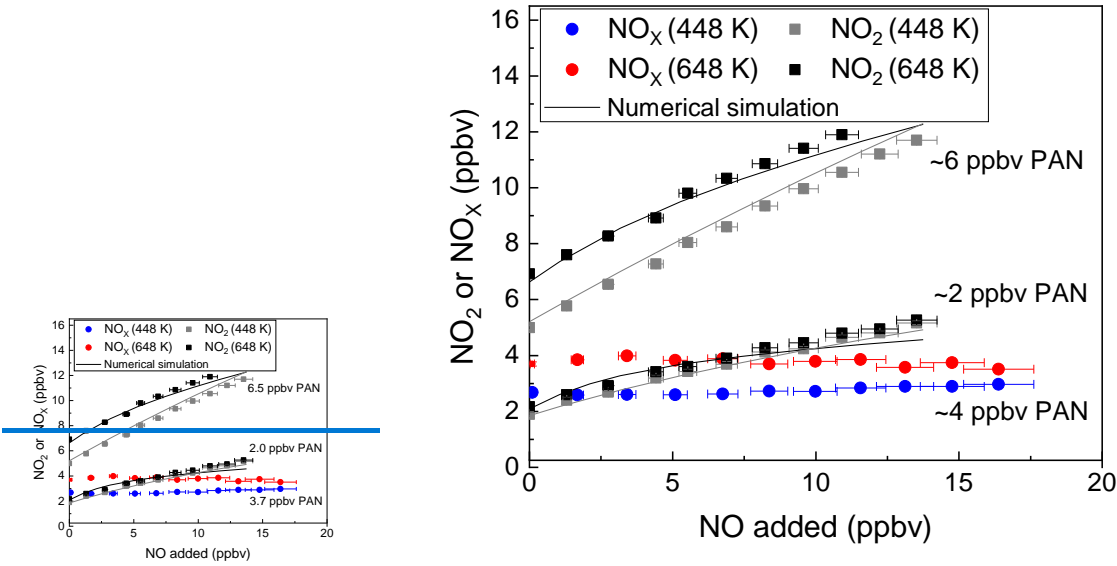


Figure 5: Measured mixing ratios of NO₂ and NO_x during the addition of NO to PAN from the diffusion source for the cavities with inlet temperatures of 448 K and 648 K. [For each dataset, the NO₂ or NO_x measured in the room temperature cavity has already been subtracted.](#) The error bars in the x-direction consider uncertainty in the mass flows (1 % of the maximum flow of the MFC) and uncertainty in the mixing ratio of the NO bottle (5 %). The error bars in the y-direction for 448 K consider the standard deviations (1 σ) of the NO₂ mixing ratios both at 448 K and at room temperature. The error bars in the y-direction for 648 K account for the standard deviations (1 σ) of the NO₂ mixing ratios both at 648 K and at room temperature. The black and grey solid lines show the numerical simulation.

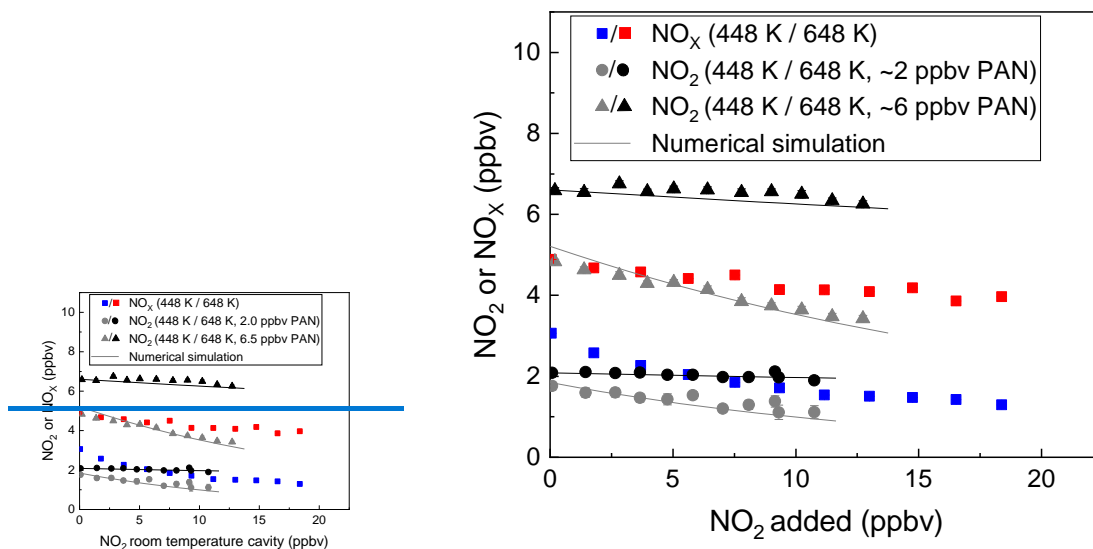


Figure 6: Measured mixing ratios of NO_x and NO_2 during the addition of NO_2 (measured with the cavity with inlet at room temperature) to PAN from the diffusion source. [For each dataset, the \$\text{NO}_2\$ or \$\text{NO}_x\$ measured in the room temperature cavity has already been subtracted.](#) The inlet temperatures were 448 K and 648 K. The error bars in the x-direction represent standard deviation (1σ) of the NO_2 mixing ratio at room temperature, those in the y-direction for 648 K account for uncertainty (1σ) in the NO_2 mixing ratios both at 648 K and at room temperature. The error bars in the y-direction for 448 K account for the standard deviations (1σ) of the NO_2 mixing ratios both at 448 K and at room temperature. The black and grey solid lines are the results of numerical simulations.

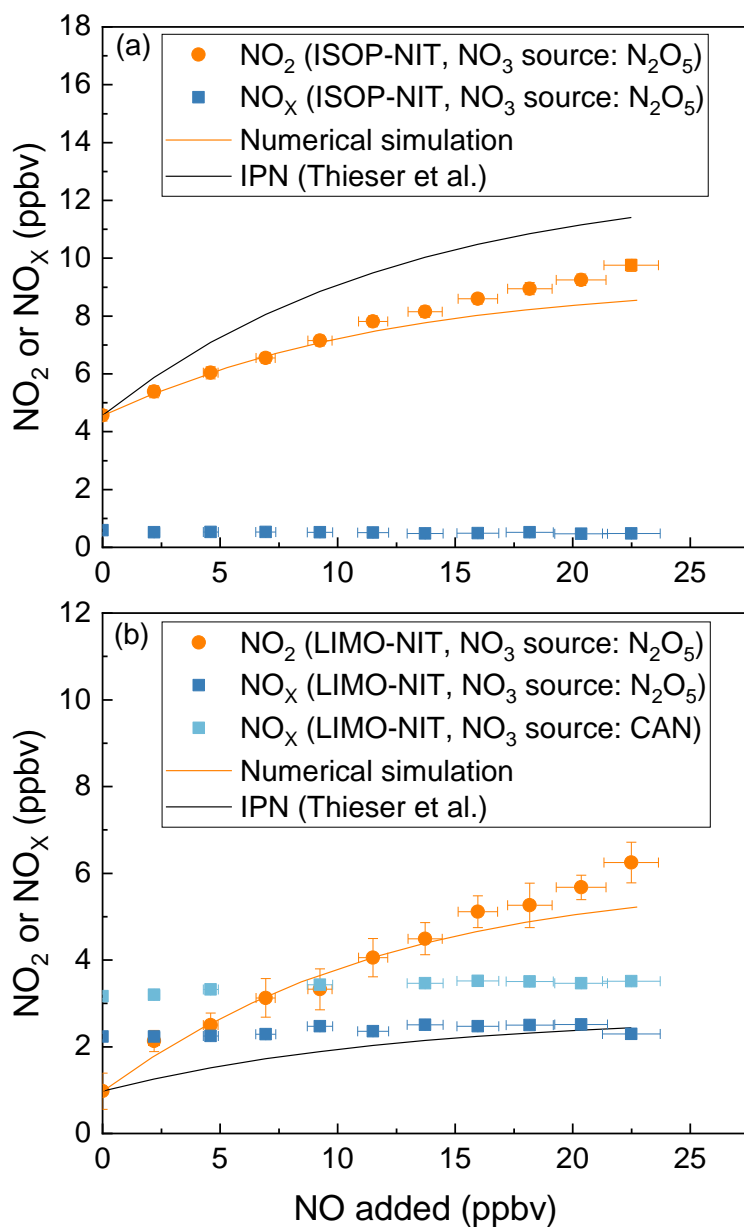


Figure 7: Addition of NO to flowing samples of either (a) isoprene derived nitrates (ISOP-NIT) or (b) limonene derived nitrates (LIMO-NIT). NO_3 was either generated with an N_2O_5 diffusion source or via cerium(IV) ammonium nitrate photolysis (CAN). The error bars in the x-direction consider uncertainty in the mass flows (1 % of the maximum flow of the MFC) and uncertainty in the mixing ratio of the NO bottle (5 %). The error bars in the y-direction consider the standard deviations (1σ) of the NO_2 mixing ratios both at 648 K and at room temperature. The orange lines are the results of numerical simulations of the data at 648 K. The black lines are calculated from the expression: $\text{NO}_2 = 1 + 1.8(\exp(-0.08 \cdot \text{NO}(\text{ppbv})))$ (Thieser et al., 2016) as derived for addition of NO to IPN. The NO_2 or NO_x measured in the room temperature cavity has been subtracted from that measured in the cavity associated with the 648 K TD-inlet.