

Schneider et al. “CARIBIC-AMS: A fully automated aerosol mass spectrometer for operation on routine passenger flights (IAGOS-CARIBIC): Instrument description and first flight application in the UTLS”

Reply to Reviewer #2

Reviewer comments in black

Our replies in red

General comments

This manuscript provides a first characterization of the CARIBIC-AMS, an airborne instrument based on commercial Aerodyne mini-AMS that is part of the IAGOS-CARIBIC research payload. Unlike other airborne particle mass spectrometers that can rely on human input during or at least after each flight, this particular instrument is required to operate in a fully autonomous manner over the course of several flights. Given that IAGOS-CARIBIC operates exclusively on commercial airliners, the reliability of power and communications is typically a lot worse than on most research platforms. While the instrument testing reported here was cut short by COVID, this work does report successful operation for a good portion of that testing period (36 flights, plus a recent campaign in 2024 on a different platform, which is unambiguously a great achievement, for which I want to congratulate the authors

As noted above, this is not a new instrument, but the adaptation of a commercial instrument that has/will operate on a long-term mission to sample the global UT/LS (and some random snippets of the lower troposphere). Hence for a characterization paper like this I would expect it to describe, in addition to the actual modifications, both the operations and analytical performance in enough detail to serve as a guide for future data users/modelers to use the data properly and have a handle on the uncertainties. This paper is fairly detailed on both the motivation and modifications but has a few gaps when describing the operations (the reader learns a great deal on the general CARIBIC schedule of operations, but rather less on the specifics of the CARIBICAMS operation). However, it does not describe the analytical performance. While the predeployment calibrations are described in detail, no field calibrations are shown. And in lieu of instrumental validation by multiflight instrumental comparisons and performance metrics, the paper chooses to narratively highlight the sulfate measurement on two flight segments. Detection limits are shown and mentioned in the abstract, but it is unclear if these are specific to the single flight segment shown (so “best of”) or an actual average of the usable flight segments.

The authors explicitly write in the conclusions that the “metrology paper” will be next. And I certainly agree that it makes sense to leave most of these details for a paper written on the new version of the instrument that is going to start flying shortly on the new CARIBIC platform. Nevertheless, in this manuscript some metrics need to be shown to support that despite all the operational challenges, the instrument actually quantifies PM consistently. Showing, as the authors do in Section 3, examples of AMS sulfate tracking stratospheric markers does not really do that, it just shows that the instrument recorded data and there were no inlet leaks. What needs to be shown is a) how well did the CARIBIC-AMS data agree with collocated instruments and b) are there systematic biases due to the way it is operated (e.g. does the instrument do worse or better on Flight #6 vs Flight #1 of a sequence?). This does

not need to be shown for every possible metric (that's paper #2); e.g. just focusing on the (mentioned in the text) agreement between the AMS and the filter sampler would likely be sufficient. But without that, it is impossible to evaluate if the modifications were successful in terms of making the CARIBICAMS a quantitative instrument.

I also find some of the AMS specific details to be confusing, and hope that the authors can clarify them, given that this paper is probably going to be read widely. This paper describes the first deployment of an important new analytical resource to investigate the UT/LS, and therefore is certainly a good fit for AMT.

Thank you for the detailed review and the suggestion for improvement of the manuscript. The major and minor comments are answered below. Here we respond to the additional questions and remarks in the text above:

To the points a) and b) from above:

- a) Agreement with collocated instruments: We include below a comparison with a UHSAS during TPEx for the flight that we presented here and for another flight from a recently submitted paper. For the IAGOS-CARIBIC flights, we will contact the data owners of the collocated OPC (even though it detects only particles larger than 250 nm) and ask to provide the full size distribution which is not available up to now.
- b) The instrument generally operates better during the later flights of a sequence, since power down time between two flights is generally much shorter than power down time before the first flight (due to transport from our lab to KIT and then to the airport).

To the remark concerning field calibrations: We do not / did not intend to perform field calibrations. The way the operation of IAGOS-CARIBIC is (and has been) planned is the following: The instrument is calibrated in the lab at MPIC. One day before a flight sequence, it is brought to KIT where it is installed into the measurement container which is then transported to the airport and installed into the aircraft. After the flight sequence, the container is transported back to KIT, the AMS is brought back to MPIC where the next calibration is/will be done.

To the remark of “agreement between the AMS and the filter sampler”: We assume this refers to lines 401-402 where we stated that the presented example data from November 2019 data “lie in a similar range as previous IAGOS-CARIBIC data” published between 2013 and 2015. Thus, this is not a direct comparison that we can focus on.


Major comments:

- Characterization of the particle range sampled by the instrument: For any model/measurement or two instrument comparison, a well characterized operational particle range is key. For the CARIBIC-AMS, that would be a product of the aircraft inlet transmission, the transmission of transfer plumbing and of the AMS inlet (both their custom CPI and the PM1 lens). For the aircraft inlet, the authors reference Herrman et al 2001 and Brenninkmeijer 2007, which given the submicron focus of the instrument is perfectly

adequate. However, there is no characterization of either plumbing losses or AMS inlet losses. It is mentioned in L128 that the plumbing losses were calculated, but no results are shown.


We will add an expanded section describing the transmission efficiency of the aircraft line and the sampling lines to the CARBIC-AMS.

1) The sampling efficiency of the aircraft inlet is shown here:

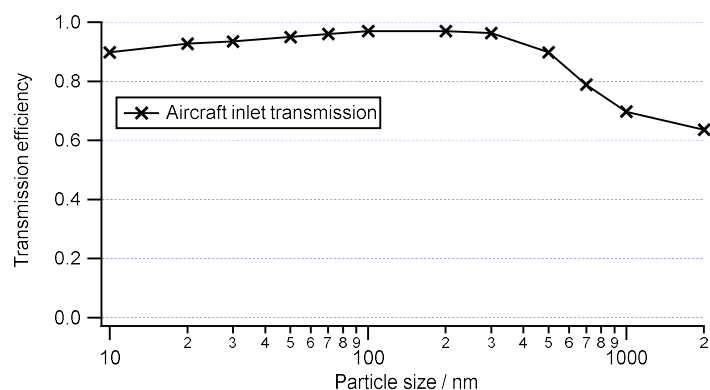


For the plumbing inside the aircraft, we used the Particle Loss Calculator (PLC, von der Weiden et al., 2009) in an expanded version that allows to vary the pressure. We calculated the transmission of the sampling lines between aircraft inlet and flow splitter to the CARIBIC-AMS and the transmission of the plumbing inside the CARIBIC-AMS rack. The calculations were made for an ambient pressure of 300 hPa, a flow rate of 24 l/m between inlet and container and the respective flow rates after the flow splitter inside the container to the splitter to the CARIBIC-AMS. The plumbing transmission inside the CARIBIC-AMS rack was also measured in the laboratory.


2) Transmission of Aircraft inlet line until the splitter to the CARIBIC-AMS:

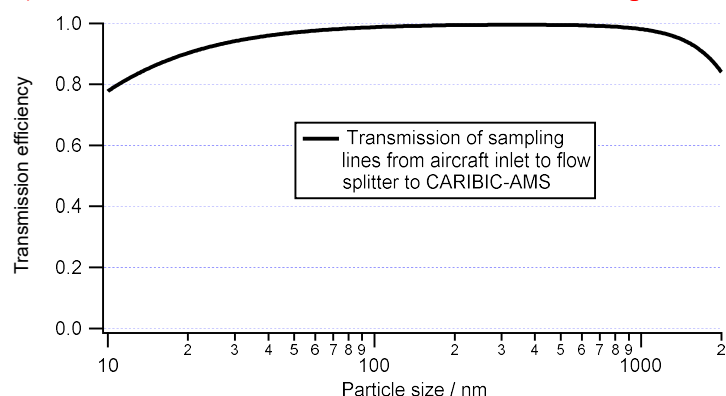

- 3) Transmission of the plumbing inside the CARIBIC-AMS rack (1/8" lines, flow 0.3 l min⁻¹), measured in the laboratory and calculated:

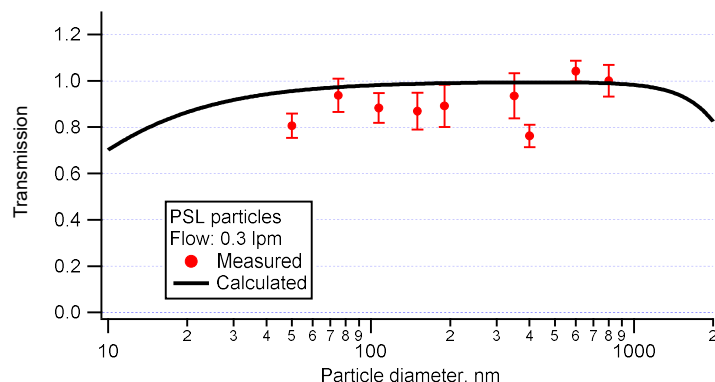

- 4) all transmission efficiencies together:

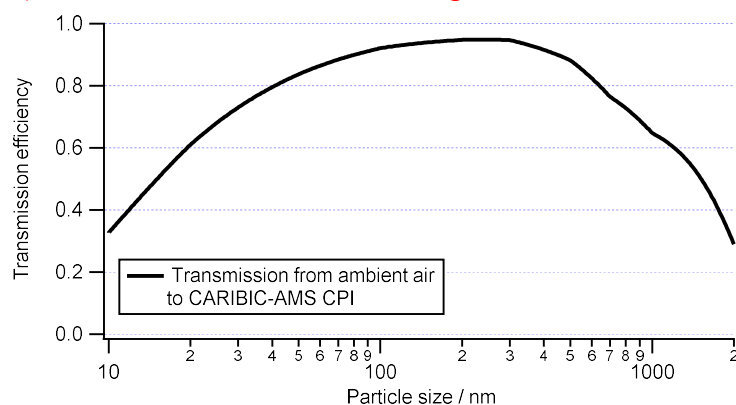

Regarding the AMS inlet losses:

- For the actual AMS lens, Liu et al, 2007 is referenced. As discussed in e.g. Knote et al, 2011, there are significant discrepancies both at the high and low end of the curve between Liu et al, 2007 and other reports of AMS transmission. Given that the accumulation mode in the stratosphere goes well above the PM₁ lens cut (e.g. Brock et al, 2021, Fig. 11), while in the upper troposphere the sampling of particle growth events on the low end of the transmission range is expected, both of these uncertainties will matter for accurate quantification. And they are somewhat dependent on instrument-specific parameters (quality of the alignment, lens vintage, lens pressure), hence an instrument specific characterization is needed, or, in the short term, at least some spot-check confirmation that the actual transmission does indeed follow one of the reference curves.

We have not performed a measurement of the transmission of the PM₁ lens of the CARIBIC-AMS. We had assumed that the transmission measurements of the PM₁ lens as published by Liu et al. (2007) are valid also for our lens. We will do this measurement, but this will not be possible in the time frame needed for the revision of this manuscript. See also reply to the following comment.

- Then there is the issue of the relatively novel CPI used in this work. While Molleker et al 2020 does characterize the transmission performance of the CPI+PM_{2.5} lens in detail, I am not aware of a similar characterization for this CPI+PM₁ lens, so the exact impact of the CPI on

the lens transmission above is unclear. The authors do report that the comparisons in Mei et al, 2020 suggest serious losses at low altitudes. While I agree that this is unlikely to matter for the portions of the atmosphere sampled by the CARIBIC-AMS, it does (as the authors acknowledge) matter for understanding the sensitivity calibrations on the ground. The authors write: "For this purpose, the mass-based IE calibration as described above is done at various pressures and a pressure-dependent IE is used for the data evaluation" (L287-289). Since said calibration is done at a constant calibrant size, this seems to imply that the authors assume the losses in the CPI at high pressure to be size-independent. This is to me a counterintuitive assumption that needs more support/explanation, since it's central to the instrument's performance.

As said before, we have not done the measurement of the inlet (CPI + PM1 lens) transmission, because we relied on published data on the PM1 lens (e.g., Liu et al., 2007) and the CPI with PM2.5 lens (Molleker et al., 2020). However, we agree that the combination of CPI and PM1 lens appears to have a different transmission characteristic than the CPI in combination with the PM2.5 lens. The measurement will be made in our lab as soon as possible, but currently the CARIBIC-AMS needs to undergo some hardware modification for the installation in the new container setup on the A350. Therefore, these measurements need more time and can't be part of the current paper. The comparison with a UHSAS shown below indicate that the losses are not severe for altitudes above 8000 m.

We use the same combination of CPI and PM1 lens in the C-ToF-AMS that is used on other aircraft, mainly on HALO (e.g., Schulz et al., 2018; Mei et al., 2020; Reifenberg et al., 2022), and as mentioned above, we find good transmission properties above about 2000 m altitude. However, if it turns out that the combination CPI + PM2.5 lens indeed gives better transmission values, we will consider changing to the PM2.5 lens.

○ Again, while these might seem like minor points, if we take Fig 11-1 in Brock et al, 2021, there is a ~40% difference in accumulation sulfate mass if one were to apply the Liu vs Knote lens transmission. This uncertainty is not reflected in the 35% accuracy estimate by Bahreini et al, 2009, is dependent on the specific air mass sampled and hence should be treated (and discussed) separately. If none of this calibration data is available, then at least the effect of the various literature transmission curves and the "pressure dependent IE" on the final reported concentration needs to be discussed when compared to other instruments.

It should be noted that Liu et al. (2007) report on laboratory measurements, while Knote et al. (2011) summarizes available transmission measurements and use a linear parameterization of these data. Thus, the "Knote lens transmission" is not necessarily a better or more representative transmission curve than that inferred from individual measurements.

However, we agree that the size distributions in Fig 11-1 of Brock et al. (2021) suggest that the upper size cut of the inlet system of the CARIBIC-AMS leads to additional uncertainty due to inlet transmission, especially for particles in the micrometer size range as observed in the stratosphere by Brock et al. (2021). On the other hand, many of the IAGOS-CARIBIC data will be recorded in the upper troposphere due to the typical flight altitudes of passenger aircraft where particles are likely smaller than in the lowermost stratosphere.

We will include a discussion on the uncertainty by the lens cut-off and the extension of accumulation mode beyond the lens transmission.

- Instrumental Collection Efficiency: The current manuscript does not mention collection efficiency (CE) (Canagaratna et al, 2007) at all, which for an AMS-style instrument sampling the free troposphere is a strange omission. This might be warranted if the instrument had a capture vaporizer (Xu et al, 2017, Hu et al, 2017) that mostly obviates the need for a particle bounce correction factor. Now, the authors do not specify what vaporizer was used (please add this!) but both Fig 1 and the mention of a "tungsten vaporizer" strongly implies that this is a standard vaporizer as described in Canagaratna et al 2007. Hence a bounce correction (Middlebrook et al, 2012) is needed for this instrument (and for all the data presented in Section 3) and should be described and discussed. The authors might also want to explain in this context the reasons for that particular vaporizer choice, which seems counterintuitive to me. One item I would like the authors to specifically address in this context is how the high ammonium detection limits of the CARIBIC-AMS will affect the accuracy of the CE correction at different altitudes. While averaging can be used to improve the CE accuracy in the stratosphere, this is probably not the case during ascent/descent. If so, what are the consequences for data reporting?

Yes, we use a standard vaporizer in the CARIBIC-AMS. We will add this information in the revised version.

The reason for choosing a standard vaporizer is the measurement of size distributions. As reported in Hu et al. (2017) and Hu et al. (2020), the capture vaporizer broadens the size distributions. The authors argue that this problem may only be of limited importance for field measurements, but we decided that with including the ePTof mode and the synchronization with the ToF pulser, the best possible chopper configuration for size distribution measurements should be preferred. However, we don't rule out that we will test a capture vaporizer in future experiments.

The collection efficiency (CE) is applied only during data evaluation and can therefore be adjusted to the hardware setup (e.g. vaporizer type) and also to possible newer parameterizations. Thus, the CE is not part of the hardware modifications and software procedures required for automation, which are the focus of this paper.

The data examples shown in the paper were calculated with the simple approach of a constant CE of 0.5. We will add this information in the revised version.


However, for future routine evaluation of IAGOS-CARIBIC data, we will apply the composition dependent CE of Middlebrook et al. (2012). The high detection limit especially of ammonium and the therefore limited time resolution are certainly a problem for the ascent and descent phases. We will include a discussion on this in the revised version.

- Sensitivity Calibrations: Section 2.3.2. summarizes some pre-deployment calibrations. Fig 5 and 6a certainly have value in terms of showing that the instrument post reconfiguration was working well. But as noted, for a field instrument it would be much more valuable to show the timeseries (or set of regressions in Fig 5) for the in-field calibrations between 2018 and 2020 to assess instrument stability (particularly the calibration pairs before/after one set of flights). If the testing was too rough on the instrument, this might not be possible, but again, with 36 flights there should be some good data to show.

Here we have to emphasize that we do not perform in-field calibrations. The IAGOS-CARIBIC container is removed from the aircraft after each flight sequence and brought back to the KIT lab. From there, we transported the instrument to the MPIC lab where all calibrations and performance checks are done. Thus, the pre- (or post-) deployment calibrations shown in section 2.3.3 are representative for the standard operation of the instrument.

The purpose of Fig 6b is not clear. First of all, the uncertainty bands shown seem incorrect. This is a test of RIE fidelity, and the uncertainty for those is 15% (2 sigma) per Bahreini et al, not 35% (which is the total uncertainty). Secondly, previous work has shown no such discrepancy for mixtures (e.g. Jimenez et al, 2016, Xu et al, 2018). Hence the reasons for this disagreement, if real, need to be explained better. There could be issues with different transmission efficiencies for both instruments, different choices in acquisition cycle, or something else entirely. I think it could also be removed, since it does not really provide much context on the overall instrument performance (a correlation/dual timeseries of ambient measurements on the ground might in any case be more appropriate).

Thanks for pointing out the mistake in the uncertainty for the RIE. Bahreini et al. (2009) in fact report 10% for ammonium and 15% for sulfate. However, the comparison for nitrate also needs an uncertainty, which following this argumentation would not exist, by definition of RIE. Nevertheless, we changed the uncertainty range to 15%:

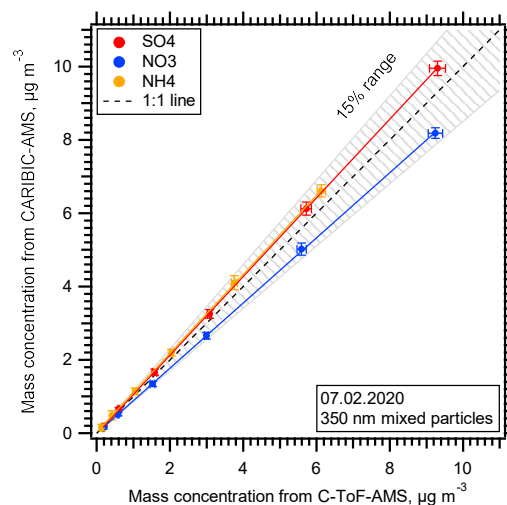

We still think that the figure is useful because it shows the reproducibility of two different AMS instruments. To our opinion, a comparison with well defined (350 nm) laboratory generated aerosol particles appears favourable over a comparison with unknown ambient aerosol.

- Size resolved measurements and AMS operation. The description of the ePToF custom implementation and subsequent calibrations is good, although I would suggest to the authors to consider using an alternative figure that shows the (significant) increase in S/N and resolution a bit more convincingly. Also, it should probably be noted somewhere that the theoretical resolution is 1/127 (Hadamard sequence length). However, as the paper is written it is completely unclear if any size dependent measurements were taken in flight. The larger point is that there could be a bit more detail on exactly how the AMS acquisition is run. The authors write that the typical MS acquisition is 30 seconds long, but it is unclear how

many open/closed cycles this encompasses and what the effective duty cycle for sampling is. When are the ePToF runs scheduled? And does the instrument operate on a fixed time basis or not?

The intention of Figure 7 was to show the raw data as they were measured for conditions representative for the upper troposphere ($p = 300$ hPa, particle concentration 100 cm^{-3}). That the increase in S/N for a short sampling time of 8 seconds is not as significant as might have been expected is surprising but cannot be ignored here.

As mentioned above in the reply to reviewer #1, we have not used the ePToF mode in flight yet. The synchronization between the ToF pulser and the chopper was not ready during the IAGOS-CARIBIC flights between 2018 and 2020. For the TPEX mission, we did not use ePToF but decided to maximize the time spent in mass spectrum mode to obtain the best possible signal-to-noise ratio with a highest possible time resolution. The reason for this was that the objective of TPEX was small scale mixing at the tropopause.

We will clarify this in the revised version.

Regarding the timing:

For flights when we tried ePToF, we used 20 seconds in MS mode and 10 seconds in ePToF mode. In the MS mode we used 5 seconds “open” and 5 seconds “closed”.

In flights without trying ePToF (because we had realized before that it won't work) we used 20 seconds time resolution, i.e. also twice 5 sec open and 5 secs closed.

The sampling duty cycles were 72% for the 30 sec saving with ePToF and 75% for the 20 sec saving w/o ePToF.

During the IAGOS-CARIBIC flights from 2018 to 2020, the instrument did not operate on a fixed time base.

However, it must be emphasized that these settings are subject to change based on improvements in detection limit and sensitivity, as well as from experience and results from future flight application. The IAGOS database can cope with different time resolution settings, so there is no need to define and fix the time resolution and time steps in advance.


- Detection limits: The estimation of the detection limits from the closed signal seems very reasonable, but since the instrument takes automated blanks it would be good to show a comparison of the calculated DLs with the ones derived from the statistics of the blanks. More generally, while it is great that the authors reported these DLs, as noted above it is very unclear for what conditions these are specified. Do these only apply to Flight 508? I think it would be a lot more informative to:

- a) Report average DLs for the stable stratospheric periods of all available flights
- b) Show the change of these DLs for a range of flights. Ideally other species besides sulfate should be shown, since e.g. ammonium and OA are much more likely to greatly improve with additional pumping over the course of the flight/circuit.

For the abstract, again it would be good to specify what these DLs refer to. It might be simpler and easier to follow to just write that the DLs will scale with $1/\sqrt{N}$ for longer averaging times, instead of quoting 5 min DLs

It has been explained in Drewnick et al. (2009) that the continuous method for determining AMS detection limits by using the background signal yields more realistic results than the filter method. The main purpose of the blank filter is to determine the gas-phase contributions to certain ions.

In the first flight on November 5, 2019 (Fig. 9 in the preprint), the instrument took 4 blank filters. The detection limits calculated (after Drewnick et al., 2009) as $3 \times \sigma_{\text{Filter}}$ are similar but lower than those inferred from the background signal mode:

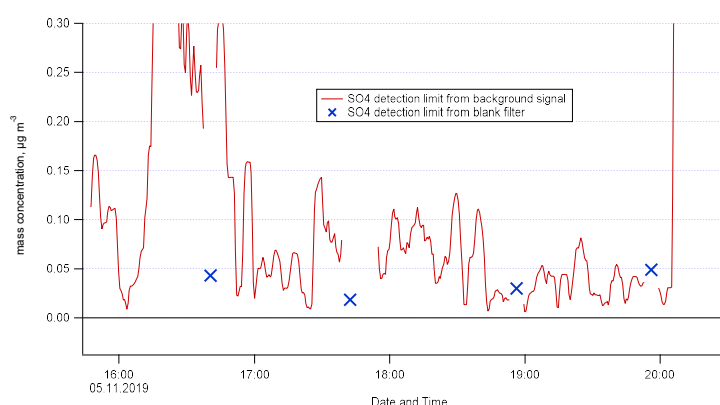

The reason for the suggested restriction to stratospheric periods for the detection limits is not clear to us. To our opinion, the detection limits depend on the background in the vacuum chamber and by that on pumping time. The DLs should not depend on altitude or ambient pressure (because the CPI keeps the inlet mass flow constant), and also not on the composition of the ambient air. Maybe the higher ozone volume mixing ratio in the stratosphere plays a role, but that is unlikely and speculative. An analysis of stratospheric flight parts versus upper tropospheric flight is not subject of this technical paper.

We will modify the abstract according the reviewer's suggestion and report only the 30-sec DL. Also, we will add more DL values from different flights in the revised version.


- Section 3: Validation. Section 3.1 puts the measurements in an appropriate context and helps the reader re-digest the information from the Ops section, but I would suggest adding some AMS context from my previous comments (e.g. discussion of CE and particle size range). Section 3.2 on the other hand does not really introduce anything new. Instead, as noted in the general comments, this would be the place where some instrument comparisons over several flights are shown and discussed (either filters or volume size distributions). Given the teething problems of the instrument, this data is likely going to be noisy and will suggest low accuracies that will hopefully soon be superseded by version 2 of the instrument. This is understandable and can be properly contextualized in the text, but the data should still be shown.

We will add the discussion of CE and size range to section 3.1 in the revised version. Section 3.2 was indented to demonstrate the operation of the instrument under research campaign conditions in a manual operation mode, mainly because between

March 2020 and summer 2020 there was no other opportunity to operate the instrument on an aircraft. Furthermore, with respect to validation and comparison, unfortunately during the IAGOS-CARIBIC flights between Oct 2018 to March 2020, the OPSS (Hermann et al., 2016) of TROPOS was not operational.


The optical particle counter operated by FZ Julich detects particles only above a diameter of 250 nm. This may still be useful for comparison, but the data are not publically available in full detail on the Zenodo data base (Zahn et al., 2025). We will contact the data owners and ask for the full size distribution for the flights shown in Fig. 9.

During the TPEx mission, a UHSAS was operated in parallel to the CARIBIC-AMS. We converted the AMS mass concentration data with the density inferred from the composition to a volume concentration. The AMS data were evaluated with a constant CE of 0.5. The comparison is shown in the following figure:

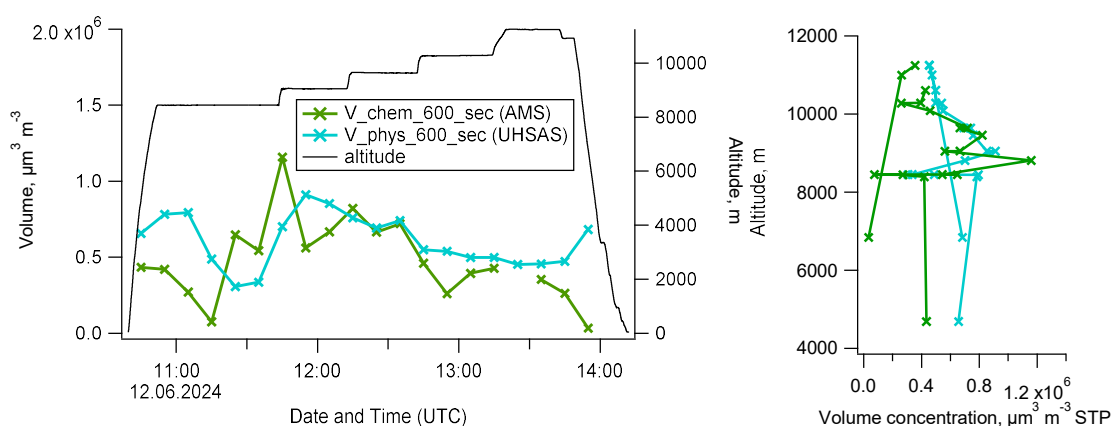

The agreement is overall satisfying, but indicates that the deviations are larger at lower altitudes (below 8 km).


See also Figure E10 in the recently submitted manuscript by Joppe et al. (2025) that presents data from the same campaign but another flight:

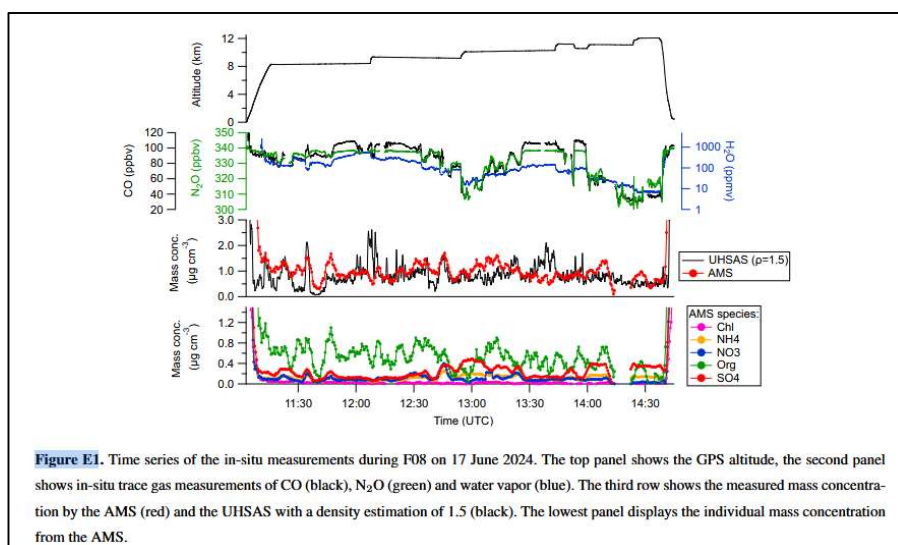

Minor comments:

- Single Ion Calibration: This is a minor point, but I am not following the need for periodic single ion calibrations during flight. The single ion calibration at this point (post-2014) just supplies a scaling factor (the SI) to convert signal to counts per second. Historically, this calibration also included the spectral baseline fit, but that has been automated since 2016 and is taken on a per-run basis. Now, the in-flight SI is needed to scale it to the SI of the sensitivity calibration. BUT once the instrument is running and the SI has been characterized once, the variability of the SI is fully captured by the airbeam variability (especially in an instrument with a well-working CPI). So while the ability to do this calibration on the fly e.g. in case of in-flight instrument reboot is important and impressive to have implemented, I would really appreciate it if the authors could explain their rationale for why periodic SI calibrations are needed. As a side note, it would be nice to see a figure with either the airbeam or SI change for a couple of flights.

The figure below shows an example of measured airbeam and SI values during a flight sequence (March 2020, the last flight sequence of IAGOS-CARIBIC). It can clearly be seen that the SI values (red points) change over time, and that the airbeam basically follows the SI, but decreases at the beginning of each flight

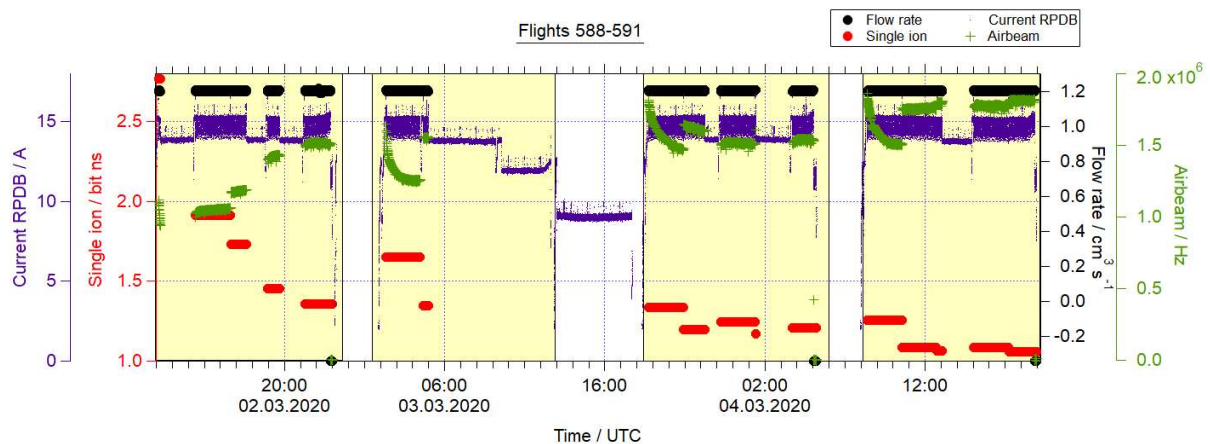

We assume that this is due to the fact that the initial SI calibration is done right before starting the measurement. At this point the pressure has just dropped below 3×10^{-6} hPa and it is likely that the background signal is still too high and thus the airbeam is high at the beginning and decreases over time during the first phase of each flight.

In the course of all flights, the SI decreases and the airbeam increases again accordingly. We therefore think that an SI calibration later in the flight is more reliable than directly at the beginning, but still the data suggest that it is worthwhile to repeat it several times during a flight.

(For the periodic SI calibration during flight, we use the “SingleIon” routine in the AMS DAQ version 5.0.6)

- Figure 3: It would be very helpful if the different operation states described in the text are added to the figure (maybe as shaded bars). Also, please clarify the units for the Yaxis. Are these A at 24 V? It might be clearer to use W(att) here.

Yes, it's A at 24 V. For clarity, we will change the units to Watts and add the operation states to the figure in the revised version.

- Section 2.2.3 is not a straightforward read, since it tries to combine both topological and process details into one narrative. One suggestion to make it more accessible is to add a simple diagram showing the network/software topology/hierarchy and referring to it in the text.

We will add a diagram in the revised version.

- The units used in the paper are $\mu\text{g m}^{-3}$ STP. STP is not defined anywhere, and since the atmospheric community is not exactly known for its general adherence to SI units I would strongly urge the authors to spell out what they mean in the text.

STP stands for Standard Temperature (273.15 K or 0°C) and Pressure (1000 hPa). We will include the following reference:

'STP' in *IUPAC Compendium of Chemical Terminology*, 5th ed. International Union of Pure and Applied Chemistry; 2025. Online version 5.0.0, 2025.
<https://doi.org/10.1351/goldbook.S06036>

- Line 19: Instead of “part” maybe “module” would read better?

Will be changed in revised version

- Line 25: “Due to **the** short time”

Will be changed in revised version

- Line 86: I would recommend adding the mission description paper for Atom here as well for completeness:

C. R. Thompson, S. C. Wofsy, M. J. Prather, P. A. Newman, T. F. Hanisco, T. B. Ryerson, D. W. Fahey, E. C. Apel, C. A. Brock, W. H. Brune, K. Froyd, J. M. Katich, J. M. Nicely, J. Peischl, E. Ray, P. R. Veres, S. Wang, H. M. Allen, E. Asher, H. Bian, D. Blake, I. Bourgeois, J. Budney, T. Paul Bui, A. Butler, P. Campuzano-Jost, C. Chang, M. Chin, R. Commane, G. Correa, J. D. Crounse, B. Daube, J. E. Dibb, J. P. Digangi, G. S. Diskin, M. Dollner, J. W. Elkins, A. M. Fiore, C. M. Flynn, H. Guo, S. R. Hall, R. A. Hannun, A. Hills, E. J. Hints, A. Hodzic, R. S. Hornbrook, L. Greg Huey, J. L. Jimenez, R. F. Keeling, M. J. Kim, A. Kupc, F. Lacey, L. R. Lait, J.-F. Lamarque, J. Liu, K. Mckain, S. Meinardi, D. O. Miller, S. A. Montzka, F. L. Moore, E. J. Morgan, D. M. Murphy, L. T. Murray, B. A. Nault, J. Andrew Neuman, L. Nguyen, Y. Gonzalez, A. Rollins, K. Rosenlof, M. Sargent, G. Schill, J. P. Schwarz, J. M. St. Clair, S. D. Steenrod, B. B. Stephens, S. E. Strahan, S. A. Strode, C. Sweeney, A. B. Thames, K. Ullmann, N. Wagner, R. Weber, B. Weinzierl, P. O. Wennberg, C. J. Williamson, G. M. Wolfe, L. Zeng, THE NASA ATMOSPHERIC TOMOGRAPHY (ATom) MISSION: Imaging the Chemistry of the Global Atmosphere. *Bull. Am. Meteorol. Soc.* **1**, 1–53 (2021).

Will be added in revised version

- L161: “**into** one new housing”

Will be changed in revised version

- L244: “Thus, flow calibrations and size calibration will not change, need to be calibrated

only once, and later on only have to be checked.”. Agreed. But can you elaborate on how often these checks are done in practice?

This is not defined yet. The goal is to do these checks on a routine basis between the flight sequences. It is currently foreseen that the instrument will be brought back from KIT to MPIC after the IACOS-CARIBIC container is back at KIT after a flight sequence of four or six consecutive flights. The time the instrument remains at our lab is then about 2 or 3 weeks. However, this requires that the personal resources are available, and also assumes that no other instrumental problems have occurred. If no instrumental issues have occurred, the data will be downloaded, the IE calibration, flow and size calibrations checks and other routine checks of instrumental performance will be done.

- L387: “...than at the end of the flight”

Will be changed in revised version

References:

- Bahreini, R., Ervens, B., Middlebrook, A. M., Warneke, C., de Gouw, J. A., DeCarlo, P. F., Jimenez, J. L., Brock, C. A., Neuman, J. A., Ryerson, T. B., Stark, H., Atlas, E., Brioude, J., Fried, A., Holloway, J. S., Peischl, J., Richter, D., Walega, J., Weibring, P., Wollny, A. G., and Fehsenfeld, F. C.: Organic aerosol formation in urban and industrial plumes near Houston and Dallas, Texas, *Journal of Geophysical Research: Atmospheres*, 114, <https://doi.org/10.1029/2008JD011493>, 2009.
- Brock, C. A., Froyd, K. D., Dollner, M., Williamson, C. J., Schill, G., Murphy, D. M., Wagner, N. J., Kupc, A., Jimenez, J. L., Campuzano-Jost, P., Nault, B. A., Schroder, J. C., Day, D. A., Price, D. J., Weinzierl, B., Schwarz, J. P., Katich, J. M., Wang, S., Zeng, L., Weber, R., Dibb, J., Scheuer, E., Diskin, G. S., DiGangi, J. P., Bui, T., Dean-Day, J. M., Thompson, C. R., Peischl, J., Ryerson, T. B., Bourgeois, I., Daube, B. C., Commane, R., and Wofsy, S. C.: Ambient aerosol properties in the remote atmosphere from global-scale in situ measurements, *Atmos. Chem. Phys.*, 21, 15023-15063, [10.5194/acp-21-15023-2021](https://doi.org/10.5194/acp-21-15023-2021), 2021.
- Drewnick, F., Hings, S. S., Alfarra, M. R., Prevot, A. S. H., and Borrmann, S.: Aerosol quantification with the Aerodyne Aerosol Mass Spectrometer: detection limits and ionizer background effects, *Atmos. Meas. Tech.*, 2, 33-46, [10.5194/amt-2-33-2009](https://doi.org/10.5194/amt-2-33-2009), 2009.
- Hermann, M., Weigelt, A., Assmann, D., Pfeifer, S., Müller, T., Conrath, T., Voigtländer, J., Heintzenberg, J., Wiedensohler, A., Martinsson, B. G., Deshler, T., Brenninkmeijer, C. A. M., and Zahn, A.: An optical particle size spectrometer for aircraft-borne measurements in IAGOS-CARIBIC, *Atmos. Meas. Tech.*, 9, 2179-2194, [10.5194/amt-9-2179-2016](https://doi.org/10.5194/amt-9-2179-2016), 2016.
- Hu, W., Campuzano-Jost, P., Day, D. A., Croteau, P., Canagaratna, M. R., Jayne, J. T., Worsnop, D. R., and Jimenez, J. L.: Evaluation of the new capture vaporizer for aerosol mass spectrometers (AMS) through field studies of inorganic species, *Aerosol Sci. Technol.*, 51, 735-754, [10.1080/02786826.2017.1296104](https://doi.org/10.1080/02786826.2017.1296104), 2017.
- Hu, W., Campuzano-Jost, P., Day, D. A., Nault, B. A., Park, T., Lee, T., Pajunoja, A., Virtanen, A., Croteau, P., Canagaratna, M. R., Jayne, J. T., Worsnop, D. R., and Jimenez, J. L.: Ambient Quantification and Size Distributions for Organic Aerosol in Aerosol Mass Spectrometers with the New Capture Vaporizer, *ACS Earth and Space Chemistry*, 4, 676-689, [10.1021/acsearthspacechem.9b00310](https://doi.org/10.1021/acsearthspacechem.9b00310), 2020.
- Joppe, P., Schneider, J., Wilsch, J., Bozem, H., Breuninger, A., Curtius, J., Ebert, M., Emig, N., Hoor, P., Ismayil, S., Kandler, K., Kunkel, D., Kurth, I., Lachnitt, H. C., Li, Y., Miltenberger, A., Richter, S., Rolf, C., Schneider, L., Schwenk, C., Spelten, N., Vogel, A. L., Cheng, Y., and Borrmann, S.:

- Transport of Biomass Burning Aerosol into the Extratropical Tropopause Region over Europe via Warm Conveyor Belt Uplift, *EGUsphere*, 2025, 1-39, 10.5194/egusphere-2025-1346, 2025.
- Knote, C., Brunner, D., Vogel, H., Allan, J., Asmi, A., Äijälä, M., Carbone, S., van der Gon, H. D., Jimenez, J. L., Kiendler-Scharr, A., Mohr, C., Poulain, L., Prévôt, A. S. H., Swietlicki, E., and Vogel, B.: Towards an online-coupled chemistry-climate model: evaluation of trace gases and aerosols in COSMO-ART, *Geosci. Model Dev.*, 4, 1077-1102, 10.5194/gmd-4-1077-2011, 2011.
- Liu, P. S. K., Deng, R., Smith, K. A., Williams, L. R., Jayne, J. T., Canagaratna, M. R., Moore, K., Onasch, T. B., Worsnop, D. R., and Deshler, T.: Transmission efficiency of an aerodynamic focusing lens system: Comparison of model calculations and laboratory measurements for the Aerodyne Aerosol Mass Spectrometer, *Aerosol Sci. Technol.*, 41, 721-733, 10.1080/02786820701422278, 2007.
- Mei, F., Wang, J., Comstock, J. M., Weigel, R., Krämer, M., Mahnke, C., Shilling, J. E., Schneider, J., Schulz, C., Long, C. N., Wendisch, M., Machado, L. A. T., Schmid, B., Krisna, T., Pekour, M., Hubbe, J., Giez, A., Weinzierl, B., Zoeger, M., Pöhlker, M. L., Schlager, H., Cecchini, M. A., Andreae, M. O., Martin, S. T., de Sá, S. S., Fan, J., Tomlinson, J., Springston, S., Pöschl, U., Artaxo, P., Pöhlker, C., Klimach, T., Minikin, A., Afchine, A., and Borrmann, S.: Comparison of aircraft measurements during GoAmazon2014/5 and ACRIDICON-CHUVA, *Atmos. Meas. Tech.*, 13, 661-684, 10.5194/amt-13-661-2020, 2020.
- Middlebrook, A. M., Roya, B., L., J. J., and Canagaratna, M. R.: Evaluation of Composition-Dependent Collection Efficiencies for the Aerodyne Aerosol Mass Spectrometer using Field Data, *Aerosol Sci. Technol.*, 46, 258-271, 10.1080/02786826.2011.620041, 2012.
- Molleker, S., Helleis, F., Klimach, T., Appel, O., Clemen, H. C., Dragoneas, A., Gurk, C., Hünig, A., Köllner, F., Rubach, F., Schulz, C., Schneider, J., and Borrmann, S.: Application of an O-ring pinch device as a constant-pressure inlet (CPI) for airborne sampling, *Atmos. Meas. Tech.*, 13, 3651-3660, 10.5194/amt-13-3651-2020, 2020.
- Reifenberg, S. F., Martin, A., Kohl, M., Bacer, S., Hamryszczak, Z., Tadic, I., Röder, L., Crowley, D. J., Fischer, H., Kaiser, K., Schneider, J., Dörich, R., Crowley, J. N., Tomsche, L., Marsing, A., Voigt, C., Zahn, A., Pöhlker, C., Holanda, B. A., Krüger, O., Pöschl, U., Pöhlker, M., Jöckel, P., Dorf, M., Schumann, U., Williams, J., Bohn, B., Curtius, J., Harder, H., Schlager, H., Lelieveld, J., and Pozzer, A.: Numerical simulation of the impact of COVID-19 lockdown on tropospheric composition and aerosol radiative forcing in Europe, *Atmos. Chem. Phys.*, 22, 10901-10917, 10.5194/acp-22-10901-2022, 2022.
- Schulz, C., Schneider, J., Amorim Holanda, B., Appel, O., Costa, A., de Sá, S. S., Dreiling, V., Fütterer, D., Jurkat-Witschas, T., Klimach, T., Knote, C., Krämer, M., Martin, S. T., Mertes, S., Pöhlker, M. L., Sauer, D., Voigt, C., Walser, A., Weinzierl, B., Ziereis, H., Zöger, M., Andreae, M. O., Artaxo, P., Machado, L. A. T., Pöschl, U., Wendisch, M., and Borrmann, S.: Aircraft-based observations of isoprene-epoxydiol-derived secondary organic aerosol (IEPOX-SOA) in the tropical upper troposphere over the Amazon region, *Atmos. Chem. Phys.*, 18, 14979-15001, 10.5194/acp-18-14979-2018, 2018.
- von der Weiden, S. L., Drewnick, F., and Borrmann, S.: Particle Loss Calculator – a new software tool for the assessment of the performance of aerosol inlet systems, *Atmos. Meas. Tech.*, 2, 479-494, 10.5194/amt-2-479-2009, 2009.