


Figure 9. Calibration (a) of simulated soil respiration rates (May 1998- Dec 2000) and validation period (June, 2022 – May, 2023)

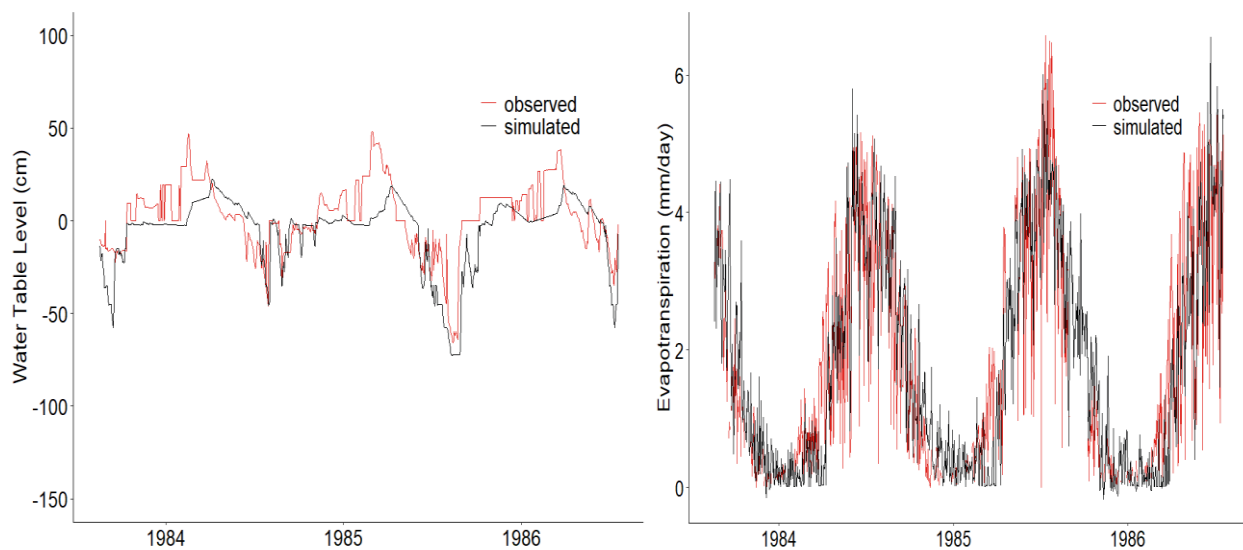

Figures 5 & 8: Calibration period of simulated water table level (left) and evapotranspiration (right) from 1983 to 1987