

Dear reviewer,

Based on your general comments, we would like to express our gratitude for recognizing that this effort can complement INTERMAGNET standards and benefit the global community working on long-term geomagnetic observations. We have considered each of your recommendations and made an effort to address them since we think that supporting the article's statements about data quality enhances this work. Along with the basic writing and English, we also believed that there were certain coherence and structural issues that were assessed and solved.

You can find in blue your comments and in black our response.

According to your comments those issues were added:

GENERAL COMMENTS

However, some aspects of the manuscript need improvement. The discussion of benefits is often too general and theoretical. Although many advantages of the QMS are listed (e.g., clear goals, risk analysis, continuous improvement), the paper lacks concrete, measurable examples that show how these benefits translated into better data quality, more efficient operations, or problem-solving at Teoloyucan. It would be necessary to include specific evidence - such as improvements in baselines determination.

Recommendation: Accept with major revisions, focused on:

- Adding specific, measurable outcomes to support the claimed benefits,
- Correcting structural inconsistencies (especially regarding figures and references),
- Improving the overall clarity and language quality of the text.

Several specific aspects were included, related with both the operation and the data.

-Figure 5 was changed to show in detail the possible risks during the observatory operation and how these risks can be managed to reduce the consequences:

Risk	Event that can cause	Probability/ frequency	Consequence /damage	Risk assessment (F vs D)	Mitigation actions	Occured	Consequence	Risk reassessment (F vs D)	New mitigation actions
Pandemic/strikes	No access to the facilities	Probable	Critical	9	Alternate center for downloading and processing information	No	None	6	None
Lack of supplier inventory	Not being able to replace faulty equipment/Stop recording data	Probable	Critical	9	Look for another provider	No	None	6	None
Long acquisition times	Not being able to replace faulty equipment/Stop recording data	Probable	Critical	9	Constant communication with the administration	No	None	6	None
Extreme phenomena	Stop recording data	Remote	Catastrophic	8	Backup equipment	No	None	8	None
Theft/vandalism	Stop recording data	Remote	Catastrophic	8	Surveillance and access control	No	None	8	None
Magnetic noise	Noisy data	Remote	Critical	6	Constant data quality control and surveys to detect Magnetic objects	No	None	6	None
Instrumental damage	Stop recording data	Probable	Catastrophic	12	Backup instruments	No	None	8	None
Lack of internet for streaming	Real-time reporting of data cannot be performed	Probable	Critical	9	Have a second way to download data	Yes	It affected the website display time	9	Have a second way to download data and request support from RedUNAM
Logical errors on the server		Probable	Critical	9	Second server that can perform the processing	No	None	9	None
Power outage		Probable	Critical	9	Backup power system in case of prolonged power outages	No	None	9	None

Figure 5. Reduced risk matrix of the Magnetic Service

-Figure 6 was improved to detail the activities and responsibilities of the staff:

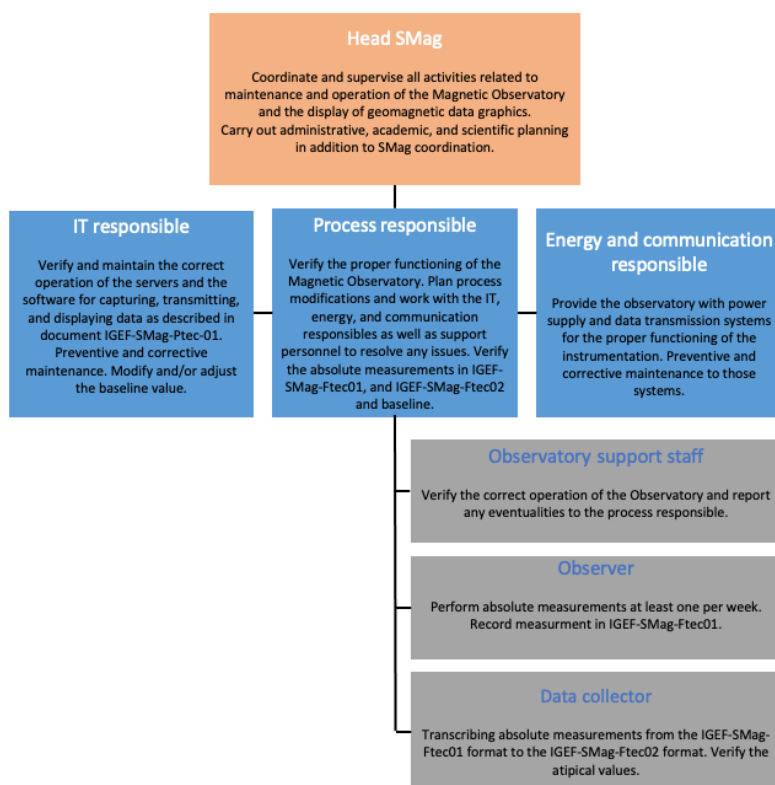


Figure 6. Magnetic Service organizational chart

-Instrumental control and logbook were described with more specific activities. If considered additional charts could be added to should the flagging of the activities and events on the observatory graphs:

Line 164 -169: Within the *management documents*, in the part corresponding to *instrument control*, there is a format (SMag IGEF-FPG02-01) that contains the inventory of instruments and servers, their characteristics, and their location. There is also a format (SMag IGEF-FPG02-03) that tracks instrument maintenance, such as routine cleaning of servers, antivirus revision, delta F measurement, theodolite maintenance, comparison with Theo 010A DI-flux, cleaning, verification and adjustment, and internal cleaning of LEMI 025 memory, among others (Bracke, 2025), The instruments maintenance format, includes the equipment, activity, responsible, date of last maintenance and date for the next, it is also link to a calendar to remind the activity.

Complementary to the records of the equipment and its maintenance, there is a logbook to record failures that occur in the equipment or systems, record any maintenance activity, either preventive or corrective, and record changes or events that produce disturbances in data that affect data quality.

-Figure 7 was improved:

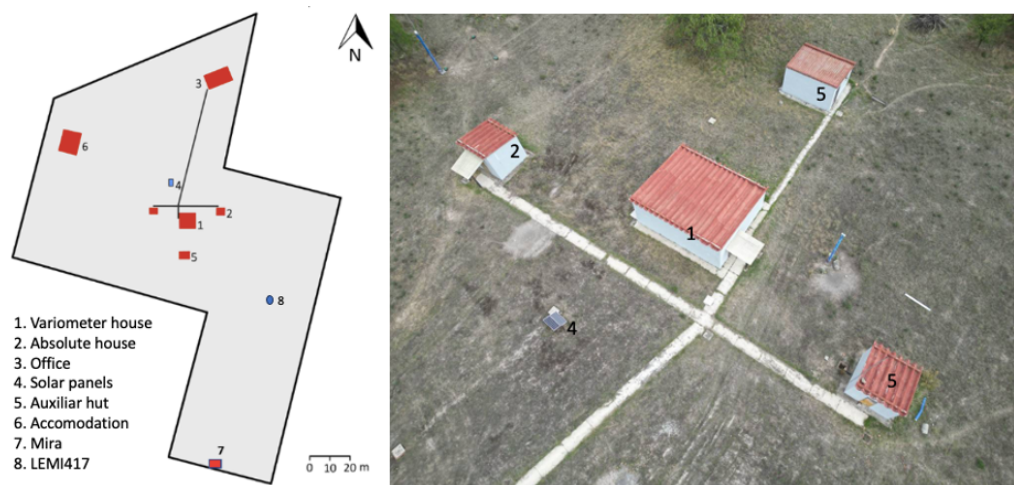


Figure 7. a) TEO's schematic drawing and b) aerial photo

-A variometer section was added to describe the specific activities of quality control: thermal stability (Figure 10), comparison with another variometer (LEMI417) in the observatory (Figure 11) and with other close latitude observatory, San Juan (SJG)(Figure 12).:

Line 246: To control the proper operation of the variometer, several continuous tests are performed. The variometer LEMI 025 is in the variometer house in an isolated room, temperature control is performed to check the thermal stability (Figure 10).

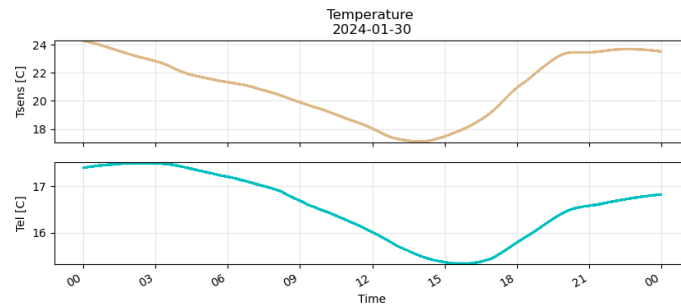


Figure 10. Temperature at the variometer house. Above temperature at the sensor, below temperature at the electronic unit. (Elaborated with Magpy V2, (Leonhardt et al., 2025))

It is also compared to a variometer LEMI 417 located outside, 50 m from the variometer house (Figure 11):

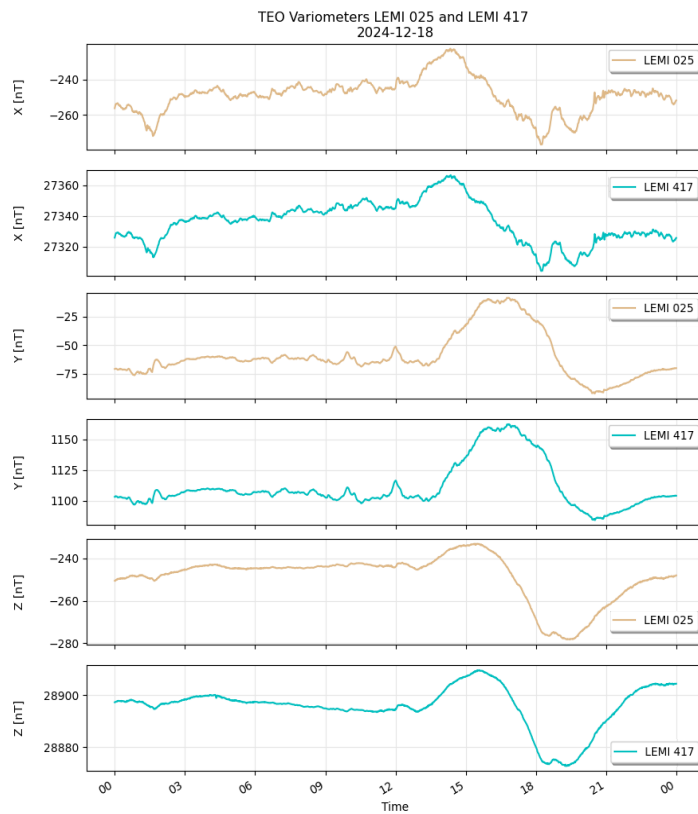


Figure 11. Variometers comparison: LEMI 025 vs LEMI 417. X, Y, Z components. (Elaborated with Magpy V2, (Leonhardt, et al., 2025))

It also is compared daily to another observatory at a similar latitude (18.111°N , 293.85°E), San Juan (SJG) and used to observe and remove spikes (Figure 12):

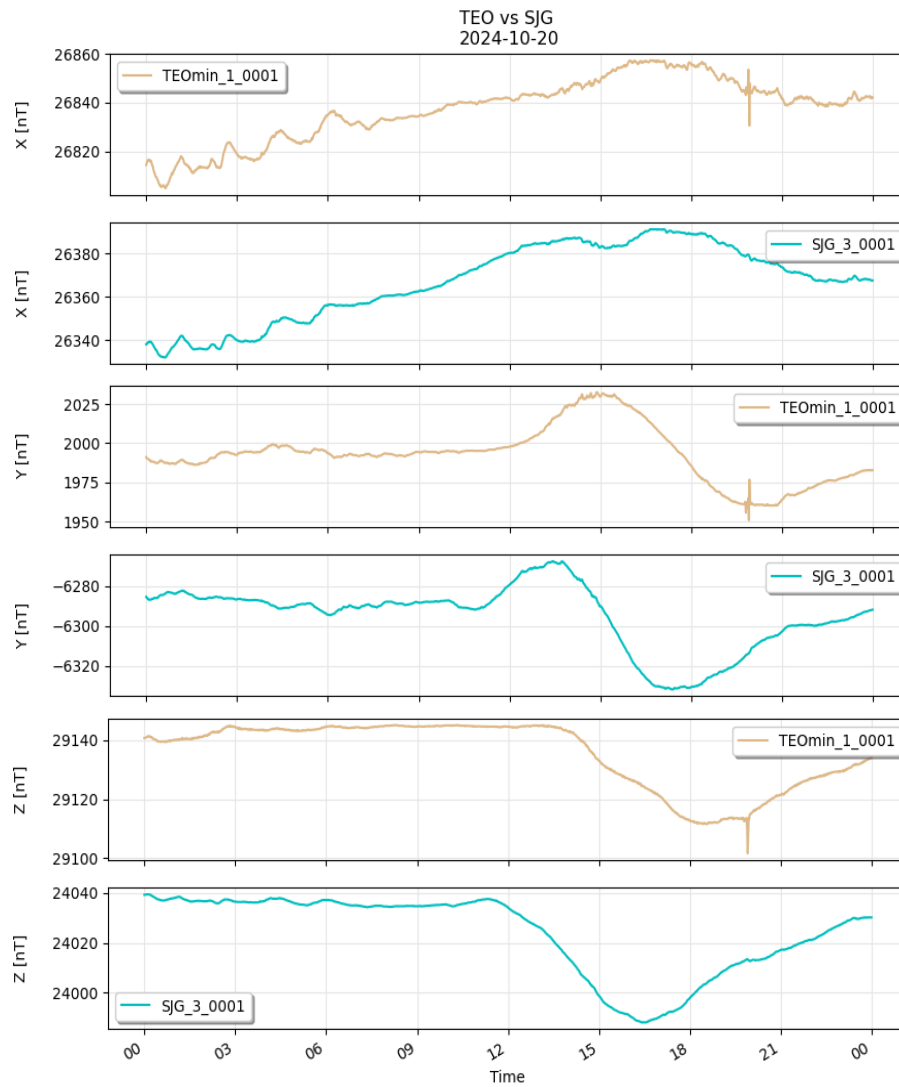


Figure 12. Teoloyucan Magnetic Observatory (TEO) compare with San Juan Magnetic Observatory (SJG). X, Y, Z components. (Elaborated with Magpy V2, (Leonhardt et al., 2025))

-Also, was added a paragraph about absolute measurements, inter comparison with other DI-flux measurements (Theo010A) and with other observatories instruments in the IAGA Workshop. And a description and graph (Figure 14) of basevalues and baselines calculation utilizing the Magpy V2 software.

Line 29: It also describes how to perform absolute measurements (Rasson, 2004) and the format (IGEF-SMag-Ftec01-01) where the measurements are recorded (Figure 13). Absolute measurements are performed at least once a week by the observer, avoiding intervals of magnetic activity and to ensure that no magnetic materials, which would cause jumps in baselines are present, inside or outside the absolute (or variometer) buildings, or with the observer (Bracke, 2025).

Line 297: Then this information is captured by the data collector in the format (IGEF-SMag-Ftec01-02) and double-checked by the process responsible to avoid capture errors or identify spikes. It is also important to consider that few times a year the absolute measurement is performed with a DI-flux Zeiss Theo 010A from MinGEO to compare results. And that observers participate in the IAGA workshops on Geomagnetic Observatory Instruments, Data Acquisition and Processing also to compare the absolute measurements.

With this format the baseline is generated. Complementary, these basevalues are adapted to calculate the observatory baseline using the Magpy software (Leonhardt et al., 2025), along with variometer, and total intensity data (Figure 14):

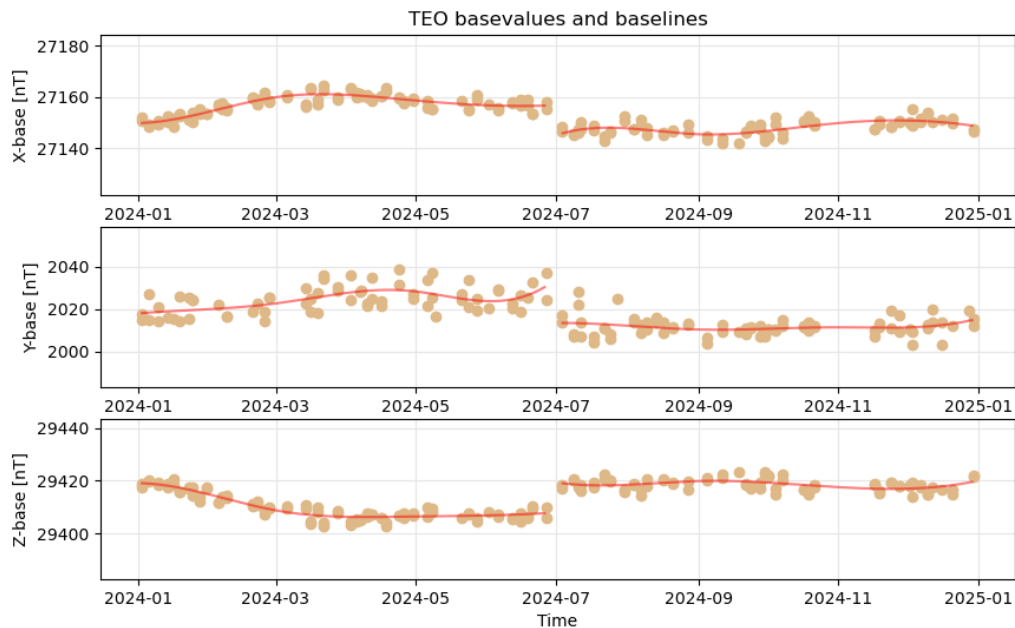


Figure 14. Basevalues and baselines for TEO 2024. XYZ (calculated and elaborated with Magpy V2 (Leonhardt et al., 2025))

It is important to mention that this procedure includes only the display of geomagnetic data in quasi-real time, i.e. reported data: Vector measurements performed by a continually recording magnetometer are typically variation measurements and variation data and as considered since Technical Manual V4.0 (1999), variometer data are corrected to near absolute values using the best available baseline estimates at the time of transmission (Bracke, 2025)

- Conclusions were modified specifying benefits in the operation and quality data. Including the percentage of annual data (96.49%-2022, 95.66%-2023, 99.43%-2024).

Line 348: 4. Conclusions

Certification under the ISO 9001:2015 standard has been designed for industry and business; however, it can be used in academic and research environments, as has been seen in this case. Its usefulness for this case has been mainly to document in detail the operation and generation of a final product under quality standards such as TEO's Graphic Display of Geomagnetic Data (Figure 18a), and for more information about the certificate or the QMS, consult the QR code (Figure 18b).

This certification includes only the display of geomagnetic data in quasi-real time, i.e. reported data: variometer data corrected to near absolute values using the best available baseline estimates at the time of transmission. Based on the results obtained, it is considered to extend the scope of the certification to the procedure for generating adjusted and definitive data. Risks were managed and decreased, contributing to achieve the quality objective of the QMS, was satisfied acquiring more than 90% of data per year (96.49%-2022, 95.66%-2023, 99.43%-2024). Continuous checking of the data and activity log, helps to control the data quality.

There are several advantages of implementing a QMS and obtaining an ISO 9001:2015 certification including setting clear objectives, systematically analyzing risks, creating a culture of continuous improvement, promoting context analysis through a SWOT, and strategic planning based on this knowledge, and semiannual audits. Elaboration of all the documents associated with the operating procedures of a geomagnetic observatory and the continuity of the processes mentioned above guarantee TEO's operation, including both production of data and its availability in real time for users.

- Additionally, the structure of the manuscript is somewhat inconsistent. Several figures (1, 2, 4, 6, 12, and 13) are not referenced in the text, and some citations are unclear or incomplete. These issues have to be addressed to improve the clarity and coherence of the article.

References to Figure 1, 2,4,6, 12 and 13 (now 16 and 17) were added to text:

Line 37: It has operated in the town of Teoloyucan, State of Mexico (Figure 1), since August 1914,

Line 49: The present operational buildings were constructed during this period (Figure 2).

Line 136: As show in Figure 4, this analysis offers different possibilities;

Line 156: For the operation of the Magnetic Observatory of Teoloyucan, the Magnetic Service defined the following organization chart (Figure 6):

Line 325: On the website, the day before, current day, weekly, and 27-day (Carrington rotation) graphs are shown for the present day, but any previous day can be consulted (Figures 16 and 17).

SPECIFIC COMMENTS

- Line 41. Reference to the wrong figure, because Figure 3 is about “Structure of a Quality Management ...”

Corrected, it was Figure 2 and the place of the reference was changed.

Line 49: The present operational buildings were constructed during this period (Figure 2).

- Line 53. What does the abbreviation DFI mean? It is not explained anywhere.

Explained and the beginning of the Introduction:

Line 30: The components of the magnetic field vector, include total intensity (F), horizontal (H), vertical (Z), north (X), east (Y), declination (D), and inclination (I).

- Line 64. The abbreviation DI is introduced but not used later.

A paragraph was added to name the components of the magnetic field vector.

Line 30: The components of the magnetic field vector, include total intensity (F), horizontal (H), vertical (Z), north (X), east (Y), declination (D), and inclination (I).

- Line 65. This is the first time the abbreviation QMS is used. It's better to write the full name here with "QMS" in parentheses, even though the full name appears in the title of the article.

Corrected. Quality Management System (QMS)

Line 12: Given the nature of Quality Management Systems (QMS) based on ISO 9001:2015

- Lines 79,84. This item is missing from the References.

The reference was added:

Line 390: Godínez-Méndez, W.: The Implementation of Quality Management Systems in Law Libraries: Esquemas de trabajo híbrido y nuevos escenarios internacionales en las bibliotecas jurídicas, edited by Hernández Pacheco, Federico. ISBN: 978-607-30-7824-5, 2023.

- Line 221. There should probably be a reference to Fig. 7 here.

Reference to Figure 7 corrected.

Line 225: A schematic drawing of the Teoloyucan Magnetic Observatory is shown in Figure 7: absolute and variometer houses, two auxiliary huts, and an office.

- Line 225. There is an unnecessary comma after the word "hut." The whole sentence is complicated and hard to read.

Corrected. The paragraph was rewritten more clearly, and Figure 7 has been updated with the right names.

Line 228: The observatory was built following the established standards: the absolute observations house has two pillars for measurements, is built of non-magnetic materials, and has a window to observe the azimuth mark, located 70 m away; the variometer house consists of an outer corridor and an inner isolated room. The inner room is equipped with five solid pillars, is built of non-magnetic materials. In one of those pillars is the LEMI 025 sensor. In the outer corridor is located the electronics of the LEMI 025, in the norther part the GSM90 magnetometer, and in the other side the power and transmission systems. The instruments are powered by solar panels (Figure 7). The data are transmitted by optic fiber to the office since 2022, to avoid problems due to currents induced by lightning strikes. Instruments are shown in Figure 8.

Line 314 It's worth making the whole References section consistent with the chosen style, as much as possible.

All References were checked and corrected.

- Line 315. Punctuation. It's worth to add the DOI: <https://doi.org/10.1093/labmed/27.6.375>

Added

Line 382: Berte, L., and Nevalainen, D.: Managers' Documentation Pyramid for a Quality System. V. 27, N. 6 Laboratory Medicine, <https://doi.org/10.1093/labmed/27.6.375>, 1996.

- Line 331. This item is listed in the References but is not cited anywhere in the article.

It was added The missing reference was added:

Line 202 Besides being a standard requirement, audits enable confirming if the QMS complies with both its own and the standard's requirements, as well as whether its deployment and operation are successful. Even though it could seem like a laborious process at first, having these systematic evaluations allows one to ensure that every item outlined in the technical procedure and the QMS is promptly addressed (Kaziliūnas, 2010),

Line 338 Should be probably: Rasson, J.L., Toh, H., Yang, D. (2011). The Global Geomagnetic Observatory Network. In: Mande, M., Korte, M. (eds) Geomagnetic Observations and Models. IAGA Special Sopron Book Series, Vol 5. Springer, Dordrecht. https://doi.org/10.1007/978-90-481-9858-0_1

Corrected.

Line 409 Rasson, J. L., Toh, H., and Yang, D.: The Global Geomagnetic Observatory Network, in: Geomagnetic Observations and Models, edited by Mande, M. and Korte, M, IAGA Special Sopron Book Series 5Springer Netherlands, 1-25, <https://doi.org/10.1007/978-90-481-9858-01>, 2011.

TECHNICAL CORRECTIONS

- Lines 30,65,85 The author "Brake" is missing in the References. It is probably meant to be "Bracke."

Corrected

Line 30, 66, 95, 165, 294 (Bracke, 2025)

- Line 35 There is a missing dot after "al"

Corrected:

Line 35 Rasson et al., 2011

- Line 81 It should be “Figure 3” (the dot is not needed)

Corrected:

Line 90 **Figure 3:**

- Line 283 There is a missing comma after the word "however"

Added

Line 349 however, it can be used in academic and research environments,

Line 339 There is missing “d” in “edited”

Added

Line 410 edited by Mande, M. and Korte,

