

Operational performance of the Vaisala CL61 ceilometer for atmospheric profiling

Viet Le¹, Ewan J. O'Connor¹, Maria Filioglou², and Ville Vakkari^{1,3}

¹Finnish Meteorological Institute, Helsinki, 00101, Finland

²Finnish Meteorological Institute, Atmospheric Research Centre of Eastern Finland, Kuopio, Finland

³Atmospheric Chemistry Research Group, Chemical Resource Beneficiation, North-West University, Potchefstroom, 2520, South Africa

Correspondence: Viet Le (viet.le@fmi.fi)

Abstract. The Vaisala CL61 is a new generation elastic backscatter lidar that extends conventional ~~ceilometer~~-Automatic Lidar-Ceilometer capabilities by providing depolarization ratio measurements. Reliable use of these measurements, however, requires thorough evaluation and characterisation of the instrument performance and subsequent corrections applied.

~~This study introduces a methodology for identifying the background signal and suitable liquid cloud layers for assessing the~~
5 ~~long-term behavior~~ In this study, performance of multiple CL61 instruments ~~deployed across various sites across different sites~~
over 3 years period have been assessed. Results indicate some ~~variability differences~~ between instruments, with most of these
early production units exhibiting a pronounced decrease in laser power over time, accompanied by an increase in background
noise likely due to weaker return signal. Normally, the instrument scales the internal calibration factor to compensate for
changes in laser power and thus provide consistent attenuated backscatter coefficient values from profile to profile over time.
10 However, for the instrument at the Lindenberg site, by performing manual calibration with atmospheric targets it ~~was~~-is noted
that once the laser power dropped below 40% there ~~was~~-is no further compensation in the internal calibration factor.

The instrumental background noise and bias, characterized using the termination hood, ~~were~~-are found to vary with temperature. A method ~~was~~-has been developed for correcting ~~for~~ the instrumental bias and for estimating the associated uncertainty. Additionally, an ~~aerosol inversion approach is presented for retrieving the profile of aerosol particle backscatter coefficient,~~
15 ~~aerosol depolarization ratio, and their corresponding uncertainties~~approach to estimate the uncertainty of volume and particle
backscatter and linear depolarization ratio is presented. In a case study ~~, the aerosol inverted and representing low aerosol load~~
condition in Finland, the bias-corrected ~~depolarization ratio was~~-particle linear depolarization ratio has been found to deviate by
up to 0.1 from the original instrument-provided ~~measurement~~volume linear depolarization ratio. This demonstrates the importance of accounting for the molecular contribution ~~when qualitatively in both volume backscatter and linear depolarization ratio~~
20 when quantitatively interpreting aerosol measurements ~~at by~~ the CL61 ~~ceilometer operating wavelength of 905 nm~~Automatic
Lidar-Ceilometer operating at the wavelength of 910.55 nm. Finally, signal loss in one unit ~~was traced to optical lens fogging~~
has been traced to fogging of the inside surface of the window, and attributed to insufficient internal heating linked to the
instrument's firmware behavior.

1 Introduction

25 ~~Ceilometers~~ Automatic Lidar-Ceilometer (ALC) are ground-based elastic backscatter lidars originally developed for the automated detection of cloud base height to support aviation and meteorological operations. Over the past two decades, advancements in both hardware and data processing have greatly enhanced their capabilities (Cimini et al., 2020). Notably, improvements in signal quality, particularly in signal-to-noise ratio, now enable ~~ceilometers~~ ALC to provide profiles of attenuated backscatter coefficient with sufficient dynamic range to permit the observation of a wide range of atmospheric phenomena, including rainfall (e.g. Rocadenbosch et al., 2020; Roschke et al., 2025), fog (e.g. Haeffelin et al., 2016; Ribaud et al., 2021), icing (e.g. Härmäläinen et al., 2020), and even the quantitative estimation of aerosol concentrations (e.g. Shang et al., 2021; Filioglou et al., 2025). ~~Ceilometer~~ ALC data are also increasingly used to estimate atmospheric boundary layer height (e.g. Kotthaus et al., 2023), which is a critical parameter for numerical weather prediction and air quality models (e.g. Uzan et al., 2020; Barragán et al., 2023). Their ability to operate autonomously and reliably in challenging environmental conditions, as well as being eye-safe, makes them well-suited for long-term monitoring and integration into operational networks of national meteorological services and research institutions (e.g. Hirsikko et al., 2014). Many such organizations are actively investigating the use of ~~ceilometer~~ ALC profile data to improve forecast model performance (e.g. Warren et al., 2018; Illingworth et al., 2019).

Vaisala has recently introduced the CL61 ceilometer which is an ALC with the capability of measuring the volume linear depolarization ratio, $\delta\delta_y$, which is the ratio of the perpendicular to the parallel component of the backscattered signal relative to the emitted polarization. This ratio provides insight into particle sphericity (e.g. Burton et al., 2012; Mamouri and Ansmann, 2016; Baars et al., 2017) and is essential for distinguishing various aerosol types (e.g. Illingworth et al., 2015; Nicolae et al., 2018; Floutsi et al., 2023; Filioglou et al., 2023; Le et al., 2024) such as pollen, smoke, dust, marine, and volcanic ash. It is also utilized in determining cloud phase (Sassen, 1991) and in the retrieval of cloud microphysical properties (Donovan et al., 2015).

To fully leverage the broad range of applications enabled by the CL61 ~~ceilometer~~, including its new capability to measure ~~the depolarization ratio~~ $\delta\delta_y$, careful quality control of the backscattered signal from both polarizations is essential. Environmental conditions, such as temperature and relative humidity, can influence lidar performance (Campbell et al., 2002), making it necessary to assess their impact on data quality. For instance, Hervo et al. (2016) identified and corrected a temperature-dependent effect on the overlap function of a Lufft CHM15K ceilometer, which arises from temperature-induced changes in the laser as well as in the instrument's optical and electronic components. Similarly, the older Vaisala CL31 ceilometer has been known to have backscatter artifacts below approximately 70 m (Van der Kamp, 2008; Martucci et al., 2010; Tsaknakis et al., 2011), prompting many studies to omit these near-surface measurements. Identifying and correcting such artifacts in the CL61 would enable reliable observations extending ~~all the way to the surface~~ down to heights that overlap with surface-based observations. This capability is especially valuable for studying near-surface meteorological phenomena such as fog, haze, and emissions from ground-level aerosol sources.

In this study, we present a long-term evaluation of the CL61 ~~ceilometer~~ceilometers conducted at four different ACTRIS cloud profiling sites in Finland and Germany. Our analysis focuses on the impact of laser power on signal quality, the temperature sensitivity of the ~~optical path~~, instrumental background and methods for its correction. Additionally, we demonstrate our calculation of the uncertainty in the volume and particle ~~depolarization ratio~~linear depolarization ratio (δ_v and δ_p respectively). Finally, we report instances of signal loss attributed to ~~lens fogging~~fogging of the inside surface of the window, observed in some of the CL61 units.

2 Instrument description

The CL61 ceilometer, manufactured by Vaisala, is a coaxial ~~lidar~~ALC system operating at a wavelength of 910.55 nm and equipped with depolarization measurement capability. Its key technical specifications are summarized in Table 1. In brief, the CL61 utilizes an InGaAs diode laser that emits linearly ~~polarised~~polarized pulses with an energy of 3.9 μJ at a repetition rate of 9.5 kHz. The instrument features a single-lens optical design and performs depolarization measurements using a single-receiver with an avalanche photodiode (APD) detector that switches between two polarising filters (one perpendicular and one parallel to the polarisation of the transmitted pulses) in the same coaxial optical path. The CL61 alternates the acquisition of each polarization every 0.2 s, while using the same receiver module for both channels. Consequently, receiver sensitivity calibration is not required. The maximum detection range of CL61 is 15.4 km.

The overlap functions are shown in Fig. S1. Full overlap between the transmitted laser beam and the receiver field of view is achieved at approximately 250 m ~~above ground level, with a maximum detection range of 15.4 km.~~ range for the instrument at Kenttäröva. The instruments at Vehmasmäki and Hyytiälä have different overlap functions, with approximately 95% overlap at 250 m range and complete overlap at approximately 550 m range. The overlap function is reported only in the new firmware data and remains constant throughout the period. No overlap function was reported for the instrument at Lindenberg.

Data collected up to December 2024 from four CL61 ~~ceilometers~~ deployed at four different ACTRIS Cloudnet sites were analyzed. Three of these instruments are situated in Finland: Hyytiälä, Vehmasmäki, and Kenttäröva, while the fourth is located in Lindenberg, Germany. The firmware versions of the instruments, along with their respective periods of validity, are presented in Table 2. The data from this study were obtained from the ACTRIS Cloudnet data portal (Görsdorf et al., 2025).

The CL61 is equipped with an internal heater to stabilize the temperatures of the laser and optical components. It includes a window heater and blower to maintain stable window conditions, as the window's transmission efficiency significantly affects the backscattered signal (see Sect. 4.3). The instrument's firmware continuously monitors and reports various housekeeping variables, such as internal temperature, laser temperature, window condition (calculated internally on a scale from 0% for a fully obstructed window to 100% for a clean window), and the status of the window blower heater. The quantity and type of variables reported may differ based on the firmware version.

Table 1. Specifications of the CL61 (CL61 User Guide: <https://docs.vaisala.com/r/M212475EN-E/en-US>, last access: 21 July 2025).

Specification	Values
Laser wavelength	910.55 nm
Laser	InGaAs diode
Beam divergence	$\pm 0.2 \text{ mrad} \times \pm 0.35 \text{ mrad}$
<u>Receiver field-of-view</u>	<u>$\pm 0.56 \text{ mrad}$</u>
Measurement maximum range	15400 m
Reporting range resolution	4.8 m
Measurement interval	5 s
Pulse duration	160ns (at Full Width Half Maximum)
Pulse frequency	9.5 kHz
Maximum pulse energy	$4.7 \mu\text{J}$
<u>Height of complete overlap</u>	<u>250 m (in Kenttäröva) and 550 m (in Vehmasmäki and Hyytiälä)</u>

Table 2. Firmware version of the CL61 across all the site locations.

Site and coordinate	Time	Firmware version
Vehmasmäki 62.738°N, 27.543°E	2022-01-01 to 2022-06-14	not stated
	2022-06-15 to 2023-04-27	1.1.10
	2023-04-28 to 2024-12-31	1.2.7
Hyytiälä 61.844°N, 24.287°E	2022-01-01 to 2022-11-20	not stated
	2022-11-21 to 2023-11-22	1.1.10
	2023-11-23 to 2024-12-31	1.2.7
Kenttäröva 67.987°N, 24.243°E	2022-01-01 to 2022-06-20	not stated
	2022-06-21 to 2024-12-31	1.2.7
Lindenberg 52.208°N, 14.118°E	2024-03-01 to 2024-12-31	1.1.10

3 Methods

The CL61 operates by emitting pulses of linear polarized laser light into the atmosphere and recording the backscattered signal. The received power per laser pulse is described by the lidar equation (Wandinger, 2005):

$$90 \quad P(r) = \frac{1}{r^2} C_L O(r) \beta(r) e^{-2 \int_0^r \alpha(r') dr'} + B. \quad (1)$$

Here, $O(r)$ is the overlap function that is unique to each instrument and is provided by the manufacturer. The coefficients α and β represent atmospheric extinction and backscatter, respectively, B is the background ~~noise~~signal, and C_L represents the lidar constant. This constant encapsulates the system-specific characteristics of the lidar, such as its receiver optics and laser properties. It is initially determined and provided by the manufacturer, but it may drift over time as the instrument
95 ages and its performance changes. Although the internal firmware attempts to monitor and compensate for these changes, additional calibration, such as absolute calibration using stratocumulus clouds (O'Connor et al., 2004; Hopkin et al., 2019), is still necessary.

The instrument provides two main output signals, $ppol$ and $xpol$ in arbitrary unit [a.u.], which represent the estimated normalized and background-, range- and overlap-corrected parallel- and cross-polarized components of the attenuated backscattered signal ($^{\parallel} \beta'$ and $^{\perp} \beta'$ respectively). They can be defined as:

$$ppol = ^{\parallel} \frac{(P(r) - B)r^2}{C_L O(r)} \frac{(P(r) - B_{estimated})r^2}{C_L O(r)} = ^{\parallel} \beta', \quad (2)$$

$$xpol = ^{\perp} \frac{(P(r) - B)r^2}{C_L O(r)} \frac{(P(r) - B_{estimated})r^2}{C_L O(r)} = ^{\perp} \beta'. \quad (3)$$

where $B_{estimated}$ is the internally estimated background signal by the instrument. The instrument also provides the total attenuated backscatter signal being the sum of the attenuated backscatter from all polarizations:

$$105 \quad \beta' = ^{\parallel} \beta' + ^{\perp} \beta', \quad (4)$$

and the volume linear depolarization ratio being:

$$\delta_v = \frac{^{\perp} \beta'}{^{\parallel} \beta'}. \quad (5)$$

4 Methods

3.1 ~~Background noise~~Residual background signal

110 The observed backscattered signal detected by a lidar consists of the true atmospheric signal and the background ~~noise~~signal (Cao et al., 2013). The true atmospheric signal consists of backscattered contributions from particles (β_p) and molecular scattering (β_{mol}), whilst the background ~~noise~~signal includes contributions from both ~~solar radiation P_{solar} and instrument-related~~

115 ~~$P_{instrument}$ noise~~ atmospheric background signal $P_{atmosphere}$ (such as solar radiation, moonlight, or artificial light) and instrumental background $P_{instrument}$ signal (dark signal). Although the instrument already determines and performs the background correction internally, residual background components may still remain in the measured signal, ~~as such as the dark signal~~ observed during termination hood measurements (see Sect 3.1.1). Therefore, we extend Eqs. 2 and 3 to account for ~~background noise~~, ~~B_{bk}~~ the residual background signal (hereafter referred to as the background signal), B_{res} , that is not removed by the internal correction:

$$ppol = \parallel \frac{(P(r) - B)r^2}{C_{LO}(r)} \frac{(P(r) - B_{estimated})r^2}{C_{LO}(r)} + \parallel \frac{B_{bk}(r)r^2}{C_{LO}(r)} \frac{B_{res}(r)r^2}{C_{LO}(r)} = \parallel \beta'_{corrected} + \parallel \frac{B_{bk}(r)r^2}{C_{LO}(r)} \frac{B_{res}(r)r^2}{C_{LO}(r)}, \quad (6)$$

$$120 \quad xpol = \perp \frac{(P(r) - B)r^2}{C_{LO}(r)} \frac{(P(r) - B_{estimated})r^2}{C_{LO}(r)} + \perp \frac{B_{bk}(r)r^2}{C_{LO}(r)} \frac{B_{res}(r)r^2}{C_{LO}(r)} = \perp \beta'_{corrected} + \perp \frac{B_{bk}(r)r^2}{C_{LO}(r)} \frac{B_{res}(r)r^2}{C_{LO}(r)}. \quad (7)$$

To eliminate the range dependence from the background terms, we divide each expression by r^2 , yielding:

$$\frac{ppol}{r^2} = \frac{\parallel \beta'}{r^2} \frac{\parallel \beta'_{corrected}}{r^2} + \parallel \frac{B_{bk}(r)}{C_{LO}(r)} \frac{B_{res}(r)}{C_{LO}(r)}, \quad (8)$$

$$\frac{xpol}{r^2} = \frac{\perp \beta'}{r^2} \frac{\perp \beta'_{corrected}}{r^2} + \perp \frac{B_{bk}(r)}{C_{LO}(r)} \frac{B_{res}(r)}{C_{LO}(r)}. \quad (9)$$

For simplicity, we define the background terms as:

$$125 \quad P_{bkres}(r) \equiv \frac{B_{bk}(r)}{C_{LO}(r)} \frac{B_{res}(r)}{C_{LO}(r)}, \quad (10)$$

where ~~$P_{bk}(r)$~~ ~~$P_{res}(r)$~~ = ~~$P_{solar}(r)$~~ ~~$P_{atmosphere}(r)$~~ + ~~$P_{instrument}(r)$~~ ~~$P_{instrument}(r)$~~ .

To derive the $\beta'_{corrected}$, the background signals need to be quantified. Since the measured $ppol$ and $xpol$ signals include contributions from background ~~noise signal~~ in their respective polarization channels, it is necessary to estimate the background ~~noise signal~~ separately for each polarization ($\parallel P_{res}$ and $\perp P_{res}$). To achieve this, a background identification methodology has
130 been developed. It identifies regions within the dataset that are free of aerosols and hydrometeors, where the ~~$ppol$ and $xpol$~~ ~~$\frac{ppol}{r^2}$ and $\frac{xpol}{r^2}$~~ values are assumed to predominantly represent background ~~noisesignal~~.

The methodology proceeds as follows. First, the data is averaged over 5-minute intervals. The $\frac{ppol}{r^2}$ and $\frac{xpol}{r^2}$ profiles are then decomposed using the stationary wavelet transform (SWT) with the bior.1 wavelet, implemented via PyWavelets (Nason and Silverman, 1995; Lee et al., 2019). Subsequently, ~~noise the background signal~~ variance is reduced by applying a hard-threshold shrinkage function to the approximation and detail coefficients from levels 1 through 7, using minimax thresholding (Nason and Silverman, 1995). The profile is reconstructed via the inverse stationary wavelet transform. Finally, the ~~noise background~~ range gates are identified as regions with values below half of the previously computed minimax threshold. The mean and variance of the background are computed from the original, non-averaged data with the identified background range gates using 5-minute time intervals and 2 km range-bin intervals.
135

140 An example of this methodology applied to data in Kenttäröva on 2024-03-28 is illustrated in Fig. 1. During daylight hours, solar radiation significantly increases the variance ($\sigma_{\parallel P_{\text{res}}}^2$ and $\sigma_{\perp P_{\text{res}}}^2$) of the background ~~noise in both $\frac{ppol}{r^2}$ and $\frac{xpol}{r^2}$ signal,~~ resulting in a daytime variance much higher than that observed at night, as shown in panels (g) and (h). Above the aerosol and cloud layers, both the mean ~~and $(\mu_{\parallel P_{\text{res}}}$ and $\mu_{\perp P_{\text{res}}})$ and~~ variance of the background ~~$\frac{ppol}{r^2}$ and $\frac{xpol}{r^2}$ signals~~ signals in both polarizations remain relatively stable with range, or at least exhibit considerably smaller variations compared to the diurnal

145 fluctuations.

By applying this methodology to the full dataset, we obtained the time series of $P_{bk}(r) - P_{\text{res}}$ for all instruments in both polarizations. Comparing these background ~~noise levels~~ signals with other housekeeping parameters, such as laser power, enables us to evaluate the operational performance of each instrument. Moreover, since each ~~noise background~~ component is quantified independently, we can correct the signal and estimate its uncertainty in both ~~polarization~~ polarizations $ppol$ and $xpol$

150 and, consequently, in the derived linear depolarization ratio.

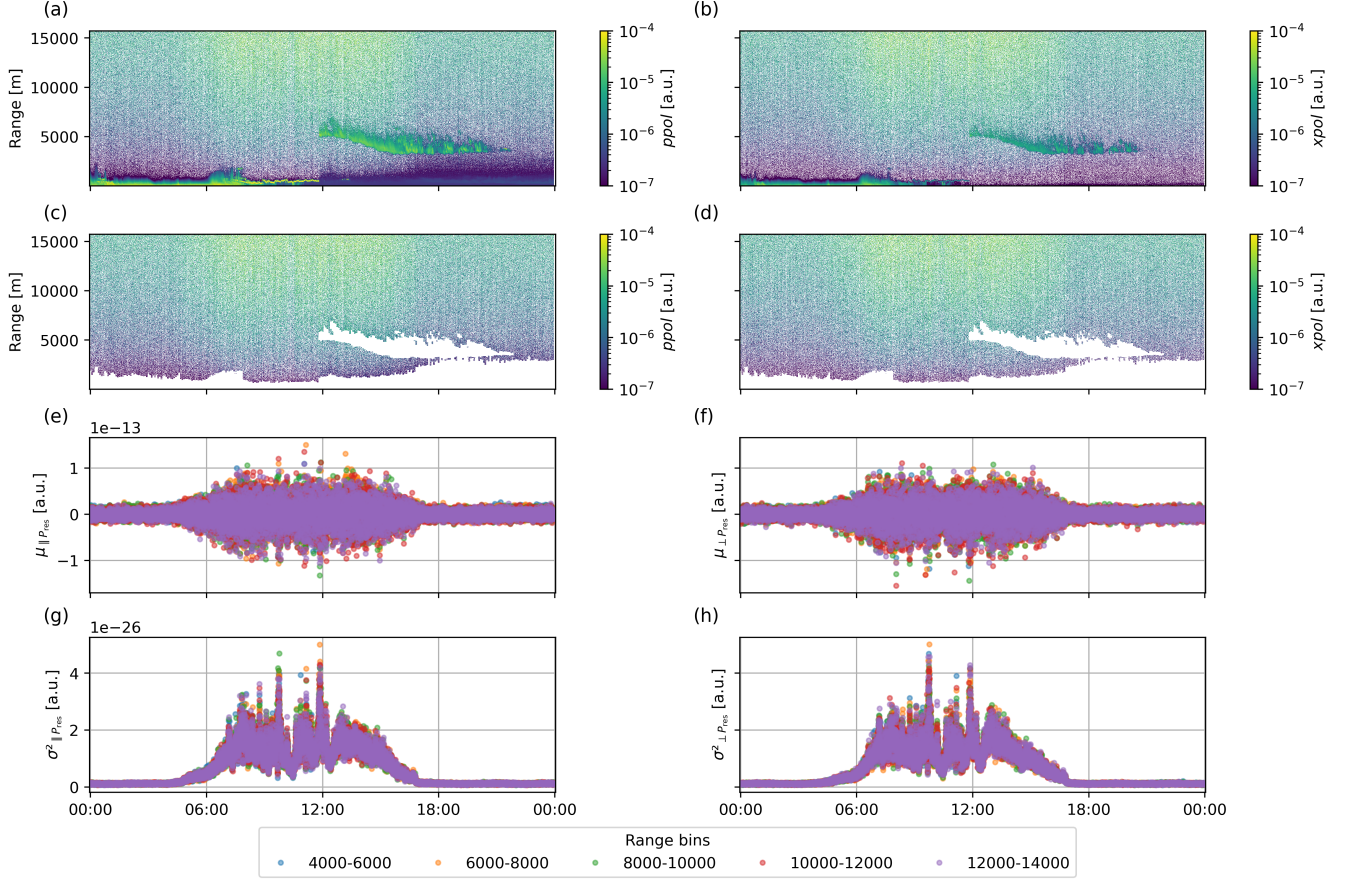


Figure 1. Time series from Kenttäröva on 2024-03-28 showing: a) $ppol$, b) $xpol$, c) background $ppol$, and d) background $xpol$. Subplots e–h display the background signals at different range bins from 4000 – 6000 m, 6000 – 8000 m, 8000 – 10000 m, 10000 – 12000 m, 12000 – 14000 m, with color indicating the range bin: e) $\#_{ppol} \mu_{\perp P_{res}}$, f) $\#_{xpol} \mu_{\perp P_{res}}$, g) $\sigma_{ppol}^2 \sigma_{\perp P_{res}}^2$, and h) $\sigma_{xpol}^2 \sigma_{\perp P_{res}}^2$. These parameters are computed at a 10-second temporal resolution using all data within each range bin.

3.1.1 Instrumental ~~noise~~background signal



Figure 2. A termination hood (Vaisala CL61TERMHOOD) place on top of the CL61 in ~~Hyytiälä~~Hyytiälä.

To obtain the ~~instrument's noise level~~instrumental background signal, a termination hood (Vaisala CL61TERMHOOD) was placed over the window of each ceilometer located in Finland. The hood was applied without ~~notifying the instrument, so that it operated as it would under normal~~modifying the instrument's internal operating parameters, ensuring that all measurements reflected normal operational conditions. The hood's material and design totally attenuate the outgoing laser beam, preventing any backscatter signal from reaching the detector. As a result, the measured signal can be attributed entirely to the instrumental noise term, i.e. $\frac{ppol}{r^2} = \frac{P_{instrument}(r)}{r^2}$, $\frac{xpol}{r^2} = \frac{P_{instrument}(r)}{r^2}$ during the termination hood measurementbackground signal adjusted by the overlap correction. Although the overlap correction remains constant for each instrument, it was reverted to accurately interpret the instrumental background signal in the near range $P_{instrument}O(r)$.

Figure 3 presents example profiles of $ppol$ and $xpol$ both before and during the termination hood measurements. Before the termination hood was applied, the μ_{ppol} and μ_{xpol} profiles in the aerosol and hydrometeor-free region above 5 km closely follow the theoretical molecular ~~backscatter~~ β_{mol} attenuated backscatter coefficient β'_{mol} (Fig. 3b and c), indicating that the CL61 ceilometer is sensitive to molecular scattering. The ~~method for calculating~~ β_{mol} is described in the following section β'_{mol} profile was calculated following the method described by Bucholtz (1995) using meteorological input data from a numerical weather prediction model available from the ACTRIS Cloudnet data portal (O'Connor, 2025). At ranges above 10 km, however, the molecular signal becomes indistinguishable from noise. The ~~standard deviation profiles~~, σ_{ppol}/r^2 and σ_{xpol}/r^2 variance profiles, σ^2_{ppol}/r^2 and σ^2_{xpol}/r^2 , also remain relatively constant in this region (Fig. 3f and g).

During the termination hood measurement, ~~the instrumental noise profiles~~ $P_{instrument}(r)$ remain $\mu_{P_{instrument}O(r)}$ from both polarizations remains relatively stable above 1.2 km, but ~~increase~~increases significantly below this range (Figs. 3d, e, h, and

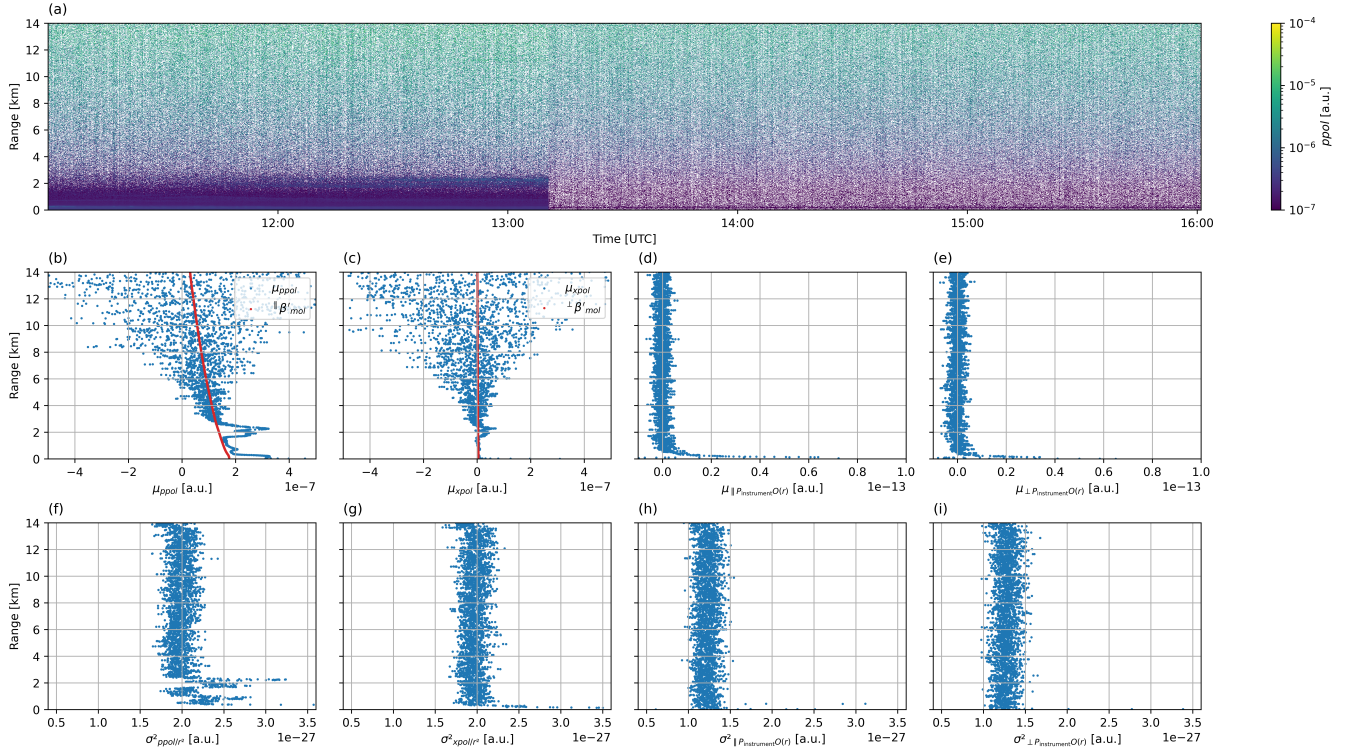


Figure 3. Measurements at Kenttäröva on 5 March 2024. a) the time series of $ppol$. Panels b, c, f, g, display the averaged profiles in time at each range gate before the termination hood measurement (from 11 to 13 UTC): b) μ_{ppol} and $\pm \beta_{mot} \parallel \beta'_{mol}$, c) μ_{xpol} and $\pm \beta_{mot} \perp \beta'_{mol}$, f) σ_{ppol/r^2}^2 , g) σ_{xpol/r^2}^2 . Panels d, e, h, i, display the averaged profiles in time at each range gate during the termination hood measurement at 19 °C (from 14 to 15 UTC): d) $\mu_{ppol/r^2} \parallel P_{instrument} O(r)$, e) $\mu_{xpol/r^2} \perp P_{instrument} O(r)$, h) $\sigma_{ppol/r^2}^2 \parallel P_{instrument} O(r)$, i) $\sigma_{xpol/r^2}^2 \perp P_{instrument} O(r)$.

170 i). This increase ~~indicates~~ suggests the presence of a signal bias at lower ranges that has not been corrected by the firmware and will be investigated in this study. Additionally, a reduction in the ~~standard-deviation-signal variance~~ of both polarization channels is observed during the termination hood measurement (Figs. 3h, i) compared to the ~~period-before~~ previous period above the complete overlap range. This reduction is attributed to the absence of solar influence during the termination hood measurement.

175 In principle, the nighttime measurements could be used to estimate $P_{instrument}$. However, only the portion of the $P_{instrument}$ profile at higher ranges, where clouds and aerosols are absent, can be reliably estimated. An example is shown in Fig. S2 in the Supplement, where σ_{ppol/r^2}^2 agrees well between the hood termination and nighttime measurements only at ranges above approximately 2 km. This agreement is observed only under clear-sky conditions, as cloud layers at lower ranges can increase the measured background values.

180 Since the CL61 ~~cei~~lometer is a coaxial lidar, it is prone to the afterpulsing effect, such as those caused by internal reflections of the outgoing laser beam that reach the detector (Campbell et al., 2002; Welton and Campbell, 2002). ~~Additionally,~~ Hervo et al. (2016) demonstrated that the overlap function for a ceilometer made by another manufacturer (Lufft CHM15k) was sensitive to the instrument internal temperature, T , mainly due to temperature-induced changes in its optical components. ~~Although Vaisala does apply a correction for the overlap function, it~~ It is likely that this is a time-invariant correction and
 185 ~~that the bias observed is due to the combined effects of changes in afterpulsing and the possible temperature dependence of the overlap correction~~ the observed bias is temperature-dependent and is caused by variations in instrumental background associated with afterpulsing, dark signal, and optical components under different temperature conditions. To quantify ~~this effect~~ the effect of temperature, the termination hood measurement was repeated ~~for over~~ for over a range of ~~internal temperatures~~ internal temperatures T ~~over,~~ reported as internal temperature in the instrument housekeeping data, across a two-year period. ~~This approach enabled~~
 190 ~~the derivation of $\parallel P_{instrument}(r, T)$ and $\perp P_{instrument}(r, T)$, i.e. w.r.t. to T~~ Hence, the instrumental background signal mean (bias) and its variance (noise) from both polarizations with respect to internal temperature can be determined.

3.1.2 ~~Solar noise~~ Atmospheric background signal

For an accurate estimation of ~~background noise~~ the background signal, the contribution from ~~solar radiation~~ the atmospheric background signal, $P_{atmosphere}$, must be taken into account. As noted by Kotthaus et al. (2016), earlier instruments such as the
 195 CL31 incorporate a zero-bias level that compensates for temporal fluctuations in solar radiation. This is also evident in CL61 as shown in Fig. 3b and 3c, where the μ_{ppol} and μ_{xpol} values above 5 km closely follow β_{mol} , confirming the zero-mean solar radiation noise. Therefore, the firmware must have corrected the atmospheric background signal to a zero mean, leaving only its variance (noise) contributing to the background signal, which will be addressed in this study.

The solar noise variance can be seen from the diurnal pattern in Fig. ~~3 and 1g and 1h; and~~ the difference between the σ^2
 200 profiles before ~~and during the termination hood measurement in~~ (Fig. 3f, ~~g, h and i and 3g~~) and during (Fig. 3h and 3i) the termination hood measurement. Since this difference remains approximately constant at all ranges above the aerosol layer near the ground, we assume that the ~~solar noise~~ atmospheric background variance from both polarizations, $\sigma^2_{P_{solar}} - \sigma^2_{P_{atmosphere}}$, is also uniform down to the near range. ~~$\sigma^2_{P_{solar}}$ is then~~ Then, $\sigma^2_{P_{atmosphere}}$ is calculated by computing the difference between the ~~total background noise variance $\sigma^2_{P_{bk}}$~~ variance of the background signal $\sigma^2_{P_{res}}$ (obtained between 10 to 12 km using
 205 the background identification methodology) and the ~~instrumental noise variance $\sigma^2_{P_{instrument}}$~~ variance of the instrumental background signal $\sigma^2_{P_{instrument}}$ (obtained at the same range and temperature from the termination hood measurement):

$$\sigma^2_{P_{solar} P_{atmosphere}} = \sigma^2_{P_{bk}(r=10-12km)} P_{res}(r=10-12km) - \sigma^2_{P_{instrument}(r=10-12km, T)} P_{instrument}(r=10-12km, T). \quad (11)$$

Here, $\sigma^2_{P_{solar}} - \sigma^2_{P_{atmosphere}}$ is independent of the range and is obtained separately for each polarization ~~in each individual profile.~~

210 ~~As noted by Kotthaus et al. (2016), earlier instruments such as the CL31 incorporate a zero-bias level that compensates for temporal fluctuations in solar radiation. This is also evident in CL61 as shown in Fig. 2b and 2c, where the μ_{ppol} and μ_{xpol} values above 5 km closely follow β_{mol} , confirming the zero-mean solar radiation noise.~~

3.1.3 Correction for systematic bias

After measuring $P_{instrument}(r, T)$ across a range of T during the termination hood measurements, the results
 215 are stored as a lookup table containing $P_{instrument}(r, T)$ profiles at each T . The attenuated backscatter
 coefficient for each polarization can be corrected by applying the $P_{instrument}(r, T)$ value corresponding to
 the instrument's current internal temperature as follows:

$$\parallel \beta'_{corrected} = ppol - \mu \parallel P_{instrument}(r, T) \parallel P_{instrument}(r, T) r^2, \quad (12)$$

$$\perp \beta'_{corrected} = xpol - \mu \perp P_{instrument}(r, T) \perp P_{instrument}(r, T) r^2, \quad (13)$$

220 and their corresponding uncertainties given by:

$$\sigma^2 \parallel \beta'_{corrected} \parallel \beta'_{corrected} = (\sigma^2 \parallel P_{solar} \parallel P_{atmosphere} + \sigma^2 \parallel P_{instrument}(r, T) \parallel P_{instrument}(r, T)) r^2, \quad (14)$$

$$\sigma^2 \perp \beta'_{corrected} \perp \beta'_{corrected} = (\sigma^2 \perp P_{solar} \perp P_{atmosphere} + \sigma^2 \perp P_{instrument}(r, T) \perp P_{instrument}(r, T)) r^2. \quad (15)$$

The bias-corrected attenuated backscatter and-coefficient and volume linear depolarization ratio are then calculated as:

$$\beta'_{correctedcorrected} = \parallel \beta'_{corrected} + \perp \beta'_{corrected}, \quad (16)$$

$$\delta_{correctedcorrected} = \frac{\perp \beta'_{corrected} \perp \beta'_{corrected}}{\parallel \beta'_{corrected} \parallel \beta'_{corrected}}, \quad (17)$$

and their associated uncertainty, given by

$$\sigma^2 \beta'_{corrected} \beta'_{corrected} = \sigma^2 \parallel \beta'_{corrected} \parallel \beta'_{corrected} + \sigma^2 \perp \beta'_{corrected} \perp \beta'_{corrected}, \quad (18)$$

$$\sigma^2 \delta_{corrected} \delta_{corrected} = \delta^2 \left(\frac{\sigma^2 \perp \beta'_{corrected} \perp \beta'_{corrected}}{\perp \beta'^2_{corrected}} + \frac{\sigma^2 \parallel \beta'_{corrected} \parallel \beta'_{corrected}}{\parallel \beta'^2_{corrected}} \right). \quad (19)$$

3.2 Calibration

230 To ensure the CL61 produces a consistent and accurate backscatter signal, the ceilometer signal must be manually calibrated
 in addition to its internal calibration. This involves calibrating the backscatter signal from the CL61 using a reference target
 with known backscatter characteristics. Two commonly used calibration methods for deriving C_L are based on different types
 of reference targets: atmospheric molecules (Rayleigh calibration) and liquid clouds (liquid cloud calibration).

The Rayleigh calibration (Fernald et al., 1972; Klett, 1985; Biniotoglou et al., 2011; Wiegner and Geiß, 2012; Baars et al.,
 235 2016), often referred to as the backward inversion approach, is the standard method to derive the aerosol-particle backscatter
 coefficient (β_p) for most research aerosol lidars due to their sensitivity to molecular signal (Wiegner et al., 2014). As illustrated
 in Fig. 3b, the attenuated backscatter coefficient profile from CL61 closely follows the attenuated molecular backscatter coeffi-
 cient above the aerosol layer at 4 km. This indicates a significant contribution of molecular scattering to the total CL61 signal,

especially in aerosol- and hydrometeor-free regions. Therefore, the Rayleigh calibration can be applied to the CL61, provided
240 a sufficiently long averaging time (more than 2 hours) is used.

The Rayleigh calibration method requires an assumed lidar ratio for aerosol particles (S_p). At sites equipped with a sun photometer, S_p can be constrained (Wiegner and Geiß, 2012); otherwise, a value of 50 sr was used. ~~Additionally, the β_m profile is needed for the inversion and was calculated following the method described by Bucholtz (1995) using meteorological input data from a numerical weather prediction model available from the ACTRIS Cloudnet data portal (O'Connor, 2025).~~ The first
245 ~~50 μm range has been discarded due to unreliable data (see Sect. 4.5), and it has been demonstrated that the resulting loss in optical depth for ignoring near range gates is negligible (Wiegner and Geiß, 2012).~~ After the β_p profile is derived, the lidar constant C_L can be determined from the lidar equation (Wiegner and Geiß, 2012).

The liquid cloud calibration (O'Connor et al., 2004; Hopkin et al., 2019) relies on the fact that the lidar ratio for liquid water clouds at the ceilometer wavelength is known. This method involves calculating the integrated attenuated backscatter coefficient
250 for fully attenuated liquid water clouds, including the contribution from multiple scattering. The theoretical contribution from multiple scattering is computed for droplet diameters ranging from 8 to 20 μm and with the CL61 beam divergence and receiver field of view. The integrated backscatter coefficient is then scaled to fit within the expected theoretical values and this scaling factor is the calibration factor C , which is the reciprocal of the lidar constant C_L . The primary advantage of this approach over Rayleigh calibration is the substantially higher signal-to-noise ratio of the backscatter from water clouds compared to
255 the molecular backscatter. As a result, it eliminates the need for long nighttime averaging periods required to obtain a reliable molecular signal.

A methodology was developed to identify suitable liquid cloud profiles. First, ~~an example a representative~~ liquid cloud profile ~~is chosen as a reference. Then, each profile is containing a single liquid cloud layer and exhibiting complete signal attenuation approximately 200 m above the cloud base was selected as the reference profile.~~ Each *ppol* profile in the dataset
260 ~~was then~~ cross-correlated with this reference to quantify their similarity. For each time step, the ~~profile with the highest height corresponding to the maximum~~ cross-correlation value ~~is considered was identified as~~ the most similar. ~~Additionally, a liquid cloud profile is then selected if the proportion of location and treated as a pseudo in-cloud β' to height.~~ Next, the ~~sum of the profile ratio of total in-cloud β' exceeds 90% as this ensures,~~ calculated over a 150 m layer centered at the pseudo in-cloud height, to the integrated β' of the entire profile was computed. A profile was classified as containing a liquid cloud if this ratio
265 ~~exceeded 90%, ensuring~~ that the integrated β' ~~is not impacted was not significantly influenced~~ by strong aerosol loading or precipitation. ~~Additionally, the cross-correlation value at the identified height was required to exceed 5×10^{-7} . This threshold was selected to ensure that at least 1000 valid data points were available for each month.~~

To ensure robust data fitting, the cloud calibration is performed monthly using all suitable liquid cloud observations detected from the methodology. To validate the cloud calibration results, Rayleigh calibration was also computed occasionally when
270 possible. Data from a co-located sun photometer was used to constrain the lidar ratio for Rayleigh calibration. If no sun photometer data is available, a lidar ratio of 50 sr is used.

The calibrated volume attenuated backscatter coefficient and its uncertainty can then be determined as ÷follows, assuming the cloud calibration factor has an uncertainty of approximately 10% (Hopkin et al., 2019):

$$\beta'_v = \beta'_{\text{correctedcorrected}} \cdot C, \quad (20)$$

$$275 \quad \sigma^2_{\beta'_v} = (\sigma^2_{\beta'_{\text{corrected}}\beta'_{\text{corrected}}} + 0.01 \cdot \beta'^2_{\text{corrected}}) \cdot C^2. \quad (21)$$

For those instruments where ~~terminal~~termination hood measurements are not available:

$$\beta'_v = \beta' \cdot C, \quad (22)$$

$$\sigma_{\beta'_v} = (\sigma^2_{P_{\text{solar}}P_{\text{atmosphere}}} + 0.01 \cdot \beta'^2) \cdot C^2 = (\sigma^2_{\parallel P_{\text{solar}}\parallel P_{\text{atmosphere}}} + \sigma^2_{\perp P_{\text{solar}}\perp P_{\text{atmosphere}}} + 0.01 \cdot \beta'^2) \cdot C^2. \quad (23)$$

The calibration is assumed to affect both polarization channels equally. Hence, ~~δ~~δ_{corrected} remains unchanged.

280 3.3 Aerosol particle inversion

The ~~aerosol~~ particle backscatter coefficient profile (β_p) is retrieved using the forward Klett solution (Klett, 1985) after applying the previously derived cloud calibration factor and assuming that the instrument does not undergo significant degradation within a one-month period. Similar to the previous section, the first 50 m range has been discarded. The cloud calibration factor is estimated to have an uncertainty of approximately 10% (Hopkin et al., 2019). The forward inversion does not require extensive
285 temporal averaging. When available, sun photometer observations are used to constrain the lidar ratio S_p ; otherwise, a constant value of 50 sr is applied to all aerosol layers in the retrieval.

Let $\beta_p = f(\beta'_v, C, S_p)$ represent the inversion function; then the uncertainty of β_p is calculated as

$$\sigma^2_{\beta_p} = \left(\frac{\partial f}{\partial \beta'_v} \sigma_{\beta'_v} \right)^2 + \left(\frac{\partial f}{\partial C} \sigma_C \right)^2 + \left(\frac{\partial f}{\partial S} \sigma_{\underline{S}S_p} \right)^2. \quad (24)$$

The partial derivatives can be approximated using central differences:

$$290 \quad \frac{\partial f}{\partial \beta'_v} \sigma_{\beta'_v} \approx \frac{f(\beta'_v + \sigma_{\beta'_v}, C, S_p) - f(\beta'_v - \sigma_{\beta'_v}, C, S_p)}{2}, \quad (25)$$

$$\frac{\partial f}{\partial C} \sigma_C \approx \frac{f(\beta'_v, C_{\max}, S_p) - f(\beta'_v, C_{\min}, S_p)}{2}, \quad (26)$$

$$\frac{\partial f}{\partial S} \sigma_{S_p} \approx \frac{f(\beta'_v, C, S_{p,\max}) - f(\beta'_v, C, S_{p,\min})}{2}. \quad (27)$$

with $C_{\min} = 0.9 \cdot C$, $C_{\max} = 1.1 \cdot C$, $S_{p,\min} = S_p - 10$ and $S_{p,\max} = S_p + 10$

Following (Biele et al., 2000; Freudenthaler et al., 2009), the particle linear depolarization ratio (δ_p) is then obtained as

$$295 \quad \delta_p = \frac{(1 + \delta_m)\delta_v R - (1 + \delta_v)\delta_m}{(1 + \delta_m)R - (1 + \delta_v)}, \quad (28)$$

where the backscatter ratio R is defined as

$$R = \frac{\beta_p + \beta_m}{\beta_m}, \quad (29)$$

and δ_v is the volume linear depolarization ratio, which is ~~$\delta_{corrected}$~~ $\delta_{corrected}$ in Eq. 17, or $\frac{x_{pol}}{p_{pol}}$ for instruments lacking ~~terminal~~ termination hood measurements.

300 The molecular depolarization ratio (δ_m) is estimated following Tomasi et al. (2005), accounting for major atmospheric gases and the influence of water vapor. The input data for these calculations are taken from a numerical weather prediction model (ECMWF IFS forecast) provided via the ACTRIS Cloudnet data portal (O'Connor, 2024).

The uncertainty of δ_p can be determined using partial derivatives

$$\sigma_{\delta_p}^2 = \left(\frac{\partial \delta_p}{\partial \delta_m} \sigma_{\delta_m} \right)^2 + \left(\frac{\partial \delta_p}{\partial \delta_v} \sigma_{\delta_v} \right)^2 + \left(\frac{\partial \delta_p}{\partial R} \sigma_R \right)^2. \quad (30)$$

305 Assuming σ_{β_m} and σ_{δ_m} are negligible and approximating ~~$\sigma_R \approx \sigma_{\beta_p} \sigma_R \approx \frac{\sigma_{\beta_p}}{\beta_m}$~~ , this reduces to

$$\sigma_{\delta_p}^2 \approx \left(\frac{\partial \delta_p}{\partial \delta_v} \sigma_{\delta_v} \right)^2 + \left(\frac{\partial \delta_p}{\partial R} \frac{\sigma_{\beta_p}}{\beta_m} \right)^2. \quad (31)$$

The partial derivatives are calculated as:

$$\frac{\partial \delta_p}{\partial \delta_v} = \frac{(1 + \delta_m)^2 R (R - 1)}{((1 + \delta_m)R - (1 + \delta_v))^2}, \quad (32)$$

$$\frac{\partial \delta_p}{\partial R} = \frac{(1 + \delta_m)(1 + \delta_v)(\delta_m - \delta_v)}{((1 + \delta_m)R - (1 + \delta_v))^2}. \quad (33)$$

4.1 Background noise

Figure 4 shows the time series of background noise (variance of the background signal), normalized by integration time assuming Poisson statistics ($\sigma_{\text{ppt}/r^2}^2 \times t_{\text{integration}}$), alongside the laser power. Most instruments (except for Vehmasmäki) exhibit a gradual decline in laser power, accompanied by corresponding increases in background noise, likely due to weaker
 315 return signal. These changes often occur in discrete steps rather than as a continuous trend. Notably, fluctuations in background noise are consistently related to changes in laser power. Periods of restored laser power and decreased background noise align with documented hardware interventions, such as transmitter replacements at Vehmasmäki (Dec 2022; Fig. 4a) and Hyytiälä (Feb 2024; Fig. 4b).

At Hyytiälä and Kenttäröva, laser power gradually decreases from 100% to around 40% over two years. In contrast, the
 320 CL61 at Vehmasmäki maintains a consistently high laser power, ranging between 90% and 100% throughout the same period, with only a slight decrease during the summer, likely to regulate the internal temperature to prevent overheating. Meanwhile, the CL61 at Lindenberg experienced a sharp decline in laser power, from 80% to below 10% within just one year of operation. We also found that changes in the firmware version do not appear to have any noticeable effect on background noise levels.

The relationship between background noise, normalized by integration time, and laser power across several instruments is
 325 illustrated in Fig. 5. Nighttime measurements (23:00 to 01:00 local time), shown in blue, are unaffected by solar radiation, while all-day measurements are displayed in grey. It is important to note that the selected nighttime window is arbitrary and used solely for this analysis; for instance, locations such as Kenttäröva experience no true nighttime during summer. The nighttime data clearly indicate that a decrease in laser power leads to an increase in background noise across all instruments. Daytime background noise is generally higher due to solar radiation, which varies with factors such as solar angle, cloud height,
 330 and surface albedo, making direct comparisons more complex. Nevertheless, the figure suggests that lower laser power also contributes to increased noise levels during daytime conditions.

An increase in background noise can significantly reduce an instrument's ability to detect weak aerosol signals. This effect is clearly illustrated in Fig. S1-S3 in the supplement. On 7 March 2024, an elevated aerosol layer was observed above 3 km in Lindenberg, indicated by enhanced attenuated backscatter coefficient values compared to those at lower altitudes between
 335 1 – 3 km (Fig. S1aS3a, c). However, by 2 December 2024, a reduction in laser power led to a higher noise floor, which meant that if a similar aerosol layer were present, it would no longer be distinguishable from the background noise (Fig. S1bS3b, c).

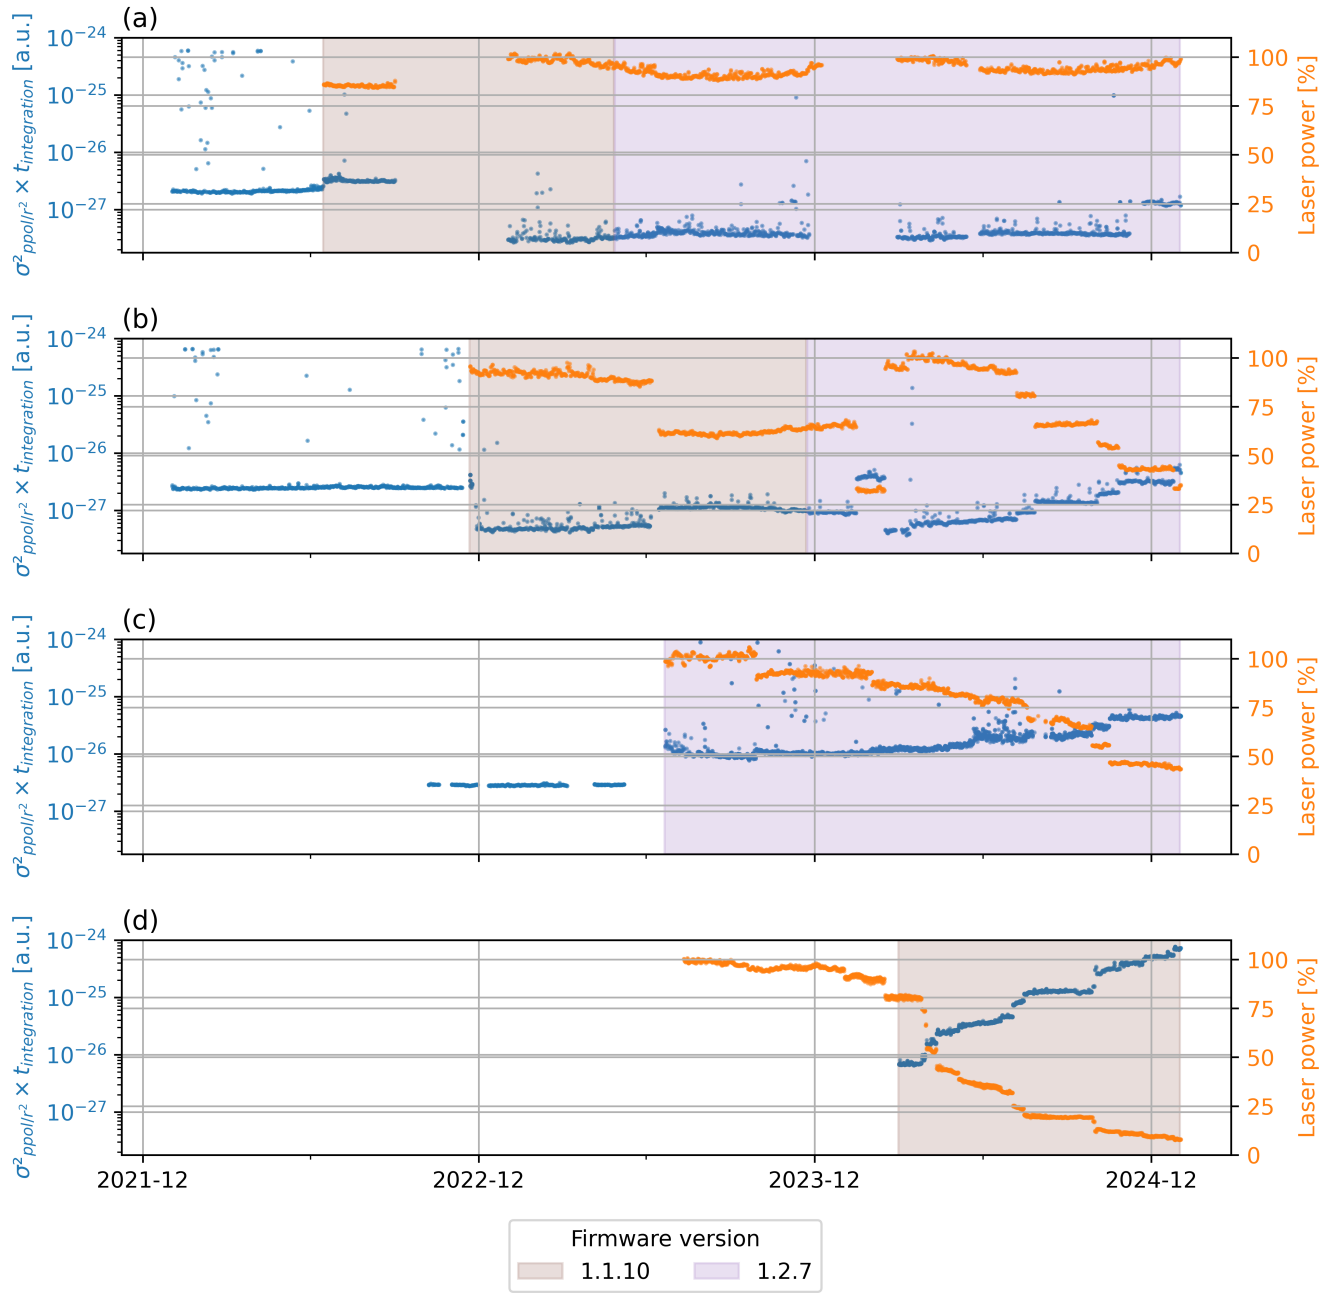


Figure 4. Time series of nighttime background ~~noise~~-signal variance normalized by the integration time ($\sigma^2_{ppol/r^2} \times t_{integration}$), and the laser power are shown for (a) Vehmasmäki, (b) Hyytiälä, (c) Kenttäröva, and (d) Lindenberg. Shaded regions denote different firmware versions; unshaded areas represent periods with no recorded firmware version and laser power.

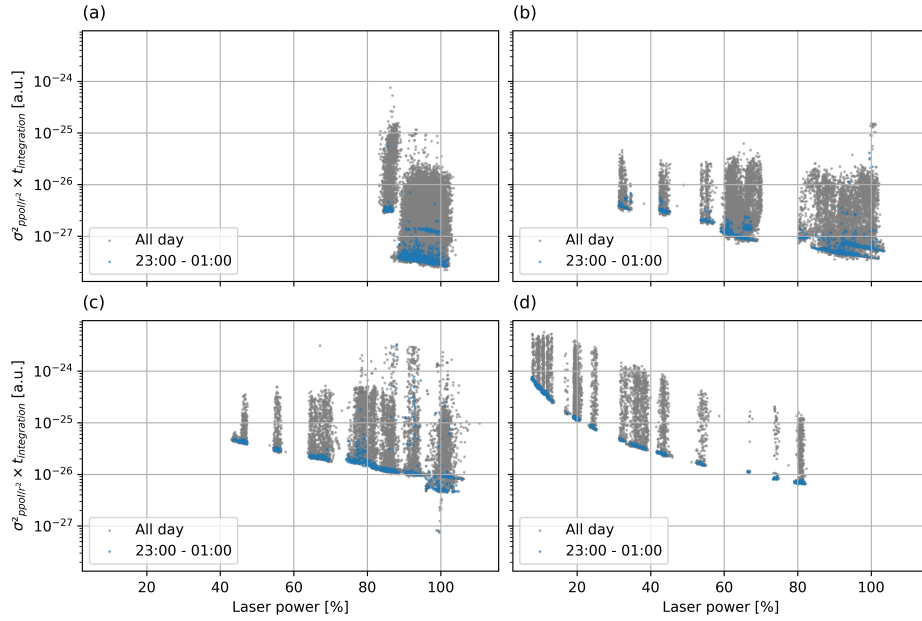


Figure 5. Variance of background noise as a function of laser power percentage, normalized by integration time, at the following locations: a) Vehmasmäki, b) Hyytiälä, c) Kenttäröva, and d) Lindenberg. Blue points represent data collected during nighttime hours (23:00–01:00 local time), while grey points include all available data.

4.2 Instrumental ~~noise~~background

In this section, we examine how the instrumental ~~bias~~ ($\mu_{ppol/r^2}, \mu_{xpol/r^2}$) ~~background bias~~ ($\mu_{P_{instrument}Q(r)}$) and noise ($\sigma_{ppol/r^2}^2, \sigma_{xpol/r^2}^2$) ~~with the overlap correction reverted, obtained during the termination hood measurement,~~ vary with temperature and
340 over time. The termination hood measurement was deployed multiple times at Vehmasmäki, Hyytiälä, and Kenttäröva. Figure 6 presents the instrumental ~~noise-background~~ profiles recorded during these termination hood measurement periods, which have been averaged and grouped according to the instruments' internal temperatures.

For the instruments located in Hyytiälä and Kenttäröva, the ~~μ_{ppol/r^2} values~~ $\mu_{P_{instrument}Q(r)}$ profiles remain relatively stable around zero from the far range down to about 2 km, then increase sharply as the range decreases. On the other hand, ~~the~~
345 ~~instrument~~ in Vehmasmäki, ~~it~~ also remains near zero at far range, but ~~its~~ μ_{ppol/r^2} $\mu_{P_{instrument}Q(r)}$ begins to increase ~~already~~ ~~at~~ around 5 km and continues to rise toward shorter ranges. Meanwhile, the μ_{xpol/r^2} $\mu_{P_{instrument}Q(r)}$ profiles for all three instruments remain near zero from the far range to about 2 km, after which they increase rapidly with decreasing range.

Overall, the internal temperature T has a more pronounced effect on the ~~mean-instrumental-noise~~ $\mu_{P_{instrument}Q(r)}$ pro-
files below 1 km than at higher ranges. In particular, ~~both~~ μ_{ppol/r^2} ~~and~~ μ_{xpol/r^2} ~~profiles~~ ~~the~~ $\mu_{P_{instrument}Q(r)}$ ~~profiles in both~~
350 ~~polarizations~~ deviate substantially from zero ~~at~~ below 200 m (see Fig. 7) across all instruments. Notably, each instrument shows the same small peak in ~~both~~ μ_{ppol/r^2} ~~and~~ μ_{xpol/r^2} ~~profiles~~ ~~the instrumental background bias in both polarizations~~ at approximately 150 m.

All instruments exhibit profiles of σ_{ppol/r^2}^2 ~~and~~ σ_{xpol/r^2}^2 ~~which are~~ $\sigma_{P_{instrument}Q(r)}^2$ ~~in both polarizations that remain~~ constant above 500 m, followed by a sharp increase below this range. These ~~variance~~ ~~instrumental background noise~~ profiles show
355 a pronounced sensitivity to internal temperature ~~, with lower temperatures producing higher~~ σ_{ppol/r^2} ~~(from 4°C to 38°C).~~ ~~Notably, very low temperatures are associated with elevated instrumental background noise across the entire measurement range.~~ This can be explained by the effect of the internal heater. As the internal temperature falls below an instrument-specific threshold (15 °C for Hyytiälä and σ_{xpol/r^2} ~~throughout the entire range~~ Kenttäröva), the internal heater is turned on. This leads to an increase in $\sigma_{P_{instrument}Q(r)}^2$, with the effect becoming more pronounced as the temperature decreases. When the internal
360 temperature is high and the internal heater is off, internal temperature positively correlates with $\sigma_{P_{instrument}Q(r)}^2$.

~~For all~~ Similar to Figs. 6 and 7, Figs. S4 and S5 show the same profiles obtained during the termination hood measurements, but include range correction and the instrument-provided overlap correction. These profiles of $ppol$ and $xpol$ provide a direct quantification of the impact of instrumental background bias and noise on the measurements and their dependence on temperature. For all CL61 instruments, the ~~signal~~ ~~instrumental~~ biases, μ_{ppol} and μ_{xpol} , remain below the order of 10^{-7} ,
365 while the noise terms, σ_{ppol}^2 and σ_{xpol}^2 , remain below the order of 10^{-11} . These biases are even smaller below 5 km. Below a range of 1 km, μ_{ppol} remains below 5×10^{-9} and μ_{xpol} below 3×10^{-9} . These small biases are usually negligible comparing to the typical atmospheric signal. However, at very clean sites such as Kenttäröva, the instrumental bias in $xpol$ can still affect the retrieved aerosol depolarization ratio, particularly under conditions of low depolarization. An example is shown in Fig. S6, which presents measurements from Kenttäröva on 2023-10-03 under weakly depolarizing aerosol conditions. During
370 this period, the $xpol$ profile below 400 m is on the order of 10^{-9} , while $ppol$ remains on the order of 10^{-6} . As a result, the

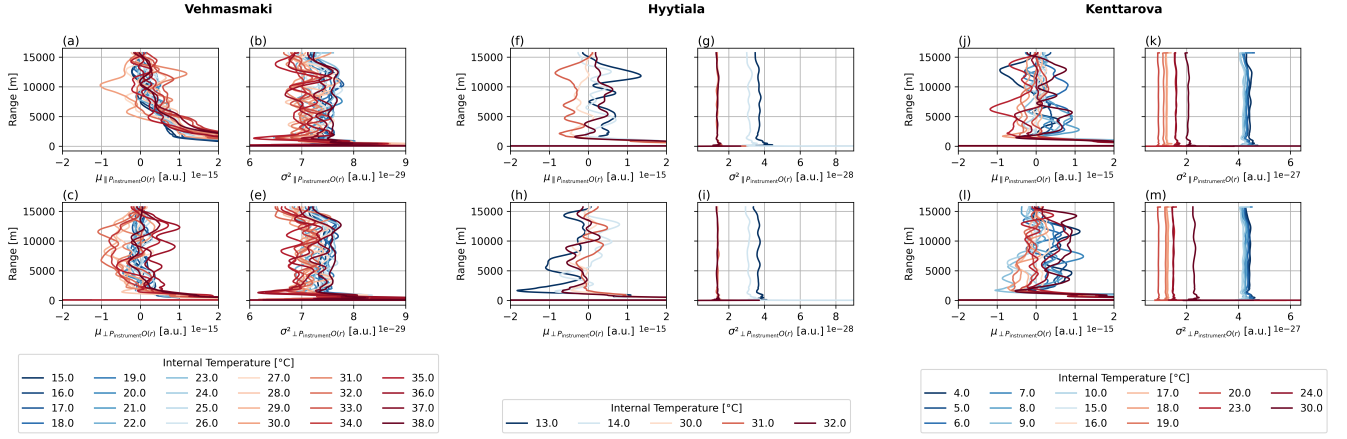


Figure 6. Termination hood profiles at various internal temperatures (color-coded) across different sites. In Vehmasmaki: a) $\mu_{\perp} P_{\text{instrument}} Q(r)$, b) $\sigma_{\perp} P_{\text{instrument}} Q(r)$, c) $\mu_{\parallel} P_{\text{instrument}} Q(r)$, and d) $\sigma_{\parallel} P_{\text{instrument}} Q(r)$. In Hyyttiala: f) $\mu_{\perp} P_{\text{instrument}} Q(r)$, g) $\sigma_{\perp} P_{\text{instrument}} Q(r)$, h) $\mu_{\parallel} P_{\text{instrument}} Q(r)$, and i) $\sigma_{\parallel} P_{\text{instrument}} Q(r)$. In Kenttaroava: j) $\mu_{\perp} P_{\text{instrument}} Q(r)$, k) $\sigma_{\perp} P_{\text{instrument}} Q(r)$, l) $\mu_{\parallel} P_{\text{instrument}} Q(r)$, and m) $\sigma_{\parallel} P_{\text{instrument}} Q(r)$.

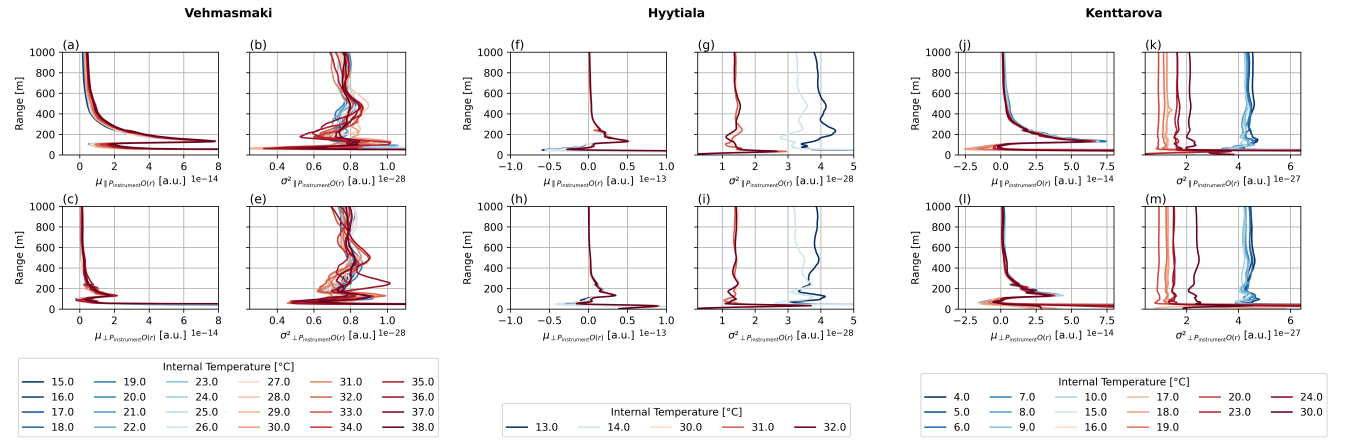


Figure 7. Termination hood profiles at various internal temperatures (color-coded) across different sites only up to 1000 m range. In Vehmasmaki: a) $\mu_{\perp} P_{\text{instrument}} Q(r)$, b) $\sigma_{\perp} P_{\text{instrument}} Q(r)$, c) $\mu_{\parallel} P_{\text{instrument}} Q(r)$, and d) $\sigma_{\parallel} P_{\text{instrument}} Q(r)$. In Hyyttiala: f) $\mu_{\perp} P_{\text{instrument}} Q(r)$, g) $\sigma_{\perp} P_{\text{instrument}} Q(r)$, h) $\mu_{\parallel} P_{\text{instrument}} Q(r)$, and i) $\sigma_{\parallel} P_{\text{instrument}} Q(r)$. In Kenttaroava: j) $\mu_{\perp} P_{\text{instrument}} Q(r)$, k) $\sigma_{\perp} P_{\text{instrument}} Q(r)$, l) $\mu_{\parallel} P_{\text{instrument}} Q(r)$, and m) $\sigma_{\parallel} P_{\text{instrument}} Q(r)$.

instrumental bias becomes relatively significant for $xpol$, leading to a noticeable, although quantitatively small, reduction in δ (from 0.002 to 0.001 at 200 m) after the bias correction is applied. Furthermore, the previously mentioned peak at 150 m is clearly visible in this case and is effectively mitigated after the removal of the instrumental bias.

For all instruments, the signal near the surface exhibits much more rapid fluctuations than at higher range gates. Figure S2 S7 displays example profiles of $ppol$, $xpol$, and the instrument's internal temperature during a termination hood measurement at Kenttäröva, revealing periodic variations in the signal below 50 m. To investigate this, the Fourier transforms of these signals were computed at each range gate over time and compared to that of the laser temperature recorded simultaneously. The results show that both the signals and the laser temperature exhibit a coincident spectral peak at approximately 0.0079 Hz (about 120 s), indicating a strong influence of laser temperature on the signals. Furthermore, additional distinct peaks in the signal spectra imply the presence of other instrument-related effects. Overall, these periodic variations appear sporadically across all instruments, with no consistent pattern indicating when they appear or disappear. Given the difficulty in developing a reliable correction method, we recommend excluding measurements below 50 m.

Figure S3 in the supplement

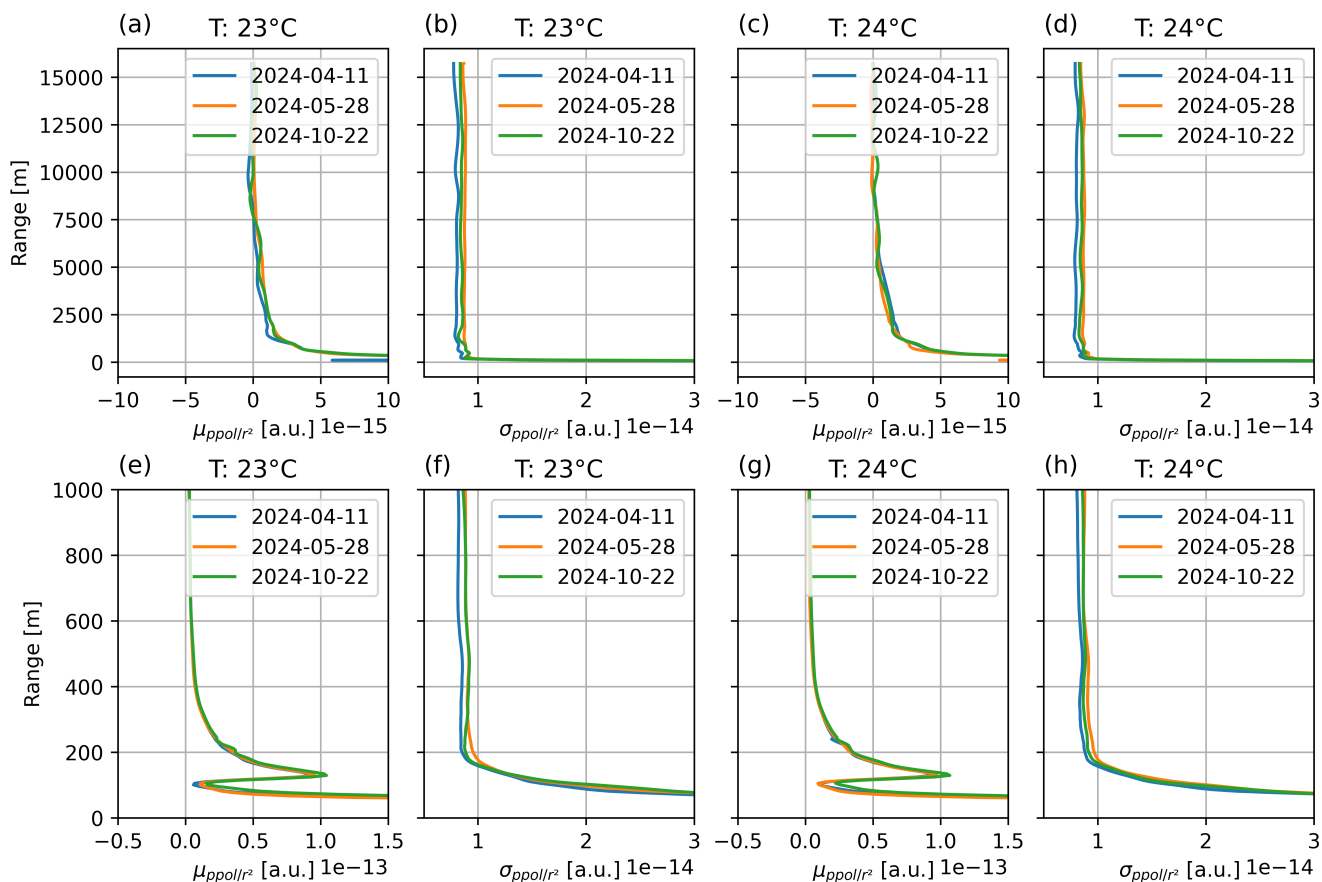


Figure 8. Calibration profiles in Vehmasmäki at 23°C and 24°C, recorded at three different time points over a six-month period in 2024.

Figure 8 shows how the instrumental bias during the termination hood measurement at Vehmasmäki varies over time under consistent internal temperature conditions. Overall, Over a six-month period, the calibration profiles at a fixed internal

~~temperature remain consistent for at least one month, but small deviations can emerge over a six-month period. As a result each~~
~~temperature show only minor fluctuations. Therefore,~~ we recommend performing ~~the termination hood measurement checks~~
~~every few months during continuous operation~~ termination hood checks at least once across the operating temperature range to
~~determine the instrumental background bias and noise.~~

Figure 9 presents the time series of calibration factor from the cloud calibration and Rayleigh calibration methods for all the ceilometers. Detailed results of the cloud calibration factors derived from liquid cloud signals at each site are presented in Figures [S4S8–S7S11](#). Overall, the calibration factors obtained from the two methods agree well within their respective uncertainties. In Lindenberg, the calibration factor from the cloud calibration exhibits an approximate threefold decline over time, reflecting notable signal degradation. During this degradation period, Rayleigh calibration could not be performed because the elevated background-noise level (see Section 4.1) obscured the molecular return. In contrast, the other instruments show only short-term fluctuations without any clear long-term trend. Two periods with notable deviations in the calibration factor were also identified: June to October 2023 and November to December 2024 in Vehmasmäki. The issue in the CL61 ceilometer at Vehmasmäki is due to the fogged window that attenuates the outgoing signal. This will be analyzed in more detail in the following section.

Across all instruments, the calibration factor generally stays within the range of 0.9 to 1.5 as long as laser power remains above 40%, aside from occasional deviations due to specific instrument issues. In Vehmasmäki, as the laser power remains above 90%, the calibration factor fluctuates around 1 within 10% fluctuation. In [Hyytiälä](#), the highest changes in calibration factor is observed when the instrument's laser power is below 80% with the firmware 1.1.10 and then below 60% with the firmware 1.2.7. However, the calibration factor remains relatively stable at 1.25 even when the laser power drops from 100% to 40% with the firmware 1.2.7. In Kenttäröva, laser power percentages were not recorded before June 2023, but the observed increase in the calibration factor is likely linked to a decrease in laser power. After a new transmitter was installed, the calibration factor returned to around 1. In Lindenberg, a noticeable decline in the cloud calibration factor was observed as laser power dropped from 40% to 10%. It is still to be ascertained whether this trend also appears in instruments running the newer firmware version 1.2.7.

Figure [S8–S12](#) demonstrates the utility of cloud calibration for two cases; one with 80% laser power on 2024-03-03 and another with just 10% on 2024-11-16. This indicates that the method can still be used in situations with low laser power and since the internal calibration value may not scale with low laser power values, regular cloud calibration is necessary to understand instrument performance and continue to provide profiles that can be used quantitatively, especially for laser power values below 40%.

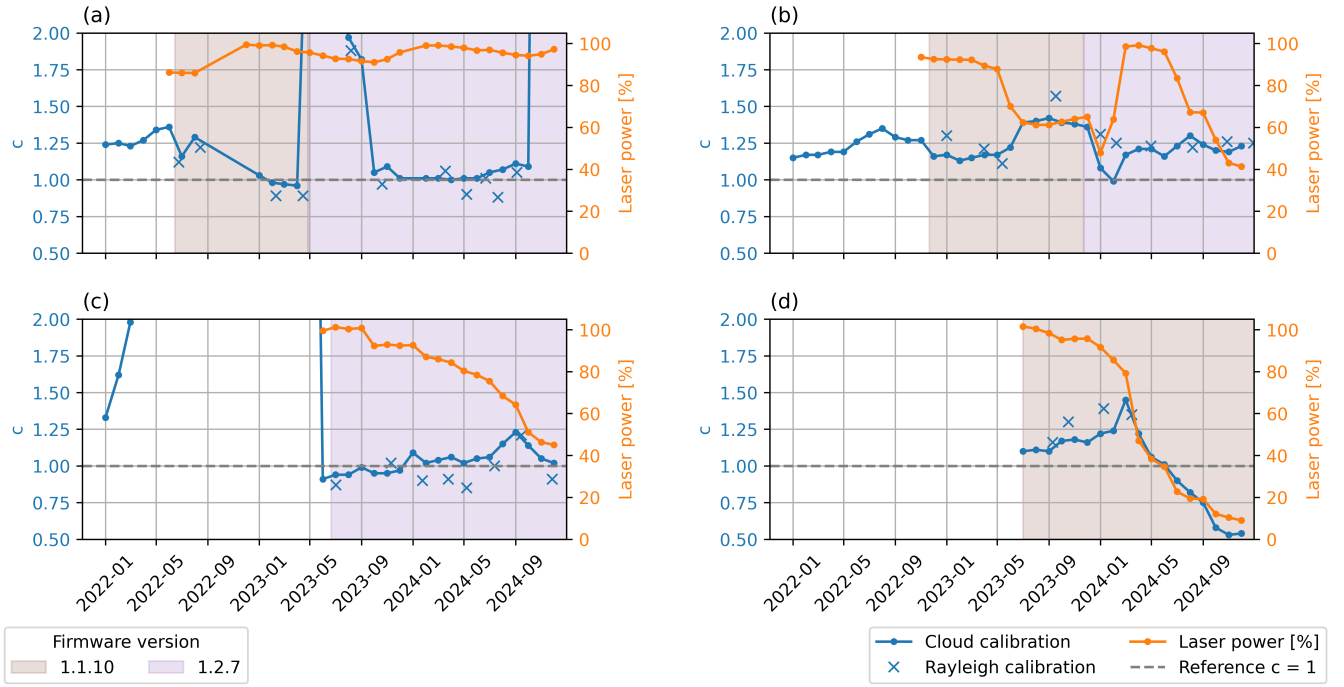


Figure 9. Time series of the calibration factor from cloud calibration, Rayleigh calibration and laser power at four sites: a) Vehmasmäki, b) Hyytiälä, c) Kenttäröva, and d) Lindenberg. The dashed line indicates a calibration factor of $c = 1$. Periods corresponding to different firmware versions are highlighted with shaded areas.

4.4 Signal correction and uncertainty estimation

After recording the termination hood profiles at different temperatures and determining the calibration factor, the correction and forward Klett inversion can be applied, and the associated uncertainty can be estimated using the method described in Sect. 3.3. Example results of this procedure are illustrated in Figs. 10 and 11 showcasing a typical Finnish low aerosol load condition in Kenttärova. During this period, the calibration factor was close to 1. On this date (Fig. 11), aerosol was present below 1000 m within the boundary layer close to the ground, while several layers of clouds extended from 2 km up to 3.5 km. Fig. Figure 10 presents the β , δ and their associated uncertainties in the aerosol layer below 1000 m obtained in the same day from a measurement profile recorded at 13:00 UTC-01 UTC on the same day.

In this below 1000 m range, the instrument-bias-corrected β_v -corrected β'_v differs only slightly from the original uncorrected β , with values β'_v , with the difference ranging from 1×10^{-9} to $2.5 \times 10^{-9} \text{ sr}^{-1} \text{ m}^{-1}$ (Fig. 10a). This difference is expected to be even relatively smaller within the clouds, where the signal is stronger and the instrumental bias decreases with increasing range. In contrast, the aerosol-backscatter-particle backscatter coefficient β_p is substantially lower than β - β'_v by approximately $1.5 \times 10^{-7} \text{ sr}^{-1} \text{ m}^{-1}$, indicating a significant contribution from molecular scattering. The $\sigma_{\beta_v}^2$ - $\sigma_{\beta'_v}^2$ and $\sigma_{\beta_p}^2$ profiles are relatively similar to each other, and they both increase exponentially with height (Fig. 10b).

Similarly, the original uncorrected (δ) and the instrument-bias corrected (δ_v) profiles differ only slightly, by the difference is about 0.001 to 0.005 (Fig. 10c) while δ itself being around 0.07. In contrast, the aerosol-particle linear depolarization ratio δ_p is substantially higher, differing from the original δ by approximately 0.1 -with δ_p at around 0.1 to 0.15. For example, during pollen seasons in Finland, δ_p has been observed at 0.23 for pine and 0.26 for birch at this wavelength (Filioglou et al., 2023). The variances ($\sigma_{\delta_v}^2$, $\sigma_{\delta_p}^2$) are comparable below 200 m, but at higher ranges, $\sigma_{\delta_p}^2$ becomes markedly larger.

Overall, the pronounced differences between β - β'_v and β_p , as well as between δ - δ_v and δ_p , highlight the importance of accounting for the molecular contribution when performing quantitative assessments of aerosol measurement with this instrument CL61 for low aerosol load conditions in Finland. While the difference between β and β_v - β'_v (and δ and δ_v) may be small, the hood-termination-termination hood remains important as it allows the estimation of measurement uncertainty-uncertainties. Averaging multiple profiles reduces the uncertainties, as illustrated in Fig. S13, which shows the profiles averaged over 10 minutes.

Figure 11 illustrates the time series of β_v - β'_v , δ_v , β_p , and δ_p profiles, along with their corresponding variances on the same day. Similar to Fig. 10, β_v - β'_v is higher than β_p while δ_v is lower than β_p - δ_p in this period. The profiles of $\sigma_{\beta_v}^2$ - $\sigma_{\beta'_v}^2$ and $\sigma_{\beta_p}^2$ vary with time during this period, with exhibiting an exponential increase with range. On the other hand, the $\sigma_{\delta_v}^2$ and $\sigma_{\delta_p}^2$ profiles demonstrate a more pronounced dependence on the signal magnitude (Fig. 11 d and h), with stronger atmospheric signals resulting in smaller uncertainties.

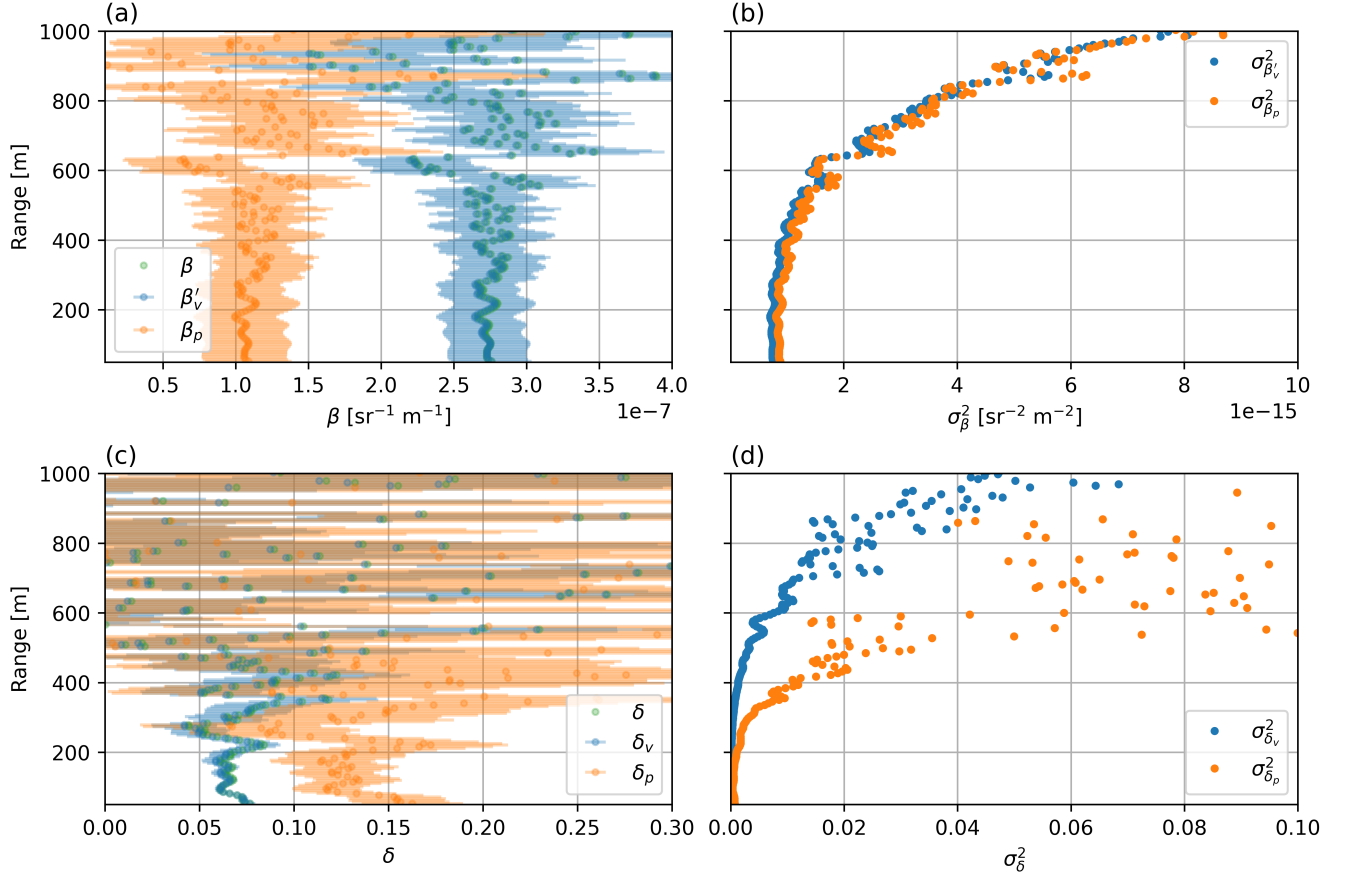


Figure 10. Example of uncorrected and corrected profiles in [Kentärova-Kentärova](#) measured at 2024-06-04 13:01 UTC. a) β ([instrument provided](#)), β_v ([bias corrected and calibrated](#)), β_p , b) $\sigma_{\beta_v}^2$, $\sigma_{\beta_p}^2$, c) δ ([instrument provided](#)), δ_v ([bias corrected and calibrated](#)), δ_p , d) $\sigma_{\delta_v}^2$, $\sigma_{\delta_p}^2$.

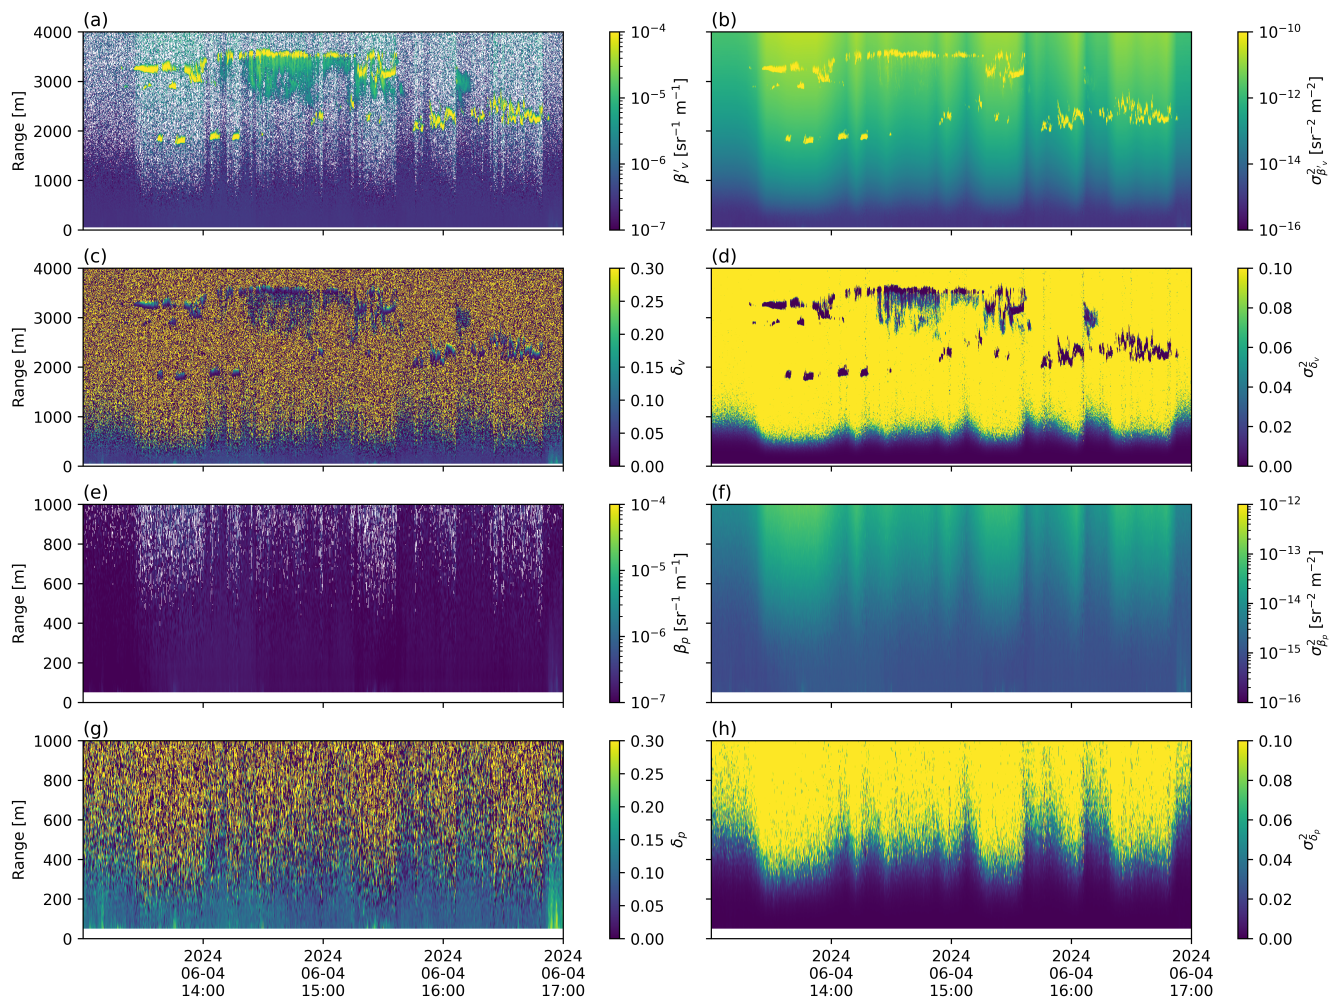


Figure 11. An example of corrected and calibrated profile in Kenttärova on 2024-06-04 13:00 - 17:00 UTC (same day as Fig. 10). a) β'_v , b) $\sigma_{\beta'_v}^2$, c) δ_v , d) $\sigma_{\delta_v}^2$, e) β_p , f) $\sigma_{\beta_p}^2$, g) δ_p , and h) $\sigma_{\delta_p}^2$. For particle properties in panels e-h, profiles are shown only up to 1 km range.

4.5 Signal loss

As previously noted, abrupt changes in the cloud calibration factor at Vehmasmäki were observed from June to October 2023 and again from November to December 2024. Similar deviations are present during the same periods as seen in the window condition housekeeping variable (Fig. S9S14). These patterns indicate that an obstruction, likely on the instrument window, was attenuating both outgoing and incoming laser beams.

Figure 12 illustrates a specific example from 19 May, 2023. On this date, a sudden drop in the attenuated backscatter signal below 2000 m occurred just before 06:00 UTC. At the same time, the window condition value sharply declined from around 100% to 70%. This coincided with the automatic deactivation of the window blower heater. Housekeeping data, including internal temperature and relative humidity, were used to estimate the internal dew point, which was then compared to external air temperature. When the window blower heater was off, the window cooled to match the outside air temperature. Once the window temperature dropped below the internal dew point, condensation began to form on the ~~surface~~inside surface of the window and attenuated the signal. This occurred despite the measured internal relative humidity remaining below 70%. This is because the measurement does not represent the relative humidity at the window surface, where temperature is closer to ambient temperature.

Since condensation affects the entire signal profile and the degree of attenuation depends on its severity, it is not possible to precisely quantify the signal loss or reconstruct the original profile. ~~To mitigate this issue, we recommend~~This issue could be mitigated by keeping both the window blower and heater ~~on~~always on. However, at the time of this writing, this is not possible (personal communication with Vaisala). Additionally, hardware modifications may be required to maintain a sufficiently low internal dew point and prevent fogging.

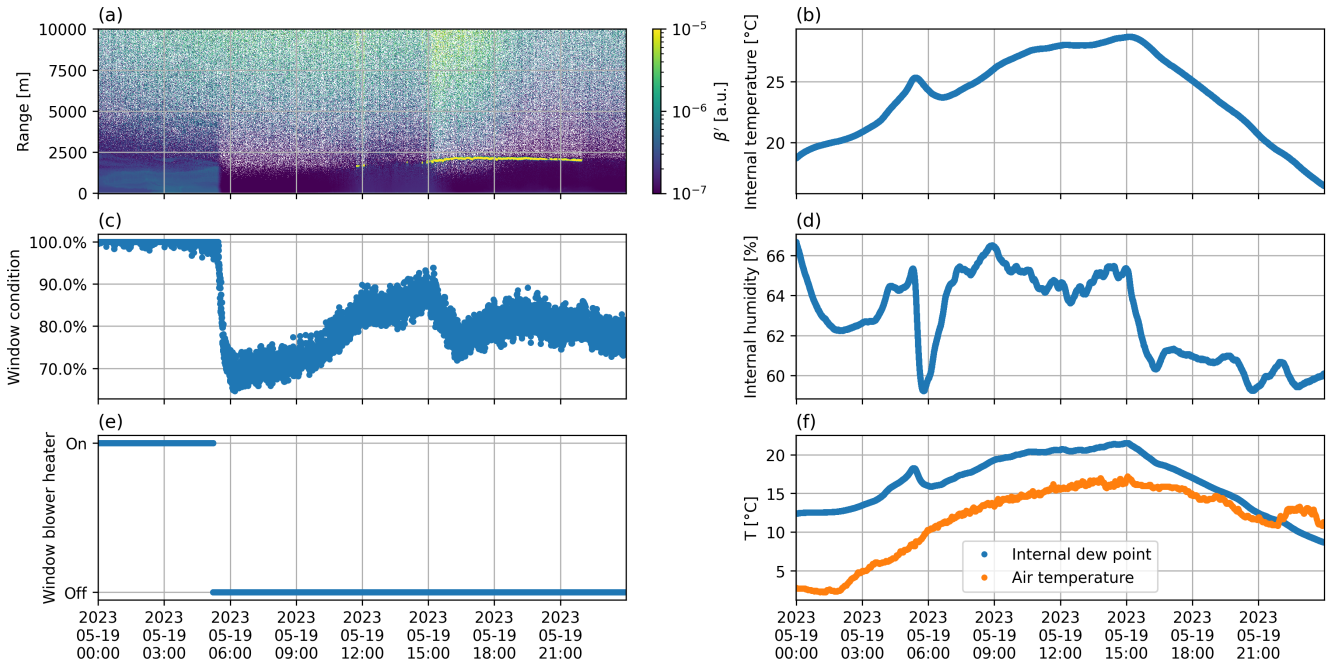


Figure 12. Measurements from Vehmasmäki on 2023-05-19 a) β' , b) Internal temperature, c) window condition, d) internal-Internal humidity, e) Window blower heater, f) Calculated dew point and measured outside air temperature, e) window-blower-heater.

In this study, we ~~present a methodology for identifying the background signal and selecting suitable liquid cloud layers for quantifying temporal variations in~~ quantify the temporal variability of background noise and ~~determining the calibration factor over time.~~ calibration factors for the CL61 ALC across multiple sites over a three-year period using methodologies adapted from existing approaches. In all instruments, a reduction in laser power leads to increased background noise. For most instruments, internal scaling of the calibration ~~constant factor~~ effectively compensates for changes in laser power. However, for the instrument at the Lindenberg site with an older firmware, this compensation becomes insufficient when laser power drops below 40%, resulting in a drift in the calibration factor. Therefore, regular cloud calibration is necessary to ensure quantitatively reliable profiles, especially when the laser power falls below 40%. Some deviations in the calibration factor were linked with ~~internal fogging of the~~ inside surface of the window.

Termination hood measurements were performed on selected instruments and proved effective in characterizing the ~~instrument noise profile and the temperature dependence of the overlap function~~ instrumental background bias and noise profiles and their temperature dependence. Notably, differences in the instrumental bias were observed between parallel and perpendicular polarizations. The calibration profiles also reveal periodic variations in the near range signal below 50 m in both polarizations. As they appear sporadically, we recommend discarding the first 50 m of measurements. Instrumental bias profiles were obtained across a range of internal temperatures and were subsequently used to correct the bias and estimate its associated uncertainty. These profiles remained stable for at least one month for a given internal temperature, although small deviations appeared over a six-month period. Consequently, we recommend making termination-hood measurements ~~every six months during continuous operation~~ at least once across the operating temperature range to determine the instrumental noise.

In a representative summer case study at Kenttärova, the instrumental bias corrected attenuated backscatter coefficient and ~~depolarization ratio β_v~~ volume linear depolarization ratio β'_v and δ_v differ only slightly from their uncorrected counterparts β and δ , up to $2.5 \times 10^{-9} \text{ sr}^{-1} \text{ m}^{-1}$ and 0.005 respectively, reflecting the relatively small instrumental bias in both polarization channels compared with the atmospheric signal. Nevertheless, the termination hood measurements remain crucial, as they allow the instrumental ~~noise background~~ to be quantified and ~~thus enable the derivation of measurement uncertainties.~~ The study also highlights the importance of accounting for the molecular contribution when quantitatively interpreting aerosol measurements with the CL61 ceilometer. We ~~subsequently used to estimate the uncertainties of β_p and δ_p , as presented in this study.~~ For typical low aerosol load conditions in Finland, as in this study case, we found that the difference between β_p and β is approximately $1.5 \times 10^{-7} \text{ sr}^{-1} \text{ m}^{-1}$, and that between δ and δ_p is roughly 0.1 in the near surface layer. ~~These differences can be substantial when aerosol loading is low but they may also vary depending on the aerosol properties and prevailing atmospheric conditions.~~

Additionally, some instruments experienced signal loss caused by the fogging of the ~~optical lens~~ inside surface of the window, which resulted in degraded data quality. Identifying and excluding such periods is essential for ensuring the integrity of the dataset and the reliability of subsequent analyses.

Data availability. The CL61 and model data used in this study are provided by the Aerosol, Clouds and Trace Gases Research Infrastructure (ACTRIS) and are available respectively from the ACTRIS Data Centre using the following DOIs: 10.60656/57adeb3f598243f2 and 10.60656/d2626d9dd3454006). The CL61 raw data was obtained from the landing page of the DOI.

Author contributions. VL, EOC and MF performed the termination hood calibrations. VL prepared the manuscript. EOC, MF, VV contributed remarks and revisions on the manuscript.

Competing interests. The authors declare that they have no conflict of interest.

Acknowledgements. Financial support by Magnus Ehrnrooth Foundation is gratefully acknowledged. This project was supported by the Research Council of Finland (grant no 337552, 343359). The authors also gratefully acknowledge the support of Vaikuttavuussäätiö (the Finnish Research Impact Foundation) through the Tandem Industry Academia (TIA) program. We also acknowledge ACTRIS, the Finnish Meteorological Institute, and the Lindenberg Meteorological Observatory - Richard Assmann Observatory (MOL-RAO) for providing the data set which is available for download from <https://cloudnet.fmi.fi>.

References

- 510 Baars, H., Kanitz, T., Engelmann, R., Althausen, D., Heese, B., Komppula, M., Preißler, J., Tesche, M., Ansmann, A., Wandinger, U., Lim, J. H., Young Ahn, J., Stachlewska, I. S., Amiridis, V., Marinou, E., Seifert, P., Hofer, J., Skupin, A., Schneider, F., Bohlmann, S., Foth, A., Bley, S., Pfüller, A., Giannakaki, E., Lihavainen, H., Viisanen, Y., Kumar Hooda, R., Pereira, S. N., Bortoli, D., Wagner, F., Mattis, I., Janicka, L., Markowicz, K. M., Achtert, P., Artaxo, P., Pauliquevis, T., Souza, R. A., Prakesh Sharma, V., Gideon Van Zyl, P., Paul Beukes, J., Sun, J., Rohwer, E. G., Deng, R., Mamouri, R. E., and Zamorano, F.: An overview of the first decade of PollyNET: An emerging network of automated Raman-polarization lidars for continuous aerosol profiling, *Atmospheric Chemistry and Physics*, 16, 5111–5137, <https://doi.org/10.5194/acp-16-5111-2016>, 2016.
- 515 Baars, H., Seifert, P., Engelmann, R., and Wandinger, U.: Target categorization of aerosol and clouds by continuous multiwavelength-polarization lidar measurements, *Atmospheric Measurement Techniques*, 10, 3175–3201, <https://doi.org/10.5194/amt-10-3175-2017>, 2017.
- 520 Barragán, R., Molero, F., Salvador, P., Theobald, M. R., Vivanco, M. G., Rodríguez-Sánchez, A., Gil, V., Garrido, J. L., Pujadas, M., and Artíñano, B.: Study of the Effect of Different Atmospheric Conditions on the Temporal Evolution of the Mixing Layer over Madrid during the Year 2020 by Means of Two Different Methods: Ceilometer Signals and the ECMWF-IFS Meteorological Model, *Remote Sensing*, 15, 5583, <https://doi.org/10.3390/rs15235583>, 2023.
- Biele, J., Beyerle, G., and Baumgarten, G.: Polarization lidar: Corrections of instrumental effects, *Optics Express*, 7, 427–435, <https://doi.org/10.1364/OE.7.000427>, 2000.
- 525 Biniotoglou, I., Amodeo, A., D’Amico, G., Giunta, A., Madonna, F., Mona, L., and Pappalardo, G.: Examination of possible synergy between lidar and ceilometer for the monitoring of atmospheric aerosols, in: *Lidar Technologies, Techniques, and Measurements for Atmospheric Remote Sensing VII*, vol. 8182, pp. 48–60, SPIE, <https://doi.org/10.1117/12.897530>, 2011.
- Bucholtz, A.: Rayleigh-scattering calculations for the terrestrial atmosphere, *Applied Optics*, 34, 2765–2773, <https://doi.org/10.1364/AO.34.002765>, 1995.
- 530 Burton, S. P., Ferrare, R. A., Hostetler, C. A., Hair, J. W., Rogers, R. R., Obland, M. D., Butler, C. F., Cook, A. L., Harper, D. B., and Froyd, K. D.: Aerosol classification using airborne High Spectral Resolution Lidar measurements—methodology and examples, *Atmospheric Measurement Techniques*, 5, 73–98, <https://doi.org/10.5194/amt-5-73-2012>, 2012.
- Campbell, J. R., Hlavka, D. L., Welton, E. J., Flynn, C. J., Turner, D. D., Spinhirne, J. D., Scott, V. S., and Hwang, I. H.: Full-Time, Eye-Safe Cloud and Aerosol Lidar Observation at Atmospheric Radiation Measurement Program Sites: Instruments and Data Processing, *Journal of Atmospheric and Oceanic Technology*, 19, 431–442, [https://doi.org/10.1175/1520-0426\(2002\)019<0431:FTESCA>2.0.CO;2](https://doi.org/10.1175/1520-0426(2002)019<0431:FTESCA>2.0.CO;2), 2002.
- 535 Cao, N., Zhu, C., Kai, Y., and Yan, P.: A method of background noise reduction in lidar data, *Applied Physics B*, 113, 115–123, <https://doi.org/10.1007/s00340-013-5447-9>, 2013.
- Cimini, D., Haeffelin, M., Kotthaus, S., Löhnert, U., Martinet, P., O’Connor, E., Walden, C., Coen, M. C., and Preissler, J.: Towards the profiling of the atmospheric boundary layer at European scale—introducing the COST Action PROBE, *Bulletin of Atmospheric Science and Technology*, 1, 23–42, <https://doi.org/10.1007/s42865-020-00003-8>, 2020.
- 540 Donovan, D. P., Klein Baltink, H., Henzing, J. S., De Roode, S. R., and Siebesma, A. P.: A depolarisation lidar-based method for the determination of liquid-cloud microphysical properties, *Atmospheric Measurement Techniques*, 8, 237–266, <https://doi.org/10.5194/amt-8-237-2015>, 2015.

- 545 Fernald, F. G., Herman, B. M., and Reagan, J. A.: Determination of Aerosol Height Distributions by Lidar, *Journal of Applied Meteorology and Climatology*, 11, 482–489, [https://doi.org/10.1175/1520-0450\(1972\)011<0482:DOAHDB>2.0.CO;2](https://doi.org/10.1175/1520-0450(1972)011<0482:DOAHDB>2.0.CO;2), 1972.
- Filioglou, M., Leskinen, A., Vakkari, V., O'Connor, E., Tuononen, M., Tuominen, P., Laukkanen, S., Toiviainen, L., Saarto, A., Shang, X., Tiitta, P., and Komppula, M.: Spectral dependence of birch and pine pollen optical properties using a synergy of lidar instruments, *Atmospheric Chemistry and Physics*, 23, 9009–9021, <https://doi.org/10.5194/acp-23-9009-2023>, 2023.
- 550 Filioglou, M., Tiitta, P., Shang, X., Leskinen, A., Ahola, P., Pätsi, S., Saarto, A., Vakkari, V., Isopahkala, U., and Komppula, M.: Lidar estimates of birch pollen number, mass, and CCN-related concentrations, *Atmospheric Chemistry and Physics*, 25, 1639–1657, <https://doi.org/10.5194/acp-25-1639-2025>, 2025.
- Floutsi, A. A., Baars, H., Engelmann, R., Althausen, D., Ansmann, A., Bohlmann, S., Heese, B., Hofer, J., Kanitz, T., Haarig, M., Ohneiser, K., Radenz, M., Seifert, P., Skupin, A., Yin, Z., Abdullaev, S. F., Komppula, M., Filioglou, M., Giannakaki, E., Stachlewska, I. S., Janicka, L., Bortoli, D., Marinou, E., Amiridis, V., Gialitaki, A., Mamouri, R.-E., Barja, B., and Wandinger, U.: DeLiAn – a growing collection of depolarization ratio, lidar ratio and Ångström exponent for different aerosol types and mixtures from ground-based lidar observations, *Atmospheric Measurement Techniques*, 16, 2353–2379, <https://doi.org/10.5194/amt-16-2353-2023>, 2023.
- 555 Freudenthaler, V., Esselborn, M., Wiegner, M., Heese, B., Tesche, M., Ansmann, A., Müller, D., Althausen, D., Wirth, M., Fix, A., Ehret, G., Knippertz, P., Toledano, C., Gasteiger, J., Garhammer, M., and Seefeldner, M.: Depolarization ratio profiling at several wavelengths in pure Saharan dust during SAMUM 2006, *Tellus B*, 61, 165–179, <https://doi.org/10.1111/j.1600-0889.2008.00396.x>, 2009.
- 560 Görsdorf, U., Komppula, M., Moisseev, D., and O'Connor, E.: Custom collection of lidar data from Hyttiälä, Kenttäröva, Lindenberg, and Vehmasmäki between 1 Oct 2021 and 31 Dec 2024, <https://doi.org/10.60656/D2626D9DD3454006>, 2025.
- Haeffelin, M., Laffineur, Q., Bravo-Aranda, J.-A., Drouin, M.-A., Casquero-Vera, J.-A., Dupont, J.-C., and De Backer, H.: Radiation fog formation alerts using attenuated backscatter power from automatic lidars and ceilometers, *Atmospheric Measurement Techniques*, 9, 5347–5365, <https://doi.org/10.5194/amt-9-5347-2016>, 2016.
- 565 Hervo, M., Poltera, Y., and Haeferle, A.: An empirical method to correct for temperature-dependent variations in the overlap function of CHM15k ceilometers, *Atmospheric Measurement Techniques*, 9, 2947–2959, <https://doi.org/10.5194/amt-9-2947-2016>, 2016.
- Hirsikko, A., O'Connor, E. J., Komppula, M., Korhonen, K., Pfüller, A., Giannakaki, E., Wood, C. R., Bauer-Pfundstein, M., Poikonen, A., Karppinen, T., Lonka, H., Kurri, M., Heinonen, J., Moisseev, D., Asmi, E., Aaltonen, V., Nordbo, A., Rodriguez, E., Li-havainen, H., Laaksonen, A., Lehtinen, K. E. J., Laurila, T., Petäjä, T., Kulmala, M., and Viisanen, Y.: Observing wind, aerosol particles, cloud and precipitation: Finland's new ground-based remote-sensing network, *Atmospheric Measurement Techniques*, 7, 1351–1375, <https://doi.org/10.5194/amt-7-1351-2014>, 2014.
- 570 Hopkin, E., Illingworth, A. J., Charlton-Perez, C., Westbrook, C. D., and Ballard, S.: A robust automated technique for operational calibration of ceilometers using the integrated backscatter from totally attenuating liquid clouds, *Atmospheric Measurement Techniques*, 12, 4131–4147, <https://doi.org/10.5194/amt-12-4131-2019>, 2019.
- Hämäläinen, K., Hirsikko, A., Leskinen, A., Komppula, M., O'Connor, E. J., and Niemelä, S.: Evaluating atmospheric icing forecasts with ground-based ceilometer profiles, *Meteorological Applications*, 27, e1964, <https://doi.org/10.1002/met.1964>, 2020.
- Illingworth, A. J., Barker, H. W., Beljaars, A., Ceccaldi, M., Chepfer, H., Clerbaux, N., Cole, J., Delanoë, J., Domenech, C., Donovan, D. P., Fukuda, S., Hirakata, M., Hogan, R. J., Huenerbein, A., Kollias, P., Kubota, T., Nakajima, T., Nakajima, T. Y., Nishizawa, T., Ohno, Y., Okamoto, H., Oki, R., Sato, K., Satoh, M., Shephard, M. W., Velázquez-Blázquez, A., Wandinger, U., Wehr, T., and Van Zadelhoff, G. J.: The earthcare satellite : The next step forward in global measurements of clouds, aerosols, precipitation, and radiation, *Bulletin of the American Meteorological Society*, 96, 1311–1332, <https://doi.org/10.1175/BAMS-D-12-00227.1>, 2015.
- 580

- Illingworth, A. J., Cimini, D., Haeferle, A., Haeffelin, M., Hervo, M., Kotthaus, S., Löhnert, U., Martinet, P., Mattis, I., O'Connor, E. J., and Potthast, R.: How Can Existing Ground-Based Profiling Instruments Improve European Weather Forecasts?, *Bulletin of the American Meteorological Society*, 100, 605–619, <https://doi.org/10.1175/BAMS-D-17-0231.1>, 2019.
- Klett, J. D.: Lidar inversion with variable backscatter/extinction ratios, *Applied Optics*, 24, 1638–1643, <https://doi.org/10.1364/AO.24.001638>, 1985.
- Kotthaus, S., O'Connor, E., Munkel, C., Charlton-Perez, C., Haeffelin, M., Gabey, A. M., and Grimmond, C. S. B.: Recommendations for processing atmospheric attenuated backscatter profiles from Vaisala CL31 ceilometers, *Atmospheric Measurement Techniques*, 9, 3769–3791, <https://doi.org/10.5194/amt-9-3769-2016>, 2016.
- Kotthaus, S., Bravo-Aranda, J. A., Collaud Coen, M., Guerrero-Rascado, J. L., Costa, M. J., Cimini, D., O'Connor, E. J., Hervo, M., Alados-Arboledas, L., Jiménez-Portaz, M., Mona, L., Ruffieux, D., Illingworth, A., and Haeffelin, M.: Atmospheric boundary layer height from ground-based remote sensing: a review of capabilities and limitations, *Atmospheric Measurement Techniques*, 16, 433–479, <https://doi.org/10.5194/amt-16-433-2023>, 2023.
- Le, V., Lobo, H., O'Connor, E. J., and Vakkari, V.: Long-term aerosol particle depolarization ratio measurements with HALO Photonics Doppler lidar, *Atmospheric Measurement Techniques*, 17, 921–941, <https://doi.org/10.5194/amt-17-921-2024>, 2024.
- Lee, G., Gommers, R., Waselewski, F., Wohlfahrt, K., and O'Leary, A.: PyWavelets: A Python package for wavelet analysis, *Journal of Open Source Software*, 4, 1237, <https://doi.org/10.21105/joss.01237>, 2019.
- Mamouri, R. E. and Ansmann, A.: Potential of polarization lidar to provide profiles of CCN-and INP-relevant aerosol parameters, *Atmospheric Chemistry and Physics*, 16, 5905–5931, <https://doi.org/10.5194/acp-16-5905-2016>, 2016.
- Martucci, G., Milroy, C., and O'Dowd, C. D.: Detection of Cloud-Base Height Using Jenoptik CHM15K and Vaisala CL31 Ceilometers, *Journal of Atmospheric and Oceanic Technology*, 27, 305–318, <https://doi.org/10.1175/2009JTECHA1326.1>, 2010.
- Nason, G. P. and Silverman, B. W.: *The Stationary Wavelet Transform and some Statistical Applications*, pp. 281–299, Springer New York, New York, NY, https://doi.org/10.1007/978-1-4612-2544-7_17, 1995.
- Nicolae, D., Vasilescu, J., Talianu, C., Biniotoglou, I., Nicolae, V., Andrei, S., and Antonescu, B.: A neural network aerosol-typing algorithm based on lidar data, *Atmospheric Chemistry and Physics*, 18, 14 511–14 537, <https://doi.org/10.5194/acp-18-14511-2018>, 2018.
- O'Connor, E.: Model data from Kenttärova on 5 March 2024, <https://hdl.handle.net/21.12132/1.b218f85f5ed14149>, 2024.
- O'Connor, E.: Custom collection of model data from Hyytiälä, Kenttärova, Lindenberg, and Vehmasmäki between 1 Oct 2021 and 31 Dec 2024, <https://doi.org/10.60656/57ADEB3F598243F2>, 2025.
- O'Connor, E. J., Illingworth, A. J., and Hogan, R. J.: A technique for autocalibration of cloud lidar, *Journal of Atmospheric and Oceanic Technology*, 21, 777–786, [https://doi.org/10.1175/1520-0426\(2004\)021<0777:ATFAOC>2.0.CO;2](https://doi.org/10.1175/1520-0426(2004)021<0777:ATFAOC>2.0.CO;2), 2004.
- Ribaud, J.-F., Haeffelin, M., Dupont, J.-C., Drouin, M.-A., Toledo, F., and Kotthaus, S.: PARAFOG v2.0: a near-real-time decision tool to support nowcasting fog formation events at local scales, *Atmospheric Measurement Techniques*, 14, 7893–7907, <https://doi.org/10.5194/amt-14-7893-2021>, 2021.
- Rocadenbosch, F., Barragán, R., Frasier, S. J., Waldinger, J., Turner, D. D., Tanamachi, R. L., and Dawson, D. T.: Ceilometer-Based Rain-Rate Estimation: A Case-Study Comparison With S-Band Radar and Disdrometer Retrievals in the Context of VORTEX-SE, *IEEE Transactions on Geoscience and Remote Sensing*, 58, 8268–8284, <https://doi.org/10.1109/TGRS.2020.2984458>, 2020.
- Roschke, J., Witthuhn, J., Klingebiel, M., Haarig, M., Foth, A., Kötsche, A., and Kalesse-Los, H.: Discriminating between “drizzle or rain” and sea salt aerosols in Cloudnet for measurements over the Barbados Cloud Observatory, *Atmospheric Measurement Techniques*, 18, 487–508, <https://doi.org/10.5194/amt-18-487-2025>, 2025.

- Sassen, K.: The Polarization Lidar Technique for Cloud Research: A Review and Current Assessment, *Bulletin of the American Meteorological Society*, 72, 1848–1866, [https://doi.org/10.1175/1520-0477\(1991\)072<1848:TPLTFC>2.0.CO;2](https://doi.org/10.1175/1520-0477(1991)072<1848:TPLTFC>2.0.CO;2), 1991.
- Shang, X., Mielonen, T., Lipponen, A., Giannakaki, E., Leskinen, A., Buchard, V., Darmenov, A. S., Kukkurainen, A., Arola, A., O'Connor, E., Hirsikko, A., and Komppula, M.: Mass concentration estimates of long-range-transported Canadian biomass burning aerosols from a multi-wavelength Raman polarization lidar and a ceilometer in Finland, *Atmospheric Measurement Techniques*, 14, 6159–6179, <https://doi.org/10.5194/amt-14-6159-2021>, 2021.
- Tomasi, C., Vitale, V., Petkov, B., Lupi, A., and Cacciari, A.: Improved algorithm for calculations of Rayleigh-scattering optical depth in standard atmospheres, *Applied Optics*, 44, 3320–3341, <https://doi.org/10.1364/AO.44.003320>, 2005.
- Tsaknakis, G., Papayannis, A., Kokkalis, P., Amiridis, V., Kambezidis, H. D., Mamouri, R. E., Georgoussis, G., and Avdikos, G.: Inter-comparison of lidar and ceilometer retrievals for aerosol and Planetary Boundary Layer profiling over Athens, Greece, *Atmospheric Measurement Techniques*, 4, 1261–1273, <https://doi.org/10.5194/amt-4-1261-2011>, 2011.
- Uzan, L., Egert, S., Khain, P., Levi, Y., Vadislavsky, E., and Alpert, P.: Ceilometers as planetary boundary layer height detectors and a corrective tool for COSMO and IFS models, *Atmospheric Chemistry and Physics*, 20, 12 177–12 192, <https://doi.org/10.5194/acp-20-12177-2020>, 2020.
- Van der Kamp, D.: Ceilometer observations of Vancouver's urban boundary layer : validation and mixed-layer height estimation, Ph.D. thesis, University of British Columbia, <https://doi.org/10.14288/1.0066572>, 2008.
- Wandinger, U.: Introduction to Lidar, in: *Lidar: Range-Resolved Optical Remote Sensing of the Atmosphere*, edited by Weitkamp, C., pp. 1–18, Springer New York, New York, NY, https://doi.org/10.1007/0-387-25101-4_1, 2005.
- Warren, E., Charlton-Perez, C., Kotthaus, S., Lean, H., Ballard, S., Hopkin, E., and Grimmond, S.: Evaluation of forward-modelled attenuated backscatter using an urban ceilometer network in London under clear-sky conditions, *Atmospheric Environment*, 191, 532–547, <https://doi.org/10.1016/j.atmosenv.2018.04.045>, 2018.
- Welton, E. J. and Campbell, J. R.: Micropulse Lidar Signals: Uncertainty Analysis, *Journal of Atmospheric and Oceanic Technology*, 19, 2089–2094, [https://doi.org/10.1175/1520-0426\(2002\)019<2089:MLSUA>2.0.CO;2](https://doi.org/10.1175/1520-0426(2002)019<2089:MLSUA>2.0.CO;2), 2002.
- Wiegner, M. and Geiß, A.: Aerosol profiling with the Jenoptik ceilometer CHM15kx, *Atmospheric Measurement Techniques*, 5, 1953–1964, <https://doi.org/10.5194/amt-5-1953-2012>, 2012.
- Wiegner, M., Madonna, F., Biniotoglou, I., Forkel, R., Gasteiger, J., Geiß, A., Pappalardo, G., Schäfer, K., and Thomas, W.: What is the benefit of ceilometers for aerosol remote sensing? An answer from EARLINET, *Atmospheric Measurement Techniques*, 7, 1979–1997, <https://doi.org/10.5194/amt-7-1979-2014>, 2014.