

1 **CRUX-1.0: An automatic GHG and Ozone observation system for**
2 **inland Antarctica Plateau**

3 **Biao Tian^{1,2}, Minghu Ding^{*1,7}, Kongju Zhu¹, Xu Yao³, Yixi Zhao¹, Wenqian Zhang¹, Diyi**
4 **Yang⁴, Weijun Sun⁵, Yining Yu¹, Shoudong Zhao¹, Yige Cui¹, Chuanjin Li³, Jie Tang¹, Cunde**
5 **Xiao⁶, Tong Zhu², Renhe Zhang⁷**

6 ¹ State Key Laboratory of Disaster Weather Science and Technology, Chinese Academy of
7 Meteorological Sciences, Beijing 100081, China

8 ² College of Environmental Sciences and Engineering, Peking University, Beijing 100871, China

9 ³ Polar Research Institute of China, Shanghai, 200136, China

10 ⁴ Haining Meteorological Bureau, Haining 314400, China

11 ⁵ College of Geography and Environment, Shandong Normal University, Jinan, 250014, China

12 ⁶ State Key Laboratory of Earth Surface Processes and Resource Ecology, Beijing Normal
13 University, Beijing 100875, China

14 ⁷ Key Laboratory of Polar Atmosphere-ocean-ice System for Weather and Climate, Ministry of
15 Education, Shanghai 200438, China

16 ^{*}Corresponding authors. E-mail: dingminghu@foxmail.com (Minghu Ding)

17
18 **Abstract:** Antarctic inland regions, as critical hubs for global climate change monitoring, suffer
19 from a lack of reliable long-term greenhouse gas (GHG) observation systems due to **extremely**
20 **low temperatures**, strong winds, and limited logistical/energy support. To address this gap, the
21 CRUX-1.0 automatic observation system was developed and deployed at Taishan Station (inland
22 Antarctic Plateau) during the 39th and 40th CHINARE **(Chinese National Antarctic Research**
23 **Expedition)**, targeting simultaneous monitoring of CO₂ and surface ozone (O₃). Integrating four
24 core subsystems—analysis, calibration, temperature control, and data communication—the system
25 is specifically engineered for harsh polar environments with low power consumption (<350 W)
26 and autonomous operation capability. The operational analysis based on **a one-month continuous**
27 field experiment showed its stable performance: CO₂ measurements achieved a coefficient of
28 variation (CV) <**5.6%** (nearing 0% post-calibration), while O₃ measurements maintained a CV
29 <5.6%. The average concentrations (**CO₂: 420.7±0.7 ppm**; O₃: 20.1±0.8 ppb) closely aligned with
30 regional background levels and South Pole Station data, confirming high reliability. With its
31 robust adaptability, CRUX-1.0 could be extended to other polar or high-altitude regions, further
32 enhancing the global atmospheric monitoring network's coverage and capability.

33 **Keywords:** GHG, Ozone, automatic observation system, Antarctica

34
35 **1. Introduction**

36 Observing atmospheric composition and greenhouse gases is a critical global issue, as it serves as
37 a key benchmark for assessing global changes and formulating policies such as the Paris
38 Agreement and Conference of the Parties (COP) negotiations. Currently, global atmospheric
39 background stations provide a significant amount of observational data, but their distribution
40 remains uneven. In fact, there are notable disparities in greenhouse gas concentrations across
41 different regions. For example, high-latitude and polar regions, including Antarctica, suffer from a
42 lack of observation stations, making it difficult to monitor the atmospheric composition in these

删除[Biao]: extreme low temperatures

删除[Biao]: expeditions

删除[Biao]: A one month continuous

删除[Biao]: 3

删除[Biao]: 1.5

areas (Das et al., 2016; Liu et al., 2024). The absence of sufficient observation capacity in these regions highlights the need for enhanced monitoring systems. In particular, the challenging environmental conditions and logistical difficulties in these regions necessitate advancements in observation technologies and improved support for maintaining such systems. Given these challenges, there is a growing demand for increasing the capacity of remote, unattended observation systems to better capture the atmospheric background in these critical areas (Köne and Büke, 2010).

Autonomous and unattended atmospheric observation technology has achieved initial applications across multiple global spheres. Its core technologies (low-power hardware, automated quality control, and remote data transmission) provide a feasible solution for long-term monitoring in remote/extreme regions. In the marine boundary layer, the autonomous ozone measurement system (equipped with PSI and 2B Technologies sensors) developed by the Woods Hole Oceanographic Institution has successfully operated for over one month in an unattended mode on Atlantic buoys and the Chesapeake Bay Lighthouse Tower, thanks to its waterproof packaging, automatic valve protection (to cope with high winds and sea fog), and fault self-correcting controller. Among them, the 2B sensor consumes less than 4 W of power, which is compatible with the energy constraints of marine platforms (Hints et al., 2004). In the atmospheric background monitoring at fixed terrestrial stations, the 300-meter tall tower station in Bialystok, Poland, has implemented quasi-continuous observations of multiple species such as CO₂, O₂/N₂, and CH₄ since 2005. By automatically calibrating the CO₂/O₂ sensors every 40 hours, the gas chromatography module every 5 days, and conducting weekly flask sampling for quality control, the station has ensured data continuity for more than 3 years. Additionally, multi-height sampling has enabled effective differentiation between local and regional GHG signals (Popa et al., 2010). In the field of mobile observation, the MPAL vehicle-mounted monitoring platform of the University of Michigan achieves 6.5 hours of continuous operation of all instruments relying on LiFeMnPO₄ battery packs. Through automatic PM sampling loss correction and weekly comparison with fixed stations, it completed 84 days of observations with over 260,000 1-second resolution data points in Detroit, verifying the spatiotemporal coverage advantages of mobile unattended platforms (Xia et al., 2023). Furthermore, the REA-FTIR flux system at the Shoalhaven Farm in Australia completed 3 weeks of unattended simultaneous flux observations of CO₂, CH₄, and N₂O relying on 3G remote monitoring and automatic sampling bag switching, and also proposed an innovative method for estimating N₂O background fluxes via CO₂ tracer (Griffith et al., 2009).

The observation of greenhouse gases and other atmospheric components in Antarctica presents significant challenges, particularly regarding conducting unattended monitoring. The extreme environmental conditions, including low temperatures, strong winds, and long periods of darkness, pose technical difficulties for maintaining continuous observation systems (Griffiths et al., 2020). Moreover, logistical support in such a remote region is limited, making it hard to deploy and maintain equipment effectively. Over the years, targeted efforts have been made to address these challenges, with some advances in equipment adaptation, energy management, and data reliability: (1) British Antarctic Survey (BAS) Autonomous Ozone Network (2007–present): BAS deployed a network of 2B Technologies ozone monitors (ultraviolet photometry, 5 min sampling interval, 11–13 W power consumption) across 8 sites, from the southeastern coast of the Weddell Sea to the Antarctic Plateau (Bauguitte et al., 2011). The system relied on "solar-wind hybrid power + lead-acid batteries" (10–14 days of backup) and passive insulation with intake heating to avoid

87 icing. It delivered 5 years of continuous data (2007–2012), with spring ozone concentrations
88 averaging 28 ± 3 ppb along the coast (vs. 35 ± 2 ppb on the plateau) and a data continuity rate of
89 85%. This work first confirmed that ozone depletion rates were higher at polar vortex edges (0.8
90 ppb/day) than inland (0.3 ppb/day). However, limitations emerged: passive insulation failed at
91 -60°C (causing 15% winter data loss), wind turbine blade icing halted power supply for 12
92 consecutive days in 2009, and the lack of automatic calibration required manual on-site
93 zero-checks, increasing operational costs (Bauguitte et al., 2011).

94 (2) Chinese Kunlun Station (Dome A) Ozone Monitoring (2016): During the 2016 Chinese
95 National Antarctic Research Expedition (CHINARE), Ding et al. (2020a) deployed a 2B
96 Technologies Model 205 ozone monitor (10 min sampling interval, 5 W power consumption) at
97 Dome A (80.25°S), leveraging the PLATO astronomical observatory module's shared diesel
98 generator and 50 kWh battery for power. The instrument operated continuously for 1 year,
99 capturing the first annual ozone dataset for Antarctica's highest-latitude inland region—with polar
100 night concentrations averaging 32 ± 4 ppb and summer concentrations 29 ± 2 ppb (15% lower than
101 at Dome C). Data continuity reached 99.5%, validating the Model 205's suitability for extreme
102 cold. Nevertheless, the system suffered from energy dependency (Ding et al., 2020a).

103 (3) Terra Nova Bay Station Stratospheric NO_2 Monitoring (2000): Bortoli et al. (2002) deployed a
104 GASCOD UV-Visible spectrometer (423–460 nm wavelength, 0.5 nm resolution) at Terra Nova
105 Bay Station for unattended NO_2 observations. Key adaptations included a 30° inclined quartz
106 window to reduce snow accumulation, 24-hour continuous measurement (with integration time
107 auto-adjusted from 2–5 seconds at noon to 5–10 minutes at twilight), and a built-in mercury lamp
108 for daily grating calibration (spectral accuracy < 0.2 nm). Invalid data were screened via the "Flux
109 Index (FI)" (values $< 5 \times 10^{-5}$ mV/ms rejected). The system yielded 1996 data showing NO_2 slant
110 column densities (sc) dropping from 1.2×10^{17} to 4×10^{16} molecule/ cm^2 in austral autumn and
111 rebounding in spring—confirming coupling between photochemical loss and dynamic transport. It
112 also quantified temperature-dependent errors: NO_2 sc increased by 3.5%–4% for every 10K rise in
113 cross-section temperature. However, heavy snow in August 1996 covered the quartz window,
114 causing a 7-day data gap, and mercury lamp intensity declined at -10°C , leading to two failed
115 calibrations.

116 The Antarctic inland plateau faces unique challenges including ultra-low temperatures (below
117 -40°C), polar night (over 3 months without effective illumination), and extremely low logistical
118 accessibility. Existing global unattended monitoring schemes (such as solar-powered supply for
119 marine platforms, mains-powered calibration for terrestrial tall towers, and 3G communication for
120 farmland systems) cannot be directly adapted to this region. Therefore, developing a fully
121 automated greenhouse gases and surface ozone observation system tailored to the Antarctic inland
122 plateau, which fills the gap in unattended monitoring of the atmospheric background in the polar
123 inland, is of crucial significance for understanding the polar feedback of the global climate system.

124 Building on these experiences, a new system to monitor greenhouse gases and surface ozone was
125 developed in 2022/2023 and deployed at the Antarctic inland Taishan Station. The preliminary

126 system only operated for 3 days due to excessive power consumption: the temperature control
127 module accounted for 70% of the total power (peak 3 kW), which overloaded the power supply.
128 The power allocation was 2.1 kW for temperature control and 0.9 kW for
129 analysis/calibration/communication modules. As a result, an improved system named CRUX-1.0

130 (The name "CRUX" is inspired by constellation of Crux is one of the most prominent and easily

删除[Biao]: But it only lasts 3 days for its high requirement
on power consumption (The energy consumption of the
temperature control module accounts for 70%, 3 kW at the
peak.), which leads to overloading of the green power
generation device.

recognizable constellations in the southern hemisphere sky) was developed with 350 W power limitation and tested at Tulihe, China, during cold season (-20 to -40 °C). Then in February 2024, it was deployed at Taishan Station on the Antarctic ice sheet. This system successfully operated for one month before the power supply broke down, providing valuable data on the atmospheric composition in this extreme environment. Here in this paper, we will introduce the detailed design of the system and its performance in Antarctica.

2 Site Descriptions

Atmospheric CO₂ and O₃ observational data in this study were obtained from one self-developed unattended monitoring system and four WMO-certified long-term monitoring stations with mature observation networks. The authoritative sources and verification channels for 2024 observational data are specified as follows: CO₂ data were retrieved from the World Data Centre for Greenhouse Gases (WDCGG) of the World Meteorological Organization/Global Atmosphere Watch (WMO/GAW, <https://gaw.kishou.go.jp/data/>), while surface ozone data were derived from the European Database for Atmospheric Sounding (EBAS, <https://ebas-data.nilu.no/Pages/DataSetList.aspx>). All datasets were verified via the WMO/GAW quality control system to ensure cross-station consistency and comparability (Global Atmosphere Watch, [GAW], 2001).

2.1 Taishan Station

Taishan Station (72.01°S, 92.08°E; 2621 m a.s.l.) is located on the Antarctic ice sheet (Figure 1). It is situated on the high Antarctic Plateau, an area characterized by extreme environmental conditions. The station experiences strong katabatic winds and is positioned in a region with limited access to logistics and power resources, making it a challenging site for long-term atmospheric monitoring. The climate at Taishan Station is typical of the high Antarctic interior, where temperatures are consistently low throughout the year. The long-term data from September 2012 to July 2021 revealed an annual average air temperature of -35.4°C, with a relative humidity of 67%, an air pressure of 699 hPa, and an average wind speed of 10.9 m/s (Ding et al., 2022). The temperature exhibits significant seasonal variation, with a clear "coreless" winter, meaning that there is no distinct temperature minimum, which is common in the interior of Antarctica due to the unique seasonal sunlight patterns (Figure 2). Furthermore, temperature variability is much greater during the austral winter (2.46°C) than during the austral summer (1.67°C), reflecting the greater frequency of weather events and atmospheric disturbances during the colder months (Ding et al., 2020b; 2022).

删除[Biao]:

删除[Biao]: World Meteorological Organization

删除[Biao]: WMO

删除[Biao]: 18

删除[Biao]: ; Montzka et al., 2015; Platt & Lunder, 2024

删除[Biao]: a, b, c, d

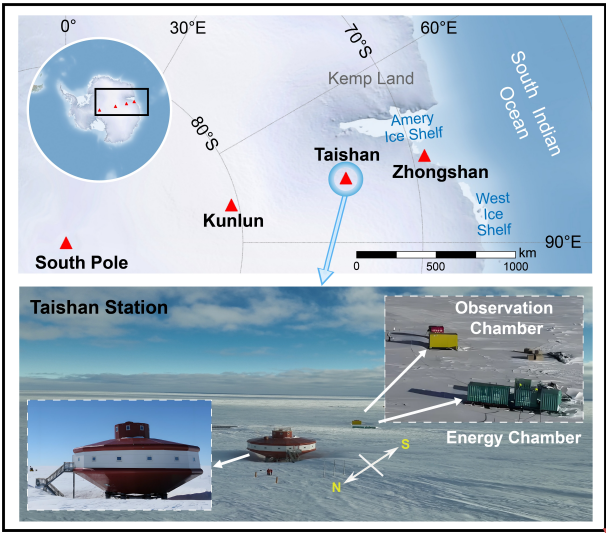


Fig. 1 Geographical distributions of Taishan station


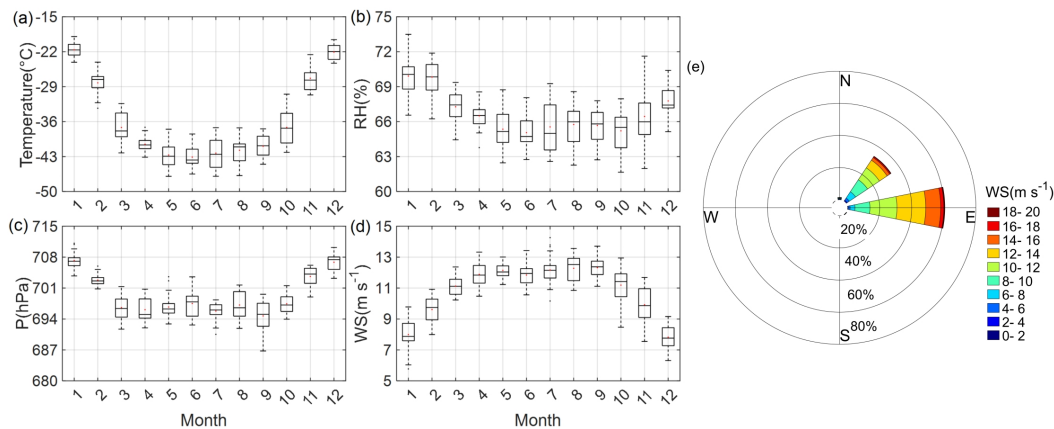


Fig. 2: Multiyear monthly average temperature (a), relative humidity (b), atmospheric pressure (c), wind speed, and wind direction (d, e) at Taishan Station.


The CRUX-1.0 fully automated unattended observation system was deployed at Taishan Station from February 10 to March 9, 2024. This system has achieved simultaneous monitoring of CO₂ and O₃ and obtained continuous observation data. Specifically, the CRUX-1.0 system is installed in a yellow observation cabin, which is located approximately 100 meters to the southeast of the green-colored unattended generator cabin (Figure 1). Given that easterly winds prevail at Taishan Station, the air inlet of the observation cabin is positioned on the upwind side of the generator cabin, which effectively minimizes the potential interference of the monitoring results from the exhaust emissions of the generator cabin. Detailed technical parameters and operational mechanisms of this system will be elaborated in Section 3.

2.2 Other Observation Stations

This study adopts four representative Global Atmosphere Watch (GAW) background stations covering polar, mid-latitude coastal and alpine regions for atmospheric comparative analysis. The Amundsen-Scott South Pole Station (SPO; 90°S, 24.8°W; 2837 m a.s.l.) is a NOAA-operated Antarctic background station, performing hourly in-situ CO₂ and O₃ observations with biweekly flask sampling and weekly NOAA-2016 scale calibration (Mahesh et al., 2003). It maintains a 98.8% data continuity rate and provides benchmark Antarctic atmospheric background data (Prinn

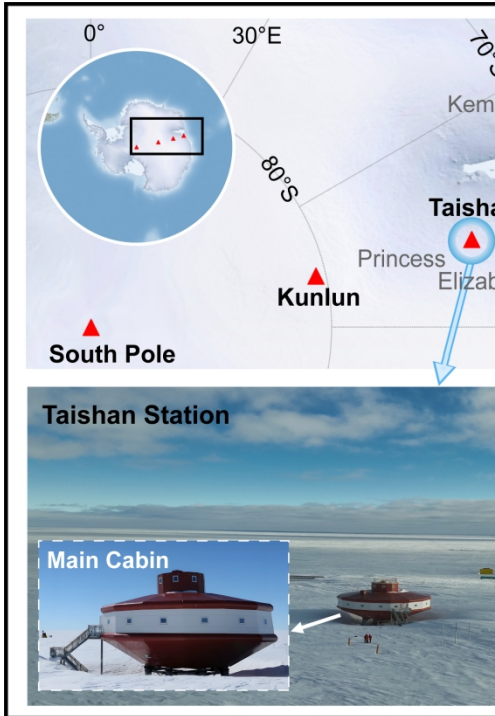

删除[Biao]:

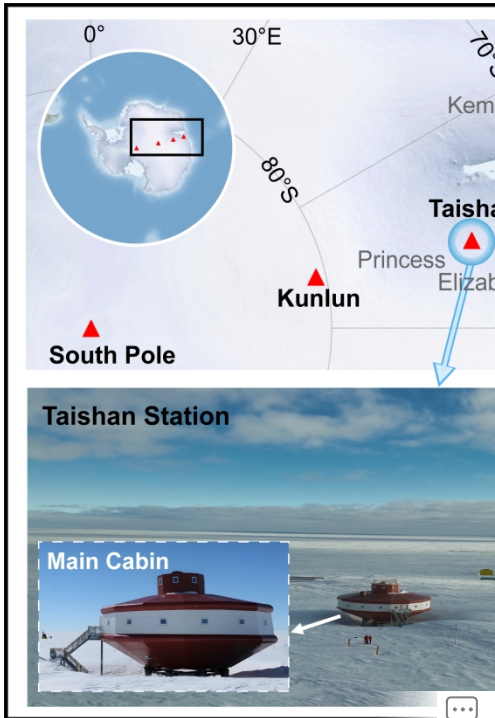

删除[Biao]:

et al., 2018). Barrow Station (BRW; 71.32°N, 156.61°W; 11 m a.s.l.), a key NOAA GMCC Arctic coastal station, conducts hourly CO₂ and O₃ monitoring and biweekly flask cross-validation. Influenced by North American emissions and Arctic atmospheric circulation, BRW captures both pristine Arctic background air masses and regional pollution episodes, with all data standardized to 10-min intervals via NOAA quality control protocols (Heintzenberg, 1989). The long-term NOAA-operated Mauna Loa Station (MLO; 19.54°N, 155.58°W; 3397 m a.s.l.), established in 1958, hosts the world's longest continuous greenhouse gas observation records. It implements hourly WMO GAW-calibrated CO₂ and O₃ monitoring and daily flask sampling, and its remote marine location minimizes anthropogenic interference to ensure reliable mid-latitude baseline observations (Keeling et al., 1976). As a high-altitude alpine background station under the ACTRIS network, Jungfraujoch Station (JFJ; 46.54°N, 7.96°E; 3580 m a.s.l.) monitors CO₂ and O₃ at 6-min intervals, with weekly flask sampling and monthly systematic calibration, effectively reflecting mid-latitude European atmospheric trace gas variations (Kubistin et al., 2014). The station maintains a long-term data completeness of approximately 92% under routine quality assurance (Sturm et al., 2012). Notably, systematic biases between NOAA and ACTRIS datasets are less than 1% for CO₂ and 3% for O₃, which are sufficiently small to be negligible for regional and global comparative analyses (Prinn et al., 2018).

3. Design of the observation system

The preliminary version of the unmanned automatic observation system, CRUX-1.0, is designed with 4 main modules: a sampling and calibration module, an analysis module, a temperature control module and a data communication module.

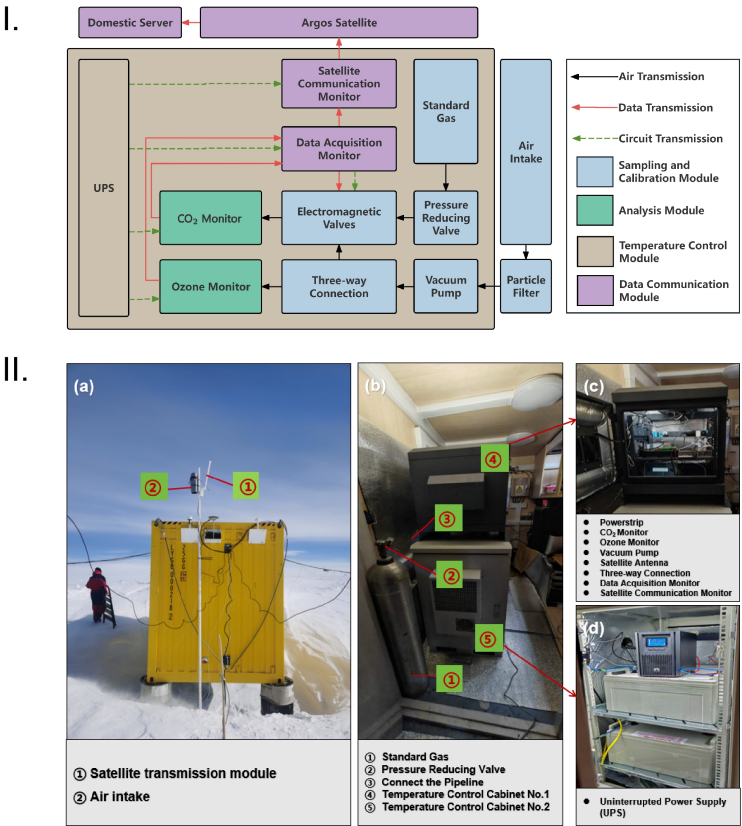


Fig. 3 Functional and structural layout (I) and onsite installation and layout (II) of the unmanned automated CO₂ and surface ozone observation system at Taishan Station

删除[Biao]: 2.2.1 South Pole Station

Amundsen-Scott South Pole Station (SPO; 90°S, 24.8°W; 2837 m a.s.l.) is a manned baseline station located at the geographic South Pole, representing the coastal-inland transitional atmospheric conditions of Antarctica. Atmospheric CO₂ and O₃ are monitored using in-situ GC-MS and UV spectrometers with a 1-h sampling frequency, operated by the NOAA Global Monitoring Laboratory. Air samples are collected biweekly in paired glass flasks for offline verification, with weekly automatic calibration against NOAA-2016 standard scales (Montzka et al., 2015; Mahesh et al., 2003). The station's data continuity rate is 98.8%, and its observations are widely recognized as a benchmark for Antarctic coastal atmospheric background (Prinn et al., 2018).

2.2.2 Barrow Station

Barrow Station (BRW; 71.32°N, 156.61°W; 11 m a.s.l.), operated by NOAA's GMCC program, is a key Arctic coastal background station. The station monitors CO₂ and O₃ with NDIR analyzers and UV spectrometers at a 1-h temporal resolution, with additional flask sampling every 2 weeks for cross-validation. Affected by North American regional emissions and Arctic atmospheric circulation, BRW captures both baseline Arctic air masses and episodic pollution transport events (e.g., Eurasian arctic haze; Bodhaine et al., 1981). Data from BRW were averaged to 10-min intervals, with QC procedures following NOAA's standard protocols (Dutton et al., 2002).

2.2.3 Mauna Loa Station

Mauna Loa Station (MLO; 19.54°N, 155.58°W; 3397 m a.s.l.) is a global benchmark mid-latitude marine background station, operated by NOAA since 1958. Its CO₂ observations provide the longest continuous record of atmospheric greenhouse gas concentrations worldwide, with measurements conducted via hourly NDIR analysis and daily flask sampling. O₃ is monitored using UV absorption sensors with 1-h resolution, calibrated against WMO GAW standards. The station's remote location on the Hawaiian volcanic summit, dominated by westerly winds from the Pacific Ocean, minimizes local anthropogenic interference, making it ideal for capturing mid-latitude baseline atmospheric conditions (Keeling et al., 1976).

2.2.4 Jungfraujoch Station

Jungfraujoch Station (JFJ; 46.54°N, 7.96°E; 3580 m a.s.l.) is a high-altitude mid-latitude alpine background station in the Swiss Alps, managed by the ACTRIS network. It conducts in-situ monitoring of CO₂ (via Maihak broad-band infrared analyzers) and O₃ (via UV spectrometers) with a 6-min averaging frequency, supplemented by weekly flask sampling. The station is sensitive to European regional atmospheric circulation and photochemical activity, capturing distinct diurnal and seasonal fluctuations in trace gas concentrations (Kubistin et al., 2014). Data consistency is maintained through monthly cross-calibration with reference gas mixtures, with a

3.1 Sampling and Calibration Module

3.1.1 Sampling

The sampling module is responsible for collecting atmospheric gas samples and ensuring their consistent flow into the analysis module for evaluation (see Figure 3-I). It consists of several key components that work together to maintain a stable and reliable system. The intake port, positioned at a height of 2.9 m (see Figure 3-II-a), ensures that the air samples are representative of the surrounding atmosphere and not influenced by local pollutants or snow. Furthermore, the inlet is installed with a Thermo-5030i pre-filter matched with a 47 mm-diameter, 5.0 μm MILLIPORE PTFE membrane filter. This filter can efficiently block blown snow particles and coarse dust, effectively avoiding pipeline clogging induced by frequent blowing snow in Antarctica and enhancing the environmental suitability of the sampling setup. This elevated position and filter are crucial for ensuring that the collected data are as accurate as possible.

删除[Biao]: The intake port is also equipped with a particle filter to prevent the intake of snowflakes, dust, and other large particles that could contaminate the samples.

The gas flow controller, which includes a vacuum pump (Kamoer KZP-PE model: low rate ≥ 7 L/min; power ≤ 12 W; positive pressure ≥ 0.2 MPa), standard gas cylinder pressure-reducing valve, and flow controller, ensures that the gas is drawn into the system at a constant rate (see Figure 3-II-b,c). The vacuum pump helps maintain a positive pressure airflow, whereas the flow controller regulates the gas flow for consistent sampling. Additionally, the system incorporates three-way and electromagnetic valves to allow the sampling system to switch between different sampling points or introduce calibration gases as needed. The overall design of the sampling module considers the dominant wind direction at Taishan Station, with the intake positioned in the upwind direction of the energy bin to minimize contamination from emissions. This thoughtful design ensures that the sampling module operates efficiently, even in harsh Antarctic environments.

3.1.2 Calibration

The calibration module is designed to eliminate instrument drift through standard gas calibration, ensuring the accuracy and stability of the observation data. The standard gas cylinder pressure-reducing valve controls the output pressure of the standard air, with the secondary gauge set to 2 psi. This setting ensures that the instrument's intake pressure is met while conserving the standard air as much as possible, thereby extending its usage duration. Each standard gas cylinder is certified for high precision and traceability and is equipped with a single-stage pressure-reducing valve. The cylinders are connected to the electromagnetic valve via 1/8-inch stainless steel tubing, ensuring the stability of the gas concentrations during transmission.

删除[Biao]: 1

The electromagnetic valve is powered and controlled by the CR1000 data logger, which operates the valve at scheduled intervals through a prewritten control program. This program switches between external air and standard air intake, ensuring a consistent and controlled flow. To maintain a constant airflow through the instrument, a flow controller is installed downstream of the electromagnetic valve, preset to a constant flow rate. This ensures precise control over the gas flow entering the monitoring sensors, improving the accuracy of the measurements.

To prevent instrument drift from affecting the observation data, the system incorporates a standard gas calibration system, following the atmospheric background observation guidelines. The data logger sends instructions to the electromagnetic valve to allow standard air to flow into the system twice daily—every 11 hours and 10 minutes for a 10-minute period. This calibration process ensures that the sensor is calibrated and that any drift is corrected while considering the limitations of energy consumption and the unmanned operating conditions at Taishan Station.

删除[Biao]: twice daily—every 11 hours for a 5-minute period

3.2 Analysis Module

3.2.1 CO₂ Monitor

To meet the energy consumption requirements at Taishan Station (where the atmospheric composition monitoring system needs to maintain a power consumption of less than 0.5 kW), a low-power LICOR-830 CO₂ analyzer (see Figure 3-II-c) is used in this experimental system. This device operates via the nondispersive infrared (NDIR) method, which consumes approximately 20 W of power. The NDIR method is considered one of the simplest yet effective technologies for gas detection because of its moderate sensitivity and fast response time. The LICOR-830 is widely used in various research fields, including agronomy, ecology, global carbon cycling, and climate change studies (Griffiths, 1983; Ekeberg, 2004; Chen et al., 2010).

The core components of the analyzer include an infrared light source, a light chamber, filters, and a detector. The working principle is as follows: infrared radiation emitted by the light source passes through the target gas in the light chamber. If the spectrum of the radiation overlaps with the absorption spectrum of the target gas, the gas absorbs photons at specific wavelengths according to the Beer–Lambert law (Kwon et al., 2009). After passing through the gas, the infrared radiation is filtered so that only the wavelengths absorbed by the gas are retained. These specific photons, which contain concentration information, are detected by the sensor, and the signal is processed to display the concentration of the greenhouse gas (Xu et al., 2022).

Prior to deployment at Taishan Station, a preexpedition laboratory experiment was conducted to quantify the precision differences between the LICOR-830 and the Picarro G2301 greenhouse gas analyzers. This experiment aimed to assess the performance of observation systems based on different principles for measuring greenhouse gases (Nan et al., 2024). Through repeatability tests, drift tests, and target gas calibration tests, it was found that the accuracy of the LICOR-830, after calibration, met the WMO requirement of less than 0.1 ppm and was comparable to the advanced international accuracy level of the Picarro G2301, demonstrating its significant application potential in greenhouse gas monitoring.

3.2.2 Ozone Monitor

For ozone monitoring, a Model 205 ozone monitor from 2B Technologies (see Figure 3-II-c) was used in this experiment. This model was previously deployed in a year-long ground-based ozone observation experiment at Kunlun Station in Antarctica in 2016, where it successfully collected comprehensive observational data (Ding et al., 2022). Model 205 has demonstrated excellent applicability in ozone concentration monitoring, both domestically and internationally. It is energy efficient, highly accurate, compact, and lightweight, making it an ideal tool for monitoring atmospheric ozone concentrations in outdoor or field environments (Ollison et al., 2013; DiGangi et al., 2018; Tian et al., 2022).

The Model 205 ozone monitor operates via ultraviolet photometry (Williams et al., 2006). The ozone concentration was measured by detecting its maximum absorption at a UV wavelength of 253.7 nm. When an air sample enters the instrument's gas flow system at a constant flow rate, two electromagnetic valves alternate in directing the sample either into the absorption chamber or through an ozone filter before entering the absorption chamber. The absorption chamber concentrates stable UV light produced by the UV light source. Owing to the absorption characteristics of ozone at 254 nm, the intensity of transmitted light as the gas passes through the chamber is detected, providing accurate and stable measurements of the ozone concentration. Instruments based on this method are widely used in pollution monitoring, including atmospheric

and water pollution (Tanimoto et al., 2006). Calibration of the ozone monitor requires an ozone calibration instrument that meets international traceability standards. Therefore, cross-concentration calibrations are performed every three months according to observation protocols. However, the calibration procedures for Antarctic ice sheet instruments differ from those at manned stations. For instance, in 2011, after the BAS team retrieved all instruments from the observation network to Halley Station, they validated them using the newly calibrated TE-Model 49C. Upon returning to Cambridge, the instruments were re-calibrated using the NPL-certified TE-Model 49iPS, confirming that the calibration parameters of the 10 instruments remained stable throughout the year's deployment, with data deviations not exceeding the initial accuracy range of 2% (Bauguitte et al., 2011). In 2016, testing at Antarctic Dome A confirmed the stable operation of the instrument in the field, and reliable observations can be obtained by conducting calibrations twice per year (Ding et al., 2020a). Owing to the overall energy consumption limitations and unattended conditions at Taishan Station, we conducted calibrations before deployment and after retrieval. This strategy could sufficient for the one-month experiment, because the 2B Model 205 monitor features ultra-low intrinsic drift (<3 ppb/year for baseline drift, <3%/year for sensitivity drift). The drift over one month was verified to be <2% in laboratory tests and Antarctic field applications (Wang et al., 2017), meeting the WMO/GAW accuracy requirement.

3.3 Temperature Control Module

The temperature control module is designed to ensure the stable operation of the monitoring equipment under extreme Antarctic conditions, especially the freezing temperatures at Taishan Station. This module includes a temperature control cabinet, a gas flow controller, and an uninterruptible power supply (UPS) (see Figure 3-II-b-④, ⑤). The temperature control cabinet is equipped with precise sensors and adjustment mechanisms that maintain a stable internal temperature range for the equipment, protecting it from extreme cold at the station.

To meet the appropriate temperature range for the operation of CO₂ and ozone monitoring while reducing the energy consumption of temperature control, the temperature control accuracy is ±1.0 °C, and the heating response time is 5 minutes, and the minimum heating temperature of the temperature control cabinet is preset to 10°C. When the internal temperature drops below 10°C, the system begins to heat; when the temperature exceeds 15°C, heating stops, ensuring that the equipment remains within a safe and optimal operating temperature range. This design ensures that the monitoring instruments are effectively protected in the extremely low-temperature environment of Taishan Station (which can reach as low as -40°C). The environmental monitoring and control system, which includes temperature regulation, is the highest power-consuming component in the entire system, with a peak power consumption of 250 W. Given the power constraints at Taishan Station, energy efficiency is a crucial consideration in the design of the temperature control system. This is balanced with the need to maintain a stable environment for the equipment.

Since the experimental system is powered by Taishan Station's external energy cabin, an uninterruptible power supply (UPS) system is installed to prevent sudden power outages or voltage instability from negatively impacting the system's operation (Figure 3-II-d). The UPS provides stable and reliable power to the entire monitoring system (see Figure 3-II-d). In the event of an external power failure, the UPS can quickly switch to backup power. The battery backup can last up to 48 hours, ensuring the continuous operation of the monitoring system and uninterrupted

删除[Biao]: ,

删除[Biao]:

data collection. This design significantly enhances the system's reliability and fault tolerance, providing a safeguard against power disruptions in the remote environment.

3.4 Data Communication Module

The satellite communication system consists of a customized bracket (with a height of 3 m) and an integrated transmitting antenna (Figure 3-II-a-①), enabling high-speed and stable data transmission to a remote data center. This module uses ARGOS (full system: Argos Data Collection System, named after the all-seeing giant Argus from Greek mythology) satellite communication technology, with a data transmission interval of 1 hour, ensuring the real-time transmission of monitored data processed by the data logger in the harsh Antarctic environment, which can avoid potential interruptions and delays that could arise with traditional ground communication methods. The stable applicability of this satellite communication module in Antarctica has been verified through testing at the Prydz Bay-Amery Ice Shelf-Dome A (PANDA) profile automatic weather station (Ding et al., 2022).

删除[Biao]: uses ARGOS satellite communication technology

The data processing and storage system uses the CR1000X measurement and control data logger (see Figure 3-II-c), a low-power device primarily used for sensor measurements, direct/remote communication connections, data analysis, external device control, and storage of data and programs. It features a sealed design to shield against radio frequency interference and a stainless steel housing. Equipped with a precise clock, it supports the BASIC-like programming language commonly used by Campbell Scientific data loggers, which includes data processing and analysis capabilities.

The CR1000X connection panel has two 12 V terminals, 16 analog measurement terminals, and detachable connectors. It is responsible for receiving raw data from two monitoring sensors, performing preprocessing, analysis, and storage. This module has powerful data processing capabilities, enabling it to filter out and correct anomalous data points in real time, ensuring the reliability of the data quality. Additionally, the module supports remote data access and download functions, allowing researchers to retrieve and analyze monitoring data at any time.

4. Experimental analysis

4.1 Observational results

From February 10 to March 12, 2024, the observation system at Taishan Station operated autonomously under unattended low-temperature conditions, with good performance, and satellite remote data transmission was normal. By analyzing the transmitted data, we found the following: in the environment at Taishan Station, where the average temperature was below -25°C in February, the internal temperature of the equipment cabinet was able to be stably maintained at $13.9 \pm 2.5^{\circ}\text{C}$ (Figure 4a), meeting the environmental temperature requirements for both types of optical cavity equipment used in this experiment.


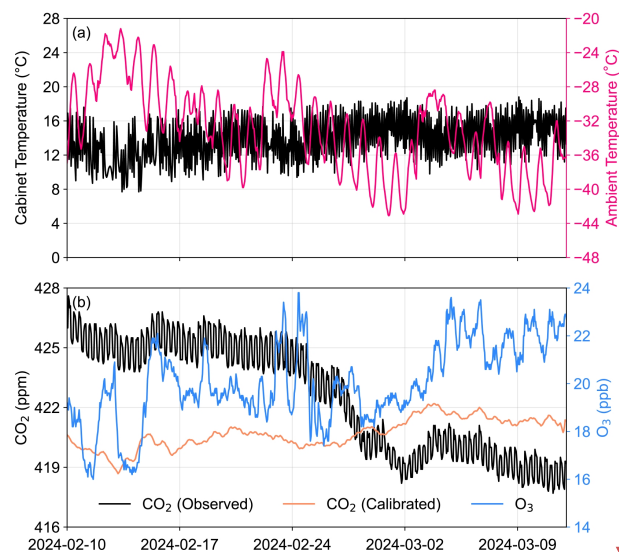


Fig. 4 Compares synchronous in-cabinet temperature (black, left axis) and outdoor ambient temperature (pink, right axis), (a), hourly average concentration of observed CO₂, hourly average concentration of calibrated CO₂ and O₃ concentration transmitted from the unattended automated observation system at Taishan Station (b).

The hourly average CO₂ concentration observed at Taishan Station was 422.6 ± 2.8 ppm (Figure 4b). To ensure the accuracy of observational data, we first analyzed concurrent meteorological parameters including wind speed and wind direction, and verified that generator exhaust exerted no direct interference on the monitoring data (Fig. S1, Supplementary Material). To constrain instrumental drift under unattended field conditions, the system executes an automatic 10-minute standard gas calibration every 11 hours; this customized calibration interval comprehensively balances drift correction efficiency, limited on-site power supply and automatic operation requirements. All CO₂ raw datasets underwent standardized multi-step QA/QC procedures sequentially: exhaust interference exclusion based on sampling layout and field wind rose statistics, wind-speed-dependent pollution screening, quantitative concentration calibration, and final 48-hour moving average smoothing for noise reduction. The daily-averaged calibrated CO₂ concentration was determined as 420.7 ± 0.7 ppm. The ozone raw datasets were calibrated using the five-point cross-concentration formula ($y = 0.994 * x - 0.495$, $R^2 = 0.9998$). This calibration function was established in laboratory before instrument shipment via systematic calibration on the Model 205 ozone analyzer with a Thermo 49ips standard ozone calibrator. Upon completion of the QA/QC procedures, the daily-averaged calibrated surface ozone concentration at Taishan Station was 20.1 ± 0.8 ppb. Full technical details of each QA/QC step are provided in Supplementary Material.

4.2 Accuracy evaluation

We evaluated system performance using WMO/GAW required indicators: CO₂ (zero drift ≤ 0.1 ppm/month, span drift $\leq 0.2\%$ FS, accuracy ± 1.5 ppm); O₃ (zero drift ≤ 0.5 ppb/month, span drift $\leq 1\%$ FS, accuracy ± 0.8 ppb), plus standard deviation and coefficient of variation (CV) (Global Atmosphere Watch [GAW], 2001). The standard deviation provides insight into the dispersion of measurement data, reflecting the precision and stability of the system. On the other hand, CV, which normalizes the standard deviation by the mean value, allows for a comparison of variability across different parameters and conditions, regardless of their magnitude. Using these two metrics,

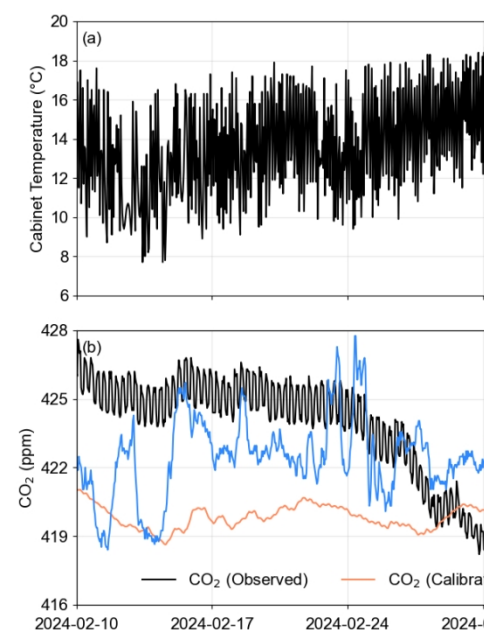

删除[Biao]:

删除[Biao]: Cabinet temperature

删除[Biao]:

删除[Biao]: From February 10 to March 12, 2024, the hourly average concentration of observed CO₂ at Taishan Station was 422.6 ± 2.8 ppm (Figure 4b). To ensure the accuracy of the observation data, the system automatically introduces standard gas every 11 hours for 10 minutes to correct the instrument measurement deviation. After data quality control, the daily average concentration of calibrated CO₂ at Taishan Station was 420.3 ± 1.5 ppm.

删除[Biao]: To assess the overall performance and stability of the system, we employed the standard deviation and coefficient of variation (CV) as key metrics.

we evaluated the precision of O₃ and CO₂ concentrations, as well as the cabinet temperature, over time.

Prior to the Antarctic field campaign, we had been completed laboratory performance intercomparison between the LICOR-830 analyzer used in this work and Picarro G2301 by means of repeatability, long-term drift and three-point cross-concentration calibration with traceable CO₂ standard gases, with related test plots (Figures S2 to S5) attached in supplementary files. The test results indicated that LICOR-830 had a repeatability of 0.4 ppm versus 0.04 ppm for Picarro G2301, alongside drift biases of -4.22 % and 0.82 % respectively; after three-concentration standard gas calibration for 1 h, LICOR-830's precision was markedly optimized to 0.026 ppm (bias: -0.11 %), while Picarro G2301's precision changed slightly to 0.0341 ppm with an accuracy of 0.03 %.

In addition, for the ozone measurement module equipped with a 2B Model 205 dual-beam UV analyzer, multi-point calibration conducted before and after field deployment meets the data quality requirement for one-year Antarctic observation ((Bauguitte et al., 2011; Ding et al., 2020a). The laboratory comparison test (Figures S6) between Model 205 and WMO reference Thermo Model 49i proved excellent measurement consistency ($R^2=0.9998$), with most absolute deviations below 4 ppb, and regular concentration-dependent bias can be fully corrected by linear fitting using pre- and post-campaign calibration results. Laboratory aging experiments demonstrate the intrinsic monthly zero drift of Model 205 is less than 0.6 ppb; after adding extra thermal drift from periodic cabinet temperature fluctuation, the total monthly drift remains below 0.7 ppb, within the WMO/GAW allowed total uncertainty of ± 0.8 ppb for O₃.


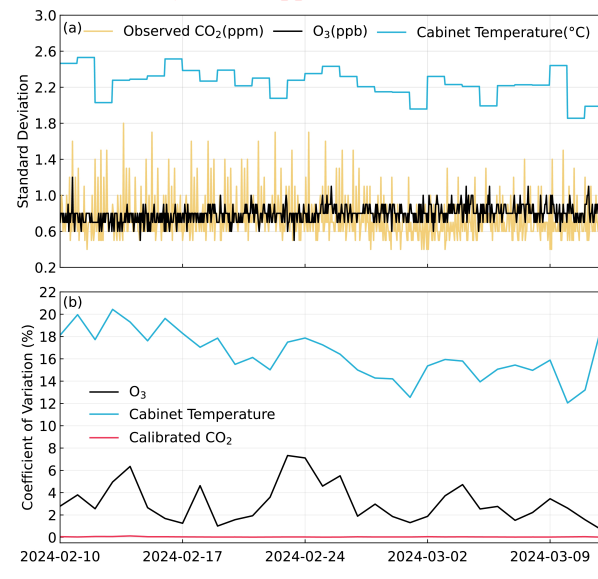


Fig. 5 Evaluation of the Precision of O₃ and CO₂ Concentrations and Cabinet Temperatures through Standard Deviation and Coefficient of Variation Analysis Standard Deviation (a) Coefficient of Variation (b)

The O₃ concentration (black line) consistently has a low standard deviation and minimal fluctuations, indicating high measurement stability. In contrast, the original CO₂ concentration (yellow line) displays substantial variation, with a peak standard deviation of 1.8, suggesting lower precision (Figure 5a). The cabinet temperature (blue line) maintains a stable standard deviation, although a stepwise decrease over time suggests some control, albeit with potential for further improvement. In terms of the CV, the O₃ concentration remains low (<6%) and continues

删除[Biao]:

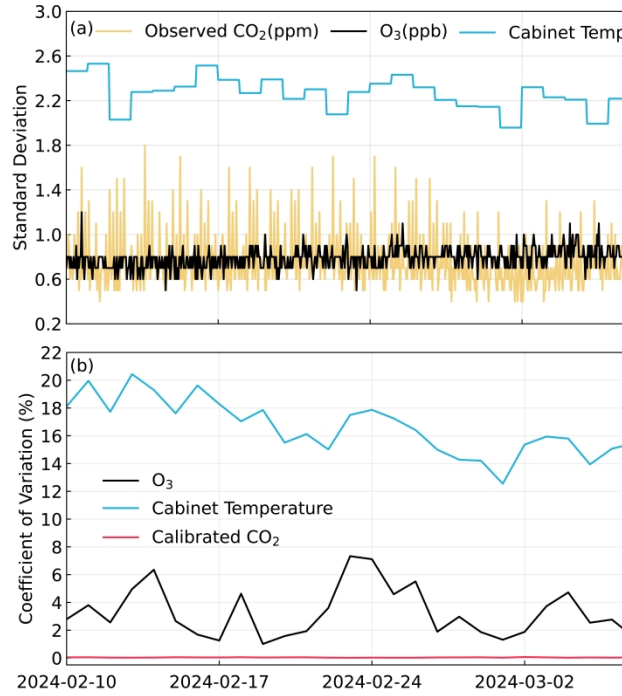

to decrease over time, reflecting enhanced measurement consistency. As illustrated in Figure 4, the ambient surface temperature at Taishan Station fluctuates widely between −45.0 °C and −20.5 °C with prominent diurnal cycles, whereas the active thermal cabinet limits internal instrument temperature within 8.0–19.0 °C with a CV of 16%–20% (± 2.5 °C fluctuation). Comparative time-series analysis of CO₂ and O₃ in Figure 4b confirms that such cabinet temperature variation only yields tiny measurement drift (≤ 0.2 ppm/h for CO₂, ≤ 0.1 ppb/h for O₃), with no significant impact on measurement results (Figure 5b). Postcalibration, the CO₂ concentration (red line) significantly decreases in CV, approaching 0%, demonstrating the effectiveness of calibration in improving measurement accuracy.

删除[Biao]: Postcalibration, the CO₂ concentration (red line) significantly decreases in CV, approaching 0%, demonstrating the effectiveness of calibration in improving measurement accuracy. However, the cabinet temperature shows a higher CV (~16%-20%), indicating notable fluctuations, possibly due to environmental factors or temperature control system design (Figure 5b).

5. Discussion

5.1 Performance Comparison

Traditional manned stations (e.g., South Pole Station) have irreplaceable advantages: real-time troubleshooting, flexible parameter adjustment, and weekly on-site calibration (measurement uncertainty <0.5 ppm, better than CRUX's ± 1.0 ppm for CO₂). However, manned observations face high logistics costs and data gaps due to extreme weather evacuations. CRUX compensates for these shortcomings: its 30-day autonomous operation cuts logistics costs by over 90%, and 48-hour UPS backup ensures data continuity during power outages. The consistency of its results with South Pole Station (CO₂: 420.7 ppm vs. 418.2 ppm; O₃: 20.1 ppb vs. 20.5 ppb) confirms it can provide comparable data quality in stable environments, serving as an effective supplement to manned observations.

删除[Biao]: Overall, while O₃ concentration measurements demonstrate high precision and stability, CO₂ concentration precision improves substantially with calibration. Temperature control remains stable but requires optimization to reduce variability and further improve measurement accuracy.

Table 1. Comparison of the Polar Automatic GHG or Ozone Observation Systems

Key Techniques	CRUX-1.0 (2024)	BAS Ozone Network (2011)	Kunlun Station Ozone Monitor (2016)
Monitoring Parameters	CO ₂ / O ₃	O ₃	O ₃
Power Consumption	<350 W	11–13 W	5 W
Temperature Control Method	Auto-temperature control (10–15°C)	Passive Insulation with intake heater	Passive Insulation
Calibration Method	CO ₂ : Automatic (Single standard gas mode, twice daily); O ₃ : Periodic calibration	On-site zero-check with manual intervention and Periodic calibration	Periodic calibration
Single Battery Backup Duration	48 hours (UPS Backup Battery)	10–14 days (Lead-Acid Batteries)	Not applicable

删除[Biao]: 3 $\pm$ 1.5

删除[Biao]: ± 0.8

删除[Biao]: 2

Data Continuity Rate	99.2%	85% (Affected by power/communica tion)	99.5%
-------------------------	-------	--	-------

458 As shown in Table 1, CRUX's strengths lie in integrated optimization for Antarctic inland
 459 conditions: (1) Balanced performance: It reduces power consumption by 92% compared to the
 460 initial 3 kW version, achieving <350 W operation while maintaining multi-parameter detection,
 461 adapting to polar green energy constraints. (2) Extreme cold reliability: Active temperature control
 462 isolates -25°C to -40°C external temperatures, and upwind intake with particle filters mitigates
 463 blowing snow interference. (3) High autonomy and accuracy: Twice-daily auto-calibration reduces
 464 CO₂ CV to near 0%. Field tests revealed minor limitation flaws: (1) Temperature control lag: A
 465 5-minute heating response delay leads to 16%–20% cabinet temperature CV, potentially causing
 466 0.2 ppm/h drift of the LICOR-830 analyzer. (2) Insufficient long-term power: 48-hour UPS
 467 backup. (3) Limited adaptability: Fixed-time calibration cannot respond to sudden sensor drift;
 468 only two parameters are monitored.

469 **5.2 Site Comparison**

470 To verify the global representativeness of measurements from CRUX-1.0 at Taishan Station,
 471 quantify the regional differences in atmospheric CO₂ and O₃ between polar and mid-latitude
 472 background regions, and validate the reliability of the unattended observation system, a
 473 comparative analysis was conducted on concurrent CO₂ and O₃ datasets from five global
 474 atmospheric background stations, which differ in geographical locations (polar vs. mid-latitude)
 475 and operational modes (unattended vs. manned). The selected stations include Taishan Station
 476 (Antarctic inland, unattended), South Pole Station (Antarctic coastal, manned), Barrow Station
 477 (Arctic coastal, manned), Mauna Loa Station (mid-latitude marine, manned), and Jungfraujoch
 478 Station (mid-latitude alpine, manned) (Figure 6a).

删除[Biao]: 2

删除[Biao]: non-negligible

删除[Biao]: To interpret the observational results from Antarctic Taishan Station in a global context and assess the performance of the CRUX-1.0 unattended system,

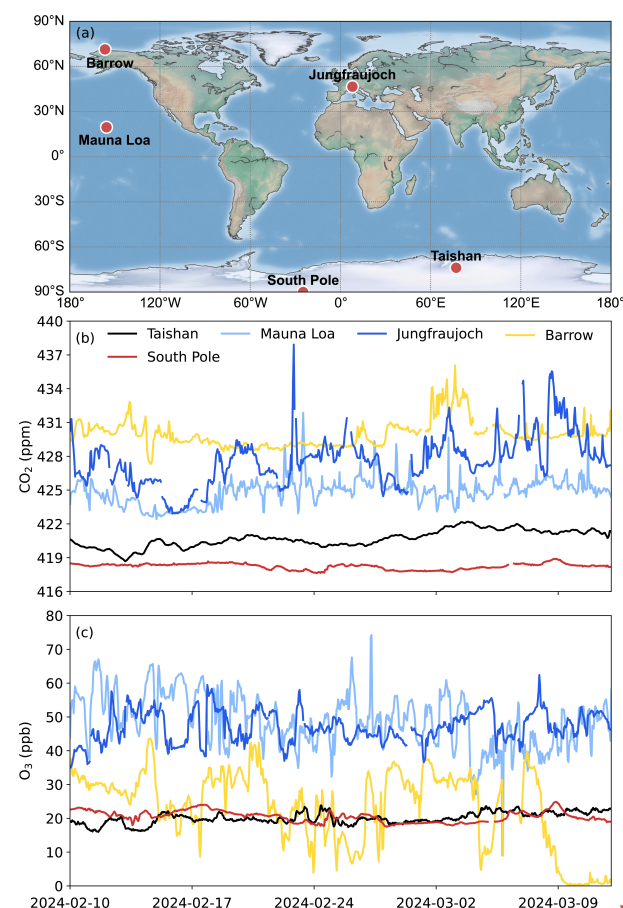


Fig. 6 (a) Global distribution of selected atmospheric background stations; (b) time series of hourly CO₂ concentrations and (c) time series of hourly surface O₃ concentrations observed at these stations during the concurrent period (10 February – 12 March 2024). This figure aims to validate the reliability and global representativeness of CRUX-1.0 measurements at Antarctic Taishan Station, reveal the distinct regional differences in atmospheric CO₂ and O₃ between polar and mid-latitude background regions, and confirm the role of the unattended system in complementing the global atmospheric observation network.

Comparative results revealed distinct regional and operational differences in both CO₂ and O₃ observations. For CO₂, polar stations (Taishan and South Pole; mean: 420.7 and 418.2 ppm; hereafter means) exhibited significantly lower baseline concentrations than mid-latitude counterparts (Mauna Loa: 424.9 ppm; Jungfraujoch: 427.6 ppm), primarily due to the absence of anthropogenic emissions in the Antarctic inland. Taishan Station also showed smaller fluctuation amplitude (± 1.5 ppm), attributed to the homogeneous air masses in the Antarctic inland circulation and interference-free operation of the unattended system, whereas mid-latitude stations displayed larger fluctuations driven by regional emission transport and diurnal cycles. For O₃, polar stations (Taishan: 20.1 ppb; South Pole: 20.5 ppb) had much lower concentrations than mid-latitude stations (Mauna Loa: 48.9 ppb; Jungfraujoch: 47.1 ppb), which was associated with weak photochemical activity in the Antarctic late summer., which was associated with the low concentrations of ozone precursors in Antarctica (due to the dual scarcity of natural and anthropogenic sources) impair the ozone formation potential, while the intense sunlight in summer, chemical depletion triggered by trace amounts of NO, and stable boundary layer conditions jointly lead to surface ozone in Antarctica being dominated by depletion during summer (Tian et al.,

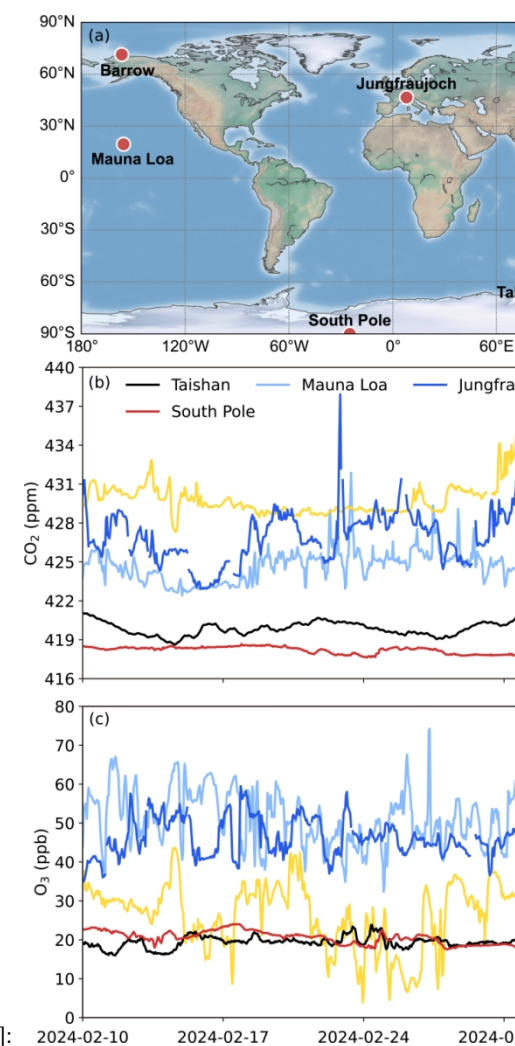


Fig. 6 Global distribution of selected atmospheric background stations (a) and their concurrent CO₂ (b) and O₃ (c) observations (2024-02-10 to 2024-03-12)

删除[Biao]: 2

2022).

5.3 Long-term deployment challenges

The one-month CRUX-1.0 deployment was designed as a proof-of-concept campaign, which has successfully validated system robustness under extreme low temperatures, core measurement performance, and full autonomous operation with satellite data transmission, fulfilling all predefined objectives. We agree that extended deployments are essential to fully characterize long-term reliability in the harsh Antarctic interior, and we are conducting iterative upgrades of the CRUX-2.0 system to address two key bottlenecks: energy supply and long-term data quality assurance.

For energy supply, CRUX-1.0 currently relies on Taishan Station’s diesel power infrastructure, which is limited by seasonal manual fuel replenishment. The upgraded CRUX-2.0 will adopt a standalone photovoltaic-battery-methanol hybrid power system with an intelligent energy management system to dynamically dispatch power sources. This self-contained design eliminates dependence on external station power and frequent on-site refueling, targeting a minimum of three months of uninterrupted unattended operation.

For long-term measurement accuracy, the single-point calibration of CRUX-1.0 is sufficient for short campaigns but has limited drift correction capacity over multi-month deployments. CRUX-2.0 integrates the ABB GLA131-GGA analyzer with a multi-channel solenoid valve manifold, enabling autonomous scheduled multi-concentration standard gas calibration to maintain GAW-compliant data accuracy throughout extended operation.

Currently, the integrated CRUX-2.0 prototype is undergoing field validation at Saishiteng Mountain (Qinghai), a high-altitude cold test site, with completion scheduled for July 2026 (Figure S7 to S10, Supplementary Material).

6. Summary

To explore a new unattended observation model suitable for monitoring greenhouse gases (GHG) and surface ozone (O₃) in the extreme environment of the Antarctic inland plateau, this study developed the CRUX-1.0 fully automated unattended observation system. Integrating four core modules—sampling and calibration, analysis, temperature control, and data communication—the system is specifically optimized for polar conditions, featuring key characteristics such as total power consumption below 350 W, active cabinet temperature regulation maintaining 10–15 °C, twice-daily automatic single-point calibration for CO₂, and a 48-hour UPS backup, making it well suited for remote sites with limited logistic support.

Deployed and operated continuously at Taishan Station (72.01°S, 92.08°E) from 10 February to 9 March 2024, the system achieved outstanding operational stability with a 99.2% data recovery rate. Observed calibrated CO₂ and O₃ concentrations (420.7±0.7 ppm and 20.1±0.8 ppb, respectively) show excellent consistency with synchronous reference measurements from South Pole Station; post-calibration CV values reach nearly 0% for CO₂ and below 5.6% for O₃, which validates the reliability of the CRUX-1.0 unattended observation framework under harsh Antarctic conditions. Compared with conventional manned observation platforms, CRUX-1.0 delivers equivalent measurement accuracy while cutting over 90% of routine logistic expenditure, offering a cost-effective supplementary solution to fill observational gaps within the global WMO/GAW polar monitoring network.

Nevertheless, CRUX-1.0 still has limitations that restrict long-term year-round deployment in polar regions: continuous PTC heating results in relatively high power consumption; only

删除[Biao]: Notably, the data continuity rate of Taishan Station (99.2%) was comparable to that of the manned South Pole Station (98.8%), verifying the reliability of the CRUX-1.0 system in extreme polar environments. While mid-latitude manned stations excel in real-time calibration

删除[Biao]: To explore a new unattended observation model suitable for monitoring greenhouse gases (GHG) and surface ozone (O₃) in the extreme environment of the Antarctic inland plateau, this study developed the CRUX-1.0 fully automated unattended observation system. Integrating four core

single-point automatic calibration is available, with limited capacity to constrain span drift over multi-month operation; no reserved hardware interfaces for expanding additional gas species; and the current energy configuration cannot sustain prolonged polar-night operation. Targeting these four prominent bottlenecks (temperature control optimization, long-duration power supply, multi-parameter synchronous measurement, and dynamic calibration), we will carry out with targeted improvements:

a. Temperature control and power consumption optimization: Building on heating scheme comparisons in this study, follow-up upgrades will test a combination of self-limiting heating tapes and aerogel thermal wrapping to implement intermittent intelligent temperature control, cutting continuous heating power demand without compromising the thermal stability of internal instruments.

b. Long-term energy supply improvement: Future deployments will adopt an optimized PV-battery-methanol hybrid power configuration to alleviate power shortage risks during multi-month polar nights.

c. Multi-parameter coordinated monitoring: The next-generation CRUX-2.0 platform reserves modular expansion interfaces to sequentially add CH₄, H₂O and other trace gas sensors, enabling synchronous multi-component atmospheric observation.

d. Dynamic automatic calibration upgrade: Following laboratory intercomparison between the ABB GLA131-GGA analyzer and the Picarro G4301, we have selected the ABB GLA131-GGA configuration; paired with multi-channel solenoid valves, this design supports automatic multi-point standard gas calibration.

The CRUX-2.0 prototype is under field validation at Saishiteng Mountain (Lenghu, Qinghai), with completion scheduled for July 2026 to further enhance the sustainability and performance of polar autonomous atmospheric monitoring.

Data availability

The in-situ CO₂ and surface ozone observation data collected at Taishan Station from 10 February to 12 March 2024 are archived and publicly available at the National Tibetan Plateau / Third Pole Environment Data Center (<https://doi.org/10.11888/Atmos.tpd.303486>). The reference CO₂ datasets for global background stations were retrieved from the World Data Centre for Greenhouse Gases (WDCGG) of WMO/GAW (<https://gaw.kishou.go.jp/data/>), and the surface ozone datasets were obtained from the European Database for Atmospheric Sounding (EBAS, <https://ebas-data.nilu.no/Pages/DataSetList.aspx>). Both public datasets are accessible in compliance with their respective official data policies.

Author contributions

Biao Tian was responsible for funding acquisition, field experiment, writing of the original draft, experimental design, and formal analysis. Minghu Ding was responsible for project administration, supervision, resources coordination, and review and editing. Kongju Zhu and Xu Yao were responsible for on-site field experiment. Yixi Zhao was responsible for formal analysis and data visualization. Wenqian Zhang was responsible for system software debugging and remote data acquisition. Diyi Yang, Weijun Sun, Yining Yu, Shoudong Zhao, Yige Cui, Chuanjin Li, Jie Tang, Cunde Xiao, Tong Zhu, and Renhe Zhang were responsible for review and editing.

删除[Biao]:

删除[Biao]: The in-situ observational datasets generated in this study, including the hourly raw and calibrated CO₂ and O₃ concentration data from the CRUX-1.0 system at Taishan Station, Antarctica, the system operation and temperature control records, and the data quality control results, are available from the corresponding author upon reasonable request.

Disclaimer

Publisher's note: Copernicus Publications remains neutral with regard to jurisdictional claims made in the text, published maps, institutional affiliations, or any other geographical representation in this paper. The authors bear the ultimate responsibility for providing appropriate place names. Views expressed in the text are those of the authors and do not necessarily reflect the views of the publisher.

Declaration of competing interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

Acknowledgments

This study was made possible with the support and assistance of the 39th and 40th Chinese National Antarctic Research Expeditions (CHINARE) team. We would like to express our heartfelt gratitude for their invaluable contributions during the data collection process.

Financial support

This work is financially supported by the National Natural Science Foundation of China (42201151) and the Basic Research Fund of Chinese Academy of Meteorological Sciences (2023Z004, 2024Z007).

References

- Bauguitte, S. J. B., Brough, N., Frey, M. M., Jones, A. E., Maxfield, D. J., Roscoe, H. K., Rose, M. C., and Wolff, E. W.: A network of autonomous surface ozone monitors in Antarctica: technical description and first results, *Atmos. Meas. Tech.*, 4, 645–658, <https://doi.org/10.5194/amt-4-645-2011>, 2011.
- Bortoli, D., and Kostadinov, I. K.: Stratospheric ozone and nitrogen dioxide amount obtained with GASCOD-type DOAS spectrometer at Terra Nova Bay Station (Antarctica) during December 2000 – January 2001, *Proceedings of SPIE*, 4544, 225–235, <https://doi.org/10.1117/12.454255>, 2002.
- Chen, H., Winderlich, J., Gerbig, C., Meinhardt, F., Rella, C. W., Crosson, E. R., and Batenburg, A. M.: High-accuracy continuous airborne measurements of greenhouse gases (CO₂ and CH₄) using the cavity ring-down spectroscopy (CRDS) technique, *Atmos. Meas. Tech.*, 3, 375–386, <https://doi.org/10.5194/amt-3-375-2010>, 2010.
- Das, S. S., Ratnam, M. V., Uma, K. N., Subrahmanyam, K. V., Girach, I. A., Patra, A. K., Aneesh, S., Suneeth, K. V., Kumar, K. K., Kesarkar, A. P., Sijikumar, S., and Ramkumar, G.: Influence of tropical cyclones on tropospheric ozone: possible implications, *Atmos. Chem. Phys.*, 16, 4837–4847, <https://doi.org/10.5194/acp-16-4837-2016>, 2016.
- DiGangi, J., Choi, Y., Nowak, J., and Davis, K. J.: ACT-America: L2 In Situ Atmospheric CO₂, CO, CH₄, and O₃ Concentrations, Eastern USA, ORNL DAAC, Oak Ridge, Tennessee, USA, <https://doi.org/10.3334/ORN LDAAC/1679>, 2018.
- Ding, M., Tian, B., Ashley, M. C. B., Putero, D., Zhu, Z., Wang, L., Yang, S., Li, C., and Xiao, C.: Year-round record of near-surface ozone and O₃ enhancement events (OEEs) at Dome A, East Antarctica, *Earth Syst. Sci. Data*, 12, 3529–3544, <https://doi.org/10.5194/essd-12-3529-2020>,

删除[Biao]: Bodhaine, B. A., Harris, J. M., and Hofmann, D. J.: Arctic haze: a review, *J. Atmos. Sci.*, 38, 2311–2327, 1981.

2020a.

Ding, M., Yang, D., van den Broeke, M. R., Allison, I., Xiao, C., Qin, D., and Huai, B.: The surface energy balance at Panda 1 Station, Princess Elizabeth Land: a typical katabatic wind region in East Antarctica, *J. Geophys. Res.-Atmos.*, 125, e2019JD030378, <https://doi.org/10.1029/2019JD030378>, 2020b.

Ding, M., Zou, X., Sun, Q., Yang, D., Zhang, W., Bian, L., Lu, C., Allison, I., Heil, P., and Xiao, C.: The PANDA automatic weather station network between the coast and Dome A, East Antarctica, *Earth Syst. Sci. Data*, 14, 5019–5035, <https://doi.org/10.5194/essd-14-5019-2022>, 2022.

Ekeberg, D., Ogner, G., and Fongen, H.: Determination of CH₄, CO₂, and N₂O in air samples and soil atmosphere by gas chromatography mass spectrometry, GC-MS, *J. Environ. Monit.*, 6, 621–623, <https://doi.org/10.1039/B401315H>, 2004.

Griffith, D., Petersen, A. K., Naylor, T., Harvey, M., and Smith, M.: Innovative techniques to measure greenhouse gas emissions from land systems, Report to the Australian Government Department of Climate Change, 0807, 1–35, 2009.

Griffiths, P. R.: Fourier transform infrared spectrometry, *Science*, 222, 297–302, <https://doi.org/10.1126/science.222.4621.297>, <https://doi.org/10.1126/science.222.4621.297>, 1983.

Griffiths, P. T., Keeble, J., Shin, Y. M., Abraham, N. L., Archibald, A. T., and Pyle, J. A.: On the changing role of the stratosphere on the tropospheric ozone budget: 1979–2010, *Geophys. Res. Lett.*, 47, e2019GL086901, <https://doi.org/10.1029/2019gl086901>, 2020.

Heintzenberg, J.: Arctic haze: air pollution in polar regions, *Ambio*, 18, 50–55, <http://www.jstor.org/stable/4313524>, 1989

Hintsa, E. J., Allsup, G. P., Eck, C. F., Hosom, D. S., Purcell, M. J., Roberts, A. A., Scott, D. R., Sholkovitz, E. R., Rawlins, W. T., Mulhall, P. A., Lightner, K., McMillan, W. W., Song, J., and Newchurch, M. J.: New ozone measurement systems for autonomous operation on ocean buoys and towers, *J. Atmos. Ocean. Tech.*, 21, 1007–1016, 2004.

Keeling, C. D.: Atmospheric CO₂ variations at Mauna Loa Observatory, Hawaii, *Tellus*, 28, 538–551, 1976.

Köne, A. Ç., and Büke, T.: Forecasting of CO₂ emissions from fuel combustion using trend analysis, *Renew. Sustain. Energy Rev.*, 14, 2906–2915, <https://doi.org/10.1016/j.rser.2010.06.006>, 2010.

Kwon, J., Ahn, G., Kim, G., Kim, J. C., and Kim, H.: A study on NDIR-based CO₂ sensor to apply remote air quality monitoring system, 2009 ICCAS-SICE, 1683–1687, 2009.

Liu, M., Song, Y., Matsui, H., Shang, F., Kang, L., Cai, X., Zhang, H., and Zhu, T.: Enhanced atmospheric oxidation toward carbon neutrality reduces methane's climate forcing, *Nat. Commun.*, 15, 1362, <https://doi.org/10.1038/s41467-024-47436-9>, 2024.

Mahesh, A., Montzka, S. A., and Dutton, G. S.: Calibration of flask sampling systems for atmospheric trace gas measurements, *J. Atmos. Ocean. Tech.*, 20, 1862–1872, 2003.

Nan, R. Q., Tian, B., Sun, W. J., Li, C. J., and Ding, M. H.: Comparative study on the precision of greenhouse gas analyzers based on LICOR-830 and Picarro G2301, *J. Shandong Norm. Univ. Nat. Sci.*, 39, 52–61, <https://10.3969/j.issn.1001-4748.2024.01.005>, 2024.

Ollison, W. M., Crow, W., and Spicer, C. W.: Field testing of new-technology ambient air ozone monitors, *J. Air Waste Manag. Assoc.*, 63, 855–863,

删除[Biao]: Dutton, E. G., Bodhaine, B. A., and Slusser, J. R.: NOAA's baseline radiation monitoring network, *Bull. Am. Meteorol. Soc.*, 83, 1719–1737, 2002.

删除[Biao]: 2004.

删除[Biao]: 1983.

删除[Biao]: Montzka, S. A., Dutton, G. S., and Hall, B. D.: NOAA's global greenhouse gas reference network, *Bull. Am. Meteorol. Soc.*, 96, 2009–2024, 2015.

678 <https://doi.org/10.1080/10962247.2013.793374>, 2013.
 679 [Popa, M. E., Gloor, M., Manning, A. C., Jordan, A., Schultz, U., Haensel, F., Seifert, T., and](#)
 680 [Heimann, M.: Measurements of greenhouse gases and related tracers at Bialystok tall tower](#)
 681 [station in Poland, Atmos. Meas. Tech., 3, 407–427, <https://doi.org/10.5194/amt-3-407-2010>,](#)
 682 [2010.](#)
 683 Prinn, R. G., Weiss, R. F., and Miller, B. R.: Intercomparison of AGAGE, NOAA, and SIO
 684 atmospheric trace gas calibration scales, Atmos. Meas. Tech., 11, 1587–1601,
 685 <https://doi.org/10.5194/amt-11-1587-2018>, 2018.
 686 Sturm, P., Wanner, H., and Schwikowski, M.: Impact of extreme weather events on high-alpine
 687 atmospheric observations at Jungfraujoch, Atmos. Res., 116, 1–12, 2012.
 688 Tanimoto, H., Mukai, H., Hashimoto, S., and Kajii, Y.: Intercomparison of ultraviolet photometry
 689 and gas-phase titration techniques for ozone reference standards at ambient levels, J.
 690 Geophys. Res.-Atmos., 111, D16305, <https://doi.org/10.1029/2005JD006646>, 2006.
 691 Tian, B., Ding, M., Putero, D., Li, C., Zhang, D., Tang, J., Zheng, X., Bian, L., and Xiao, C.:
 692 Multi-year variation of near-surface ozone at Zhongshan Station, Antarctica, Environ. Res.
 693 Lett., 17, 044021, <https://doi.org/10.1088/1748-9326/ac583c>, 2022.
 694 van den Broeke, M. R., van Lipzig, N. P. M., and van Meijgaard, E.: Momentum budget of the
 695 East Antarctic atmospheric boundary layer: results of a regional climate model, J. Atmos. Sci.,
 696 59, 3117–3129, [https://doi.org/10.1175/1520-0469\(2002\)059<3117:MBOTEA>2.0.CO;2](https://doi.org/10.1175/1520-0469(2002)059<3117:MBOTEA>2.0.CO;2),
 697 2002.
 698 van den Broeke, M. R., and van Lipzig, N. P. M.: Factors controlling the near-surface wind field in
 699 Antarctica, Mon. Weather Rev., 131, 733–743,
 700 [https://doi.org/10.1175/1520-0493\(2003\)131<0733:FCTNSW>2.0.CO;2](https://doi.org/10.1175/1520-0493(2003)131<0733:FCTNSW>2.0.CO;2), 2003.
 701 [Wang, S., Tian B., Ding M., Zhang D., Zhang T., Sun W.: Usage and performance assessment of a](#)
 702 [novelanalyzer-Model 205, OPTICAL INSTRUMENTS, 39\(2\), 58-63,](#)
 703 [https://doi.org/10.3969/j.issn. 1005-5630.2017.02.011, 2017.](#)
 704 Williams, E. J., Fehsenfeld, F. C., Jobson, B. T., and Holloway, J. S.: Comparison of ultraviolet
 705 absorbance, chemiluminescence, and DOAS instruments for ambient ozone monitoring,
 706 Environ. Sci. Technol., 40, 5755–5762, <https://doi.org/10.1021/es0606353>, 2006.
 707 [Global Atmosphere Watch \(GAW\). Global Atmosphere Watch Measurements Guide \(GAW Report](#)
 708 [No. 143\); World Meteorological Organization \(WMO\): Geneva, 2001.](#)
 709 [Xia, T., Catalan, J., Hu, C., and Batterman, S.: Development of a mobile platform for monitoring](#)
 710 [gaseous, particulate, and greenhouse gas \(GHG\) pollutants, Environ. Monit. Assess., 193, 7,](#)
 711 [https://doi.org/10.1007/s10661-020-08790-9, 2023.](#)
 712 Xu, M., Peng, B., Zhu, X., and Guo, Y.: Multi-gas detection system based on non-dispersive
 713 infrared (NDIR) spectral technology, Sensors, 22, 836, <https://doi.org/10.3390/s22030836>,
 714 2022.
 715 Yang, D., Ding, M., Dou, T., Han, W., Liu, W., Zhang, J., Du, Z., and Xiao, C.: On the differences
 716 in precipitation type between the Arctic, Antarctica, and Tibetan Plateau, Front. Earth Sci., 9,
 717 607487, <https://doi.org/10.3389/feart.2021.607487>, 2021.

删除[Biao]: Platt, U., and Lunder, C. R.: EBAS database
 quality assurance and control guidelines for ozone
 measurements, Norwegian Institute for Air Research (NILU),
 2024.

删除[Biao]: 2010.

删除[Biao]: World Meteorological Organization (WMO):
 Global Atmosphere Watch (GAW) measurement guidelines for
 greenhouse gases, WMO-TD-No. 1881, 2018.

删除[Biao]: Wu, C., Prinn, R. G., and Weiss, R. F.:
 Compatibility of air samples collected in glass and stainless
 steel flasks for halocarbon measurements, J. Atmos. Ocean.
 Tech., 18, 1743–1751, 2001.